

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN042222\
 Data File : VN072151.D
 Acq On : 22 Apr 2022 12:59
 Operator : JC\MD
 Sample : VN0422WBS02
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0422WBS02

Manual Integrations
 APPROVED

Reviewed By :John
 Carlone

Quant Time: Apr 23 03:14:41 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N033022W.M
 Quant Title : SW846 8260
 QLast Update : Thu Mar 31 01:57:54 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.933	168	195	50.000	ug/l	#-0.15
34) 1,4-Difluorobenzene	8.710	114	659937	50.000	ug/l	-0.25
63) Chlorobenzene-d5	0.000	117	0	0.000	ug/l	-11.74
72) 1,4-Dichlorobenzene-d4	13.657	152	249545	50.000	ug/l	-0.01

04/25/2022
 Supervised By :Mahesh
 Sadoda

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.098	65	270778	121634.973	ug/l	-0.34
Spiked Amount	50.000	Range	61 - 141	Recovery	= 243269.940%#	
35) Dibromofluoromethane	7.616	113	231030	59.492	ug/l	-0.40
Spiked Amount	50.000	Range	69 - 133	Recovery	= 118.980%	
50) Toluene-d8	10.316	98	812720	51.160	ug/l	-0.12
Spiked Amount	50.000	Range	65 - 126	Recovery	= 102.320%	
62) 4-Bromofluorobenzene	0.000	95	0	0.000	ug/l	
Spiked Amount	50.000	Range	58 - 135	Recovery	= 0.000%#	

04/25/2022

Target Compounds						Qvalue
3) Chloromethane	2.357	50	715	363.969	ug/l #	43
6) Chloroethane	3.175	64	278	179.129	ug/l #	1
7) Trichlorofluoromethane	3.204	101	57804	21060.284	ug/l	97
8) Diethyl Ether	3.851	74	29678	25585.570	ug/l #	12
14) Allyl chloride	4.657	41	50228	19226.652	ug/l #	67
15) Acrylonitrile	5.198	53	54	51.424	ug/l #	17
16) Acetone	4.363	43	11754	12354.718	ug/l #	61
18) Methyl Acetate	4.651	43	44862	19635.282	ug/l	97
22) Diisopropyl ether	6.498	45	2903	510.442	ug/l #	50
23) Vinyl Acetate	6.322	43	487	107.682	ug/l #	68
25) 2-Butanone	7.198	43	39637	28899.880	ug/l #	1
26) 2,2-Dichloropropane	6.945	77	109	38.004	ug/l #	53
27) cis-1,2-Dichloroethene	6.922	96	62	28.615	ug/l #	1
28) Bromochloromethane	7.592	49	608	451.437	ug/l #	8
29) Tetrahydrofuran	7.457	42	698	785.965	ug/l #	29
30) Chloroform	7.839	83	7884	2236.364	ug/l	92
31) Cyclohexane	7.798	56	122971	40618.865	ug/l #	16
32) 1,1,1-Trichloroethane	7.598	97	84229	27928.131	ug/l	94
36) 1,1-Dichloropropene	7.845	75	90496	16.688	ug/l	98
37) Ethyl Acetate	7.198	43	39637	6.678	ug/l #	78
38) Carbon Tetrachloride	7.822	117	91191	17.158	ug/l	99
39) Methylcyclohexane	9.245	83	97086	15.040	ug/l	98
40) Benzene	8.122	78	327784	19.134	ug/l	98
41) Methacrylonitrile	7.157	41	56747m	19.525	ug/l	
42) 1,2-Dichloroethane	8.204	62	113385	19.134	ug/l	96
43) Isopropyl Acetate	8.263	43	170509	17.271	ug/l	94
44) Trichloroethene	8.986	130	79665	18.051	ug/l	96
45) 1,2-Dichloropropane	9.280	63	86340	20.175	ug/l	98
46) Dibromomethane	9.380	93	62752	21.596	ug/l	98
47) Bromodichloromethane	9.586	83	117889	20.611	ug/l	98
48) Methyl methacrylate	9.286	41	37498	9.155	ug/l #	6
49) 1,4-Dioxane	9.375	88	35905	360.664	ug/l	99
51) 4-Methyl-2-Pentanone	10.210	43	561099	98.850	ug/l	95
52) Toluene	10.380	92	209346	19.332	ug/l	99
53) t-1,3-Dichloropropene	10.616	75	120931	20.173	ug/l	95
54) cis-1,3-Dichloropropene	10.051	75	135376	20.438	ug/l	95

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN042222\
 Data File : VN072151.D
 Acq On : 22 Apr 2022 12:59
 Operator : JC\MD
 Sample : VN0422WBS02
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0422WBS02

Manual Integrations
 APPROVED

Reviewed By :John
 Carlone

Quant Time: Apr 23 03:14:41 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N033022W.M
 Quant Title : SW846 8260
 QLast Update : Thu Mar 31 01:57:54 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
55) 1,1,2-Trichloroethane	10.804	97	96262	21.599	ug/l	99
56) Ethyl methacrylate	10.669	69	133213	20.953	ug/l #	89
57) 1,3-Dichloropropane	10.957	76	155541	20.874	ug/l	99
58) 2-Chloroethyl Vinyl ether	9.898	63	155595	91.065	ug/l	98
59) 2-Hexanone	11.010	43	371955	93.073	ug/l	94
60) Dibromochloromethane	11.157	129	95019	21.866	ug/l	100
61) 1,2-Dibromoethane	11.269	107	90821	20.702	ug/l	99
73) Isopropylbenzene	12.545	105	339038	16.123	ug/l	99
74) N-amyl acetate	12.357	43	105128	17.448	ug/l	93
75) 1,1,2,2-Tetrachloroethane	12.798	83	139668	19.906	ug/l	99
76) 1,2,3-Trichloropropane	12.851	75	119154m	20.612	ug/l	
77) Bromobenzene	12.827	156	96958	18.393	ug/l	97
78) n-propylbenzene	12.892	91	354821	16.041	ug/l	99
79) 2-Chlorotoluene	12.980	91	239897	16.911	ug/l	98
80) 1,3,5-Trimethylbenzene	13.039	105	287799	17.274	ug/l	97
81) trans-1,4-Dichloro-2-b...	12.592	75	35345	18.947	ug/l	97
82) 4-Chlorotoluene	13.080	91	223963	17.032	ug/l	97
83) tert-Butylbenzene	13.304	119	243747	16.004	ug/l	98
84) 1,2,4-Trimethylbenzene	13.345	105	292245	17.977	ug/l	100
85) sec-Butylbenzene	13.480	105	308163	15.609	ug/l	98
86) p-Isopropyltoluene	13.598	119	255703	16.244	ug/l	99
87) 1,3-Dichlorobenzene	13.598	146	148775	17.715	ug/l	99
88) 1,4-Dichlorobenzene	13.674	146	144857	17.680	ug/l	98
89) n-Butylbenzene	13.927	91	170700	14.620	ug/l	99
90) Hexachloroethane	14.198	117	48361	16.782	ug/l	93
91) 1,2-Dichlorobenzene	13.974	146	152684	18.519	ug/l	99
92) 1,2-Dibromo-3-Chloropr...	14.592	75	20631	18.957	ug/l	97
93) 1,2,4-Trichlorobenzene	15.257	180	61772	16.991	ug/l	97
94) Hexachlorobutadiene	15.362	225	38048	15.647	ug/l	99
95) Naphthalene	15.498	128	160444	16.848	ug/l	99
96) 1,2,3-Trichlorobenzene	15.692	180	65196	18.542	ug/l	97

04/25/2022
 Supervised By :Mahesh
 Dadoda

04/25/2022

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN042222\
 Data File : VN072151.D
 Acq On : 22 Apr 2022 12:59
 Operator : JC\MD
 Sample : VN0422WBS02
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 7 Sample Multiplier: 1


Instrument :
 MSVOA_N
 ClientSampleId :
 VN0422WBS02

Manual Integrations APPROVED

Reviewed By :John
 Carlone


Quant Time: Apr 23 03:14:41 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N033022W.M
 Quant Title : SW846 8260
 QLast Update : Thu Mar 31 01:57:54 2022
 Response via : Initial Calibration

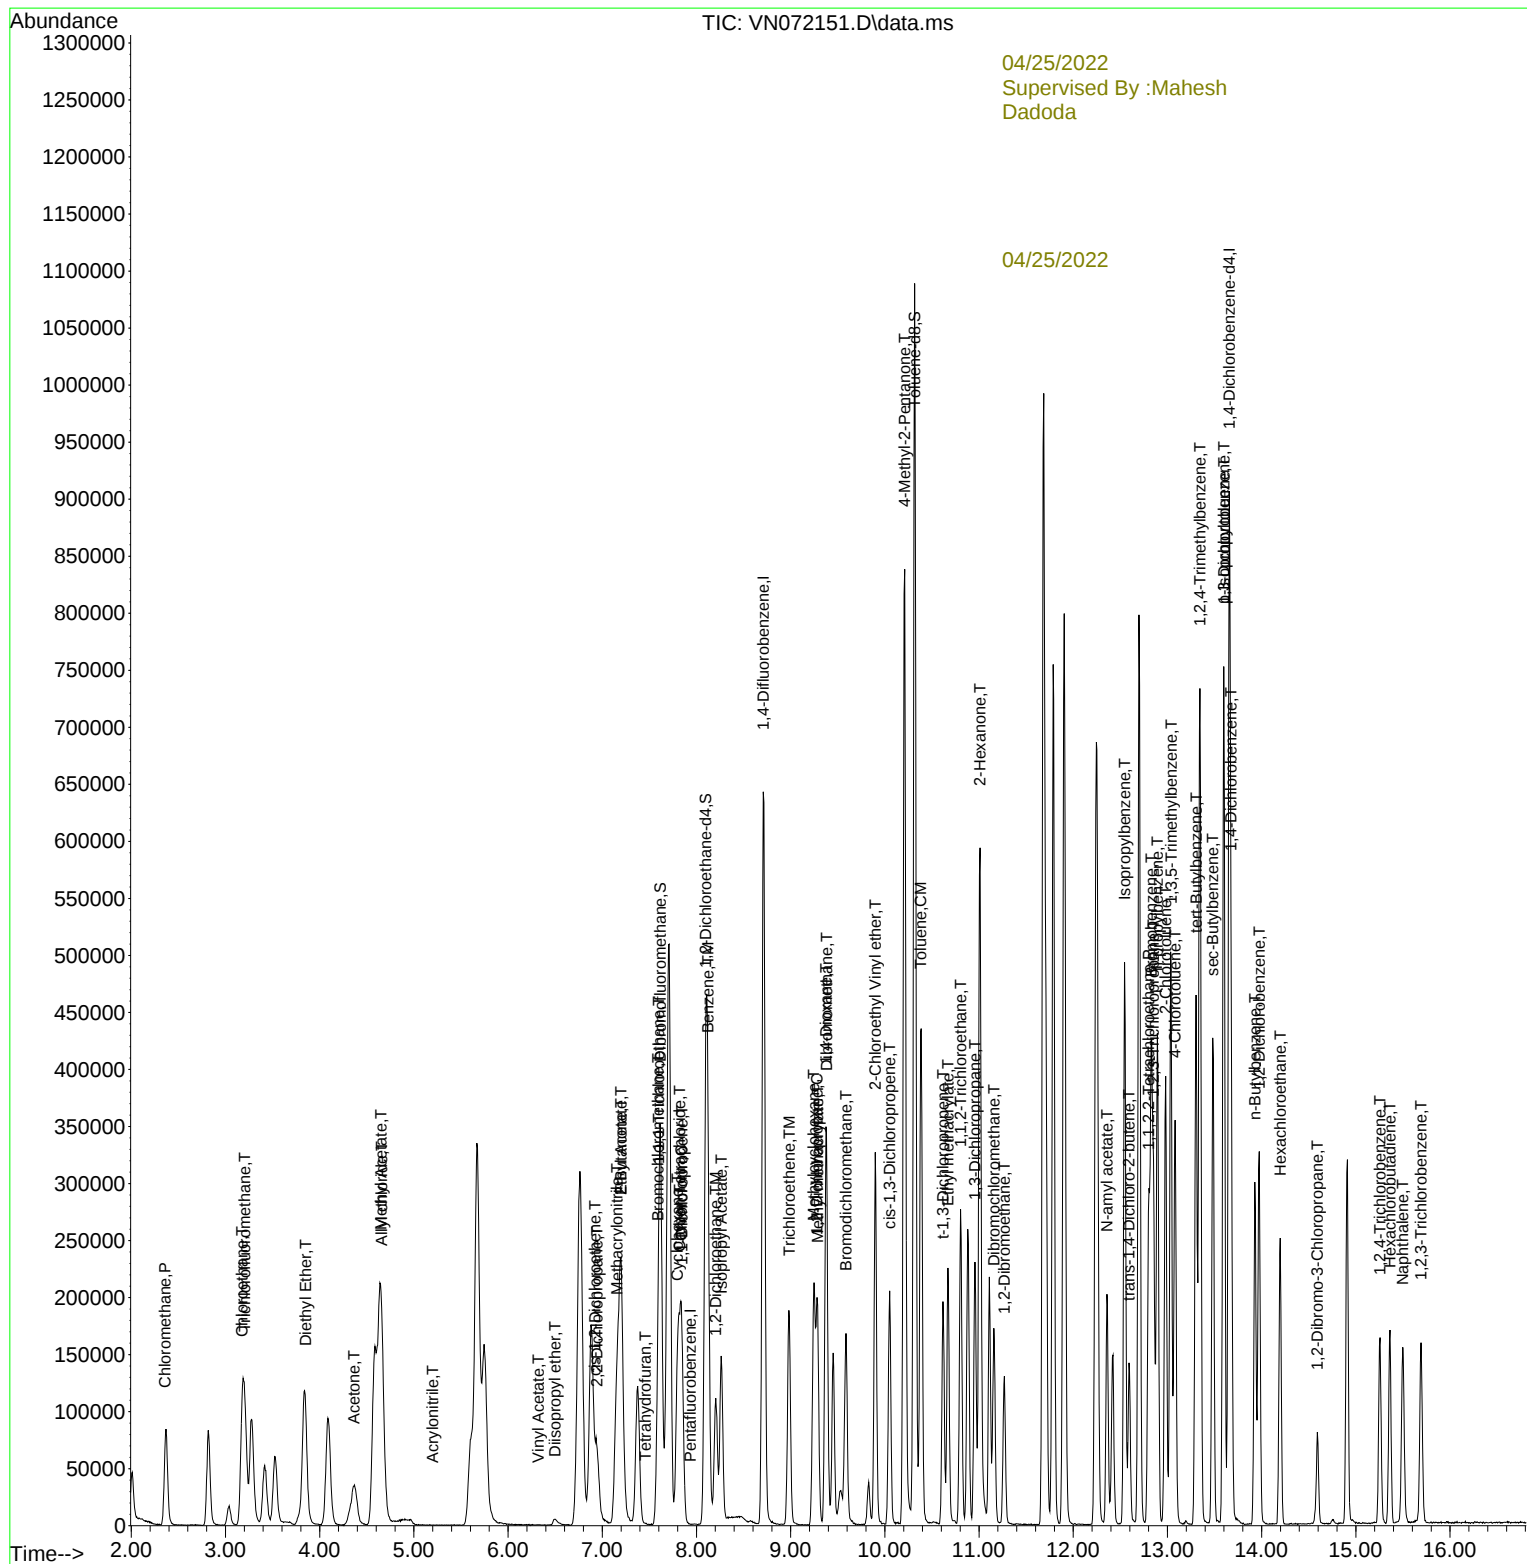



#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.933 min Scan# 1036
Delta R.T. -0.148 min
Lab File: VN072151.D
Acq: 22 Apr 2022 12:59



Instrument :
MSVOA_N
ClientSampleId :
VN0422WBS02

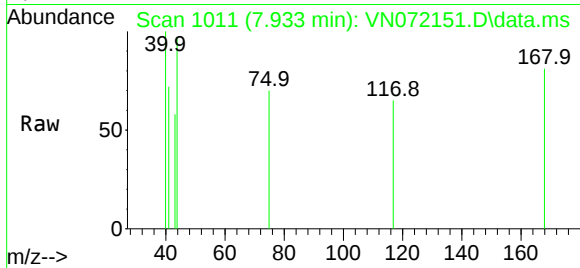

Tgt Ion:168 Resp: 199
Ion Ratio Lower Upper
168 100
99 0.0 42.3 63.5


Manual Integrations
APPROVED

Reviewed By :John
Carlone

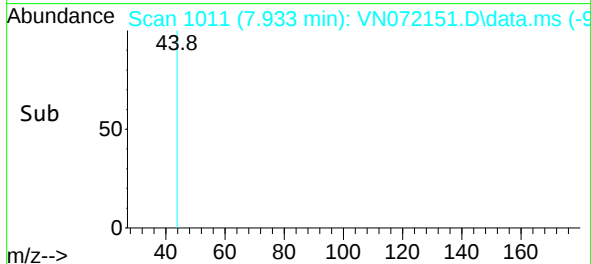




04/25/2022
Supervised By :Mahesh
Dadoda


04/25/2022



#3
Chloromethane
Concen: 363.969 ug/l
RT: 2.357 min Scan# 63
Delta R.T. 0.058 min
Lab File: VN072151.D
Acq: 22 Apr 2022 12:59


Tgt Ion: 50 Resp: 715
Ion Ratio Lower Upper
50 100
52 0.0 25.7 38.5

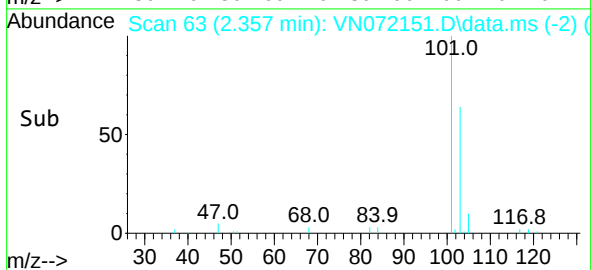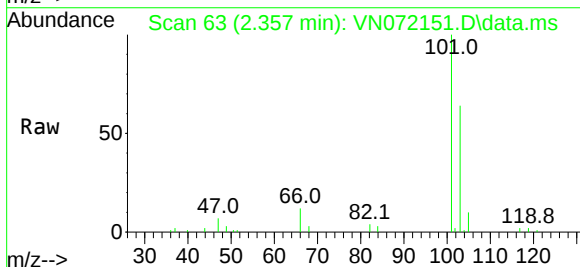



#6
Chloroethane
Concen: 179.129 ug/l
RT: 3.175 min Scan# 207
Delta R.T. 0.165 min
Lab File: VN072151.D
Acq: 22 Apr 2022 12:59



Instrument :
MSVOA_N
ClientSampleId :
VN0422WBS02

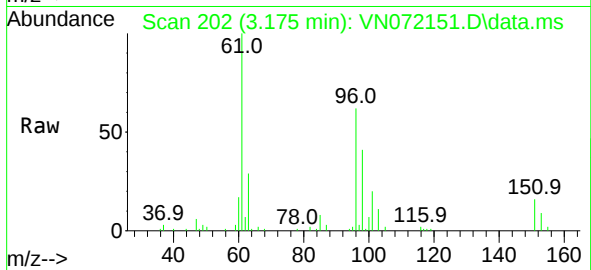

Tgt Ion: 64 Resp: 278
Ion Ratio Lower Upper
64 100
66 145.2 26.2 39.4


Manual Integrations
APPROVED

Reviewed By :John
Carlone

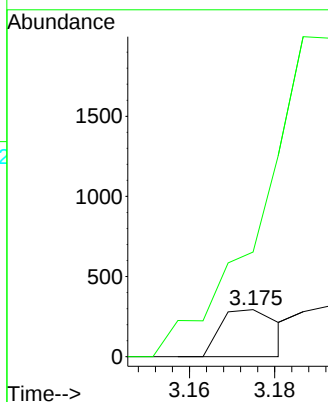




04/25/2022
Supervised By :Mahesh
Dadoda


04/25/2022

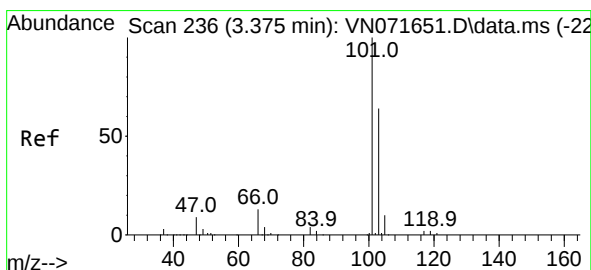

#7
Trichlorofluoromethane
Concen: 21060.284 ug/l
RT: 3.204 min Scan# 207
Delta R.T. -0.171 min
Lab File: VN072151.D
Acq: 22 Apr 2022 12:59


Tgt Ion:101 Resp: 57804
Ion Ratio Lower Upper
101 100
103 61.9 51.5 77.3

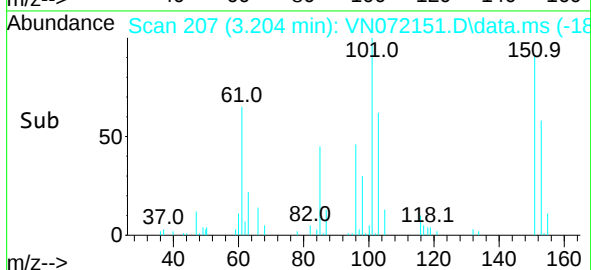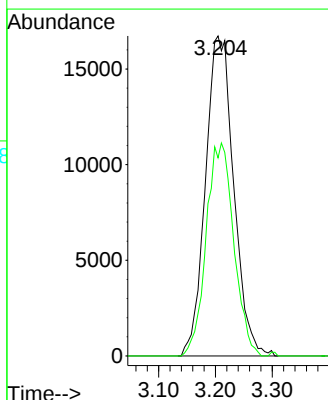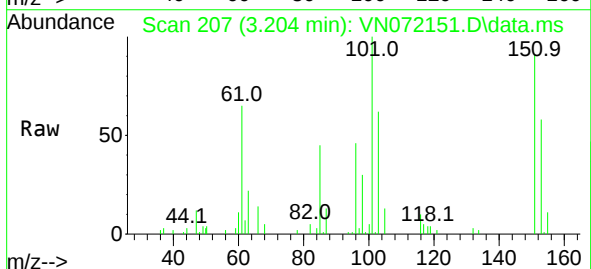



#8
Diethyl Ether
Concen: 25585.570 ug/l
RT: 3.851 min Scan# 317
Delta R.T. 0.023 min
Lab File: VN072151.D
Acq: 22 Apr 2022 12:59



Instrument :
MSVOA_N
ClientSampleId :
VN0422WBS02



Tgt Ion: 74 Resp: 29678
Ion Ratio Lower Upper
74 100
45 4.9 42.9 128.5


Manual Integrations
APPROVED

Reviewed By :John
Carlone

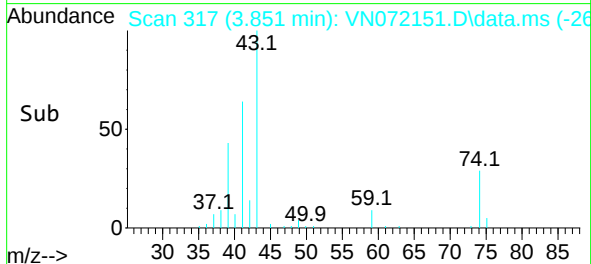


04/25/2022
Supervised By :Mahesh
Dadoda



04/25/2022




#14
Allyl chloride
Concen: 19226.652 ug/l
RT: 4.657 min Scan# 454
Delta R.T. -0.183 min
Lab File: VN072151.D
Acq: 22 Apr 2022 12:59

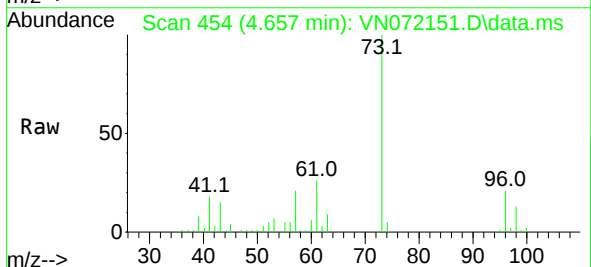


Tgt Ion: 41 Resp: 50228
Ion Ratio Lower Upper
41 100
39 53.6 53.2 79.8
76 0.0 29.9 44.9

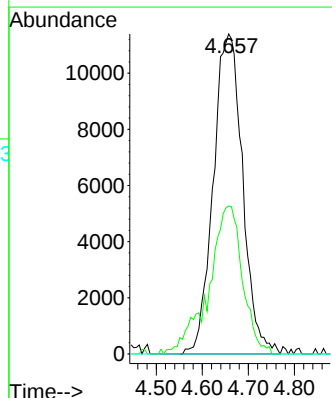



#15
Acrylonitrile
Concen: 51.424 ug/l
RT: 5.198 min Scan# 54
Delta R.T. -0.348 min
Lab File: VN072151.D
Acq: 22 Apr 2022 12:59


Instrument :
MSVOA_N
ClientSampleId :
VN0422WBS02



Tgt Ion: 53 Resp: 54
Ion Ratio Lower Upper
53 100
52 0.0 66.4 99.6
51 0.0 28.5 42.7


Manual Integrations
APPROVED

Reviewed By :John
Carlone

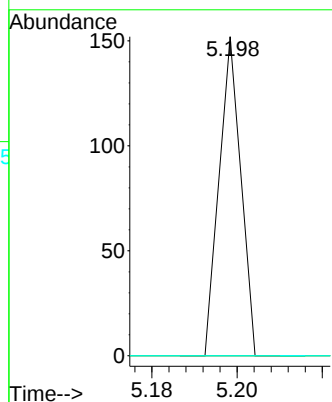




04/25/2022
Supervised By :Mahesh
Dadoda


04/25/2022



#16
Acetone
Concen: 12354.718 ug/l
RT: 4.363 min Scan# 404
Delta R.T. 0.088 min
Lab File: VN072151.D
Acq: 22 Apr 2022 12:59

Tgt Ion: 43 Resp: 11754
Ion Ratio Lower Upper
43 100
58 10.7 26.0 39.0

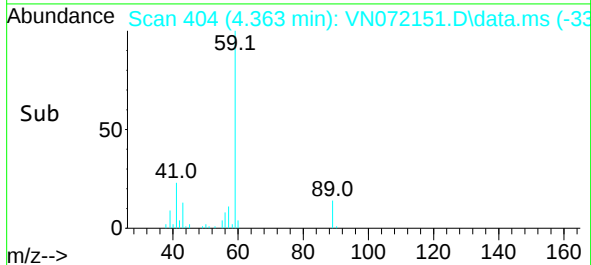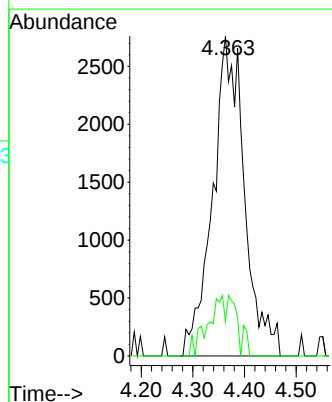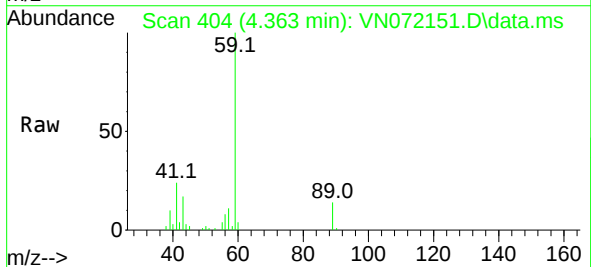





#18
Methyl Acetate
Concen: 19635.282 ug/l
RT: 4.651 min Scan# 41
Delta R.T. -0.195 min
Lab File: VN072151.D
Acq: 22 Apr 2022 12:59

Instrument :
MSVOA_N
ClientSampleId :
VN0422WBS02

Tgt Ion: 43 Resp: 4486
Ion Ratio Lower Upper
43 100
74 25.4 21.6 32.4



Manual Integrations
APPROVED

Reviewed By :John
Carlone






04/25/2022
Supervised By :Mahesh
Dadoda


04/25/2022

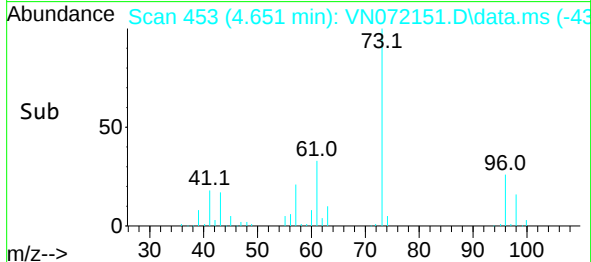

#22
Diisopropyl ether
Concen: 510.442 ug/l
RT: 6.498 min Scan# 767
Delta R.T. 0.011 min
Lab File: VN072151.D
Acq: 22 Apr 2022 12:59

Tgt Ion: 45 Resp: 2903
Ion Ratio Lower Upper
45 100
43 19.8 46.6 70.0#
87 0.0 24.3 36.5#
59 0.0 9.6 14.4#

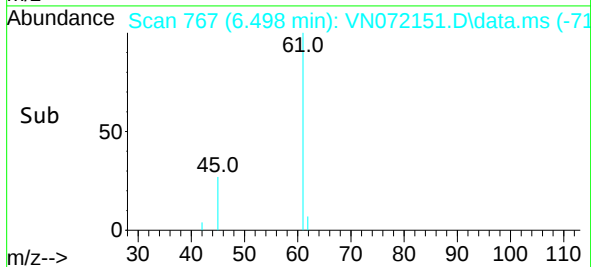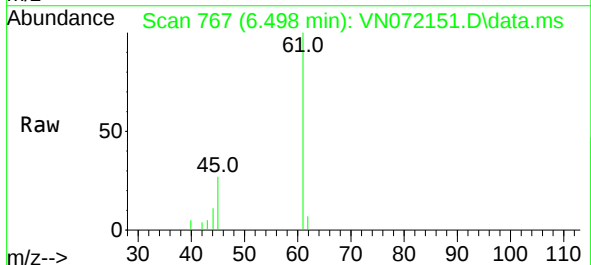





#23
 Vinyl Acetate
 Concen: 107.682 ug/l
 RT: 6.322 min Scan# 71
 Delta R.T. -0.106 min
 Lab File: VN072151.D
 Acq: 22 Apr 2022 12:59

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0422WBS02

Tgt Ion: 43 Resp: 48
 Ion Ratio Lower Upper
 43 100
 86 0.0 10.0 15.0



Manual Integrations
 APPROVED

Reviewed By :John
 Carlone






04/25/2022
 Supervised By :Mahesh
 Dadoda


04/25/2022

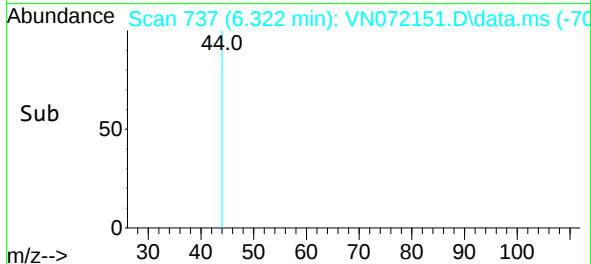

#25
 2-Butanone
 Concen: 28899.880 ug/l
 RT: 7.198 min Scan# 886
 Delta R.T. -0.130 min
 Lab File: VN072151.D
 Acq: 22 Apr 2022 12:59


Tgt Ion: 43 Resp: 39637
 Ion Ratio Lower Upper
 43 100
 72 227.0 23.7 35.5

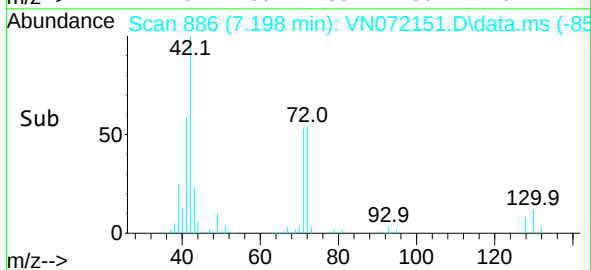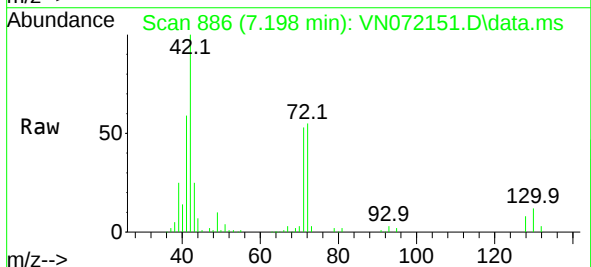



#26
2,2-Dichloropropane
Concen: 38.004 ug/l
RT: 6.945 min Scan# 843
Delta R.T. -0.377 min
Lab File: VN072151.D
Acq: 22 Apr 2022 12:59



Instrument :
MSVOA_N
ClientSampleId :
VN0422WBS02



Tgt Ion: 77 Resp: 109
Ion Ratio Lower Upper
77 100
97 0.0 11.4 34.2


Manual Integrations
APPROVED

Reviewed By :John
Carlone

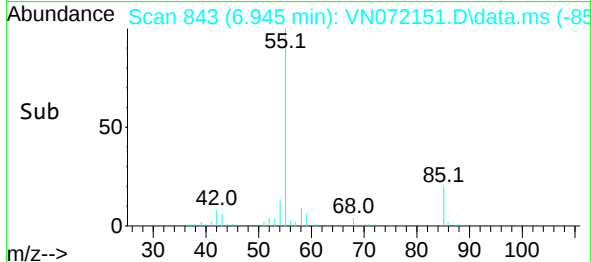


04/25/2022
Supervised By :Mahesh
Dadoda



04/25/2022




#27
cis-1,2-Dichloroethene
Concen: 28.615 ug/l
RT: 6.922 min Scan# 839
Delta R.T. -0.400 min
Lab File: VN072151.D
Acq: 22 Apr 2022 12:59

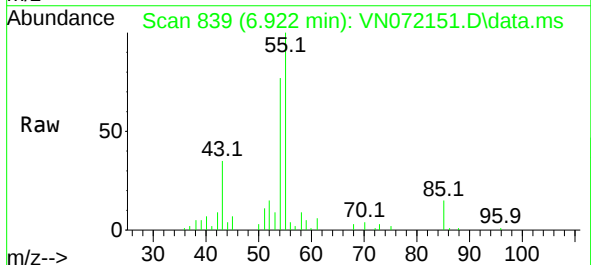


Tgt Ion: 96 Resp: 62
Ion Ratio Lower Upper
96 100
61 0.0 0.0 280.6
98 0.0 0.0 128.4

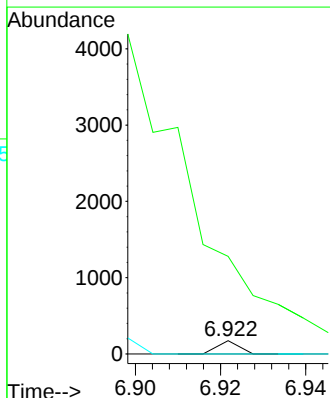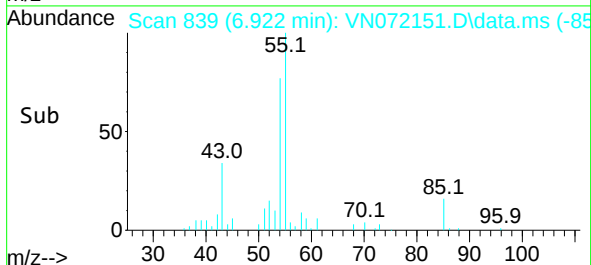



#28
Bromochloromethane
Concen: 451.437 ug/l
RT: 7.592 min Scan# 91
Delta R.T. -0.065 min
Lab File: VN072151.D
Acq: 22 Apr 2022 12:59



Instrument :
MSVOA_N
ClientSampleId :
VN0422WBS02



Tgt Ion: 49 Resp: 608
Ion Ratio Lower Upper
49 100
129 0.0 0.0 4.6
130 0.0 69.7 104.5


Manual Integrations
APPROVED

Reviewed By :John
Carlone

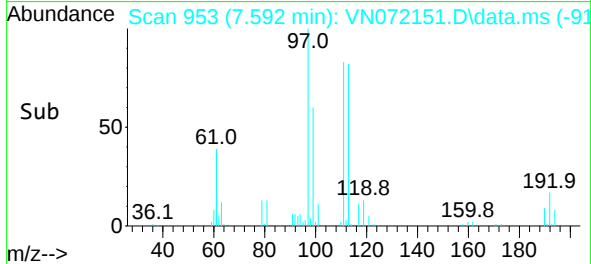


04/25/2022
Supervised By :Mahesh
Dadoda



04/25/2022




#29
Tetrahydrofuran
Concen: 785.965 ug/l
RT: 7.457 min Scan# 930
Delta R.T. -0.218 min
Lab File: VN072151.D
Acq: 22 Apr 2022 12:59

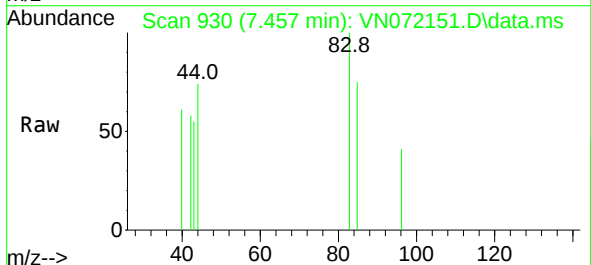

Tgt Ion: 42 Resp: 698
Ion Ratio Lower Upper
42 100
72 0.0 39.7 59.5#
71 0.0 36.6 55.0#

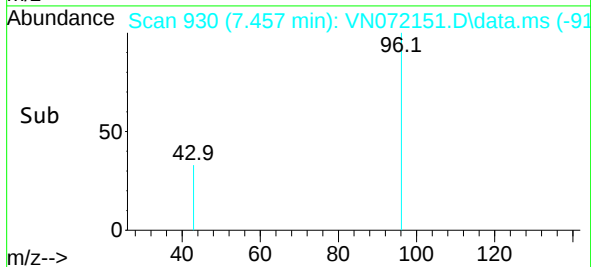





#30
Chloroform
Concen: 2236.364 ug/l
RT: 7.839 min Scan# 990
Delta R.T. 0.029 min
Lab File: VN072151.D
Acq: 22 Apr 2022 12:59

Instrument :
MSVOA_N
Client Sample Id :
VN0422WBS02

Tgt Ion: 83 Resp: 7884
Ion Ratio Lower Upper
83 100
85 58.3 51.8 77.8



Manual Integrations
APPROVED

Reviewed By :John
Carlone






04/25/2022
Supervised By :Mahesh
Dadoda


04/25/2022

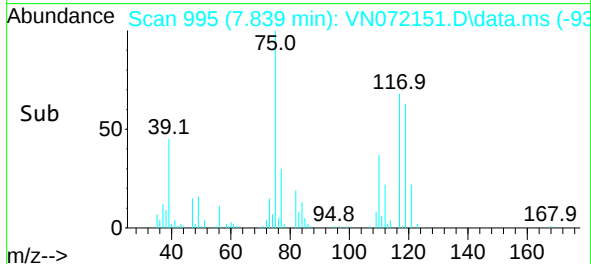

#31
Cyclohexane
Concen: 40618.865 ug/l
RT: 7.798 min Scan# 988
Delta R.T. -0.294 min
Lab File: VN072151.D
Acq: 22 Apr 2022 12:59

Tgt Ion: 56 Resp: 122971
Ion Ratio Lower Upper
56 100
69 0.0 27.8 41.8#
84 5.1 76.9 115.3#

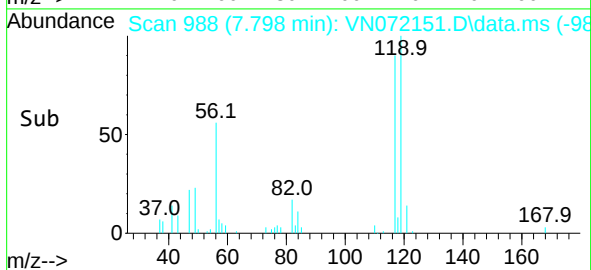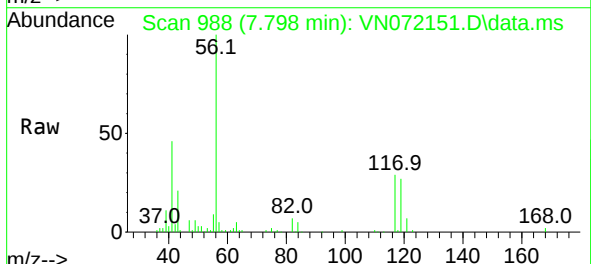



#32

1,1,1-Trichloroethane

Concen: 27928.131 ug/l

RT: 7.598 min Scan# 91

Delta R.T. -0.412 min

Lab File: VN072151.D

Acq: 22 Apr 2022 12:59

Instrument :

MSVOA_N

ClientSampleId :



VN0422WBS02

Tgt Ion:	97	Resp:	84229
Ion Ratio	Lower	Upper	
97	100		
99	59.4	50.6	76.0
61	39.4	36.0	54.0

Manual Integrations



APPROVED

Reviewed By :John
Carlone



04/25/2022
Supervised By :Mahesh
Dadoda

04/25/2022

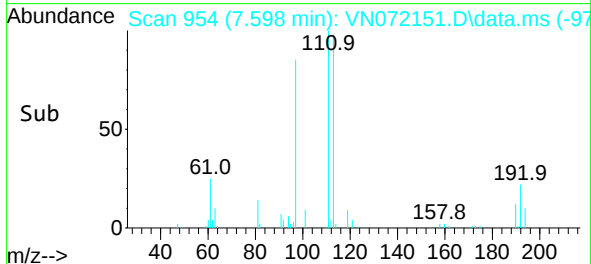

#33

1,2-Dichloroethane-d4

Concen: 121634.973 ug/l




RT: 8.098 min Scan# 1039


Delta R.T. -0.336 min

Lab File: VN072151.D

Acq: 22 Apr 2022 12:59

Tgt Ion:	65	Resp:	270778
Ion Ratio	Lower	Upper	
65	100		
67	53.8	0.0	104.8

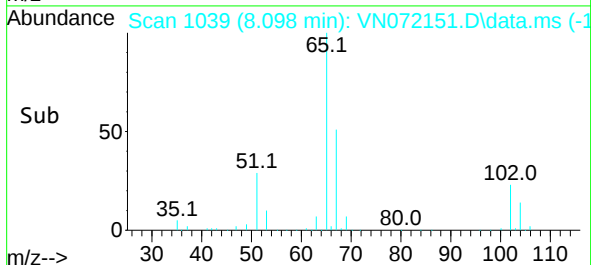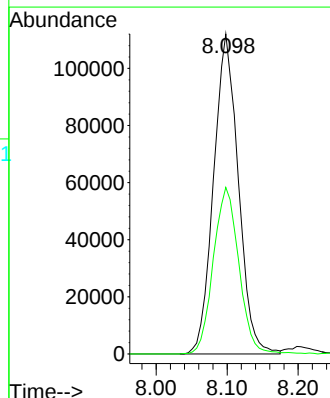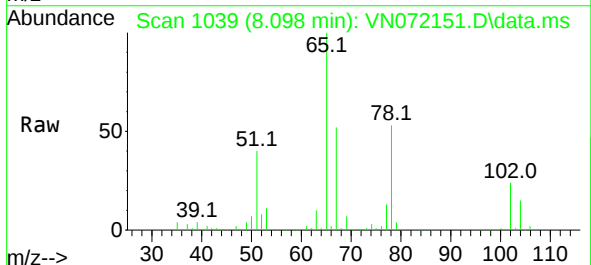



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.710 min Scan# 1186

Delta R.T. -0.253 min

Lab File: VN072151.D

Acq: 22 Apr 2022 12:59

Instrument :

MSVOA_N

ClientSampleId :



VN0422WBS02

Tgt Ion:114 Resp: 65993

Ion	Ratio	Lower	Upper
114	100		
63	18.6	0.0	40.0
88	15.1	0.0	32.6



Manual Integrations
APPROVED

Reviewed By :John
Carlone



04/25/2022
Supervised By :Mahesh
Dadoda

04/25/2022



#35

Dibromofluoromethane

Concen: 59.492 ug/l

RT: 7.616 min Scan# 957




Delta R.T. -0.400 min


Lab File: VN072151.D

Acq: 22 Apr 2022 12:59

Tgt Ion:113 Resp: 231030

Ion	Ratio	Lower	Upper
113	100		
111	102.9	81.4	122.0
192	23.3	17.0	25.6

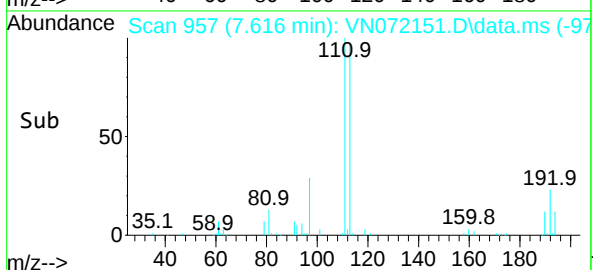



#36

1,1-Dichloropropene

Concen: 16.688 ug/l

RT: 7.845 min Scan# 904

Delta R.T. -0.371 min

Lab File: VN072151.D

Acq: 22 Apr 2022 12:59

Instrument :

MSVOA_N



ClientSampleId :

VN0422WBS02

Tgt Ion: 75	Resp: 90490
Ion Ratio	Lower Upper
75 100	
110 37.6	18.3 54.8
77 30.0	25.1 37.7



Manual Integrations
APPROVED

Reviewed By :John
Carlone



04/25/2022
Supervised By :Mahesh
Dadoda

04/25/2022



#37

Ethyl Acetate

Concen: 6.678 ug/l




RT: 7.198 min Scan# 886


Delta R.T. -0.206 min

Lab File: VN072151.D

Acq: 22 Apr 2022 12:59


Tgt Ion: 43	Resp: 39637
Ion Ratio	Lower Upper
43 100	
61 0.0	11.8 17.6#
70 9.3	9.3 13.9

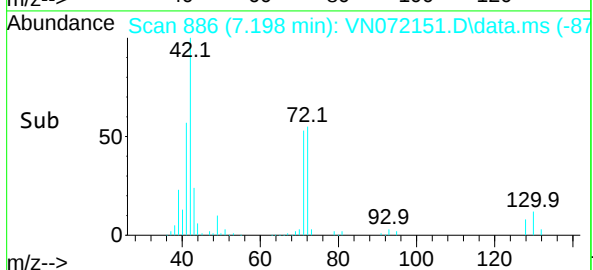



#38
Carbon Tetrachloride
Concen: 17.158 ug/l
RT: 7.822 min Scan# 9119
Delta R.T. -0.382 min
Lab File: VN072151.D
Acq: 22 Apr 2022 12:59



Instrument :
MSVOA_N
ClientSampleId :
VN0422WBS02



Tgt Ion: 117 Resp: 9119
Ion Ratio Lower Upper
117 100
119 95.1 75.8 113.8
121 29.6 24.6 37.0


Manual Integrations
APPROVED

Reviewed By :John
Carlone

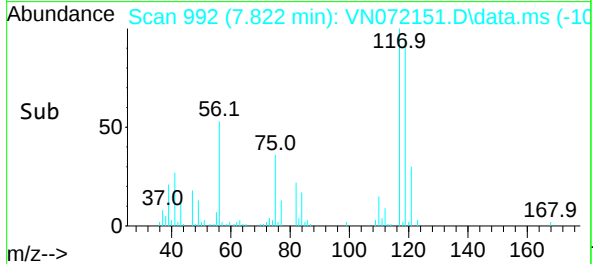


04/25/2022
Supervised By :Mahesh
Dadoda



04/25/2022




#39
Methylcyclohexane
Concen: 15.040 ug/l
RT: 9.245 min Scan# 1234
Delta R.T. -0.206 min
Lab File: VN072151.D
Acq: 22 Apr 2022 12:59

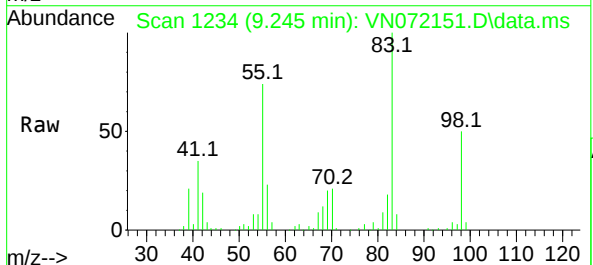


Tgt Ion: 83 Resp: 97086
Ion Ratio Lower Upper
83 100
55 74.3 57.8 86.8
98 49.7 39.4 59.2

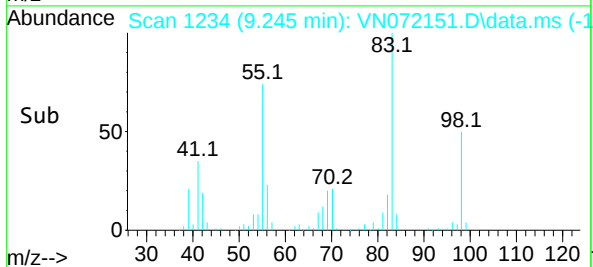



#40
Benzene
Concen: 19.134 ug/l
RT: 8.122 min Scan# 1043
Delta R.T. -0.335 min
Lab File: VN072151.D
Acq: 22 Apr 2022 12:59



Instrument :
MSVOA_N
ClientSampleId :
VN0422WBS02



Tgt Ion: 78 Resp: 327784
Ion Ratio Lower Upper
78 100
77 23.4 19.4 29.0


Manual Integrations
APPROVED

Reviewed By :John
Carlone

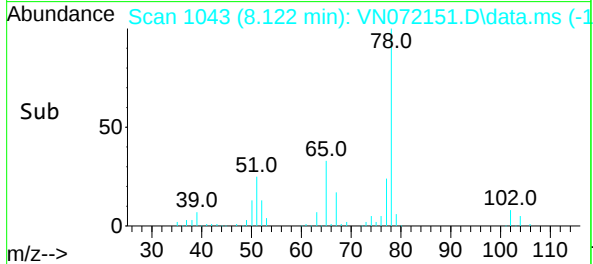




04/25/2022
Supervised By :Mahesh
Dadoda


04/25/2022



#41
Methacrylonitrile
Concen: 19.525 ug/l m
RT: 7.157 min Scan# 879
Delta R.T. -0.471 min
Lab File: VN072151.D
Acq: 22 Apr 2022 12:59

Tgt Ion: 41 Resp: 56747
Ion Ratio Lower Upper
41 100
39 70.1 48.6 73.0
67 0.0 73.4 110.2#
52 0.0 27.7 41.5#

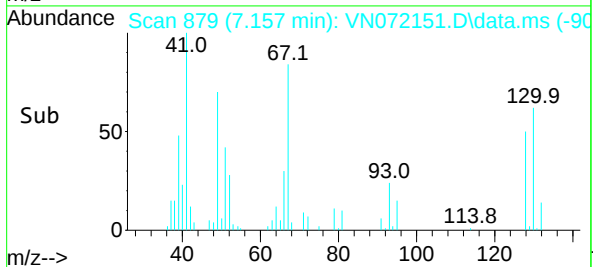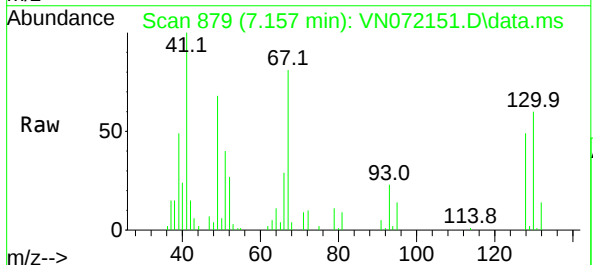



#42

1,2-Dichloroethane

Concen: 19.134 ug/l

RT: 8.204 min Scan# 1112

Delta R.T. -0.324 min

Lab File: VN072151.D

Acq: 22 Apr 2022 12:59

Instrument :

MSVOA_N

ClientSampleId :

VN0422WBS02

Tgt Ion: 62 Resp: 11338

Ion Ratio Lower Upper



62 100

98 11.2 0.0 19.4

Manual Integrations



APPROVED

Reviewed By :John
Carlone

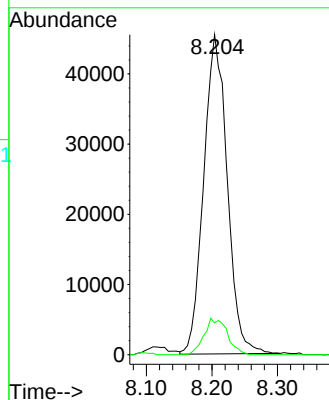

04/25/2022
Supervised By :Mahesh
Dadoda

04/25/2022



#43

Isopropyl Acetate

Concen: 17.271 ug/l

RT: 8.263 min Scan# 1067

Delta R.T. -0.288 min

Lab File: VN072151.D

Acq: 22 Apr 2022 12:59




Tgt Ion: 43 Resp: 170509


Ion Ratio Lower Upper

43 100

61 23.3 21.9 32.9


87 16.5 12.0 18.0

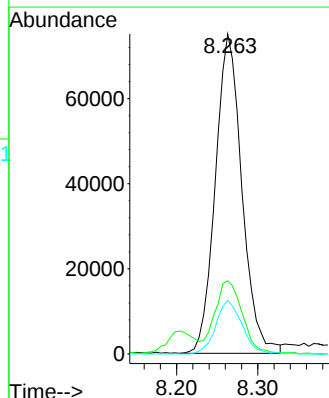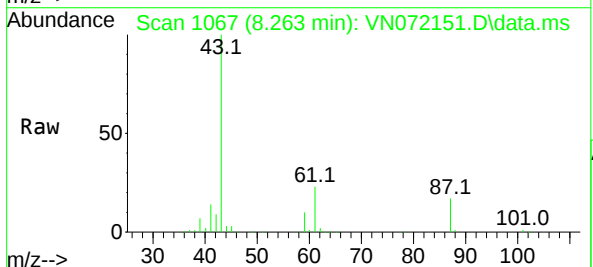



#44
Trichloroethene
Concen: 18.051 ug/l
RT: 8.986 min Scan# 1190
Delta R.T. -0.224 min
Lab File: VN072151.D
Acq: 22 Apr 2022 12:59


Instrument :
MSVOA_N
ClientSampleId :
VN0422WBS02



Tgt Ion:130 Resp: 7966
Ion Ratio Lower Upper
130 100
95 89.8 0.0 186.8


Manual Integrations
APPROVED

Reviewed By :John
Carlone




04/25/2022
Supervised By :Mahesh
Dadoda



04/25/2022




#45
1,2-Dichloropropane
Concen: 20.175 ug/l
RT: 9.280 min Scan# 1240
Delta R.T. -0.206 min
Lab File: VN072151.D
Acq: 22 Apr 2022 12:59

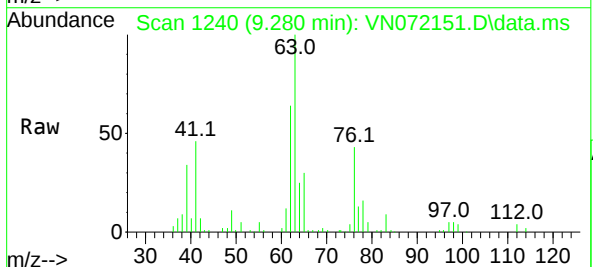


Tgt Ion: 63 Resp: 86340
Ion Ratio Lower Upper
63 100
65 30.0 24.9 37.3

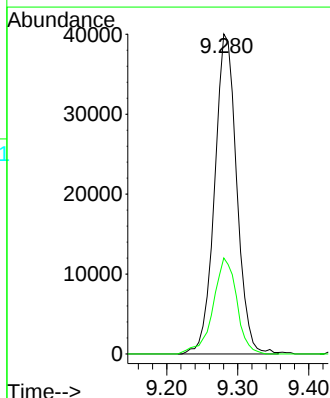



#46
Dibromomethane
Concen: 21.596 ug/l
RT: 9.380 min Scan# 11
Delta R.T. -0.195 min
Lab File: VN072151.D
Acq: 22 Apr 2022 12:59



Instrument :
MSVOA_N
ClientSampleId :
VN0422WBS02



Tgt Ion: 93 Resp: 62752
Ion Ratio Lower Upper
93 100
95 81.2 66.9 100.3
174 110.6 86.6 130.0


Manual Integrations
APPROVED

Reviewed By :John
Carlone

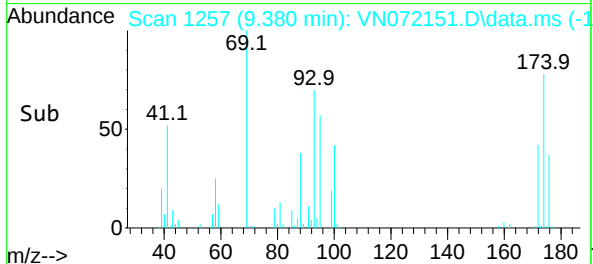


04/25/2022
Supervised By :Mahesh
Dadoda



04/25/2022




#47
Bromodichloromethane
Concen: 20.611 ug/l
RT: 9.586 min Scan# 1292
Delta R.T. -0.171 min
Lab File: VN072151.D
Acq: 22 Apr 2022 12:59

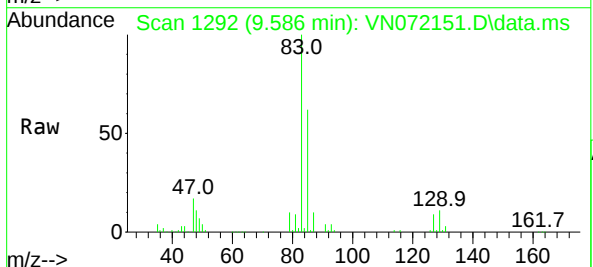

Tgt Ion: 83 Resp: 117889
Ion Ratio Lower Upper
83 100
85 61.9 50.5 75.7
127 9.0 6.8 10.2

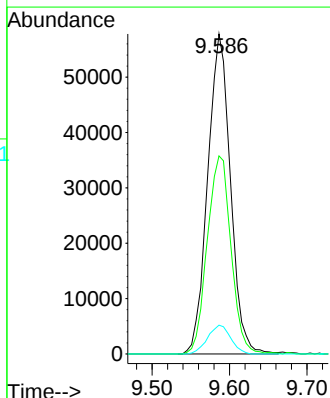



#48

Methyl methacrylate

Concen: 9.155 ug/l

RT: 9.286 min Scan# 1241

Delta R.T. -0.265 min

Lab File: VN072151.D

Acq: 22 Apr 2022 12:59

Instrument :

MSVOA_N

ClientSampleId :



VN0422WBS02

Tgt Ion: 41 Resp: 37498

Ion	Ratio	Lower	Upper
41	100		
69	0.0	74.7	112.1
39	121.8	45.6	68.4



Manual Integrations
APPROVED

Reviewed By :John
Carlone

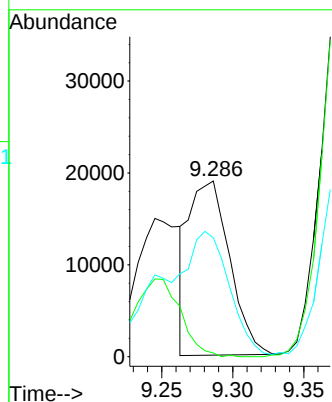

04/25/2022
Supervised By :Mahesh
Dadoda

04/25/2022



#49

1,4-Dioxane

Concen: 360.664 ug/l

RT: 9.375 min Scan# 1256




Delta R.T. -0.188 min


Lab File: VN072151.D

Acq: 22 Apr 2022 12:59

Tgt Ion: 88 Resp: 35905


Ion	Ratio	Lower	Upper
88	100		
43	25.4	20.2	30.4
58	67.0	54.2	81.4

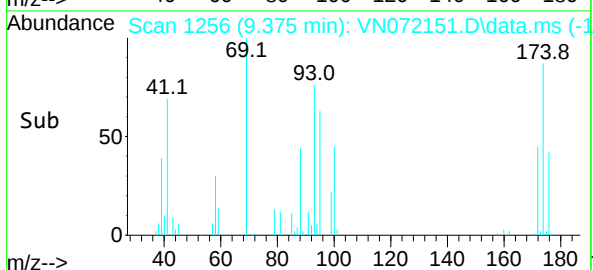

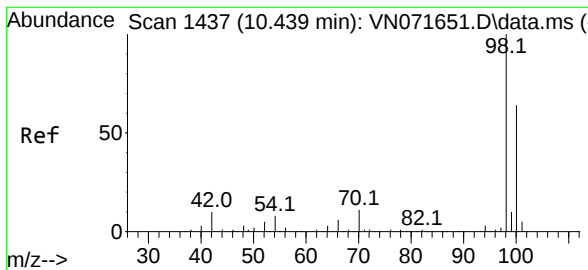

#50
Toluene-d8
Concen: 51.160 ug/l
RT: 10.316 min Scan# 1437
Delta R.T. -0.123 min
Lab File: VN072151.D
Acq: 22 Apr 2022 12:59



Instrument :
MSVOA_N
ClientSampleId :
VN0422WBS02

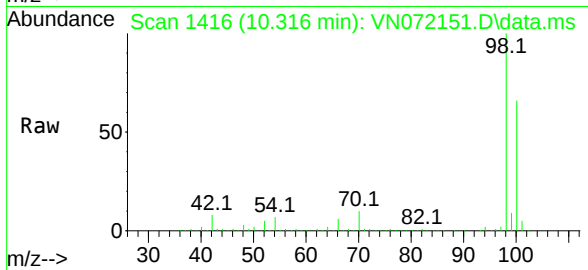

Tgt Ion: 98 Resp: 812720
Ion Ratio Lower Upper
98 100
100 65.0 52.6 78.8


Manual Integrations
APPROVED

Reviewed By :John
Carlone

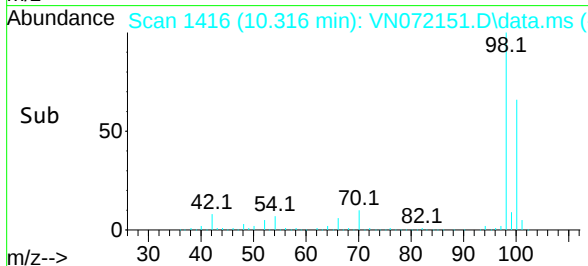


04/25/2022
Supervised By :Mahesh
Dadoda



04/25/2022

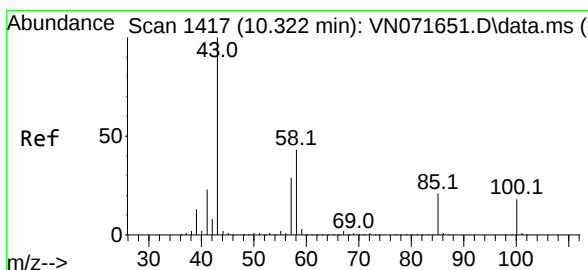


#51
4-Methyl-2-Pentanone
Concen: 98.850 ug/l
RT: 10.210 min Scan# 1398
Delta R.T. -0.112 min
Lab File: VN072151.D
Acq: 22 Apr 2022 12:59

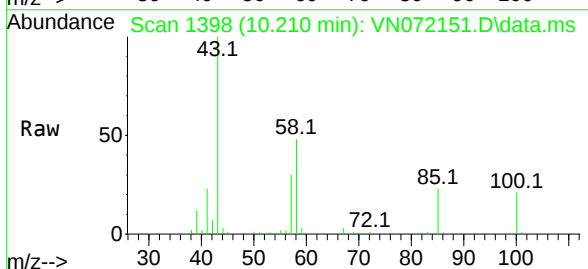


Tgt Ion: 43 Resp: 561099
Ion Ratio Lower Upper
43 100
58 46.1 34.1 51.1

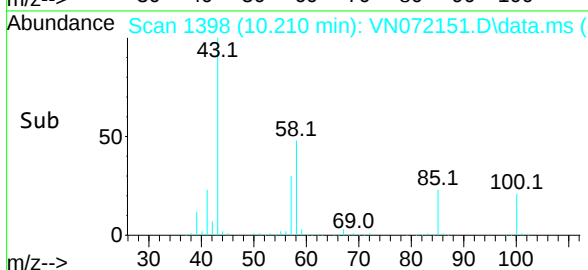



#52
Toluene
Concen: 19.332 ug/l
RT: 10.380 min Scan# 1447
Delta R.T. -0.118 min
Lab File: VN072151.D
Acq: 22 Apr 2022 12:59



Instrument :
MSVOA_N
ClientSampleId :
VN0422WBS02



Tgt Ion: 92 Resp: 209340
Ion Ratio Lower Upper
92 100
91 173.9 138.6 207.8


Manual Integrations
APPROVED

Reviewed By :John
Carlone






04/25/2022
Supervised By :Mahesh
Dadoda


04/25/2022



#53
t-1,3-Dichloropropene
Concen: 20.173 ug/l
RT: 10.616 min Scan# 1467
Delta R.T. -0.094 min
Lab File: VN072151.D
Acq: 22 Apr 2022 12:59


Tgt Ion: 75 Resp: 120931
Ion Ratio Lower Upper
75 100
77 29.2 25.6 38.4

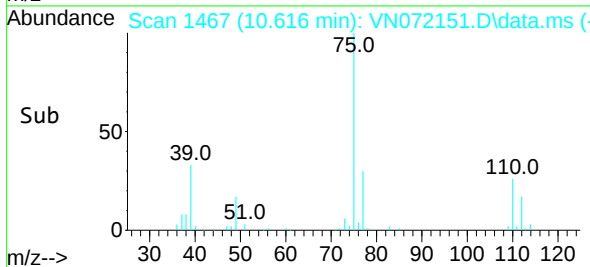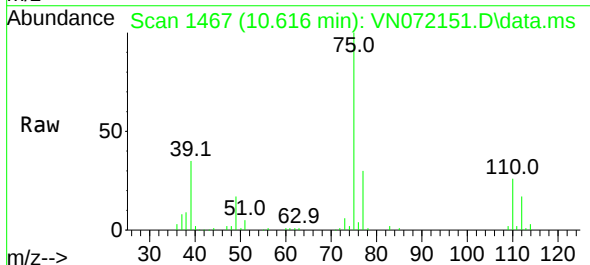



#54
cis-1,3-Dichloropropene
Concen: 20.438 ug/l
RT: 10.051 min Scan# 1498
Delta R.T. -0.135 min
Lab File: VN072151.D
Acq: 22 Apr 2022 12:59



Instrument :
MSVOA_N
ClientSampleId :
VN0422WBS02



Tgt Ion: 75 Resp: 135370
Ion Ratio Lower Upper
75 100
77 31.6 25.2 37.8
39 39.3 35.7 53.5


Manual Integrations
APPROVED

Reviewed By :John
Carlone






04/25/2022
Supervised By :Mahesh
Dadoda


04/25/2022



#55
1,1,2-Trichloroethane
Concen: 21.599 ug/l
RT: 10.804 min Scan# 1499
Delta R.T. -0.088 min
Lab File: VN072151.D
Acq: 22 Apr 2022 12:59


Tgt Ion: 97 Resp: 96262
Ion Ratio Lower Upper
97 100
83 82.9 66.2 99.4
85 53.9 43.9 65.9
99 61.3 50.6 76.0

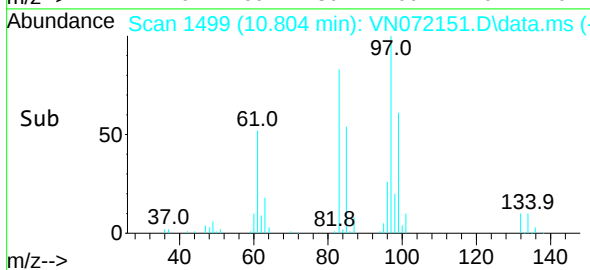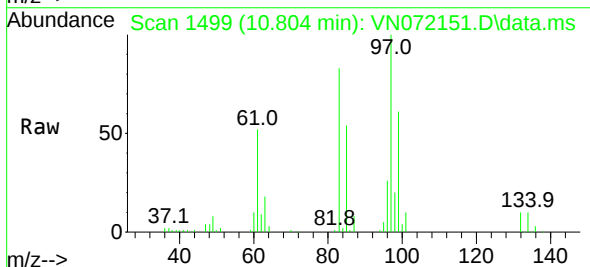



#56
Ethyl methacrylate
Concen: 20.953 ug/l
RT: 10.669 min Scan# 1490
Delta R.T. -0.082 min
Lab File: VN072151.D
Acq: 22 Apr 2022 12:59



Instrument :
MSVOA_N
ClientSampleId :
VN0422WBS02

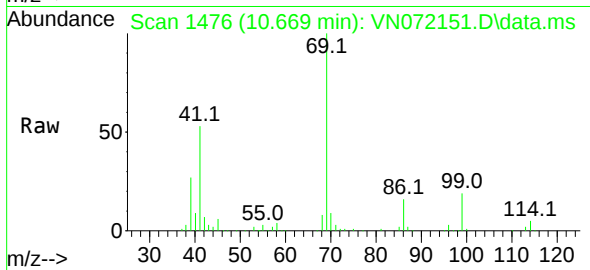

Tgt Ion: 69 Resp: 13321
Ion Ratio Lower Upper
69 100
41 52.9 47.8 71.6
39 25.9 27.3 40.9


Manual Integrations
APPROVED

Reviewed By :John
Carlone






04/25/2022
Supervised By :Mahesh
Dadoda


04/25/2022

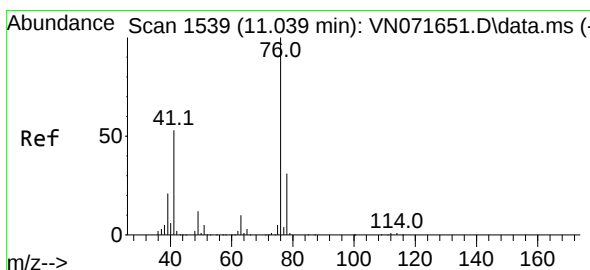

#57
1,3-Dichloropropane
Concen: 20.874 ug/l
RT: 10.957 min Scan# 1525
Delta R.T. -0.082 min
Lab File: VN072151.D
Acq: 22 Apr 2022 12:59

Tgt Ion: 76 Resp: 155541
Ion Ratio Lower Upper
76 100
78 31.9 26.2 39.2

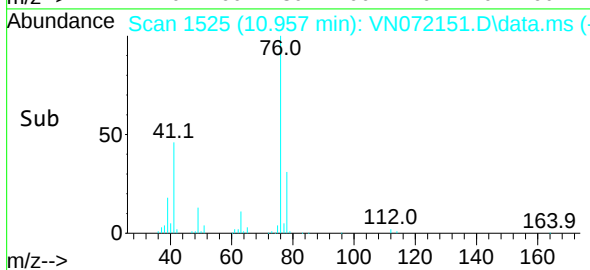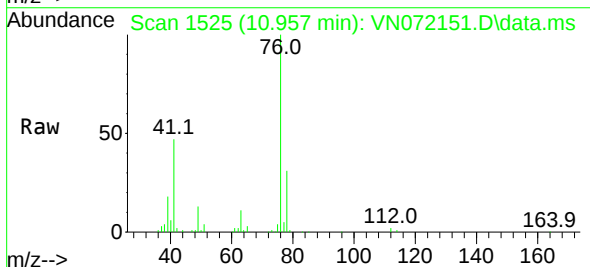





#58
2-Chloroethyl Vinyl ether
Concen: 91.065 ug/l
RT: 9.898 min Scan# 11
Delta R.T. -0.136 min
Lab File: VN072151.D
Acq: 22 Apr 2022 12:59

Instrument :
MSVOA_N
ClientSampleId :
VN0422WBS02

Tgt Ion: 63 Resp: 15559
Ion Ratio Lower Upper
63 100
106 31.8 24.6 36.8



Manual Integrations
APPROVED

Reviewed By :John
Carlone






04/25/2022
Supervised By :Mahesh
Dadoda


04/25/2022



#59
2-Hexanone
Concen: 93.073 ug/l
RT: 11.010 min Scan# 1534
Delta R.T. -0.071 min
Lab File: VN072151.D
Acq: 22 Apr 2022 12:59


Tgt Ion: 43 Resp: 371955
Ion Ratio Lower Upper
43 100
58 63.8 29.7 89.1

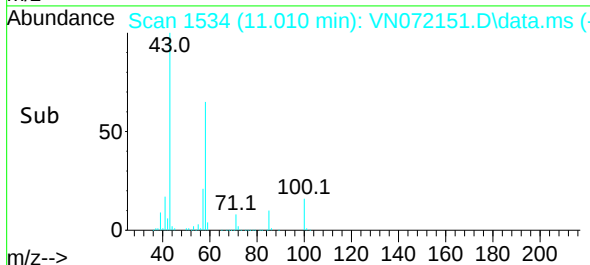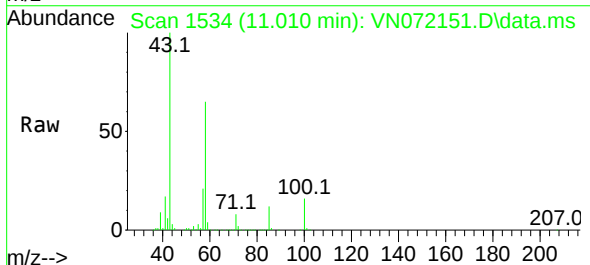



#60
Dibromochloromethane
Concen: 21.866 ug/l
RT: 11.157 min Scan# 1559
Delta R.T. -0.076 min
Lab File: VN072151.D
Acq: 22 Apr 2022 12:59



Instrument :
MSVOA_N
ClientSampleId :
VN0422WBS02



Tgt Ion:129 Resp: 95019
Ion Ratio Lower Upper
129 100
127 77.4 38.8 116.4


Manual Integrations
APPROVED

Reviewed By :John
Carlone




04/25/2022
Supervised By :Mahesh
Dadoda



04/25/2022




#61
1,2-Dibromoethane
Concen: 20.702 ug/l
RT: 11.269 min Scan# 1578
Delta R.T. -0.070 min
Lab File: VN072151.D
Acq: 22 Apr 2022 12:59

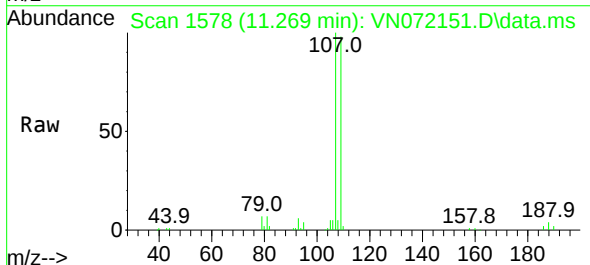

Tgt Ion:107 Resp: 90821
Ion Ratio Lower Upper
107 100
109 95.2 75.0 112.6

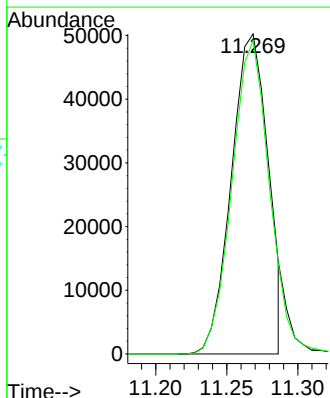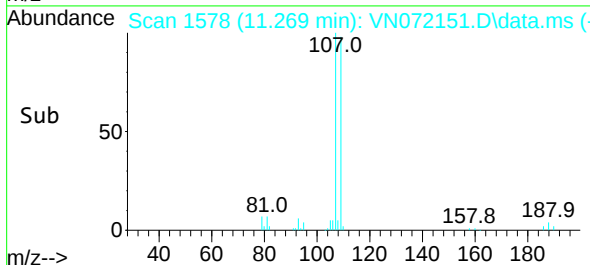

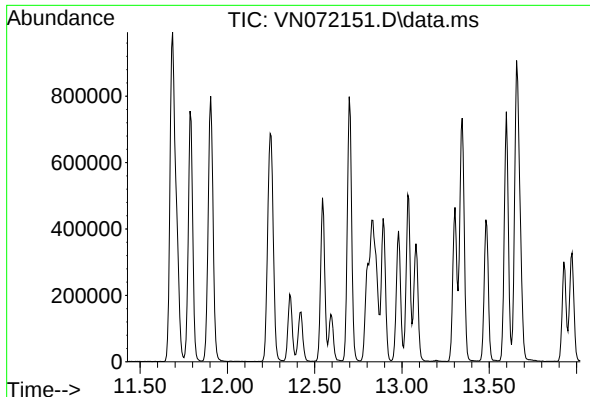

#62
4-Bromofluorobenzene
Concen: 0.000 ug/l
Expected RT: 12.73 min


Lab File: VN072151.D
Acq: 22 Apr 2022 12:59

Instrument :
MSVOA_N
ClientSampleId :
VN0422WBS02

Tgt Ion: 95
Sig Exp Ratio
95 100
174 83.8
176 81.7


Manual Integrations
APPROVED

Reviewed By :John
Carlone

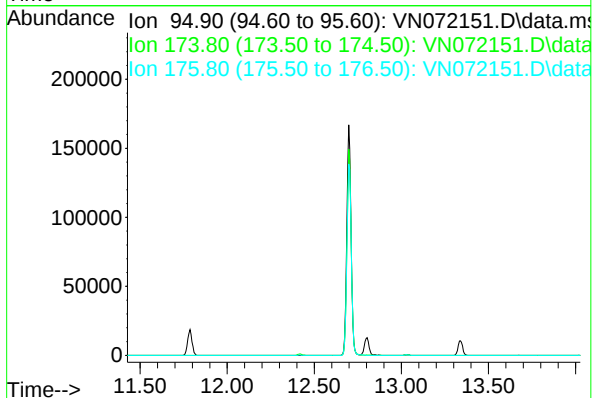

04/25/2022
Supervised By :Mahesh
Dadoda


04/25/2022

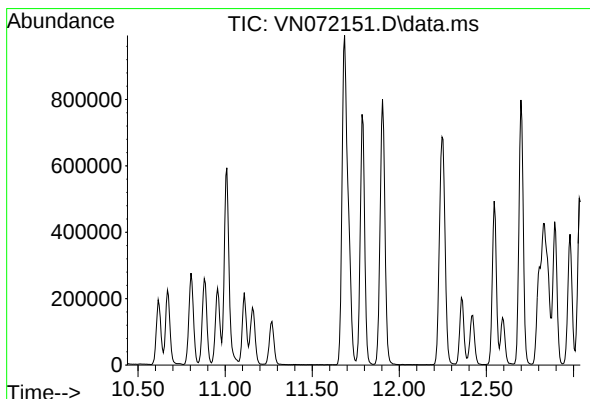


#63
Chlorobenzene-d5
Concen: 0.000 ug/l
Expected RT: 11.74 min

Lab File: VN072151.D
Acq: 22 Apr 2022 12:59


Tgt Ion: 117
Sig Exp Ratio
117 100
82 55.2
119 31.7

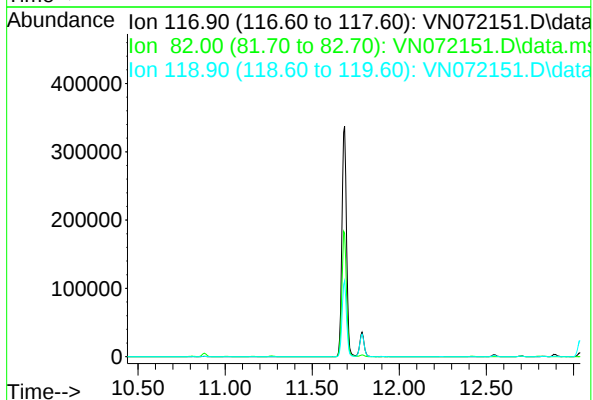



#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.657 min Scan# 1984
Delta R.T. -0.012 min
Lab File: VN072151.D
Acq: 22 Apr 2022 12:59



Instrument :
MSVOA_N
ClientSampleId :
VN0422WBS02



Tgt Ion:152 Resp: 249549
Ion Ratio Lower Upper
152 100
115 54.4 28.9 86.7
150 163.3 0.0 356.2


Manual Integrations
APPROVED

Reviewed By :John
Carlone




04/25/2022
Supervised By :Mahesh
Dadoda



04/25/2022




#73
Isopropylbenzene
Concen: 16.123 ug/l
RT: 12.545 min Scan# 1795
Delta R.T. -0.030 min
Lab File: VN072151.D
Acq: 22 Apr 2022 12:59




Tgt Ion:105 Resp: 339038
Ion Ratio Lower Upper
105 100
120 27.2 13.5 40.4

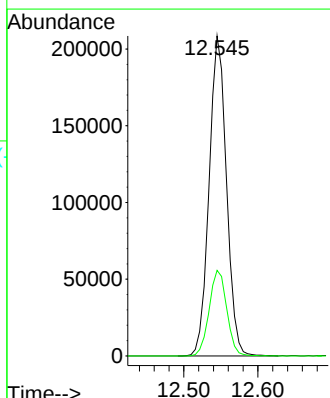



#74
N-amy1 acetate
Concen: 17.448 ug/l
RT: 12.357 min Scan# 1763
Delta R.T. -0.023 min
Lab File: VN072151.D
Acq: 22 Apr 2022 12:59



Instrument :
MSVOA_N
ClientSampleId :
VN0422WBS02

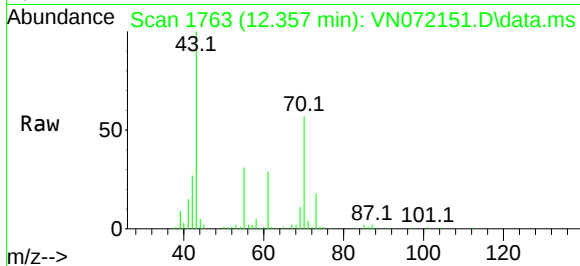

Tgt Ion: 43 Resp: 105128
Ion Ratio Lower Upper
43 100
70 54.0 39.0 58.4
55 30.6 21.1 31.7
61 28.6 21.1 31.7


Manual Integrations
APPROVED

Reviewed By :John
Carlone

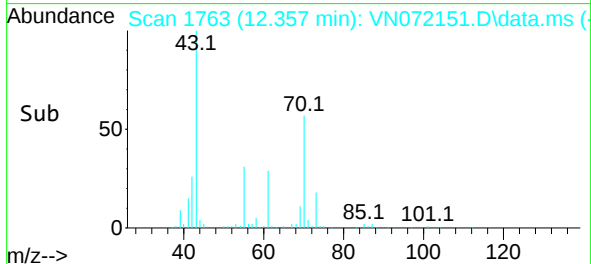


04/25/2022
Supervised By :Mahesh
Dadoda



04/25/2022




#75
1,1,2,2-Tetrachloroethane
Concen: 19.906 ug/l
RT: 12.798 min Scan# 1838
Delta R.T. -0.024 min
Lab File: VN072151.D
Acq: 22 Apr 2022 12:59

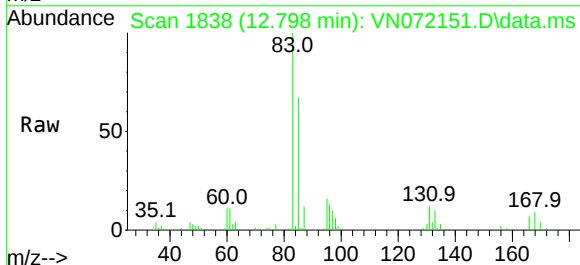

Tgt Ion: 83 Resp: 139668
Ion Ratio Lower Upper
83 100
131 11.1 5.3 15.9
85 65.4 32.3 96.9

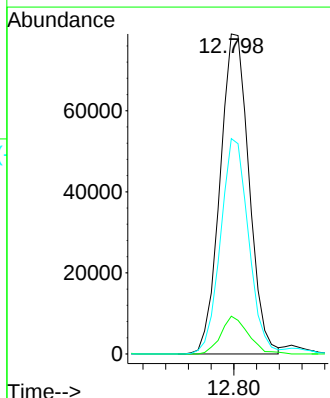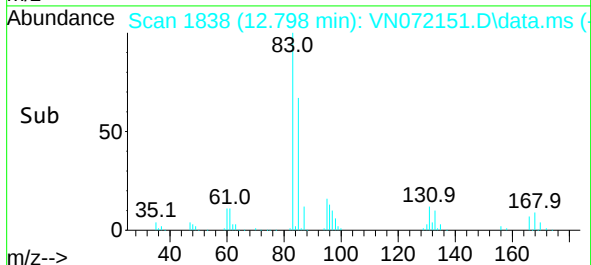



#76

1,2,3-Trichloropropane

Concen: 20.612 ug/l m

RT: 12.851 min Scan# 1847

Delta R.T. -0.023 min

Lab File: VN072151.D

Acq: 22 Apr 2022 12:59

Instrument :

MSVOA_N

ClientSampleId :

VN0422WBS02

Tgt Ion: 75 Resp: 119154

Ion Ratio Lower Upper



75 100

77 0.0 98.5 295.5

Manual Integrations



APPROVED

Reviewed By :John
Carlone



04/25/2022
Supervised By :Mahesh
Dadoda

04/25/2022



#77

Bromobenzene

Concen: 18.393 ug/l

RT: 12.827 min Scan# 1843

Delta R.T. -0.024 min

Lab File: VN072151.D

Acq: 22 Apr 2022 12:59




Tgt Ion:156 Resp: 96958


Ion Ratio Lower Upper

156 100

77 194.6 100.5 301.5

158 97.1 48.9 146.6

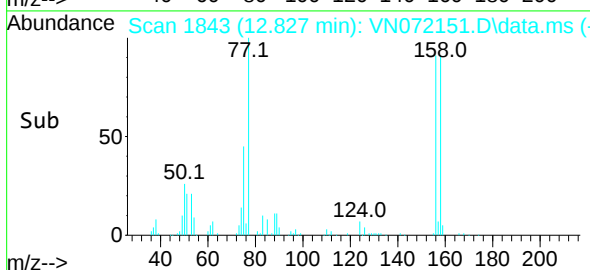



#78

n-propylbenzene

Concen: 16.041 ug/l

RT: 12.892 min Scan# 1854

Delta R.T. -0.024 min

Lab File: VN072151.D

Acq: 22 Apr 2022 12:59

Instrument :

MSVOA_N

ClientSampleId :

VN0422WBS02

Tgt Ion: 91 Resp: 35482

Ion Ratio Lower Upper



91 100

120 24.0 11.9 35.5

Manual Integrations



APPROVED

Reviewed By :John
Carlone



04/25/2022
Supervised By :Mahesh
Dadoda

04/25/2022



#79

2-Chlorotoluene

Concen: 16.911 ug/l

RT: 12.980 min Scan# 1869

Delta R.T. -0.024 min

Lab File: VN072151.D




Acq: 22 Apr 2022 12:59


Tgt Ion: 91 Resp: 239897

Ion Ratio Lower Upper

91 100


126 35.7 17.3 51.9

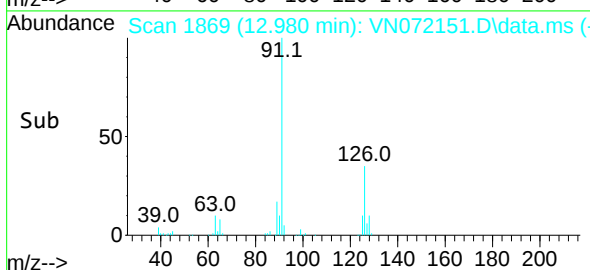

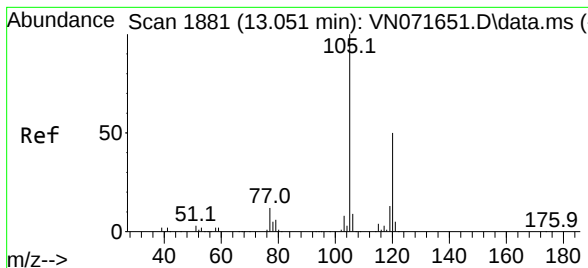

#80
1,3,5-Trimethylbenzene
Concen: 17.274 ug/l
RT: 13.039 min Scan# 11
Delta R.T. -0.012 min
Lab File: VN072151.D
Acq: 22 Apr 2022 12:59



Instrument :
MSVOA_N
ClientSampleId :
VN0422WBS02

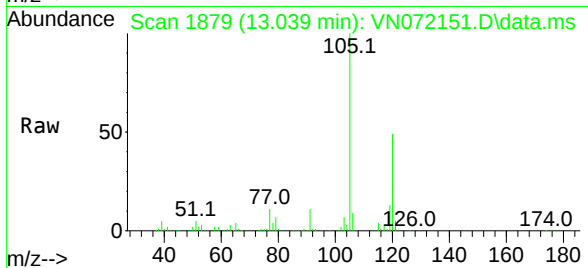

Tgt Ion:105 Resp: 287799
Ion Ratio Lower Upper
105 100
120 51.6 24.9 74.7


Manual Integrations
APPROVED

Reviewed By :John
Carlone

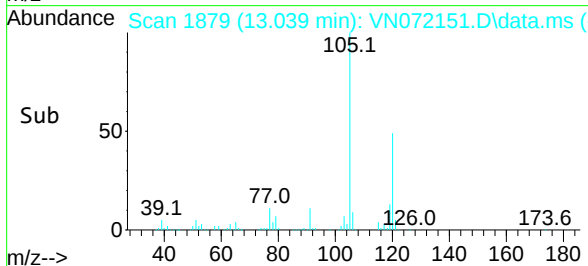




04/25/2022
Supervised By :Mahesh
Dadoda


04/25/2022

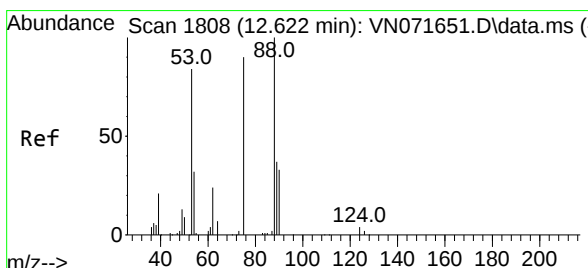

#81
trans-1,4-Dichloro-2-butene
Concen: 18.947 ug/l
RT: 12.592 min Scan# 1803
Delta R.T. -0.030 min
Lab File: VN072151.D
Acq: 22 Apr 2022 12:59

Tgt Ion: 75 Resp: 35345
Ion Ratio Lower Upper
75 100
53 92.6 78.0 117.0
89 46.3 37.2 55.8

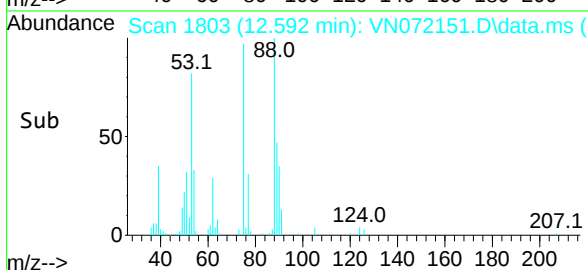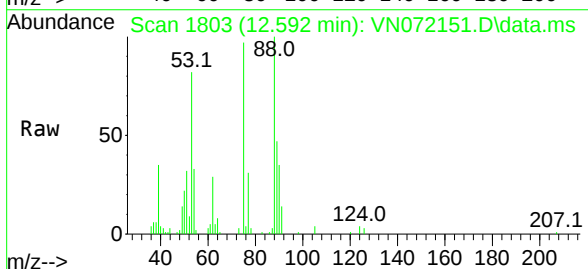





#82
4-Chlorotoluene
Concen: 17.032 ug/l
RT: 13.080 min Scan# 1889
Delta R.T. -0.018 min
Lab File: VN072151.D
Acq: 22 Apr 2022 12:59

Instrument :
MSVOA_N
ClientSampleId :
VN0422WBS02

Tgt Ion: 91 Resp: 22396
Ion Ratio Lower Upper
91 100
126 36.0 17.2 51.6



Manual Integrations
APPROVED

Reviewed By :John
Carlone






04/25/2022
Supervised By :Mahesh
Dadoda


04/25/2022



#83
tert-Butylbenzene
Concen: 16.004 ug/l
RT: 13.304 min Scan# 1924
Delta R.T. -0.012 min
Lab File: VN072151.D
Acq: 22 Apr 2022 12:59


Tgt Ion:119 Resp: 243747
Ion Ratio Lower Upper
119 100
91 60.9 31.6 94.8
134 28.1 13.7 41.1

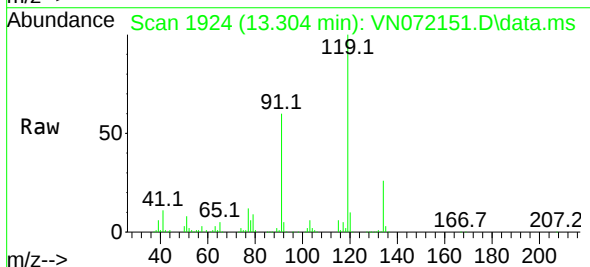



#84
1,2,4-Trimethylbenzene
Concen: 17.977 ug/l
RT: 13.345 min Scan# 1931
Delta R.T. -0.018 min
Lab File: VN072151.D
Acq: 22 Apr 2022 12:59



Instrument :
MSVOA_N
ClientSampleId :
VN0422WBS02



Tgt Ion:105 Resp: 292249
Ion Ratio Lower Upper
105 100
120 46.2 23.3 69.8


Manual Integrations
APPROVED

Reviewed By :John
Carlone

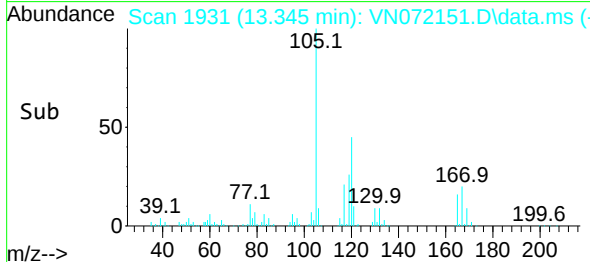


04/25/2022
Supervised By :Mahesh
Dadoda



04/25/2022




#85
sec-Butylbenzene
Concen: 15.609 ug/l
RT: 13.480 min Scan# 1954
Delta R.T. -0.018 min
Lab File: VN072151.D
Acq: 22 Apr 2022 12:59

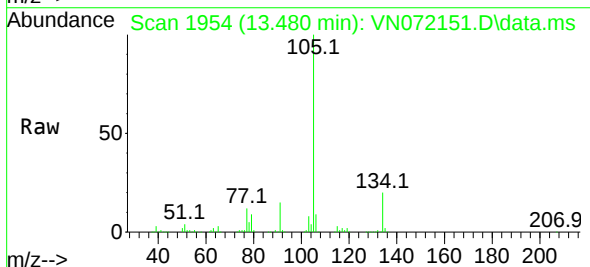

Tgt Ion:105 Resp: 308163
Ion Ratio Lower Upper
105 100
134 21.5 10.4 31.1

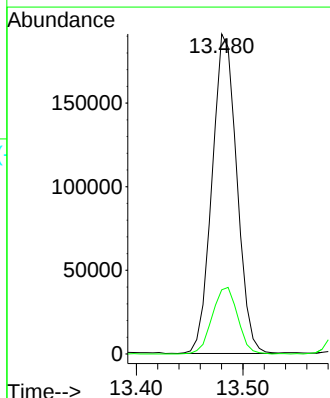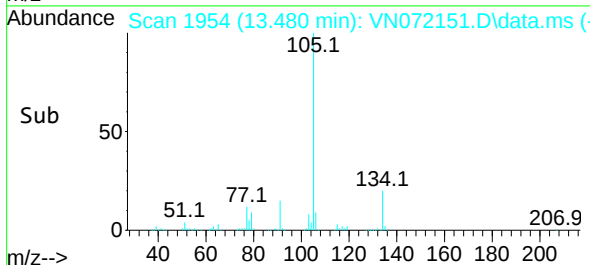





#86
p-Isopropyltoluene
Concen: 16.244 ug/l
RT: 13.598 min Scan# 1974
Delta R.T. -0.012 min
Lab File: VN072151.D
Acq: 22 Apr 2022 12:59

Instrument :
MSVOA_N
ClientSampleId :
VN0422WBS02

Tgt Ion:119 Resp: 25570
Ion Ratio Lower Upper
119 100
134 27.0 13.3 39.8
91 22.0 11.3 33.9



Manual Integrations
APPROVED

Reviewed By :John
Carlone

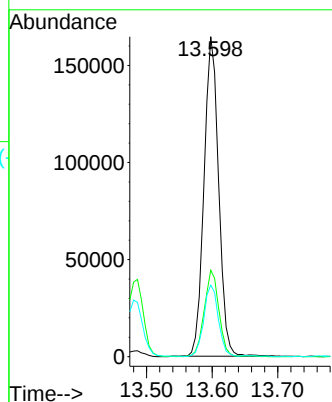




04/25/2022
Supervised By :Mahesh
Dadoda


04/25/2022



#87
1,3-Dichlorobenzene
Concen: 17.715 ug/l
RT: 13.598 min Scan# 1974
Delta R.T. -0.012 min
Lab File: VN072151.D
Acq: 22 Apr 2022 12:59

Tgt Ion:146 Resp: 148775
Ion Ratio Lower Upper
146 100
111 39.5 20.0 60.0
148 64.4 32.0 96.0

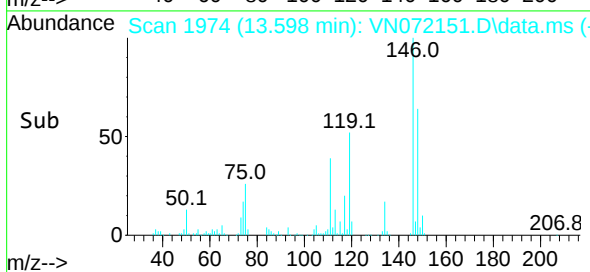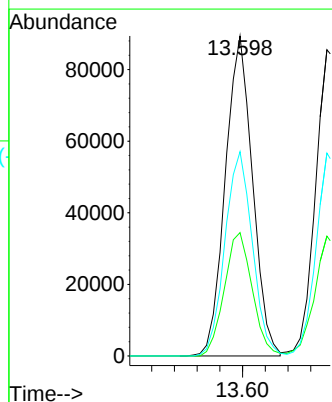





#88
1,4-Dichlorobenzene
Concen: 17.680 ug/l
RT: 13.674 min Scan# 1989
Delta R.T. -0.012 min
Lab File: VN072151.D
Acq: 22 Apr 2022 12:59

Instrument :
MSVOA_N
ClientSampleId :
VN0422WBS02

Tgt Ion:146 Resp: 14485
Ion Ratio Lower Upper
146 100
111 38.7 19.1 57.1
148 65.2 31.4 94.3



Manual Integrations
APPROVED

Reviewed By :John
Carlone






04/25/2022
Supervised By :Mahesh
Dadoda


04/25/2022



#89
n-Butylbenzene
Concen: 14.620 ug/l
RT: 13.927 min Scan# 2030
Delta R.T. -0.012 min
Lab File: VN072151.D
Acq: 22 Apr 2022 12:59


Tgt Ion: 91 Resp: 170700
Ion Ratio Lower Upper
91 100
92 53.5 26.9 80.7
134 27.6 13.6 40.8

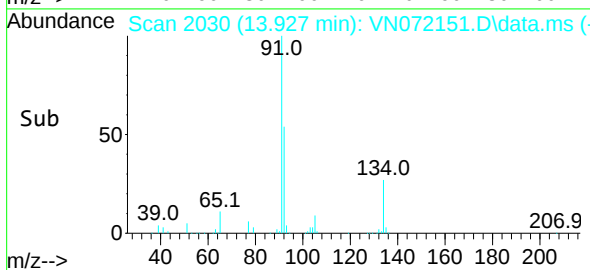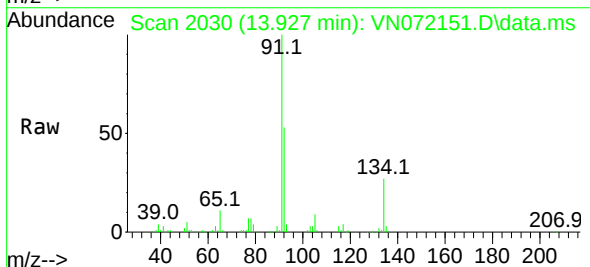



#90
Hexachloroethane
Concen: 16.782 ug/l
RT: 14.198 min Scan# 2076
Delta R.T. -0.006 min
Lab File: VN072151.D
Acq: 22 Apr 2022 12:59



Instrument :
MSVOA_N
ClientSampleId :
VN0422WBS02



Tgt Ion:117 Resp: 4836
Ion Ratio Lower Upper
117 100
201 87.6 40.6 122.0


Manual Integrations
APPROVED

Reviewed By :John
Carlone

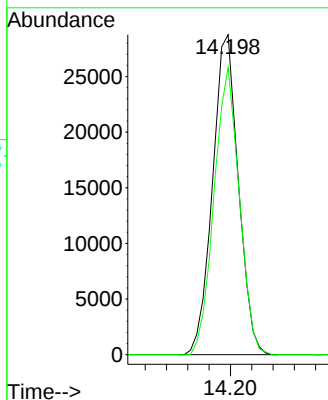


04/25/2022
Supervised By :Mahesh
Dadoda



04/25/2022




#91
1,2-Dichlorobenzene
Concen: 18.519 ug/l
RT: 13.974 min Scan# 2038
Delta R.T. -0.006 min
Lab File: VN072151.D
Acq: 22 Apr 2022 12:59

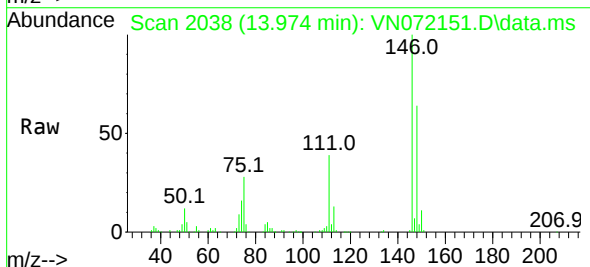


Tgt Ion:146 Resp: 152684
Ion Ratio Lower Upper
146 100
111 40.0 20.9 62.8
148 64.2 32.1 96.3

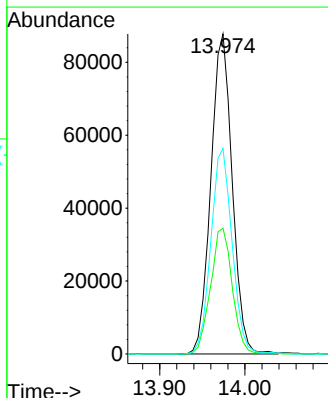



#92
 1,2-Dibromo-3-Chloropropane
 Concen: 18.957 ug/l
 RT: 14.592 min Scan# 2143
 Delta R.T. -0.006 min
 Lab File: VN072151.D
 Acq: 22 Apr 2022 12:59



Instrument :
 MSVOA_N
 ClientSampleId :
 VN0422WBS02



Tgt Ion: 75 Resp: 2063
 Ion Ratio Lower Upper
 75 100
 155 95.2 44.9 134.5
 157 117.8 59.0 176.8


Manual Integrations
 APPROVED

Reviewed By :John
 Carlone






04/25/2022
 Supervised By :Mahesh
 Dadoda


04/25/2022



#93
 1,2,4-Trichlorobenzene
 Concen: 16.991 ug/l
 RT: 15.257 min Scan# 2256
 Delta R.T. -0.000 min
 Lab File: VN072151.D
 Acq: 22 Apr 2022 12:59


Tgt Ion:180 Resp: 61772
 Ion Ratio Lower Upper
 180 100
 182 98.5 47.5 142.5
 145 28.9 14.5 43.5

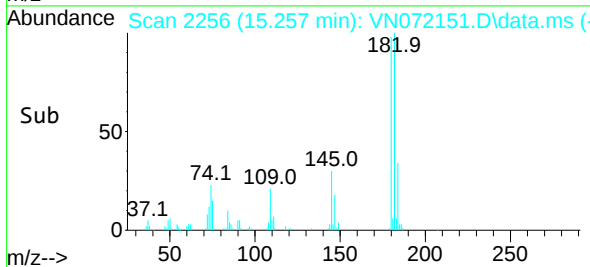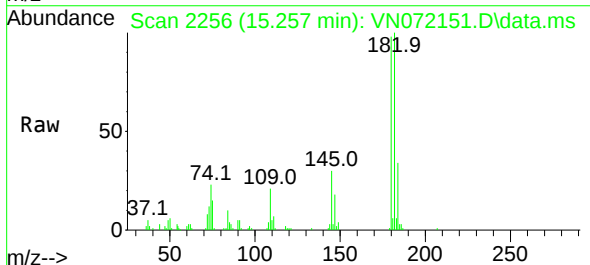



#94
Hexachlorobutadiene
Concen: 15.647 ug/l
RT: 15.362 min Scan# 2274
Delta R.T. -0.001 min
Lab File: VN072151.D
Acq: 22 Apr 2022 12:59



Instrument :
MSVOA_N
ClientSampleId :
VN0422WBS02



Tgt Ion:225 Resp: 38044
Ion Ratio Lower Upper
225 100
223 64.2 32.4 97.2
227 64.5 31.8 95.4


Manual Integrations
APPROVED

Reviewed By :John
Carlone






04/25/2022
Supervised By :Mahesh
Dadoda


04/25/2022



#95
Naphthalene
Concen: 16.848 ug/l
RT: 15.498 min Scan# 2297
Delta R.T. -0.000 min
Lab File: VN072151.D
Acq: 22 Apr 2022 12:59


Tgt Ion:128 Resp: 160444
Ion Ratio Lower Upper
128 100
127 12.4 10.3 15.5
129 11.2 8.6 13.0

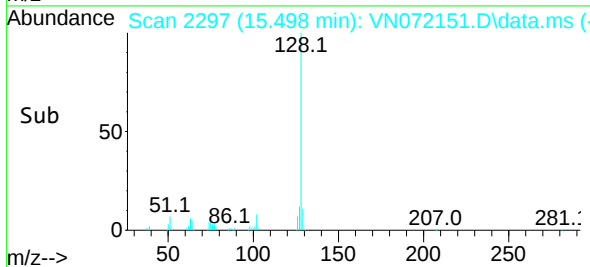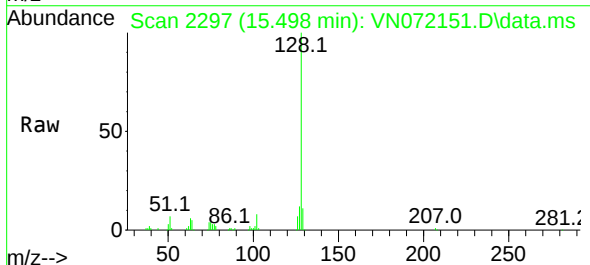



#96
 1,2,3-Trichlorobenzene
 Concen: 18.542 ug/l
 RT: 15.692 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: VN072151.D
 Acq: 22 Apr 2022 12:59



Instrument :
 MSVOA_N
 ClientSampleId :
 VN0422WBS02



Tgt Ion	Ratio	Lower	Upper
180	100		
182	92.4	47.8	143.3
145	30.7	15.5	46.5

Manual Integrations
APPROVED

Reviewed By :John
 Carlone



04/25/2022
 Supervised By :Mahesh
 Dadoda

04/25/2022