


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN042319\
 Data File : VN055191.D
 Acq On : 23 Apr 2019 8:43
 Operator : JC/SP
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N042219W.M
 Title : SW846 8260
 Last Update : Tue Apr 23 05:52:53 2019

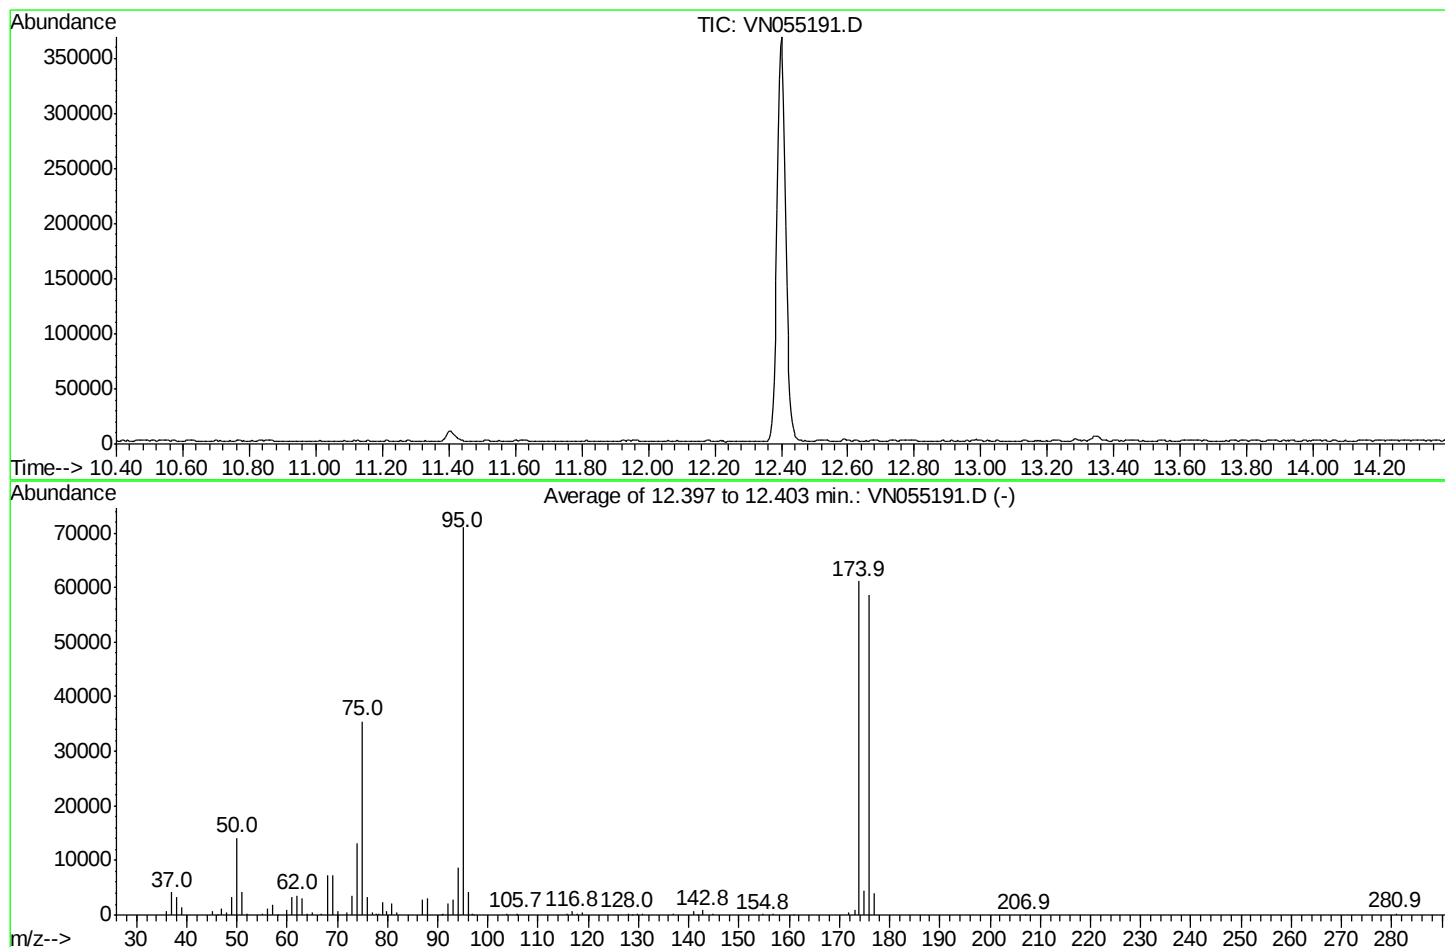

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3290

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.9	14116	PASS
75	95	30	60	49.9	35461	PASS
95	95	100	100	100.0	71032	PASS
96	95	5	9	5.8	4145	PASS
173	174	0.00	2	1.7	1038	PASS
174	95	50	100	86.2	61210	PASS
175	174	5	9	7.1	4359	PASS
176	174	95	101	95.9	58728	PASS
177	176	5	9	6.9	4033	PASS