

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN042321\
 Data File : VN066739.D
 Acq On : 23 Apr 2021 15:49
 Operator : JC/MD
 Sample : M2102-05
 Misc : 9.36g/5mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Apr 23 16:47:15 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N042121W.M
 Quant Title : SW846 8260
 QLast Update : Thu Apr 22 08:25:55 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.583	168	308464	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.514	114	473889	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.348	117	440198	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.290	152	210189	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	7.948	65	177185	47.02	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	94.04%
35) Dibromofluoromethane	7.508	113	144860	48.81	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	97.62%
50) Toluene-d8	10.026	98	574992	49.68	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	99.36%
62) 4-Bromofluorobenzene	12.349	95	202801	51.17	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	102.34%


Target Compounds						Qvalue
11) Tert butyl alcohol	4.654	59	105	0.22	ug/l #	73
13) Acrolein	3.547	56	986	1.87	ug/l	100
16) Acetone	3.761	43	1204	0.85	ug/l	91
17) Carbon Disulfide	3.954	76	2406	0.25	ug/l #	84
18) Methyl Acetate	4.260	43	3150	0.81	ug/l #	69
20) Methylene Chloride	4.445	84	1336	0.32	ug/l #	93
25) 2-Butanone	6.754	43	449	0.22	ug/l #	46
31) Cyclohexane	7.583	56	5768	0.94	ug/l #	1
36) 1,1-Dichloropropene	7.580	75	21644	4.91	ug/l #	48
38) Carbon Tetrachloride	7.583	117	26467	6.31	ug/l #	17
51) 4-Methyl-2-Pentanone	9.935	43	3094	0.75	ug/l #	59
56) Ethyl methacrylate	10.386	69	48	3.16	ug/l #	84
59) 2-Hexanone	10.748	43	148	16.68	ug/l	72
70) Styrene	11.938	104	791	3.05	ug/l #	59
71) Bromoform	12.354	173	1164	0.47	ug/l #	1
76) 1,2,3-Trichloropropane	12.349	75	92010	20.46	ug/l #	100
79) 2-Chlorotoluene	12.628	91	412	0.97	ug/l	86
81) trans-1,4-Dichloro-2-b...	12.349	75	92010	61.25	ug/l #	13
84) 1,2,4-Trimethylbenzene	12.992	105	2780	0.23	ug/l	96
85) sec-Butylbenzene	13.121	105	3176	0.22	ug/l	88
86) p-Isopropyltoluene	13.245	119	3502	0.30	ug/l #	77
87) 1,3-Dichlorobenzene	13.234	146	1889	0.29	ug/l	97
88) 1,4-Dichlorobenzene	13.234	146	1889	0.27	ug/l	98
89) n-Butylbenzene	13.596	91	2219	0.21	ug/l	87
90) Hexachloroethane	13.821	117	590	0.22	ug/l #	17
91) 1,2-Dichlorobenzene	13.620	146	1473	0.22	ug/l #	82
92) 1,2-Dibromo-3-Chloropr...	14.240	75	572	0.64	ug/l #	1
93) 1,2,4-Trichlorobenzene	14.864	180	5347	3.29	ug/l	97
94) Hexachlorobutadiene	14.948	225	1384	0.67	ug/l	90
95) Naphthalene	15.084	128	29239	4.75	ug/l	97
96) 1,2,3-Trichlorobenzene	15.261	180	7116	3.22	ug/l	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN042321\
Data File : VN066739.D
Acq On : 23 Apr 2021 15:49
Operator : JC/MD
Sample : M2102-05
Misc : 9.36g/5mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :

Quant Time: Apr 23 16:47:15 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N042121W.M
Quant Title : SW846 8260
QLast Update : Thu Apr 22 08:25:55 2021
Response via : Initial Calibration




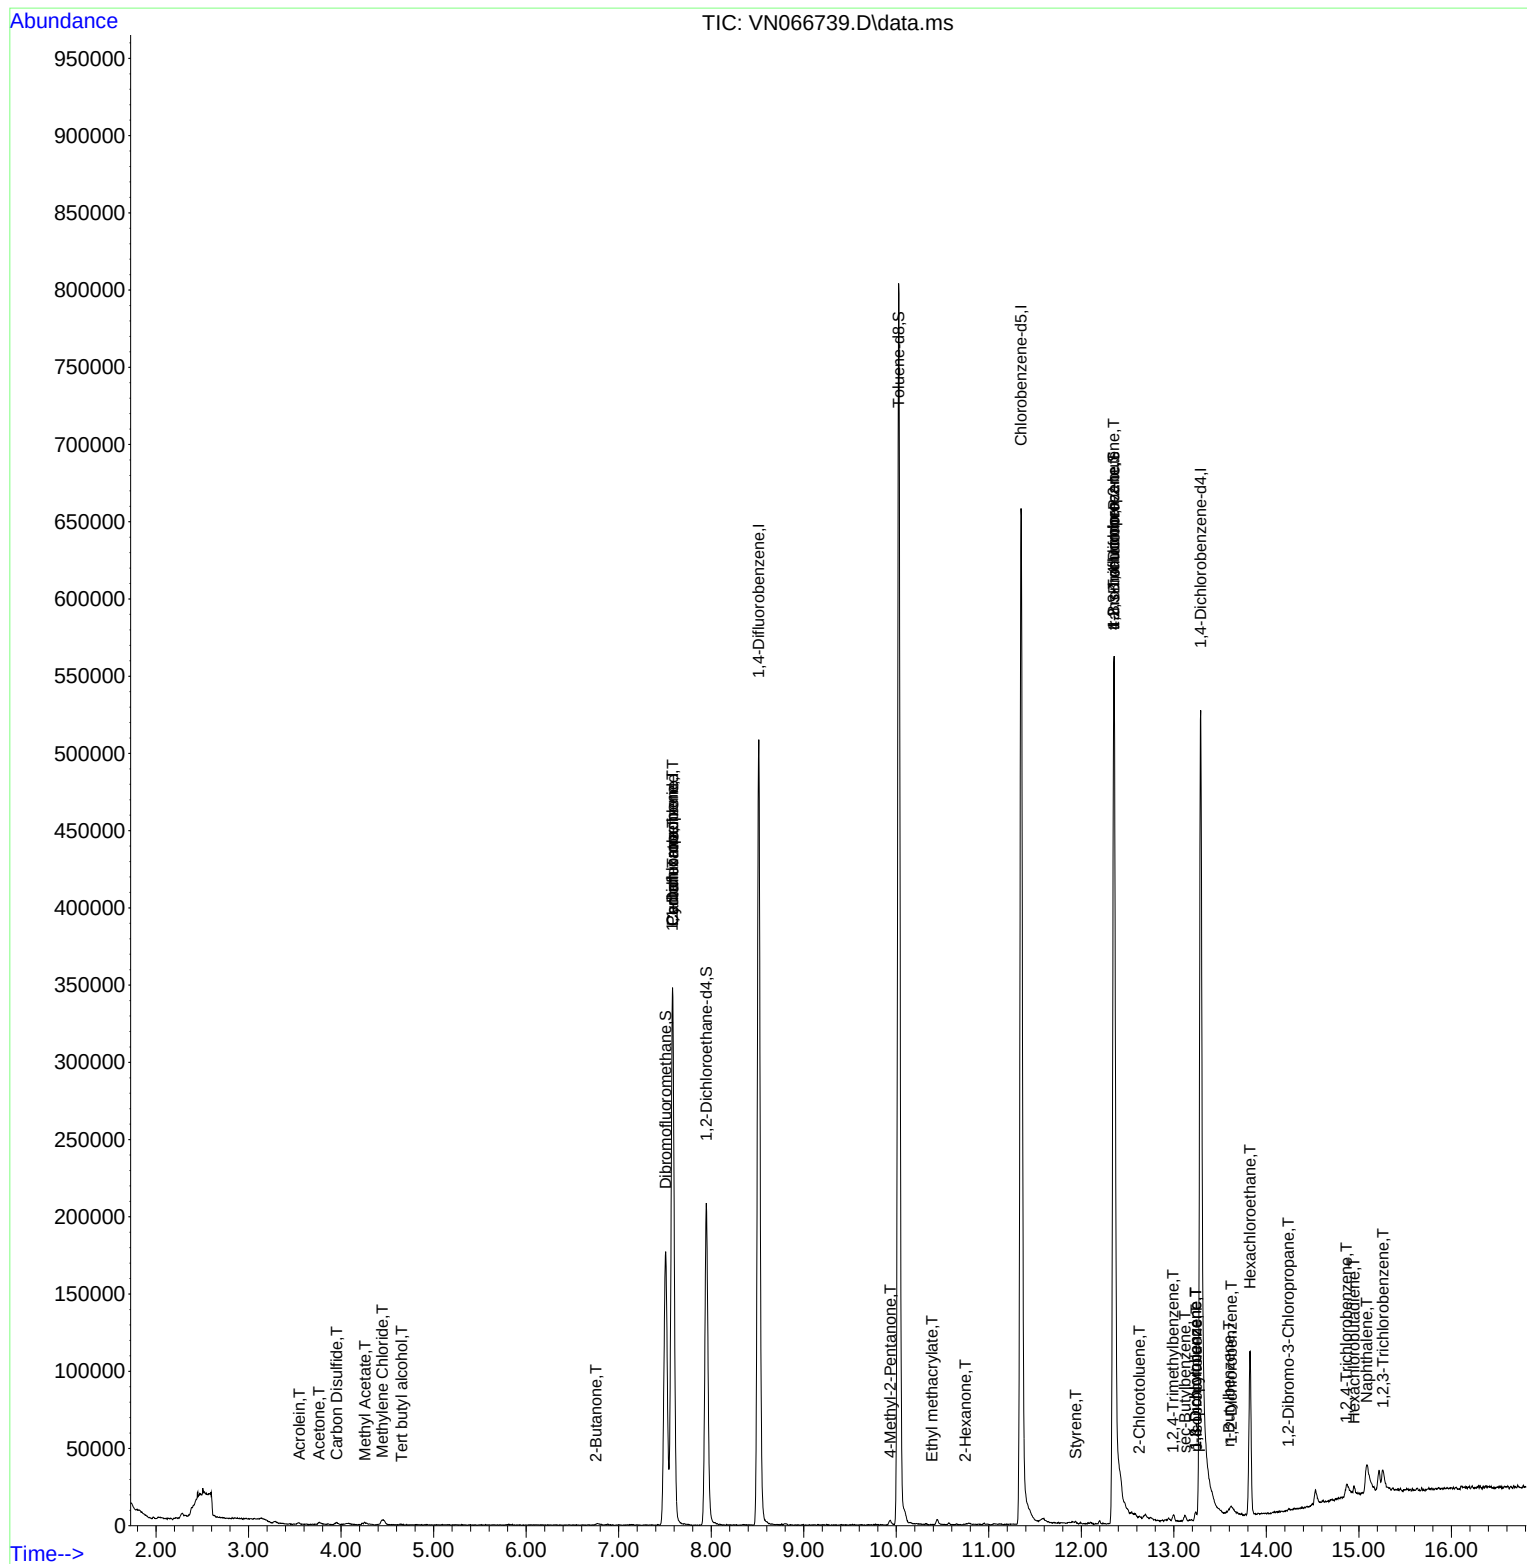


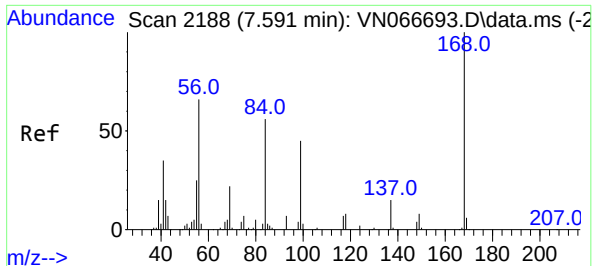

#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 7.583 min Scan# 2185
Delta R.T. -0.008 min
Lab File: VN066739.D
Acq: 23 Apr 2021 15:49




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:168 Resp: 308464
Ion Ratio Lower Upper
168 100
99 50.2 42.6 63.8

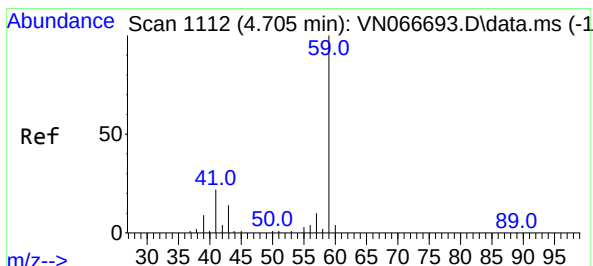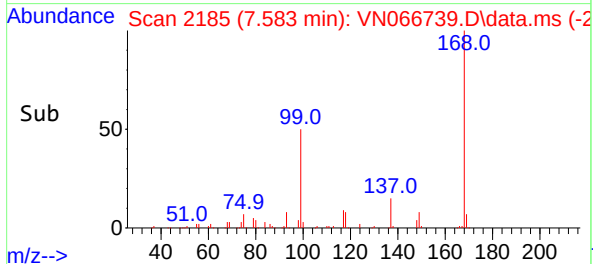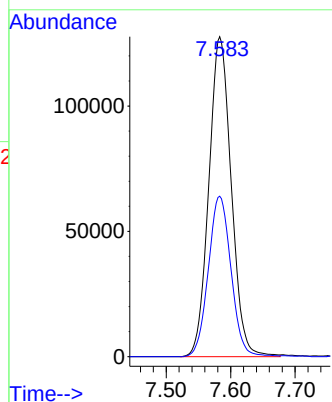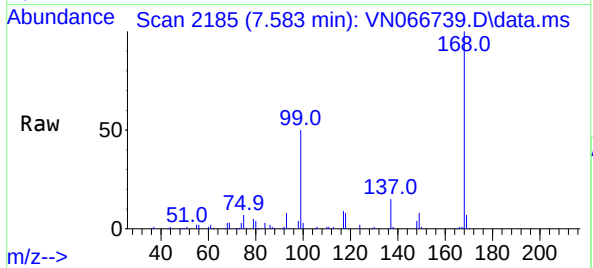

#11
Tert butyl alcohol
Concen: 0.22 ug/l
RT: 4.654 min Scan# 1093
Delta R.T. -0.051 min
Lab File: VN066739.D
Acq: 23 Apr 2021 15:49

Tgt Ion: 59 Resp: 105
Ion Ratio Lower Upper
59 100
57 0.0 8.0 12.0#


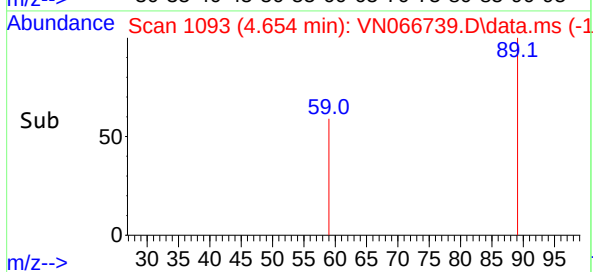
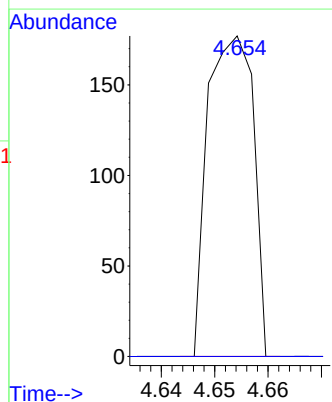
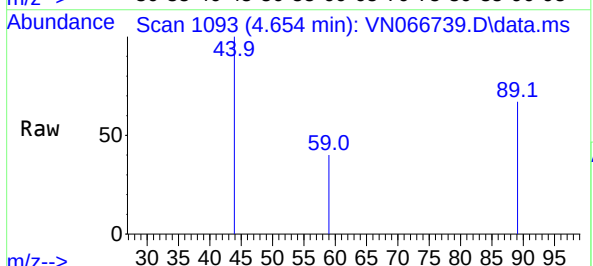




#13
Acrolein
Concen: 1.87 ug/l
RT: 3.547 min Scan# 680
Delta R.T. -0.000 min
Lab File: VN066739.D
Acq: 23 Apr 2021 15:49




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 56 Resp: 986
Ion Ratio Lower Upper
56 100
55 70.2 56.0 84.0

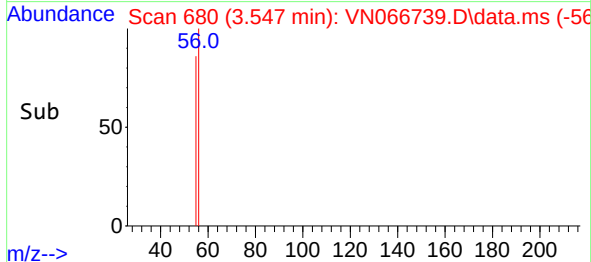

#16
Acetone
Concen: 0.85 ug/l
RT: 3.761 min Scan# 760
Delta R.T. 0.008 min
Lab File: VN066739.D
Acq: 23 Apr 2021 15:49

Tgt Ion: 43 Resp: 1204
Ion Ratio Lower Upper
43 100
58 28.9 27.0 40.6


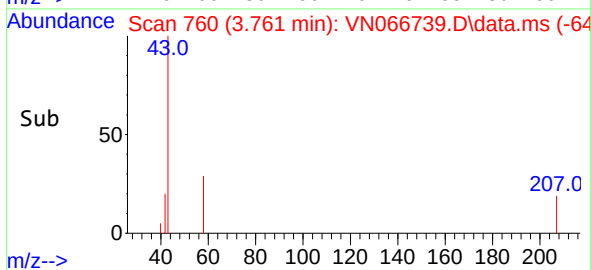




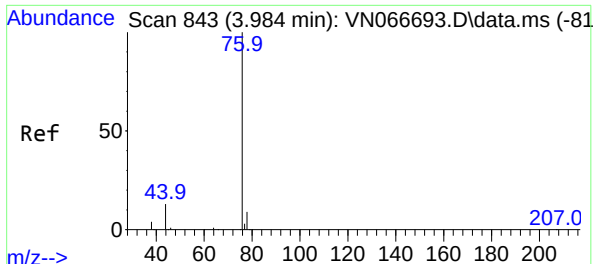

#17
Carbon Disulfide
Concen: 0.25 ug/l
RT: 3.954 min Scan# 832
Delta R.T. -0.030 min
Lab File: VN066739.D
Acq: 23 Apr 2021 15:49




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 76 Resp: 2406
Ion Ratio Lower Upper
76 100
78 15.5 7.8 11.6#

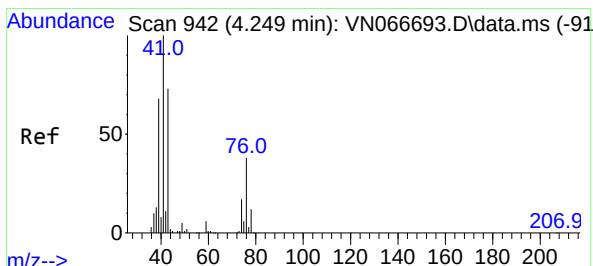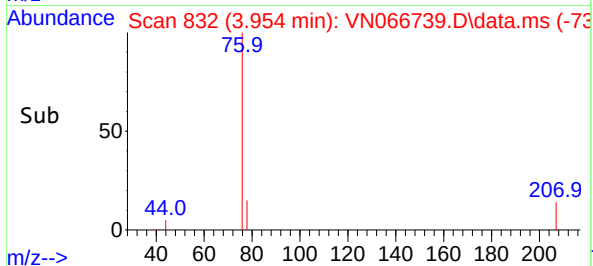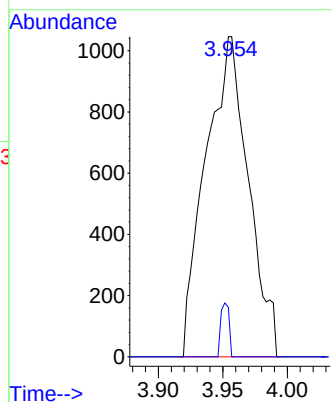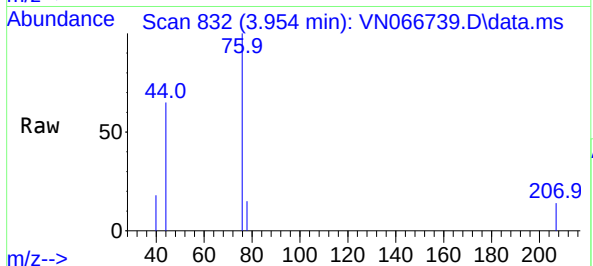

#18
Methyl Acetate
Concen: 0.81 ug/l
RT: 4.260 min Scan# 946
Delta R.T. 0.011 min
Lab File: VN066739.D
Acq: 23 Apr 2021 15:49


Tgt Ion: 43 Resp: 3150
Ion Ratio Lower Upper
43 100
74 8.8 19.5 29.3#

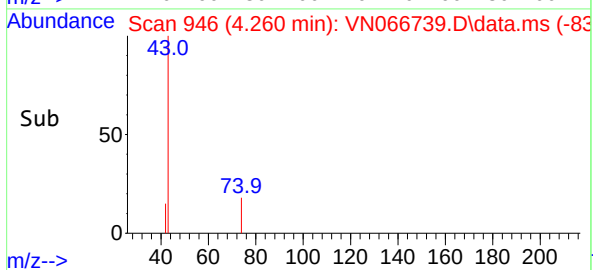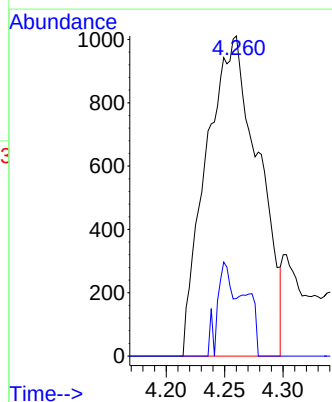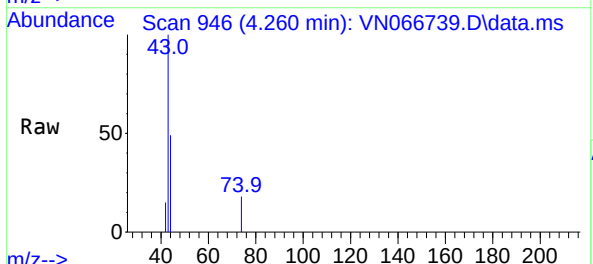






#20
Methylene Chloride
Concen: 0.32 ug/l
RT: 4.445 min Scan# 1015
Delta R.T. -0.024 min
Lab File: VN066739.D
Acq: 23 Apr 2021 15:49


Instrument :
MSVOA_N
ClientSampled :





Tgt Ion: 84 Resp: 1336
Ion Ratio Lower Upper
84 100
49 113.7 94.6 141.8
51 49.2 29.9 44.9#
86 60.4 51.4 77.2

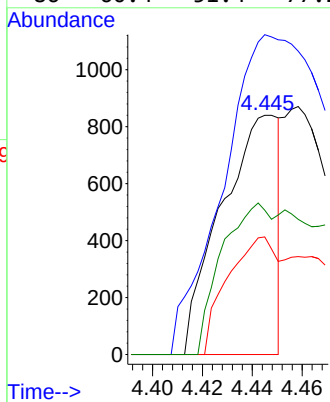


#25
2-Butanone
Concen: 0.22 ug/l
RT: 6.754 min Scan# 1876
Delta R.T. 0.008 min
Lab File: VN066739.D
Acq: 23 Apr 2021 15:49

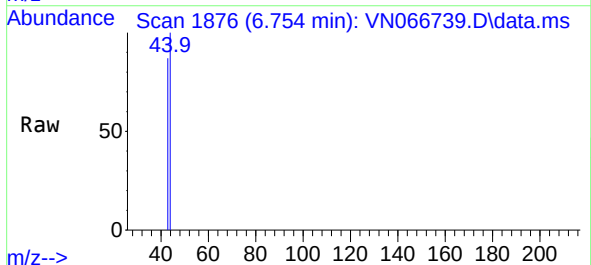

Tgt Ion: 43 Resp: 449
Ion Ratio Lower Upper
43 100
72 0.0 23.1 34.7#




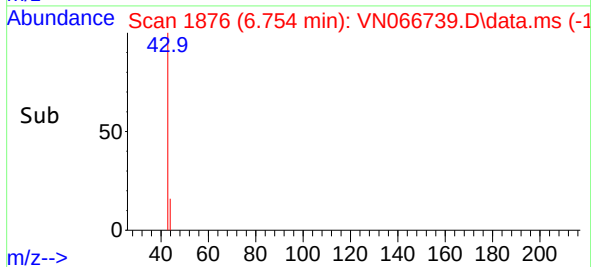




#31
Cyclohexane
Concen: 0.94 ug/l
RT: 7.583 min Scan# 2185
Delta R.T. 0.005 min
Lab File: VN066739.D
Acq: 23 Apr 2021 15:49




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 56 Resp: 5768
Ion Ratio Lower Upper
56 100
69 180.6 26.6 39.8#
84 153.7 70.4 105.6#

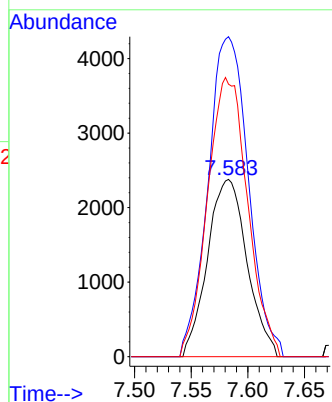

#33
1,2-Dichloroethane-d4
Concen: 47.02 ug/l
RT: 7.948 min Scan# 2321
Delta R.T. -0.005 min
Lab File: VN066739.D
Acq: 23 Apr 2021 15:49

Tgt Ion: 65 Resp: 177185
Ion Ratio Lower Upper
65 100
67 55.3 0.0 107.2

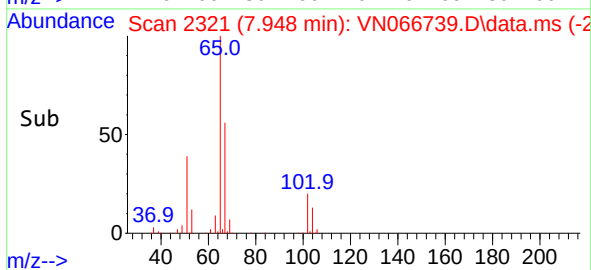




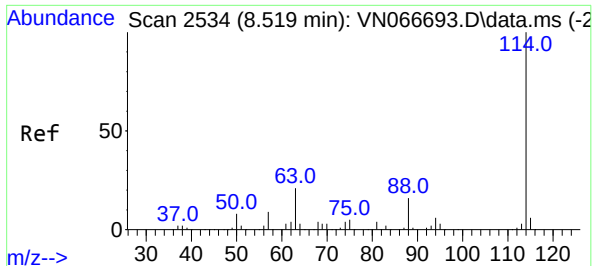


#34

1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 8.514 min Scan# 2532
Delta R.T. -0.005 min
Lab File: VN066739.D
Acq: 23 Apr 2021 15:49

Instrument :
MSVOA_N
ClientSampled :




Tgt Ion:114 Resp: 473889
Ion Ratio Lower Upper
114 100
63 20.9 0.0 38.6
88 15.5 0.0 30.6

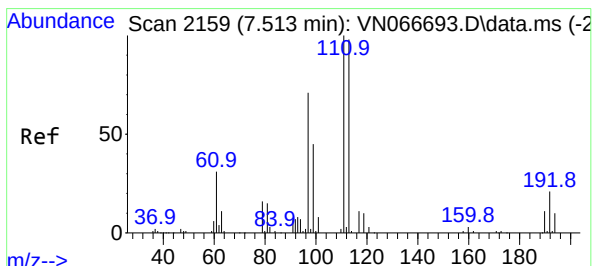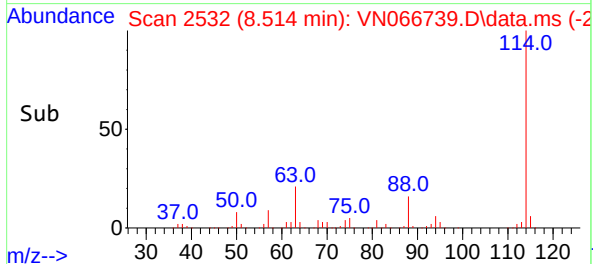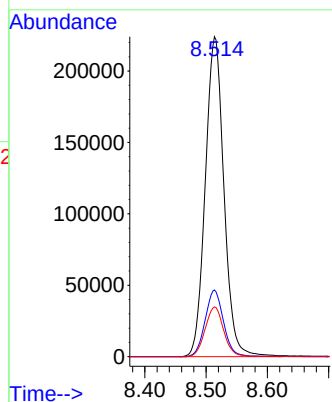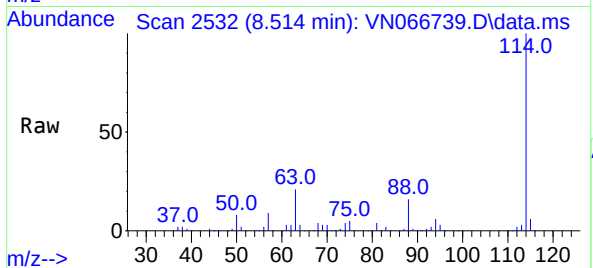


#35

Dibromofluoromethane
Concen: 48.81 ug/l
RT: 7.508 min Scan# 2157
Delta R.T. -0.005 min
Lab File: VN066739.D
Acq: 23 Apr 2021 15:49


Tgt Ion:113 Resp: 144860
Ion Ratio Lower Upper
113 100
111 101.5 82.2 123.2
192 21.2 15.4 23.0

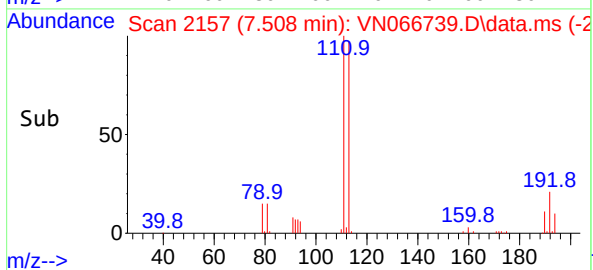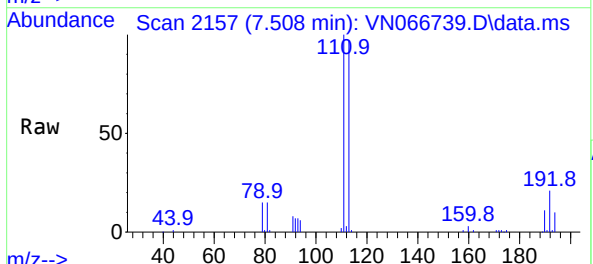






#36
1,1-Dichloropropene
Concen: 4.91 ug/l
RT: 7.580 min Scan# 2184
Delta R.T. -0.137 min
Lab File: VN066739.D
Acq: 23 Apr 2021 15:49


Instrument :
MSVOA_N
ClientSampleId :





Tgt Ion: 75 Resp: 21644
Ion Ratio Lower Upper
75 100
110 7.8 18.2 54.6#
77 0.0 24.9 37.3#

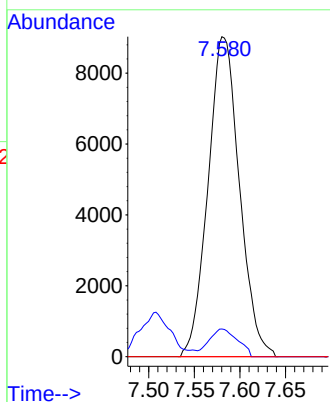


#38
Carbon Tetrachloride
Concen: 6.31 ug/l
RT: 7.583 min Scan# 2185
Delta R.T. -0.115 min
Lab File: VN066739.D
Acq: 23 Apr 2021 15:49



Tgt Ion: 117 Resp: 26467
Ion Ratio Lower Upper
117 100
119 5.5 76.0 114.0#
121 0.0 24.5 36.7#



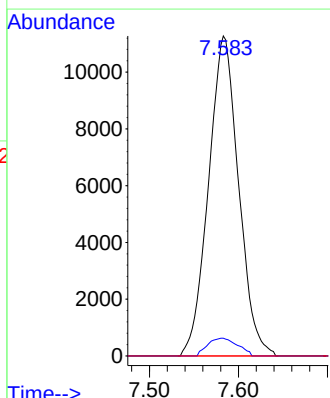





#50
Toluene-d8
Concen: 49.68 ug/l
RT: 10.026 min Scan# 3096
Delta R.T. -0.003 min
Lab File: VN066739.D
Acq: 23 Apr 2021 15:49




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 98 Resp: 574992
Ion Ratio Lower Upper
98 100
100 64.7 50.5 75.7



#51
4-Methyl-2-Pentanone
Concen: 0.75 ug/l
RT: 9.935 min Scan# 3062
Delta R.T. 0.013 min
Lab File: VN066739.D
Acq: 23 Apr 2021 15:49

Tgt Ion: 43 Resp: 3094
Ion Ratio Lower Upper
43 100
58 15.1 32.5 48.7#


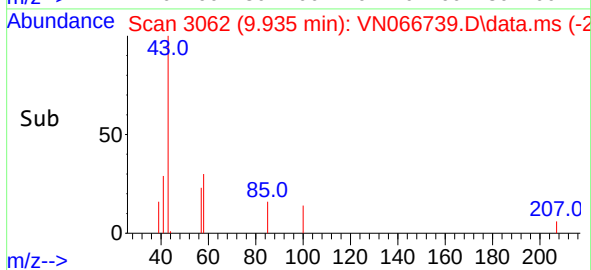






#56
Ethyl methacrylate
Concen: 3.16 ug/l
RT: 10.386 min Scan# 3230
Delta R.T. 0.016 min
Lab File: VN066739.D
Acq: 23 Apr 2021 15:49




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 69 Resp: 48
Ion Ratio Lower Upper
69 100
41 54.2 49.6 74.4
39 50.0 28.0 42.0#

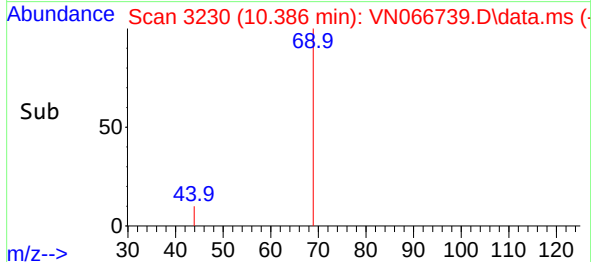

#59
2-Hexanone
Concen: 16.68 ug/l
RT: 10.748 min Scan# 3365
Delta R.T. 0.054 min
Lab File: VN066739.D
Acq: 23 Apr 2021 15:49

Tgt Ion: 43 Resp: 148
Ion Ratio Lower Upper
43 100
58 77.0 28.1 84.3


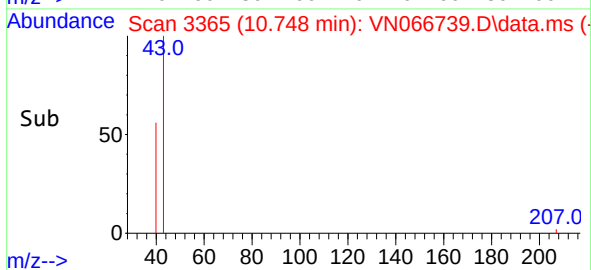






#62
4-Bromofluorobenzene
Concen: 51.17 ug/l
RT: 12.349 min Scan# 3962
Delta R.T. 0.003 min
Lab File: VN066739.D
Acq: 23 Apr 2021 15:49




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 95 Resp: 202801
Ion Ratio Lower Upper
95 100
174 85.2 0.0 169.0
176 81.1 0.0 162.4



#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.348 min Scan# 3589
Delta R.T. -0.001 min
Lab File: VN066739.D
Acq: 23 Apr 2021 15:49


Tgt Ion: 117 Resp: 440198
Ion Ratio Lower Upper
117 100
82 55.6 43.7 65.5
119 32.1 26.1 39.1

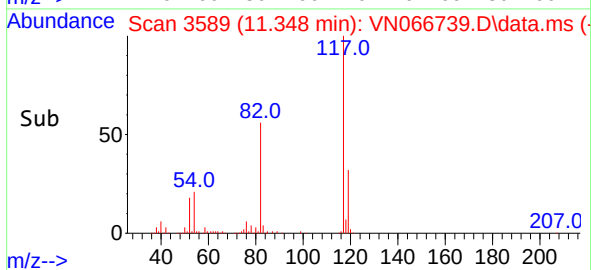






#70
Styrene
Concen: 3.05 ug/l
RT: 11.938 min Scan# 3809
Delta R.T. 0.029 min
Lab File: VN066739.D
Acq: 23 Apr 2021 15:49

Instrument :
MSVOA_N
ClientSampled :







Tgt Ion:104 Resp: 791
Ion Ratio Lower Upper
104 100
78 24.9 39.0 58.4#
103 21.6 44.5 66.7#

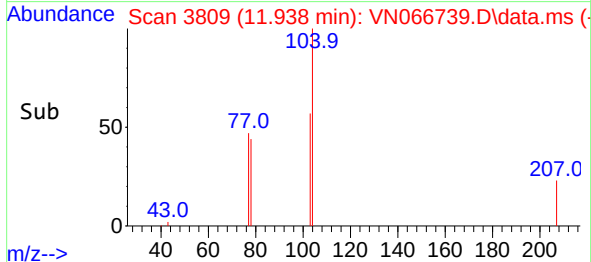

#71
Bromoform
Concen: 0.47 ug/l
RT: 12.354 min Scan# 3964
Delta R.T. 0.281 min
Lab File: VN066739.D
Acq: 23 Apr 2021 15:49

Tgt Ion:173 Resp: 1164
Ion Ratio Lower Upper
173 100
175 771.5 23.8 71.2#
254 0.0 0.0 0.0


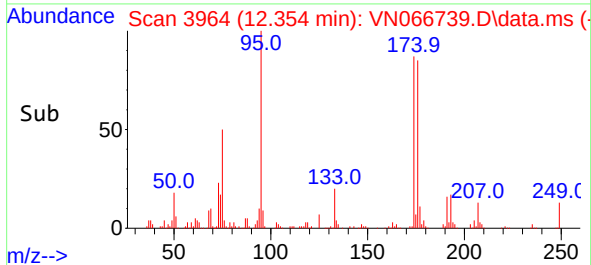

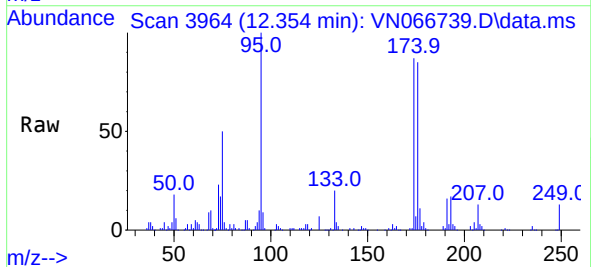




#72
 1,4-Dichlorobenzene-d4
 Concen: 50.00 ug/l
 RT: 13.290 min Scan# 4313
 Delta R.T. 0.002 min
 Lab File: VN066739.D
 Acq: 23 Apr 2021 15:49




Instrument :
 MSVOA_N
 ClientSampled :


Tgt Ion:152 Resp: 210189
 Ion Ratio Lower Upper
 152 100
 115 53.2 28.5 85.6
 150 158.0 0.0 347.6

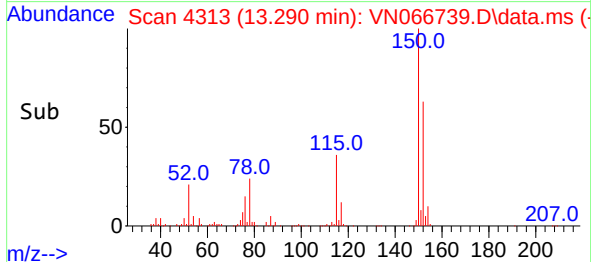

#76
 1,2,3-Trichloropropane
 Concen: 20.46 ug/l
 RT: 12.349 min Scan# 3962
 Delta R.T. -0.147 min
 Lab File: VN066739.D
 Acq: 23 Apr 2021 15:49

Tgt Ion: 75 Resp: 92010
 Ion Ratio Lower Upper
 75 100
 77 1.5 0.0 0.0#


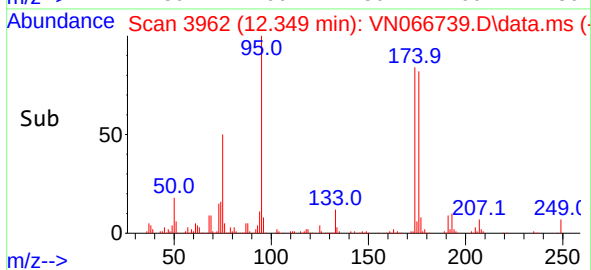




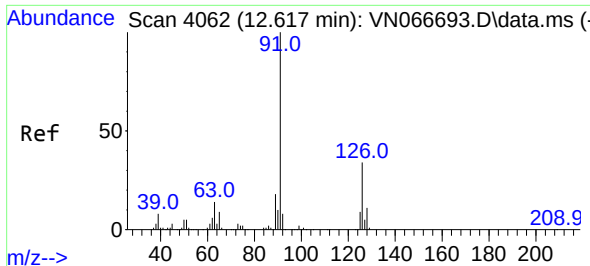

#79
2-Chlorotoluene
Concen: 0.97 ug/l
RT: 12.628 min Scan# 4066
Delta R.T. 0.011 min
Lab File: VN066739.D
Acq: 23 Apr 2021 15:49




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 91 Resp: 412
Ion Ratio Lower Upper
91 100
126 43.0 17.4 52.3

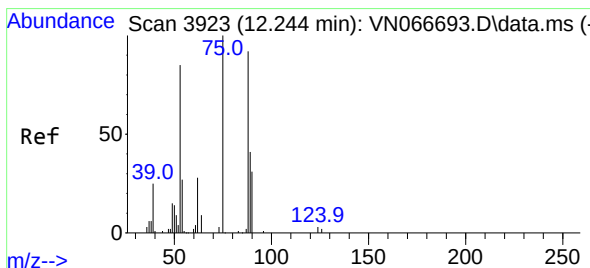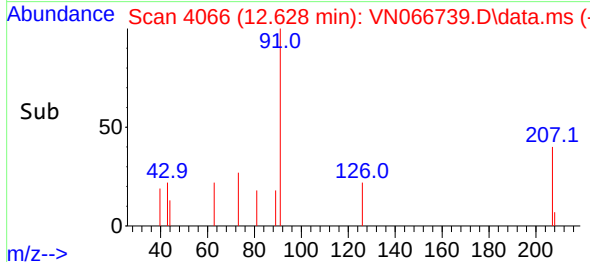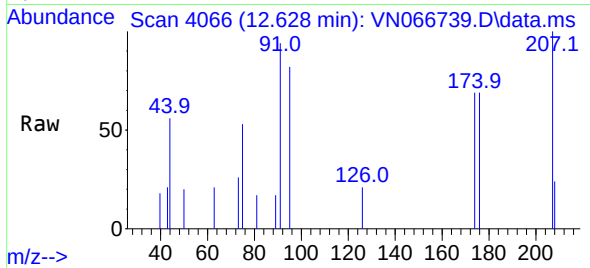

#81
trans-1,4-Dichloro-2-butene
Concen: 61.25 ug/l
RT: 12.349 min Scan# 3962
Delta R.T. 0.105 min
Lab File: VN066739.D
Acq: 23 Apr 2021 15:49





Tgt Ion: 75 Resp: 92010
Ion Ratio Lower Upper
75 100
53 0.0 74.6 111.8#
89 1.6 35.8 53.8#

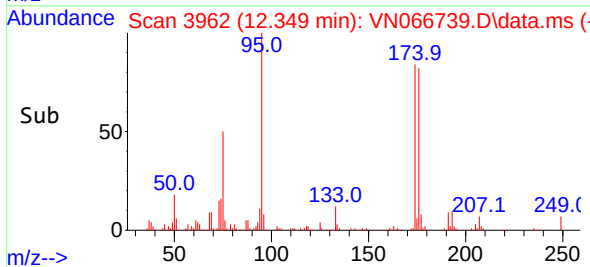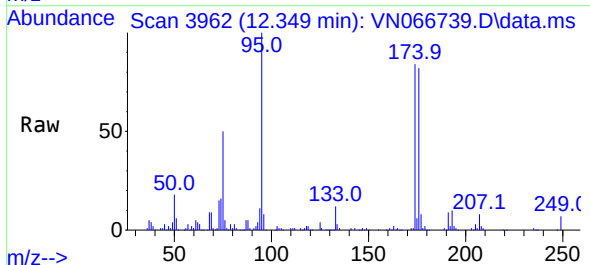






#84
1,2,4-Trimethylbenzene
Concen: 0.23 ug/l
RT: 12.992 min Scan# 4202
Delta R.T. 0.007 min
Lab File: VN066739.D
Acq: 23 Apr 2021 15:49

Tgt Ion:105 Resp: 2780
Ion Ratio Lower Upper
105 100
120 41.9 22.4 67.0

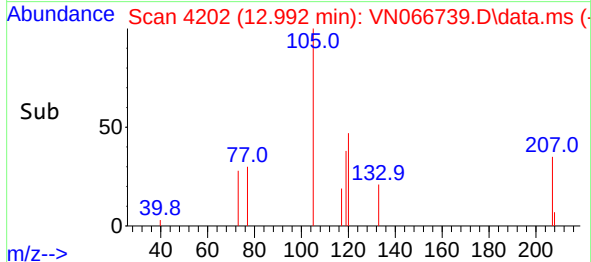


#85
sec-Butylbenzene
Concen: 0.22 ug/l
RT: 13.121 min Scan# 4250
Delta R.T. 0.005 min
Lab File: VN066739.D
Acq: 23 Apr 2021 15:49

Tgt Ion:105 Resp: 3176
Ion Ratio Lower Upper
105 100
134 14.4 10.0 30.0

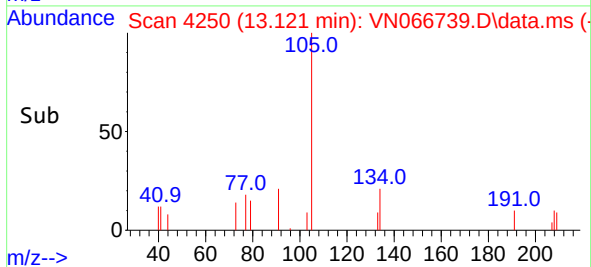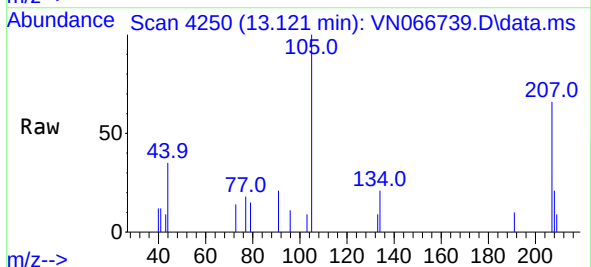





Instrument :
MSVOA_N
ClientSampled :



#86
p-Isopropyltoluene
Concen: 0.30 ug/l
RT: 13.245 min Scan# 4296
Delta R.T. 0.011 min
Lab File: VN066739.D
Acq: 23 Apr 2021 15:49




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:119 Resp: 3502
Ion Ratio Lower Upper
119 100
134 7.1 13.3 39.8#
91 20.6 11.8 35.3

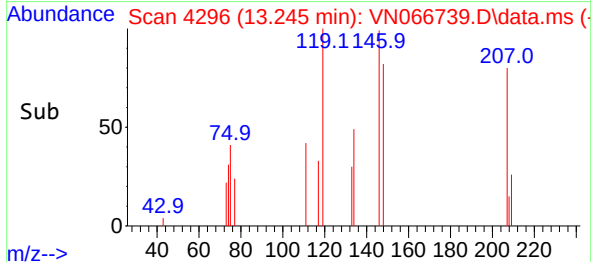

#87
1,3-Dichlorobenzene
Concen: 0.29 ug/l
RT: 13.234 min Scan# 4292
Delta R.T. 0.008 min
Lab File: VN066739.D
Acq: 23 Apr 2021 15:49

Tgt Ion:146 Resp: 1889
Ion Ratio Lower Upper
146 100
111 38.0 19.5 58.5
148 61.4 32.3 96.9


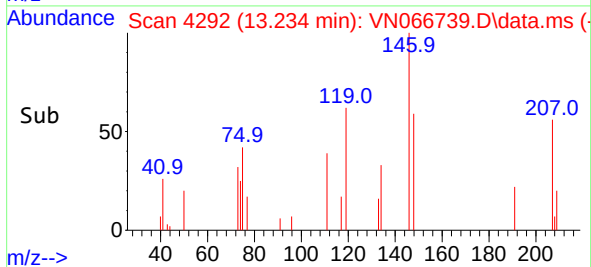

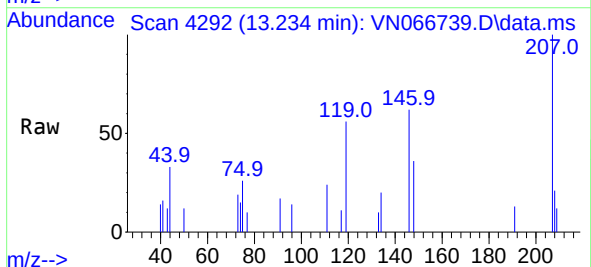




#88
1,4-Dichlorobenzene
Concen: 0.27 ug/l
RT: 13.234 min Scan# 4292
Delta R.T. -0.072 min
Lab File: VN066739.D
Acq: 23 Apr 2021 15:49




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:146 Resp: 1889
Ion Ratio Lower Upper
146 100
111 38.0 19.0 57.0
148 61.4 31.8 95.3

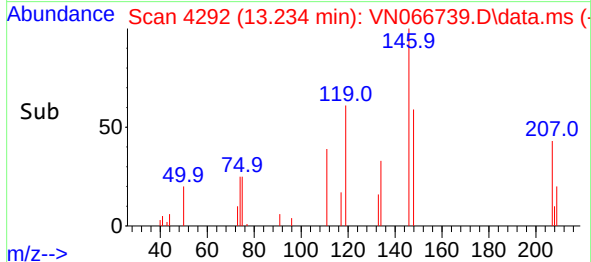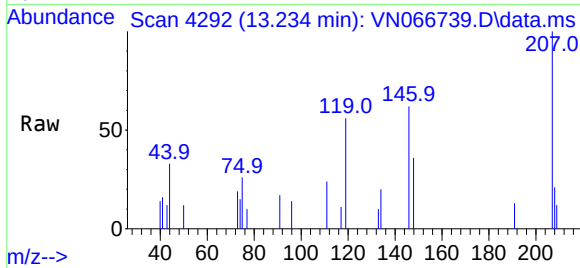

#89
n-Butylbenzene
Concen: 0.21 ug/l
RT: 13.596 min Scan# 4427
Delta R.T. 0.038 min
Lab File: VN066739.D
Acq: 23 Apr 2021 15:49

Tgt Ion: 91 Resp: 2219
Ion Ratio Lower Upper
91 100
92 58.5 26.1 78.3
134 14.5 13.0 38.9


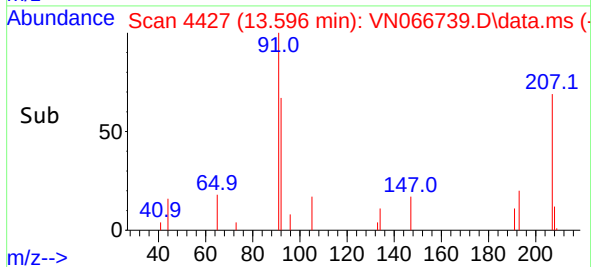

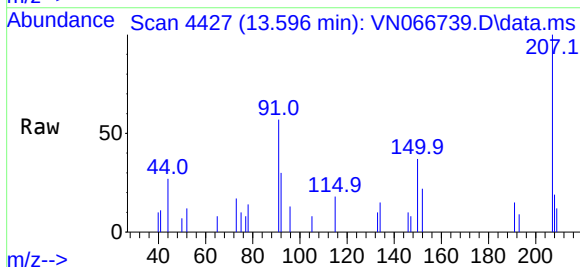




#90
Hexachloroethane
Concen: 0.22 ug/l
RT: 13.821 min Scan# 4511
Delta R.T. 0.005 min
Lab File: VN066739.D
Acq: 23 Apr 2021 15:49




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:117 Resp: 590
Ion Ratio Lower Upper
117 100
201 4.2 37.8 113.3#



#91
1,2-Dichlorobenzene
Concen: 0.22 ug/l
RT: 13.620 min Scan# 4436
Delta R.T. 0.024 min
Lab File: VN066739.D
Acq: 23 Apr 2021 15:49

Tgt Ion:146 Resp: 1473
Ion Ratio Lower Upper
146 100
111 19.8 20.1 60.3#
148 57.4 32.0 96.0


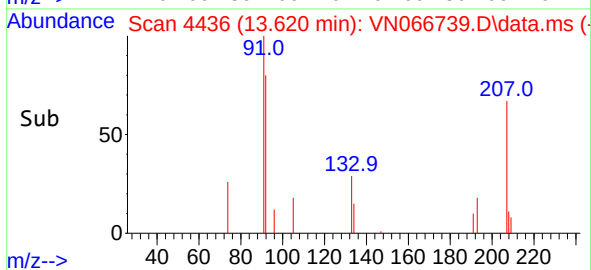




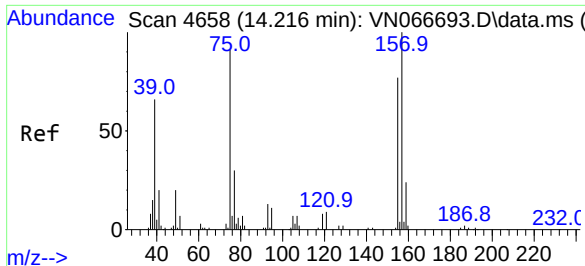

#92
1,2-Dibromo-3-Chloropropane
Concen: 0.64 ug/l
RT: 14.240 min Scan# 4667
Delta R.T. 0.024 min
Lab File: VN066739.D
Acq: 23 Apr 2021 15:49




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 75 Resp: 572
Ion Ratio Lower Upper
75 100
155 0.0 44.1 132.4#
157 0.0 56.0 168.2#

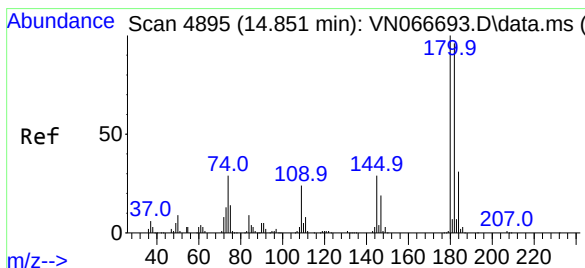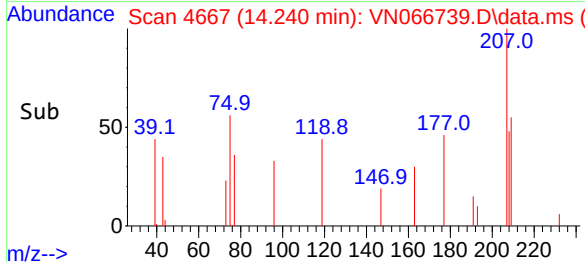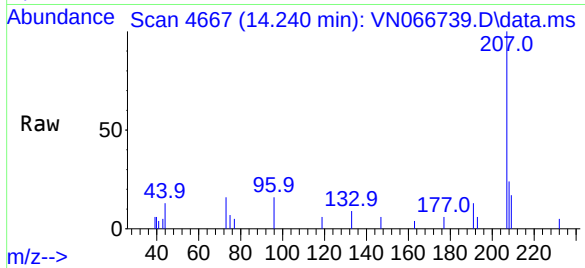

#93
1,2,4-Trichlorobenzene
Concen: 3.29 ug/l
RT: 14.864 min Scan# 4900
Delta R.T. 0.013 min
Lab File: VN066739.D
Acq: 23 Apr 2021 15:49


Tgt Ion: 180 Resp: 5347
Ion Ratio Lower Upper
180 100
182 92.5 47.3 142.0
145 27.7 15.6 46.8

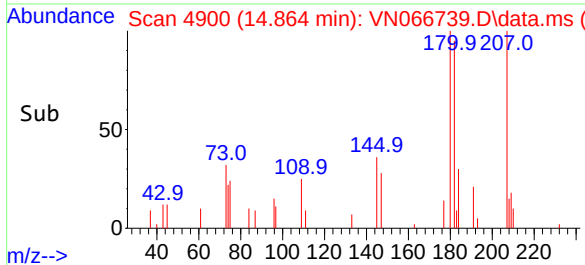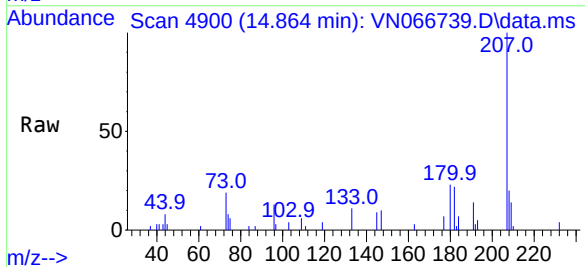






#94
Hexachlorobutadiene
Concen: 0.67 ug/l
RT: 14.948 min Scan# 4931
Delta R.T. -0.000 min
Lab File: VN066739.D
Acq: 23 Apr 2021 15:49


Instrument :
MSVOA_N
ClientSampled :





Tgt Ion:225 Resp: 1384
Ion Ratio Lower Upper
225 100
223 60.0 31.9 95.9
227 51.3 31.6 95.0

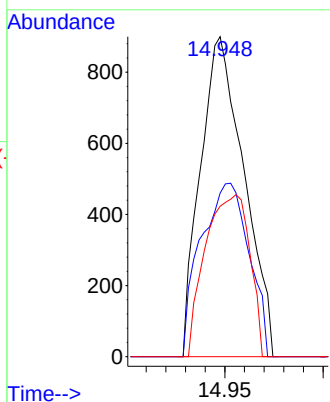


#95
Naphthalene
Concen: 4.75 ug/l
RT: 15.084 min Scan# 4982
Delta R.T. 0.013 min
Lab File: VN066739.D
Acq: 23 Apr 2021 15:49



Tgt Ion:128 Resp: 29239
Ion Ratio Lower Upper
128 100
127 13.8 10.2 15.2
129 9.3 8.6 13.0





#96
 1,2,3-Trichlorobenzene
 Concen: 3.22 ug/l
 RT: 15.261 min Scan# 5048
 Delta R.T. 0.013 min
 Lab File: VN066739.D
 Acq: 23 Apr 2021 15:49

Instrument :
 MSVOA_N
 ClientSampleId :

Tgt Ion:	180	Resp:	7116
Ion	Ratio	Lower	Upper
180	100		
182	92.3	47.4	142.3
145	31.4	16.5	49.5

