


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN042321\
Data File : VN066729.D
Acq On : 23 Apr 2021 10:32
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N042021W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Wed Apr 21 16:55:39 2021

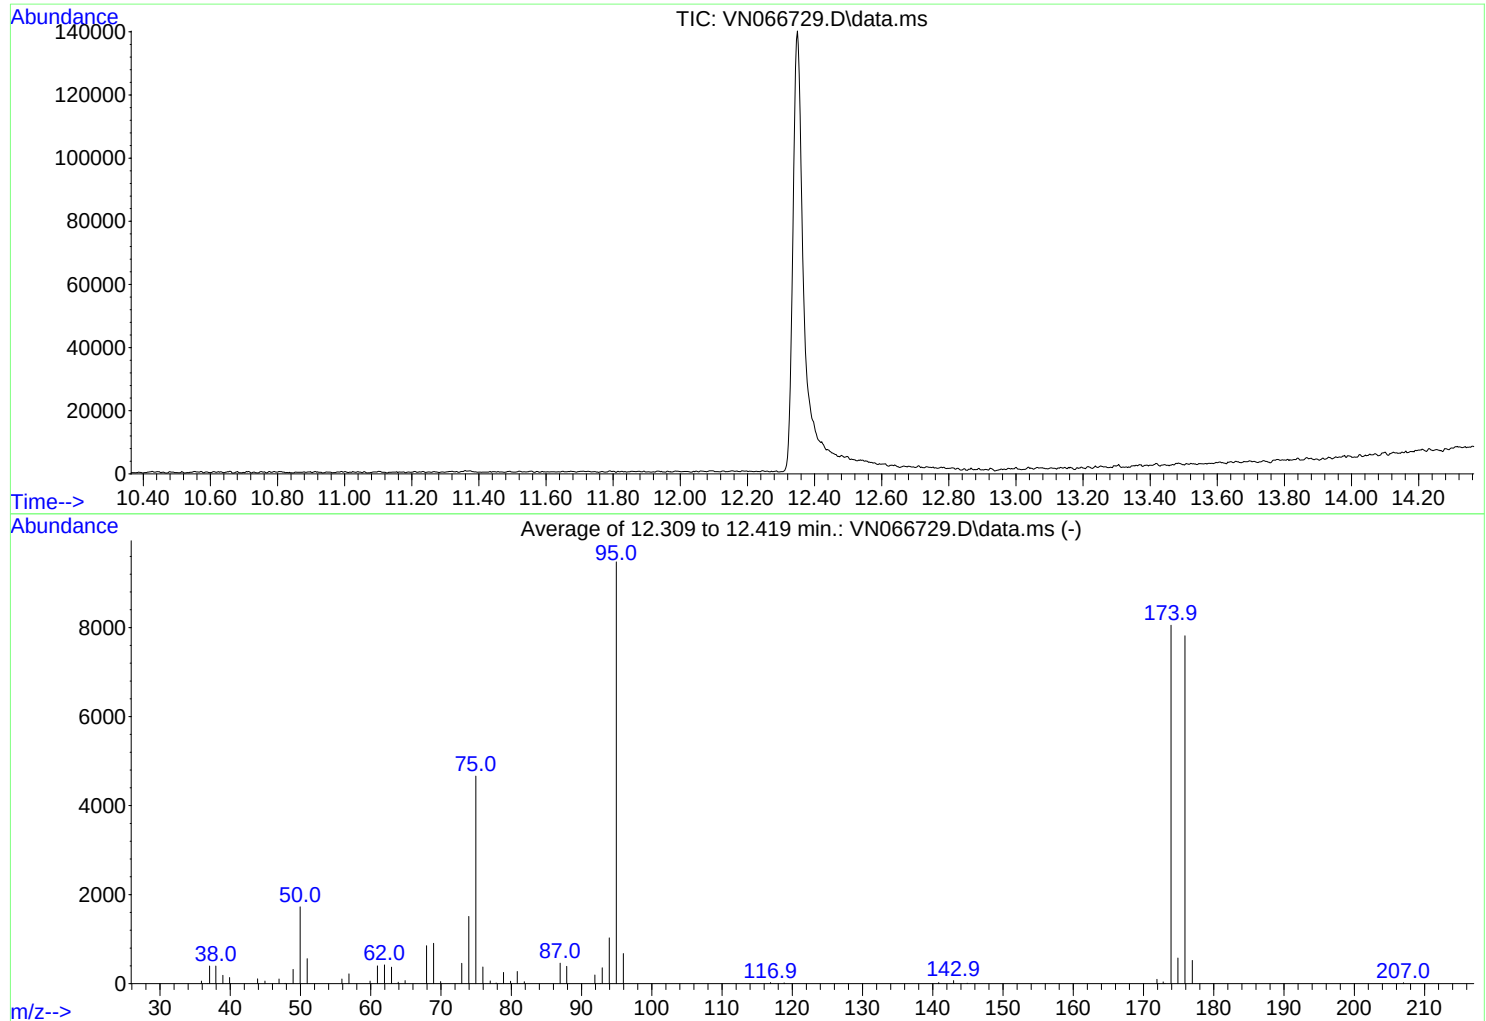

AutoFind: Averaged scan 3947 to 3988; Bkg corrected with scan 3946

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.2	1724	PASS
75	95	30	60	49.2	4663	PASS
95	95	100	100	100.0	9477	PASS
96	95	5	9	7.1	676	PASS
173	174	0.00	2	0.5	40	PASS
174	95	50	100	85.0	8054	PASS
175	174	5	9	7.2	577	PASS
176	174	95	101	97.0	7814	PASS
177	176	5	9	6.7	521	PASS