


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN042321\
Data File : VN066729.D
Acq On : 23 Apr 2021 10:32
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N042121W.M
Title : SW846 8260
Last Update : Thu Apr 22 08:25:55 2021

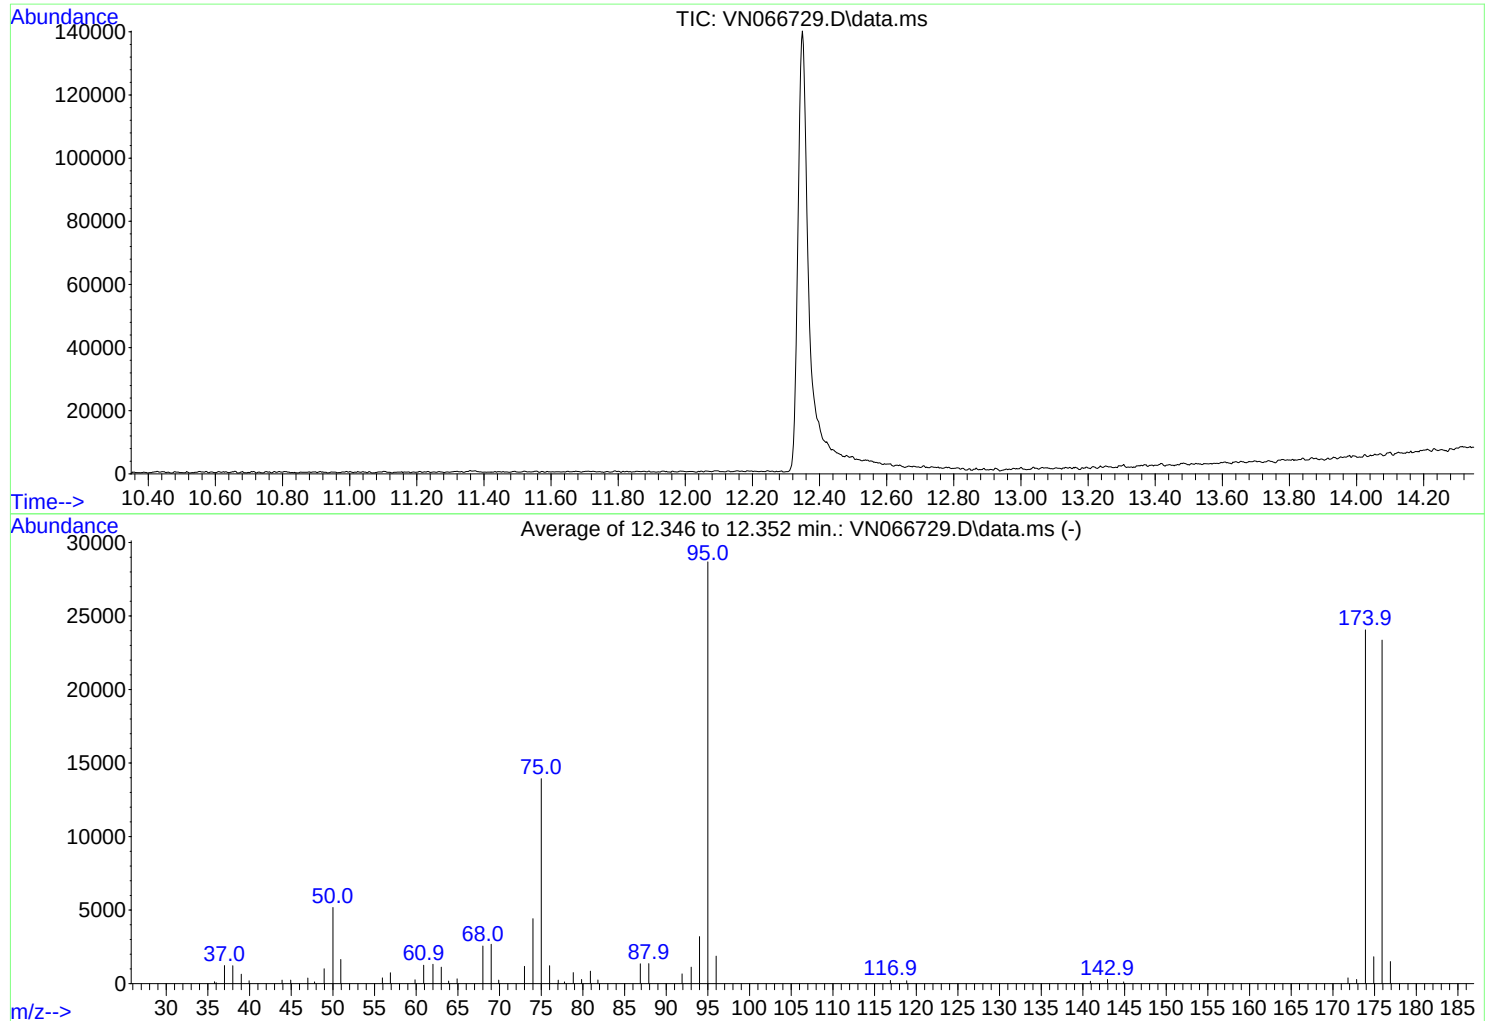

AutoFind: Scans 3961, 3962, 3963; Background Corrected with Scan 3945

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.1	5181	PASS
75	95	30	60	48.6	13933	PASS
95	95	100	100	100.0	28683	PASS
96	95	5	9	6.5	1873	PASS
173	174	0.00	2	1.2	283	PASS
174	95	50	100	83.9	24056	PASS
175	174	5	9	7.6	1823	PASS
176	174	95	101	97.1	23365	PASS
177	176	5	9	6.4	1501	PASS