

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN042321\  
 Data File : VN066736.D  
 Acq On : 23 Apr 2021 14:33  
 Operator : JC/MD  
 Sample : M2150-01  
 Misc : 5.00mL/MSVOA\_N/WATER  
 ALS Vial : 8 Sample Multiplier: 1

Instrument :  
 MSVOA\_N  
 ClientSampleId :  
 TWP-20

Integration Parameters: RTEINT3.P  
 Integrator: RTE  
 Smoothing : OFF Filtering: 5  
 Sampling : 1 Min Area: 0 % of largest Peak  
 Start Thrs: 0.2 Max Peaks: 100  
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\624N042021W.M  
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

Signal : TIC: VN066736.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 3.764       | 743           | 761         | 783          | rBV2     | 7220           | 21143         | 2.79%           | 0.700%        |
| 2         | 7.116       | 1986          | 2011        | 2041         | rBV2     | 112173         | 314782        | 41.46%          | 10.427%       |
| 3         | 7.956       | 2304          | 2324        | 2353         | rBV      | 112631         | 273772        | 36.06%          | 9.068%        |
| 4         | 8.519       | 2512          | 2534        | 2560         | rBV      | 257153         | 542978        | 71.52%          | 17.985%       |
| 5         | 10.029      | 3081          | 3097        | 3126         | rBV      | 404369         | 759156        | 100.00%         | 25.146%       |
| 6         | 11.351      | 3572          | 3590        | 3617         | rBV      | 311934         | 616883        | 81.26%          | 20.433%       |
| 7         | 12.349      | 3944          | 3962        | 3997         | rBV      | 159425         | 375768        | 49.50%          | 12.447%       |
| 8         | 13.247      | 4287          | 4297        | 4306         | rBV8     | 3831           | 7657          | 1.01%           | 0.254%        |
| 9         | 13.491      | 4375          | 4388        | 4405         | rBV2     | 38918          | 82105         | 10.82%          | 2.720%        |
| 10        | 14.529      | 4767          | 4775        | 4788         | rVB4     | 13756          | 24780         | 3.26%           | 0.821%        |




Sum of corrected areas: 3019024

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN042321\  
Data File : VN066736.D  
Acq On : 23 Apr 2021 14:33  
Operator : JC/MD  
Sample : M2150-01  
Misc : 5.00mL/MSVOA\_N/WATER  
ALS Vial : 8 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
TWP-20

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\624N042021W.M  
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

TIC Library : C:\DATABASE\NIST02.L  
TIC Integration Parameters: LSCINT.P

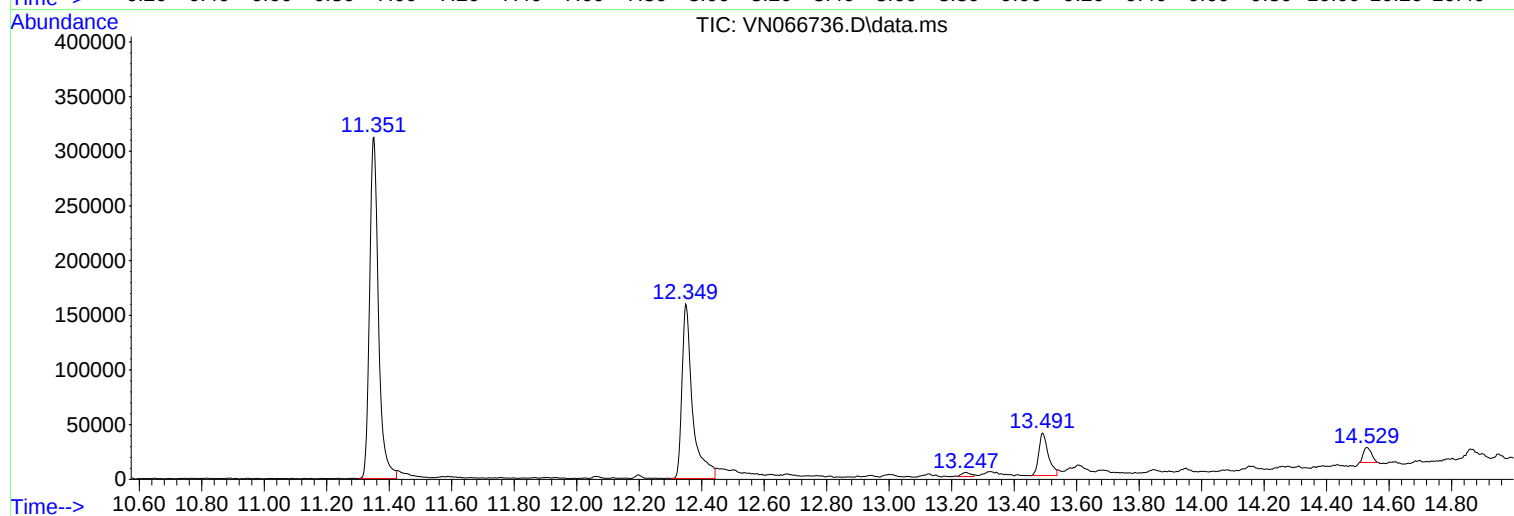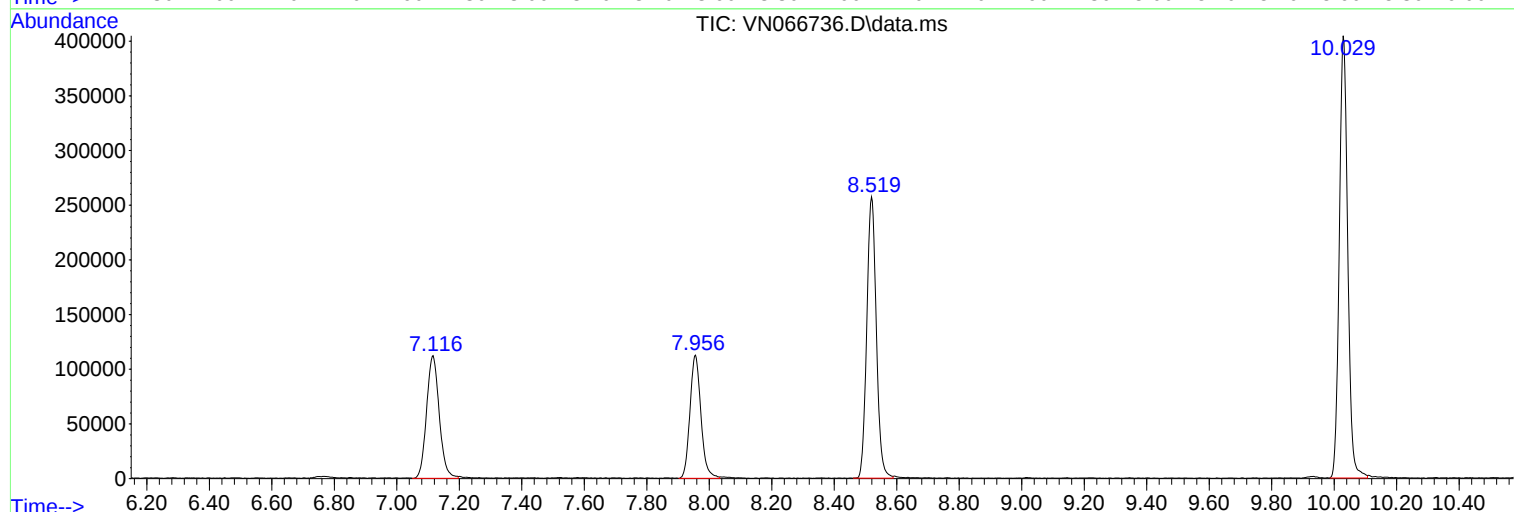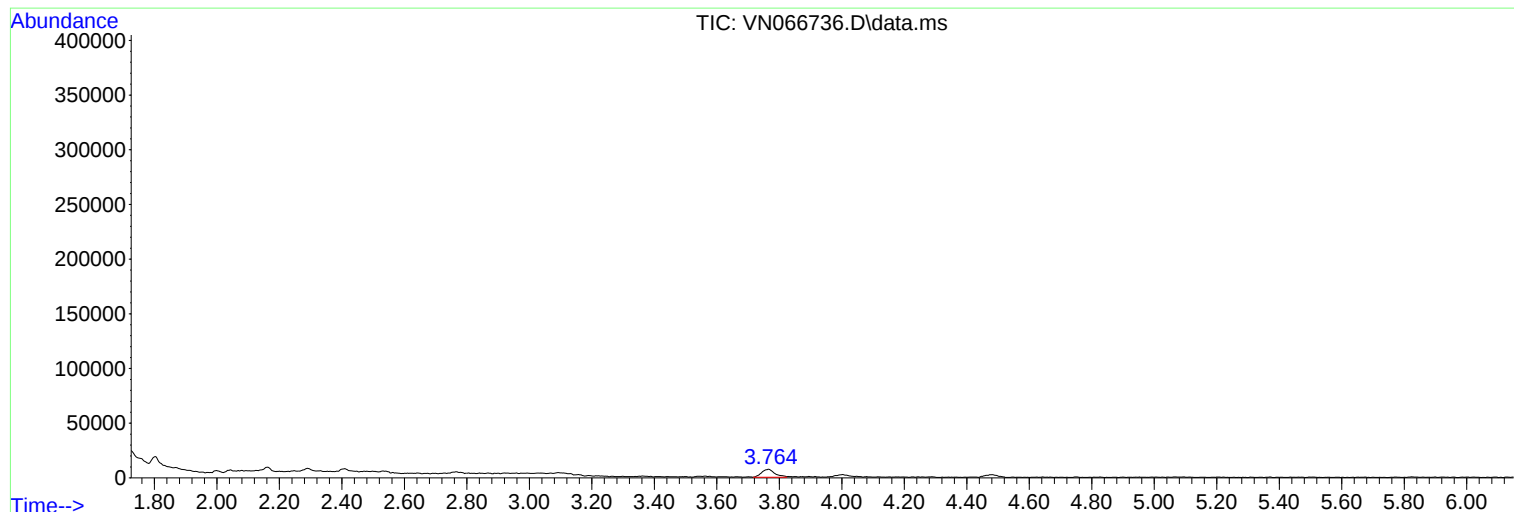

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN042321\  
Data File : VN066736.D  
Acq On : 23 Apr 2021 14:33  
Operator : JC/MD  
Sample : M2150-01  
Misc : 5.00mL/MSVOA\_N/WATER  
ALS Vial : 8 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
TWP-20

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\624N042021W.M  
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

TIC Library : C:\DATABASE\NIST02.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN042321\  
Data File : VN066736.D  
Acq On : 23 Apr 2021 14:33  
Operator : JC/MD  
Sample : M2150-01  
Misc : 5.00mL/MSVOA\_N/WATER  
ALS Vial : 8 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
TWP-20

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\624N042021W.M  
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

TIC Library : C:\DATABASE\NIST02.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |    |      |      |
|------------------|----|---------|-------|----------|-----------------------|----|------|------|
|                  |    |         |       |          | #                     | RT | Resp | Conc |

-----