


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN042325\
Data File : VN086371.D
Acq On : 23 Apr 2025 08:43
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N042325W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Thu Apr 24 04:42:24 2025

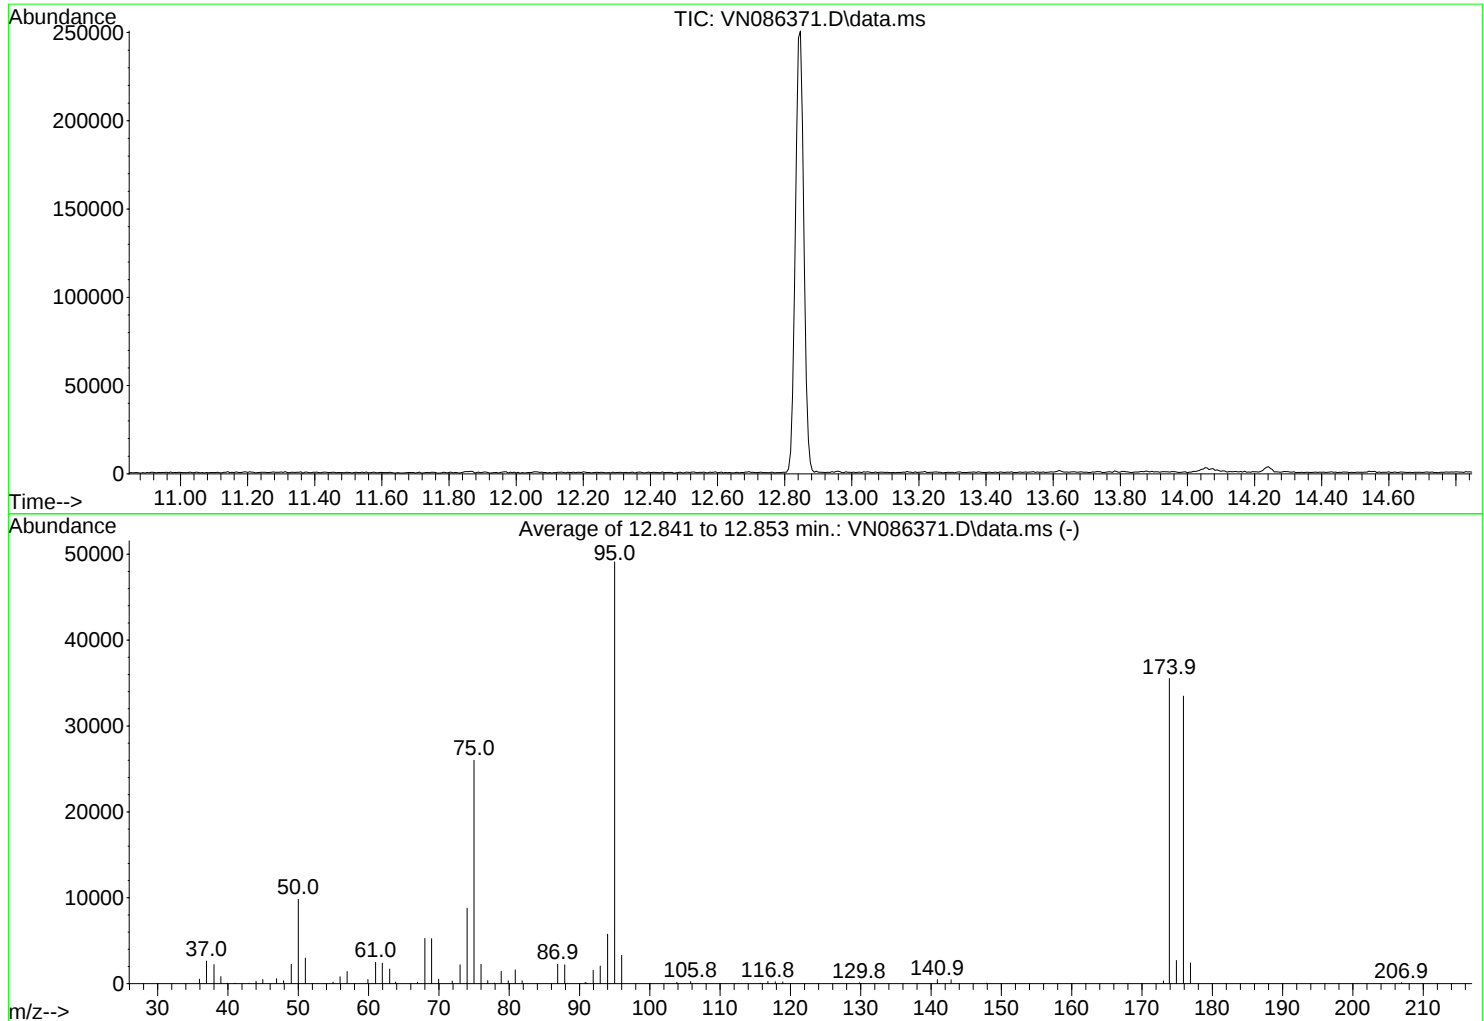

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.0	9823	PASS
75	95	30	60	53.0	26013	PASS
95	95	100	100	100.0	49115	PASS
96	95	5	9	6.7	3299	PASS
173	174	0.00	2	0.9	324	PASS
174	95	50	100	72.3	35525	PASS
175	174	5	9	7.6	2695	PASS
176	174	95	101	94.3	33483	FAIL*
177	176	5	9	7.2	2405	PASS