
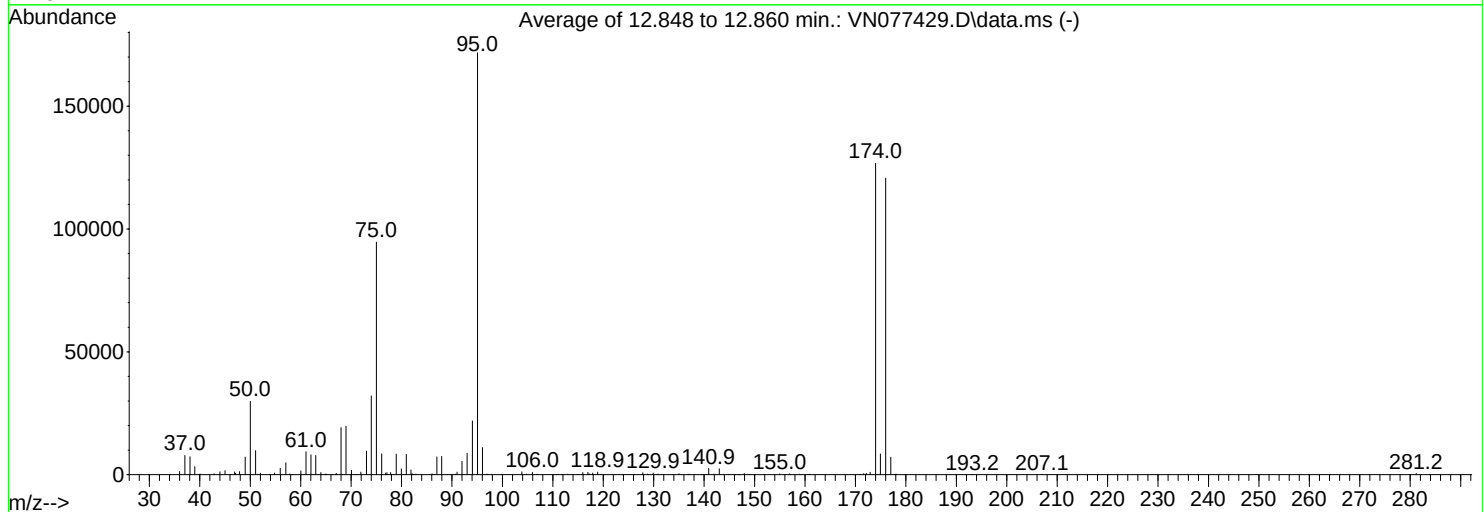


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN042423\
Data File : VN077429.D
Acq On : 24 Apr 2023 08:51
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM041823WMA.M
Title : VOC Analysis
Last Update : Tue Apr 25 03:03:54 2023

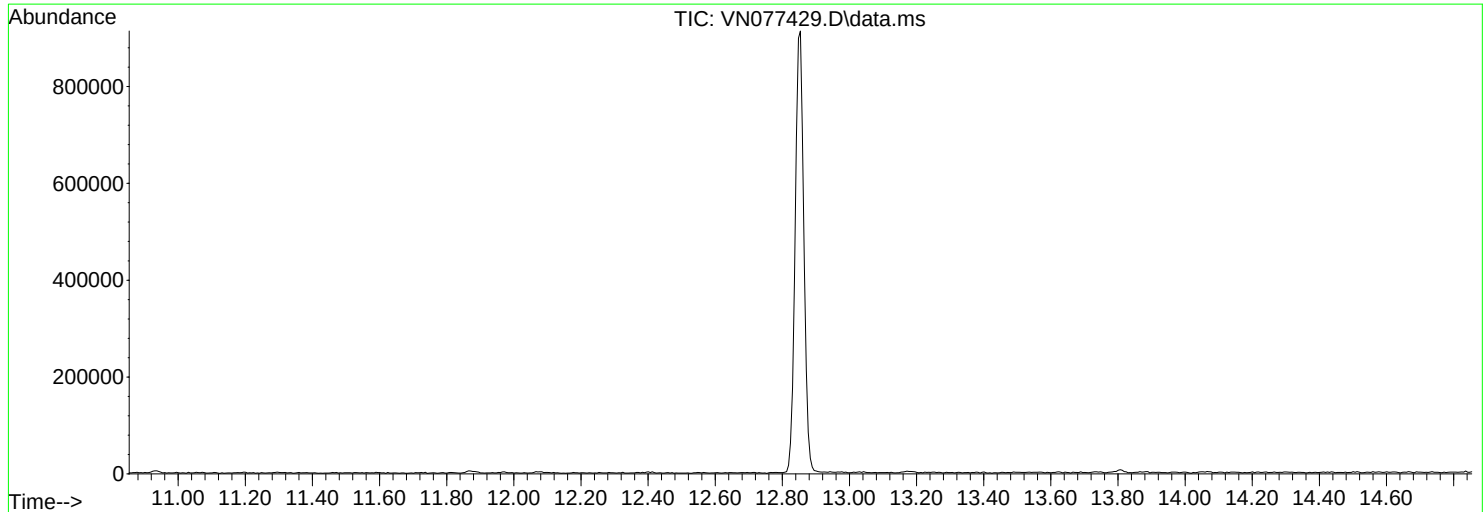

AutoFind: Scans 1855, 1856, 1857; Background Corrected with Scan 1846

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.4	29851	PASS
75	95	30	80	55.1	94691	PASS
95	95	100	100	100.0	171733	PASS
96	95	5	9	6.4	11045	PASS
173	174	0.00	2	0.8	985	PASS
174	95	50	120	73.8	126744	PASS
175	174	5	9	6.6	8409	PASS
176	174	95	101	95.3	120749	PASS
177	176	5	9	5.9	7126	PASS