


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN042423\
Data File : VN077443.D
Acq On : 25 Apr 2023 02:51
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM041823WMA.M
Title : VOC Analysis
Last Update : Tue Apr 25 03:03:54 2023

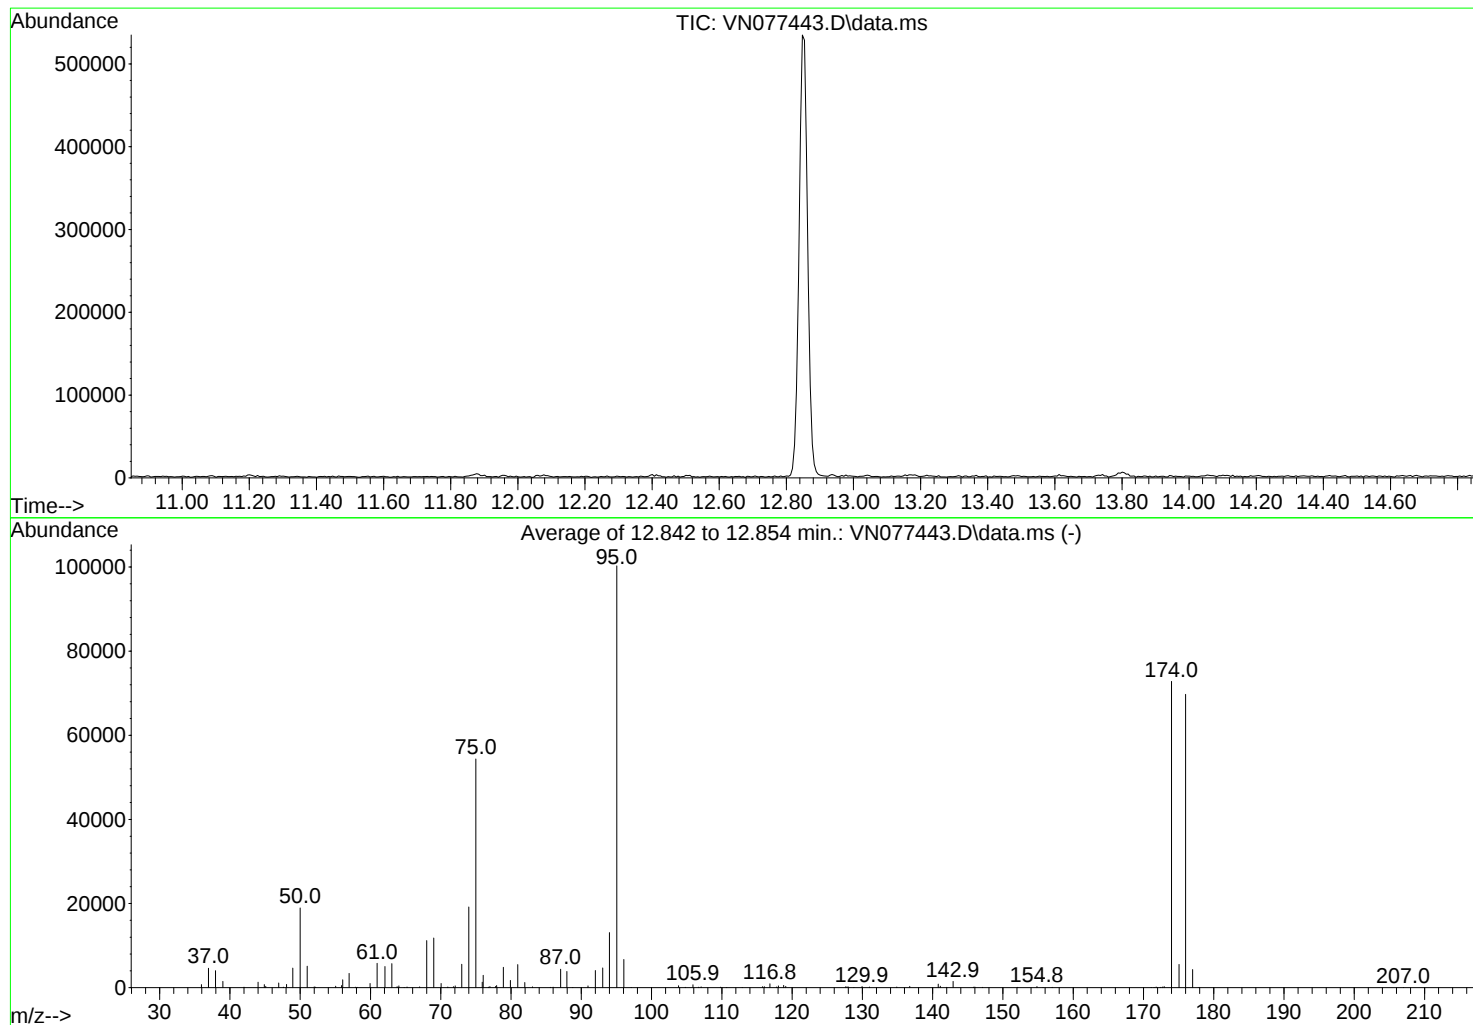

AutoFind: Scans 1854, 1855, 1856; Background Corrected with Scan 1847

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.9	18928	PASS
75	95	30	80	54.2	54365	PASS
95	95	100	100	100.0	100288	PASS
96	95	5	9	6.7	6703	PASS
173	174	0.00	2	0.4	274	PASS
174	95	50	120	72.6	72813	PASS
175	174	5	9	7.6	5526	PASS
176	174	95	101	95.8	69747	PASS
177	176	5	9	6.2	4306	PASS