

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN042425\
 Data File : VN086395.D
 Acq On : 24 Apr 2025 12:46
 Operator : JC\MD
 Sample : VN0424WBL01
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0424WBL01

Quant Time: Apr 25 01:40:23 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N042325W.M
 Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 QLast Update : Thu Apr 24 04:42:24 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	7.812	128	23712	30.000	ug/l	0.00
28) 1,4-Difluorobenzene	9.100	114	143523	30.000	ug/l	0.00
57) Chlorobenzene-d5	11.865	117	125380	30.000	ug/l	0.00

System Monitoring Compounds						
27) 1,2-Dichloroethane-d4	8.577	65	70798	30.968	ug/l	0.00
Spiked Amount	30.000	Range	91 - 110	Recovery	=	103.233%
60) 4-Bromofluorobenzene	12.847	95	67645	27.451	ug/l	0.00
Spiked Amount	30.000	Range	63 - 112	Recovery	=	91.500%
63) Toluene-d8	10.565	98	211128	30.608	ug/l	0.00
Spiked Amount	30.000	Range	91 - 112	Recovery	=	102.033%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN042425\
Data File : VN086395.D
Acq On : 24 Apr 2025 12:46
Operator : JC\MD
Sample : VN0424WBL01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0424WBL01

Quant Time: Apr 25 01:40:23 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N042325W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
QLast Update : Thu Apr 24 04:42:24 2025
Response via : Initial Calibration




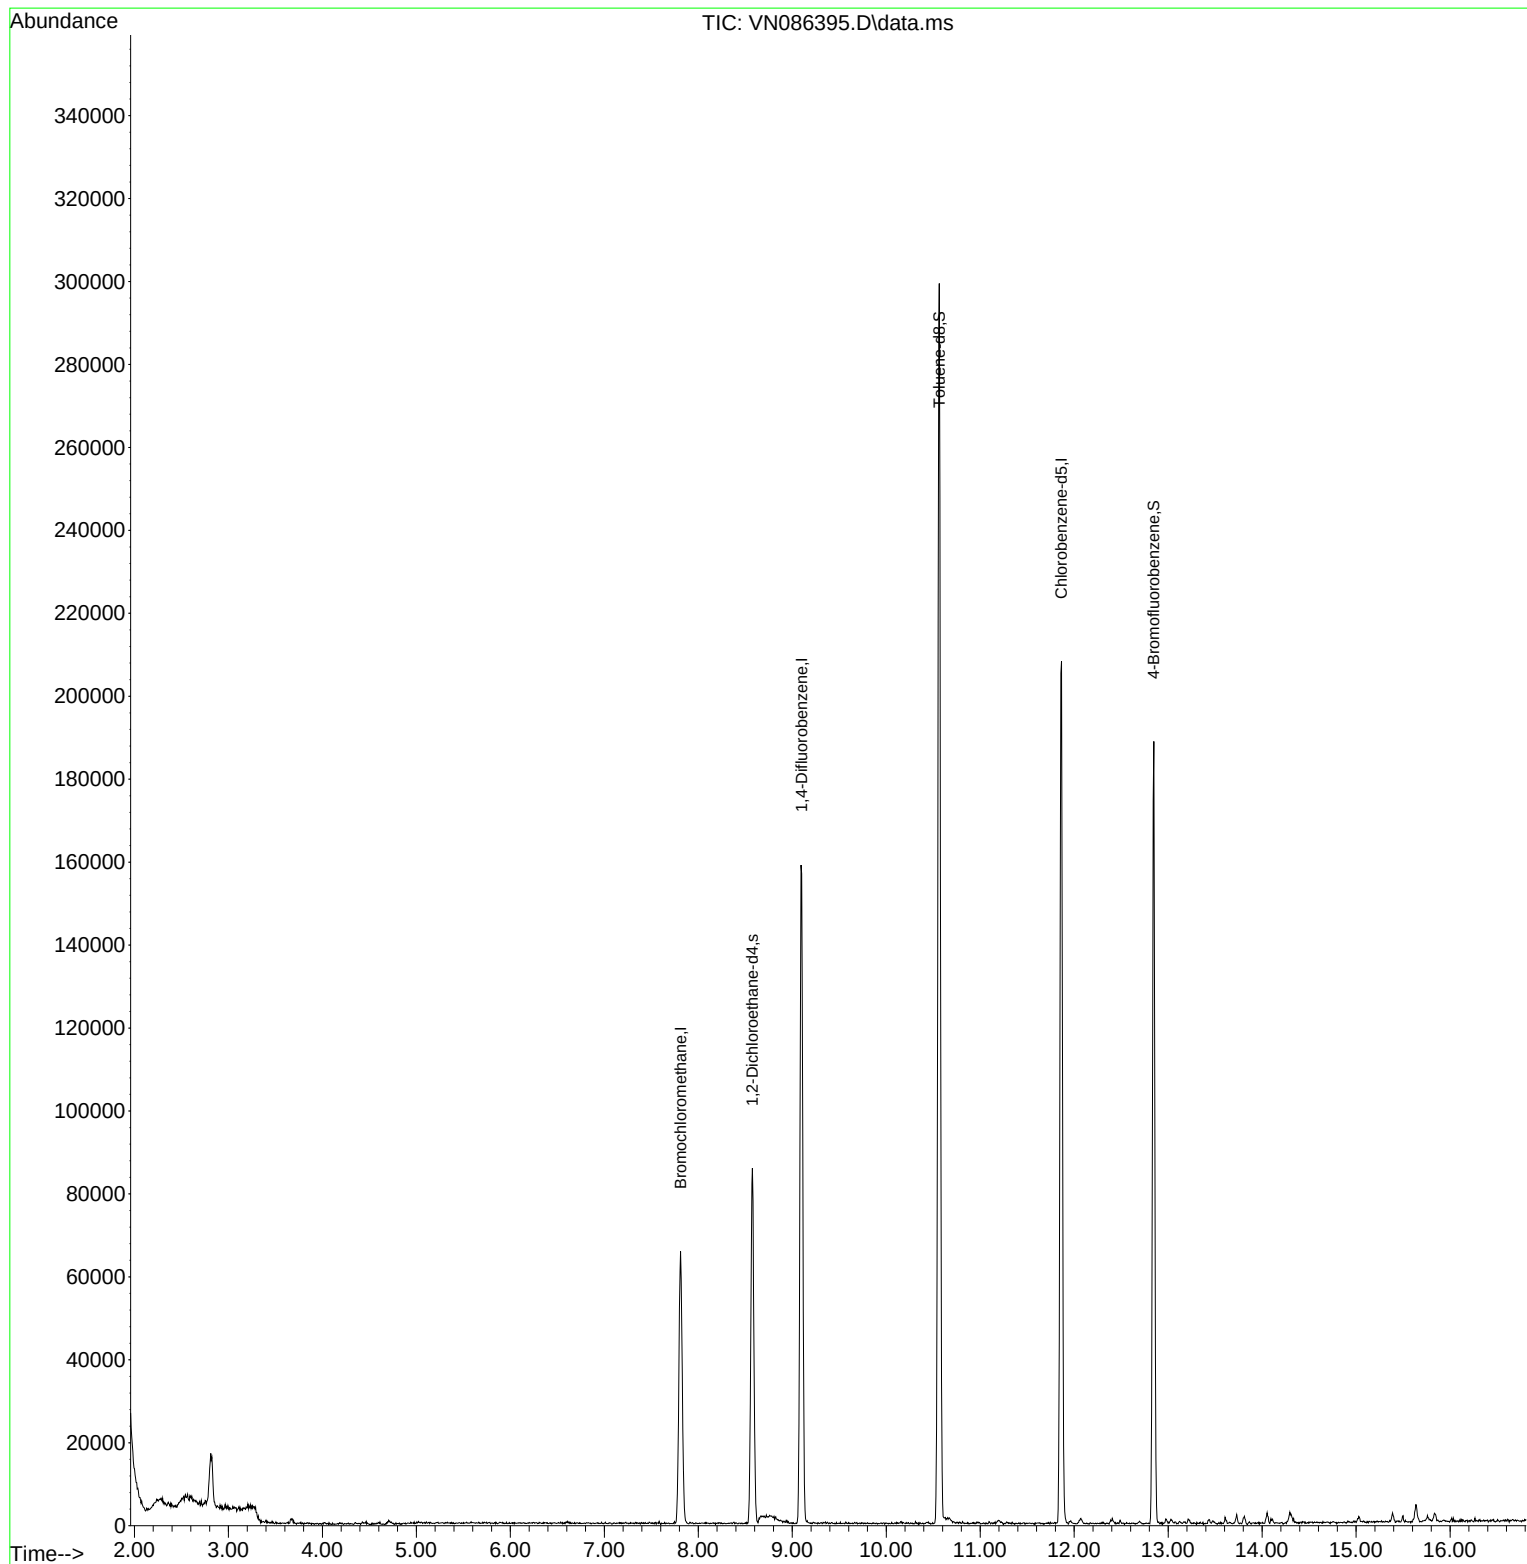


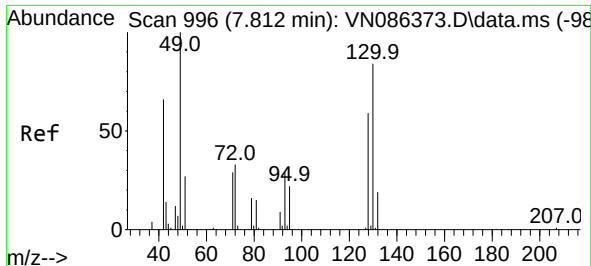

#1
Bromochloromethane
Concen: 30.000 ug/l
RT: 7.812 min Scan# 996
Delta R.T. -0.000 min
Lab File: VN086395.D
Acq: 24 Apr 2025 12:46




Instrument :
MSVOA_N
ClientSampleId :
VN0424WBL01


Tgt Ion:128 Resp: 23712
Ion Ratio Lower Upper
128 100
49 166.5 0.0 433.8
130 128.3 0.0 325.0

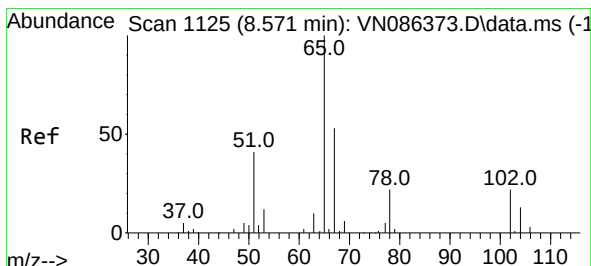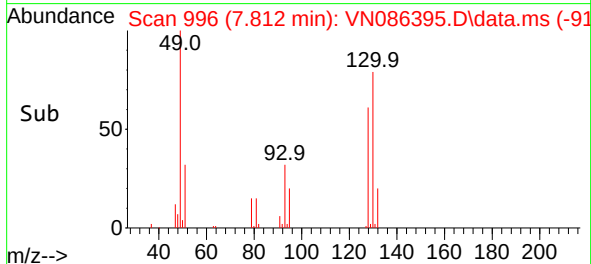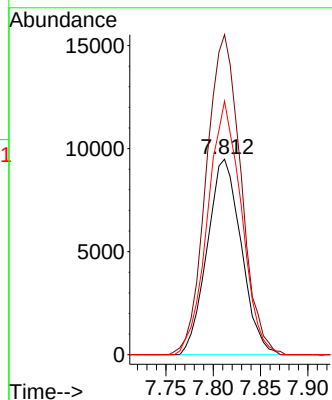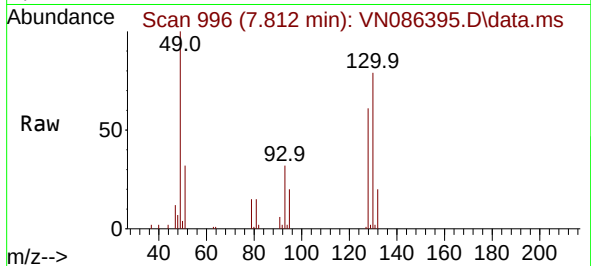

#27
1,2-Dichloroethane-d4
Concen: 30.968 ug/l
RT: 8.577 min Scan# 1126
Delta R.T. 0.006 min
Lab File: VN086395.D
Acq: 24 Apr 2025 12:46

Tgt Ion: 65 Resp: 70798
Ion Ratio Lower Upper
65 100
67 52.3 42.5 63.7

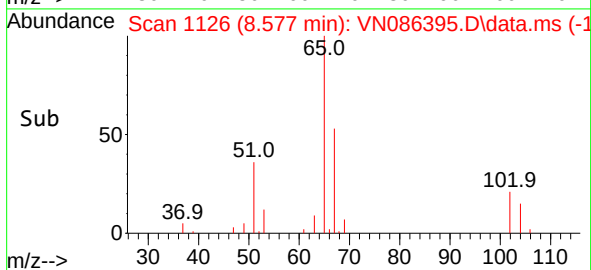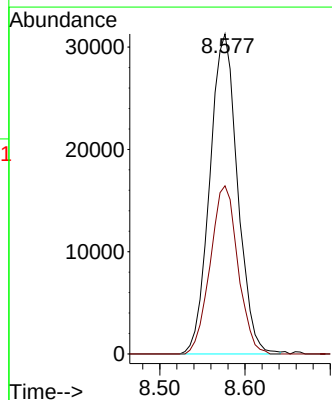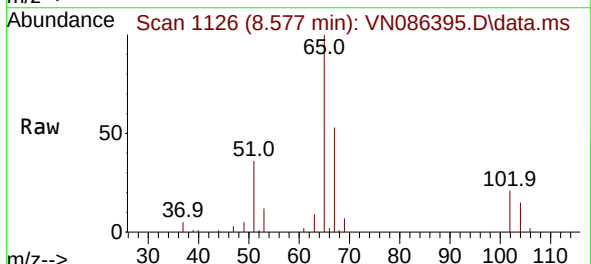

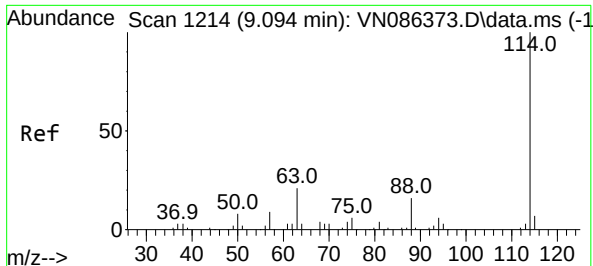

#28

1,4-Difluorobenzene

Concen: 30.000 ug/l

RT: 9.100 min Scan# 1

Delta R.T. 0.006 min

Lab File: VN086395.D

Acq: 24 Apr 2025 12:46

Instrument :

MSVOA_N

ClientSampleId :

VN0424WBL01





Tgt Ion:114 Resp: 143523

Ion Ratio Lower Upper

114 100

63 21.2 16.7 25.1

88 15.4 12.6 19.0

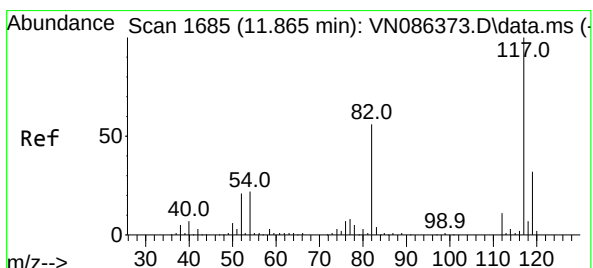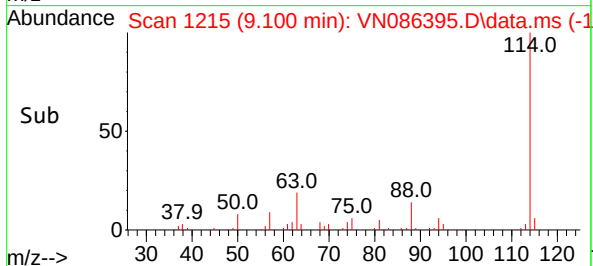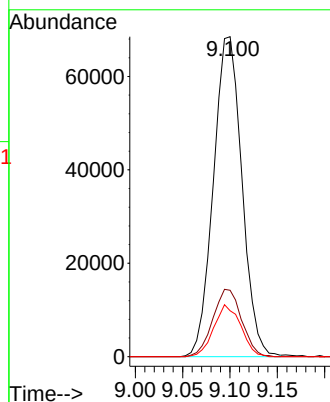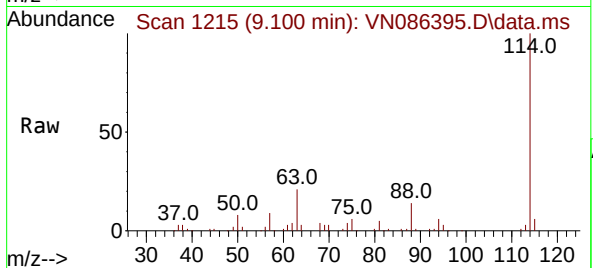

#57

Chlorobenzene-d5

Concen: 30.000 ug/l

RT: 11.865 min Scan# 1685

Delta R.T. -0.000 min

Lab File: VN086395.D

Acq: 24 Apr 2025 12:46




Tgt Ion:117 Resp: 125380


Ion Ratio Lower Upper

117 100

82 56.5 45.5 68.3

119 31.7 25.9 38.9


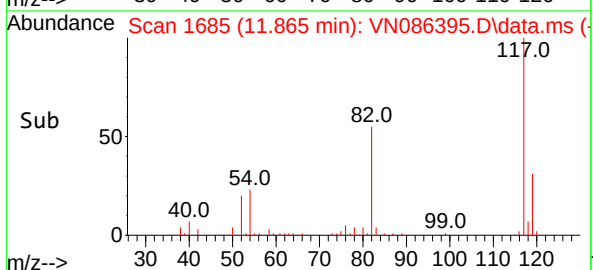
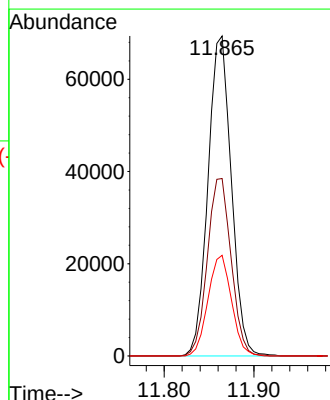
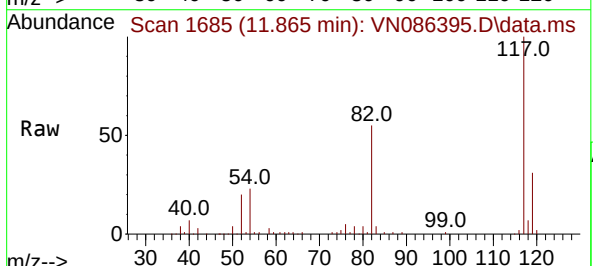


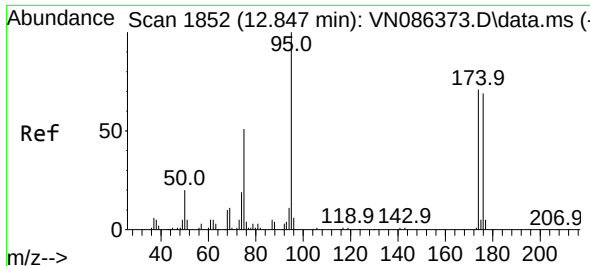

#60
4-Bromofluorobenzene
Concen: 27.451 ug/l
RT: 12.847 min Scan# 11
Delta R.T. -0.000 min
Lab File: VN086395.D
Acq: 24 Apr 2025 12:46

Instrument :
MSVOA_N
ClientSampleId :
VN0424WBL01

Tgt Ion: 95 Resp: 67645
Ion Ratio Lower Upper
95 100
174 69.4 56.6 84.8
176 68.3 53.3 79.9

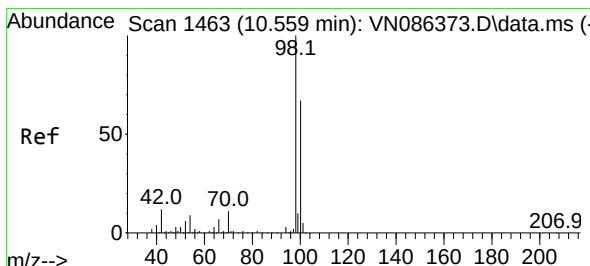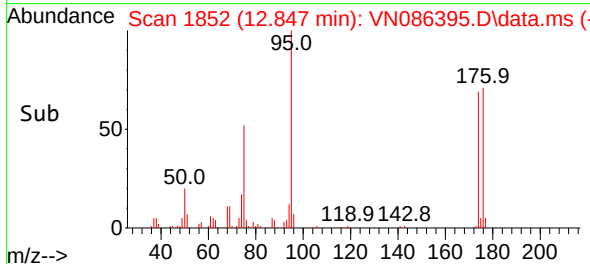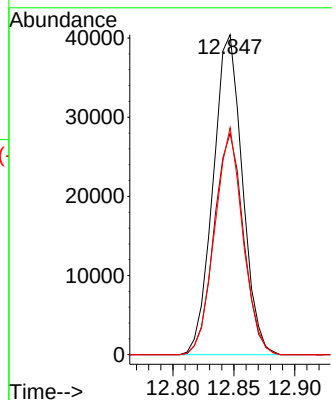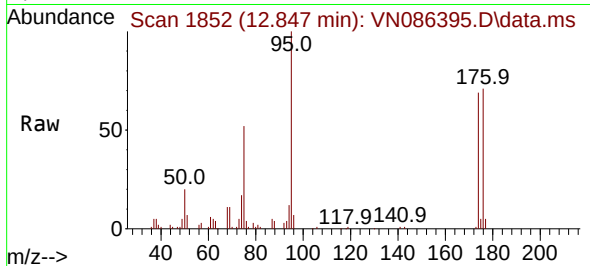

#63
Toluene-d8
Concen: 30.608 ug/l
RT: 10.565 min Scan# 1464
Delta R.T. 0.006 min
Lab File: VN086395.D
Acq: 24 Apr 2025 12:46

Tgt Ion: 98 Resp: 211128
Ion Ratio Lower Upper
98 100
100 65.1 53.1 79.7

