

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN042522\
 Data File : VN072180.D
 Acq On : 25 Apr 2022 15:27
 Operator : JC\MD
 Sample : N2524-05 5X
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 33656-57

Quant Time: Apr 26 05:39:27 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N033022W.M
 Quant Title : SW846 8260
 QLast Update : Thu Mar 31 01:57:54 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.086	168	526387	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.963	114	890866	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.739	117	953925	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.668	152	379107	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.433	65	261373	43.495	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery =	86.980%		
35) Dibromofluoromethane	8.016	113	251648	48.004	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery =	96.000%		
50) Toluene-d8	10.439	98	1118205	52.143	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery =	104.280%		
62) 4-Bromofluorobenzene	12.727	95	401885	57.945	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery =	115.900%		
Target Compounds						Qvalue
3) Chloromethane	2.293	50	1732	0.327	ug/l #	88
11) Tert butyl alcohol	5.363	59	1270	1.302	ug/l #	85
16) Acetone	4.298	43	16406	6.388	ug/l #	85
18) Methyl Acetate	4.863	43	5225	Below Cal		99
25) 2-Butanone	7.334	43	7255	1.960	ug/l #	85
31) Cyclohexane	8.081	56	8535	1.044	ug/l #	11
36) 1,1-Dichloropropene	8.086	75	32836	4.485	ug/l #	49
37) Ethyl Acetate	7.334	43	7255	0.905	ug/l #	67
38) Carbon Tetrachloride	8.086	117	44759	6.239	ug/l #	17
40) Benzene	8.457	78	740501	32.021	ug/l	98
43) Isopropyl Acetate	8.598	43	8162	0.612	ug/l #	53
49) 1,4-Dioxane	9.569	88	285	Below Cal	#	25
51) 4-Methyl-2-Pentanone	10.333	43	2293	0.299	ug/l	88
52) Toluene	10.504	92	495762	33.914	ug/l	100
53) t-1,3-Dichloropropene	10.504	75	5107	0.631	ug/l #	1
55) 1,1,2-Trichloroethane	10.757	97	4073	0.677	ug/l #	19
59) 2-Hexanone	11.074	43	2347	0.435	ug/l	79
60) Dibromochloromethane	10.969	129	1569	0.267	ug/l #	11
64) Tetrachloroethene	10.974	164	1650	0.262	ug/l #	79
67) Ethyl Benzene	11.845	91	48317	1.494	ug/l	98
68) m/p-Xylenes	11.945	106	118399	9.530	ug/l	97
69) o-Xylene	12.280	106	63394	5.141	ug/l	96
70) Styrene	12.286	104	61179	3.274	ug/l	96
76) 1,2,3-Trichloropropane	12.727	75	188289	21.440	ug/l #	1
80) 1,3,5-Trimethylbenzene	13.057	105	10163	0.402	ug/l	96
81) trans-1,4-Dichloro-2-b...	12.727	75	188289	66.441	ug/l #	11
84) 1,2,4-Trimethylbenzene	13.363	105	36221	1.467	ug/l	98
85) sec-Butylbenzene	13.363	105	36221	1.208	ug/l #	56
93) 1,2,4-Trichlorobenzene	15.257	180	1110	2.262	ug/l	96
95) Naphthalene	15.504	128	475038	29.227	ug/l	100
96) 1,2,3-Trichlorobenzene	15.704	180	1501	2.659	ug/l	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN042522\
Data File : VN072180.D
Acq On : 25 Apr 2022 15:27
Operator : JC\MD
Sample : N2524-05 5X
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
33656-57

Quant Time: Apr 26 05:39:27 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N033022W.M
Quant Title : SW846 8260
QLast Update : Thu Mar 31 01:57:54 2022
Response via : Initial Calibration




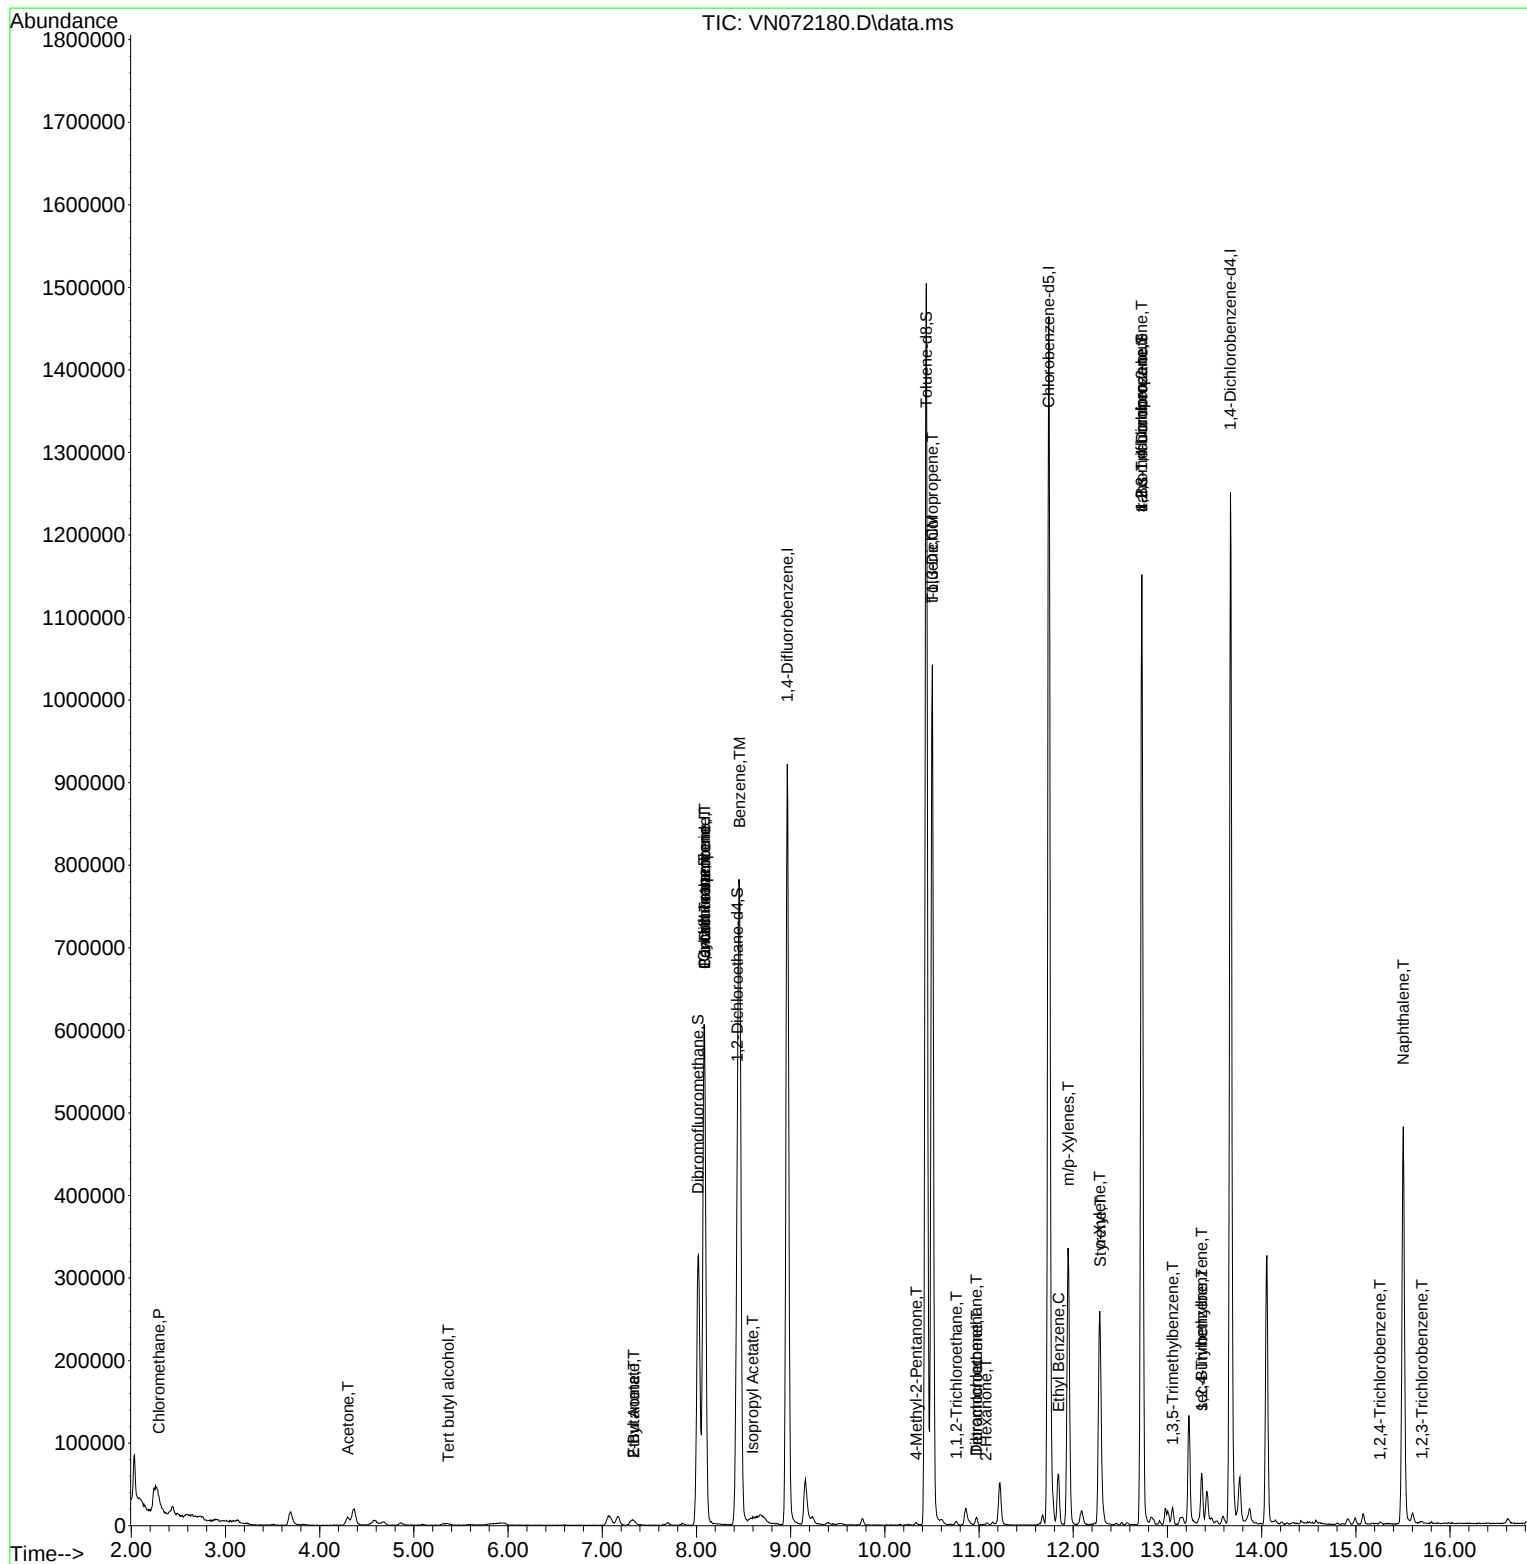




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.086 min Scan# 10
Delta R.T. 0.005 min
Lab File: VN072180.D
Acq: 25 Apr 2022 15:27




Instrument :
MSVOA_N
ClientSampleId :
33656-57


Tgt Ion:168 Resp: 526387
Ion Ratio Lower Upper
168 100
99 50.2 42.3 63.5

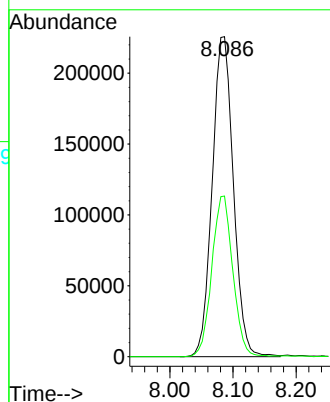

#3
Chloromethane
Concen: 0.327 ug/l
RT: 2.293 min Scan# 52
Delta R.T. -0.006 min
Lab File: VN072180.D
Acq: 25 Apr 2022 15:27

Tgt Ion: 50 Resp: 1732
Ion Ratio Lower Upper
50 100
52 25.3 25.7 38.5#


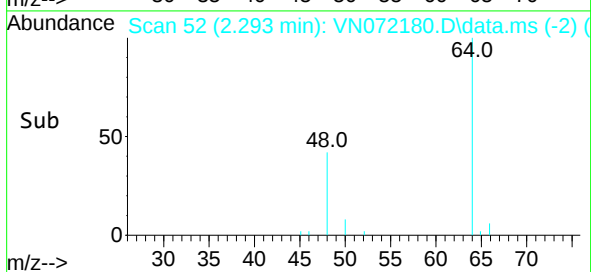
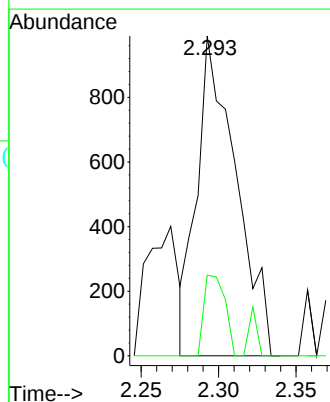
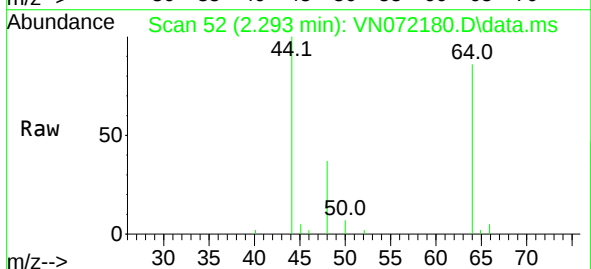




#11
Tert butyl alcohol
Concen: 1.302 ug/l
RT: 5.363 min Scan# 51
Delta R.T. 0.006 min
Lab File: VN072180.D
Acq: 25 Apr 2022 15:27




Instrument :
MSVOA_N
ClientSampleId :
33656-57


Tgt Ion: 59 Resp: 1270
Ion Ratio Lower Upper
59 100
57 4.9 8.3 12.5#

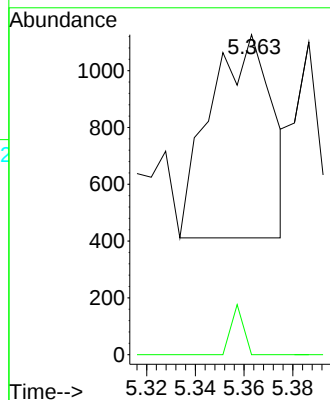

#16
Acetone
Concen: 6.388 ug/l
RT: 4.298 min Scan# 393
Delta R.T. 0.023 min
Lab File: VN072180.D
Acq: 25 Apr 2022 15:27

Tgt Ion: 43 Resp: 16406
Ion Ratio Lower Upper
43 100
58 40.8 26.0 39.0#



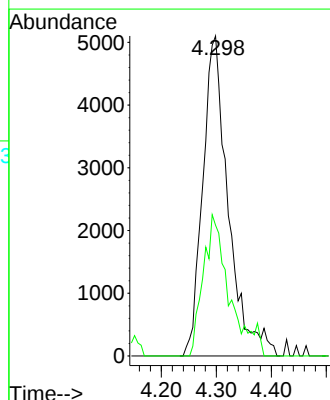





#18
Methyl Acetate
Concen: Below Cal
RT: 4.863 min Scan# 41
Delta R.T. 0.017 min
Lab File: VN072180.D
Acq: 25 Apr 2022 15:27




Instrument :
MSVOA_N
ClientSampleId :
33656-57


Tgt Ion: 43 Resp: 5225
Ion Ratio Lower Upper
43 100
74 27.4 21.6 32.4



#25
2-Butanone
Concen: 1.960 ug/l
RT: 7.334 min Scan# 909
Delta R.T. 0.006 min
Lab File: VN072180.D
Acq: 25 Apr 2022 15:27


Tgt Ion: 43 Resp: 7255
Ion Ratio Lower Upper
43 100
72 37.6 23.7 35.5#

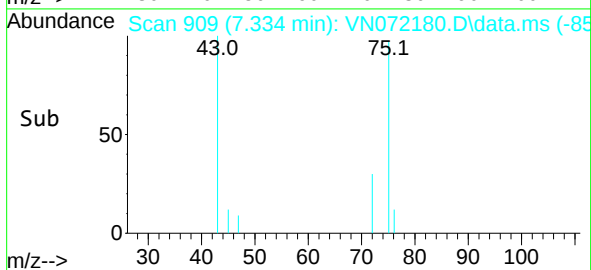






#31
Cyclohexane
Concen: 1.044 ug/l
RT: 8.081 min Scan# 1036
Delta R.T. -0.011 min
Lab File: VN072180.D
Acq: 25 Apr 2022 15:27

Instrument :
MSVOA_N
ClientSampleId :
33656-57







Tgt Ion: 56 Resp: 8535
Ion Ratio Lower Upper
56 100
69 165.6 27.8 41.8#
84 134.3 76.9 115.3#

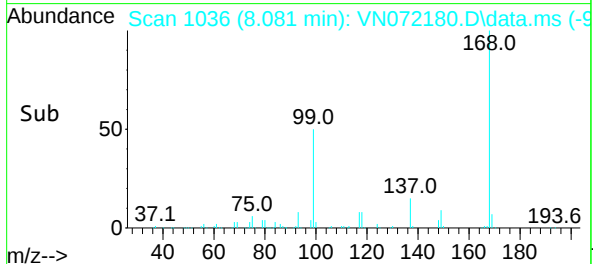

#33
1,2-Dichloroethane-d4
Concen: 43.495 ug/l
RT: 8.433 min Scan# 1096
Delta R.T. -0.001 min
Lab File: VN072180.D
Acq: 25 Apr 2022 15:27

Tgt Ion: 65 Resp: 261373
Ion Ratio Lower Upper
65 100
67 53.7 0.0 104.8

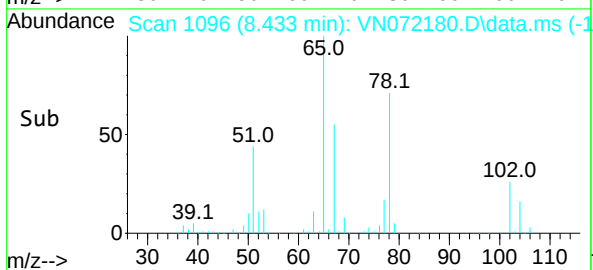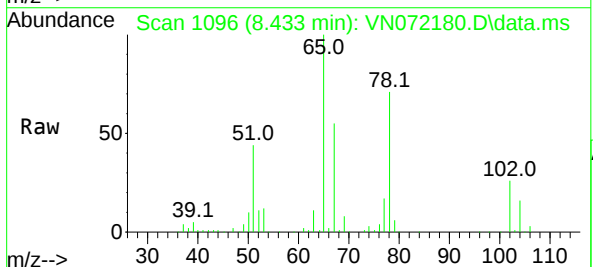

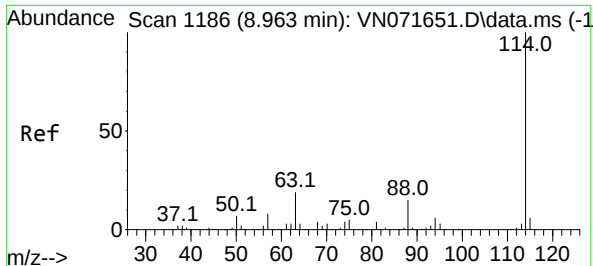

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.963 min Scan# 1186

Delta R.T. -0.000 min

Lab File: VN072180.D

Acq: 25 Apr 2022 15:27

Instrument :

MSVOA_N

ClientSampleId :

33656-57





Tgt Ion:114 Resp: 890866

Ion Ratio Lower Upper

114 100

63 18.1 0.0 40.0

88 15.2 0.0 32.6

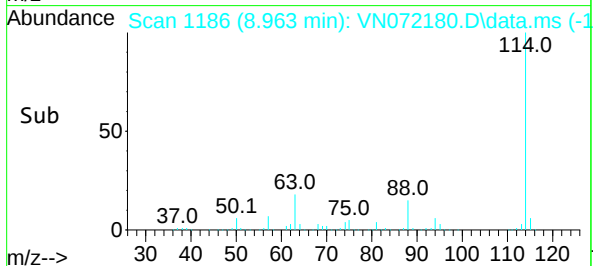

#35

Dibromofluoromethane

Concen: 48.004 ug/l

RT: 8.016 min Scan# 1025

Delta R.T. -0.000 min

Lab File: VN072180.D

Acq: 25 Apr 2022 15:27




Tgt Ion:113 Resp: 251648


Ion Ratio Lower Upper

113 100

111 102.7 81.4 122.0

192 23.7 17.0 25.6

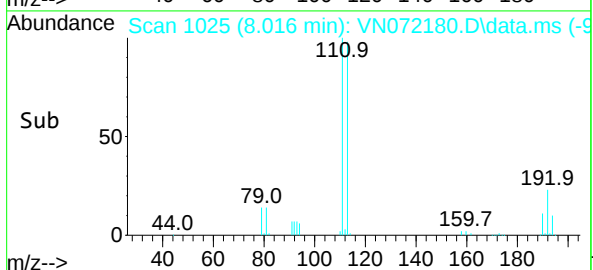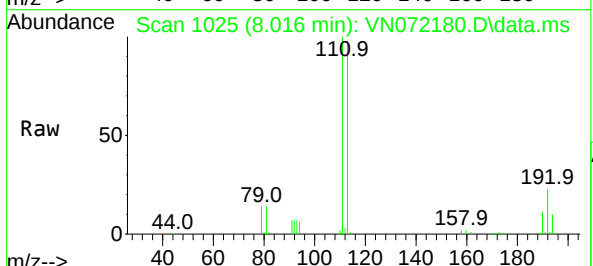

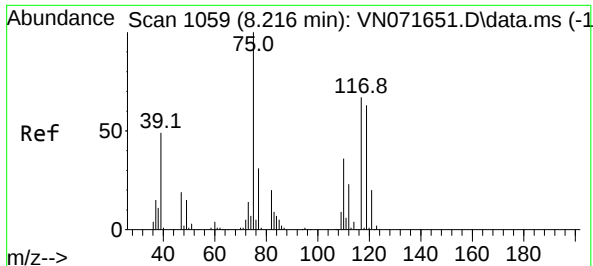

#36

1,1-Dichloropropene

Concen: 4.485 ug/l

RT: 8.086 min Scan# 1

Delta R.T. -0.130 min

Lab File: VN072180.D

Acq: 25 Apr 2022 15:27

Instrument :

MSVOA_N

ClientSampleId :

33656-57





Tgt Ion: 75 Resp: 32836

Ion Ratio Lower Upper

75 100

110 9.6 18.3 54.8#

77 0.0 25.1 37.7#

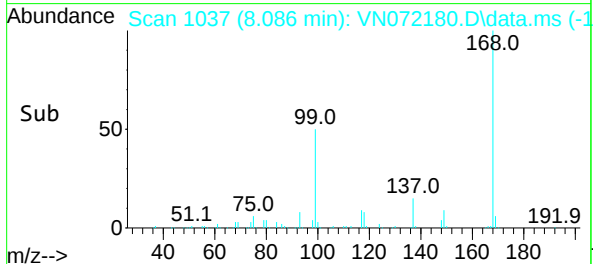

#37

Ethyl Acetate

Concen: 0.905 ug/l

RT: 7.334 min Scan# 909

Delta R.T. -0.070 min

Lab File: VN072180.D

Acq: 25 Apr 2022 15:27




Tgt Ion: 43 Resp: 7255


Ion Ratio Lower Upper

43 100

61 0.0 11.8 17.6#

70 0.0 9.3 13.9#


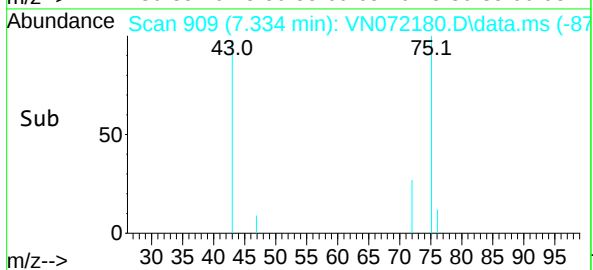

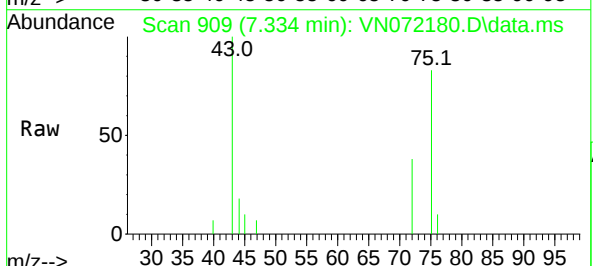


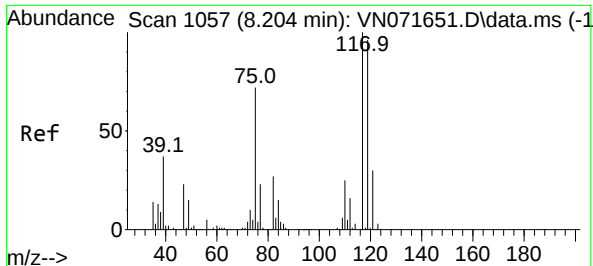

#38
Carbon Tetrachloride
Concen: 6.239 ug/l
RT: 8.086 min Scan# 1107
Delta R.T. -0.118 min
Lab File: VN072180.D
Acq: 25 Apr 2022 15:27




Instrument :
MSVOA_N
ClientSampleId :
33656-57


Tgt Ion:117 Resp: 44759
Ion Ratio Lower Upper
117 100
119 6.0 75.8 113.8#
121 0.0 24.6 37.0#

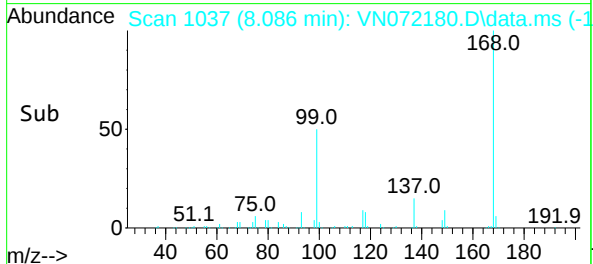

#40
Benzene
Concen: 32.021 ug/l
RT: 8.457 min Scan# 1100
Delta R.T. -0.000 min
Lab File: VN072180.D
Acq: 25 Apr 2022 15:27

Tgt Ion: 78 Resp: 740501
Ion Ratio Lower Upper
78 100
77 23.4 19.4 29.0

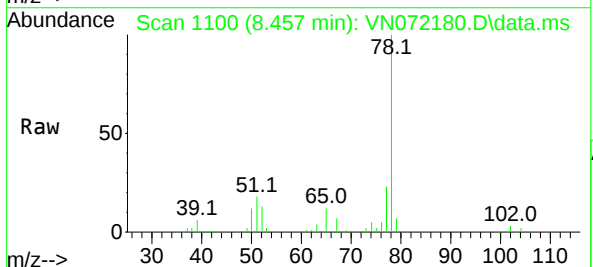

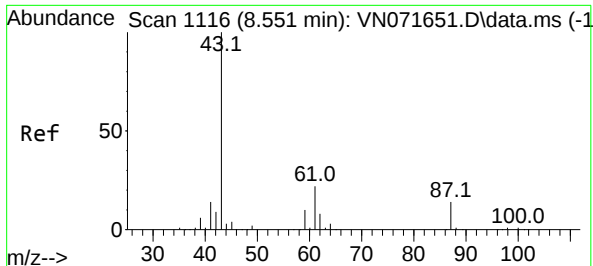

#43

Isopropyl Acetate

Concen: 0.612 ug/l

RT: 8.598 min Scan# 1116

Delta R.T. 0.047 min

Lab File: VN072180.D

Acq: 25 Apr 2022 15:27

Instrument :

MSVOA_N

ClientSampleId :

33656-57




Tgt Ion: 43 Resp: 8162

Ion Ratio Lower Upper

43 100

61 0.0 21.9 32.9#

87 0.0 12.0 18.0#

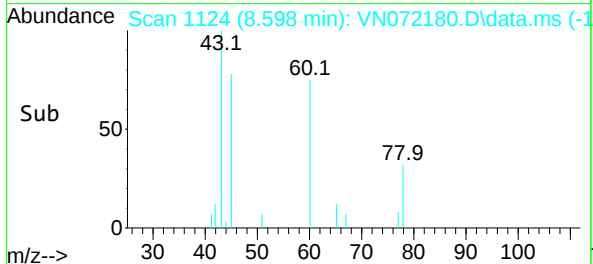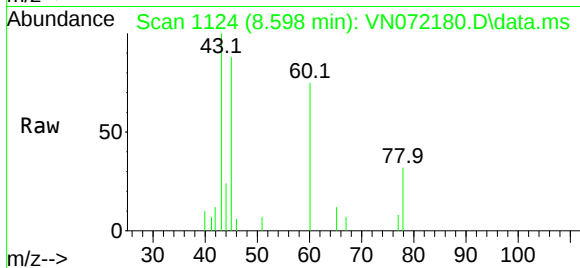

#49

1,4-Dioxane

Concen: Below Cal

RT: 9.569 min Scan# 1289

Delta R.T. 0.006 min

Lab File: VN072180.D

Acq: 25 Apr 2022 15:27




Tgt Ion: 88 Resp: 285


Ion Ratio Lower Upper

88 100

43 0.0 20.2 30.4#

58 0.0 54.2 81.4#


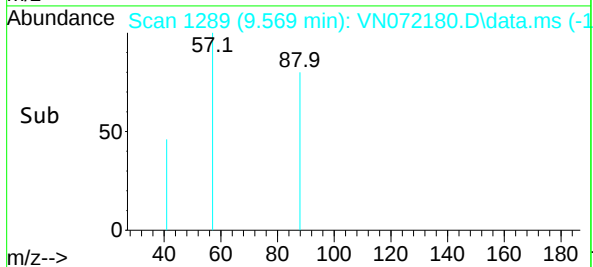

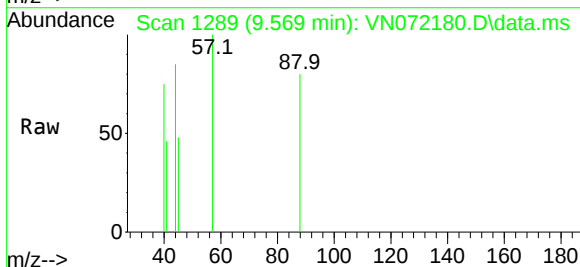




#50
Toluene-d8
Concen: 52.143 ug/l
RT: 10.439 min Scan# 1437
Delta R.T. 0.000 min
Lab File: VN072180.D
Acq: 25 Apr 2022 15:27




Instrument :
MSVOA_N
ClientSampleId :
33656-57


Tgt Ion: 98 Resp: 1118205
Ion Ratio Lower Upper
98 100
100 65.1 52.6 78.8



#51
4-Methyl-2-Pentanone
Concen: 0.299 ug/l
RT: 10.333 min Scan# 1419
Delta R.T. 0.011 min
Lab File: VN072180.D
Acq: 25 Apr 2022 15:27

Tgt Ion: 43 Resp: 2293
Ion Ratio Lower Upper
43 100
58 34.9 34.1 51.1


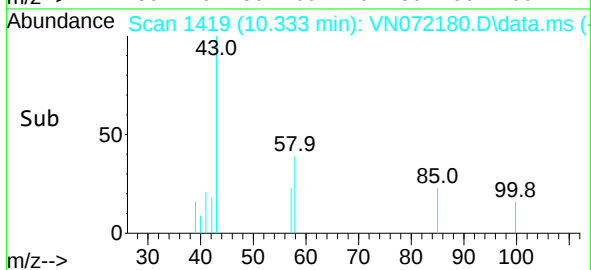

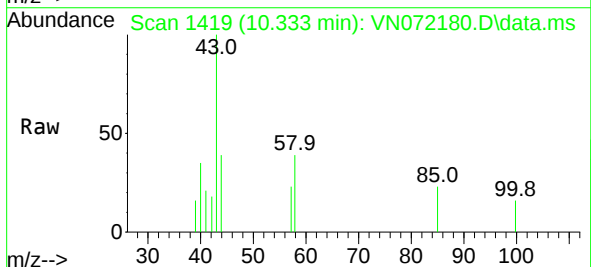




#52
Toluene
Concen: 33.914 ug/l
RT: 10.504 min Scan# 1448
Delta R.T. 0.006 min
Lab File: VN072180.D
Acq: 25 Apr 2022 15:27




Instrument :
MSVOA_N
ClientSampleId :
33656-57


Tgt Ion: 92 Resp: 495762
Ion Ratio Lower Upper
92 100
91 172.5 138.6 207.8

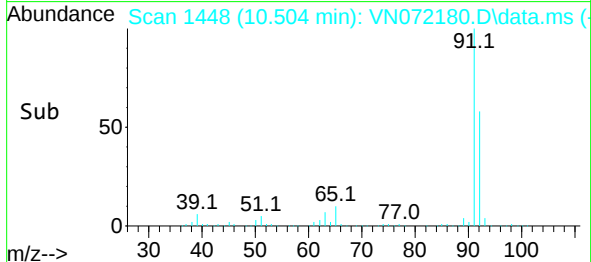

#53
t-1,3-Dichloropropene
Concen: 0.631 ug/l
RT: 10.504 min Scan# 1448
Delta R.T. -0.206 min
Lab File: VN072180.D
Acq: 25 Apr 2022 15:27

Tgt Ion: 75 Resp: 5107
Ion Ratio Lower Upper
75 100
77 123.2 25.6 38.4#

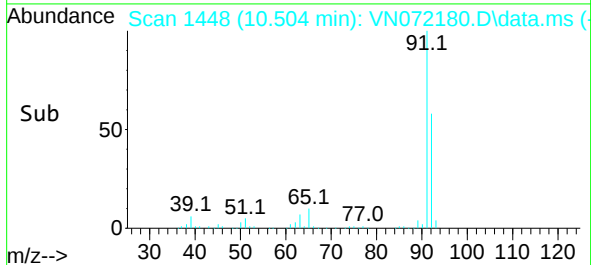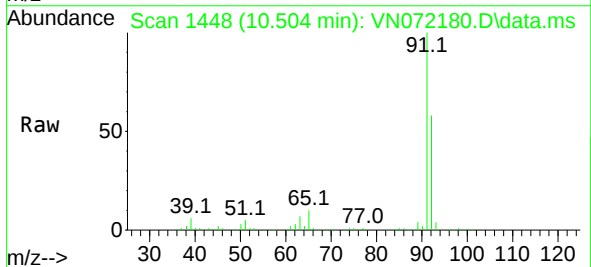



#55

1,1,2-Trichloroethane

Concen: 0.677 ug/l

RT: 10.757 min Scan# 1491

Delta R.T. -0.135 min

Lab File: VN072180.D

Acq: 25 Apr 2022 15:27

Instrument :

MSVOA_N

ClientSampleId :

33656-57

Tgt Ion: 97 Resp: 4073





Ion Ratio Lower Upper

97 100

83 0.0 66.2 99.4#

85 0.0 43.9 65.9#

99 7.3 50.6 76.0#

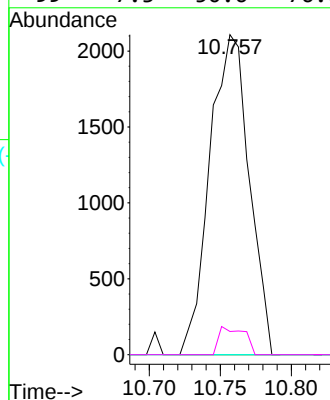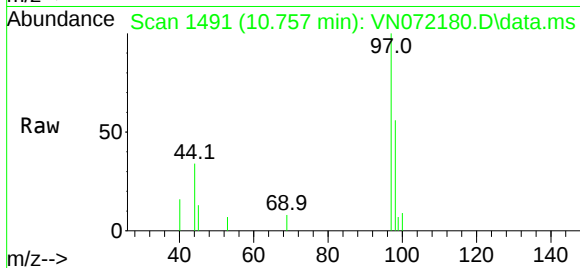

#59

2-Hexanone

Concen: 0.435 ug/l

RT: 11.074 min Scan# 1545

Delta R.T. -0.007 min

Lab File: VN072180.D




Acq: 25 Apr 2022 15:27


Tgt Ion: 43 Resp: 2347

Ion Ratio Lower Upper

43 100

58 43.7 29.7 89.1


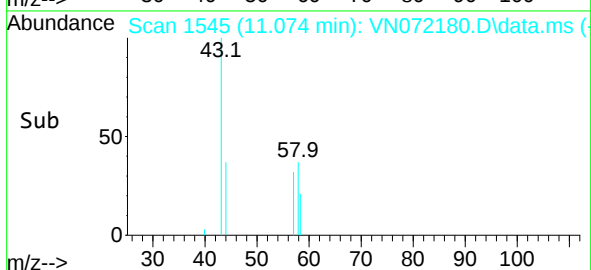
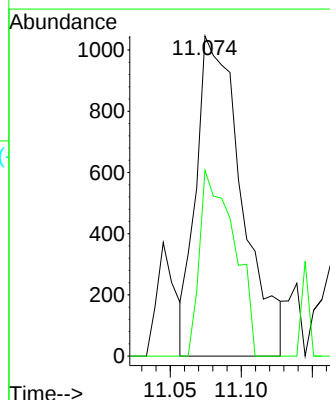
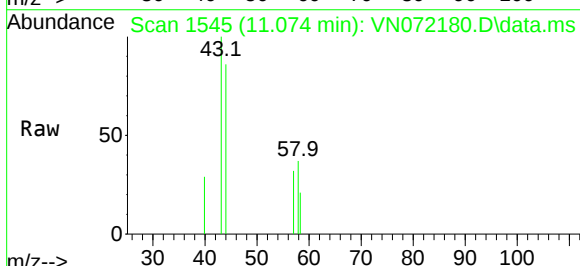




#60
Dibromochloromethane
Concen: 0.267 ug/l
RT: 10.969 min Scan# 11
Delta R.T. -0.264 min
Lab File: VN072180.D
Acq: 25 Apr 2022 15:27




Instrument :
MSVOA_N
ClientSampleId :
33656-57


Tgt Ion:129 Resp: 1569
Ion Ratio Lower Upper
129 100
127 0.0 38.8 116.4#

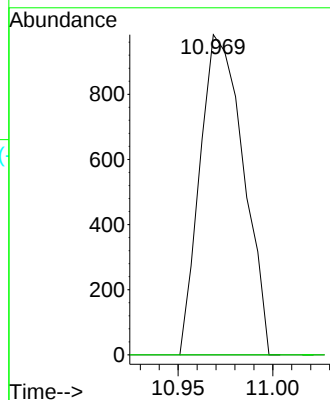

#62
4-Bromofluorobenzene
Concen: 57.945 ug/l
RT: 12.727 min Scan# 1826
Delta R.T. 0.000 min
Lab File: VN072180.D
Acq: 25 Apr 2022 15:27

Tgt Ion: 95 Resp: 401885
Ion Ratio Lower Upper
95 100
174 90.4 0.0 167.6
176 87.1 0.0 163.4


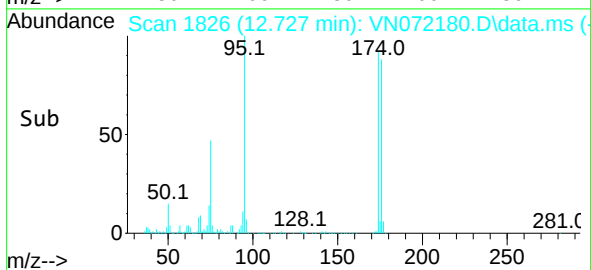
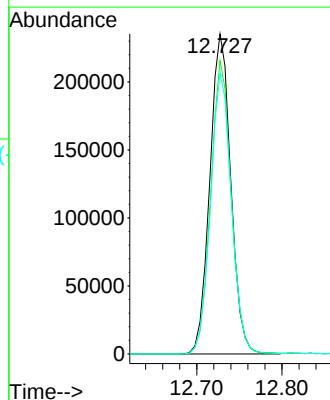





#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.739 min Scan# 117
Delta R.T. 0.000 min
Lab File: VN072180.D
Acq: 25 Apr 2022 15:27




Instrument :
MSVOA_N
ClientSampleId :
33656-57


Tgt Ion:117 Resp: 953925
Ion Ratio Lower Upper
117 100
82 54.2 44.2 66.2
119 32.2 25.4 38.0

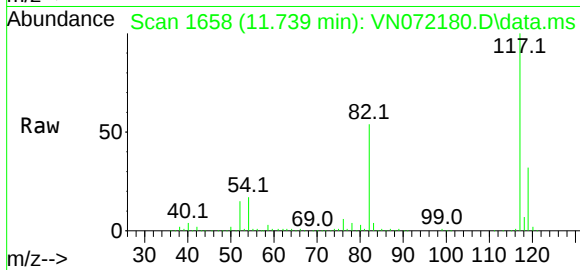

#64
Tetrachloroethene
Concen: 0.262 ug/l
RT: 10.974 min Scan# 1528
Delta R.T. -0.001 min
Lab File: VN072180.D
Acq: 25 Apr 2022 15:27

Tgt Ion:164 Resp: 1650
Ion Ratio Lower Upper
164 100
166 116.2 104.2 156.2
129 102.6 73.9 110.9
131 127.6 69.4 104.2#


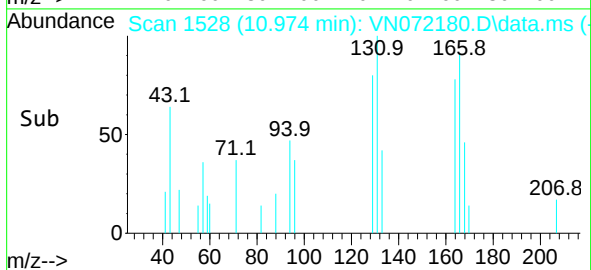

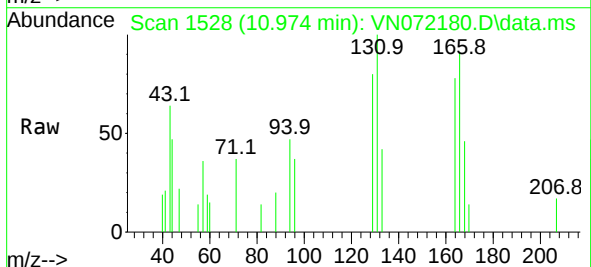




#67
Ethyl Benzene
Concen: 1.494 ug/l
RT: 11.845 min Scan# 1675
Delta R.T. 0.006 min
Lab File: VN072180.D
Acq: 25 Apr 2022 15:27




Instrument :
MSVOA_N
ClientSampleId :
33656-57


Tgt Ion: 91 Resp: 48317
Ion Ratio Lower Upper
91 100
106 32.2 24.9 37.3

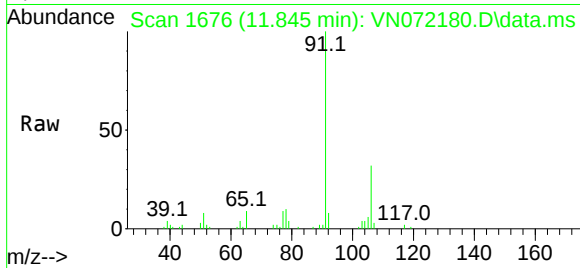

#68
m/p-Xylenes
Concen: 9.530 ug/l
RT: 11.945 min Scan# 1693
Delta R.T. -0.006 min
Lab File: VN072180.D
Acq: 25 Apr 2022 15:27

Tgt Ion:106 Resp: 118399
Ion Ratio Lower Upper
106 100
91 194.5 158.9 238.3


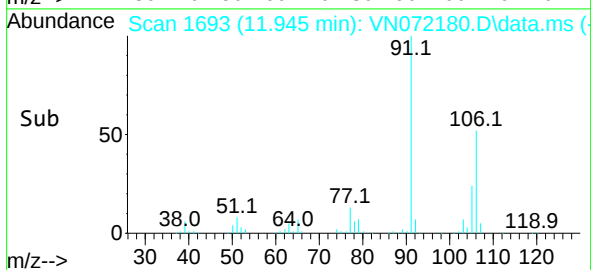

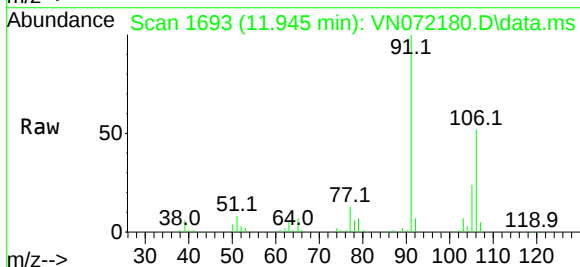




#69
o-Xylene
Concen: 5.141 ug/l
RT: 12.280 min Scan# 1749
Delta R.T. 0.005 min
Lab File: VN072180.D
Acq: 25 Apr 2022 15:27




Instrument :
MSVOA_N
ClientSampleId :
33656-57


Tgt Ion:106 Resp: 63394
Ion Ratio Lower Upper
106 100
91 205.7 106.0 318.0



#70
Styrene
Concen: 3.274 ug/l
RT: 12.286 min Scan# 1751
Delta R.T. 0.000 min
Lab File: VN072180.D
Acq: 25 Apr 2022 15:27

Tgt Ion:104 Resp: 61179
Ion Ratio Lower Upper
104 100
78 49.9 39.5 59.3
103 59.8 44.0 66.0


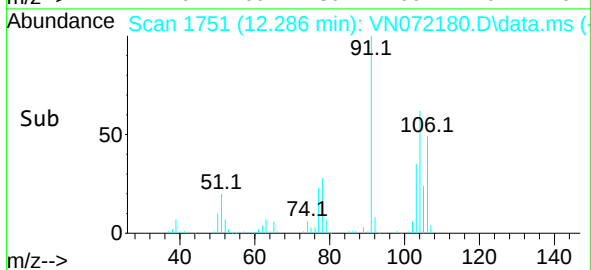

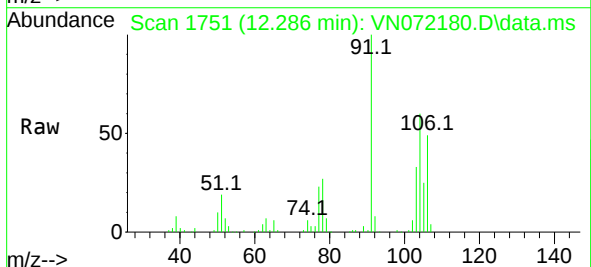




#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 13.668 min Scan# 1986
 Delta R.T. -0.001 min
 Lab File: VN072180.D
 Acq: 25 Apr 2022 15:27




Instrument :
 MSVOA_N
 ClientSampleId :
 33656-57


Tgt Ion:152 Resp: 379107
 Ion Ratio Lower Upper
 152 100
 115 55.6 28.9 86.7
 150 157.0 0.0 356.2

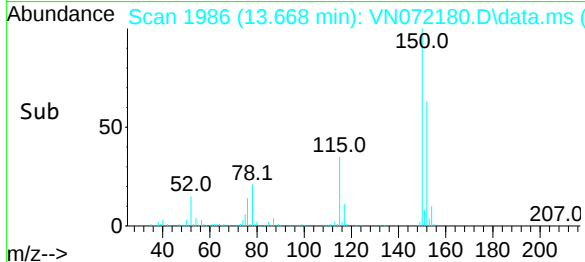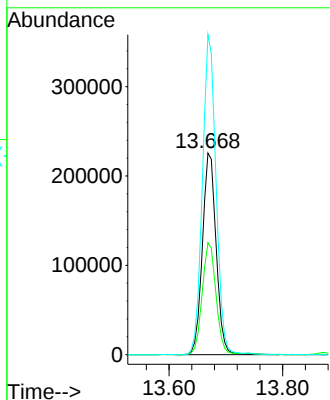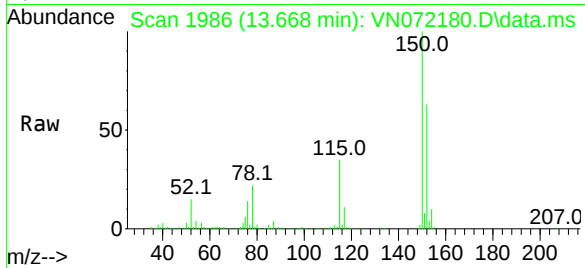

#76
 1,2,3-Trichloropropane
 Concen: 21.440 ug/l
 RT: 12.727 min Scan# 1826
 Delta R.T. -0.147 min
 Lab File: VN072180.D
 Acq: 25 Apr 2022 15:27

Tgt Ion: 75 Resp: 188289
 Ion Ratio Lower Upper
 75 100
 77 1.3 98.5 295.5#


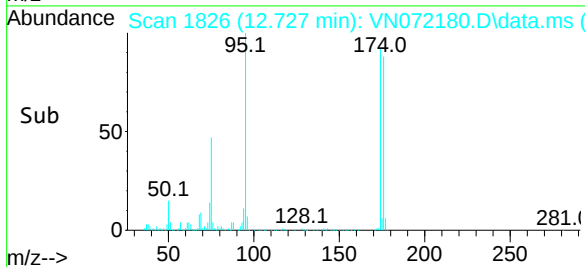
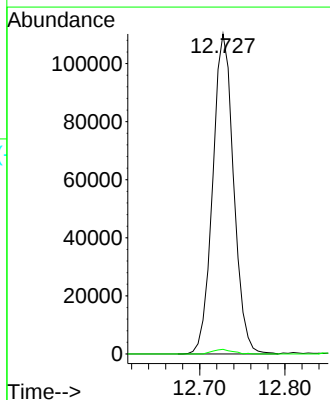
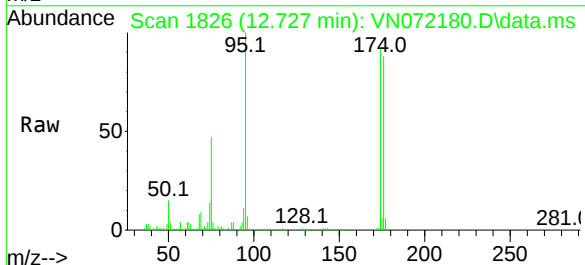


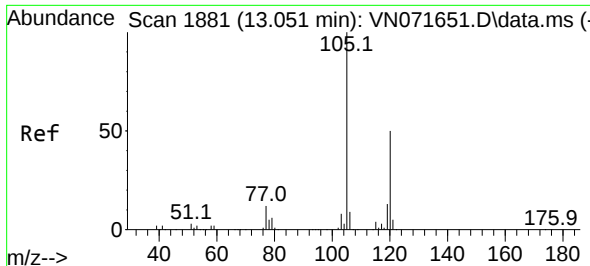

#80
1,3,5-Trimethylbenzene
Concen: 0.402 ug/l
RT: 13.057 min Scan# 1881
Delta R.T. 0.006 min
Lab File: VN072180.D
Acq: 25 Apr 2022 15:27




Instrument :
MSVOA_N
ClientSampleId :
33656-57


Tgt Ion:105 Resp: 10163
Ion Ratio Lower Upper
105 100
120 52.7 24.9 74.7

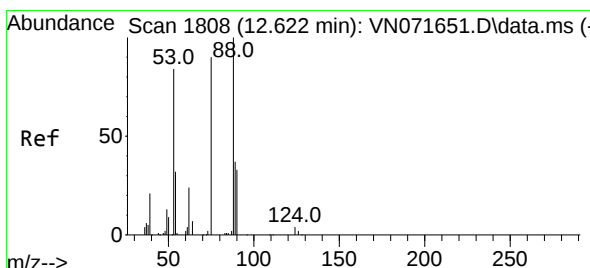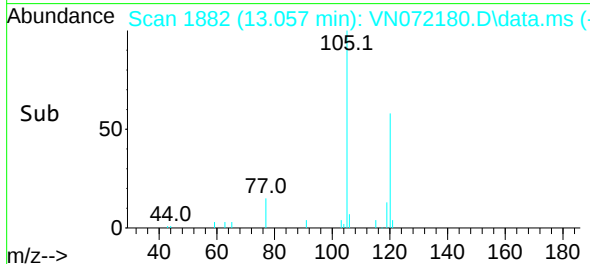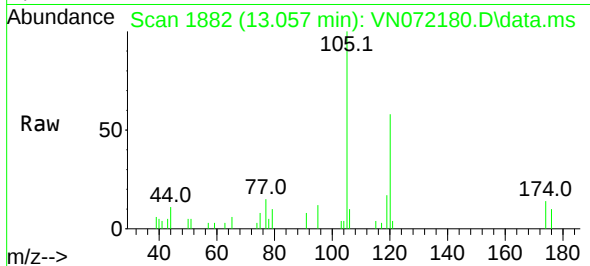

#81
trans-1,4-Dichloro-2-butene
Concen: 66.441 ug/l
RT: 12.727 min Scan# 1826
Delta R.T. 0.105 min
Lab File: VN072180.D
Acq: 25 Apr 2022 15:27

Tgt Ion: 75 Resp: 188289
Ion Ratio Lower Upper
75 100
53 0.6 78.0 117.0#
89 0.0 37.2 55.8#


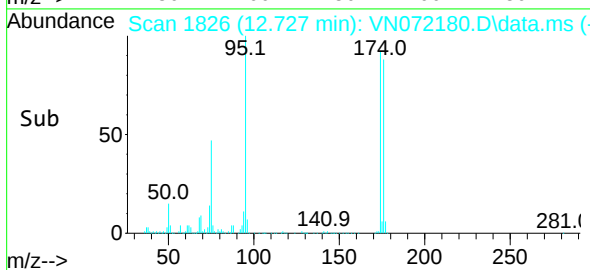

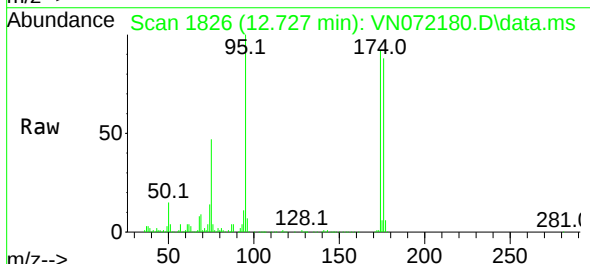




#84
1,2,4-Trimethylbenzene
Concen: 1.467 ug/l
RT: 13.363 min Scan# 1934
Delta R.T. -0.000 min
Lab File: VN072180.D
Acq: 25 Apr 2022 15:27




Instrument :
MSVOA_N
ClientSampleId :
33656-57


Tgt Ion:105 Resp: 36221
Ion Ratio Lower Upper
105 100
120 47.8 23.3 69.8



#85
sec-Butylbenzene
Concen: 1.208 ug/l
RT: 13.363 min Scan# 1934
Delta R.T. -0.135 min
Lab File: VN072180.D
Acq: 25 Apr 2022 15:27

Tgt Ion:105 Resp: 36221
Ion Ratio Lower Upper
105 100
134 0.0 10.4 31.1#


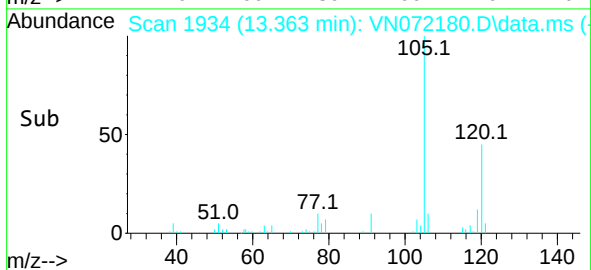

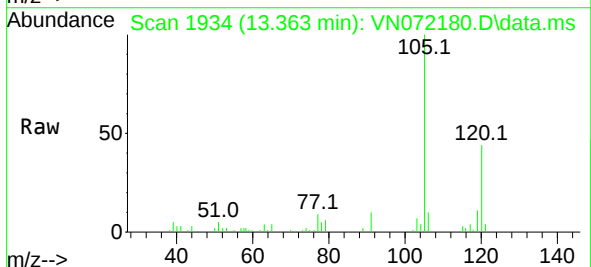


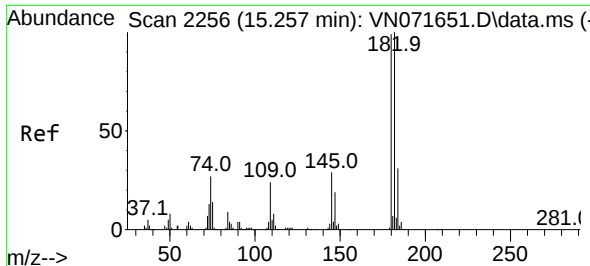

#93
 1,2,4-Trichlorobenzene
 Concen: 2.262 ug/l
 RT: 15.257 min Scan# 2110
 Delta R.T. -0.000 min
 Lab File: VN072180.D
 Acq: 25 Apr 2022 15:27




Instrument :
 MSVOA_N
 ClientSampleId :
 33656-57


Tgt Ion	Ratio	Lower	Upper
180	100		
182	97.8	47.5	142.5
145	24.8	14.5	43.5

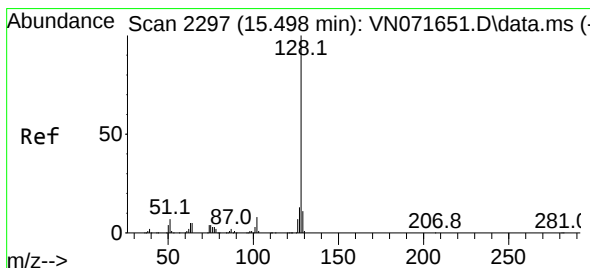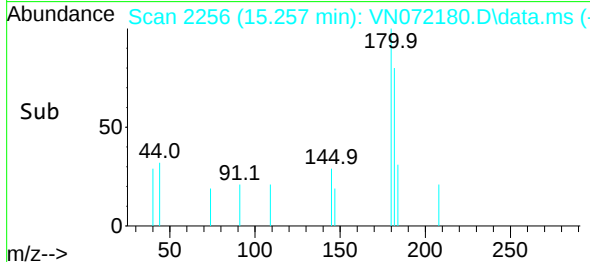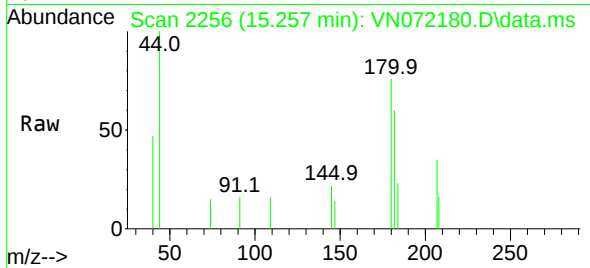

#95
 Naphthalene
 Concen: 29.227 ug/l
 RT: 15.504 min Scan# 2298
 Delta R.T. 0.006 min
 Lab File: VN072180.D
 Acq: 25 Apr 2022 15:27


Tgt Ion	Ratio	Lower	Upper
128	100		
127	12.8	10.3	15.5
129	10.9	8.6	13.0

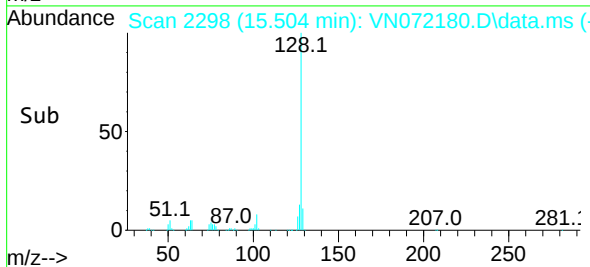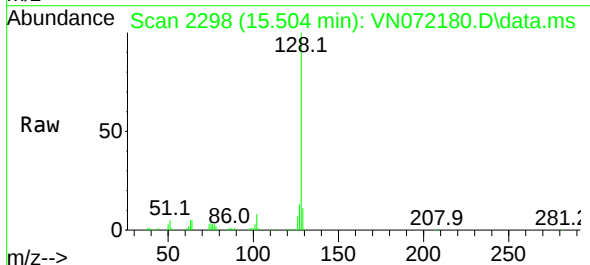



#96
 1,2,3-Trichlorobenzene
 Concen: 2.659 ug/l
 RT: 15.704 min Scan# 21
 Delta R.T. 0.012 min
 Lab File: VN072180.D
 Acq: 25 Apr 2022 15:27

Instrument :
 MSVOA_N
 ClientSampleId :
 33656-57

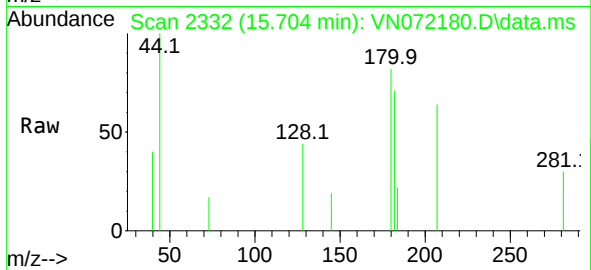

Tgt Ion:	180	Resp:	1501
Ion	Ratio	Lower	Upper
180	100		
182	102.2	47.8	143.3
145	29.7	15.5	46.5

