

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN042523\
 Data File : VN077469.D
 Acq On : 25 Apr 2023 14:06
 Operator : JC\MD
 Sample : VN0425WBL01
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0425WBL01

Quant Time: Apr 26 04:17:51 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N042423W.M
 Quant Title : SW846 8260
 QLast Update : Tue Apr 25 02:50:59 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.231	168	546217	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.101	114	992597	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.866	117	892826	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.795	152	313802	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.578	65	356267	49.985	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	99.960%
35) Dibromofluoromethane	8.172	113	309400	51.861	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	103.720%
50) Toluene-d8	10.572	98	1217679	53.255	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	106.520%
62) 4-Bromofluorobenzene	12.854	95	394635	52.753	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	105.500%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN042523\
Data File : VN077469.D
Acq On : 25 Apr 2023 14:06
Operator : JC\MD
Sample : VN0425WBL01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0425WBL01

Quant Time: Apr 26 04:17:51 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N042423W.M
Quant Title : SW846 8260
QLast Update : Tue Apr 25 02:50:59 2023
Response via : Initial Calibration




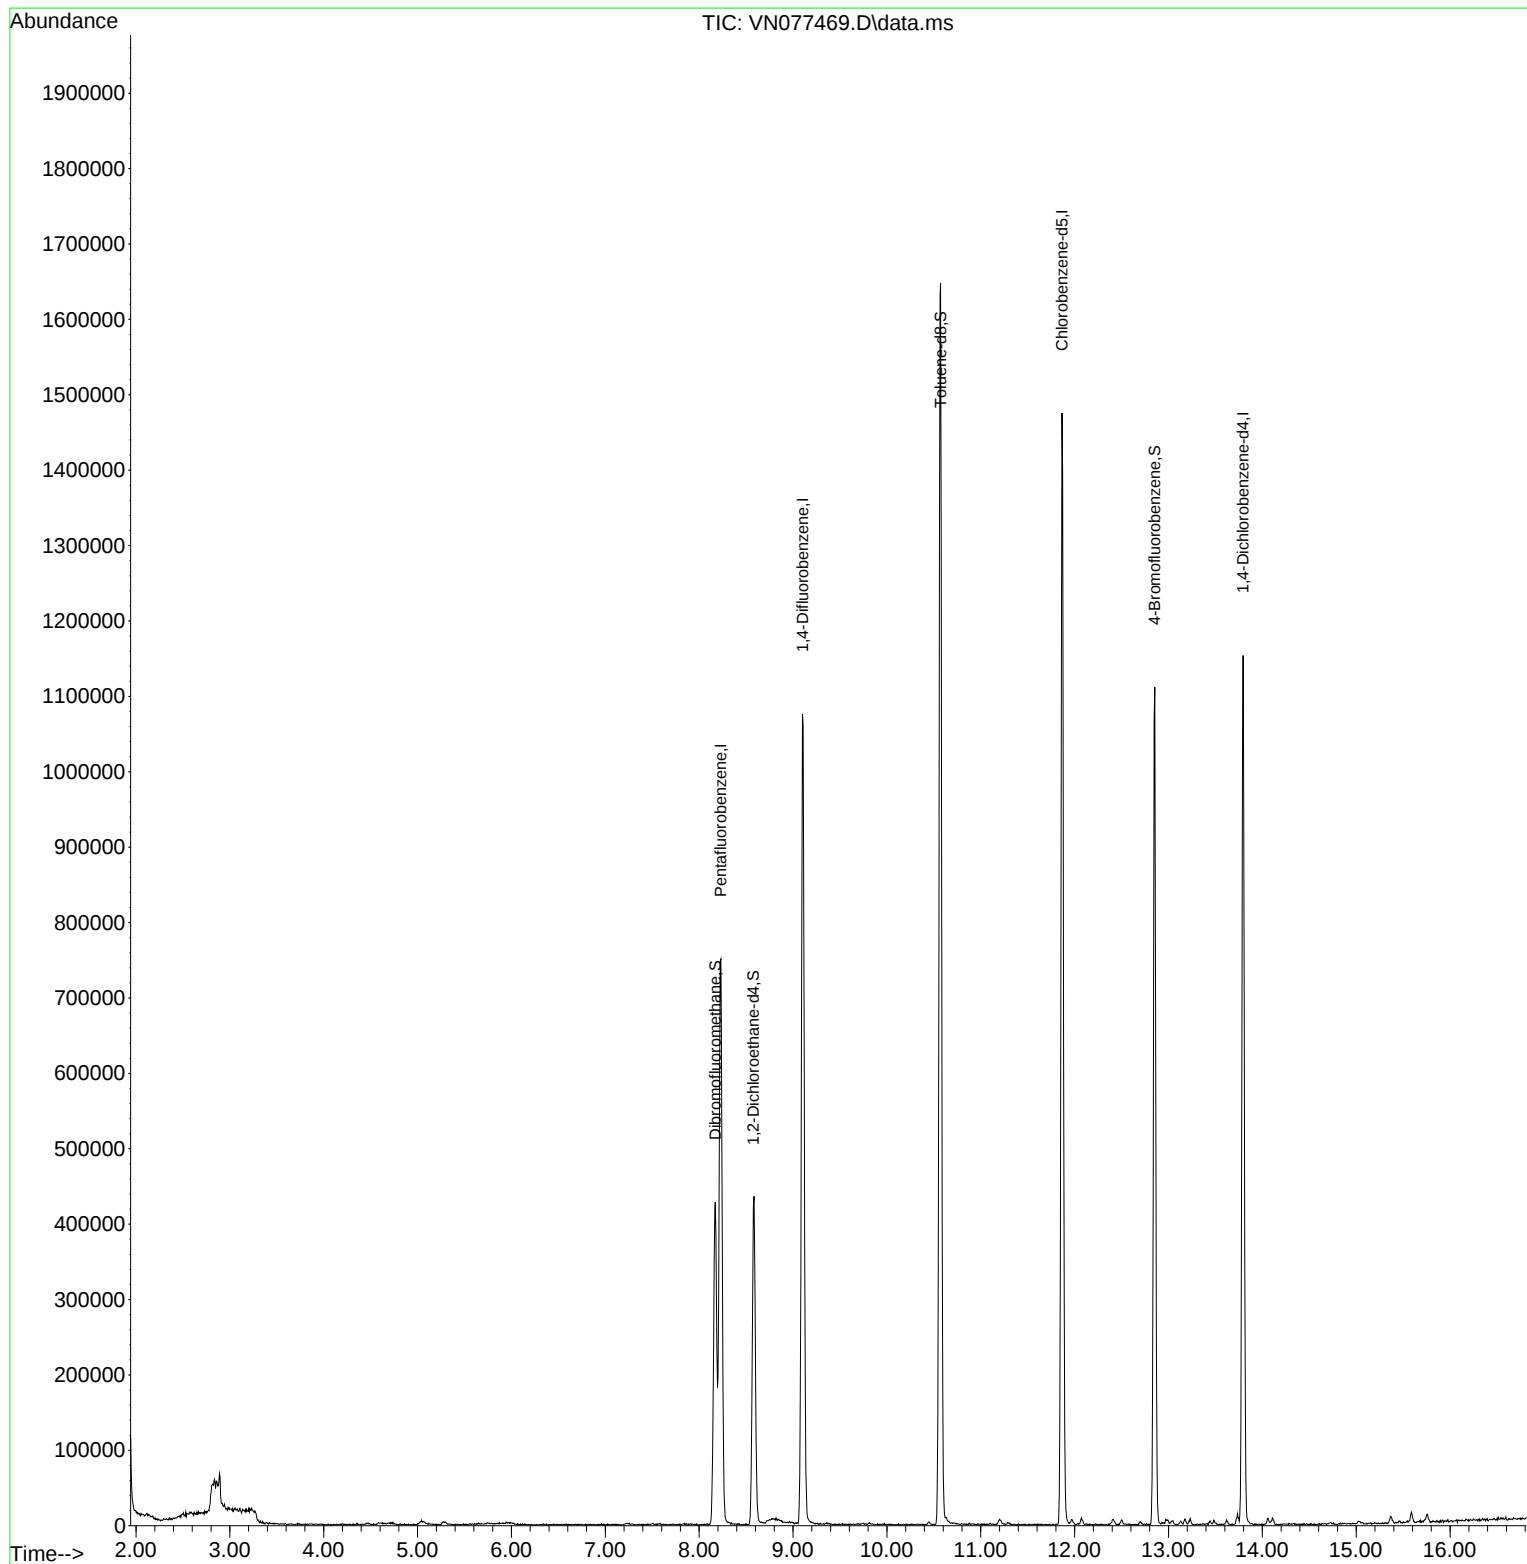


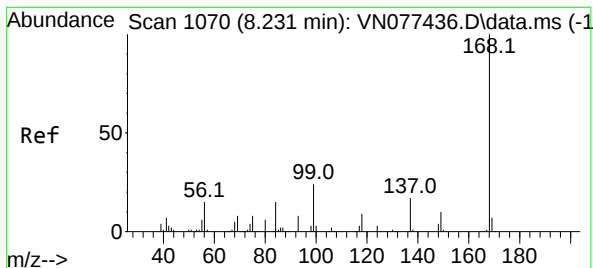

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.231 min Scan# 1129
Delta R.T. -0.000 min
Lab File: VN077469.D
Acq: 25 Apr 2023 14:06




Instrument :
MSVOA_N
ClientSampleId :
VN0425WBL01


Tgt Ion:168 Resp: 546217
Ion Ratio Lower Upper
168 100
99 65.2 53.0 79.6

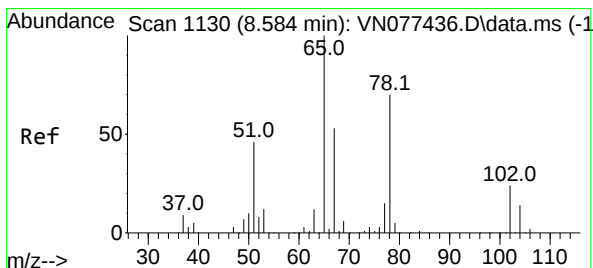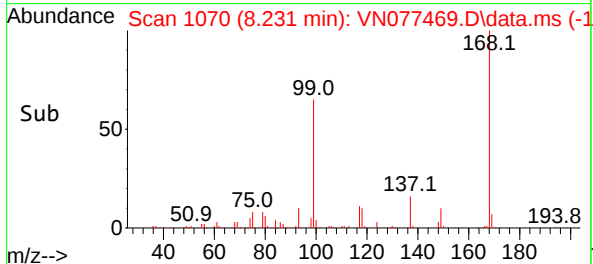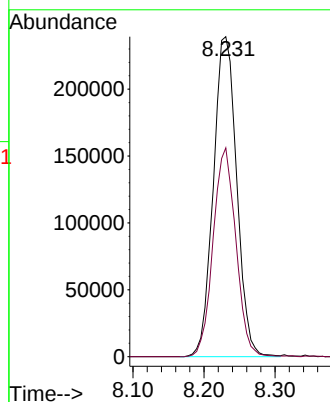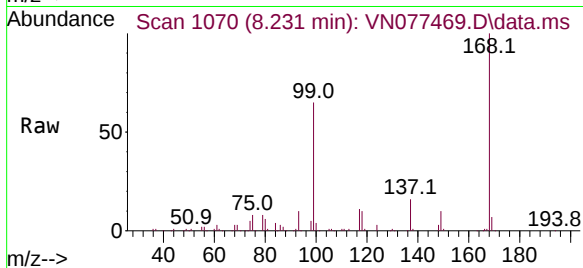

#33
1,2-Dichloroethane-d4
Concen: 49.985 ug/l
RT: 8.578 min Scan# 1129
Delta R.T. -0.006 min
Lab File: VN077469.D
Acq: 25 Apr 2023 14:06

Tgt Ion: 65 Resp: 356267
Ion Ratio Lower Upper
65 100
67 51.1 0.0 106.6

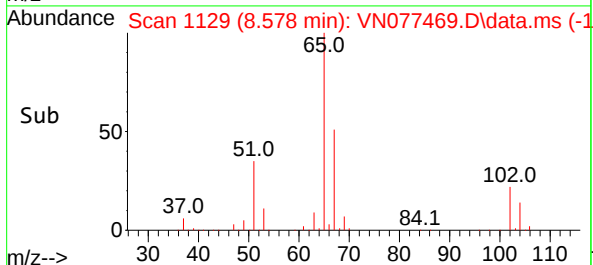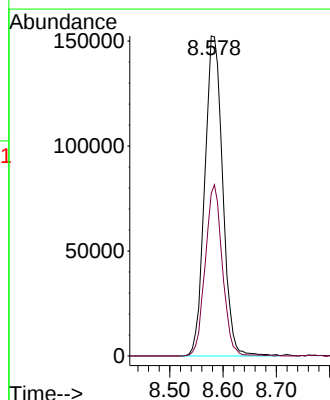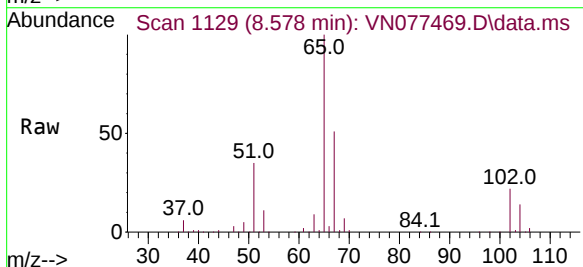

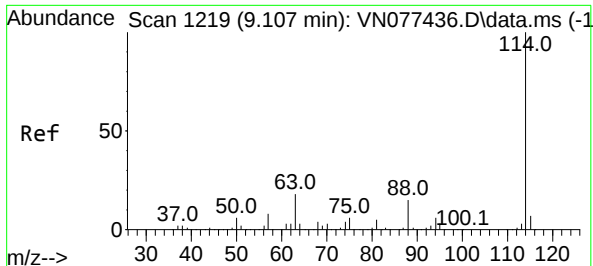

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.101 min Scan# 1

Delta R.T. -0.006 min

Lab File: VN077469.D

Acq: 25 Apr 2023 14:06

Instrument :

MSVOA_N

ClientSampleId :

VN0425WBL01





Tgt Ion:114 Resp: 992597

Ion Ratio Lower Upper

114 100

63 19.0 0.0 36.4

88 16.3 0.0 30.6

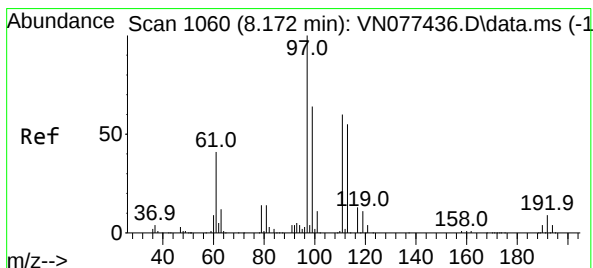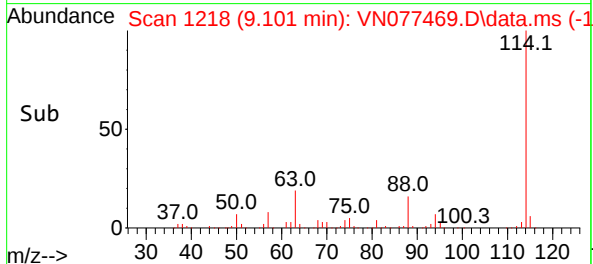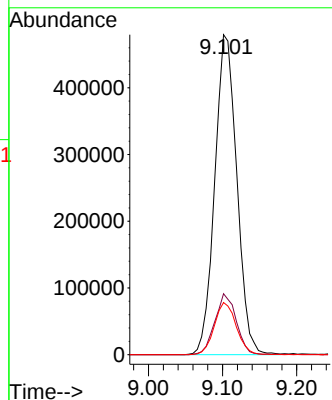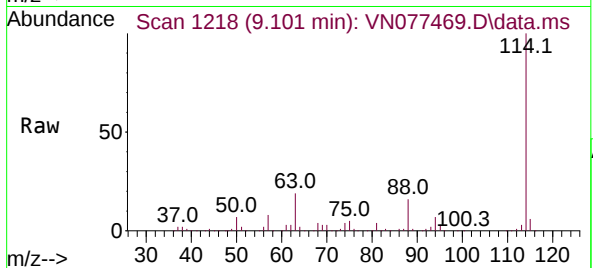

#35

Dibromofluoromethane

Concen: 51.861 ug/l

RT: 8.172 min Scan# 1060

Delta R.T. 0.000 min

Lab File: VN077469.D

Acq: 25 Apr 2023 14:06




Tgt Ion:113 Resp: 309400


Ion Ratio Lower Upper

113 100

111 103.2 82.6 123.8

192 16.0 12.7 19.1


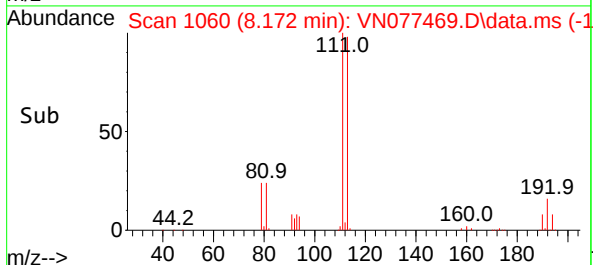
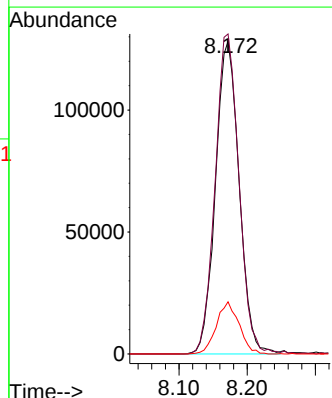
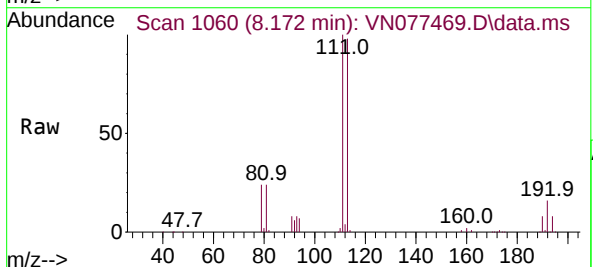


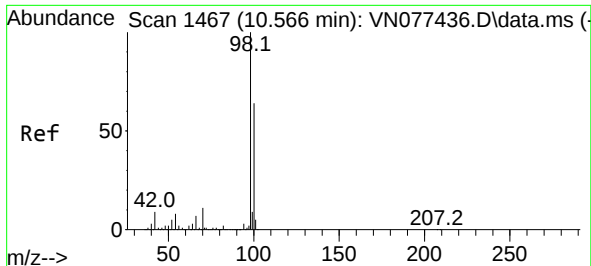

#50
Toluene-d8
Concen: 53.255 ug/l
RT: 10.572 min Scan# 1468
Delta R.T. 0.006 min
Lab File: VN077469.D
Acq: 25 Apr 2023 14:06




Instrument :
MSVOA_N
ClientSampleId :
VN0425WBL01


Tgt Ion: 98 Resp: 1217679
Ion Ratio Lower Upper
98 100
100 64.8 52.0 78.0

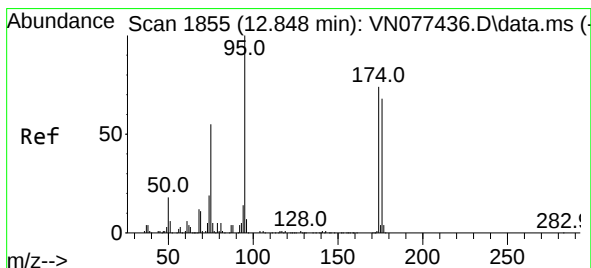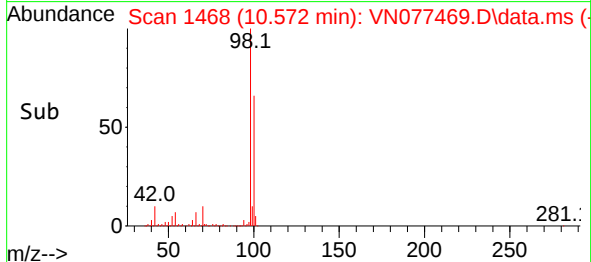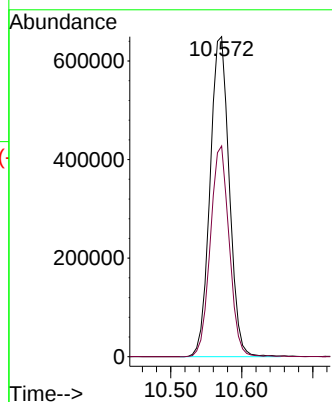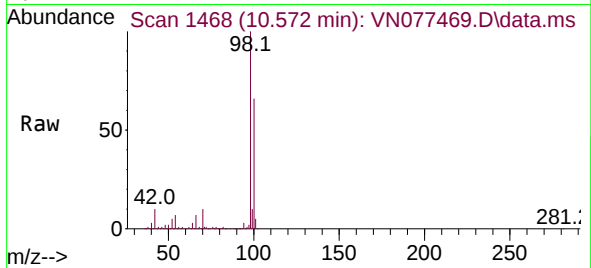

#62
4-Bromofluorobenzene
Concen: 52.753 ug/l
RT: 12.854 min Scan# 1856
Delta R.T. 0.006 min
Lab File: VN077469.D
Acq: 25 Apr 2023 14:06

Tgt Ion: 95 Resp: 394635
Ion Ratio Lower Upper
95 100
174 72.0 0.0 143.8
176 68.3 0.0 135.8


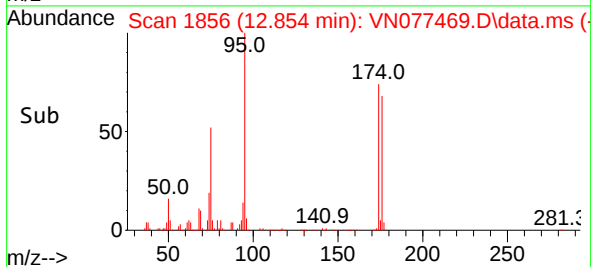
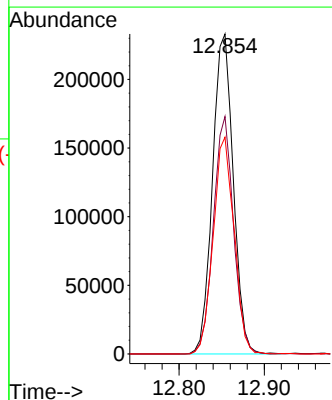
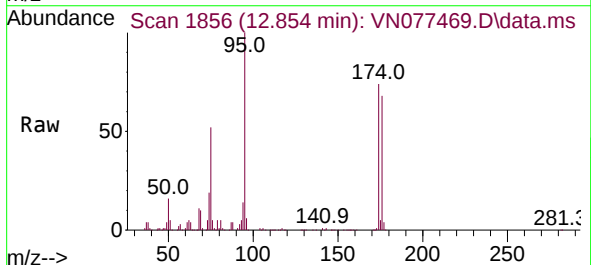


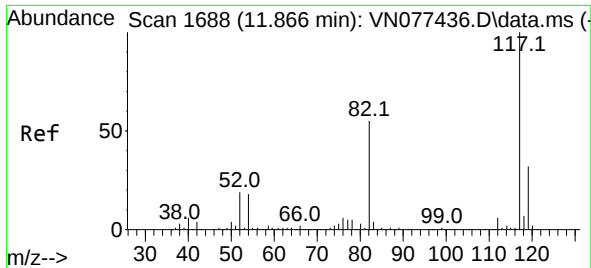

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.866 min Scan# 117
Delta R.T. 0.000 min
Lab File: VN077469.D
Acq: 25 Apr 2023 14:06

Instrument :
MSVOA_N
ClientSampleId :
VN0425WBL01

Tgt Ion:117 Resp: 892826
Ion Ratio Lower Upper
117 100
82 55.6 44.0 66.0
119 31.7 25.6 38.4

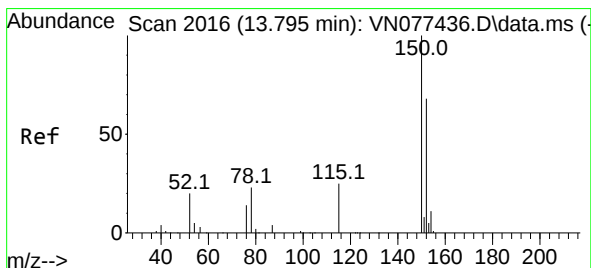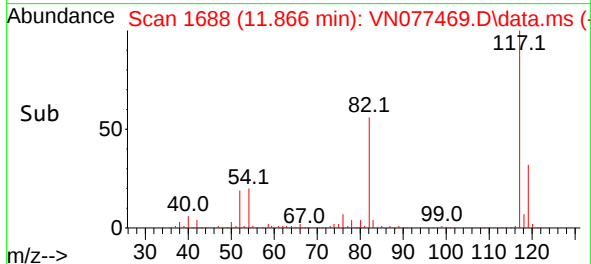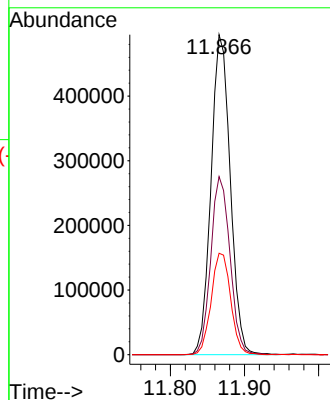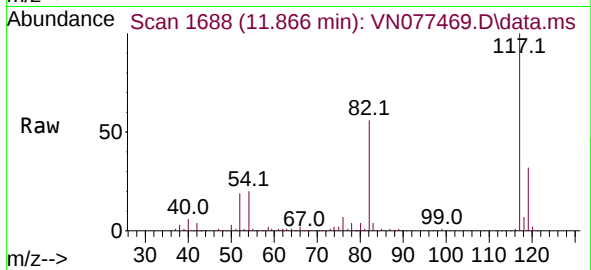

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.795 min Scan# 2016
Delta R.T. 0.000 min
Lab File: VN077469.D
Acq: 25 Apr 2023 14:06

Tgt Ion:152 Resp: 313802
Ion Ratio Lower Upper
152 100
115 64.1 32.3 96.8
150 158.9 0.0 355.8

