
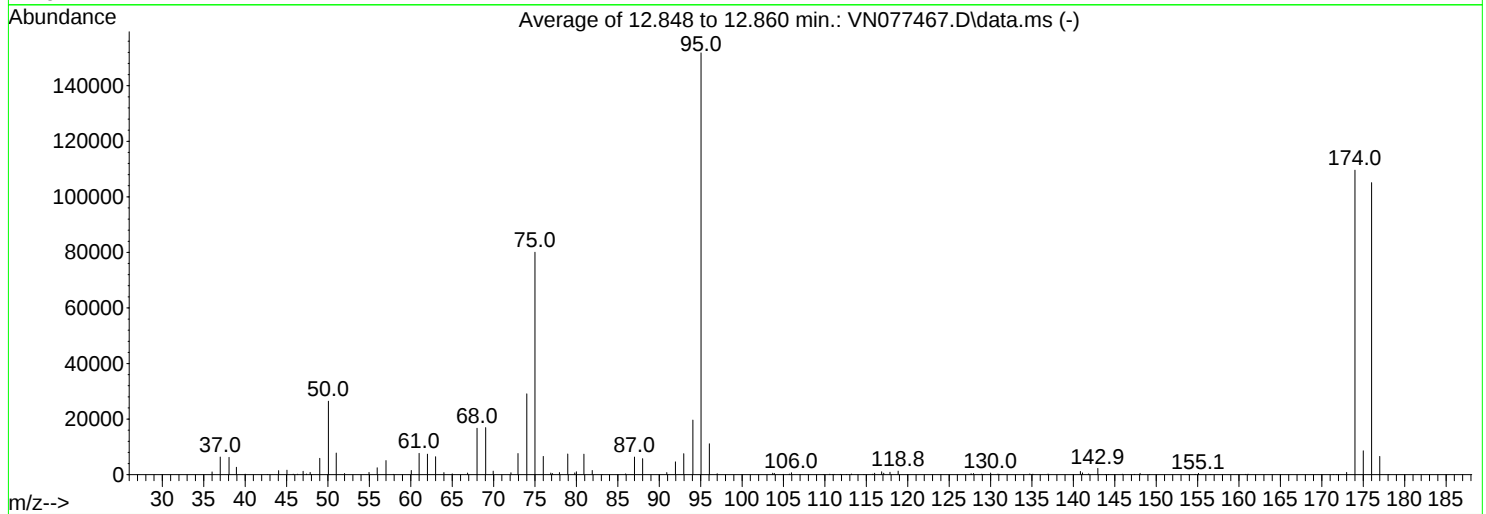


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN042523\
Data File : VN077467.D
Acq On : 25 Apr 2023 12:59
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N042423W.M
Title : SW846 8260
Last Update : Tue Apr 25 02:50:59 2023

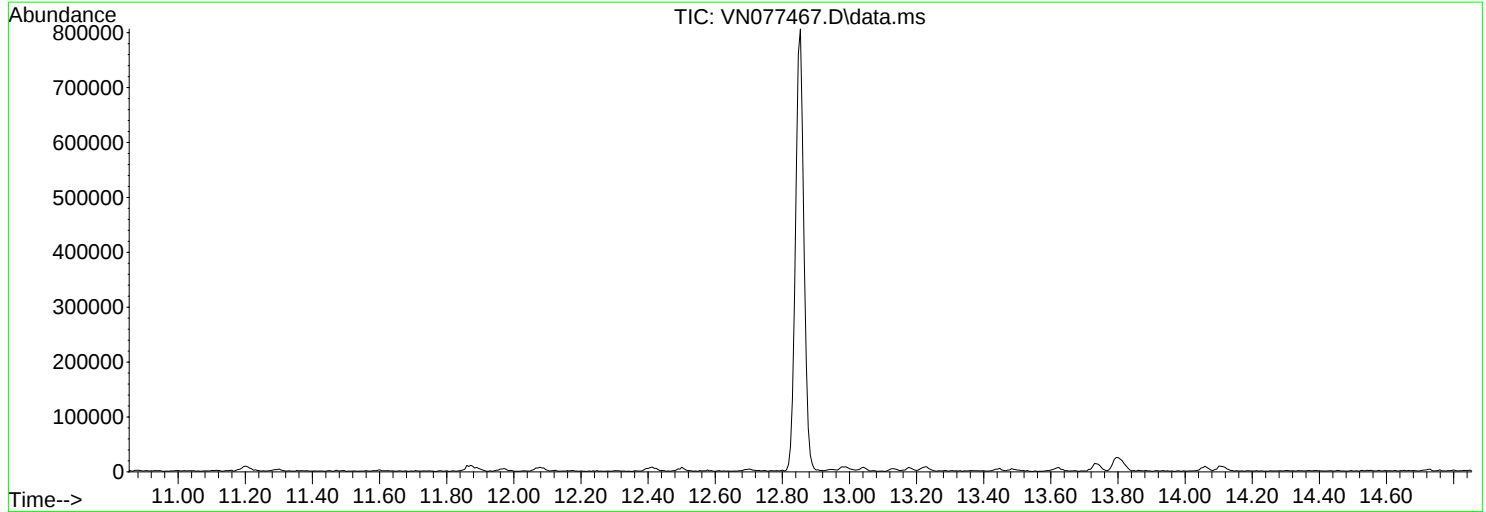

AutoFind: Scans 1855, 1856, 1857; Background Corrected with Scan 1846

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.4	26469	PASS
75	95	30	60	52.7	80061	PASS
95	95	100	100	100.0	151835	PASS
96	95	5	9	7.3	11103	PASS
173	174	0.00	2	0.7	795	PASS
174	95	50	100	72.2	109603	PASS
175	174	5	9	7.9	8614	PASS
176	174	95	101	95.9	105136	PASS
177	176	5	9	6.2	6554	PASS

Average of 12.848 to 12.860 min.: VN077467.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	965	47.40	251	61.00	7680	74.00	2910
37.00	6348	47.85	820	62.00	7389	75.00	8006
38.05	6231	49.00	5899	63.00	6444	76.00	656
38.95	2626	50.05	26469	64.00	767	76.90	59
40.00	206	51.00	7754	65.00	278	77.10	432
42.70	75	52.00	386	66.85	555	77.95	742
44.05	1425	54.95	825	68.00	16726	78.95	7435
45.05	1610	55.95	2473	69.05	16954	79.80	667
45.80	201	57.00	5084	69.95	1283	80.00	1051
46.35	175	57.90	131	72.10	719	80.90	7387
47.00	1223	60.05	1516	72.95	7614	81.90	1514

Average of 12.848 to 12.860 min.: VN077467.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
83.10	87	103.70	501	112.60	55	127.95	429
85.95	275	103.90	482	113.20	225	128.95	189
87.00	6348	104.95	128	114.70	89	129.20	63
88.00	5741	105.70	253	115.80	163	130.00	574
90.90	770	105.95	675	116.00	528	130.90	218
91.95	4605	107.00	68	116.85	1027	131.10	113
92.95	7531	109.80	52	117.10	533	134.75	274
94.05	19638	110.60	152	117.85	856	135.10	169
95.05	151835	110.90	83	118.85	1299	136.95	214
96.05	11103	111.10	130	124.00	93	140.85	1167
97.00	357	111.85	133	127.65	348	141.10	619

Average of 12.848 to 12.860 min.: VN077467.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
141.85	283	155.10	462	178.10	78		
142.95	2247	156.60	77				
143.90	83	160.80	110				
144.20	51	161.10	152				
145.00	61	171.40	92				
145.90	204	171.80	82				
147.40	105	173.00	795				
148.05	484	174.00	109603				
149.20	51	175.00	8614				
153.90	63	176.00	105136				
154.70	148	177.00	6554				

Instrument :

MSVOA_N

ClientSampleId :

BFB