

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN042524\
 Data File : VN081855.D
 Acq On : 25 Apr 2024 17:04
 Operator : JC\MD
 Sample : P2257-05
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 41C

Quant Time: Apr 26 05:38:02 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N042524W.M
 Quant Title : SW846 8260
 QLast Update : Fri Apr 26 05:26:49 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) Pentafluorobenzene	8.224	168	221533	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.100	114	410476	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	364661	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	150782	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.576	65	172536	46.146	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	92.300%
35) Dibromofluoromethane	8.165	113	124518	50.383	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	100.760%
50) Toluene-d8	10.565	98	513855	52.940	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	105.880%
62) 4-Bromofluorobenzene	12.847	95	193096	50.325	ug/l	0.00
Spiked Amount	50.000	Range	64 - 133	Recovery	=	100.660%
Target Compounds						
					Qvalue	
3) Chloromethane	2.371	50	1029	0.317	ug/l	99
5) Bromomethane	2.942	94	495	Below Cal	#	3
10) Methyl Iodide	4.612	142	941	0.407	ug/l	# 40
11) Tert butyl alcohol	5.524	59	12527	18.430	ug/l	# 81
13) Acrolein	4.183	56	895	Below Cal	#	15
16) Acetone	4.424	43	28881	21.116	ug/l	91
17) Carbon Disulfide	4.730	76	13750	1.705	ug/l	# 86
18) Methyl Acetate	5.024	43	91126	24.062	ug/l	# 89
25) 2-Butanone	7.477	43	1097857	517.345	ug/l	# 86
29) Tetrahydrofuran	7.824	42	782	0.514	ug/l	# 39
31) Cyclohexane	8.229	56	7838	1.392	ug/l	# 41
36) 1,1-Dichloropropene	8.224	75	22125	5.503	ug/l	# 49
37) Ethyl Acetate	7.477	43	1097857	252.543	ug/l	# 68
38) Carbon Tetrachloride	8.224	117	24409	6.211	ug/l	# 17
40) Benzene	8.612	78	10721	0.888	ug/l	# 89
41) Methacrylonitrile	7.765	41	650	0.234	ug/l	# 43
43) Isopropyl Acetate	8.647	43	112684	13.786	ug/l	# 53
48) Methyl methacrylate	9.659	41	24140	6.186	ug/l	# 36
49) 1,4-Dioxane	9.700	88	1474	24.853	ug/l	# 15
51) 4-Methyl-2-Pentanone	10.447	43	2159	0.469	ug/l	# 34
52) Toluene	10.629	92	9120	1.262	ug/l	91
59) 2-Hexanone	11.188	43	1237	0.361	ug/l	65
67) Ethyl Benzene	11.965	91	5656	0.382	ug/l	96
68) m/p-Xylenes	12.065	106	7754	1.468	ug/l	81
69) o-Xylene	12.400	106	3876	0.752	ug/l	94
70) Styrene	12.417	104	7571	0.849	ug/l	93
74) N-amyl acetate	12.417	43	62827	8.418	ug/l	# 1
76) 1,2,3-Trichloropropane	12.847	75	106070	27.132	ug/l	# 1
80) 1,3,5-Trimethylbenzene	13.170	105	2303	0.203	ug/l	90
81) trans-1,4-Dichloro-2-b...	12.847	75	106070	55.596	ug/l	# 13
84) 1,2,4-Trimethylbenzene	13.482	105	9758	0.861	ug/l	95
90) Hexachloroethane	14.294	117	630	0.300	ug/l	# 17
95) Naphthalene	15.647	128	4877	0.460	ug/l	# 82


(#) = qualifier out of range (m) = manual integration (+) = signals summed


Instrument :
MSVOA_N
ClientSampleId :
41C

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN042524\
Data File : VN081855.D
Acq On : 25 Apr 2024 17:04
Operator : JC\MD
Sample : P2257-05
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
41C

Quant Time: Apr 26 05:38:02 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N042524W.M
Quant Title : SW846 8260
QLast Update : Fri Apr 26 05:26:49 2024
Response via : Initial Calibration

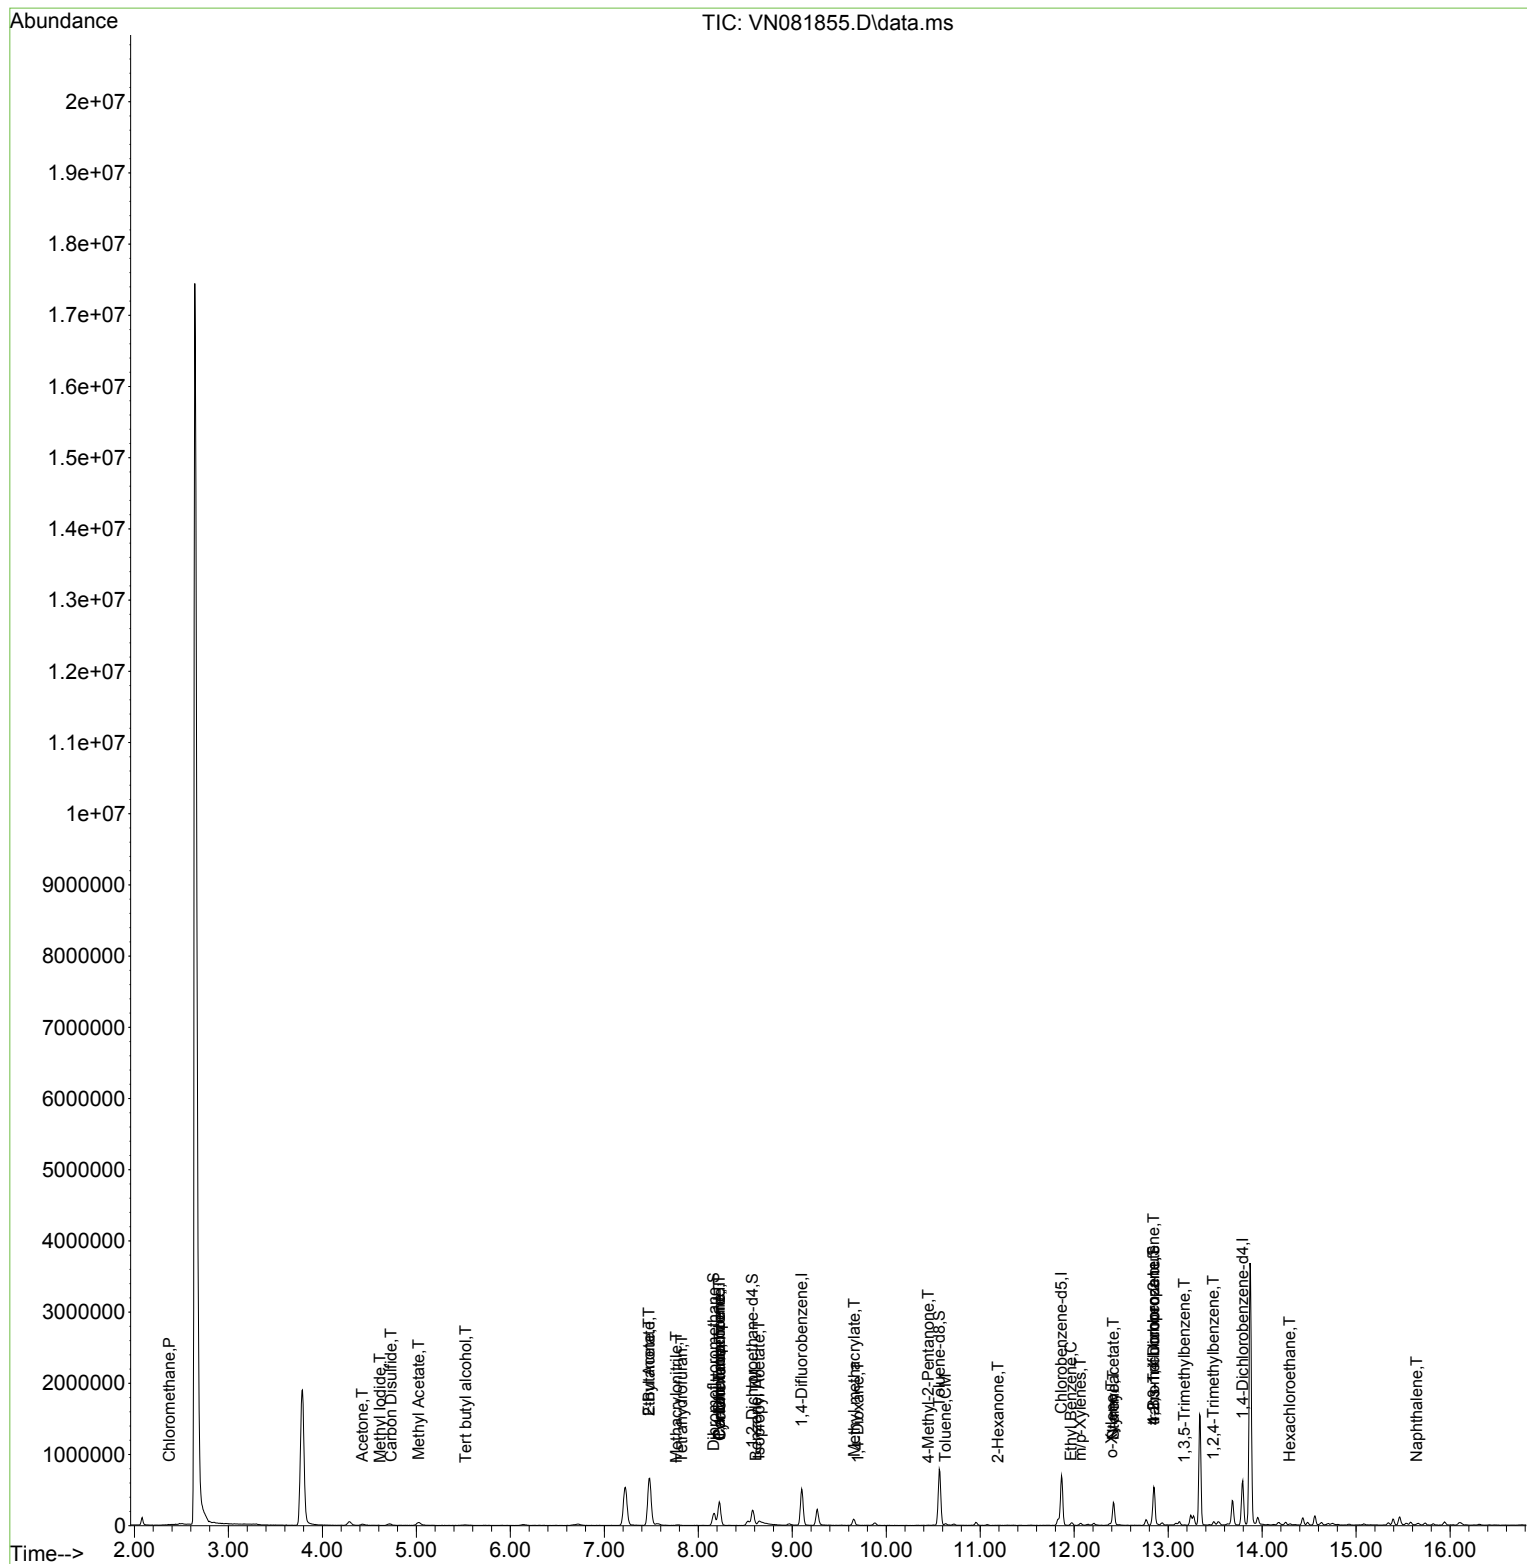



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 8.224 min Scan# 1

Delta R.T. -0.000 min

Lab File: VN081855.D

Acq: 25 Apr 2024 17:04

Instrument :

MSVOA_N

ClientSampleId :





41C

Tgt Ion:168 Resp: 221533

Ion Ratio Lower Upper

168 100

99 67.8 48.2 72.4

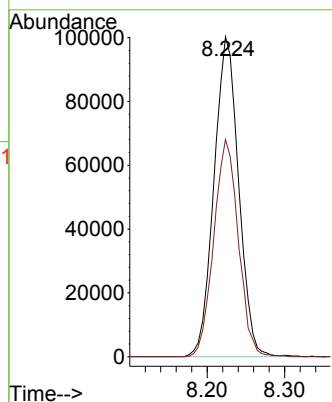

#3

Chloromethane

Concen: 0.317 ug/l

RT: 2.371 min Scan# 71

Delta R.T. 0.012 min

Lab File: VN081855.D




Acq: 25 Apr 2024 17:04


Tgt Ion: 50 Resp: 1029

Ion Ratio Lower Upper

50 100

52 31.3 25.5 38.3


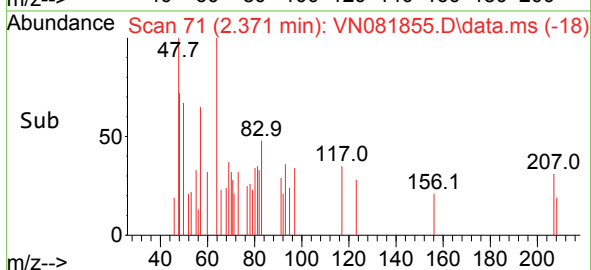






#5
Bromomethane
Concen: Below Cal
RT: 2.942 min Scan# 1
Delta R.T. -0.006 min
Lab File: VN081855.D
Acq: 25 Apr 2024 17:04




Instrument :
MSVOA_N
ClientSampleId :
41C


Tgt Ion: 94 Resp: 495
Ion Ratio Lower Upper
94 100
96 0.0 74.8 112.2#

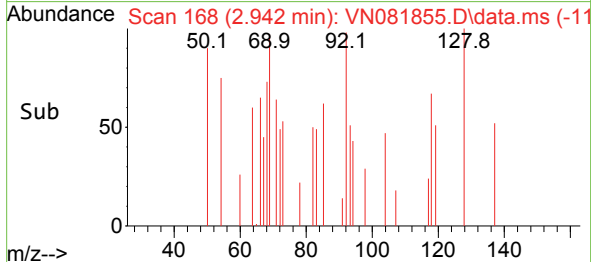

#10
Methyl Iodide
Concen: 0.407 ug/l
RT: 4.612 min Scan# 452
Delta R.T. 0.023 min
Lab File: VN081855.D
Acq: 25 Apr 2024 17:04

Tgt Ion:142 Resp: 941
Ion Ratio Lower Upper
142 100
127 0.0 35.8 53.6#
141 0.0 11.4 17.2#





#11

Tert butyl alcohol

Concen: 18.430 ug/l

RT: 5.524 min Scan# 606

Delta R.T. 0.006 min

Lab File: VN081855.D

Acq: 25 Apr 2024 17:04

Instrument :

MSVOA_N

ClientSampleId :





41C

Tgt Ion: 59 Resp: 12527

Ion Ratio Lower Upper

59 100

57 4.0 8.9 13.3#

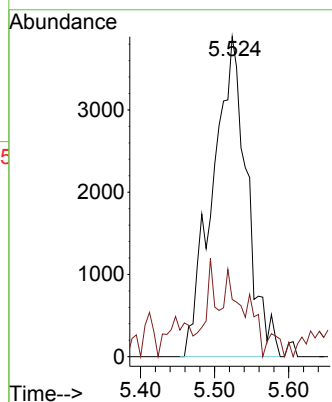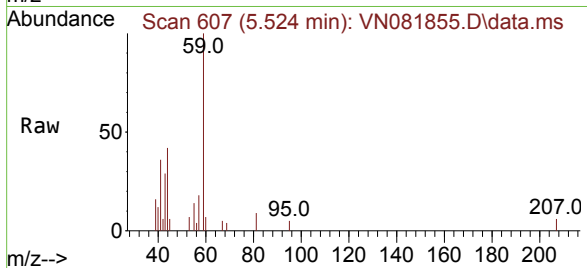

#13

Acrolein

Concen: Below Cal

RT: 4.183 min Scan# 379

Delta R.T. 0.006 min

Lab File: VN081855.D




Acq: 25 Apr 2024 17:04


Tgt Ion: 56 Resp: 895

Ion Ratio Lower Upper

56 100

55 0.0 55.8 83.8#

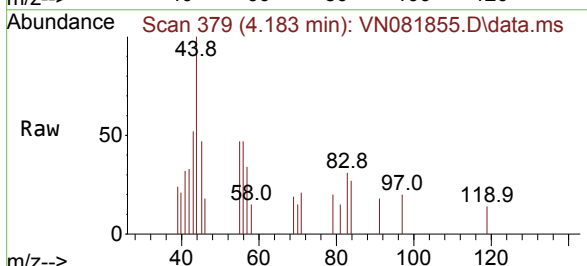



#16

Acetone

Concen: 21.116 ug/l

RT: 4.424 min Scan# 41

Delta R.T. -0.000 min

Lab File: VN081855.D

Acq: 25 Apr 2024 17:04

Instrument :

MSVOA_N

ClientSampleId :





41C

Tgt Ion: 43 Resp: 28881

Ion Ratio Lower Upper

43 100

58 26.4 25.2 37.8

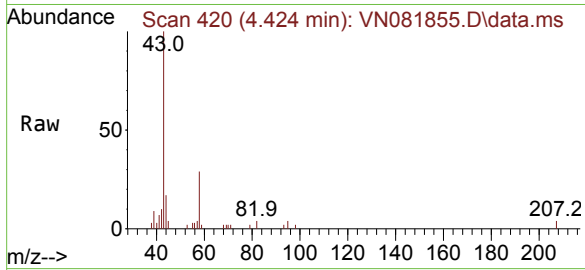

#17

Carbon Disulfide

Concen: 1.705 ug/l

RT: 4.730 min Scan# 472

Delta R.T. 0.018 min

Lab File: VN081855.D




Acq: 25 Apr 2024 17:04


Tgt Ion: 76 Resp: 13750

Ion Ratio Lower Upper

76 100

78 4.2 7.5 11.3#




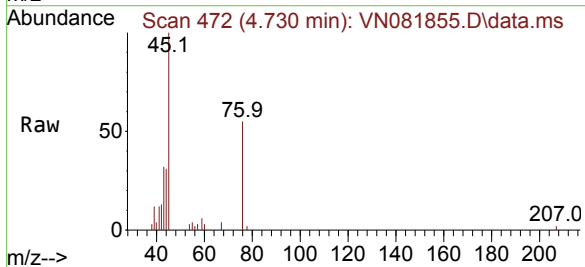




#18
Methyl Acetate
Concen: 24.062 ug/l
RT: 5.024 min Scan# 51
Delta R.T. 0.006 min
Lab File: VN081855.D
Acq: 25 Apr 2024 17:04




Instrument :
MSVOA_N
ClientSampleId :
41C


Tgt Ion: 43 Resp: 91126
Ion Ratio Lower Upper
43 100
74 22.0 22.2 33.2#

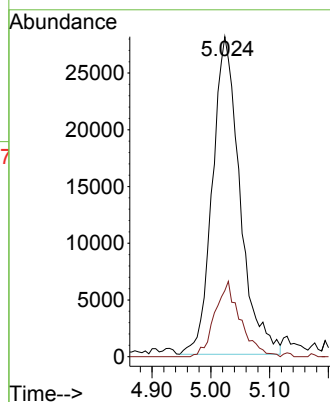

#25
2-Butanone
Concen: 517.345 ug/l
RT: 7.477 min Scan# 939
Delta R.T. -0.000 min
Lab File: VN081855.D
Acq: 25 Apr 2024 17:04

Tgt Ion: 43 Resp: 1097857
Ion Ratio Lower Upper
43 100
72 24.0 25.3 37.9#

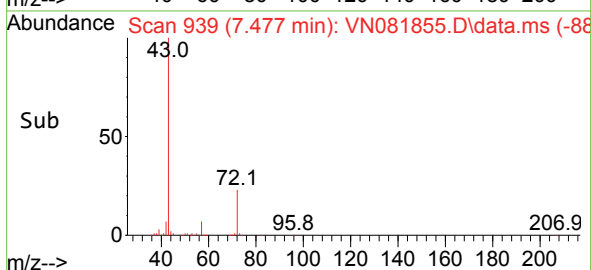



#29

Tetrahydrofuran

Concen: 0.514 ug/l

RT: 7.824 min Scan# 91

Delta R.T. -0.012 min

Lab File: VN081855.D

Acq: 25 Apr 2024 17:04

Instrument :

MSVOA_N

ClientSampleId :

41C





Tgt Ion: 42 Resp: 782

Ion Ratio Lower Upper

42 100

72 0.0 39.3 58.9#

71 14.1 37.4 56.0#



#31

Cyclohexane

Concen: 1.392 ug/l

RT: 8.229 min Scan# 1067

Delta R.T. -0.029 min

Lab File: VN081855.D

Acq: 25 Apr 2024 17:04




Tgt Ion: 56 Resp: 7838


Ion Ratio Lower Upper

56 100

69 114.2 24.4 36.6#

84 125.0 77.0 115.4#

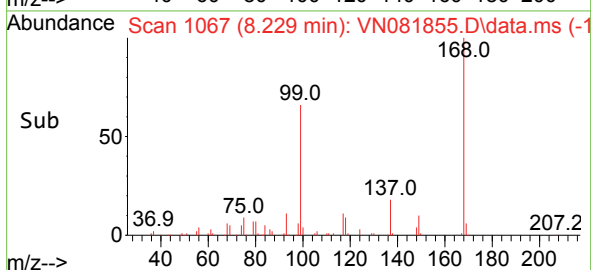



#33

1,2-Dichloroethane-d4

Concen: 46.146 ug/l

RT: 8.576 min Scan# 1126

Delta R.T. -0.000 min

Lab File: VN081855.D

Acq: 25 Apr 2024 17:04

Instrument :

MSVOA_N

ClientSampleId :





41C

Tgt Ion: 65 Resp: 172536

Ion Ratio Lower Upper

65 100

67 52.1 0.0 103.0



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.100 min Scan# 1215

Delta R.T. -0.000 min

Lab File: VN081855.D

Acq: 25 Apr 2024 17:04




Tgt Ion: 114 Resp: 410476


Ion Ratio Lower Upper

114 100

63 22.9 0.0 41.0

88 17.6 0.0 31.4

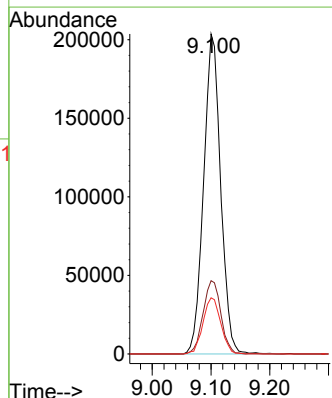



#35

Dibromofluoromethane

Concen: 50.383 ug/l

RT: 8.165 min Scan# 1056

Delta R.T. -0.000 min

Lab File: VN081855.D

Acq: 25 Apr 2024 17:04

Instrument :

MSVOA_N

ClientSampleId :

41C





Tgt Ion:113 Resp: 124518

Ion Ratio Lower Upper

113 100

111 102.5 83.4 125.2

192 15.8 14.0 21.0



#36

1,1-Dichloropropene

Concen: 5.503 ug/l

RT: 8.224 min Scan# 1066

Delta R.T. -0.147 min

Lab File: VN081855.D

Acq: 25 Apr 2024 17:04




Tgt Ion: 75 Resp: 22125


Ion Ratio Lower Upper

75 100

110 8.4 17.8 53.5#


77 0.0 25.0 37.4#








#37
Ethyl Acetate
Concen: 252.543 ug/l
RT: 7.477 min Scan# 91
Delta R.T. -0.082 min
Lab File: VN081855.D
Acq: 25 Apr 2024 17:04

Instrument :
MSVOA_N
ClientSampleId :
41C







Tgt Ion: 43 Resp: 1097857
Ion Ratio Lower Upper
43 100
61 0.0 11.3 16.9#
70 0.0 8.7 13.1#

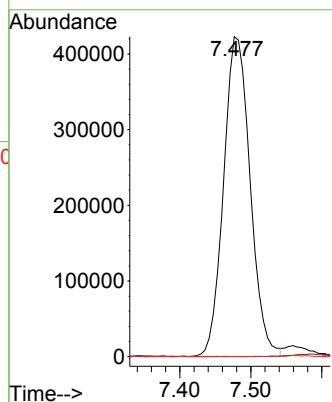

#38
Carbon Tetrachloride
Concen: 6.211 ug/l
RT: 8.224 min Scan# 1066
Delta R.T. -0.135 min
Lab File: VN081855.D
Acq: 25 Apr 2024 17:04

Tgt Ion: 117 Resp: 24409
Ion Ratio Lower Upper
117 100
119 6.5 76.5 114.7#
121 0.0 23.9 35.9#



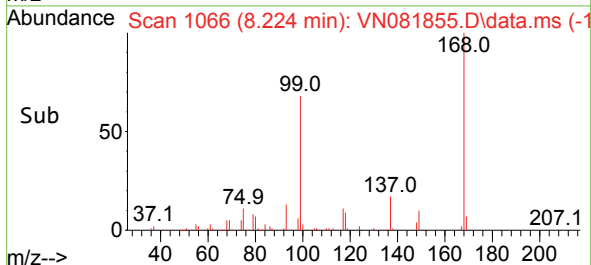





#40
Benzene
Concen: 0.888 ug/l
RT: 8.612 min Scan# 1131
Delta R.T. 0.006 min
Lab File: VN081855.D
Acq: 25 Apr 2024 17:04




Instrument :
MSVOA_N
ClientSampleId :
41C


Tgt Ion: 78 Resp: 10721
Ion Ratio Lower Upper
78 100
77 19.3 20.0 30.0#

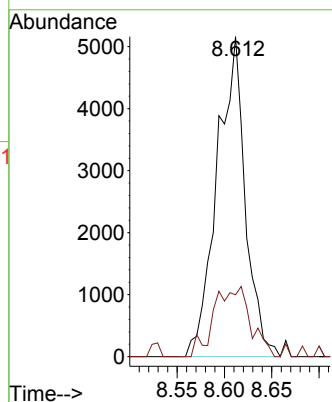

#41
Methacrylonitrile
Concen: 0.234 ug/l
RT: 7.765 min Scan# 988
Delta R.T. -0.012 min
Lab File: VN081855.D
Acq: 25 Apr 2024 17:04


Tgt Ion: 41 Resp: 650
Ion Ratio Lower Upper
41 100
39 131.1 46.6 69.8#
67 59.7 67.3 100.9#
52 0.0 27.3 40.9#

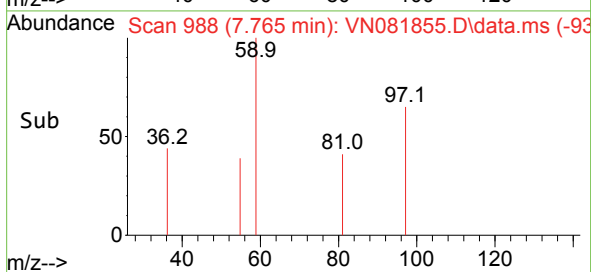






#43
Isopropyl Acetate
Concen: 13.786 ug/l
RT: 8.647 min Scan# 1138
Delta R.T. -0.041 min
Lab File: VN081855.D
Acq: 25 Apr 2024 17:04

Instrument :
MSVOA_N
ClientSampleId :
41C







Tgt Ion: 43 Resp: 112684
Ion Ratio Lower Upper
43 100
61 0.8 22.8 34.2#
87 0.0 12.0 18.0#

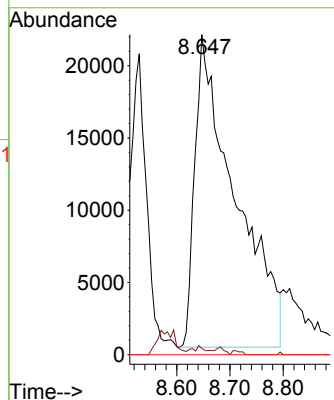

#48
Methyl methacrylate
Concen: 6.186 ug/l
RT: 9.659 min Scan# 1310
Delta R.T. -0.024 min
Lab File: VN081855.D
Acq: 25 Apr 2024 17:04

Tgt Ion: 41 Resp: 24140
Ion Ratio Lower Upper
41 100
69 1.1 77.9 116.9#
39 54.0 50.9 76.3



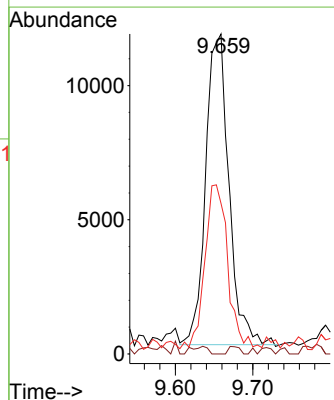
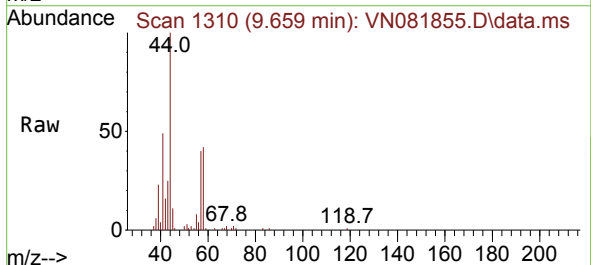




#49
1,4-Dioxane
Concen: 24.853 ug/l
RT: 9.700 min Scan# 11
Delta R.T. 0.006 min
Lab File: VN081855.D
Acq: 25 Apr 2024 17:04




Instrument :
MSVOA_N
ClientSampleId :
41C


Tgt Ion: 88 Resp: 1474
Ion Ratio Lower Upper
88 100
43 70.4 19.0 28.6#
58 0.0 50.6 76.0#

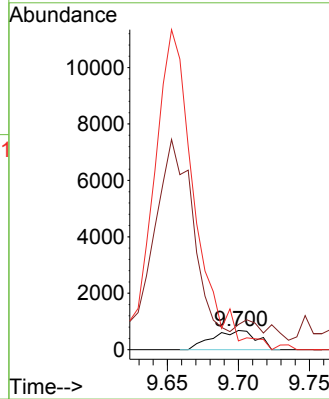

#50
Toluene-d8
Concen: 52.940 ug/l
RT: 10.565 min Scan# 1464
Delta R.T. -0.000 min
Lab File: VN081855.D
Acq: 25 Apr 2024 17:04

Tgt Ion: 98 Resp: 513855
Ion Ratio Lower Upper
98 100
100 65.3 51.8 77.6

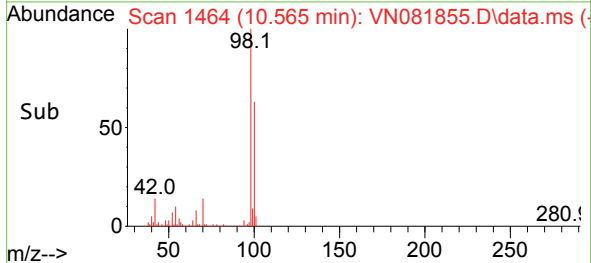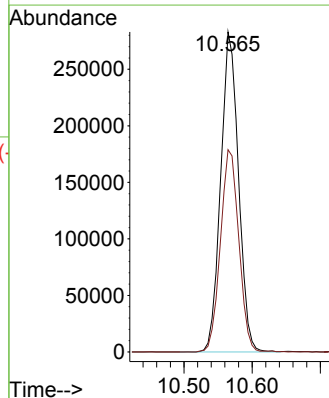



#51

4-Methyl-2-Pentanone

Concen: 0.469 ug/l

RT: 10.447 min Scan# 1444

Delta R.T. -0.000 min

Lab File: VN081855.D

Acq: 25 Apr 2024 17:04

Instrument :

MSVOA_N

ClientSampleId :





41C

Tgt Ion: 43 Resp: 2159

Ion Ratio Lower Upper

43 100

58 0.0 33.2 49.8#

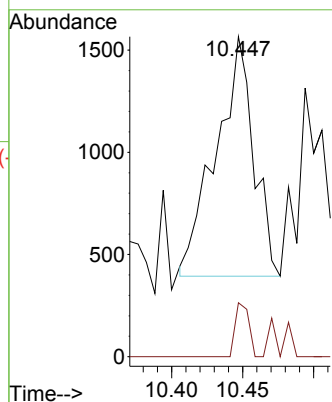

#52

Toluene

Concen: 1.262 ug/l

RT: 10.629 min Scan# 1475

Delta R.T. -0.000 min

Lab File: VN081855.D




Acq: 25 Apr 2024 17:04


Tgt Ion: 92 Resp: 9120

Ion Ratio Lower Upper

92 100

91 159.1 136.7 205.1


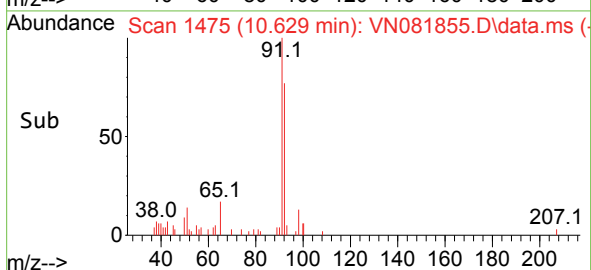






#59
2-Hexanone
Concen: 0.361 ug/l
RT: 11.188 min Scan# 1570
Delta R.T. -0.006 min
Lab File: VN081855.D
Acq: 25 Apr 2024 17:04




Instrument :
MSVOA_N
ClientSampleId :
41C


Tgt Ion: 43 Resp: 1237
Ion Ratio Lower Upper
43 100
58 31.3 28.3 84.9

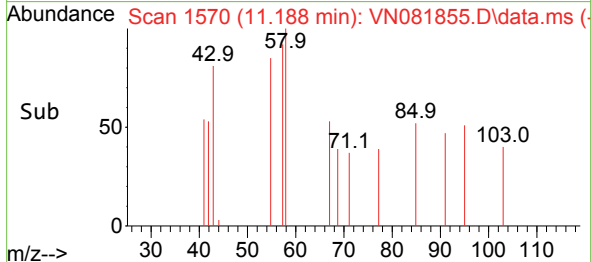

#62
4-Bromofluorobenzene
Concen: 50.325 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. -0.000 min
Lab File: VN081855.D
Acq: 25 Apr 2024 17:04

Tgt Ion: 95 Resp: 193096
Ion Ratio Lower Upper
95 100
174 61.4 0.0 160.6
176 59.2 0.0 152.8

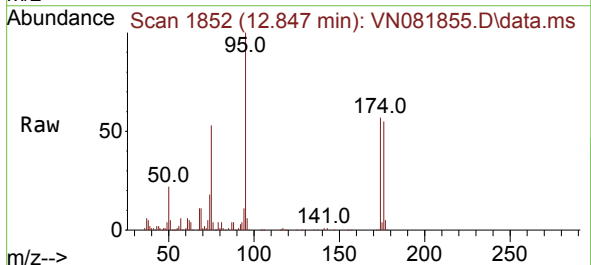

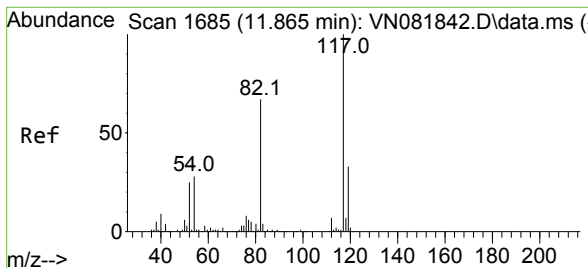

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.865 min Scan# 1

Delta R.T. -0.000 min

Lab File: VN081855.D

Acq: 25 Apr 2024 17:04

Instrument :

MSVOA_N

ClientSampleId :

41C





Tgt Ion:117 Resp: 364661

Ion Ratio Lower Upper

117 100

82 64.6 44.6 66.8

119 30.9 25.9 38.9

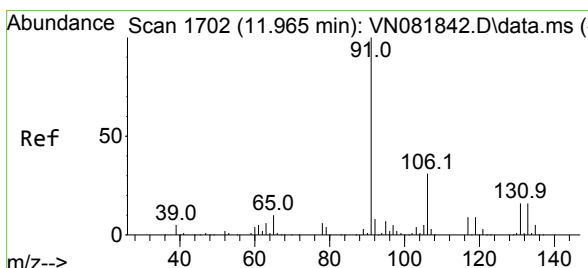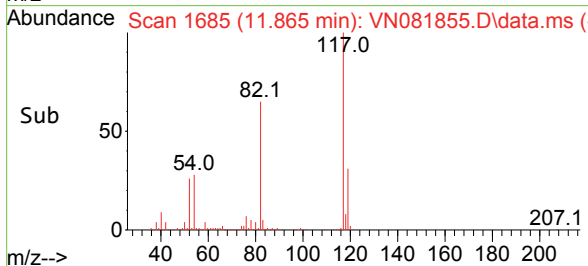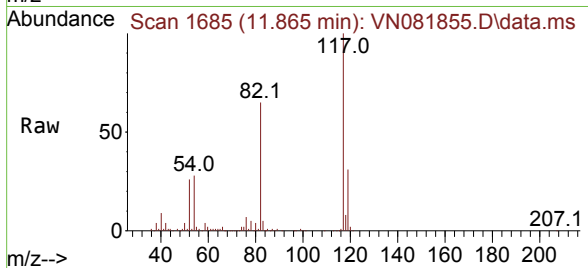

#67

Ethyl Benzene

Concen: 0.382 ug/l

RT: 11.965 min Scan# 1702

Delta R.T. -0.000 min

Lab File: VN081855.D




Acq: 25 Apr 2024 17:04


Tgt Ion: 91 Resp: 5656

Ion Ratio Lower Upper

91 100

106 29.1 25.3 37.9


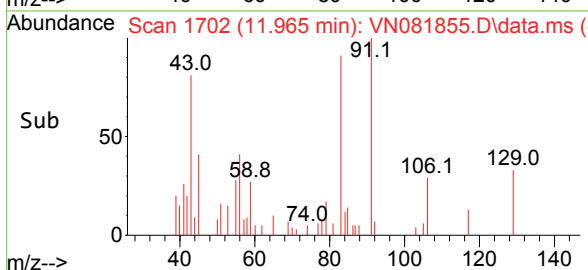

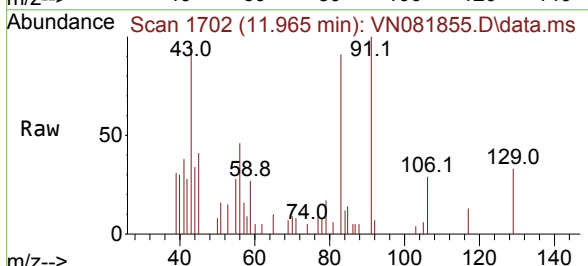




#68
m/p-Xylenes
Concen: 1.468 ug/l
RT: 12.065 min Scan# 1719
Delta R.T. -0.006 min
Lab File: VN081855.D
Acq: 25 Apr 2024 17:04




Instrument :
MSVOA_N
ClientSampleId :
41C


Tgt Ion:106 Resp: 7754
Ion Ratio Lower Upper
106 100
91 227.4 159.4 239.0

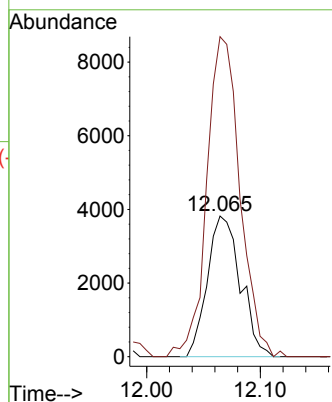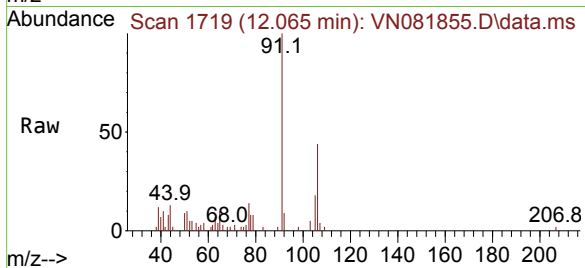

#69
o-Xylene
Concen: 0.752 ug/l
RT: 12.400 min Scan# 1776
Delta R.T. -0.000 min
Lab File: VN081855.D
Acq: 25 Apr 2024 17:04

Tgt Ion:106 Resp: 3876
Ion Ratio Lower Upper
106 100
91 219.4 104.7 314.1

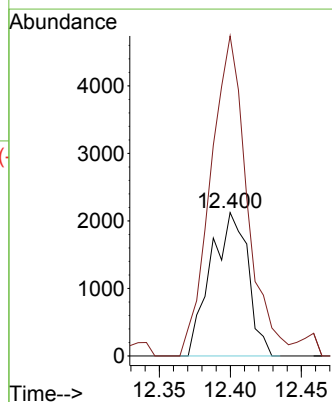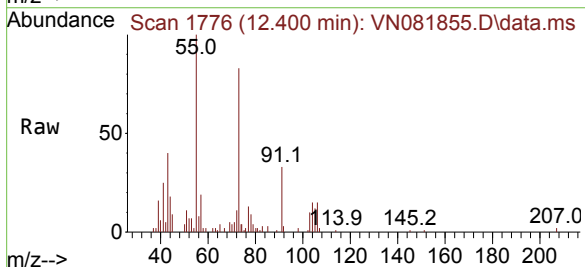

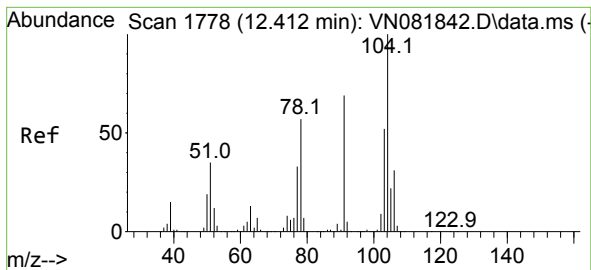

#70

Styrene

Concen: 0.849 ug/l

RT: 12.417 min Scan# 11

Delta R.T. 0.006 min

Lab File: VN081855.D

Acq: 25 Apr 2024 17:04

Instrument :

MSVOA_N

ClientSampleId :

41C





Tgt Ion:104 Resp: 7571

Ion Ratio Lower Upper

104 100

78 57.3 38.6 58.0

103 53.6 43.8 65.6

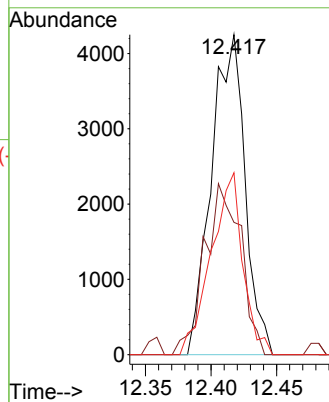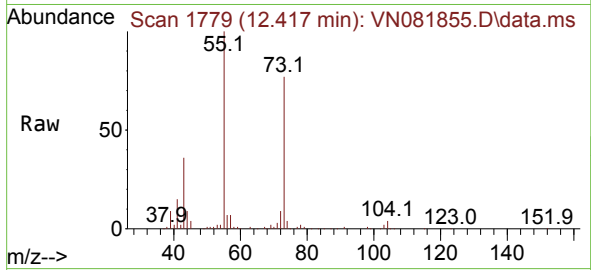

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.794 min Scan# 2013

Delta R.T. -0.000 min

Lab File: VN081855.D

Acq: 25 Apr 2024 17:04




Tgt Ion:152 Resp: 150782


Ion Ratio Lower Upper

152 100

115 66.9 30.4 91.3


150 158.0 0.0 353.2

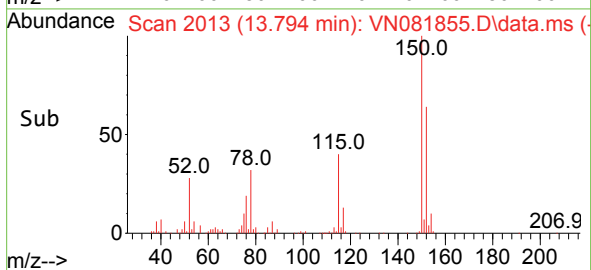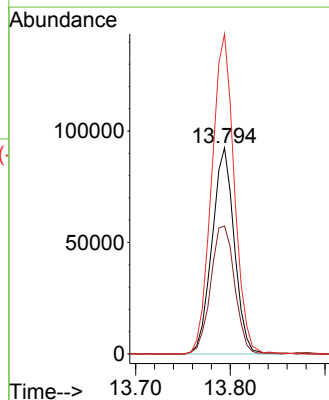






#74
N-amy1 acetate
Concen: 8.418 ug/l
RT: 12.417 min Scan# 11
Delta R.T. -0.077 min
Lab File: VN081855.D
Acq: 25 Apr 2024 17:04


Instrument :
MSVOA_N
ClientSampleId :
41C





Tgt Ion:	43	Resp:	62827
Ion	Ratio	Lower	Upper
43	100		
70	4.0	39.0	58.4#
55	267.4	21.3	31.9#
61	0.1	20.5	30.7#




#76
1,2,3-Trichloropropane
Concen: 27.132 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. -0.147 min
Lab File: VN081855.D
Acq: 25 Apr 2024 17:04



Tgt Ion:	75	Resp:	106070
Ion	Ratio	Lower	Upper
75	100		
77	1.2	90.5	271.3#



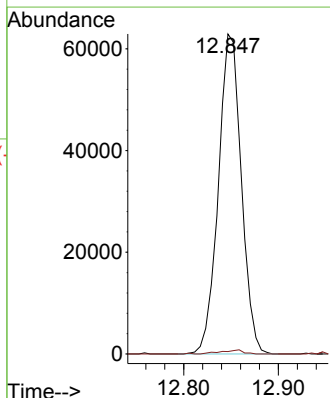
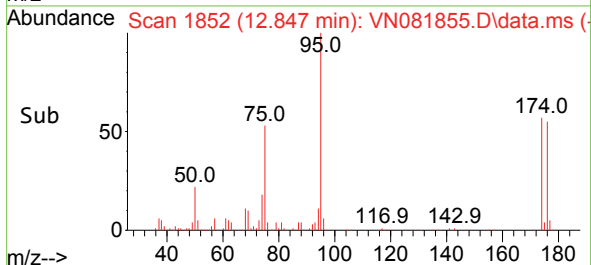


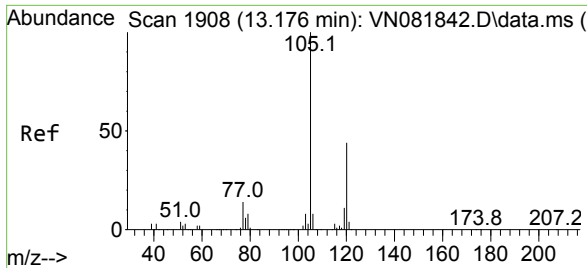

#80
 1,3,5-Trimethylbenzene
 Concen: 0.203 ug/l
 RT: 13.170 min Scan# 1908
 Delta R.T. -0.006 min
 Lab File: VN081855.D
 Acq: 25 Apr 2024 17:04




Instrument :
 MSVOA_N
 ClientSampleId :
 41C


Tgt Ion:105 Resp: 2303
 Ion Ratio Lower Upper
 105 100
 120 42.9 24.8 74.3

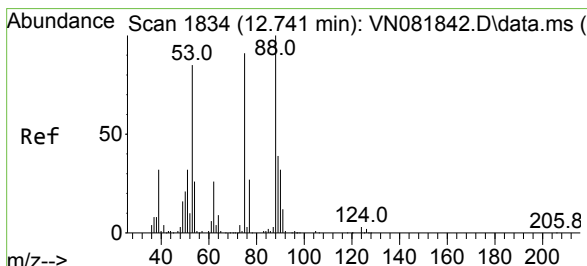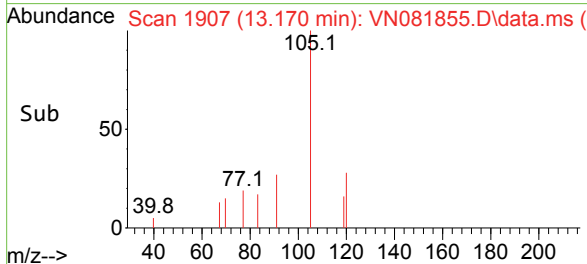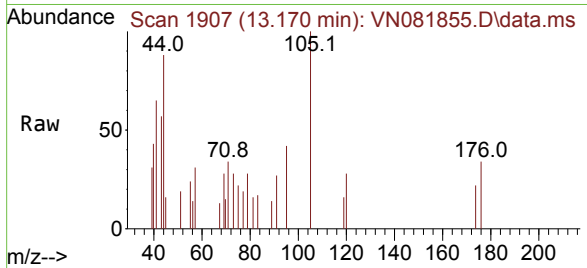

#81
 trans-1,4-Dichloro-2-butene
 Concen: 55.596 ug/l
 RT: 12.847 min Scan# 1852
 Delta R.T. 0.106 min
 Lab File: VN081855.D
 Acq: 25 Apr 2024 17:04

Tgt Ion: 75 Resp: 106070
 Ion Ratio Lower Upper
 75 100
 53 0.3 72.9 109.3#
 89 0.2 39.1 58.7#

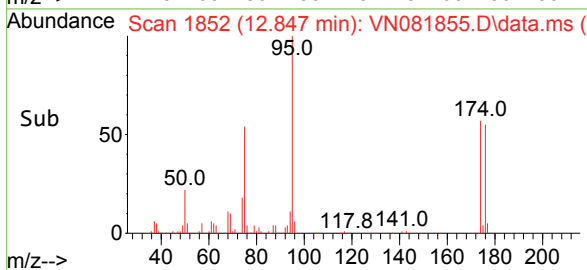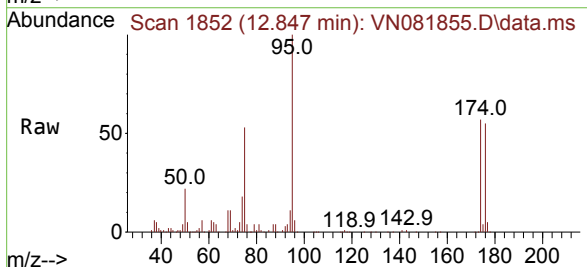

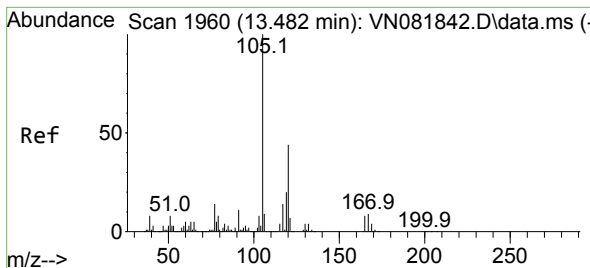

#84

1,2,4-Trimethylbenzene

Concen: 0.861 ug/l

RT: 13.482 min Scan# 1960

Delta R.T. -0.000 min

Lab File: VN081855.D

Acq: 25 Apr 2024 17:04

Instrument :

MSVOA_N

ClientSampleId :





41C

Tgt Ion:105 Resp: 9758

Ion Ratio Lower Upper

105 100

120 42.2 22.9 68.7

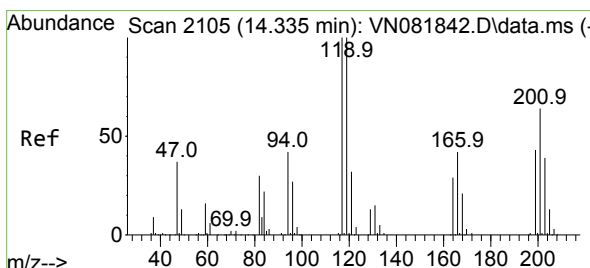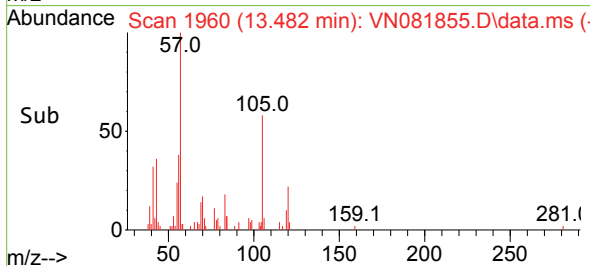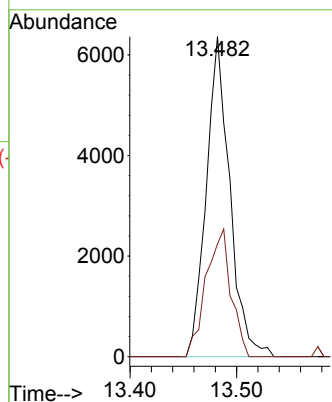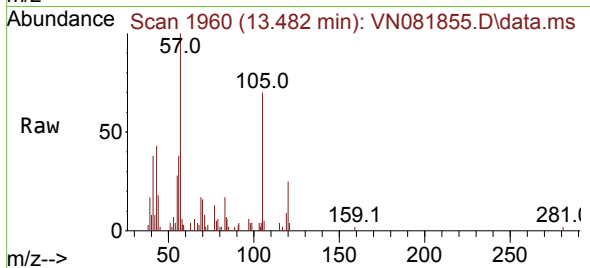

#90

Hexachloroethane

Concen: 0.300 ug/l

RT: 14.294 min Scan# 2098

Delta R.T. -0.041 min

Lab File: VN081855.D




Acq: 25 Apr 2024 17:04


Tgt Ion:117 Resp: 630

Ion Ratio Lower Upper

117 100


201 0.0 33.3 99.8#

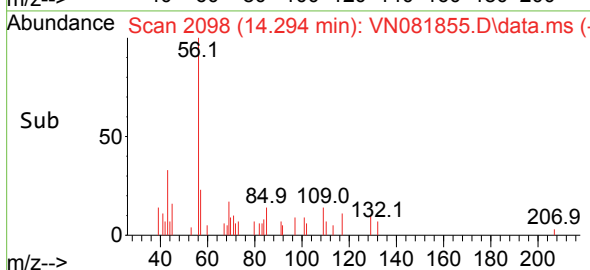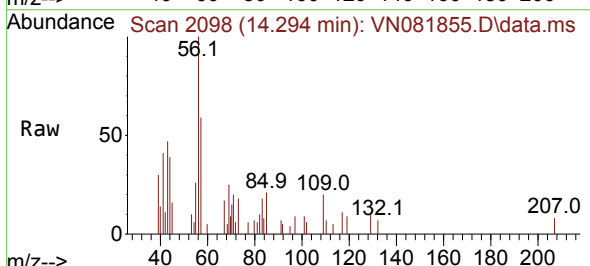



#95
Naphthalene
Concen: 0.460 ug/l
RT: 15.647 min Scan# 21
Delta R.T. 0.006 min
Lab File: VN081855.D
Acq: 25 Apr 2024 17:04

Instrument :
MSVOA_N
ClientSampleId :
41C

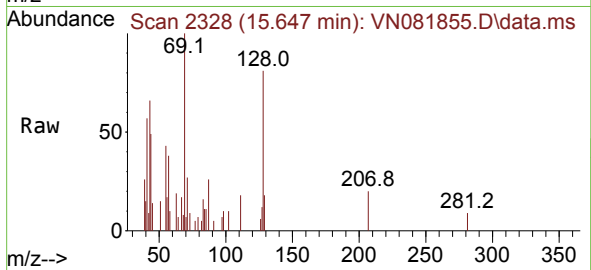

Tgt Ion:	128	Resp:	4877
Ion	Ratio	Lower	Upper
128	100		
127	8.1	10.1	15.1#
129	21.1	8.9	13.3#

