

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN042524\
 Data File : VN081860.D
 Acq On : 25 Apr 2024 19:04
 Operator : JC\MD
 Sample : P2257-11
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 416A

Quant Time: Apr 26 05:40:18 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N042524W.M
 Quant Title : SW846 8260
 QLast Update : Fri Apr 26 05:26:49 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.224	168	219308	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.100	114	406469	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.871	117	356763	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	151762	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.577	65	168844	45.617	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	91.240%
35) Dibromofluoromethane	8.165	113	122322	49.983	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	99.960%
50) Toluene-d8	10.571	98	506952	52.744	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	105.480%
62) 4-Bromofluorobenzene	12.847	95	185414	48.800	ug/l	0.00
Spiked Amount	50.000	Range	64 - 133	Recovery	=	97.600%


Target Compounds			Qvalue			
3) Chloromethane	2.365	50	1338	0.417	ug/l	90
5) Bromomethane	2.965	94	506	Below Cal		86
6) Chloroethane	3.124	64	526	0.358	ug/l #	44
11) Tert butyl alcohol	5.518	59	36947	54.910	ug/l	99
13) Acrolein	4.189	56	672	Below Cal	#	55
16) Acetone	4.430	43	22306	15.246	ug/l #	82
17) Carbon Disulfide	4.718	76	1724	0.216	ug/l #	74
18) Methyl Acetate	5.036	43	3978	1.061	ug/l #	74
20) Methylene Chloride	5.283	84	1003	0.316	ug/l #	50
25) 2-Butanone	7.483	43	40594	19.323	ug/l #	82
29) Tetrahydrofuran	7.836	42	460	0.305	ug/l #	40
31) Cyclohexane	8.224	56	7594	1.362	ug/l #	5
36) 1,1-Dichloropropene	8.224	75	22999	5.777	ug/l #	50
37) Ethyl Acetate	7.483	43	40594	9.430	ug/l #	68
38) Carbon Tetrachloride	8.236	117	23905	6.143	ug/l #	14
40) Benzene	8.606	78	25479	2.132	ug/l	98
41) Methacrylonitrile	7.777	41	3600	1.311	ug/l #	35
43) Isopropyl Acetate	8.665	43	45036	5.564	ug/l #	52
48) Methyl methacrylate	9.718	41	930	0.241	ug/l #	25
49) 1,4-Dioxane	9.700	88	2876	48.970	ug/l #	83
51) 4-Methyl-2-Pentanone	10.441	43	4734	1.039	ug/l	99
52) Toluene	10.630	92	14977	2.092	ug/l	99
59) 2-Hexanone	11.206	43	958	0.283	ug/l	82
67) Ethyl Benzene	11.965	91	8322	0.574	ug/l	100
68) m/p-Xylenes	12.071	106	10133	1.961	ug/l	93
69) o-Xylene	12.400	106	5340	1.058	ug/l	98
70) Styrene	12.424	104	3206	0.367	ug/l #	67
74) N-amyl acetate	12.424	43	19003	2.530	ug/l #	1
76) 1,2,3-Trichloropropane	12.847	75	103204	26.228	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.847	75	103204	53.745	ug/l #	13
84) 1,2,4-Trimethylbenzene	13.488	105	8123	0.712	ug/l	88
95) Naphthalene	15.641	128	154007	14.424	ug/l	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN042524\
Data File : VN081860.D
Acq On : 25 Apr 2024 19:04
Operator : JC\MD
Sample : P2257-11
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
416A

Quant Time: Apr 26 05:40:18 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N042524W.M
Quant Title : SW846 8260
QLast Update : Fri Apr 26 05:26:49 2024
Response via : Initial Calibration

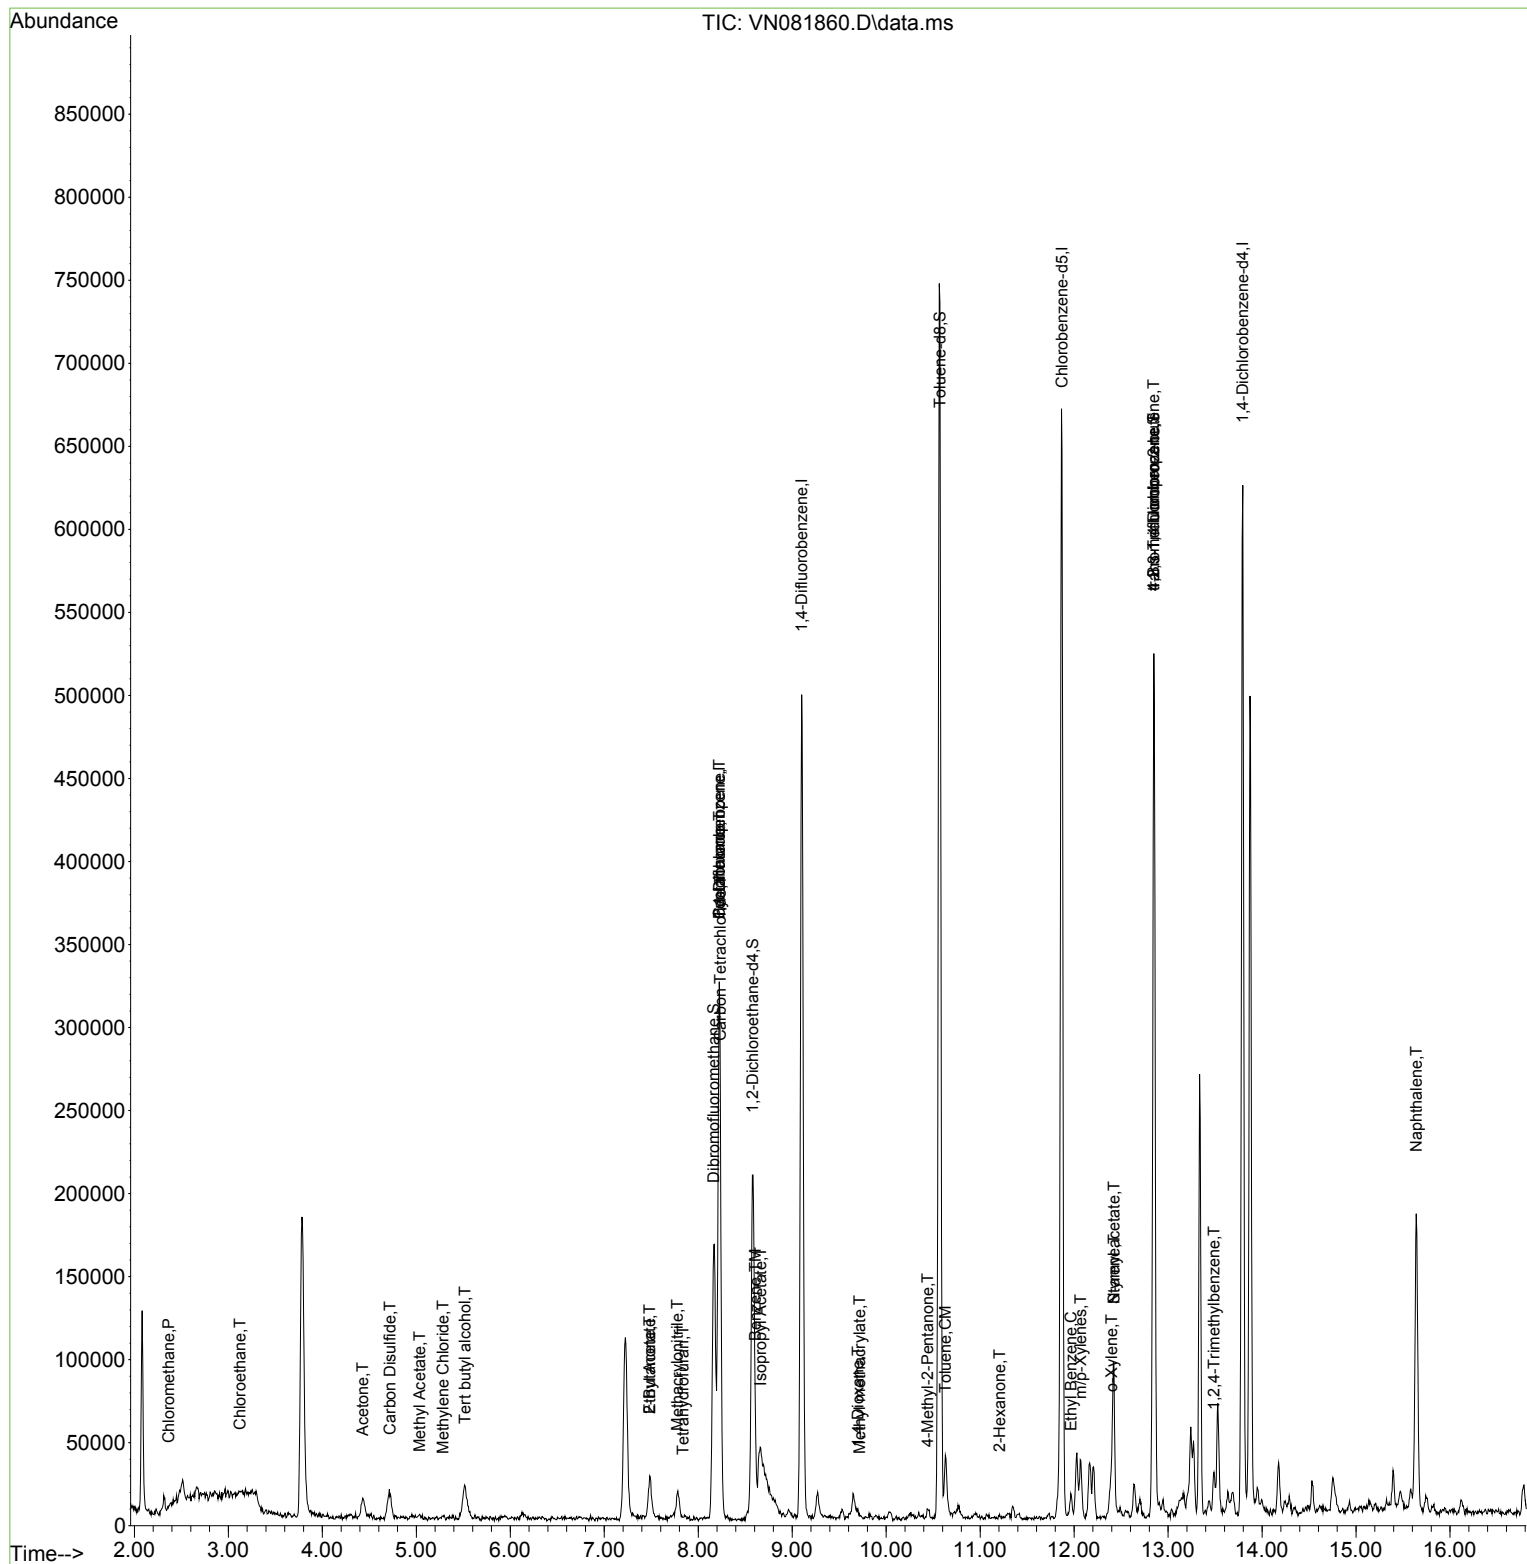



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 8.224 min Scan# 1

Delta R.T. -0.000 min

Lab File: VN081860.D

Acq: 25 Apr 2024 19:04

Instrument :

MSVOA_N

ClientSampleId :





416A

Tgt Ion:168 Resp: 219308

Ion Ratio Lower Upper

168 100

99 65.0 48.2 72.4

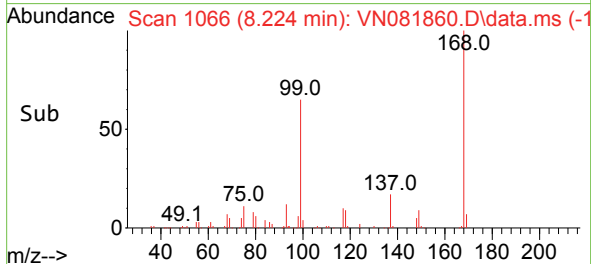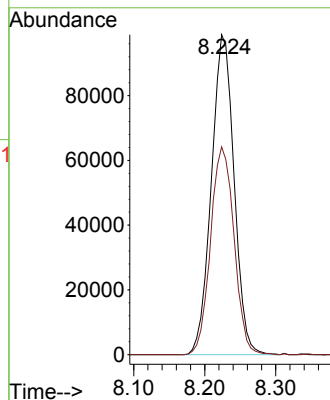

#3

Chloromethane

Concen: 0.417 ug/l

RT: 2.365 min Scan# 70

Delta R.T. 0.006 min

Lab File: VN081860.D




Acq: 25 Apr 2024 19:04


Tgt Ion: 50 Resp: 1338

Ion Ratio Lower Upper

50 100

52 37.4 25.5 38.3



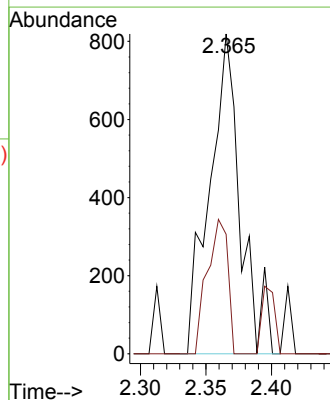





#5
Bromomethane
Concen: Below Cal
RT: 2.965 min Scan# 11
Delta R.T. 0.017 min
Lab File: VN081860.D
Acq: 25 Apr 2024 19:04




Instrument :
MSVOA_N
ClientSampleId :
416A


Tgt Ion: 94 Resp: 506
Ion Ratio Lower Upper
94 100
96 107.2 74.8 112.2

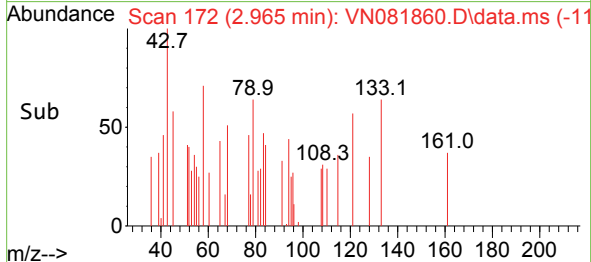

#6
Chloroethane
Concen: 0.358 ug/l
RT: 3.124 min Scan# 199
Delta R.T. 0.000 min
Lab File: VN081860.D
Acq: 25 Apr 2024 19:04

Tgt Ion: 64 Resp: 526
Ion Ratio Lower Upper
64 100
66 0.0 24.7 37.1#




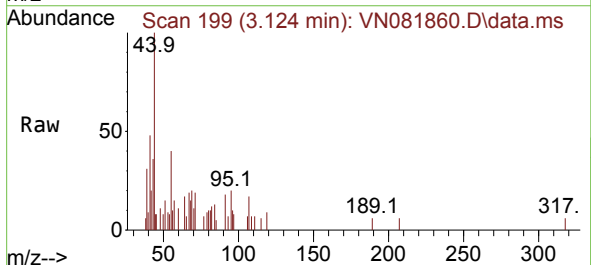




#11
Tert butyl alcohol
Concen: 54.910 ug/l
RT: 5.518 min Scan# 606
Delta R.T. 0.000 min
Lab File: VN081860.D
Acq: 25 Apr 2024 19:04




Instrument :
MSVOA_N
ClientSampleId :
416A


Tgt Ion: 59 Resp: 36947
Ion Ratio Lower Upper
59 100
57 11.4 8.9 13.3

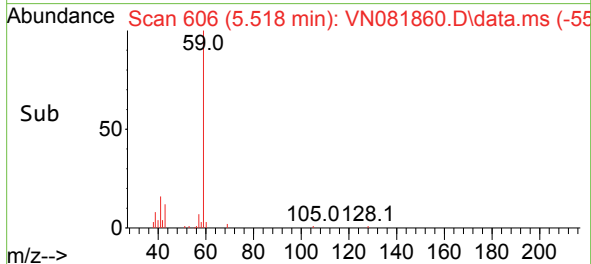

#13
Acrolein
Concen: Below Cal
RT: 4.189 min Scan# 380
Delta R.T. 0.012 min
Lab File: VN081860.D
Acq: 25 Apr 2024 19:04

Tgt Ion: 56 Resp: 672
Ion Ratio Lower Upper
56 100
55 32.9 55.8 83.8#









#16
Acetone
Concen: 15.246 ug/l
RT: 4.430 min Scan# 41
Delta R.T. 0.006 min
Lab File: VN081860.D
Acq: 25 Apr 2024 19:04




Instrument :
MSVOA_N
ClientSampleId :
416A


Tgt Ion: 43 Resp: 22306
Ion Ratio Lower Upper
43 100
58 41.5 25.2 37.8#

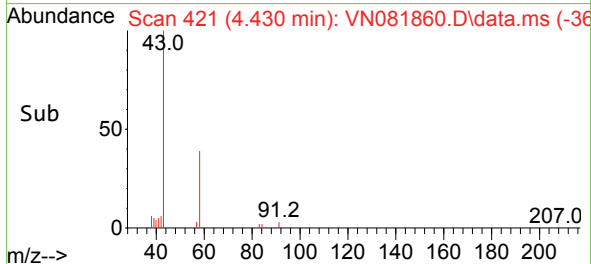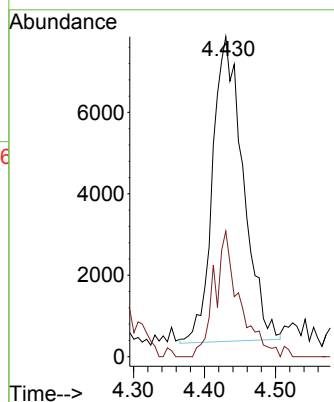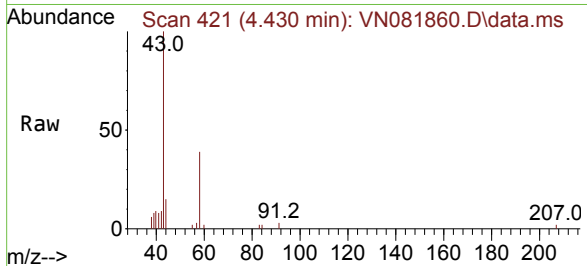

#17
Carbon Disulfide
Concen: 0.216 ug/l
RT: 4.718 min Scan# 470
Delta R.T. 0.006 min
Lab File: VN081860.D
Acq: 25 Apr 2024 19:04

Tgt Ion: 76 Resp: 1724
Ion Ratio Lower Upper
76 100
78 0.0 7.5 11.3#



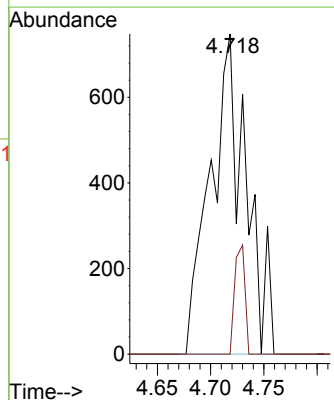
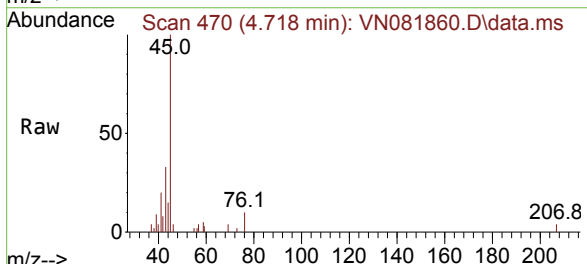




#18
Methyl Acetate
Concen: 1.061 ug/l
RT: 5.036 min Scan# 51
Delta R.T. 0.018 min
Lab File: VN081860.D
Acq: 25 Apr 2024 19:04




Instrument :
MSVOA_N
ClientSampleId :
416A


Tgt Ion: 43 Resp: 3978
Ion Ratio Lower Upper
43 100
74 14.3 22.2 33.2#

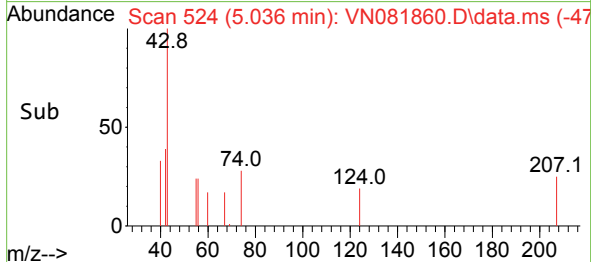

#20
Methylene Chloride
Concen: 0.316 ug/l
RT: 5.283 min Scan# 566
Delta R.T. 0.006 min
Lab File: VN081860.D
Acq: 25 Apr 2024 19:04

Tgt Ion: 84 Resp: 1003
Ion Ratio Lower Upper
84 100
49 50.9 84.9 127.3#
51 0.0 27.0 40.6#
86 34.8 52.3 78.5#




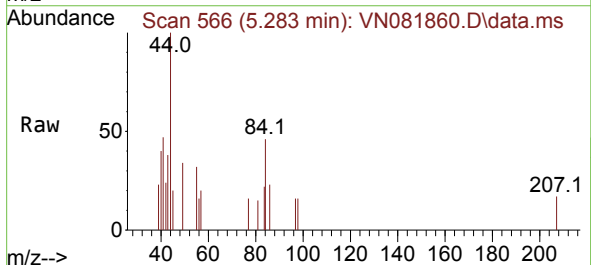




#25
2-Butanone
Concen: 19.323 ug/l
RT: 7.483 min Scan# 940
Delta R.T. 0.006 min
Lab File: VN081860.D
Acq: 25 Apr 2024 19:04




Instrument :
MSVOA_N
ClientSampleId :
416A


Tgt Ion: 43 Resp: 40594
Ion Ratio Lower Upper
43 100
72 21.4 25.3 37.9#

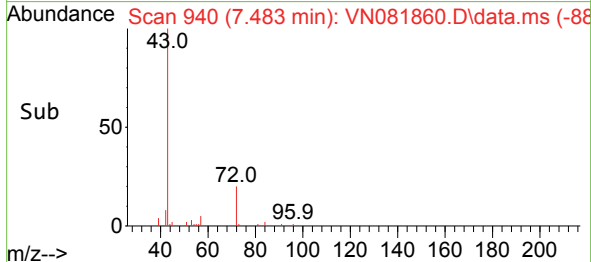

#29
Tetrahydrofuran
Concen: 0.305 ug/l
RT: 7.836 min Scan# 1000
Delta R.T. 0.000 min
Lab File: VN081860.D
Acq: 25 Apr 2024 19:04


Tgt Ion: 42 Resp: 460
Ion Ratio Lower Upper
42 100
72 0.0 39.3 58.9#
71 15.0 37.4 56.0#

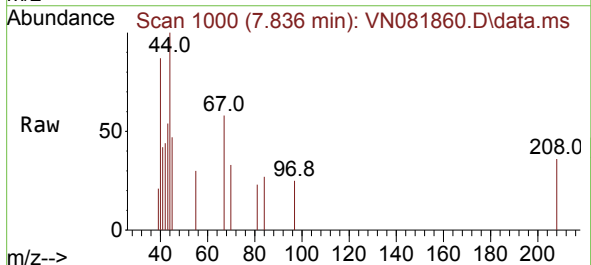






#31
Cyclohexane
Concen: 1.362 ug/l
RT: 8.224 min Scan# 1066
Delta R.T. -0.035 min
Lab File: VN081860.D
Acq: 25 Apr 2024 19:04

Instrument :
MSVOA_N
ClientSampleId :
416A







Tgt Ion: 56 Resp: 7594
Ion Ratio Lower Upper
56 100
69 160.3 24.4 36.6#
84 144.4 77.0 115.4#

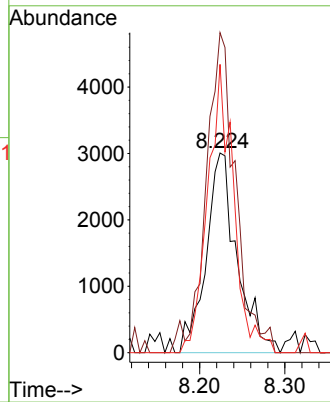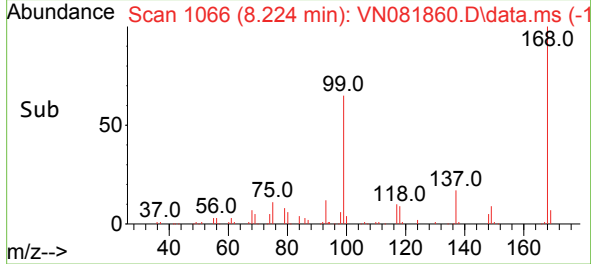

#33
1,2-Dichloroethane-d4
Concen: 45.617 ug/l
RT: 8.577 min Scan# 1126
Delta R.T. 0.000 min
Lab File: VN081860.D
Acq: 25 Apr 2024 19:04

Tgt Ion: 65 Resp: 168844
Ion Ratio Lower Upper
65 100
67 53.6 0.0 103.0


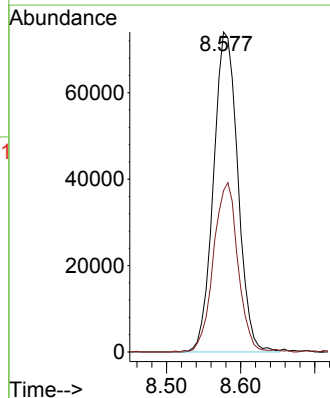






#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 9.100 min Scan# 11
Delta R.T. 0.000 min
Lab File: VN081860.D
Acq: 25 Apr 2024 19:04




Instrument :
MSVOA_N
ClientSampleId :
416A


Tgt Ion:114 Resp: 406469
Ion Ratio Lower Upper
114 100
63 23.5 0.0 41.0
88 16.6 0.0 31.4

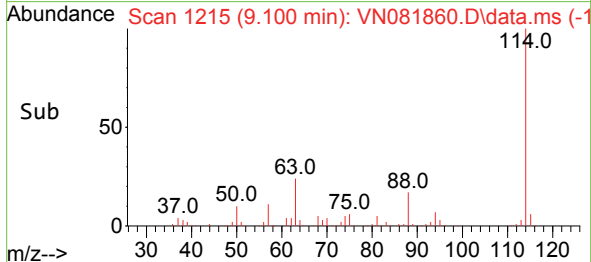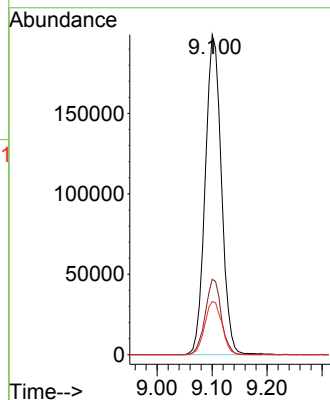

#35
Dibromofluoromethane
Concen: 49.983 ug/l
RT: 8.165 min Scan# 1056
Delta R.T. 0.000 min
Lab File: VN081860.D
Acq: 25 Apr 2024 19:04

Tgt Ion:113 Resp: 122322
Ion Ratio Lower Upper
113 100
111 103.1 83.4 125.2
192 17.2 14.0 21.0

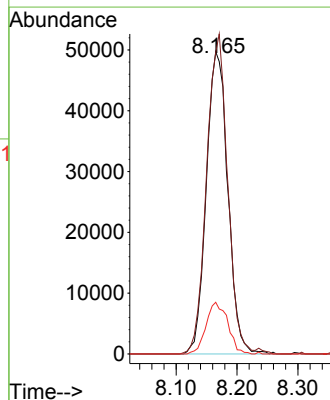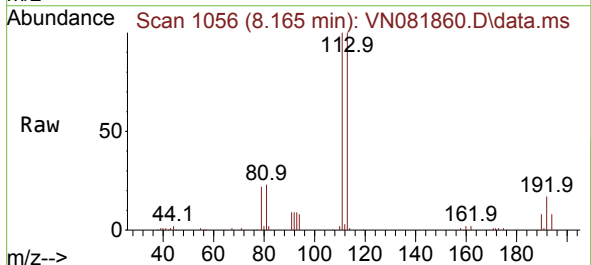



#36

1,1-Dichloropropene

Concen: 5.777 ug/l

RT: 8.224 min Scan# 1066

Delta R.T. -0.147 min

Lab File: VN081860.D

Acq: 25 Apr 2024 19:04

Instrument :

MSVOA_N

ClientSampleId :

416A





Tgt Ion: 75 Resp: 22999

Ion Ratio Lower Upper

75 100

110 10.2 17.8 53.5#

77 0.0 25.0 37.4#

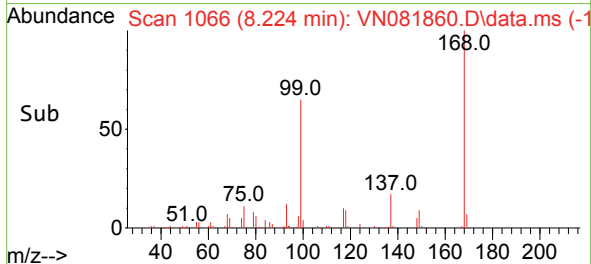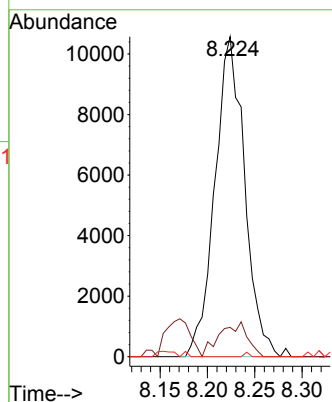

#37

Ethyl Acetate

Concen: 9.430 ug/l

RT: 7.483 min Scan# 940

Delta R.T. -0.076 min

Lab File: VN081860.D

Acq: 25 Apr 2024 19:04




Tgt Ion: 43 Resp: 40594


Ion Ratio Lower Upper

43 100

61 0.0 11.3 16.9#

70 0.0 8.7 13.1#





#38

Carbon Tetrachloride

Concen: 6.143 ug/l

RT: 8.236 min Scan# 1068

Delta R.T. -0.123 min

Lab File: VN081860.D


Acq: 25 Apr 2024 19:04

Instrument :

MSVOA_N

ClientSampleId :

416A






Tgt Ion:117 Resp: 23905

Ion Ratio Lower Upper

117 100

119 2.8 76.5 114.7#

121 0.0 23.9 35.9#

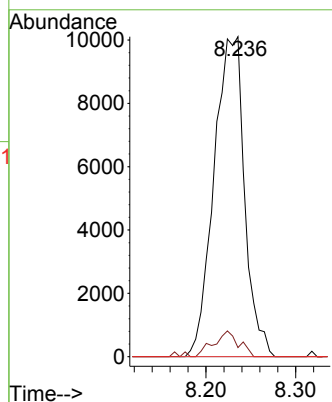

#40

Benzene

Concen: 2.132 ug/l

RT: 8.606 min Scan# 1131

Delta R.T. 0.000 min

Lab File: VN081860.D




Acq: 25 Apr 2024 19:04


Tgt Ion: 78 Resp: 25479

Ion Ratio Lower Upper

78 100

77 26.1 20.0 30.0




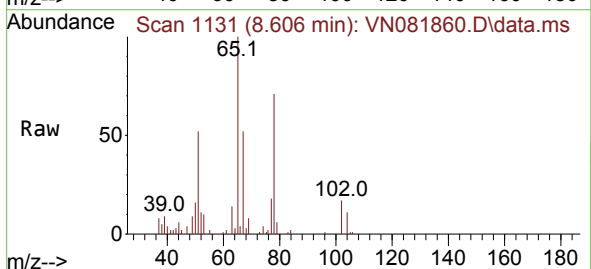




#41
Methacrylonitrile
Concen: 1.311 ug/l
RT: 7.777 min Scan# 990
Delta R.T. 0.000 min
Lab File: VN081860.D
Acq: 25 Apr 2024 19:04




Instrument :
MSVOA_N
ClientSampleId :
416A


Tgt Ion: 41	Resp: 3600
Ion Ratio	Lower Upper
41 100	
39 37.8	46.6 69.8#
67 0.0	67.3 100.9#
52 0.0	27.3 40.9#

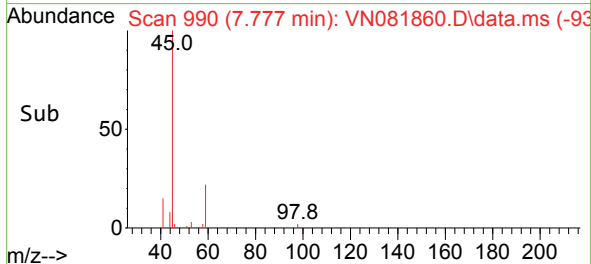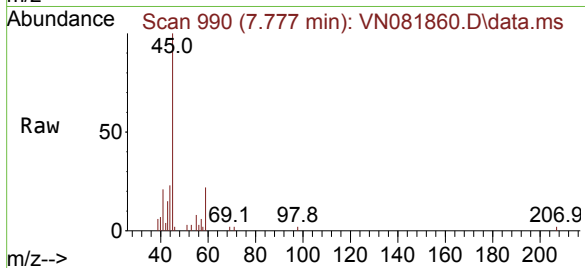

#43
Isopropyl Acetate
Concen: 5.564 ug/l
RT: 8.665 min Scan# 1141
Delta R.T. -0.023 min
Lab File: VN081860.D
Acq: 25 Apr 2024 19:04

Tgt Ion: 43	Resp: 45036
Ion Ratio	Lower Upper
43 100	
61 0.0	22.8 34.2#
87 0.1	12.0 18.0#




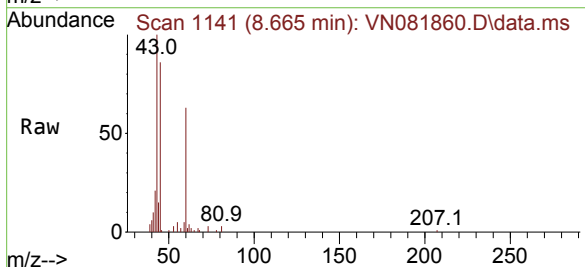




#48
Methyl methacrylate
Concen: 0.241 ug/l
RT: 9.718 min Scan# 11
Delta R.T. 0.035 min
Lab File: VN081860.D
Acq: 25 Apr 2024 19:04




Instrument :
MSVOA_N
ClientSampleId :
416A


Tgt Ion: 41 Resp: 930
Ion Ratio Lower Upper
41 100
69 0.0 77.9 116.9#
39 34.1 50.9 76.3#

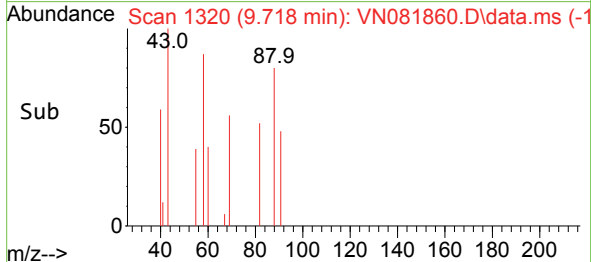

#49
1,4-Dioxane
Concen: 48.970 ug/l
RT: 9.700 min Scan# 1317
Delta R.T. 0.006 min
Lab File: VN081860.D
Acq: 25 Apr 2024 19:04

Tgt Ion: 88 Resp: 2876
Ion Ratio Lower Upper
88 100
43 0.0 19.0 28.6#
58 67.2 50.6 76.0




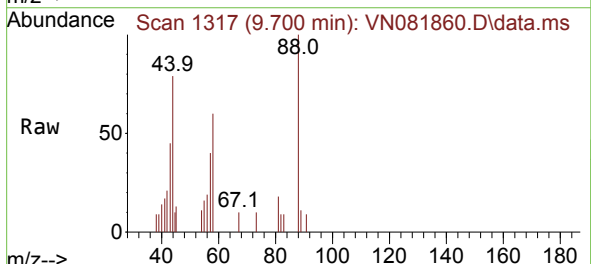




#50
Toluene-d8
Concen: 52.744 ug/l
RT: 10.571 min Scan# 1465
Delta R.T. 0.006 min
Lab File: VN081860.D
Acq: 25 Apr 2024 19:04




Instrument :
MSVOA_N
ClientSampleId :
416A


Tgt Ion: 98 Resp: 506952
Ion Ratio Lower Upper
98 100
100 64.9 51.8 77.6

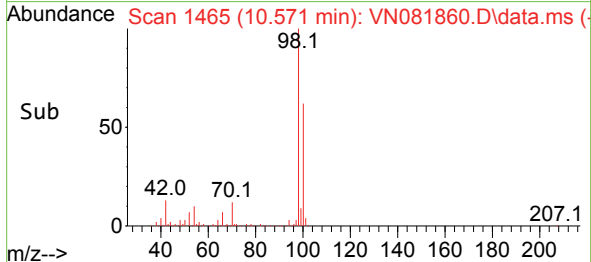

#51
4-Methyl-2-Pentanone
Concen: 1.039 ug/l
RT: 10.441 min Scan# 1443
Delta R.T. -0.006 min
Lab File: VN081860.D
Acq: 25 Apr 2024 19:04

Tgt Ion: 43 Resp: 4734
Ion Ratio Lower Upper
43 100
58 40.8 33.2 49.8

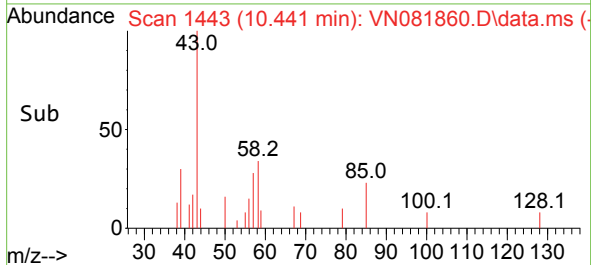



#52

Toluene

Concen: 2.092 ug/l

RT: 10.630 min Scan# 1475

Delta R.T. 0.000 min

Lab File: VN081860.D

Acq: 25 Apr 2024 19:04

Instrument :

MSVOA_N

ClientSampleId :





416A

Tgt Ion: 92 Resp: 14977

Ion Ratio Lower Upper

92 100

91 172.4 136.7 205.1

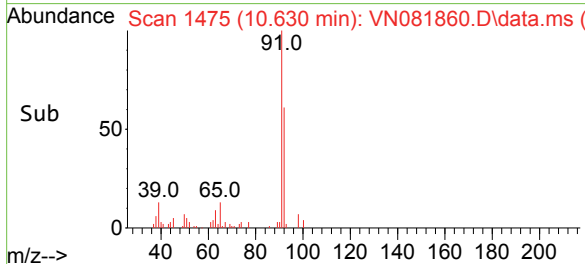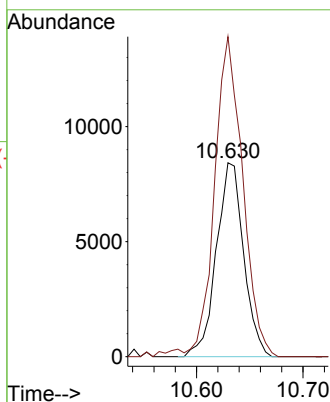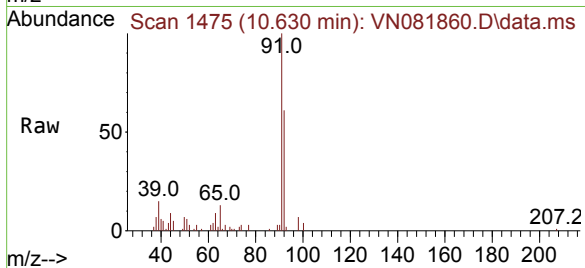

#59

2-Hexanone

Concen: 0.283 ug/l

RT: 11.206 min Scan# 1573

Delta R.T. 0.012 min

Lab File: VN081860.D




Acq: 25 Apr 2024 19:04


Tgt Ion: 43 Resp: 958

Ion Ratio Lower Upper

43 100

58 43.6 28.3 84.9


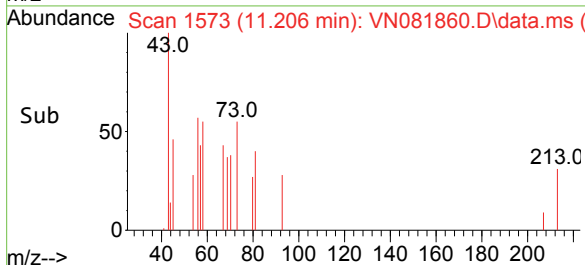
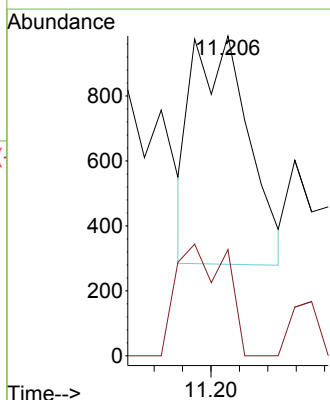
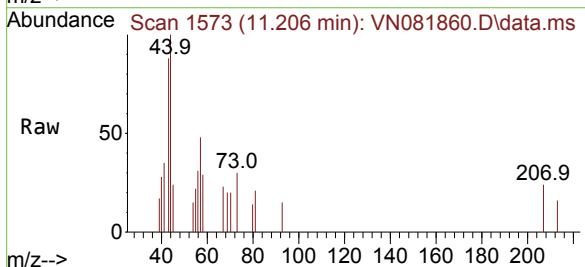


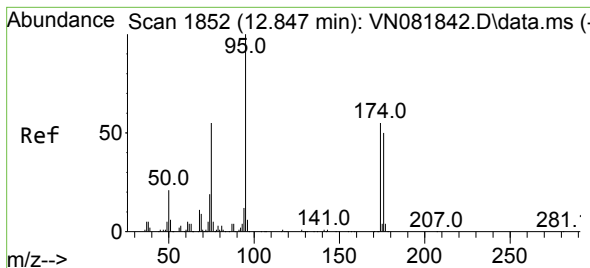

#62
4-Bromofluorobenzene
Concen: 48.800 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. 0.000 min
Lab File: VN081860.D
Acq: 25 Apr 2024 19:04




Instrument :
MSVOA_N
ClientSampleId :
416A


Tgt Ion: 95 Resp: 185414
Ion Ratio Lower Upper
95 100
174 63.7 0.0 160.6
176 61.7 0.0 152.8

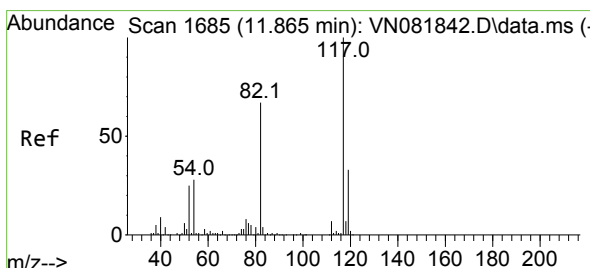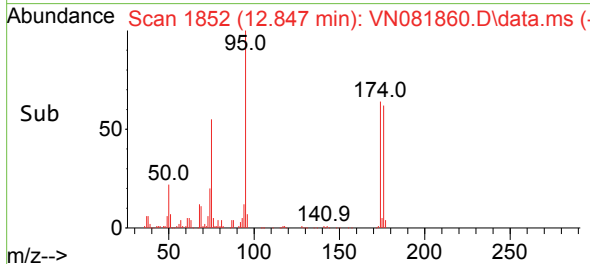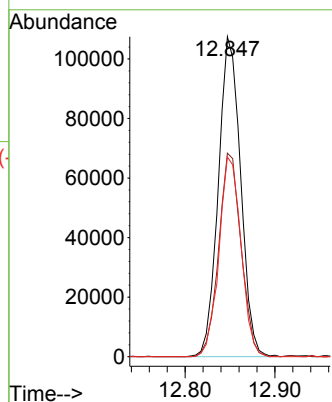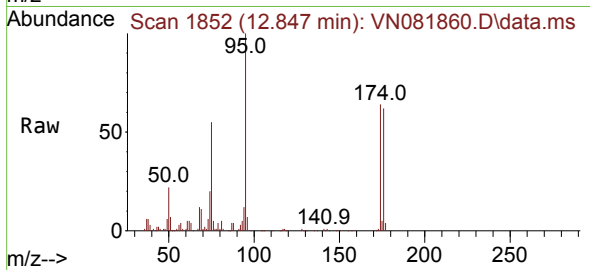

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.871 min Scan# 1686
Delta R.T. 0.006 min
Lab File: VN081860.D
Acq: 25 Apr 2024 19:04

Tgt Ion: 117 Resp: 356763
Ion Ratio Lower Upper
117 100
82 59.7 44.6 66.8
119 30.9 25.9 38.9


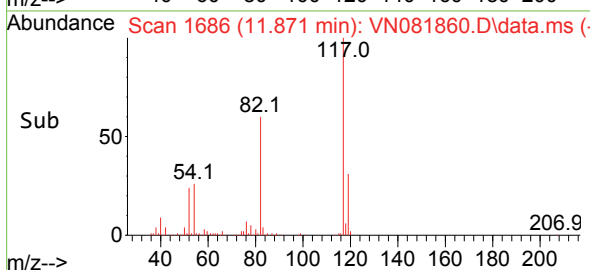

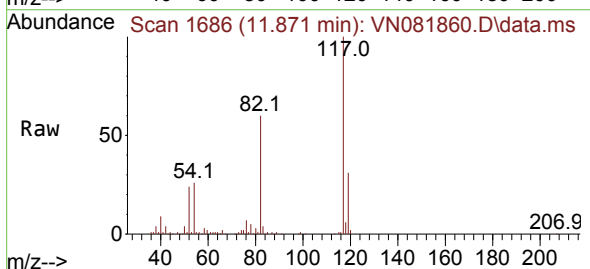


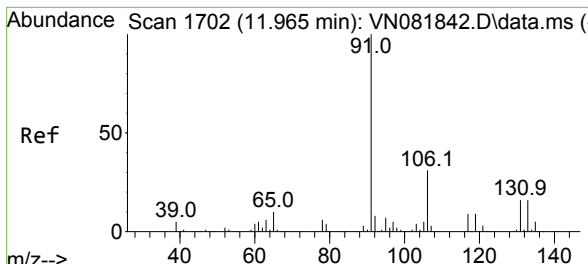

#67
Ethyl Benzene
Concen: 0.574 ug/l
RT: 11.965 min Scan# 1702
Delta R.T. 0.000 min
Lab File: VN081860.D
Acq: 25 Apr 2024 19:04




Instrument :
MSVOA_N
ClientSampleId :
416A


Tgt Ion:	91	Resp:	8322
Ion Ratio	Lower	Upper	
91	100		
106	31.7	25.3	37.9

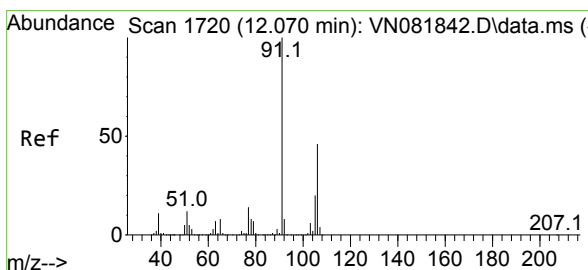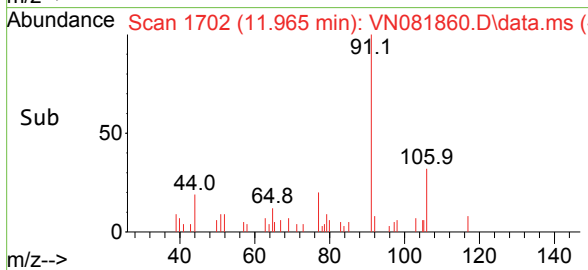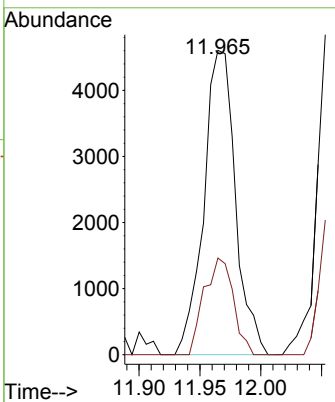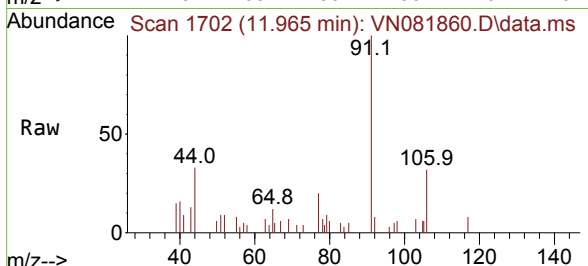

#68
m/p-Xylenes
Concen: 1.961 ug/l
RT: 12.071 min Scan# 1720
Delta R.T. 0.000 min
Lab File: VN081860.D
Acq: 25 Apr 2024 19:04

Tgt Ion:	106	Resp:	10133
Ion Ratio	Lower	Upper	
106	100		
91	210.0	159.4	239.0

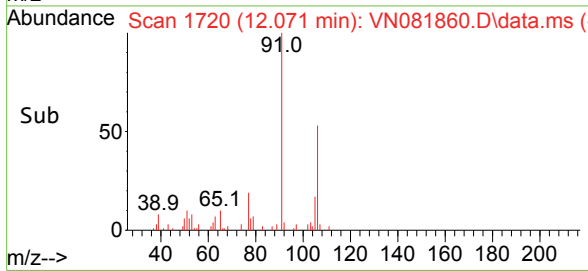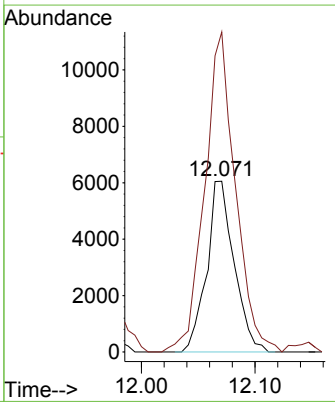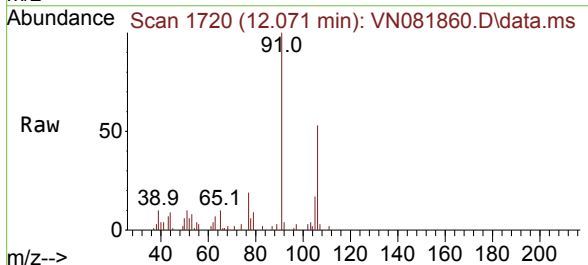



#69

o-Xylene

Concen: 1.058 ug/l

RT: 12.400 min Scan# 1776

Delta R.T. 0.000 min

Lab File: VN081860.D

Acq: 25 Apr 2024 19:04

Instrument :

MSVOA_N

ClientSampleId :





416A

Tgt Ion:106 Resp: 5340

Ion Ratio Lower Upper

106 100

91 212.2 104.7 314.1

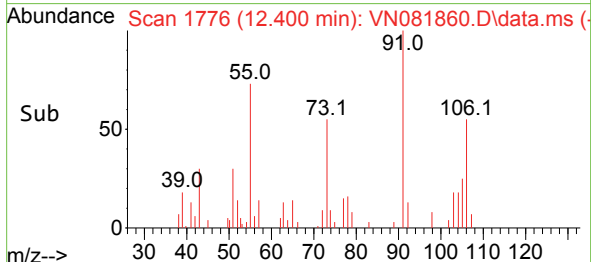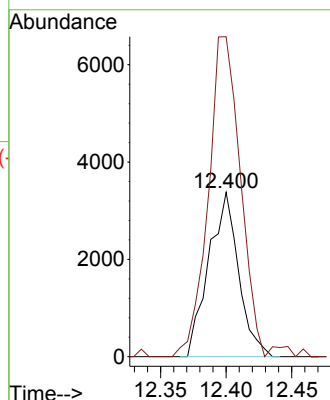

#70

Styrene

Concen: 0.367 ug/l

RT: 12.424 min Scan# 1780

Delta R.T. 0.012 min

Lab File: VN081860.D

Acq: 25 Apr 2024 19:04




Tgt Ion:104 Resp: 3206


Ion Ratio Lower Upper

104 100

78 77.8 38.6 58.0#

103 71.6 43.8 65.6#

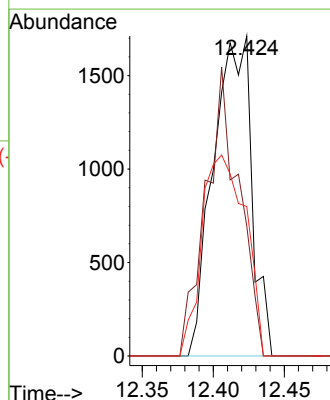

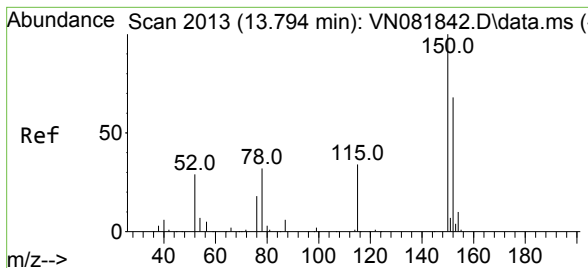

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.794 min Scan# 20

Delta R.T. 0.000 min

Lab File: VN081860.D

Acq: 25 Apr 2024 19:04

Instrument :

MSVOA_N

ClientSampleId :

416A





Tgt Ion:152 Resp: 151762

Ion Ratio Lower Upper

152 100

115 66.6 30.4 91.3

150 159.4 0.0 353.2

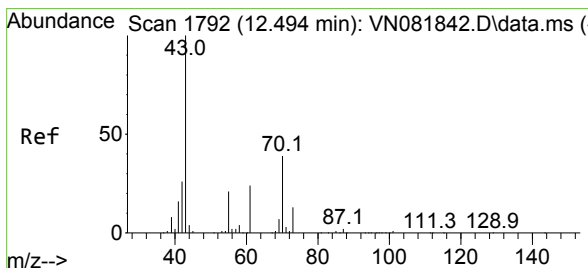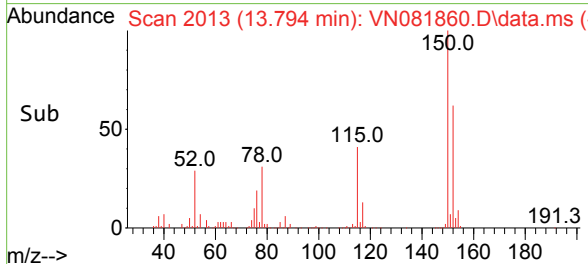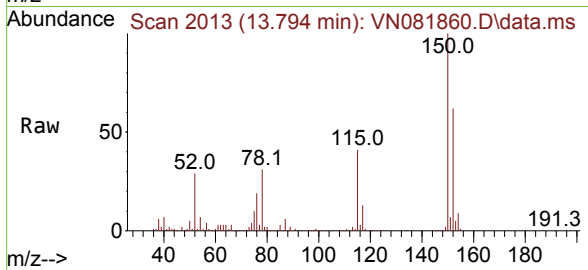

#74

N-ethyl acetate

Concen: 2.530 ug/l

RT: 12.424 min Scan# 1780

Delta R.T. -0.070 min

Lab File: VN081860.D

Acq: 25 Apr 2024 19:04

Tgt Ion: 43 Resp: 19003




Ion Ratio Lower Upper


43 100

70 2.3 39.0 58.4#

55 241.0 21.3 31.9#

61 0.0 20.5 30.7#

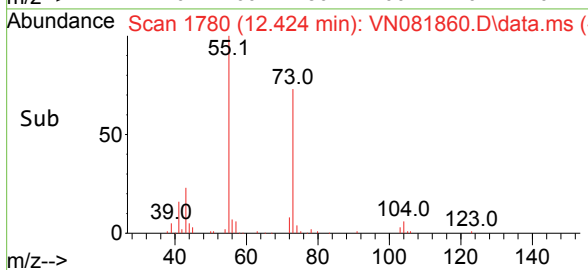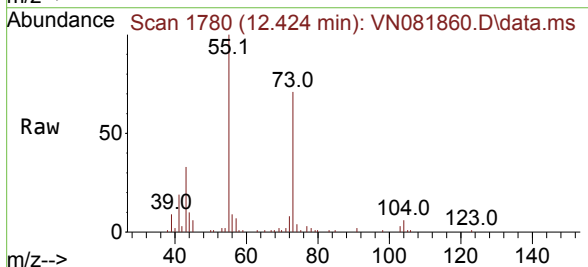



#76

1,2,3-Trichloropropane

Concen: 26.228 ug/l

RT: 12.847 min Scan# 1852

Delta R.T. -0.147 min

Lab File: VN081860.D

Acq: 25 Apr 2024 19:04

Instrument :

MSVOA_N

ClientSampleId :





416A

Tgt Ion: 75 Resp: 103204

Ion Ratio Lower Upper

75 100

77 1.2 90.5 271.3#

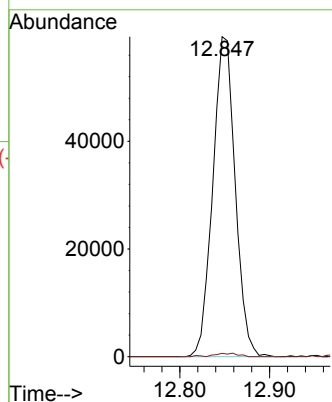

#81

trans-1,4-Dichloro-2-butene

Concen: 53.745 ug/l

RT: 12.847 min Scan# 1852

Delta R.T. 0.106 min

Lab File: VN081860.D

Acq: 25 Apr 2024 19:04




Tgt Ion: 75 Resp: 103204


Ion Ratio Lower Upper

75 100

53 0.2 72.9 109.3#

89 0.0 39.1 58.7#





#84

1,2,4-Trimethylbenzene

Concen: 0.712 ug/l

RT: 13.488 min Scan# 1960

Delta R.T. 0.006 min

Lab File: VN081860.D

Acq: 25 Apr 2024 19:04

Instrument :

MSVOA_N

ClientSampleId :





416A

Tgt Ion:105 Resp: 8123

Ion Ratio Lower Upper

105 100

120 37.7 22.9 68.7

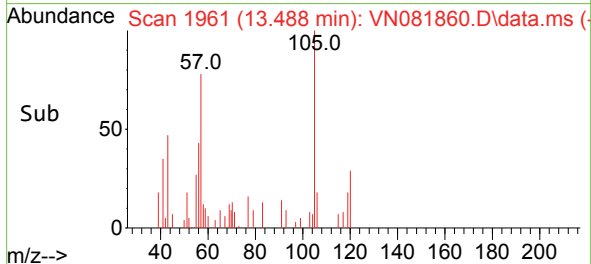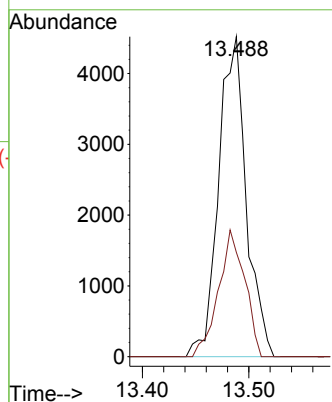

#95

Naphthalene

Concen: 14.424 ug/l

RT: 15.641 min Scan# 2327

Delta R.T. 0.000 min

Lab File: VN081860.D

Acq: 25 Apr 2024 19:04

Tgt Ion:128 Resp: 154007

Ion Ratio Lower Upper

128 100

127 12.8 10.1 15.1

129 11.4 8.9 13.3

