

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN042524\
 Data File : VN081864.D
 Acq On : 25 Apr 2024 20:40
 Operator : JC\MD
 Sample : P2246-03
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 SAW-CUTTING-LIQUID

Quant Time: Apr 26 05:41:54 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N042524W.M
 Quant Title : SW846 8260
 QLast Update : Fri Apr 26 05:26:49 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.224	168	219198	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	405914	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	355241	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	145279	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.583	65	169916	45.930	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery =	91.860%		
35) Dibromofluoromethane	8.171	113	121779	49.829	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	99.660%		
50) Toluene-d8	10.565	98	500796	52.175	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery =	104.340%		
62) 4-Bromofluorobenzene	12.853	95	182142	48.004	ug/l	0.00
Spiked Amount 50.000	Range 64 - 133		Recovery =	96.000%		
Target Compounds						Qvalue
3) Chloromethane	2.360	50	1042	0.325	ug/l #	43
5) Bromomethane	2.930	94	70	Below Cal	#	6
6) Chloroethane	3.107	64	872	0.594	ug/l	94
11) Tert butyl alcohol	5.524	59	11359	16.890	ug/l #	92
13) Acrolein	4.171	56	184	Below Cal	#	1
16) Acetone	4.430	43	60193	50.663	ug/l #	84
25) 2-Butanone	7.483	43	16769	7.986	ug/l #	78
26) 2,2-Dichloropropane	7.424	77	4881	0.938	ug/l #	53
29) Tetrahydrofuran	7.824	42	462	0.307	ug/l #	53
36) 1,1-Dichloropropene	8.224	75	20853	5.245	ug/l #	48
37) Ethyl Acetate	7.483	43	16766	3.900	ug/l #	70
38) Carbon Tetrachloride	8.224	117	22796	5.866	ug/l #	17
43) Isopropyl Acetate	8.665	43	7706	0.953	ug/l #	52
51) 4-Methyl-2-Pentanone	10.447	43	6928	1.523	ug/l	96
52) Toluene	10.630	92	2349	0.329	ug/l	97
59) 2-Hexanone	11.194	43	3780	1.116	ug/l	69
67) Ethyl Benzene	11.965	91	3090	0.214	ug/l #	85
68) m/p-Xylenes	12.071	106	2456	0.477	ug/l #	57
69) o-Xylene	12.388	106	1654	0.329	ug/l #	19
76) 1,2,3-Trichloropropane	12.847	75	98357	26.112	ug/l #	1
78) n-propylbenzene	13.041	91	9187	0.586	ug/l	97
80) 1,3,5-Trimethylbenzene	13.176	105	15582	1.426	ug/l	96
81) trans-1,4-Dichloro-2-b...	12.847	75	98357	53.506	ug/l #	13
83) tert-Butylbenzene	13.482	119	4494	0.494	ug/l #	58
84) 1,2,4-Trimethylbenzene	13.482	105	37829	3.466	ug/l	96
85) sec-Butylbenzene	13.612	105	6552	0.511	ug/l	87
86) p-Isopropyltoluene	13.723	119	6473	0.629	ug/l	93
89) n-Butylbenzene	14.053	91	10163	1.061	ug/l #	72
90) Hexachloroethane	14.335	117	4123	2.036	ug/l #	17
92) 1,2-Dibromo-3-Chloropr...	14.688	75	662	0.701	ug/l #	2
95) Naphthalene	15.641	128	24632	2.410	ug/l #	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN042524\
Data File : VN081864.D
Acq On : 25 Apr 2024 20:40
Operator : JC\MD
Sample : P2246-03
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
SAW-CUTTING-LIQUID

Quant Time: Apr 26 05:41:54 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N042524W.M
Quant Title : SW846 8260
QLast Update : Fri Apr 26 05:26:49 2024
Response via : Initial Calibration

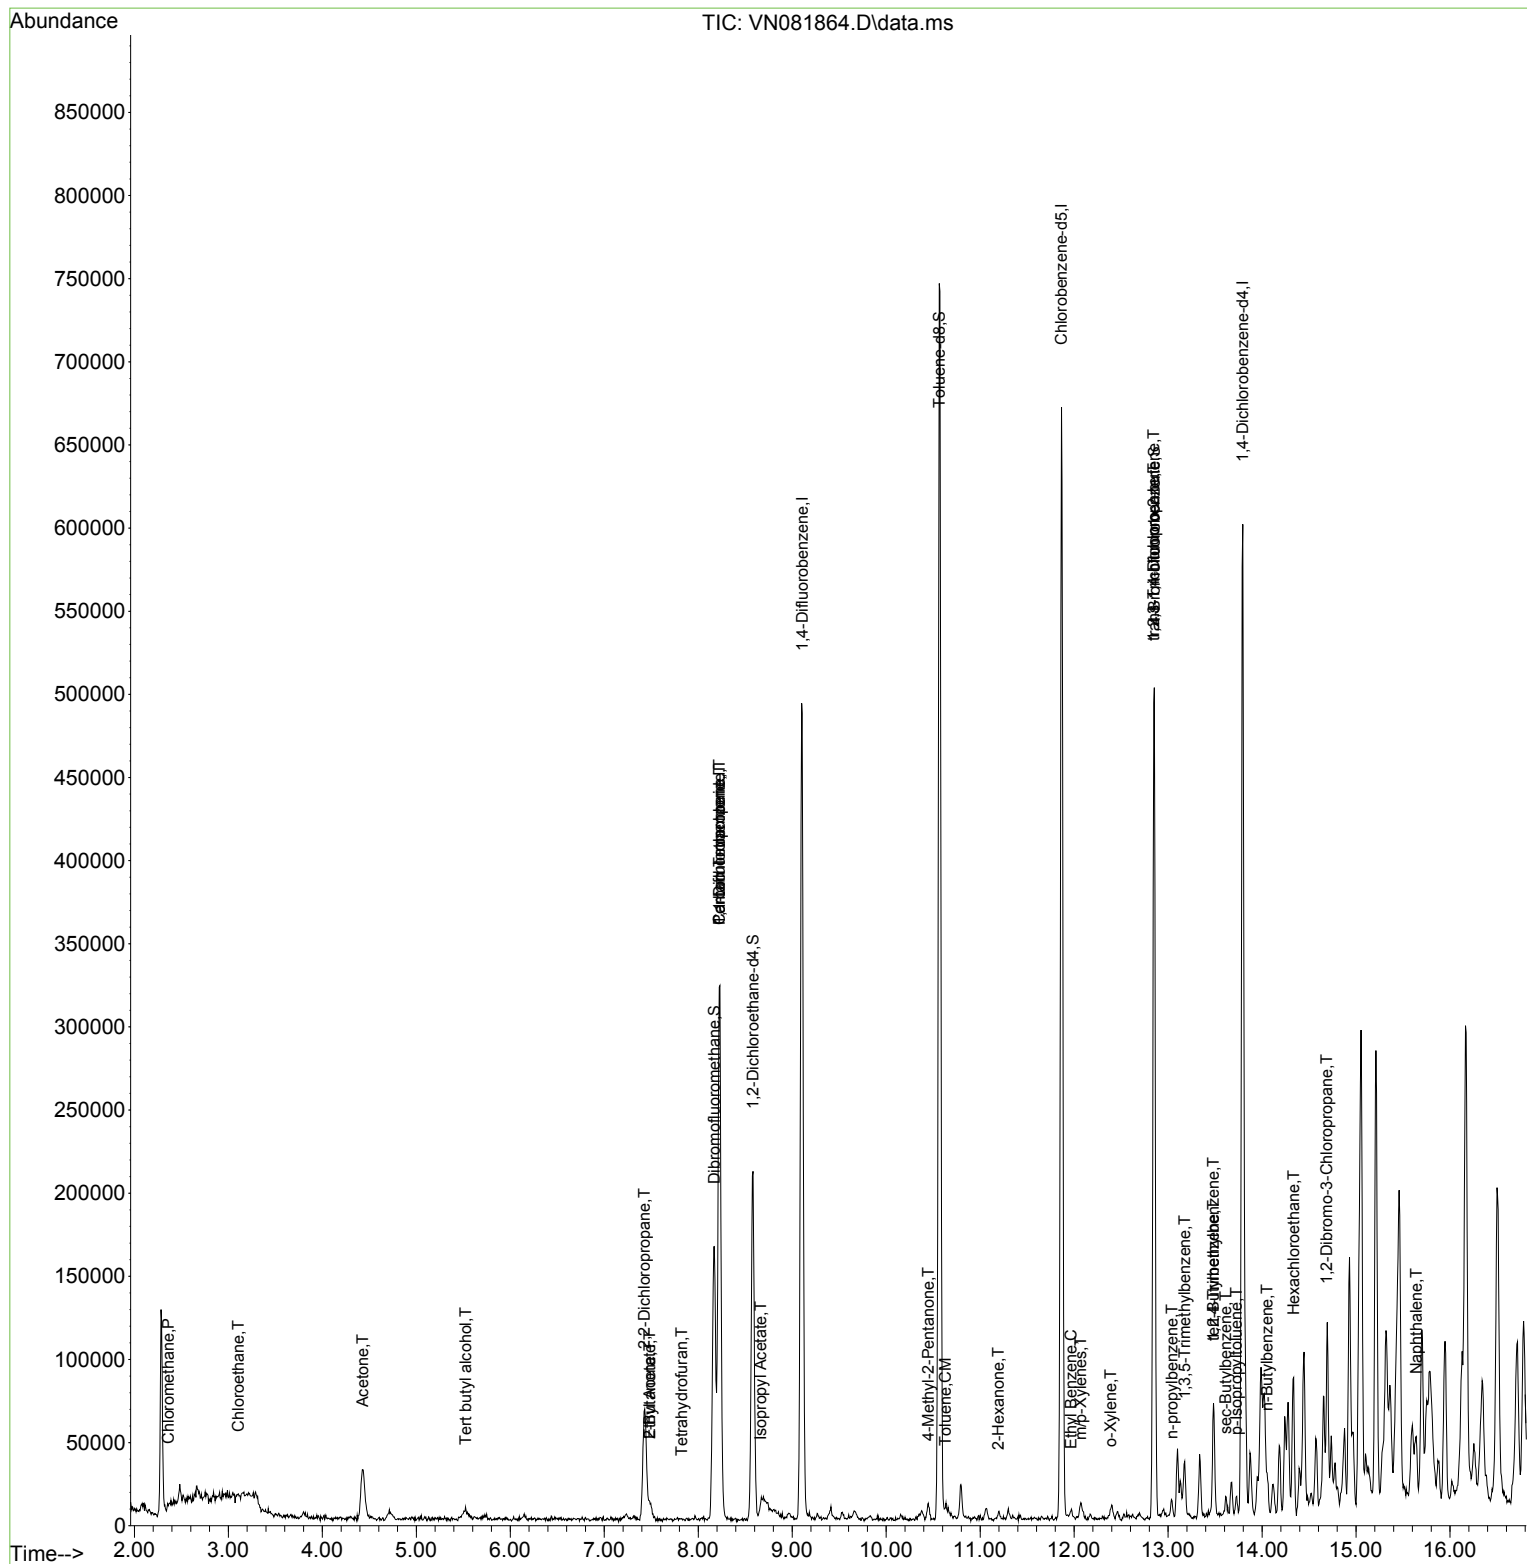



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 8.224 min Scan# 1066

Delta R.T. -0.000 min

Lab File: VN081864.D

Acq: 25 Apr 2024 20:40

Instrument :

MSVOA_N

ClientSampleId :





SAW-CUTTING-LIQUID

Tgt Ion:168 Resp: 219198

Ion Ratio Lower Upper

168 100

99 66.6 48.2 72.4

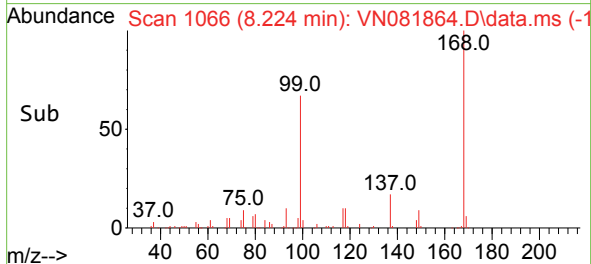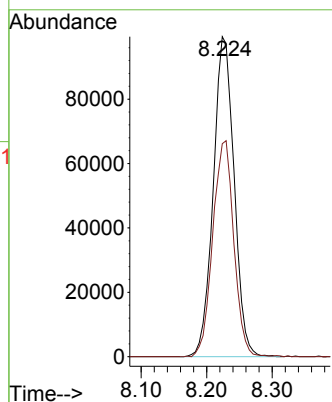

#3

Chloromethane

Concen: 0.325 ug/l

RT: 2.360 min Scan# 69

Delta R.T. 0.000 min

Lab File: VN081864.D




Acq: 25 Apr 2024 20:40


Tgt Ion: 50 Resp: 1042

Ion Ratio Lower Upper

50 100

52 0.0 25.5 38.3#


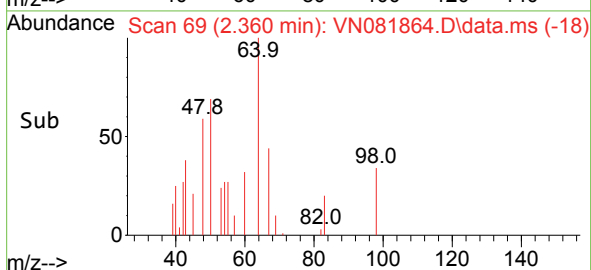






#5
Bromomethane
Concen: Below Cal
RT: 2.930 min Scan# 11
Delta R.T. -0.018 min
Lab File: VN081864.D
Acq: 25 Apr 2024 20:40




Instrument :
MSVOA_N
ClientSampleId :
SAW-CUTTING-LIQUID


Tgt Ion: 94 Resp: 70
Ion Ratio Lower Upper
94 100
96 3.0 74.8 112.2#

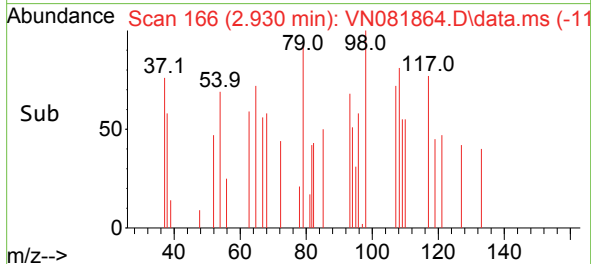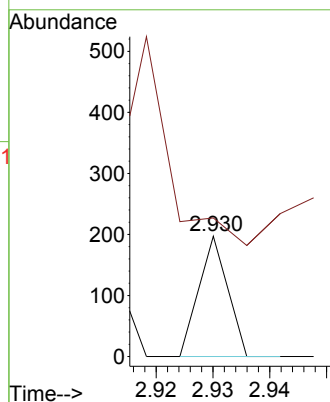

#6
Chloroethane
Concen: 0.594 ug/l
RT: 3.107 min Scan# 196
Delta R.T. -0.017 min
Lab File: VN081864.D
Acq: 25 Apr 2024 20:40

Tgt Ion: 64 Resp: 872
Ion Ratio Lower Upper
64 100
66 33.9 24.7 37.1

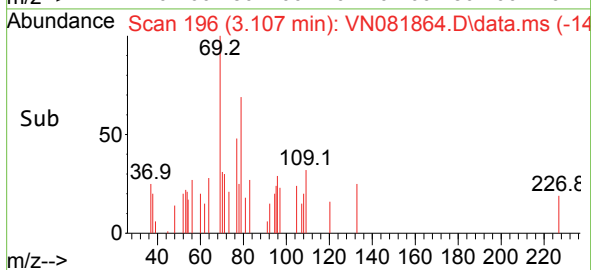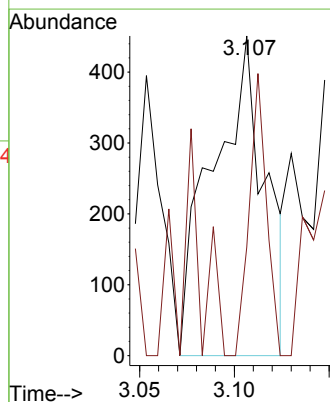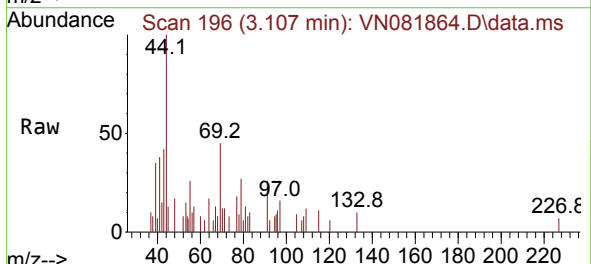



#11

Tert butyl alcohol

Concen: 16.890 ug/l

RT: 5.524 min Scan# 606

Delta R.T. 0.006 min

Lab File: VN081864.D

Acq: 25 Apr 2024 20:40

Instrument :

MSVOA_N

ClientSampleId :





SAW-CUTTING-LIQUID

Tgt Ion: 59 Resp: 11359

Ion Ratio Lower Upper

59 100

57 8.2 8.9 13.3#

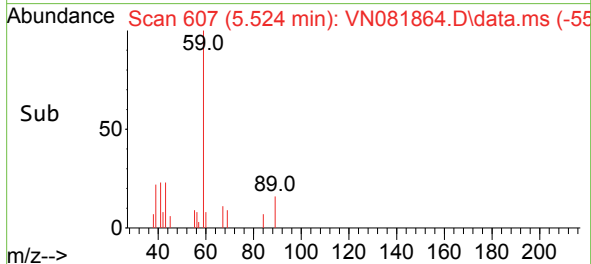

#13

Acrolein

Concen: Below Cal

RT: 4.171 min Scan# 377

Delta R.T. -0.006 min

Lab File: VN081864.D




Acq: 25 Apr 2024 20:40


Tgt Ion: 56 Resp: 184

Ion Ratio Lower Upper

56 100

55 276.6 55.8 83.8#



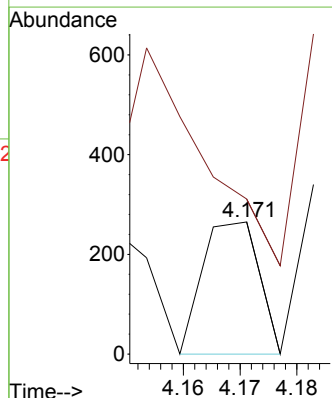
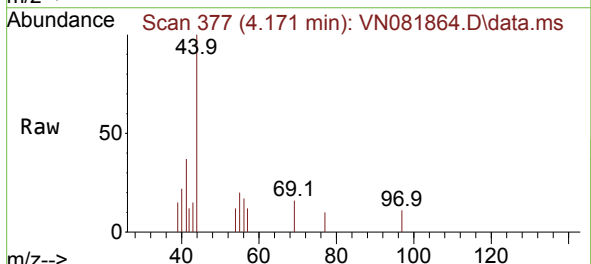




#16
Acetone
Concen: 50.663 ug/l
RT: 4.430 min Scan# 41
Delta R.T. 0.006 min
Lab File: VN081864.D
Acq: 25 Apr 2024 20:40




Instrument :
MSVOA_N
ClientSampleId :
SAW-CUTTING-LIQUID


Tgt Ion: 43 Resp: 60193
Ion Ratio Lower Upper
43 100
58 22.8 25.2 37.8#

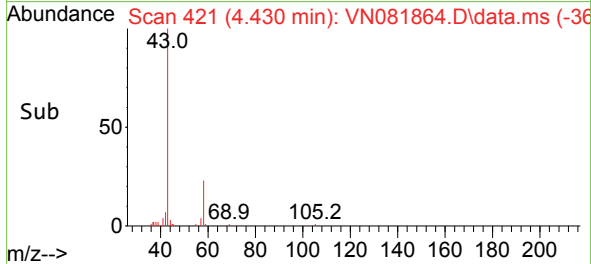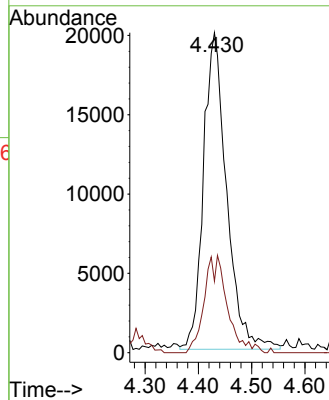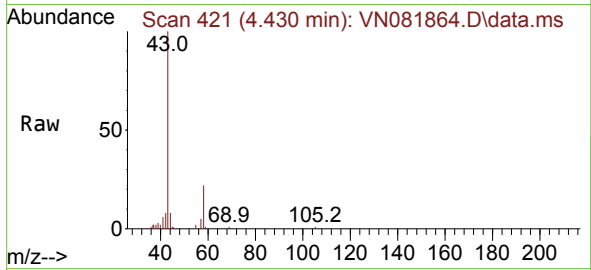

#25
2-Butanone
Concen: 7.986 ug/l
RT: 7.483 min Scan# 940
Delta R.T. 0.006 min
Lab File: VN081864.D
Acq: 25 Apr 2024 20:40

Tgt Ion: 43 Resp: 16769
Ion Ratio Lower Upper
43 100
72 19.3 25.3 37.9#



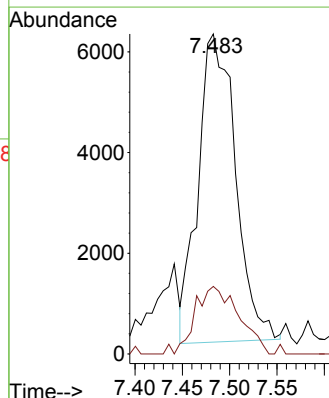
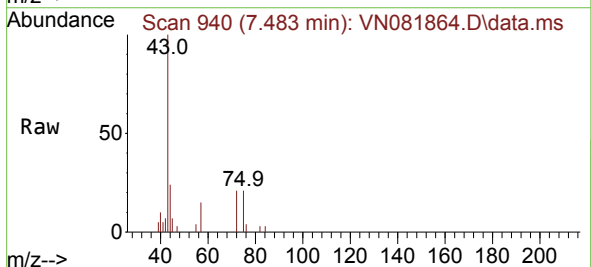




#26
2,2-Dichloropropane
Concen: 0.938 ug/l
RT: 7.424 min Scan# 91
Delta R.T. -0.065 min
Lab File: VN081864.D
Acq: 25 Apr 2024 20:40




Instrument :
MSVOA_N
ClientSampleId :
SAW-CUTTING-LIQUID


Tgt Ion: 77 Resp: 4881
Ion Ratio Lower Upper
77 100
97 0.0 11.3 33.9#

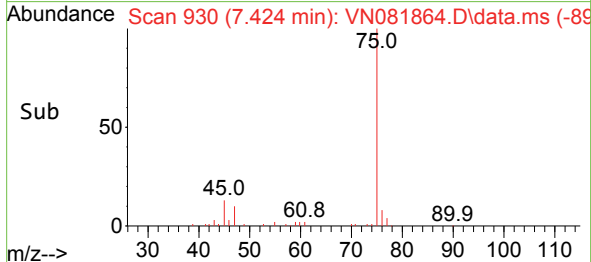

#29
Tetrahydrofuran
Concen: 0.307 ug/l
RT: 7.824 min Scan# 998
Delta R.T. -0.012 min
Lab File: VN081864.D
Acq: 25 Apr 2024 20:40

Tgt Ion: 42 Resp: 462
Ion Ratio Lower Upper
42 100
72 14.9 39.3 58.9#
71 17.7 37.4 56.0#

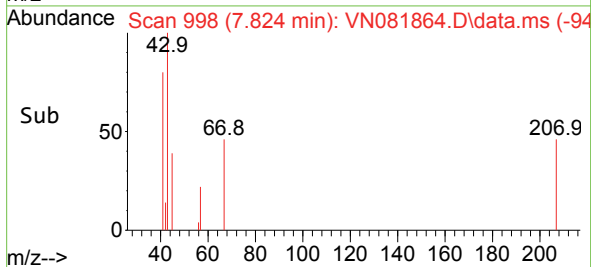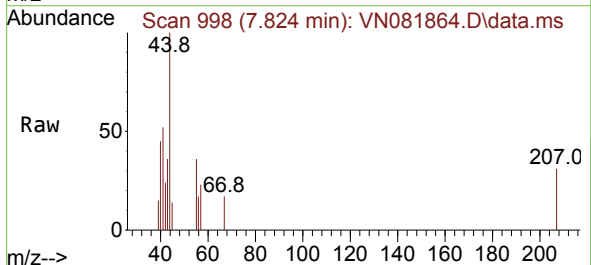



#33

1,2-Dichloroethane-d4

Concen: 45.930 ug/l

RT: 8.583 min Scan# 1126

Delta R.T. 0.006 min

Lab File: VN081864.D

Acq: 25 Apr 2024 20:40

Instrument :

MSVOA_N

ClientSampleId :





SAW-CUTTING-LIQUID

Tgt Ion: 65 Resp: 169916

Ion Ratio Lower Upper

65 100

67 51.4 0.0 103.0



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.106 min Scan# 1216

Delta R.T. 0.006 min

Lab File: VN081864.D

Acq: 25 Apr 2024 20:40




Tgt Ion: 114 Resp: 405914


Ion Ratio Lower Upper

114 100

63 21.3 0.0 41.0

88 16.6 0.0 31.4


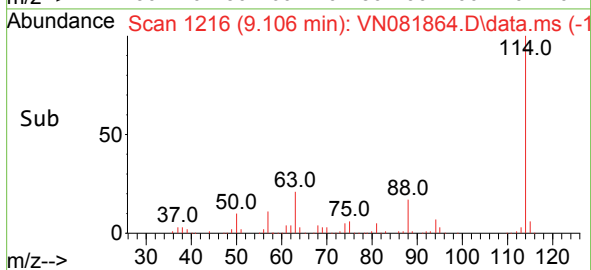

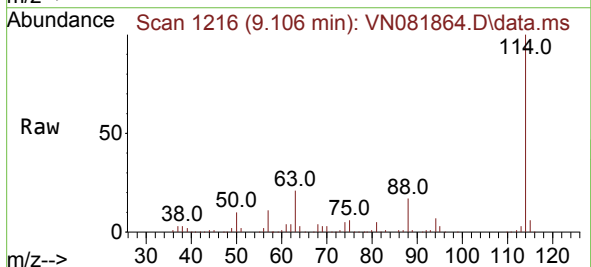




#35
Dibromofluoromethane
Concen: 49.829 ug/l
RT: 8.171 min Scan# 1056
Delta R.T. 0.006 min
Lab File: VN081864.D
Acq: 25 Apr 2024 20:40




Instrument :
MSVOA_N
ClientSampleId :
SAW-CUTTING-LIQUID


Tgt Ion:113 Resp: 121779
Ion Ratio Lower Upper
113 100
111 102.3 83.4 125.2
192 17.3 14.0 21.0

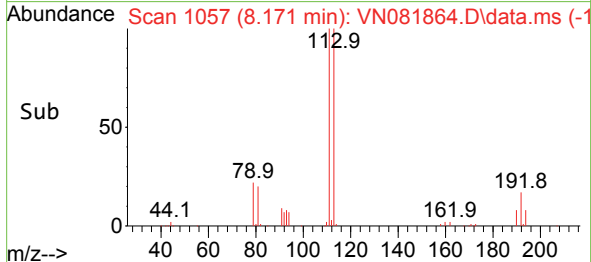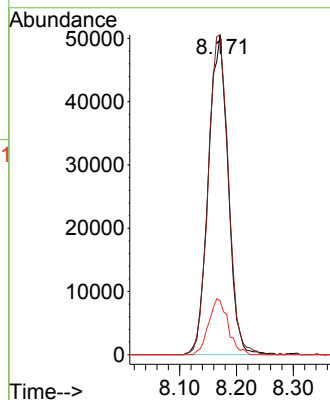

#36
1,1-Dichloropropene
Concen: 5.245 ug/l
RT: 8.224 min Scan# 1066
Delta R.T. -0.147 min
Lab File: VN081864.D
Acq: 25 Apr 2024 20:40

Tgt Ion: 75 Resp: 20853
Ion Ratio Lower Upper
75 100
110 8.1 17.8 53.5#
77 0.0 25.0 37.4#


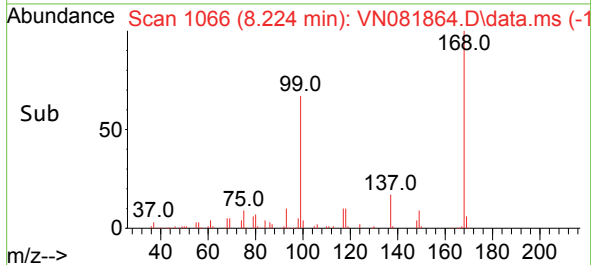
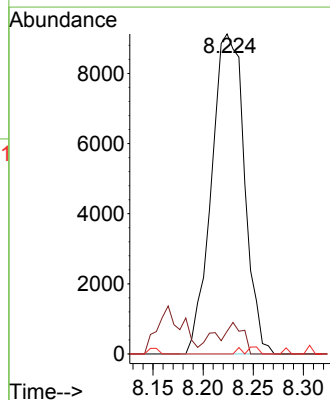
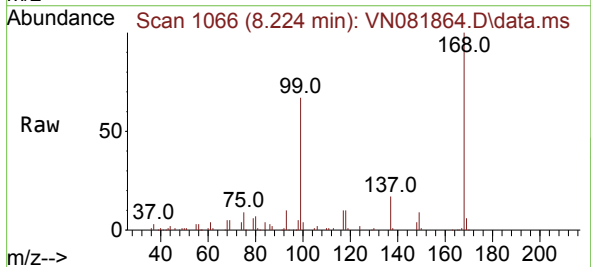




#37
Ethyl Acetate
Concen: 3.900 ug/l
RT: 7.483 min Scan# 94
Delta R.T. -0.076 min
Lab File: VN081864.D
Acq: 25 Apr 2024 20:40




Instrument :
MSVOA_N
ClientSampleId :
SAW-CUTTING-LIQUID


Tgt Ion: 43 Resp: 16766
Ion Ratio Lower Upper
43 100
61 0.0 11.3 16.9#
70 1.6 8.7 13.1#

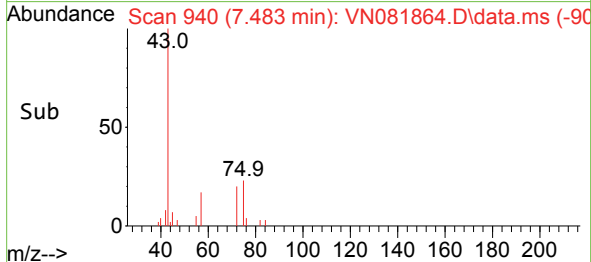

#38
Carbon Tetrachloride
Concen: 5.866 ug/l
RT: 8.224 min Scan# 1066
Delta R.T. -0.135 min
Lab File: VN081864.D
Acq: 25 Apr 2024 20:40

Tgt Ion: 117 Resp: 22796
Ion Ratio Lower Upper
117 100
119 6.7 76.5 114.7#
121 0.0 23.9 35.9#


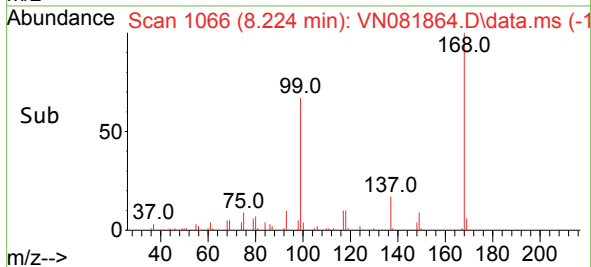

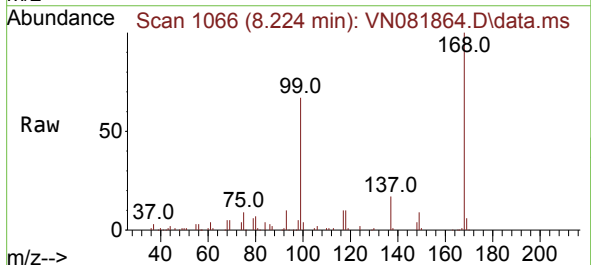




#43
Isopropyl Acetate
Concen: 0.953 ug/l
RT: 8.665 min Scan# 1141
Delta R.T. -0.023 min
Lab File: VN081864.D
Acq: 25 Apr 2024 20:40




Instrument :
MSVOA_N
ClientSampleId :
SAW-CUTTING-LIQUID


Tgt Ion: 43 Resp: 7706
Ion Ratio Lower Upper
43 100
61 0.0 22.8 34.2#
87 0.0 12.0 18.0#

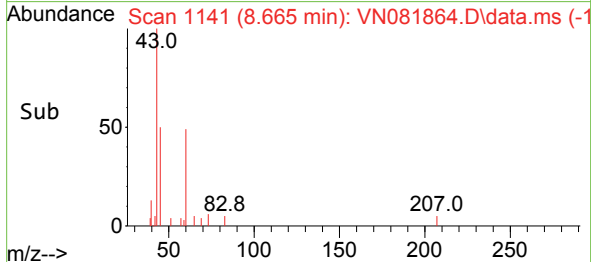

#50
Toluene-d8
Concen: 52.175 ug/l
RT: 10.565 min Scan# 1464
Delta R.T. 0.000 min
Lab File: VN081864.D
Acq: 25 Apr 2024 20:40

Tgt Ion: 98 Resp: 500796
Ion Ratio Lower Upper
98 100
100 64.5 51.8 77.6

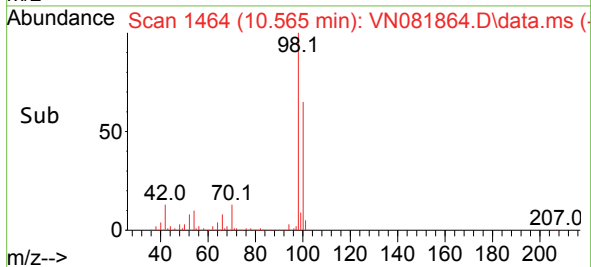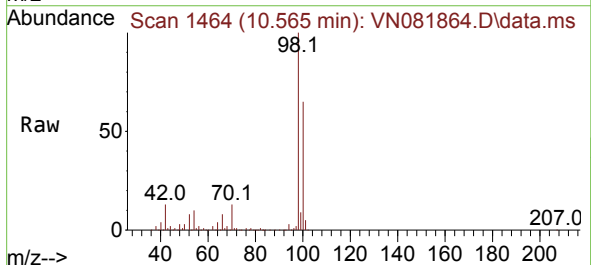

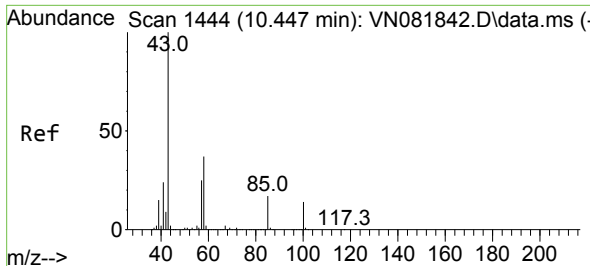

#51

4-Methyl-2-Pentanone

Concen: 1.523 ug/l

RT: 10.447 min Scan# 1444

Delta R.T. 0.000 min

Lab File: VN081864.D

Acq: 25 Apr 2024 20:40

Instrument :

MSVOA_N

ClientSampleId :





SAW-CUTTING-LIQUID

Tgt Ion: 43 Resp: 6928

Ion Ratio Lower Upper

43 100

58 39.2 33.2 49.8

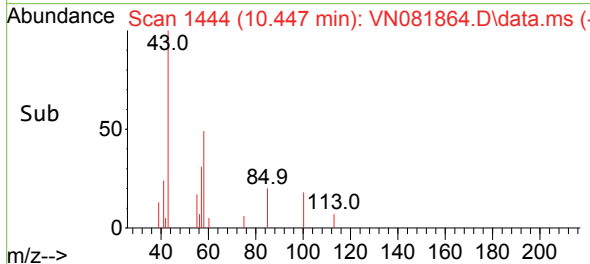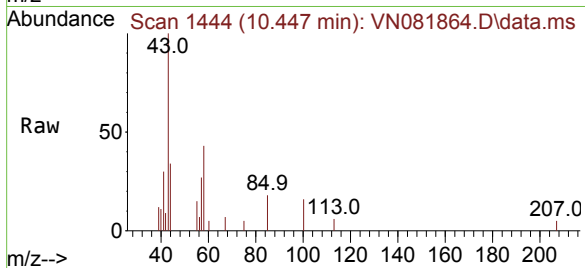

#52

Toluene

Concen: 0.329 ug/l

RT: 10.630 min Scan# 1475

Delta R.T. 0.000 min

Lab File: VN081864.D




Acq: 25 Apr 2024 20:40


Tgt Ion: 92 Resp: 2349

Ion Ratio Lower Upper

92 100

91 174.9 136.7 205.1


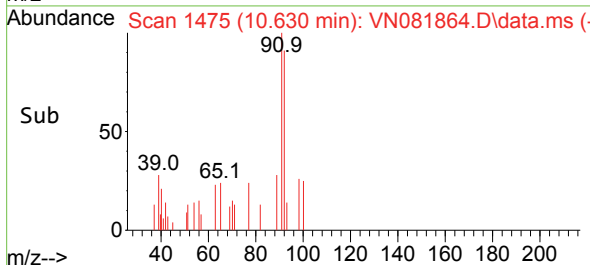
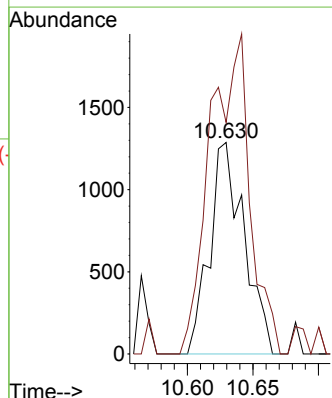
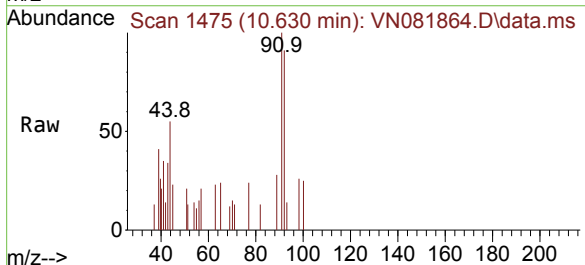




#59
2-Hexanone
Concen: 1.116 ug/l
RT: 11.194 min Scan# 111
Delta R.T. 0.000 min
Lab File: VN081864.D
Acq: 25 Apr 2024 20:40




Instrument :
MSVOA_N
ClientSampleId :
SAW-CUTTING-LIQUID


Tgt Ion: 43 Resp: 3780
Ion Ratio Lower Upper
43 100
58 34.0 28.3 84.9

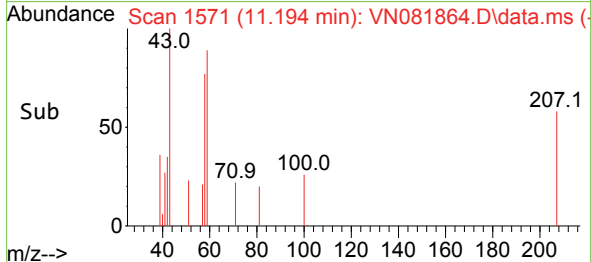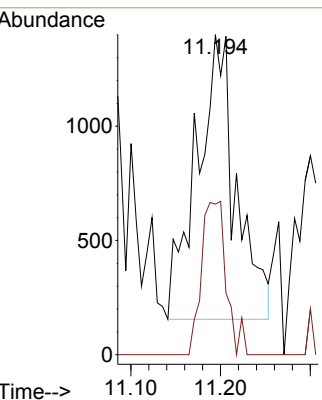

#62
4-Bromofluorobenzene
Concen: 48.004 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. 0.006 min
Lab File: VN081864.D
Acq: 25 Apr 2024 20:40

Tgt Ion: 95 Resp: 182142
Ion Ratio Lower Upper
95 100
174 63.2 0.0 160.6
176 61.6 0.0 152.8


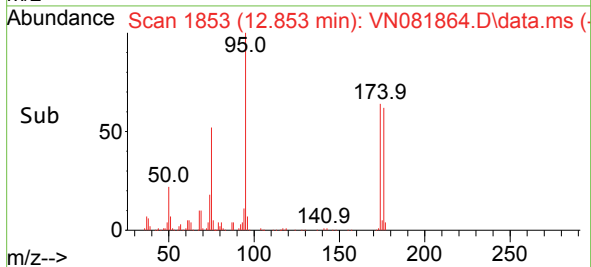
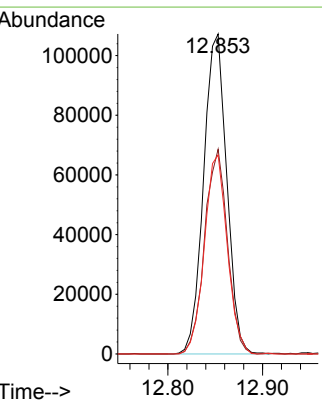
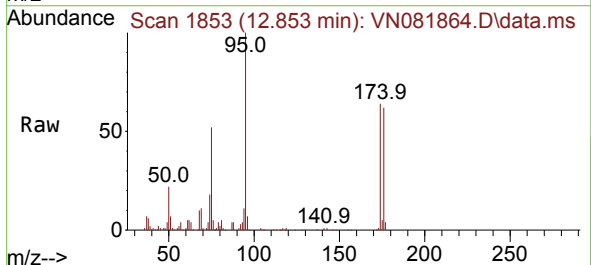


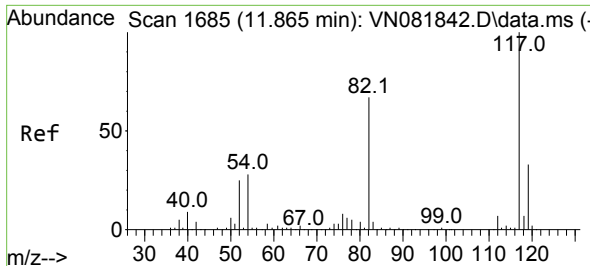

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.865 min Scan# 1170
Delta R.T. 0.000 min
Lab File: VN081864.D
Acq: 25 Apr 2024 20:40




Instrument :
MSVOA_N
ClientSampleId :
SAW-CUTTING-LIQUID


Tgt Ion:117 Resp: 355241
Ion Ratio Lower Upper
117 100
82 65.6 44.6 66.8
119 32.0 25.9 38.9

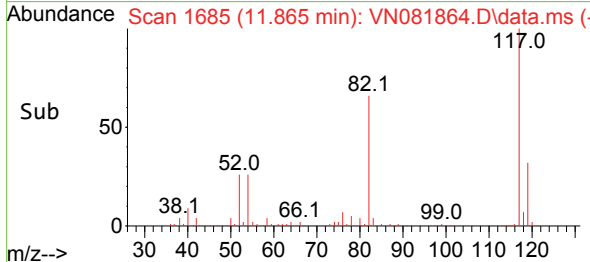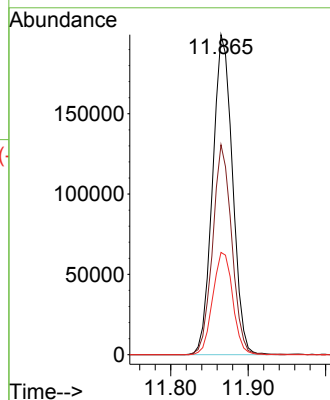

#67
Ethyl Benzene
Concen: 0.214 ug/l
RT: 11.965 min Scan# 1702
Delta R.T. 0.000 min
Lab File: VN081864.D
Acq: 25 Apr 2024 20:40

Tgt Ion: 91 Resp: 3090
Ion Ratio Lower Upper
91 100
106 23.2 25.3 37.9#


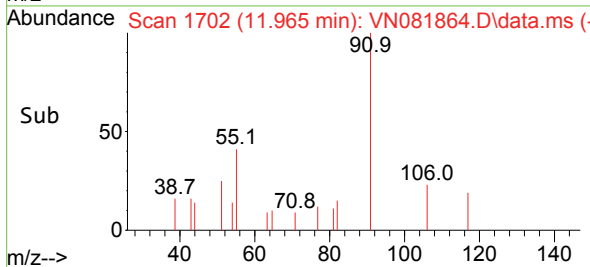
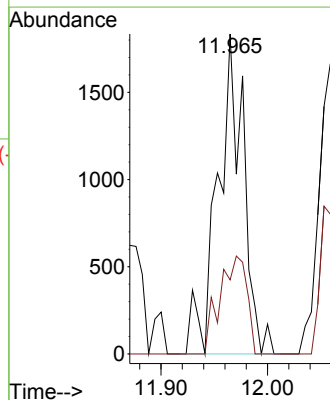
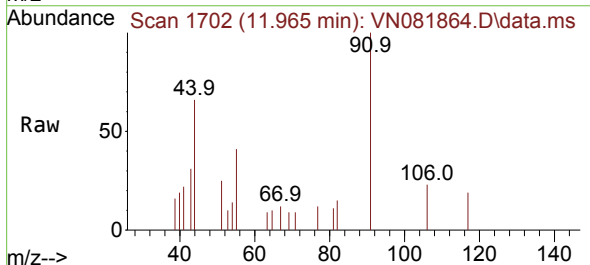




#68
m/p-Xylenes
Concen: 0.477 ug/l
RT: 12.071 min Scan# 1720
Delta R.T. 0.000 min
Lab File: VN081864.D
Acq: 25 Apr 2024 20:40




Instrument :
MSVOA_N
ClientSampleId :
SAW-CUTTING-LIQUID


Tgt Ion:106 Resp: 2456
Ion Ratio Lower Upper
106 100
91 264.7 159.4 239.0#

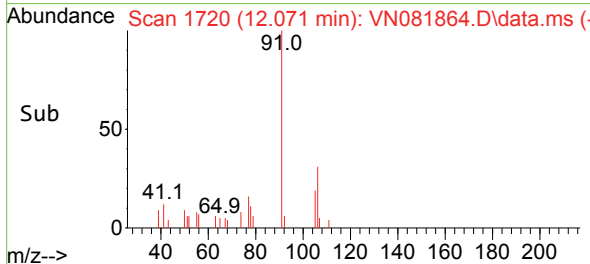

#69
o-Xylene
Concen: 0.329 ug/l
RT: 12.388 min Scan# 1774
Delta R.T. -0.012 min
Lab File: VN081864.D
Acq: 25 Apr 2024 20:40

Tgt Ion:106 Resp: 1654
Ion Ratio Lower Upper
106 100
91 334.9 104.7 314.1#

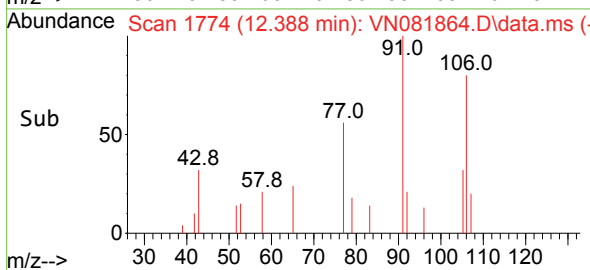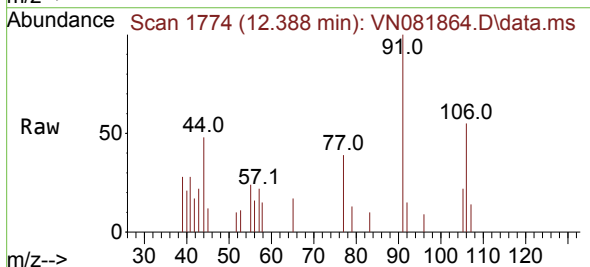



#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.794 min Scan# 20

Delta R.T. 0.000 min

Lab File: VN081864.D

Acq: 25 Apr 2024 20:40

Instrument :

MSVOA_N

ClientSampleId :

SAW-CUTTING-LIQUID





Tgt Ion:152 Resp: 145279

Ion Ratio Lower Upper

152 100

115 68.3 30.4 91.3

150 160.9 0.0 353.2

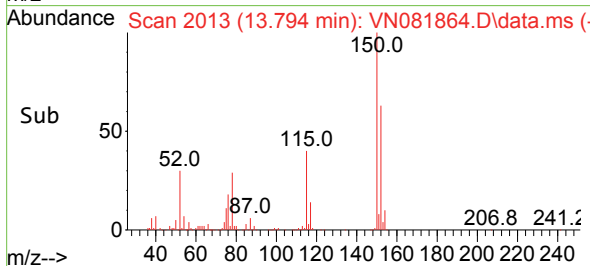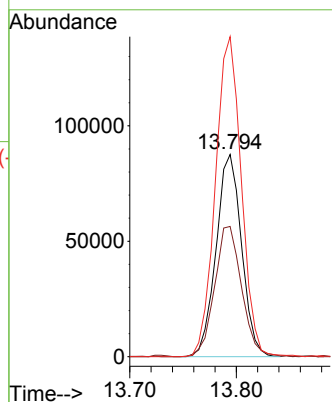

#76

1,2,3-Trichloropropane

Concen: 26.112 ug/l

RT: 12.847 min Scan# 1852

Delta R.T. -0.147 min

Lab File: VN081864.D




Acq: 25 Apr 2024 20:40


Tgt Ion: 75 Resp: 98357

Ion Ratio Lower Upper

75 100

77 0.7 90.5 271.3#

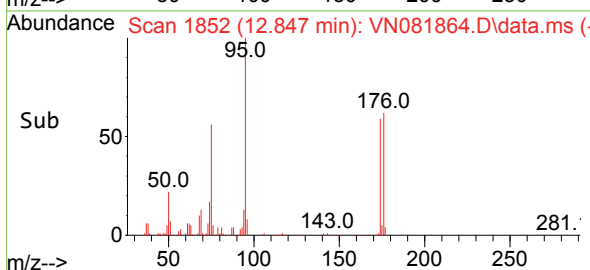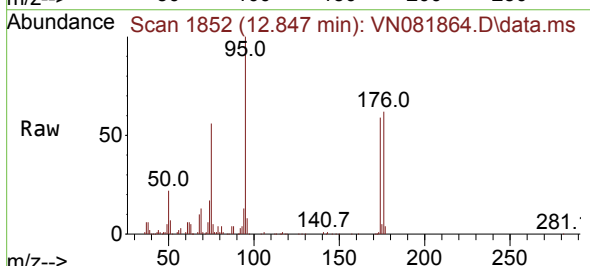



#78

n-propylbenzene

Concen: 0.586 ug/l

RT: 13.041 min Scan# 1884

Delta R.T. 0.006 min

Lab File: VN081864.D

Acq: 25 Apr 2024 20:40

Instrument :

MSVOA_N

ClientSampleId :





SAW-CUTTING-LIQUID

Tgt Ion: 91 Resp: 9187

Ion Ratio Lower Upper

91 100

120 21.8 11.7 35.0

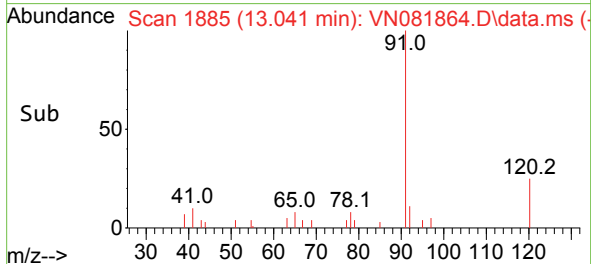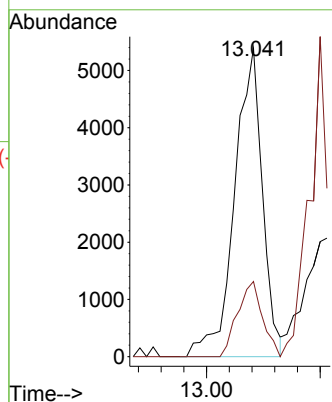

#80

1,3,5-Trimethylbenzene

Concen: 1.426 ug/l

RT: 13.176 min Scan# 1908

Delta R.T. 0.000 min

Lab File: VN081864.D




Acq: 25 Apr 2024 20:40


Tgt Ion:105 Resp: 15582

Ion Ratio Lower Upper

105 100

120 47.0 24.8 74.3


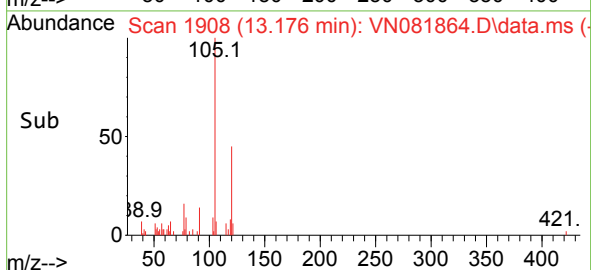






#81
 trans-1,4-Dichloro-2-butene
 Concen: 53.506 ug/l
 RT: 12.847 min Scan# 11
 Delta R.T. 0.106 min
 Lab File: VN081864.D
 Acq: 25 Apr 2024 20:40




Instrument :
 MSVOA_N
 ClientSampleId :
 SAW-CUTTING-LIQUID


Tgt Ion: 75 Resp: 98357
 Ion Ratio Lower Upper
 75 100
 53 0.2 72.9 109.3#
 89 0.1 39.1 58.7#

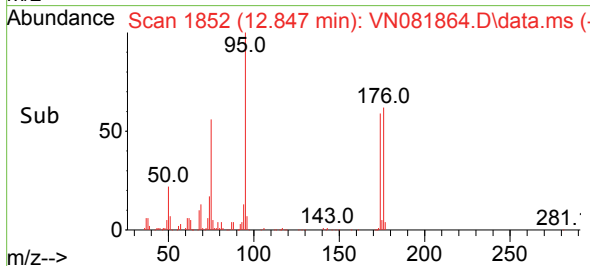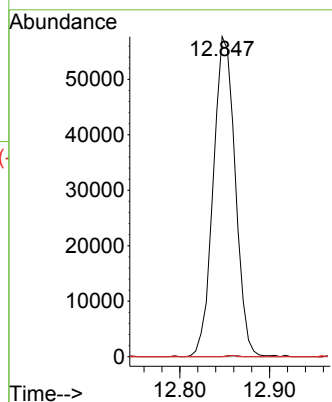

#83
 tert-Butylbenzene
 Concen: 0.494 ug/l
 RT: 13.482 min Scan# 1960
 Delta R.T. 0.041 min
 Lab File: VN081864.D
 Acq: 25 Apr 2024 20:40

Tgt Ion: 119 Resp: 4494
 Ion Ratio Lower Upper
 119 100
 91 96.4 32.6 97.8
 134 0.0 12.4 37.0#

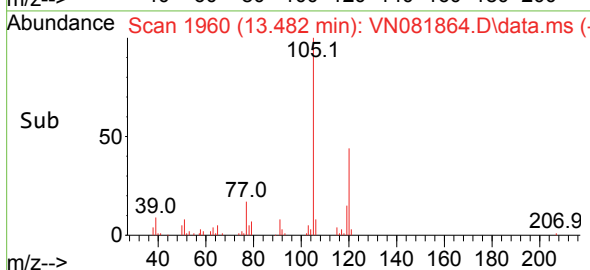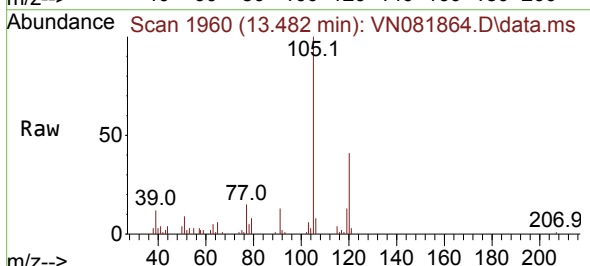

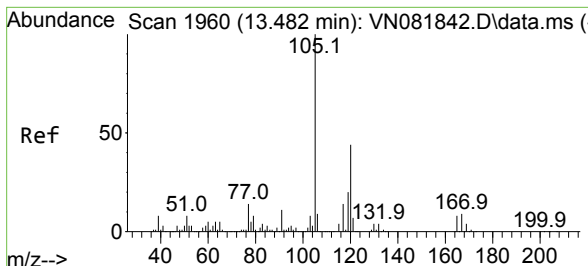

#84

1,2,4-Trimethylbenzene

Concen: 3.466 ug/l

RT: 13.482 min Scan# 1960

Delta R.T. 0.000 min

Lab File: VN081864.D

Acq: 25 Apr 2024 20:40

Instrument :

MSVOA_N

ClientSampleId :





SAW-CUTTING-LIQUID

Tgt Ion:105 Resp: 37829

Ion Ratio Lower Upper

105 100

120 43.0 22.9 68.7

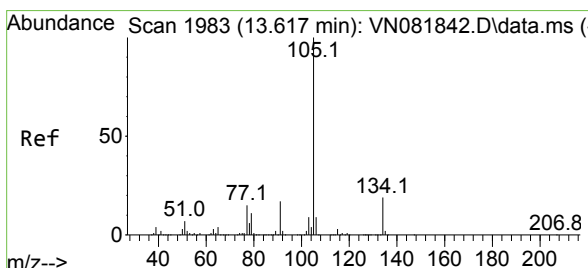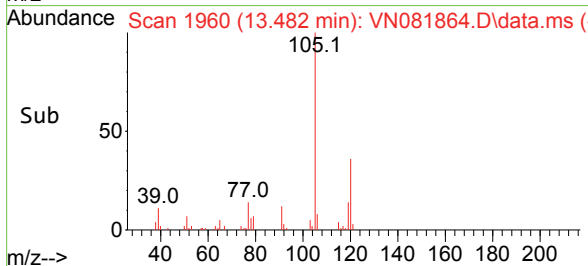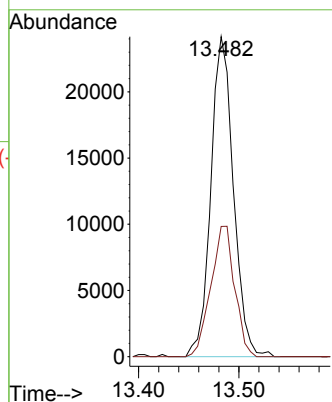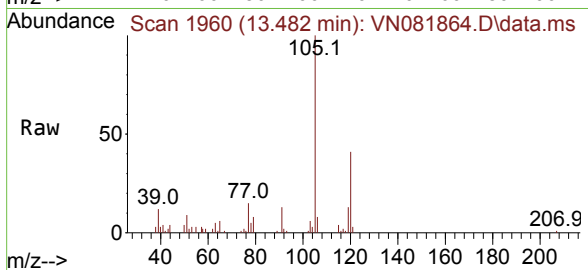

#85

sec-Butylbenzene

Concen: 0.511 ug/l

RT: 13.612 min Scan# 1982

Delta R.T. -0.006 min

Lab File: VN081864.D




Acq: 25 Apr 2024 20:40


Tgt Ion:105 Resp: 6552

Ion Ratio Lower Upper

105 100

134 26.5 10.2 30.4

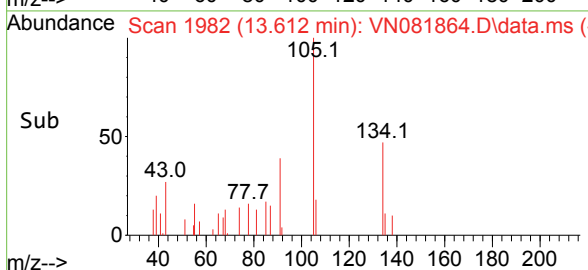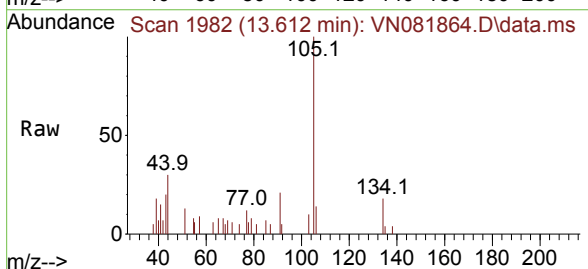



#86

p-Isopropyltoluene

Concen: 0.629 ug/l

RT: 13.723 min Scan# 2002

Delta R.T. -0.006 min

Lab File: VN081864.D

Acq: 25 Apr 2024 20:40

Instrument :

MSVOA_N

ClientSampleId :

SAW-CUTTING-LIQUID





Tgt Ion:119 Resp: 6473

Ion Ratio Lower Upper

119 100

134 27.3 13.2 39.5

91 30.0 11.8 35.3

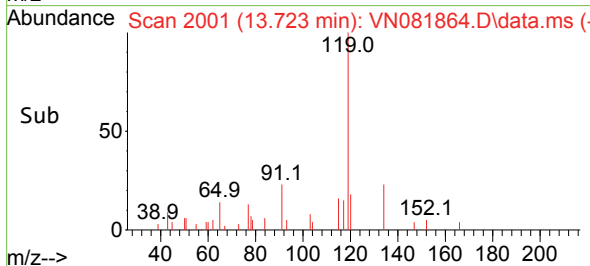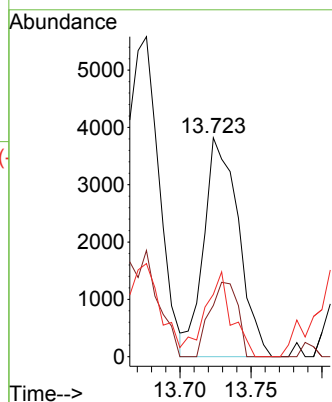

#89

n-Butylbenzene

Concen: 1.061 ug/l

RT: 14.053 min Scan# 2057

Delta R.T. -0.006 min

Lab File: VN081864.D

Acq: 25 Apr 2024 20:40




Tgt Ion: 91 Resp: 10163


Ion Ratio Lower Upper

91 100

92 63.9 26.2 78.5

134 0.0 13.2 39.5#

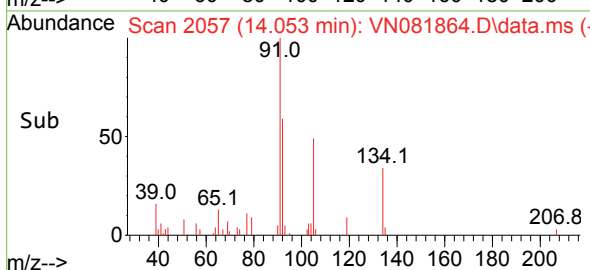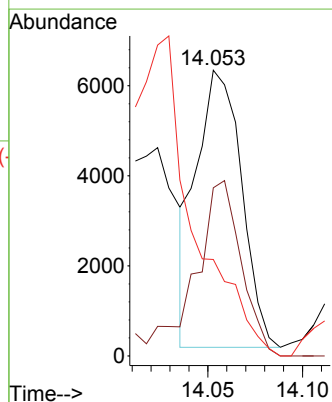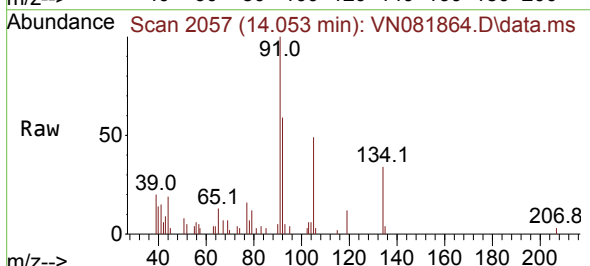



#90

Hexachloroethane

Concen: 2.036 ug/l

RT: 14.335 min Scan# 2105

Delta R.T. 0.000 min

Lab File: VN081864.D

Acq: 25 Apr 2024 20:40

Instrument :

MSVOA_N

ClientSampleId :





SAW-CUTTING-LIQUID

Tgt Ion:117 Resp: 4123

Ion Ratio Lower Upper

117 100

201 0.0 33.3 99.8#

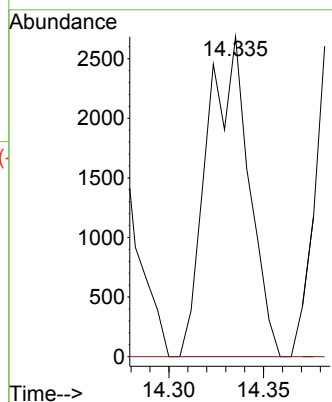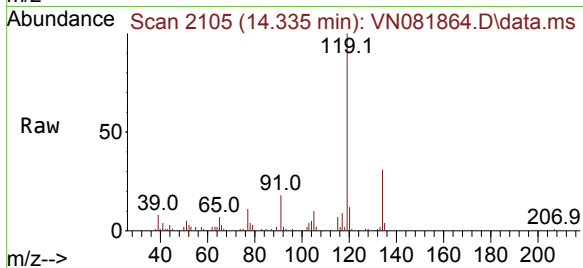

#92

1,2-Dibromo-3-Chloropropane

Concen: 0.701 ug/l

RT: 14.688 min Scan# 2165

Delta R.T. -0.029 min

Lab File: VN081864.D

Acq: 25 Apr 2024 20:40




Tgt Ion: 75 Resp: 662


Ion Ratio Lower Upper

75 100

155 0.0 42.6 128.0#

157 0.0 53.0 159.0#

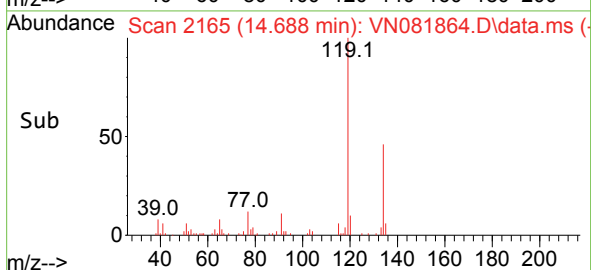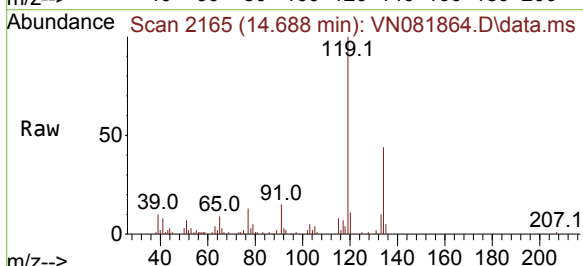

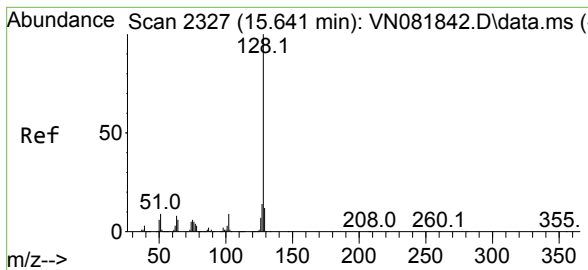

#95
Naphthalene
Concen: 2.410 ug/l
RT: 15.641 min Scan# 21
Delta R.T. 0.000 min
Lab File: VN081864.D
Acq: 25 Apr 2024 20:40

Instrument :
MSVOA_N
ClientSampleId :
SAW-CUTTING-LIQUID

Tgt Ion:	128	Resp:	24632
Ion	Ratio	Lower	Upper
128	100		
127	16.0	10.1	15.1#
129	15.9	8.9	13.3#

