
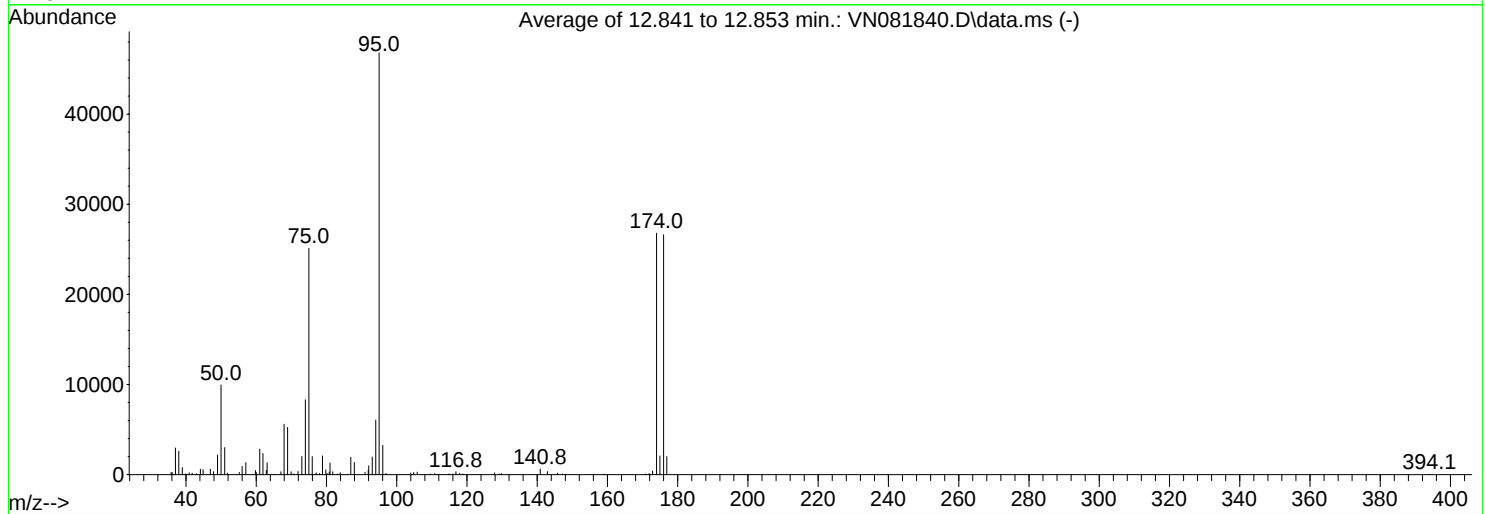


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN042524\
Data File : VN081840.D
Acq On : 25 Apr 2024 09:33
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N042524W.M
Title : SW846 8260
Last Update : Fri Apr 26 05:26:49 2024

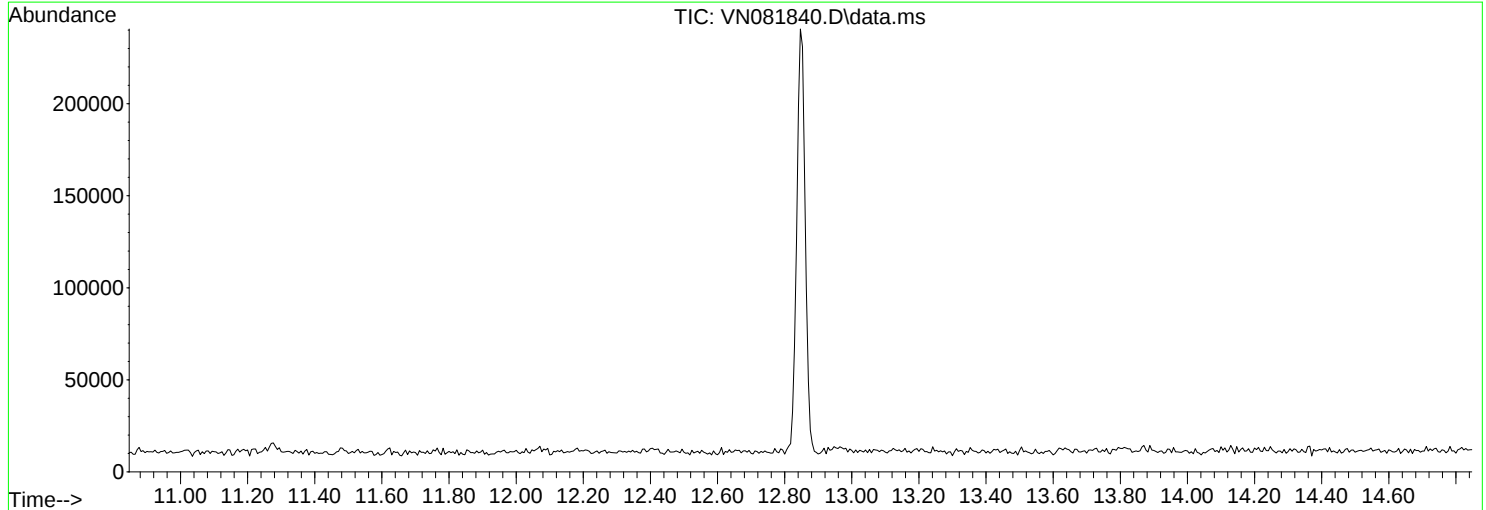

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.3	9957	PASS
75	95	30	60	53.7	25112	PASS
95	95	100	100	100.0	46795	PASS
96	95	5	9	7.0	3256	PASS
173	174	0.00	2	1.5	392	PASS
174	95	50	100	57.2	26789	PASS
175	174	5	9	7.8	2087	PASS
176	174	95	101	99.3	26613	PASS
177	176	5	9	7.6	2011	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.80	268	46.95	604	61.00	2844	73.00	200
36.10	238	47.85	330	61.95	2351	74.00	830
37.00	2971	49.00	2167	62.90	482	75.00	2511
37.95	2600	50.00	9957	63.10	1321	75.95	201
38.95	782	51.05	2997	65.10	59	76.80	61
39.80	75	51.80	182	67.05	327	77.10	192
40.95	197	55.20	256	67.95	5588	78.05	119
41.80	157	56.00	933	68.95	5242	78.85	2084
42.95	103	57.05	1339	69.95	323	79.85	538
44.10	611	59.80	469	70.70	92	80.20	129
44.90	552	60.00	253	71.90	362	80.80	282

Average of 12.841 to 12.853 min.: VN081840.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
81.00	1295	94.05	6057	115.90	70	147.20	64
81.80	323	95.00	46795	116.85	324	148.00	56
83.10	67	96.05	3256	117.95	166	159.00	56
83.95	237	96.95	137	118.70	63	170.90	72
86.10	59	104.00	173	119.00	60	171.85	121
86.95	1941	104.85	232	127.90	204	172.85	392
87.95	1344	105.85	279	129.20	67	174.00	26789
91.00	262	109.60	76	129.80	122	174.95	2087
91.90	487	110.85	121	140.85	620	176.00	26613
92.05	969	114.80	52	142.90	340	176.90	2011
93.05	1959	115.00	59	145.80	166	394.10	59

Instrument :

MSVOA_N

ClientSampleId :

BFB