

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN042621\
 Data File : VN066767.D
 Acq On : 26 Apr 2021 17:27
 Operator : JC/MD
 Sample : PB135974ZHE#03
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Apr 27 06:13:41 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N042121W.M
 Quant Title : SW846 8260
 QLast Update : Thu Apr 22 08:25:55 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.591	168	395498	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.519	114	612814	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.348	117	553952	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.287	152	244218	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	7.953	65	235488	48.74	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery =	97.48%		
35) Dibromofluoromethane	7.513	113	186707	48.65	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery =	97.30%		
50) Toluene-d8	10.029	98	752928	50.31	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery =	100.62%		
62) 4-Bromofluorobenzene	12.346	95	249561	48.69	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery =	97.38%		
Target Compounds						Qvalue
3) Chloromethane	2.037	50	1556	0.24	ug/l	90
11) Tert butyl alcohol	4.689	59	221	0.36	ug/l #	73
13) Acrolein	3.560	56	1180	1.74	ug/l #	51
16) Acetone	3.756	43	44730	24.73	ug/l	94
18) Methyl Acetate	4.260	43	4379	0.87	ug/l	90
20) Methylene Chloride	4.469	84	26333	4.90	ug/l	95
25) 2-Butanone	6.760	43	5559	2.14	ug/l #	88
29) Tetrahydrofuran	7.132	42	713	0.40	ug/l #	32
31) Cyclohexane	7.591	56	7969	1.01	ug/l #	1
36) 1,1-Dichloropropene	7.588	75	28632	5.03	ug/l #	48
37) Ethyl Acetate	6.760	43	5559	0.93	ug/l #	68
38) Carbon Tetrachloride	7.591	117	35438	6.53	ug/l #	17
43) Isopropyl Acetate	8.098	43	38429	4.02	ug/l #	87
45) 1,2-Dichloropropane	9.205	63	2442	0.49	ug/l #	44
48) Methyl methacrylate	9.117	41	7251	1.73	ug/l #	10
49) 1,4-Dioxane	9.203	88	109	2.15	ug/l #	1
51) 4-Methyl-2-Pentanone	9.922	43	10130	1.89	ug/l	92
54) cis-1,3-Dichloropropene	9.844	75	65209	8.86	ug/l #	61
56) Ethyl methacrylate	10.396	69	415	3.21	ug/l #	27
57) 1,3-Dichloropropane	10.705	76	37011	5.16	ug/l #	43
59) 2-Hexanone	10.707	43	522265	138.14	ug/l #	49
71) Bromoform	12.349	173	1512	0.49	ug/l #	1
76) 1,2,3-Trichloropropane	12.346	75	124631	23.85	ug/l #	100
79) 2-Chlorotoluene	12.614	91	51	0.94	ug/l #	40
80) 1,3,5-Trimethylbenzene	12.687	105	3751	0.25	ug/l	95
81) trans-1,4-Dichloro-2-b...	12.346	75	124631	70.50	ug/l #	12
92) 1,2-Dibromo-3-Chloropr...	14.213	75	238	0.23	ug/l #	24
93) 1,2,4-Trichlorobenzene	14.878	180	283	2.06	ug/l #	54
95) Naphthalene	15.060	128	360	1.88	ug/l #	39
96) 1,2,3-Trichlorobenzene	15.248	180	117	1.38	ug/l #	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN042621\
Data File : VN066767.D
Acq On : 26 Apr 2021 17:27
Operator : JC/MD
Sample : PB135974ZHE#03
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :

Quant Time: Apr 27 06:13:41 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N042121W.M
Quant Title : SW846 8260
QLast Update : Thu Apr 22 08:25:55 2021
Response via : Initial Calibration




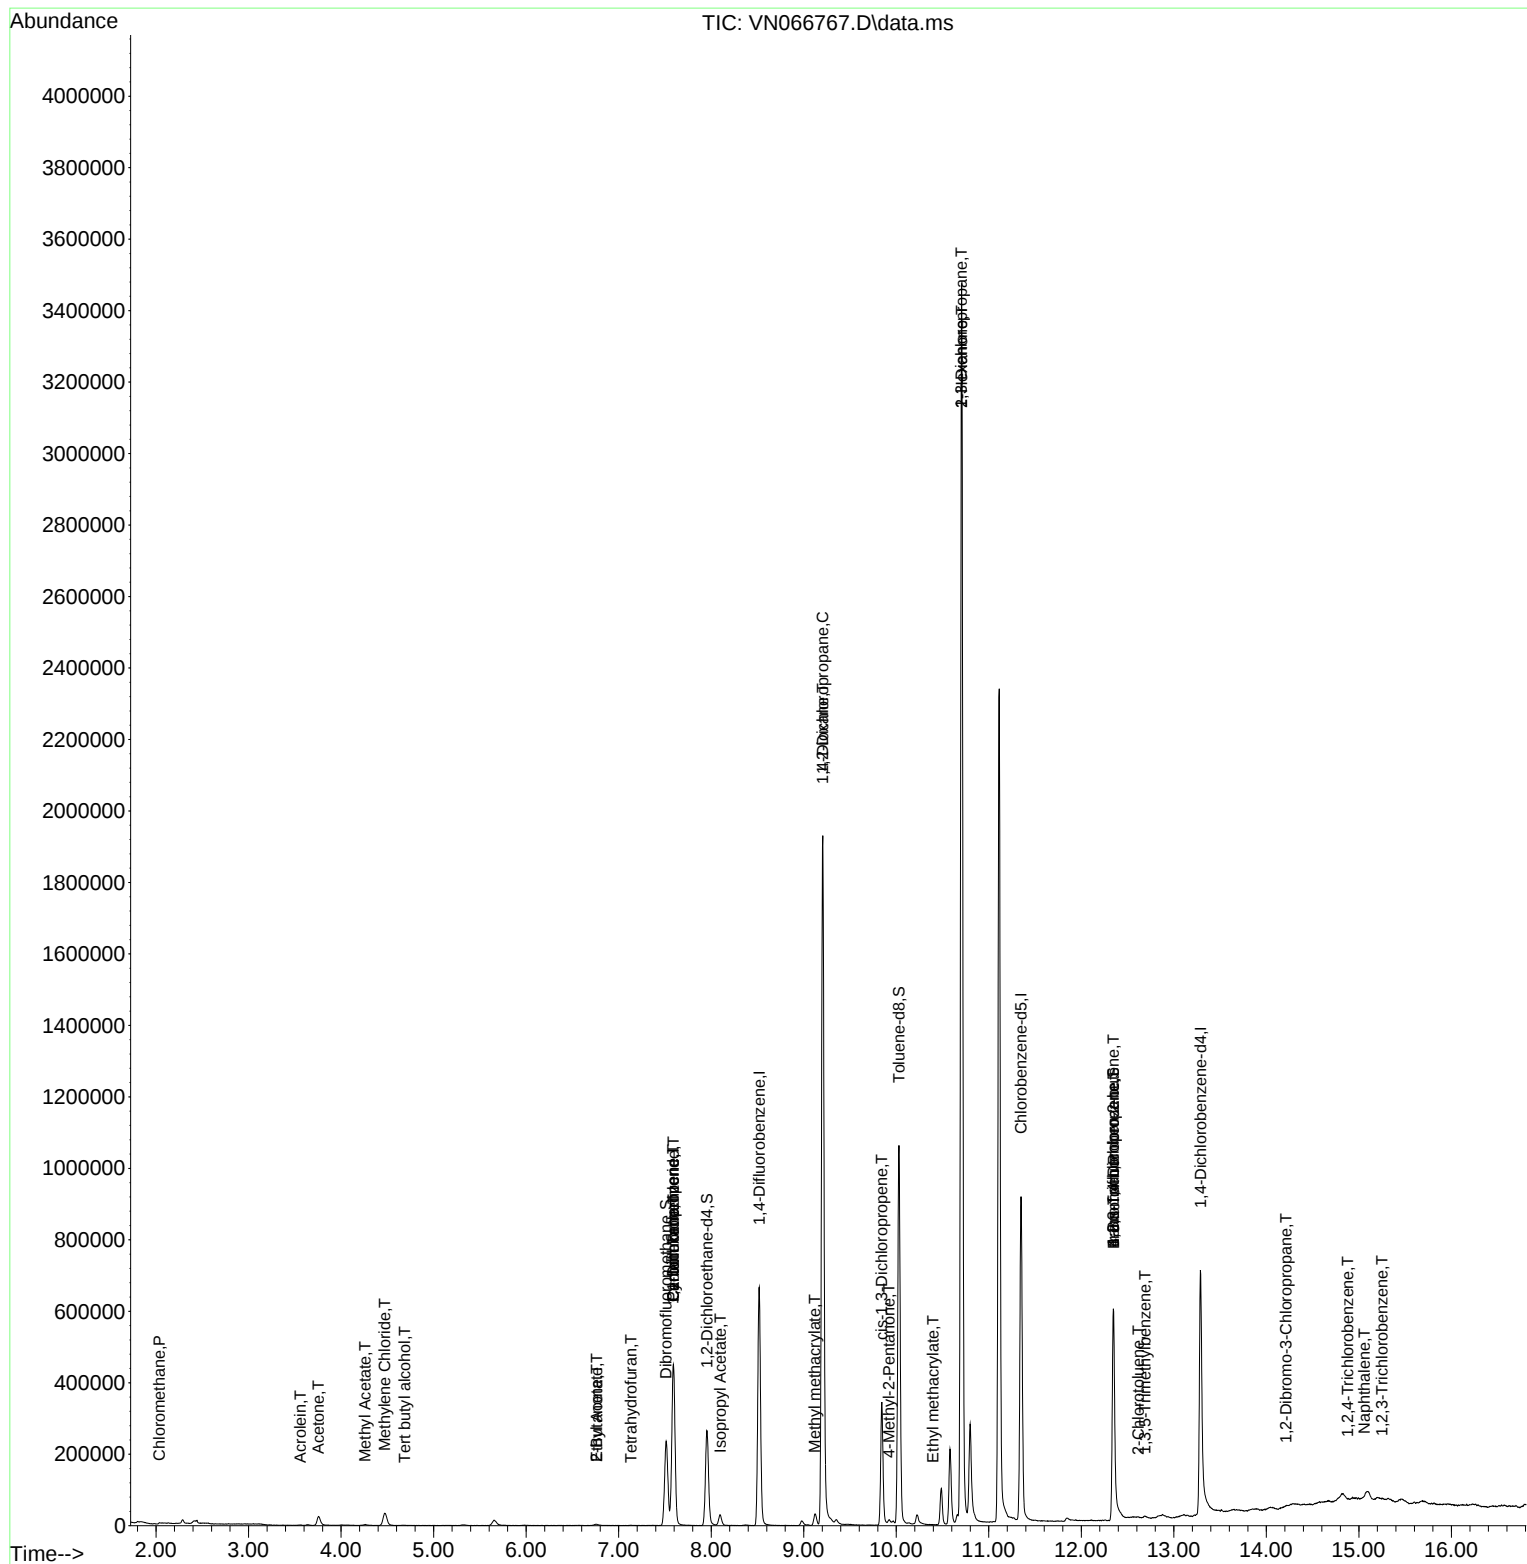




#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 7.591 min Scan# 2188
Delta R.T. -0.000 min
Lab File: VN066767.D
Acq: 26 Apr 2021 17:27




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:168 Resp: 395498
Ion Ratio Lower Upper
168 100
99 52.1 42.6 63.8

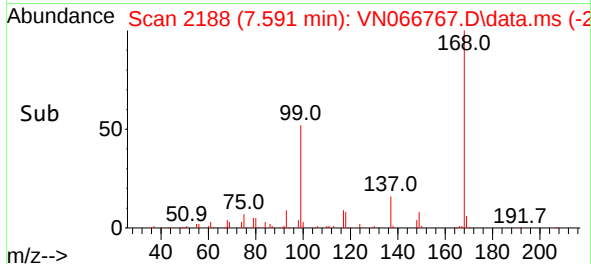

#3
Chloromethane
Concen: 0.24 ug/l
RT: 2.037 min Scan# 117
Delta R.T. 0.003 min
Lab File: VN066767.D
Acq: 26 Apr 2021 17:27


Tgt Ion: 50 Resp: 1556
Ion Ratio Lower Upper
50 100
52 37.8 25.8 38.8

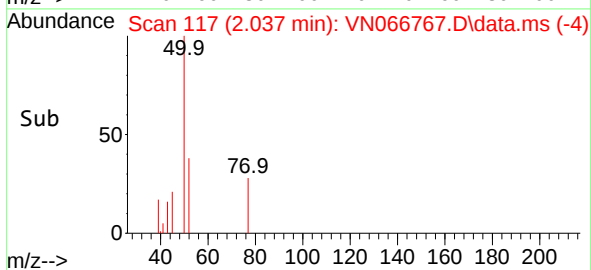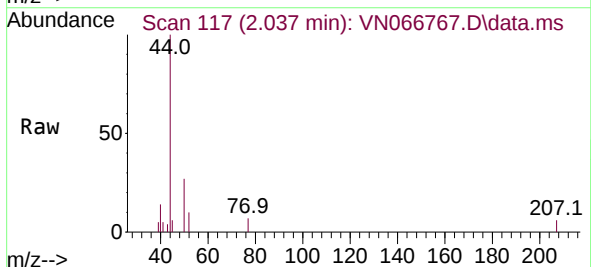






#11
Tert butyl alcohol
Concen: 0.36 ug/l
RT: 4.689 min Scan# 1106
Delta R.T. -0.016 min
Lab File: VN066767.D
Acq: 26 Apr 2021 17:27

Instrument :
MSVOA_N
ClientSampled :







Tgt Ion: 59 Resp: 221
Ion Ratio Lower Upper
59 100
57 0.0 8.0 12.0#

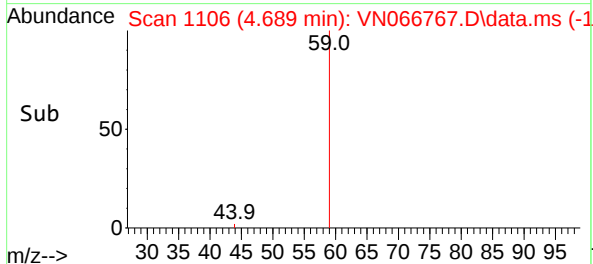

#13
Acrolein
Concen: 1.74 ug/l
RT: 3.560 min Scan# 685
Delta R.T. 0.013 min
Lab File: VN066767.D
Acq: 26 Apr 2021 17:27

Tgt Ion: 56 Resp: 1180
Ion Ratio Lower Upper
56 100
55 29.8 56.0 84.0#


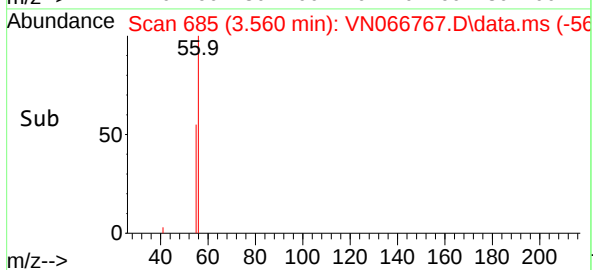
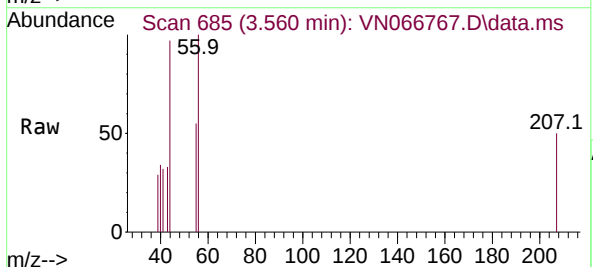



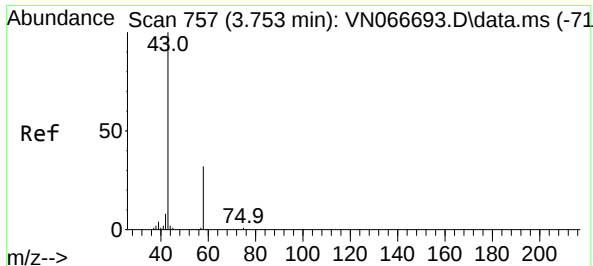

#16
Acetone
Concen: 24.73 ug/l
RT: 3.756 min Scan# 758
Delta R.T. 0.003 min
Lab File: VN066767.D
Acq: 26 Apr 2021 17:27




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 43 Resp: 44730
Ion Ratio Lower Upper
43 100
58 30.1 27.0 40.6

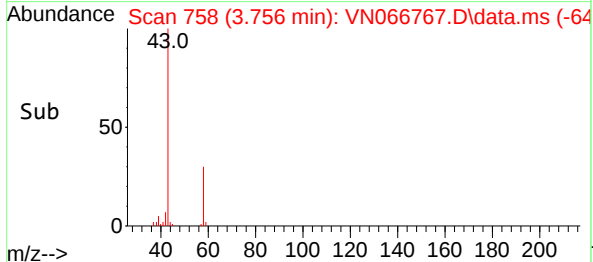

#18
Methyl Acetate
Concen: 0.87 ug/l
RT: 4.260 min Scan# 946
Delta R.T. 0.011 min
Lab File: VN066767.D
Acq: 26 Apr 2021 17:27


Tgt Ion: 43 Resp: 4379
Ion Ratio Lower Upper
43 100
74 19.6 19.5 29.3

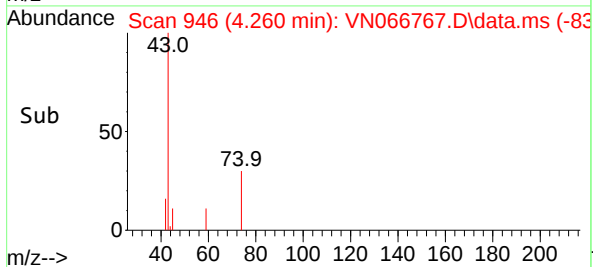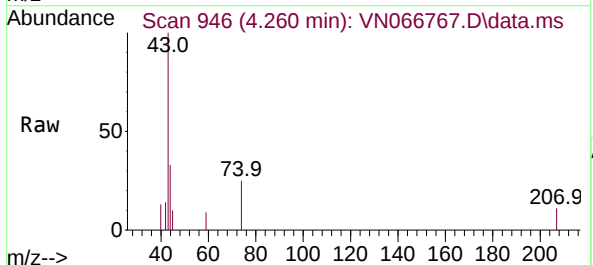



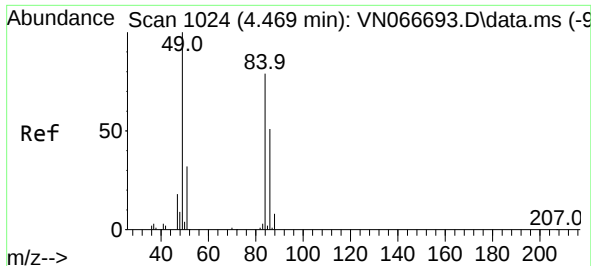


#20
Methylene Chloride
Concen: 4.90 ug/l
RT: 4.469 min Scan# 1024
Delta R.T. 0.000 min
Lab File: VN066767.D
Acq: 26 Apr 2021 17:27


Instrument :
MSVOA_N
ClientSampleId :





Tgt Ion:	84	Resp:	26333
Ion	Ratio	Lower	Upper
84	100		
49	123.8	94.6	141.8
51	35.4	29.9	44.9
86	60.3	51.4	77.2

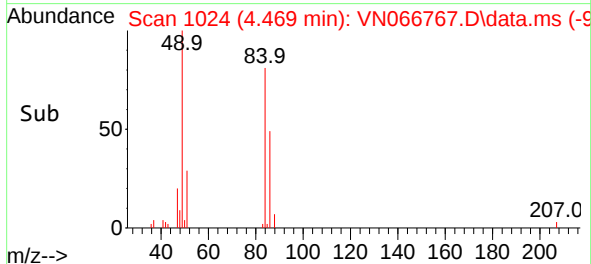


#25
2-Butanone
Concen: 2.14 ug/l
RT: 6.760 min Scan# 1878
Delta R.T. 0.014 min
Lab File: VN066767.D
Acq: 26 Apr 2021 17:27

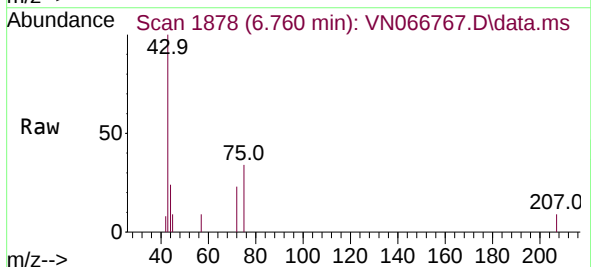

Tgt Ion:	43	Resp:	5559
Ion	Ratio	Lower	Upper
43	100		
72	22.6	23.1	34.7#



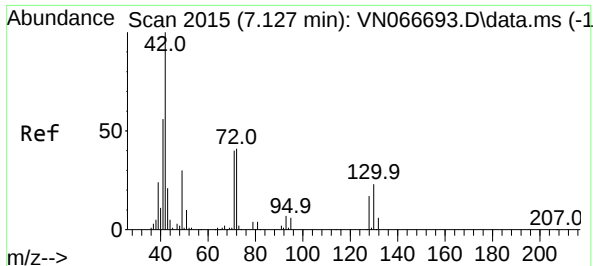

#29

Tetrahydrofuran

Concen: 0.40 ug/l


RT: 7.132 min Scan# 2017

Delta R.T. 0.005 min




Lab File: VN066767.D

Acq: 26 Apr 2021 17:27

Instrument :
MSVOA_N
ClientSampleId :



Tgt Ion:	42	Resp:	713
Ion	Ratio	Lower	Upper
42	100		
72	0.0	36.6	55.0#
71	0.0	34.3	51.5#

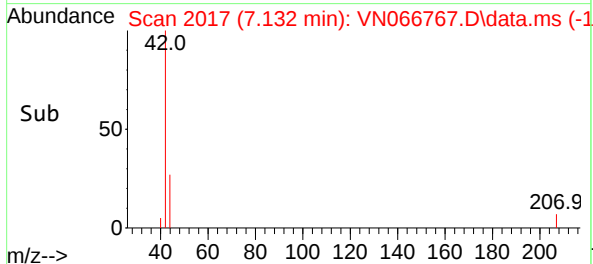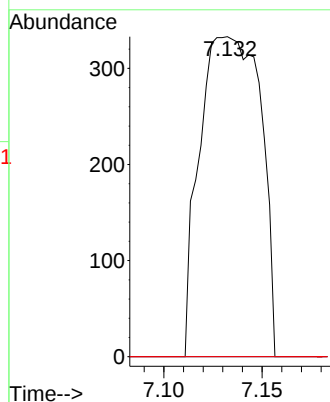

#31

Cyclohexane


Concen: 1.01 ug/l

RT: 7.591 min Scan# 2188



Delta R.T. 0.013 min


Lab File: VN066767.D

Acq: 26 Apr 2021 17:27

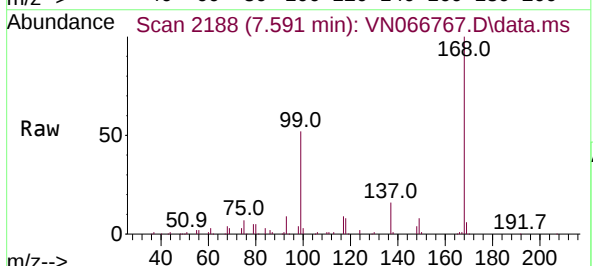

Tgt Ion:	56	Resp:	7969
Ion	Ratio	Lower	Upper
56	100		
69	172.8	26.6	39.8#
84	146.2	70.4	105.6#



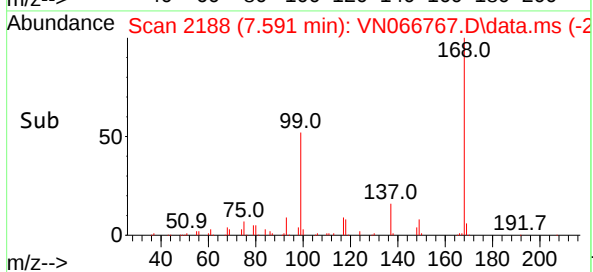
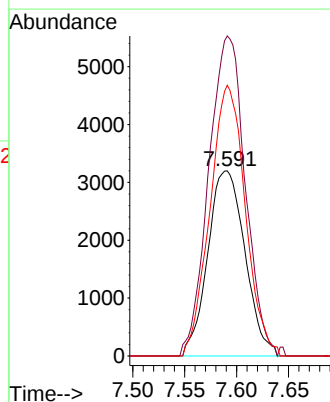


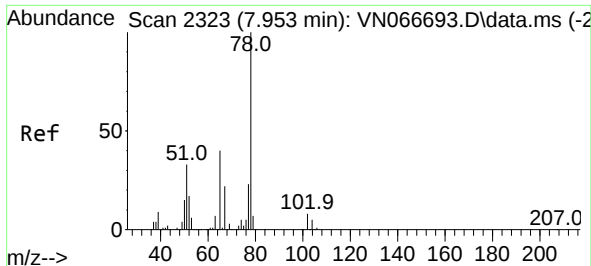

#33
 1,2-Dichloroethane-d4
 Concen: 48.74 ug/l
 RT: 7.953 min Scan# 2323
 Delta R.T. 0.000 min
 Lab File: VN066767.D
 Acq: 26 Apr 2021 17:27




Instrument :
 MSVOA_N
 ClientSampled :


Tgt Ion: 65 Resp: 235488
 Ion Ratio Lower Upper
 65 100
 67 53.4 0.0 107.2

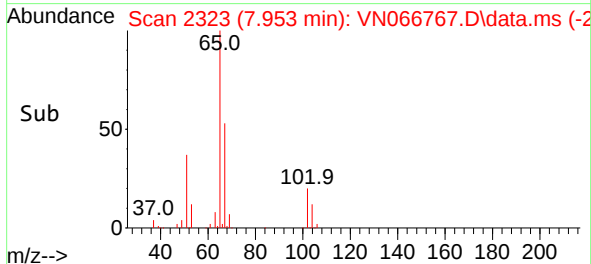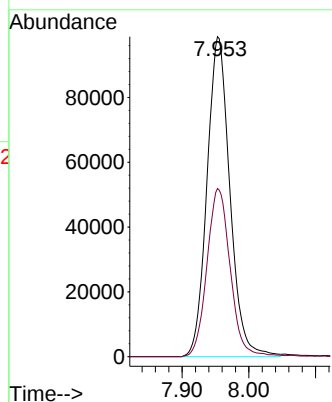

#34
 1,4-Difluorobenzene
 Concen: 50.00 ug/l
 RT: 8.519 min Scan# 2534
 Delta R.T. -0.000 min
 Lab File: VN066767.D
 Acq: 26 Apr 2021 17:27

Tgt Ion:114 Resp: 612814
 Ion Ratio Lower Upper
 114 100
 63 20.7 0.0 38.6
 88 15.7 0.0 30.6


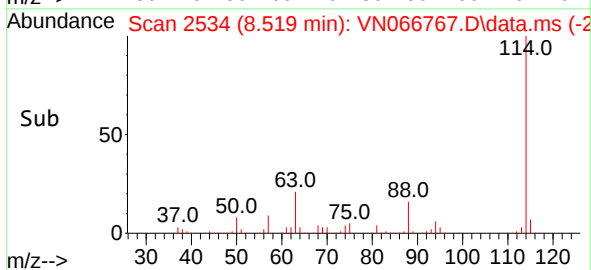
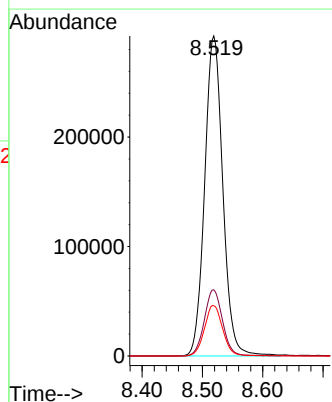
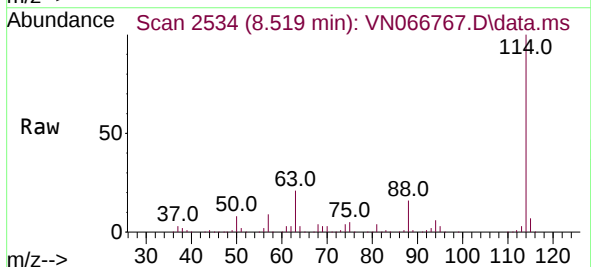


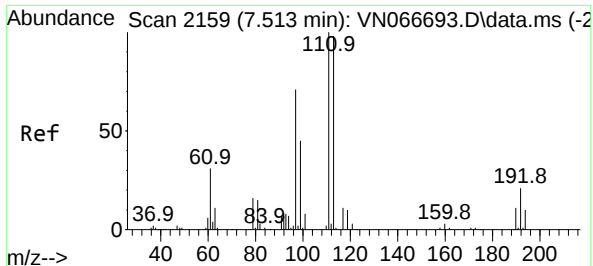

#35
Dibromofluoromethane
Concen: 48.65 ug/l
RT: 7.513 min Scan# 2159
Delta R.T. 0.000 min
Lab File: VN066767.D
Acq: 26 Apr 2021 17:27




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:113 Resp: 186707
Ion Ratio Lower Upper
113 100
111 103.3 82.2 123.2
192 20.7 15.4 23.0

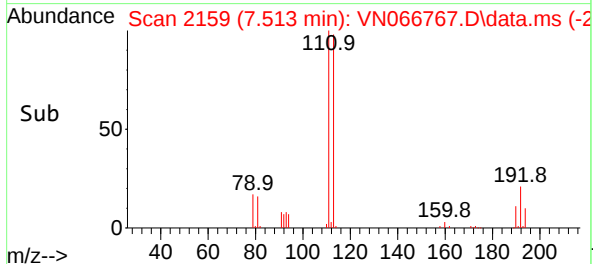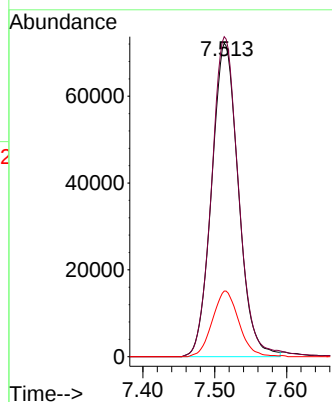

#36
1,1-Dichloropropene
Concen: 5.03 ug/l
RT: 7.588 min Scan# 2187
Delta R.T. -0.129 min
Lab File: VN066767.D
Acq: 26 Apr 2021 17:27

Tgt Ion: 75 Resp: 28632
Ion Ratio Lower Upper
75 100
110 7.7 18.2 54.6#
77 0.0 24.9 37.3#

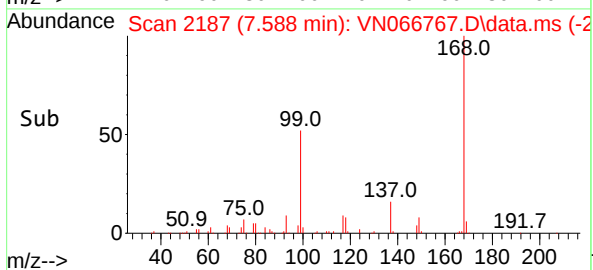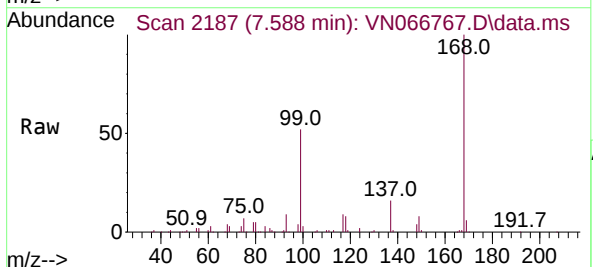

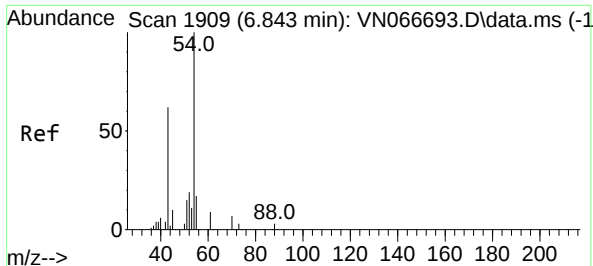

#37

Ethyl Acetate

Concen: 0.93 ug/l

RT: 6.760 min Scan# 1878





Delta R.T. -0.083 min

Lab File: VN066767.D

Acq: 26 Apr 2021 17:27

Tgt Ion:	43	Resp:	5559
Ion	Ratio	Lower	Upper
43	100		
61	0.0	11.6	17.4#
70	0.0	8.6	13.0#

Instrument :
MSVOA_N
ClientSampleId :

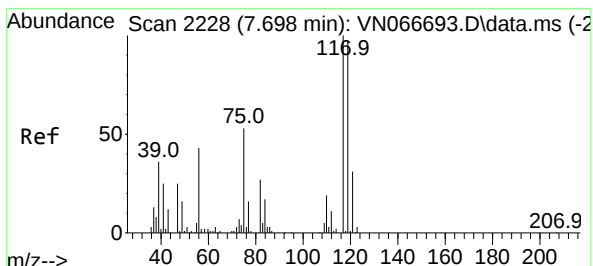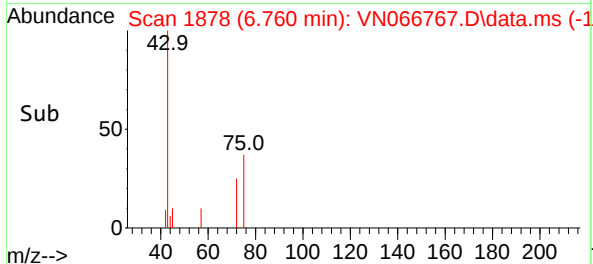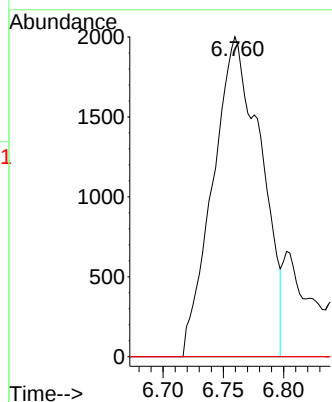

#38

Carbon Tetrachloride

Concen: 6.53 ug/l




RT: 7.591 min Scan# 2188


Delta R.T. -0.107 min

Lab File: VN066767.D

Acq: 26 Apr 2021 17:27

Tgt Ion:	117	Resp:	35438
Ion	Ratio	Lower	Upper
117	100		
119	5.4	76.0	114.0#
121	0.0	24.5	36.7#


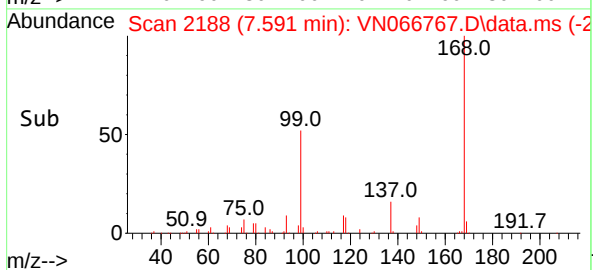

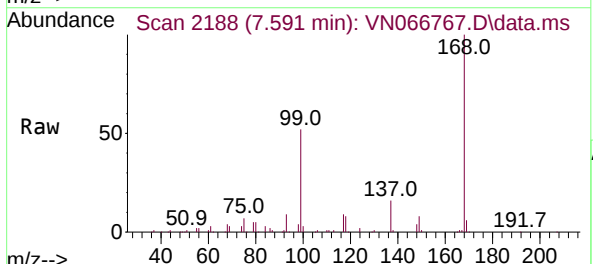


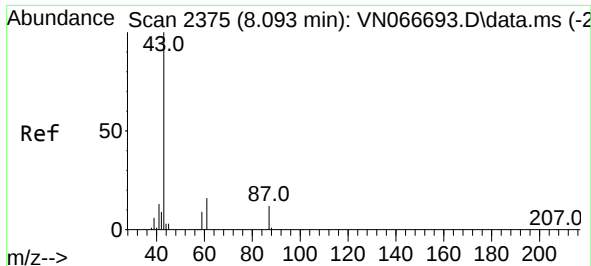

#43
Isopropyl Acetate
Concen: 4.02 ug/l
RT: 8.098 min Scan# 2377
Delta R.T. 0.005 min
Lab File: VN066767.D
Acq: 26 Apr 2021 17:27




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 43 Resp: 38429
Ion Ratio Lower Upper
43 100
61 19.1 22.5 33.7#
87 12.5 11.1 16.7

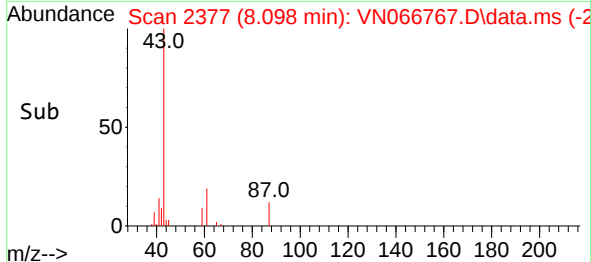

#45
1,2-Dichloropropane
Concen: 0.49 ug/l
RT: 9.205 min Scan# 2790
Delta R.T. 0.152 min
Lab File: VN066767.D
Acq: 26 Apr 2021 17:27


Tgt Ion: 63 Resp: 2442
Ion Ratio Lower Upper
63 100
65 0.0 24.9 37.3#

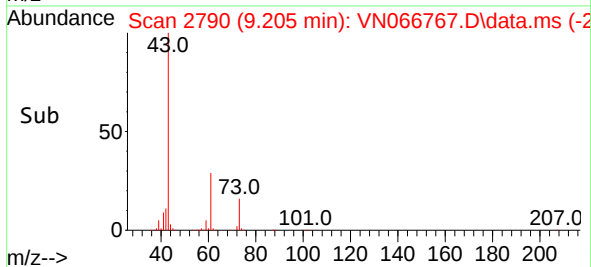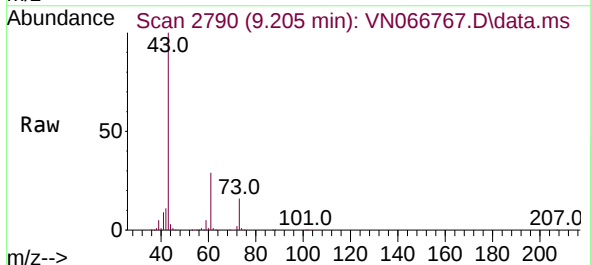



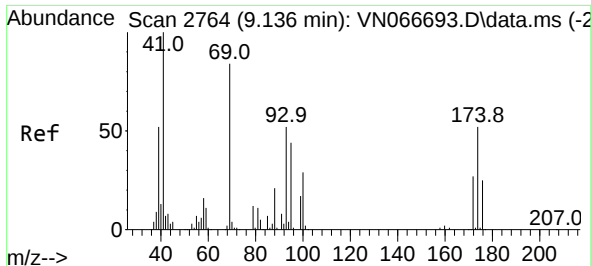


#48
Methyl methacrylate
Concen: 1.73 ug/l
RT: 9.117 min Scan# 2757
Delta R.T. -0.019 min
Lab File: VN066767.D
Acq: 26 Apr 2021 17:27

Instrument :
MSVOA_N
ClientSampleId :



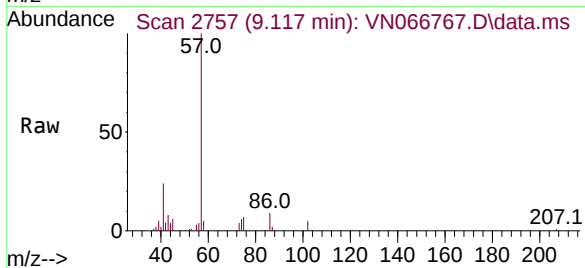



Tgt Ion: 41 Resp: 7251
Ion Ratio Lower Upper
41 100
69 0.0 75.9 113.9#
39 0.0 46.6 69.8#

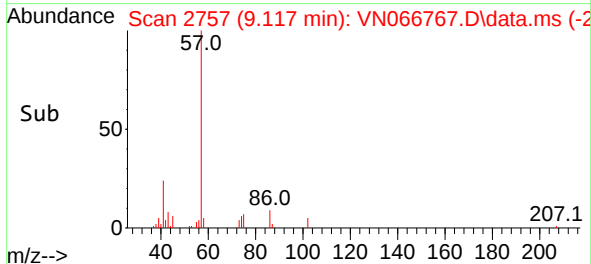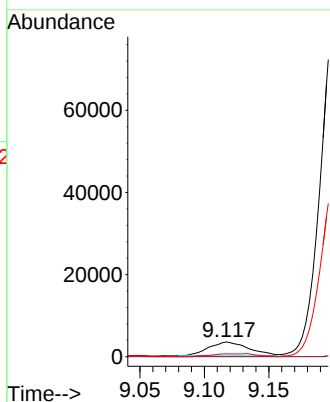

#49
1,4-Dioxane
Concen: 2.15 ug/l
RT: 9.203 min Scan# 2789
Delta R.T. 0.067 min
Lab File: VN066767.D
Acq: 26 Apr 2021 17:27

Tgt Ion: 88 Resp: 109
Ion Ratio Lower Upper
88 100
43 1817174.3 24.7 37.1#
58 6833.0 52.6 78.8#


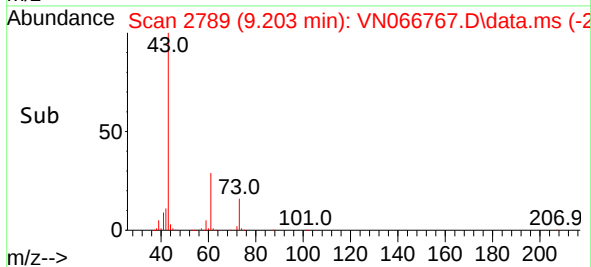

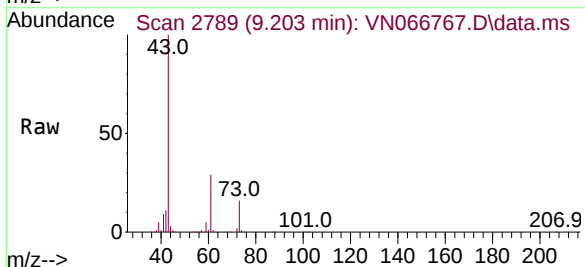


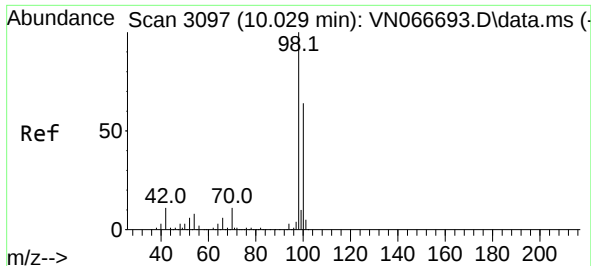

#50
Toluene-d8
Concen: 50.31 ug/l
RT: 10.029 min Scan# 3097
Delta R.T. -0.000 min
Lab File: VN066767.D
Acq: 26 Apr 2021 17:27




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 98 Resp: 752928
Ion Ratio Lower Upper
98 100
100 64.1 50.5 75.7

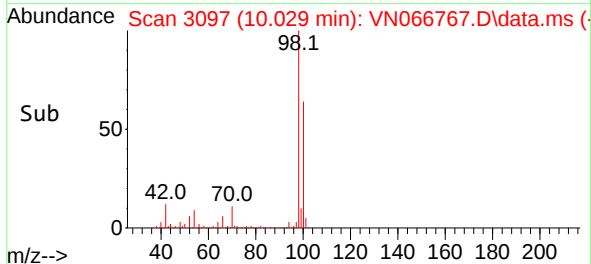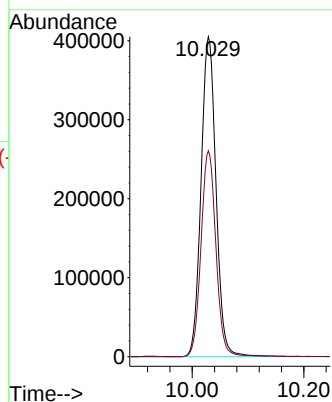

#51
4-Methyl-2-Pentanone
Concen: 1.89 ug/l
RT: 9.922 min Scan# 3057
Delta R.T. -0.000 min
Lab File: VN066767.D
Acq: 26 Apr 2021 17:27


Tgt Ion: 43 Resp: 10130
Ion Ratio Lower Upper
43 100
58 35.4 32.5 48.7

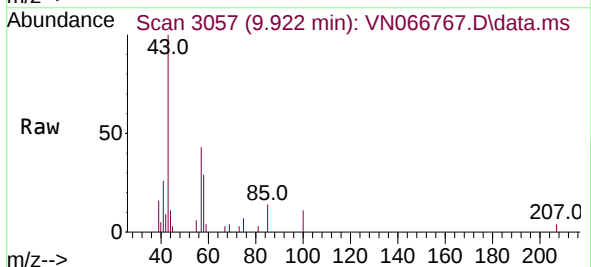



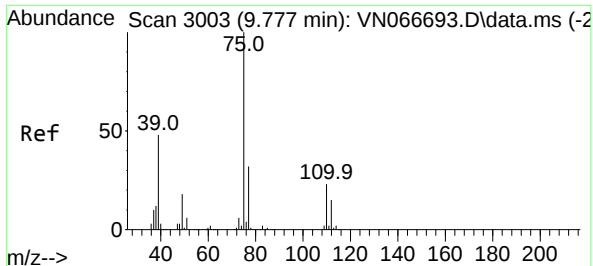


#54
cis-1,3-Dichloropropene
Concen: 8.86 ug/l
RT: 9.844 min Scan# 3028
Delta R.T. 0.067 min
Lab File: VN066767.D
Acq: 26 Apr 2021 17:27

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion: 75 Resp: 65209
Ion Ratio Lower Upper
75 100
77 0.6 24.9 37.3#
39 26.8 36.2 54.4#

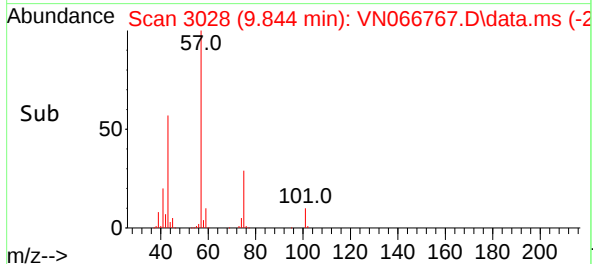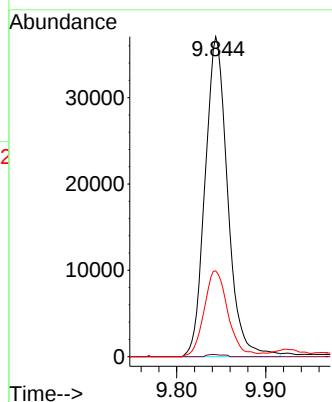

#56
Ethyl methacrylate
Concen: 3.21 ug/l
RT: 10.396 min Scan# 3234
Delta R.T. 0.026 min
Lab File: VN066767.D
Acq: 26 Apr 2021 17:27

Tgt Ion: 69 Resp: 415
Ion Ratio Lower Upper
69 100
41 0.0 49.6 74.4#
39 0.0 28.0 42.0#


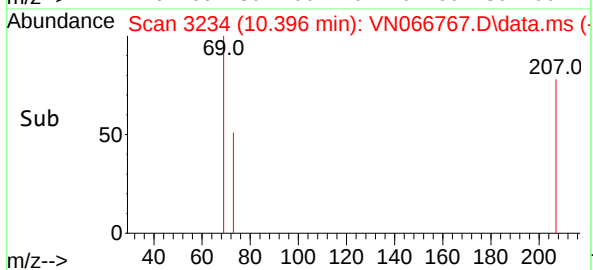

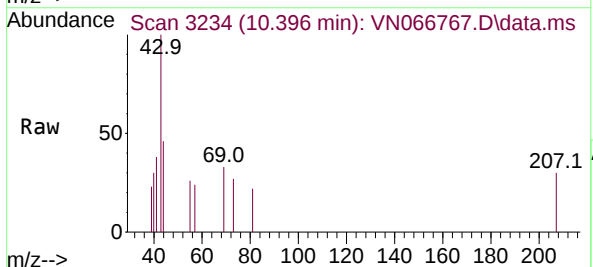


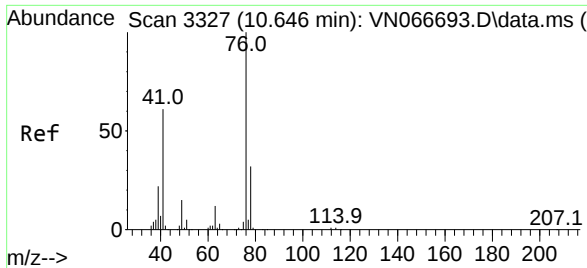

#57
1,3-Dichloropropane
Concen: 5.16 ug/l
RT: 10.705 min Scan# 3349
Delta R.T. 0.059 min
Lab File: VN066767.D
Acq: 26 Apr 2021 17:27




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 76 Resp: 37011
Ion Ratio Lower Upper
76 100
78 0.1 25.7 38.5#

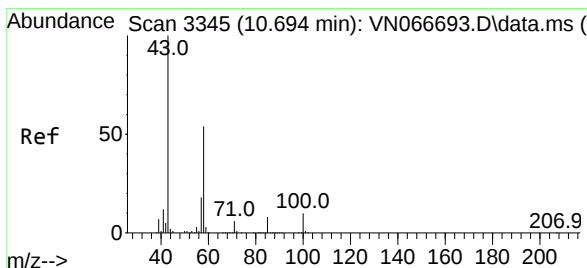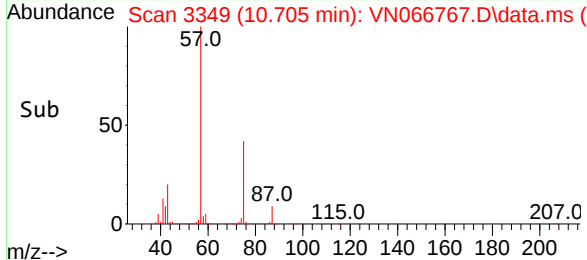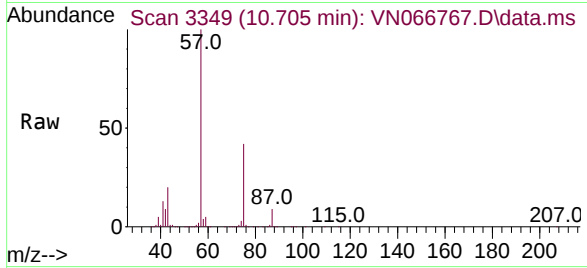

#59
2-Hexanone
Concen: 138.14 ug/l
RT: 10.707 min Scan# 3350
Delta R.T. 0.013 min
Lab File: VN066767.D
Acq: 26 Apr 2021 17:27

Tgt Ion: 43 Resp: 522265
Ion Ratio Lower Upper
43 100
58 18.6 28.1 84.3#


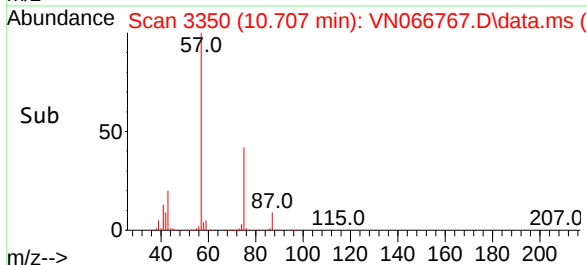
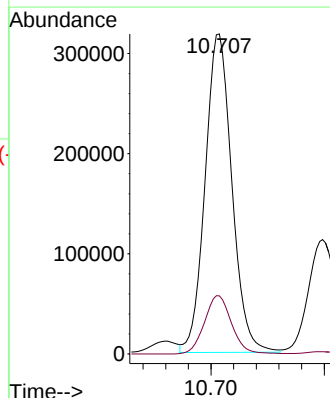
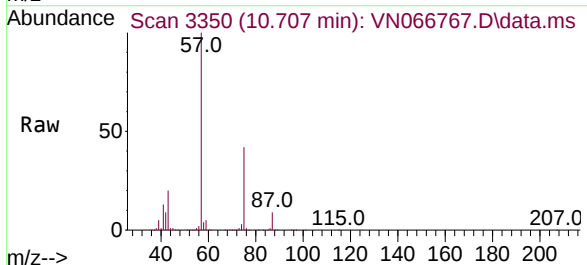


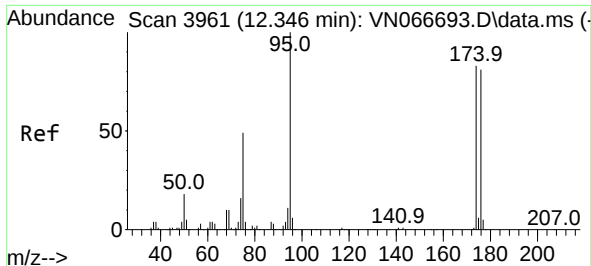

#62
4-Bromofluorobenzene
Concen: 48.69 ug/l
RT: 12.346 min Scan# 3961
Delta R.T. 0.000 min
Lab File: VN066767.D
Acq: 26 Apr 2021 17:27




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 95 Resp: 249561
Ion Ratio Lower Upper
95 100
174 82.3 0.0 169.0
176 79.3 0.0 162.4

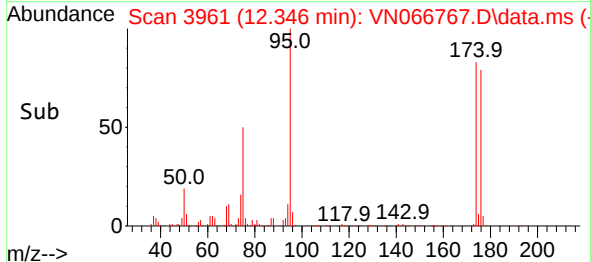

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.348 min Scan# 3589
Delta R.T. -0.001 min
Lab File: VN066767.D
Acq: 26 Apr 2021 17:27

Tgt Ion: 117 Resp: 553952
Ion Ratio Lower Upper
117 100
82 55.6 43.7 65.5
119 31.8 26.1 39.1


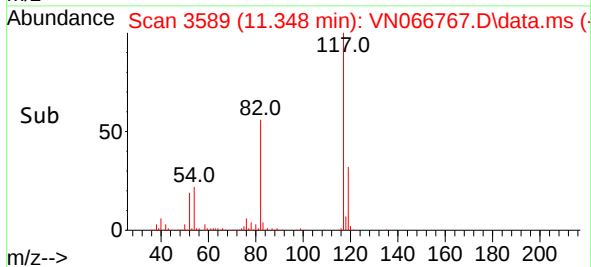

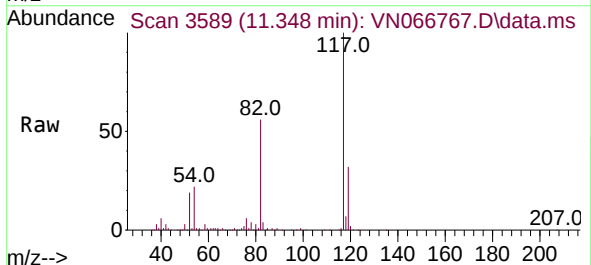


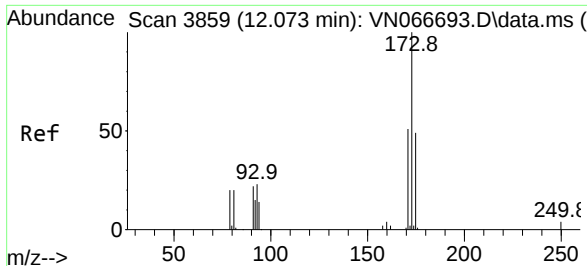

#71
Bromoform
Concen: 0.49 ug/l
RT: 12.349 min Scan# 3962
Delta R.T. 0.276 min
Lab File: VN066767.D
Acq: 26 Apr 2021 17:27




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:173 Resp: 1512
Ion Ratio Lower Upper
173 100
175 801.8 23.8 71.2#
254 0.0 0.0 0.0

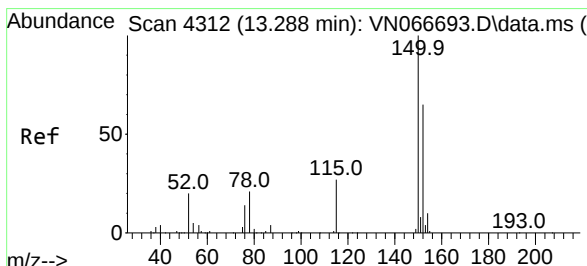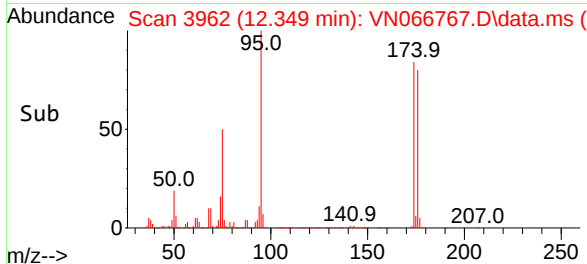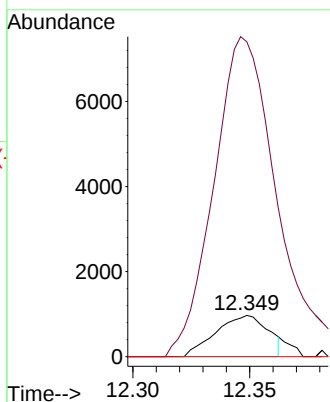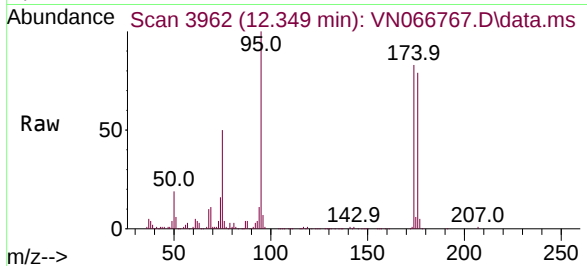

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.287 min Scan# 4312
Delta R.T. -0.001 min
Lab File: VN066767.D
Acq: 26 Apr 2021 17:27


Tgt Ion:152 Resp: 244218
Ion Ratio Lower Upper
152 100
115 58.0 28.5 85.6
150 157.8 0.0 347.6

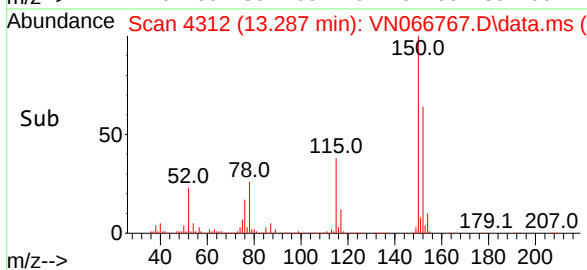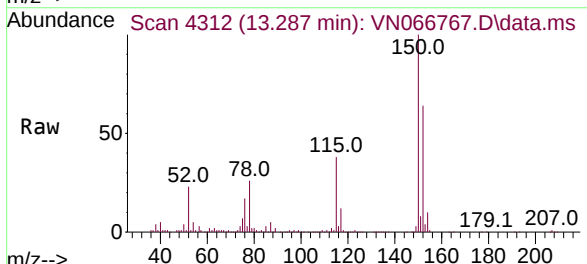



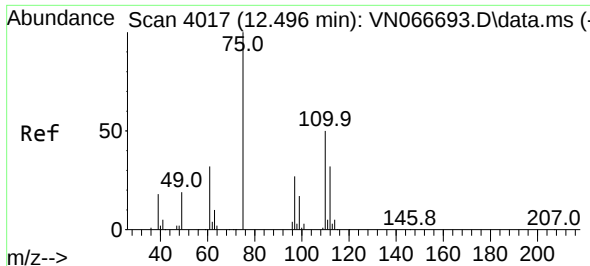


#76
1,2,3-Trichloropropane
Concen: 23.85 ug/l
RT: 12.346 min Scan# 3961
Delta R.T. -0.150 min
Lab File: VN066767.D
Acq: 26 Apr 2021 17:27

Instrument :
MSVOA_N
ClientSampled :



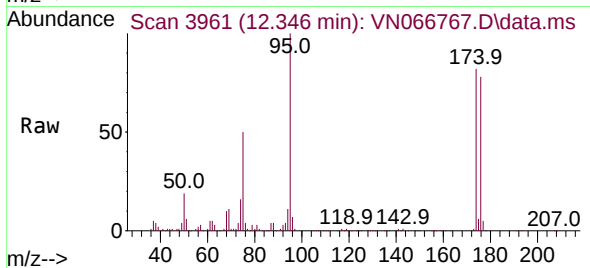



Tgt Ion: 75 Resp: 124631
Ion Ratio Lower Upper
75 100
77 1.4 0.0 0.0#

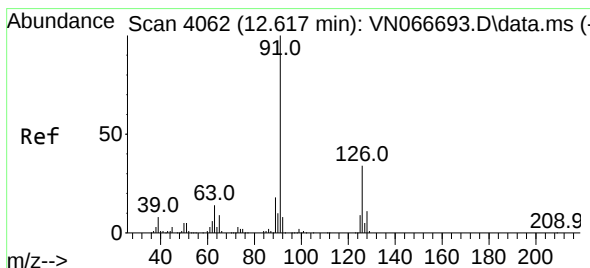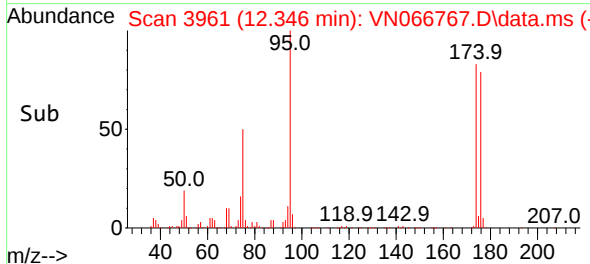

#79
2-Chlorotoluene
Concen: 0.94 ug/l
RT: 12.614 min Scan# 4061
Delta R.T. -0.003 min
Lab File: VN066767.D
Acq: 26 Apr 2021 17:27

Tgt Ion: 91 Resp: 51
Ion Ratio Lower Upper
91 100
126 0.0 17.4 52.3#


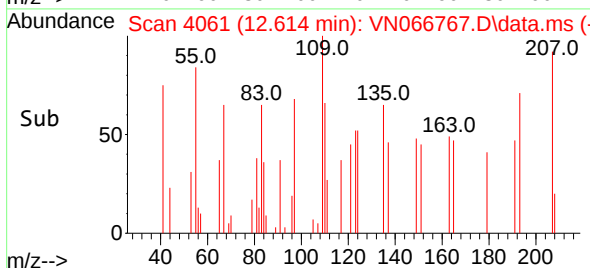

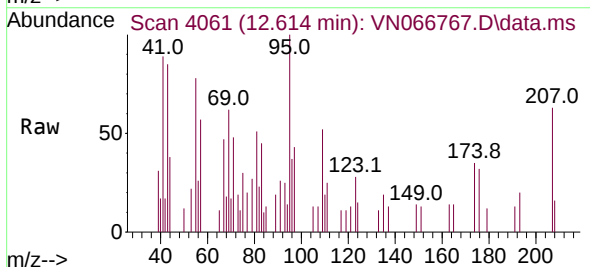


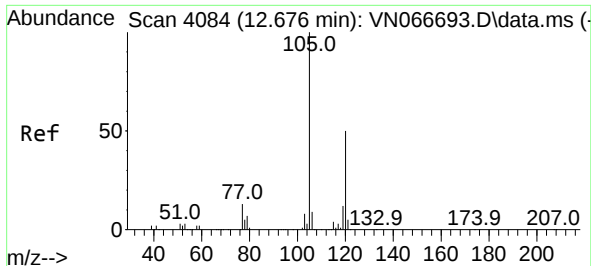

#80
1,3,5-Trimethylbenzene
Concen: 0.25 ug/l
RT: 12.687 min Scan# 4088
Delta R.T. 0.011 min
Lab File: VN066767.D
Acq: 26 Apr 2021 17:27




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:105 Resp: 3751
Ion Ratio Lower Upper
105 100
120 51.7 24.3 72.8

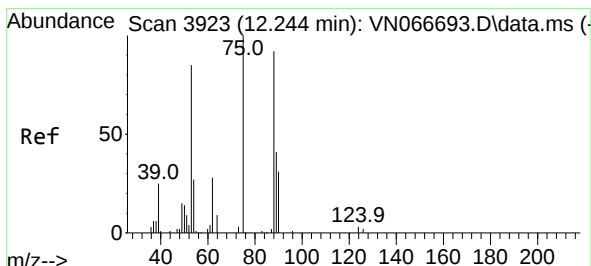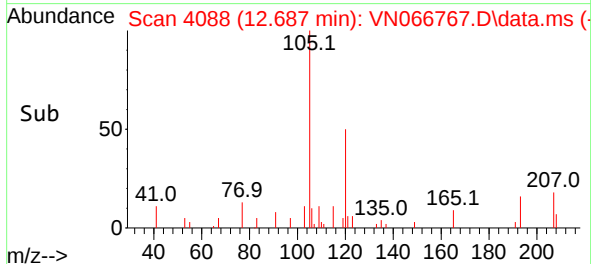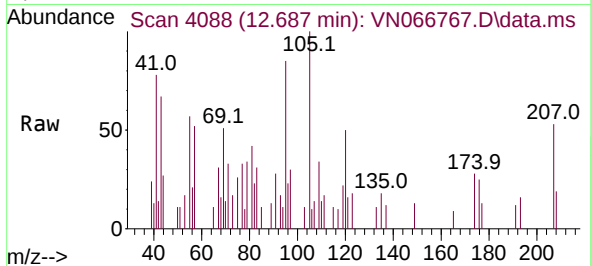

#81
trans-1,4-Dichloro-2-butene
Concen: 70.50 ug/l
RT: 12.346 min Scan# 3961
Delta R.T. 0.102 min
Lab File: VN066767.D
Acq: 26 Apr 2021 17:27

Tgt Ion: 75 Resp: 124631
Ion Ratio Lower Upper
75 100
53 0.0 74.6 111.8#
89 0.0 35.8 53.8#



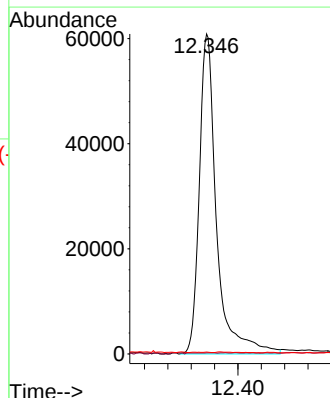
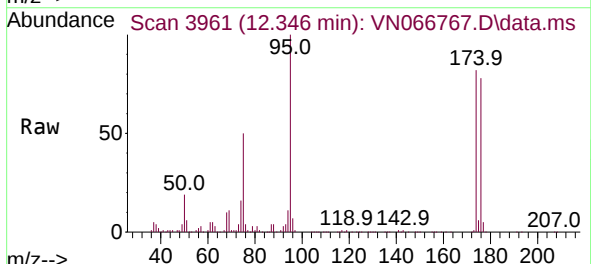


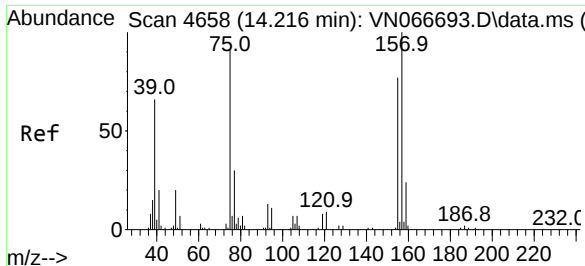

#92
 1,2-Dibromo-3-Chloropropane
 Concen: 0.23 ug/l
 RT: 14.213 min Scan# 4657
 Delta R.T. -0.003 min
 Lab File: VN066767.D
 Acq: 26 Apr 2021 17:27




Instrument :
 MSVOA_N
 ClientSampleId :


Tgt Ion: 75 Resp: 238
 Ion Ratio Lower Upper
 75 100
 155 0.0 44.1 132.4#
 157 47.5 56.0 168.2#

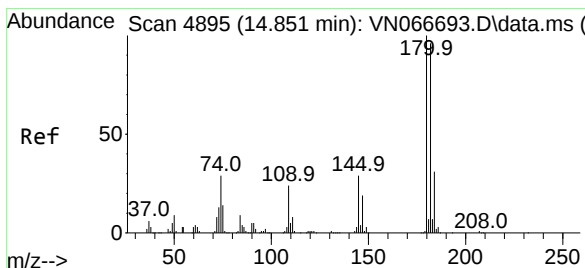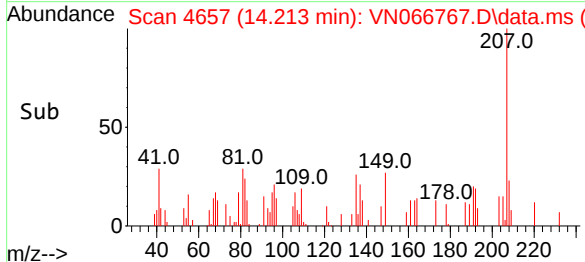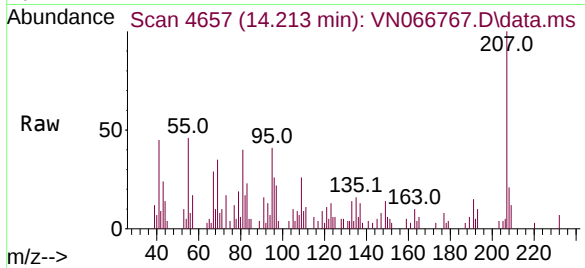

#93
 1,2,4-Trichlorobenzene
 Concen: 2.06 ug/l
 RT: 14.878 min Scan# 4905
 Delta R.T. 0.027 min
 Lab File: VN066767.D
 Acq: 26 Apr 2021 17:27

Tgt Ion: 180 Resp: 283
 Ion Ratio Lower Upper
 180 100
 182 53.7 47.3 142.0
 145 0.0 15.6 46.8#


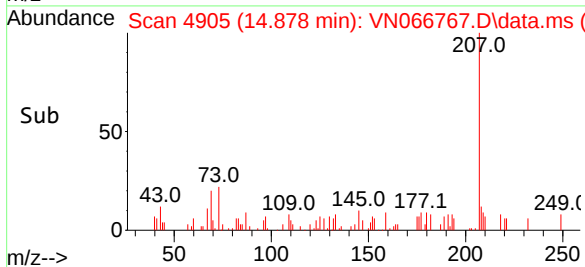

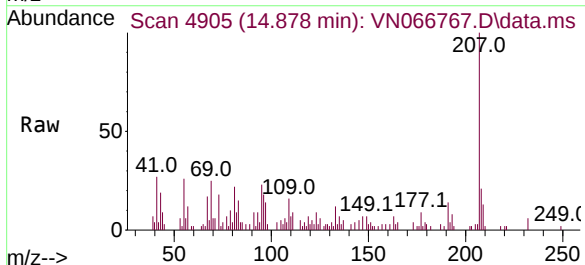


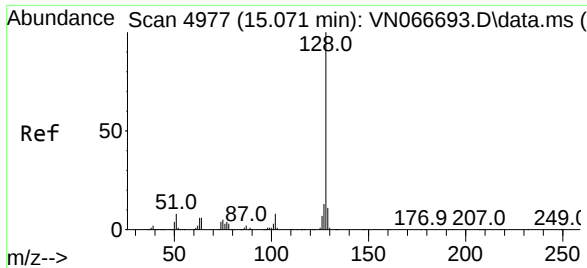

#95
Naphthalene
Concen: 1.88 ug/l
RT: 15.060 min Scan# 4973
Delta R.T. -0.011 min
Lab File: VN066767.D
Acq: 26 Apr 2021 17:27

Instrument :
MSVOA_N
ClientSampleId :

Tgt Ion:128 Resp: 360
Ion Ratio Lower Upper
128 100
127 28.9 10.2 15.2#
129 42.5 8.6 13.0#

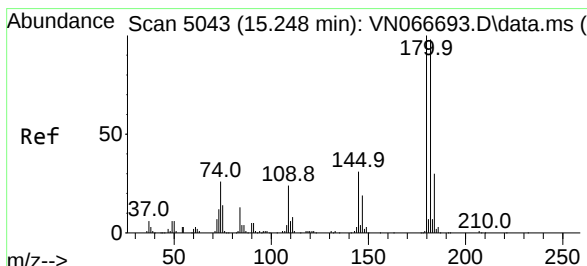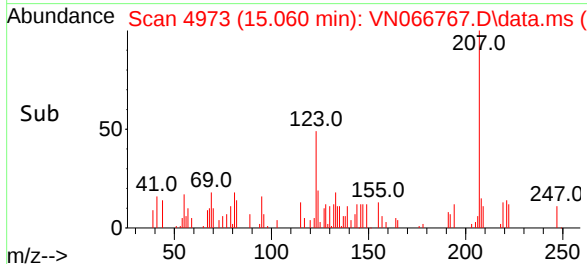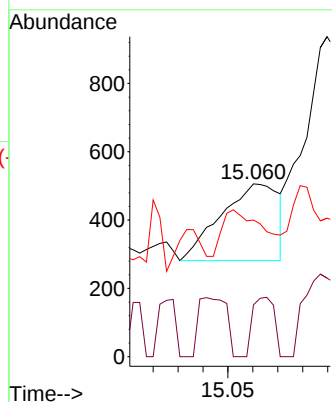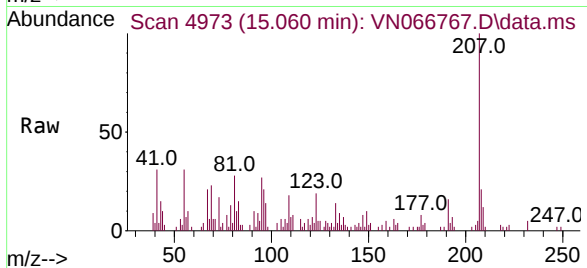

#96
1,2,3-Trichlorobenzene
Concen: 1.38 ug/l
RT: 15.248 min Scan# 5043
Delta R.T. -0.000 min
Lab File: VN066767.D
Acq: 26 Apr 2021 17:27

Tgt Ion:180 Resp: 117
Ion Ratio Lower Upper
180 100
182 0.0 47.4 142.3#
145 94.0 16.5 49.5#

