


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN042621\
Data File : VN066753.D
Acq On : 26 Apr 2021 9:44
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N042121W.M
Title : SW846 8260
Last Update : Tue Apr 27 12:28:10 2021

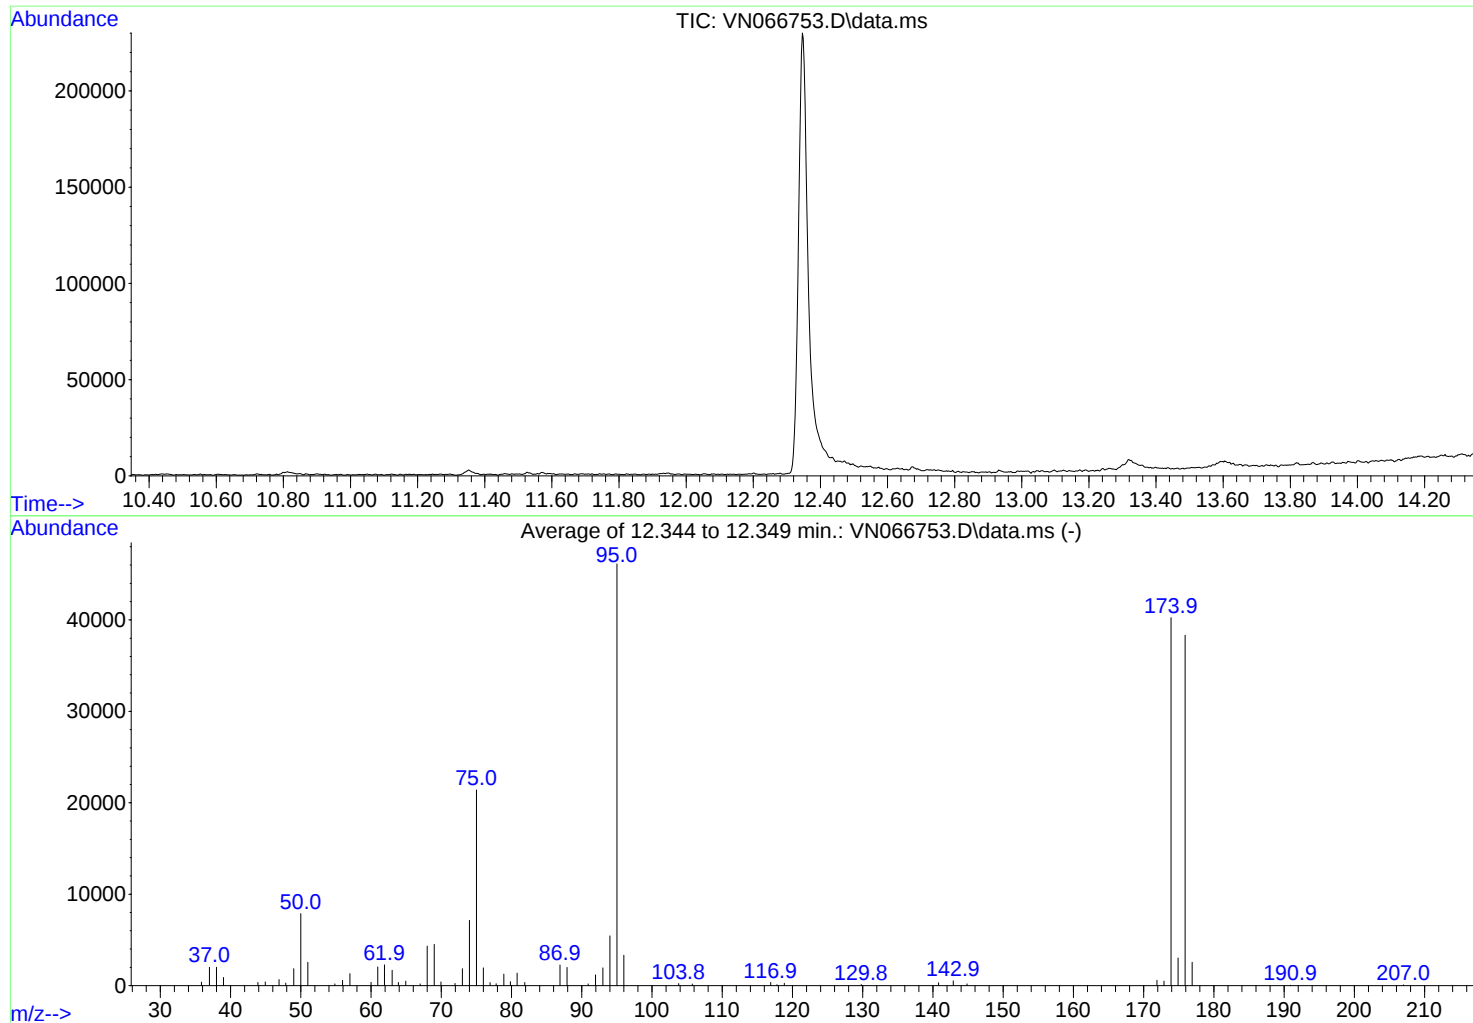

AutoFind: Scans 3960, 3961, 3962; Background Corrected with Scan 3944

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.1	7876	PASS
75	95	30	60	46.4	21411	PASS
95	95	100	100	100.0	46131	PASS
96	95	5	9	7.2	3325	PASS
173	174	0.00	2	1.2	483	PASS
174	95	50	100	87.2	40243	PASS
175	174	5	9	7.5	3033	PASS
176	174	95	101	95.2	38328	PASS
177	176	5	9	6.7	2554	PASS