

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN042624\
 Data File : VN081882.D
 Acq On : 26 Apr 2024 16:56
 Operator : JC\MD
 Sample : P2282-04
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 STORAGE-BLANK-SAMPLE-MANAG

Quant Time: Apr 26 23:03:00 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N042524W.M
 Quant Title : SW846 8260
 QLast Update : Fri Apr 26 05:26:49 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.224	168	234145	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	433725	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	391107	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	153778	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.582	65	173707	43.957	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	87.920%
35) Dibromofluoromethane	8.171	113	127112	48.676	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	97.360%
50) Toluene-d8	10.570	98	531372	51.810	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	103.620%
62) 4-Bromofluorobenzene	12.853	95	190586	47.009	ug/l	0.00
Spiked Amount	50.000	Range	64 - 133	Recovery	=	94.020%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN042624\
Data File : VN081882.D
Acq On : 26 Apr 2024 16:56
Operator : JC\MD
Sample : P2282-04
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
STORAGE-BLANK-SAMPLE-MANAG

Quant Time: Apr 26 23:03:00 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N042524W.M
Quant Title : SW846 8260
QLast Update : Fri Apr 26 05:26:49 2024
Response via : Initial Calibration




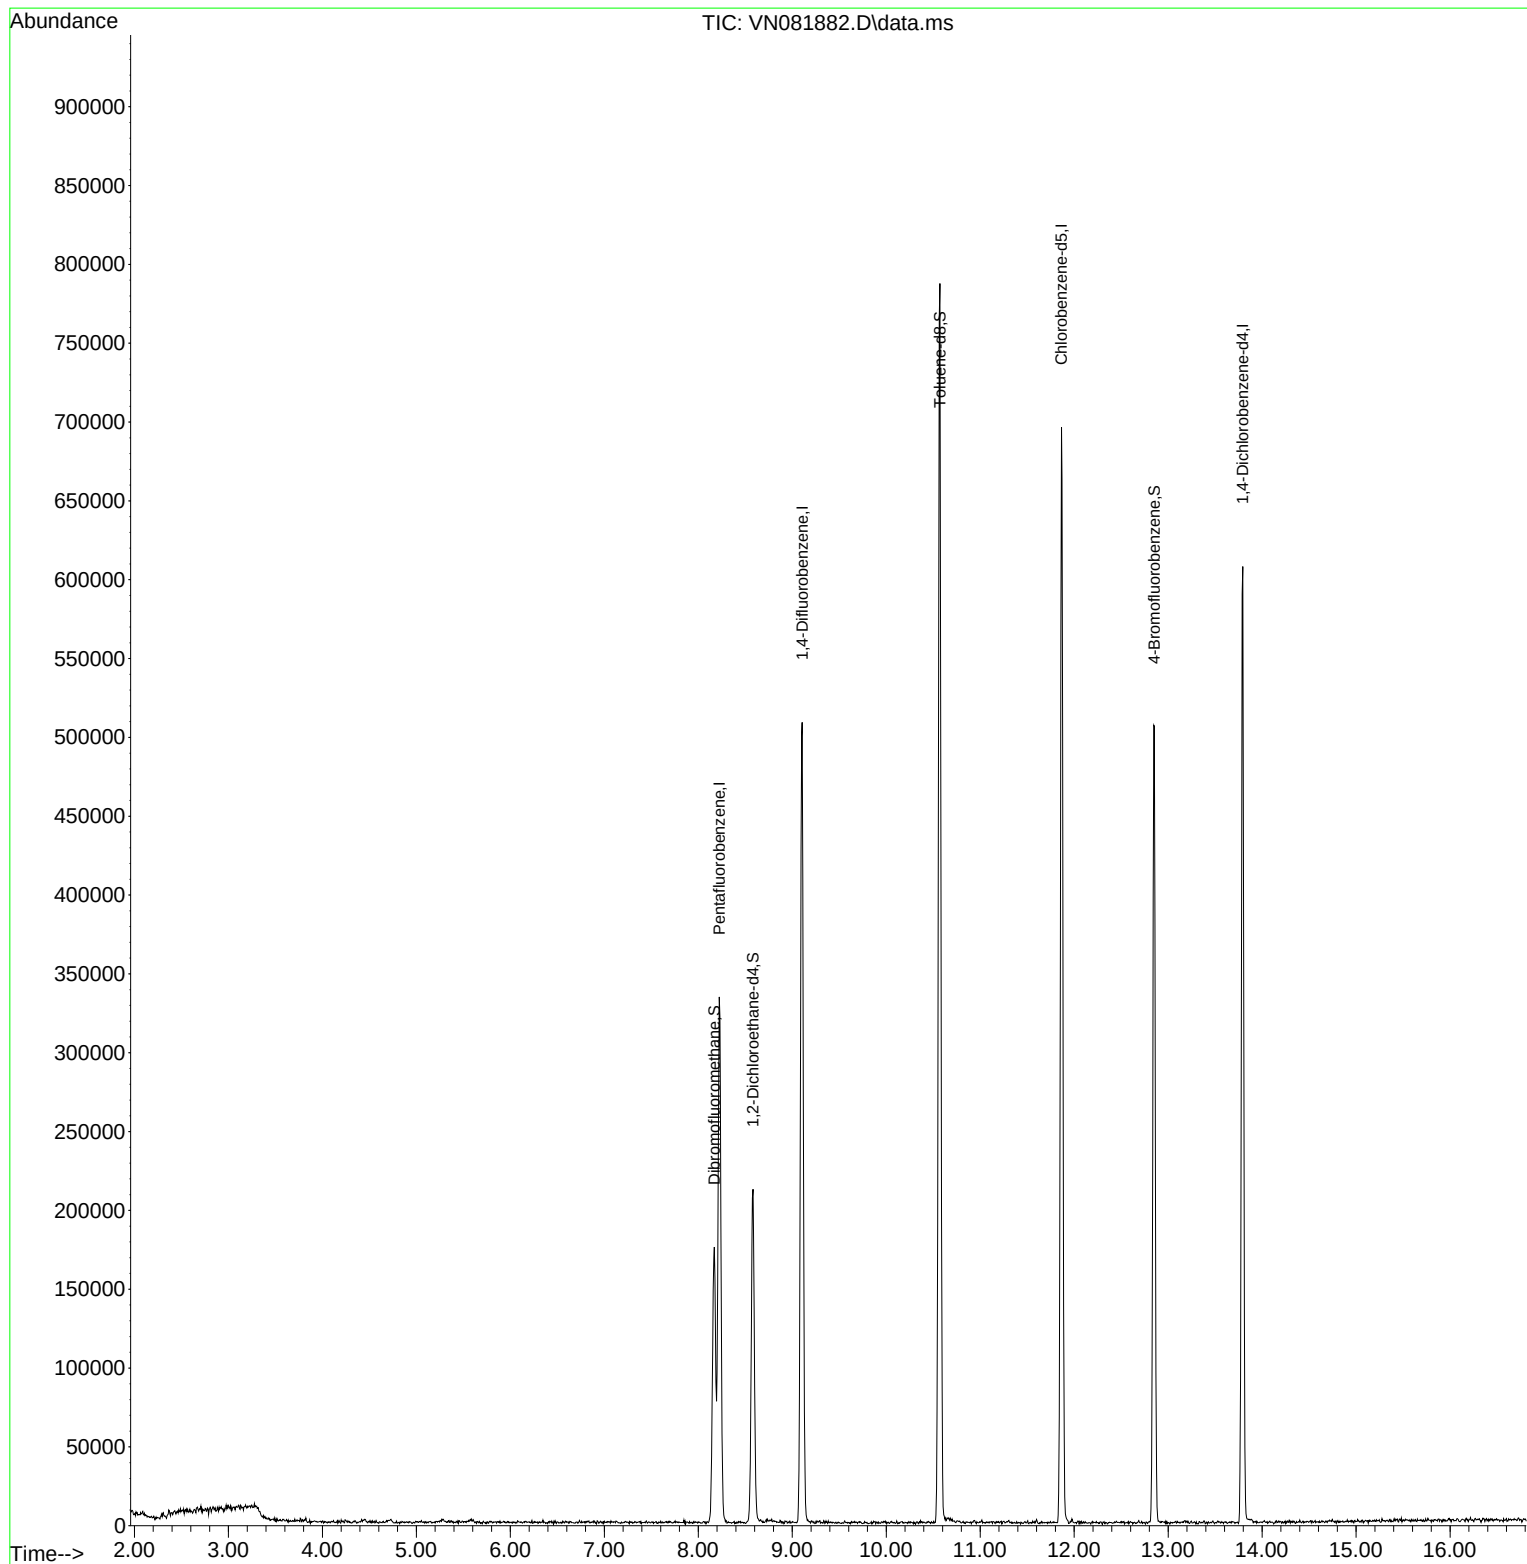


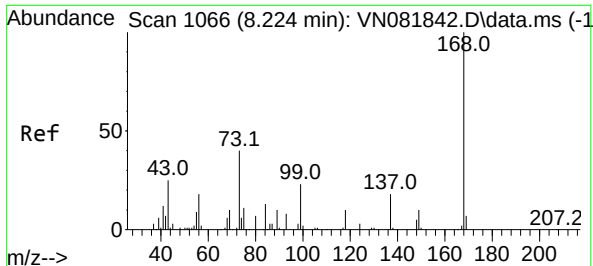

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.224 min Scan# 1066
Delta R.T. -0.000 min
Lab File: VN081882.D
Acq: 26 Apr 2024 16:56




Instrument :
MSVOA_N
ClientSampleId :
STORAGE-BLANK-SAMPLE-MANAG


Tgt Ion:168 Resp: 234145
Ion Ratio Lower Upper
168 100
99 67.5 48.2 72.4

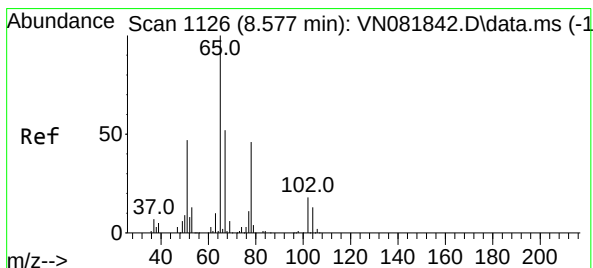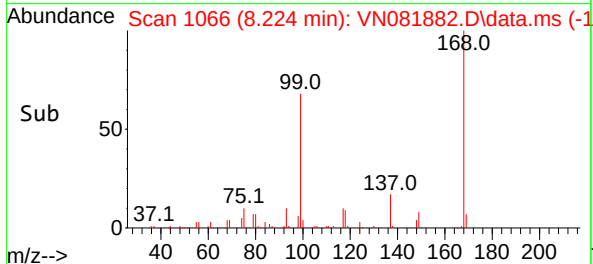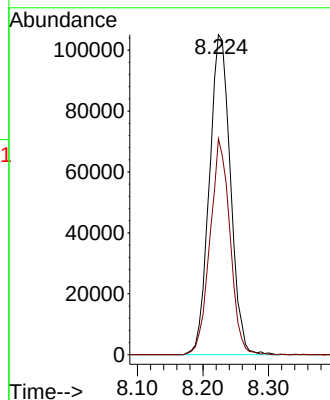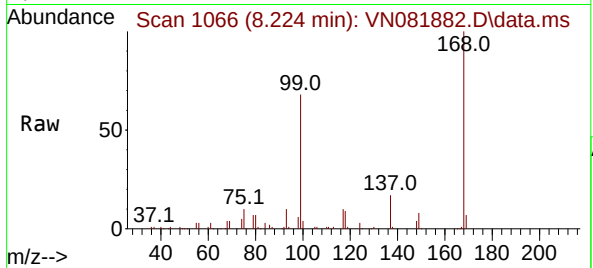

#33
1,2-Dichloroethane-d4
Concen: 43.957 ug/l
RT: 8.582 min Scan# 1127
Delta R.T. 0.006 min
Lab File: VN081882.D
Acq: 26 Apr 2024 16:56

Tgt Ion: 65 Resp: 173707
Ion Ratio Lower Upper
65 100
67 51.5 0.0 103.0

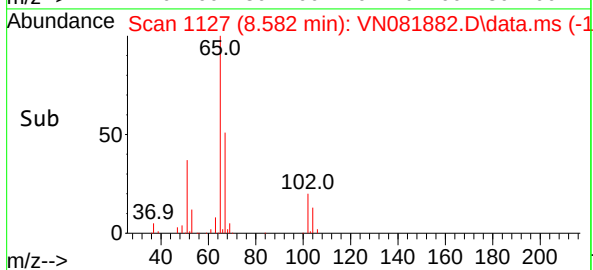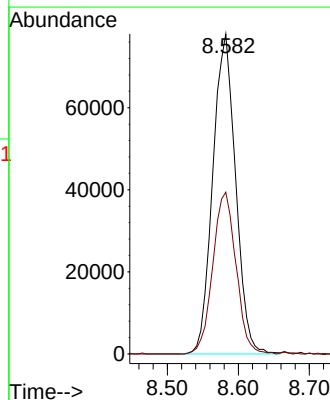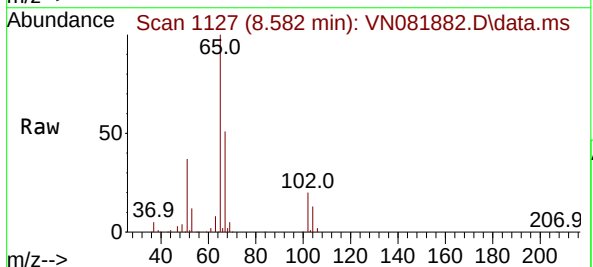

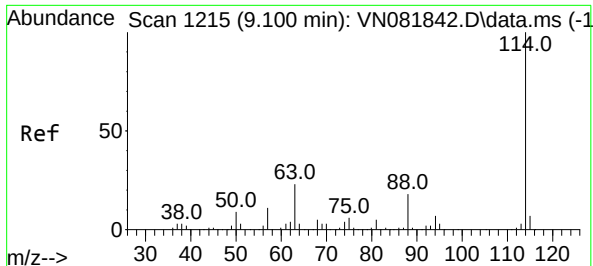

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.106 min Scan# 11

Delta R.T. 0.006 min

Lab File: VN081882.D

Acq: 26 Apr 2024 16:56

Instrument :

MSVOA_N

ClientSampleId :

STORAGE-BLANK-SAMPLE-MANAG





Tgt Ion:114 Resp: 433725

Ion Ratio Lower Upper

114 100

63 22.3 0.0 41.0

88 17.2 0.0 31.4

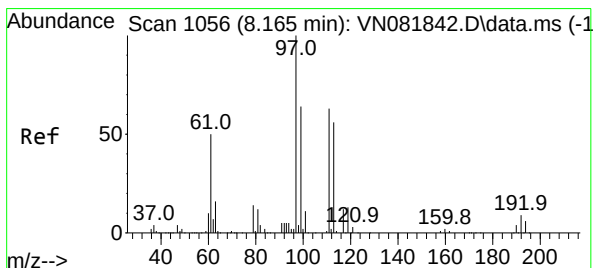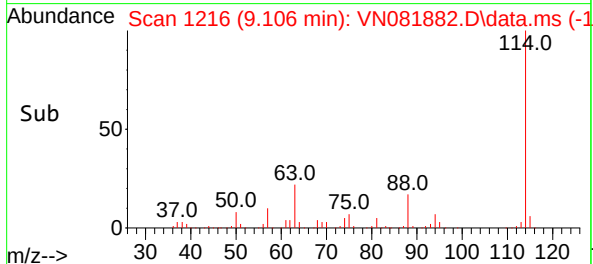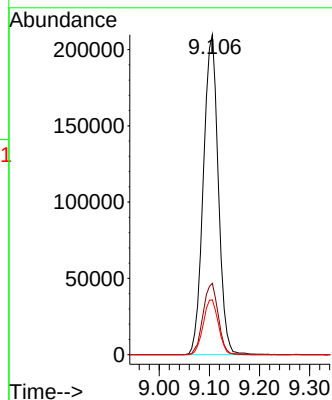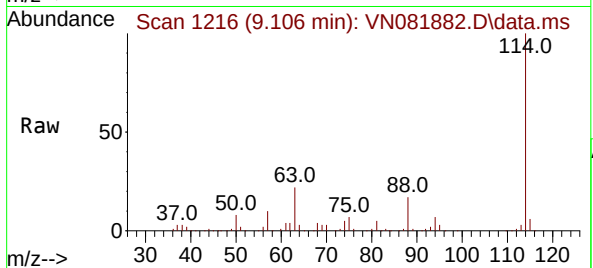

#35

Dibromofluoromethane

Concen: 48.676 ug/l

RT: 8.171 min Scan# 1057

Delta R.T. 0.006 min

Lab File: VN081882.D

Acq: 26 Apr 2024 16:56




Tgt Ion:113 Resp: 127112


Ion Ratio Lower Upper

113 100

111 104.1 83.4 125.2

192 17.1 14.0 21.0


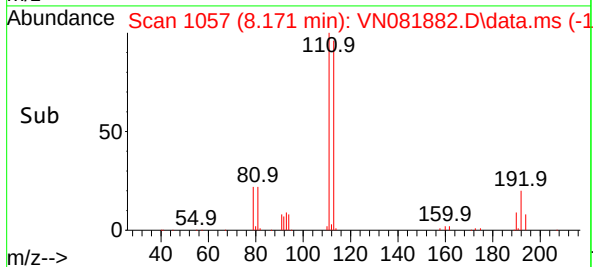
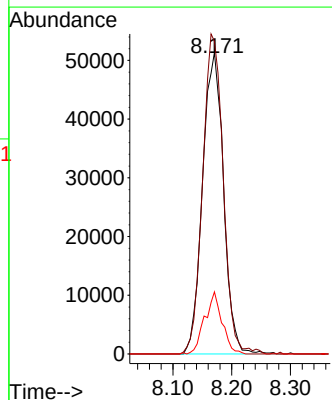
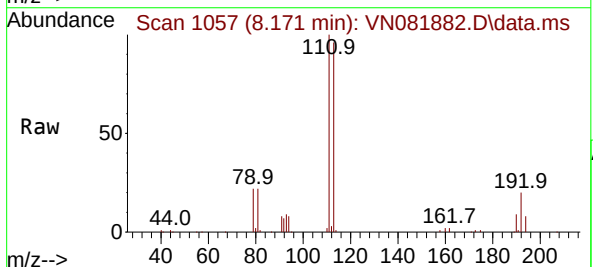


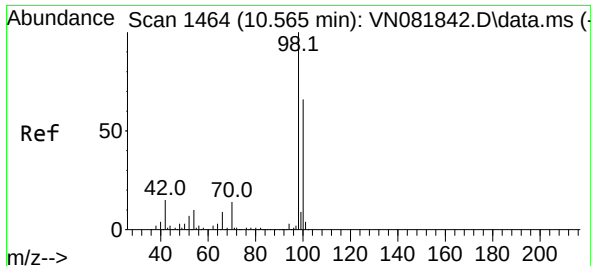

#50
Toluene-d8
Concen: 51.810 ug/l
RT: 10.570 min Scan# 1465
Delta R.T. 0.006 min
Lab File: VN081882.D
Acq: 26 Apr 2024 16:56




Instrument :
MSVOA_N
ClientSampleId :
STORAGE-BLANK-SAMPLE-MANAG


Tgt Ion: 98 Resp: 531372
Ion Ratio Lower Upper
98 100
100 65.9 51.8 77.6

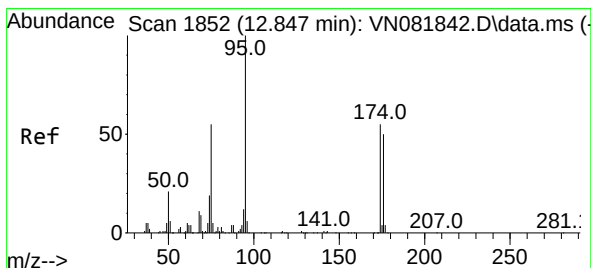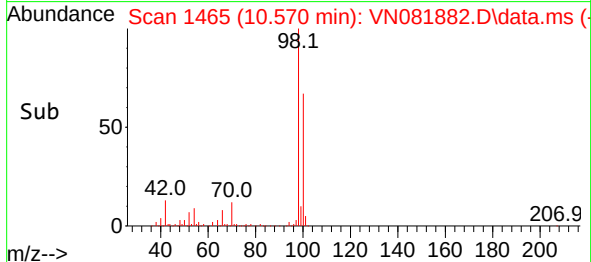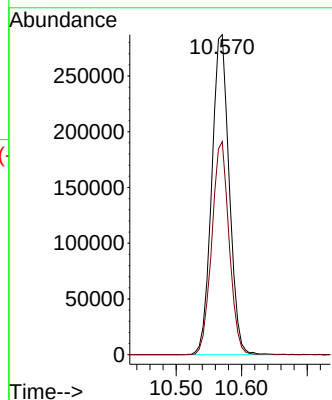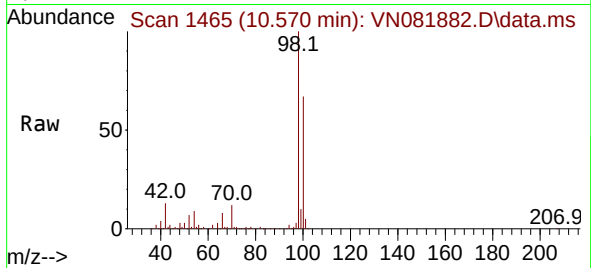

#62
4-Bromofluorobenzene
Concen: 47.009 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. 0.006 min
Lab File: VN081882.D
Acq: 26 Apr 2024 16:56

Tgt Ion: 95 Resp: 190586
Ion Ratio Lower Upper
95 100
174 66.3 0.0 160.6
176 61.5 0.0 152.8


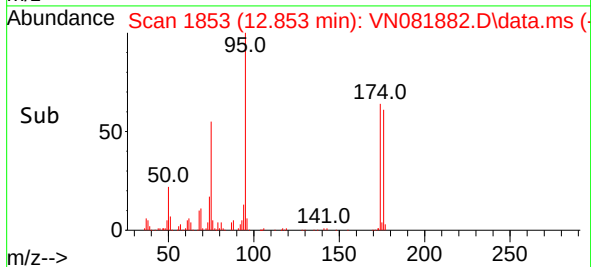
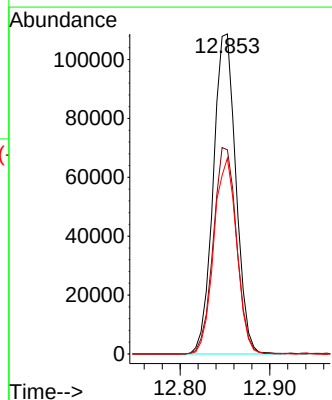
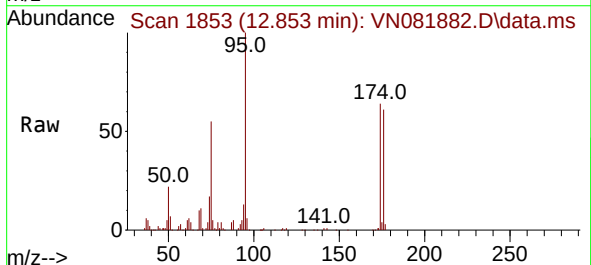


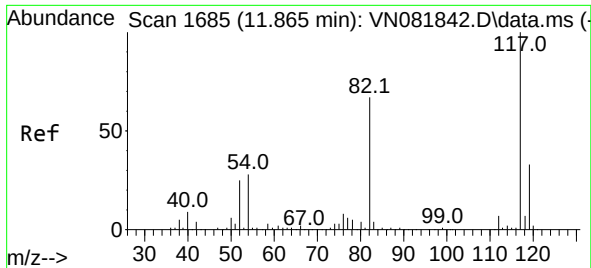

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.865 min Scan# 117
Delta R.T. -0.000 min
Lab File: VN081882.D
Acq: 26 Apr 2024 16:56

Instrument :
MSVOA_N
ClientSampleId :
STORAGE-BLANK-SAMPLE-MANAG

Tgt Ion:117 Resp: 391107
Ion Ratio Lower Upper
117 100
82 59.6 44.6 66.8
119 30.7 25.9 38.9

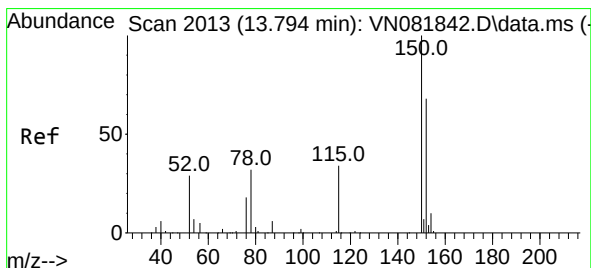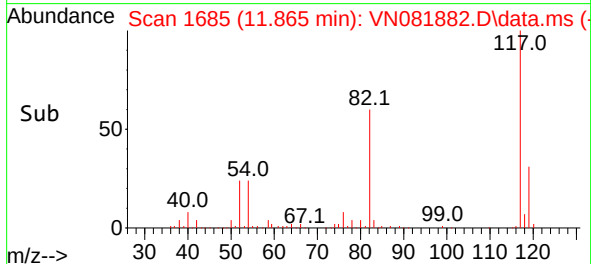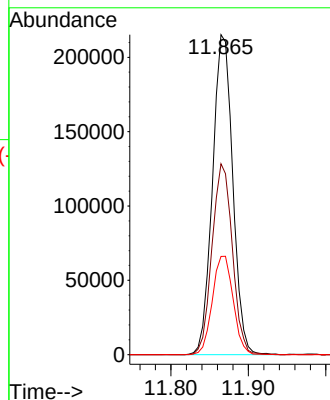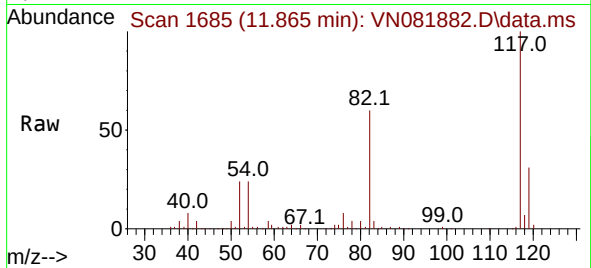

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.794 min Scan# 2013
Delta R.T. -0.000 min
Lab File: VN081882.D
Acq: 26 Apr 2024 16:56

Tgt Ion:152 Resp: 153778
Ion Ratio Lower Upper
152 100
115 65.4 30.4 91.3
150 158.5 0.0 353.2

