
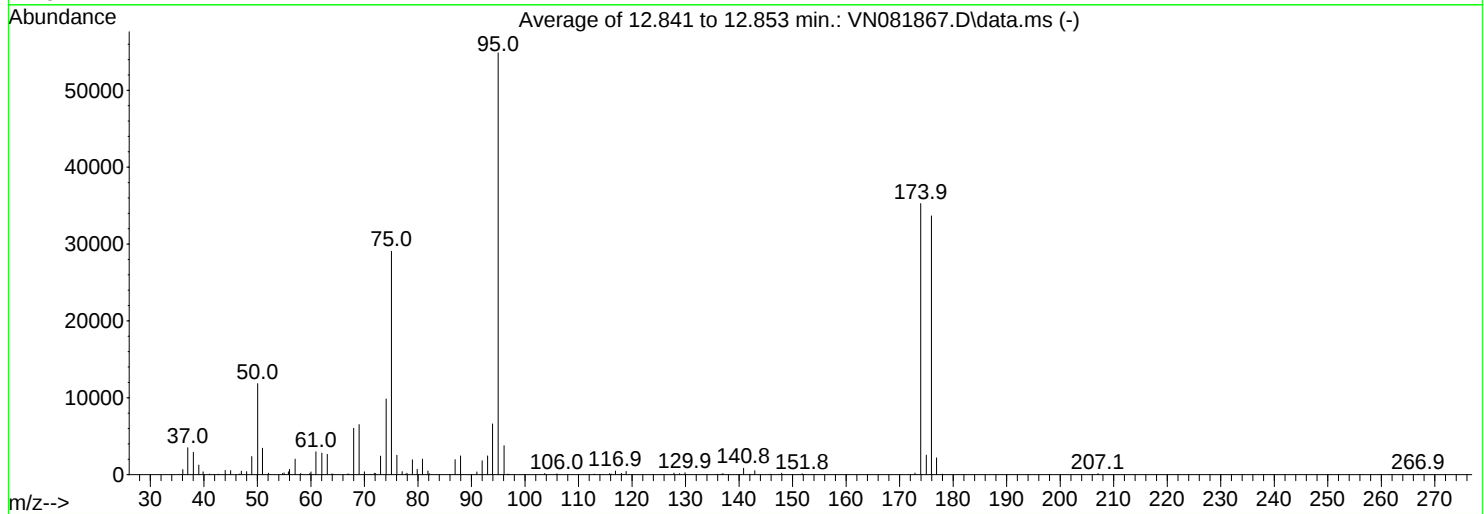


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN042624\
Data File : VN081867.D
Acq On : 26 Apr 2024 08:26
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N042524W.M
Title : SW846 8260
Last Update : Fri Apr 26 05:26:49 2024

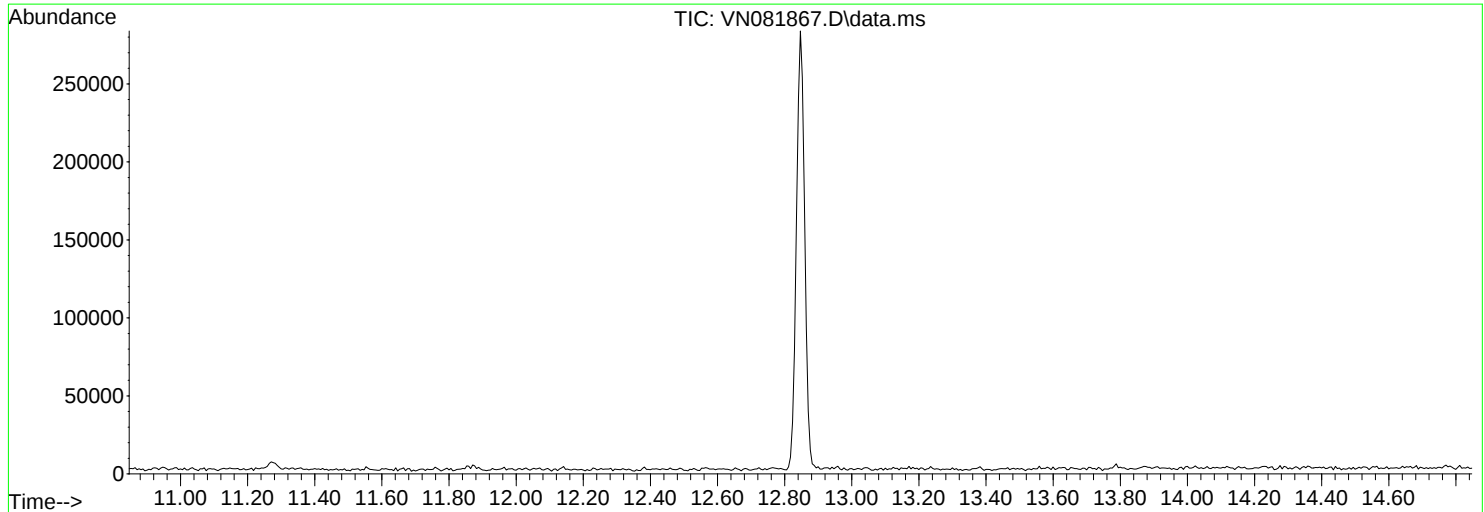

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	21.6	11848	PASS
75	95	30	60	53.0	29061	PASS
95	95	100	100	100.0	54877	PASS
96	95	5	9	6.9	3774	PASS
173	174	0.00	2	0.6	219	PASS
174	95	50	100	64.3	35269	PASS
175	174	5	9	7.2	2538	PASS
176	174	95	101	95.4	33656	PASS
177	176	5	9	6.5	2186	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	673	48.00	398	59.80	151	70.00	380
37.00	3493	48.95	2344	60.00	361	71.10	51
38.05	2908	50.05	11848	60.95	2978	71.85	18
39.05	1244	50.95	3438	62.05	2809	72.10	14
39.85	378	52.05	196	63.05	2634	73.00	2407
41.10	94	54.70	137	63.90	79	74.05	9853
42.70	67	55.00	229	64.10	87	75.05	29061
44.00	559	55.80	368	66.90	77	76.05	2524
45.00	523	56.00	698	67.10	81	77.05	391
46.70	91	57.05	2021	68.00	6032	77.70	67
47.00	466	58.10	152	69.00	6517	77.95	198

Average of 12.841 to 12.853 min.: VN081867.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
78.95	1940	95.00	54877	118.90	420	147.95	180
79.85	678	96.10	3774	127.85	210	151.80	126
80.85	2023	96.70	56	128.85	131	172.85	219
81.85	473	97.00	59	129.90	244	173.95	35269
82.10	126	103.70	153	135.90	63	175.00	2538
86.95	1963	105.95	110	136.70	65	175.95	33656
87.95	2433	113.00	55	137.00	144	176.90	2186
91.00	349	115.80	116	140.85	825	178.00	60
92.00	1807	116.10	77	142.00	58	207.05	157
93.00	2442	116.90	489	142.95	521	266.90	51
93.95	6603	118.00	163	145.80	57		