
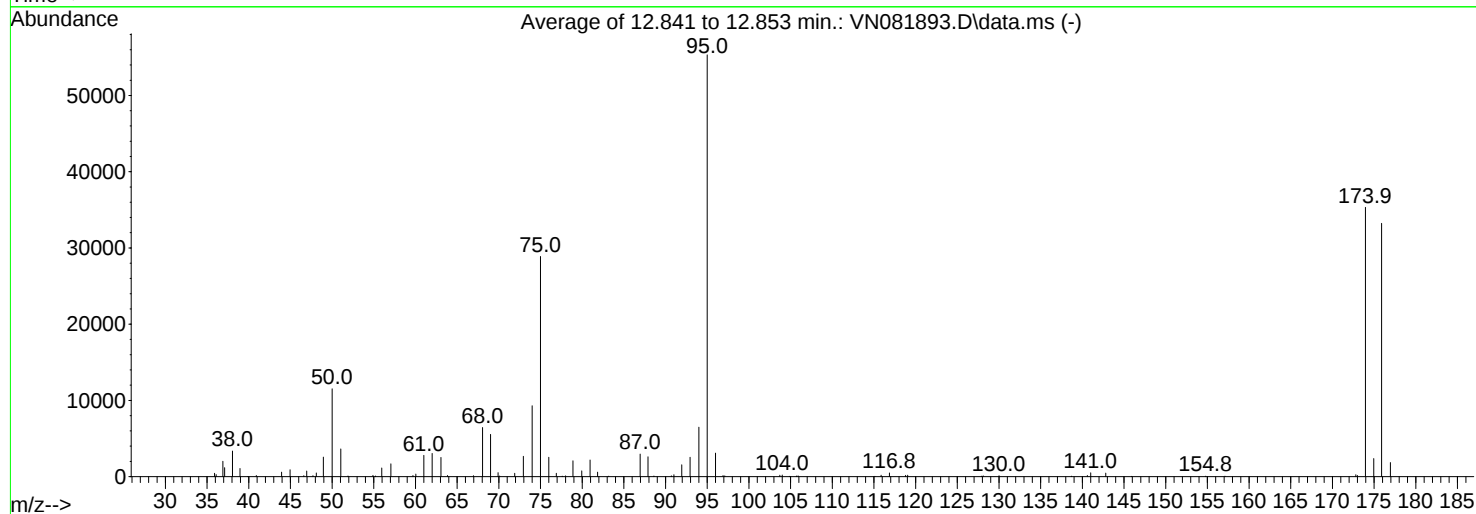


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN042624\
Data File : VN081893.D
Acq On : 27 Apr 2024 00:08
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N042524W.M
Title : SW846 8260
Last Update : Fri Apr 26 05:26:49 2024

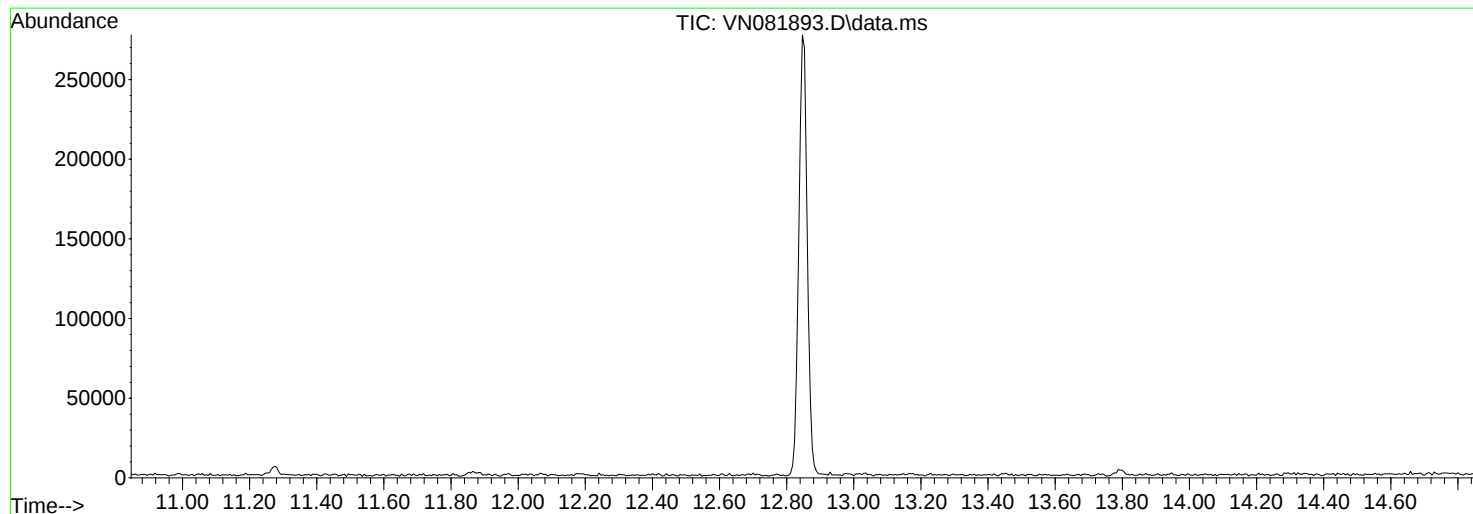

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.8	11535	PASS
75	95	30	60	52.2	28883	PASS
95	95	100	100	100.0	55331	PASS
96	95	5	9	5.6	3095	PASS
173	174	0.00	2	0.7	250	PASS
174	95	50	100	63.8	35323	PASS
175	174	5	9	6.7	2378	PASS
176	174	95	101	94.1	33235	FAIL*
177	176	5	9	5.6	1853	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	436	46.95	728	59.70	138	71.90	431
36.10	269	47.70	136	60.05	335	72.95	267
36.90	2024	48.10	489	61.00	2789	74.00	929
37.10	1185	48.95	2561	62.00	3054	75.00	2888
38.05	3351	50.00	11535	63.05	2524	76.00	2537
38.95	1073	51.05	3642	63.85	157	76.90	439
39.90	27	51.90	88	66.95	128	77.60	67
40.90	153	54.90	178	68.05	6454	78.00	102
43.95	596	55.20	90	69.00	5545	78.90	2085
44.95	903	55.95	1125	69.90	518	79.95	749
46.60	119	57.05	1674	70.10	81	80.95	2185

Average of 12.841 to 12.853 min.: VN081893.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
81.85	599	96.00	3095	118.80	168	157.10	73
83.20	54	96.90	157	119.05	182	172.80	250
86.95	2965	97.10	96	127.90	72	173.00	141
87.90	2598	103.70	184	128.10	102	173.95	35323
88.60	77	104.00	203	130.00	122	174.95	2378
90.70	110	104.90	50	138.70	66	175.90	33235
91.00	247	105.70	87	140.60	140	176.95	1853
91.95	1555	105.90	108	141.00	500		
92.95	2534	115.10	52	142.80	466		
94.00	6481	115.85	198	145.90	52		
95.00	55331	116.85	490	154.80	74		

Instrument :

MSVOA_N

ClientSampleId :

BFB