


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN042719\
Data File : VN055264.D
Acq On : 26 Apr 2019 8:52
Operator : JC/SP
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N042219W.M
Title : SW846 8260
Last Update : Tue Apr 23 05:52:53 2019

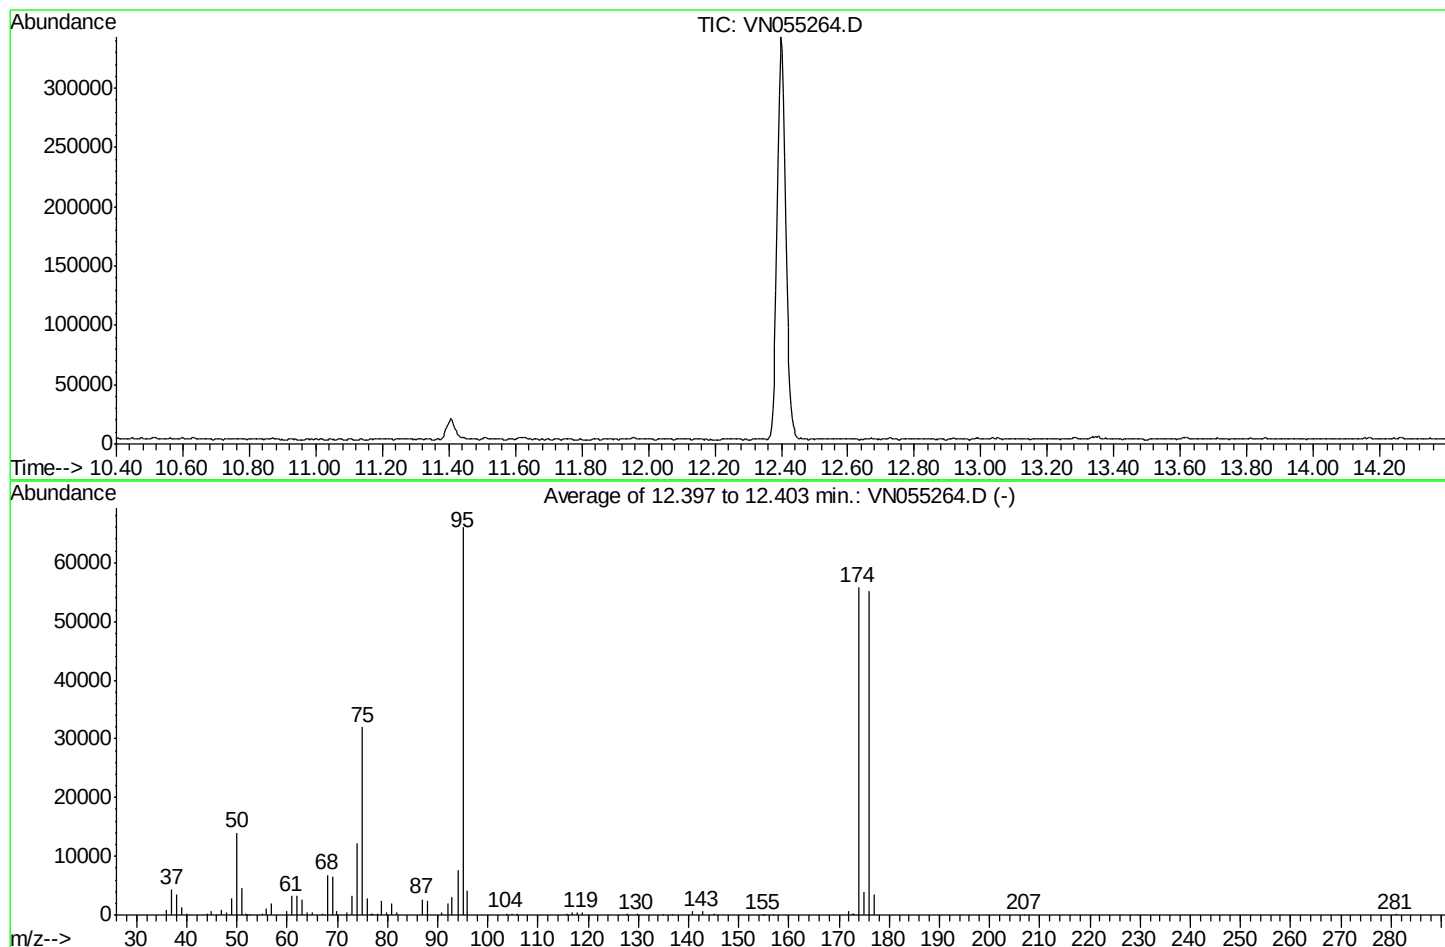

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.2	14025	PASS
75	95	30	60	48.5	32029	PASS
95	95	100	100	100.0	66029	PASS
96	95	5	9	6.3	4165	PASS
173	174	0.00	2	0.5	278	PASS
174	95	50	100	84.4	55720	PASS
175	174	5	9	6.9	3827	PASS
176	174	95	101	99.1	55234	PASS
177	176	5	9	6.2	3410	PASS