



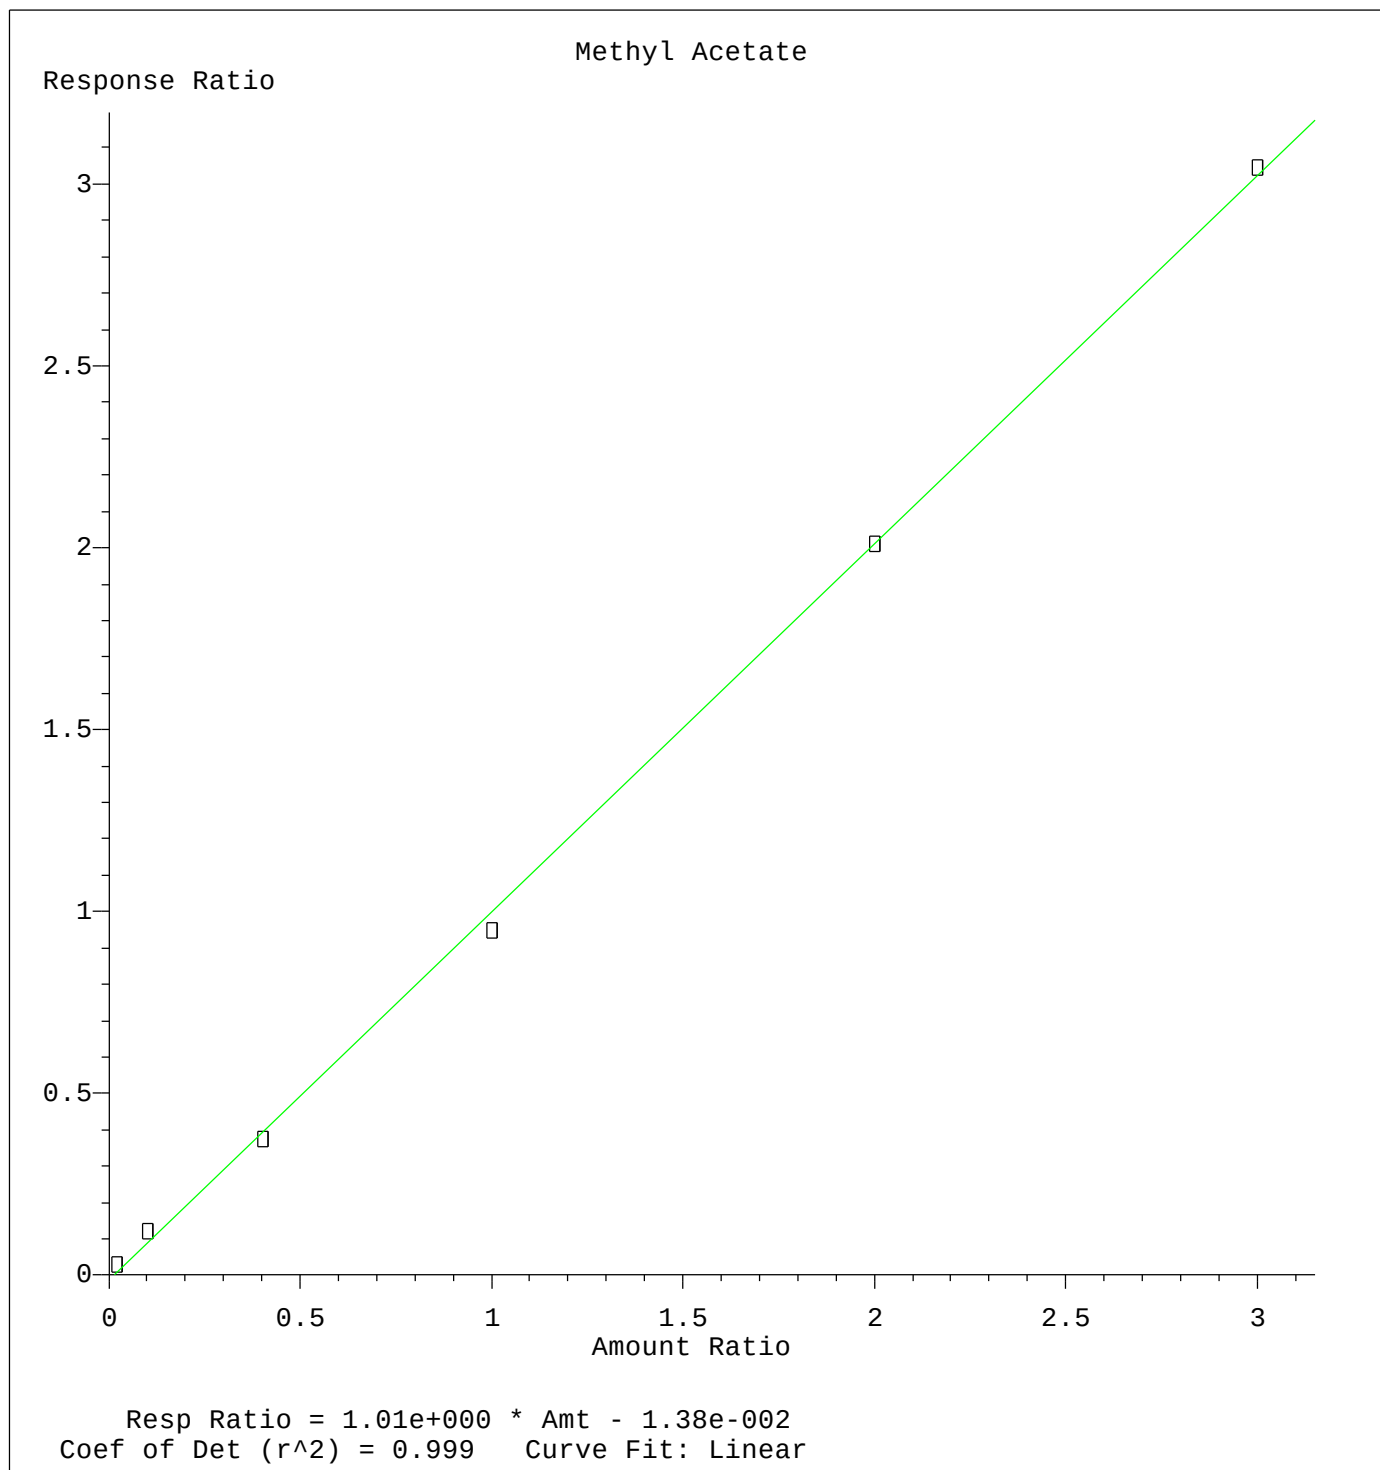

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N042720W.M
Calibration Table Last Updated: Tue Apr 28 02:20:26 2020


Methylcyclohexane

Response Ratio

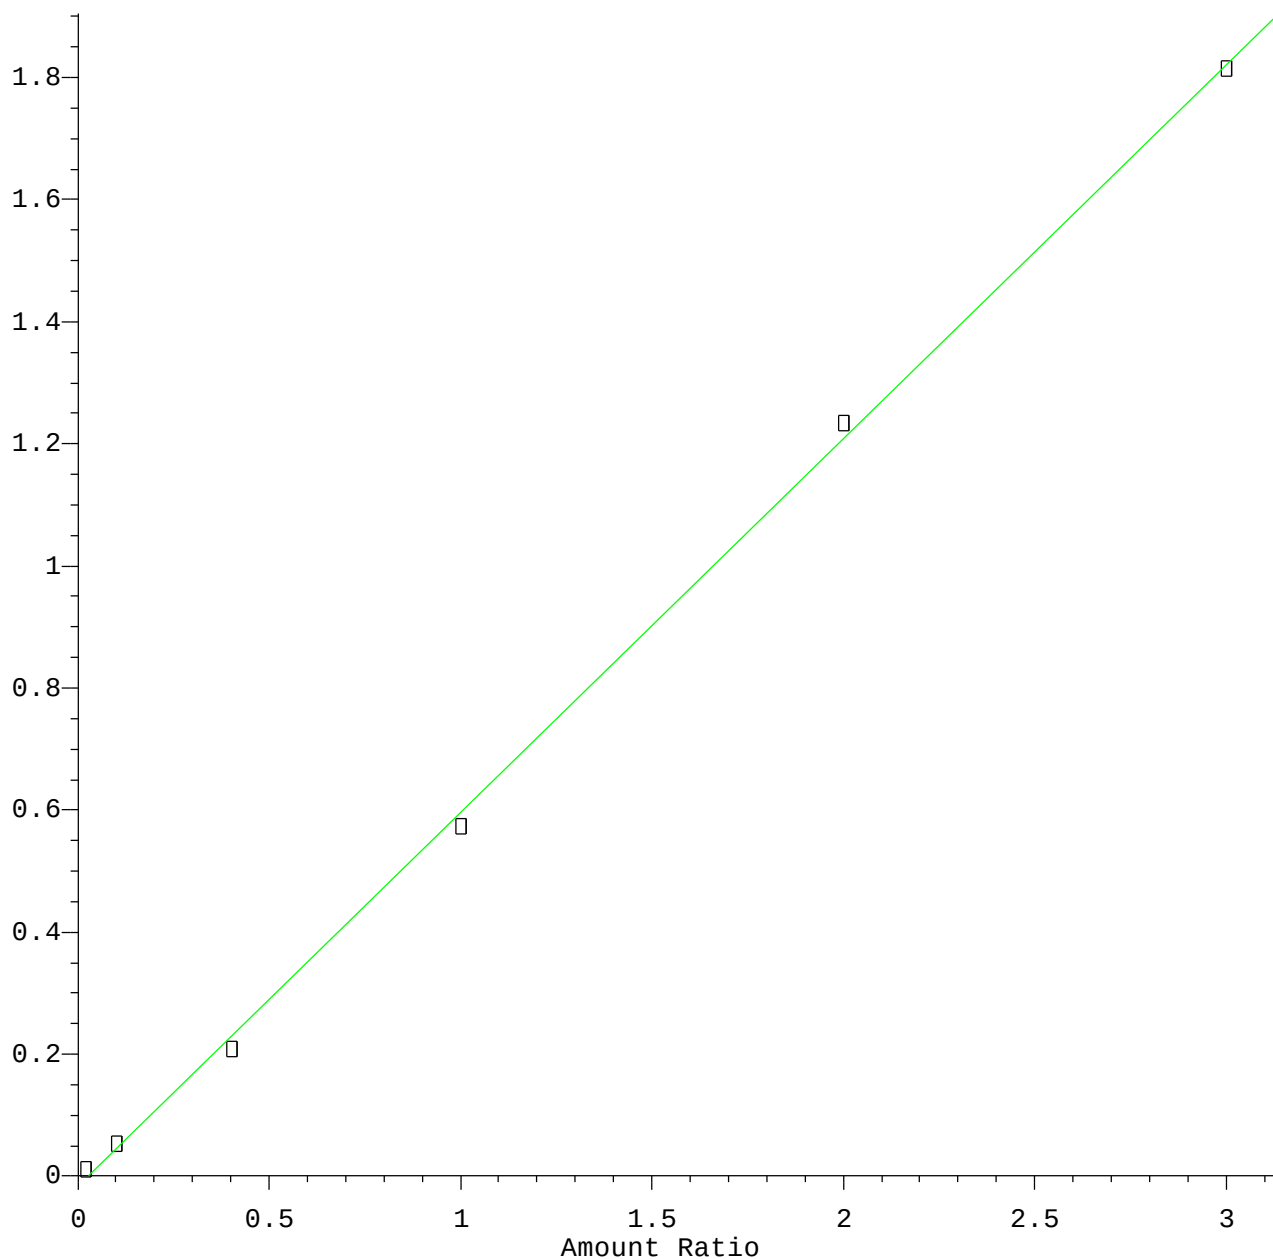


Resp Ratio = $6.12 \times 10^{-1} \times \text{Amt} - 1.71 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N042720W.M
Calibration Table Last Updated: Tue Apr 28 02:20:26 2020

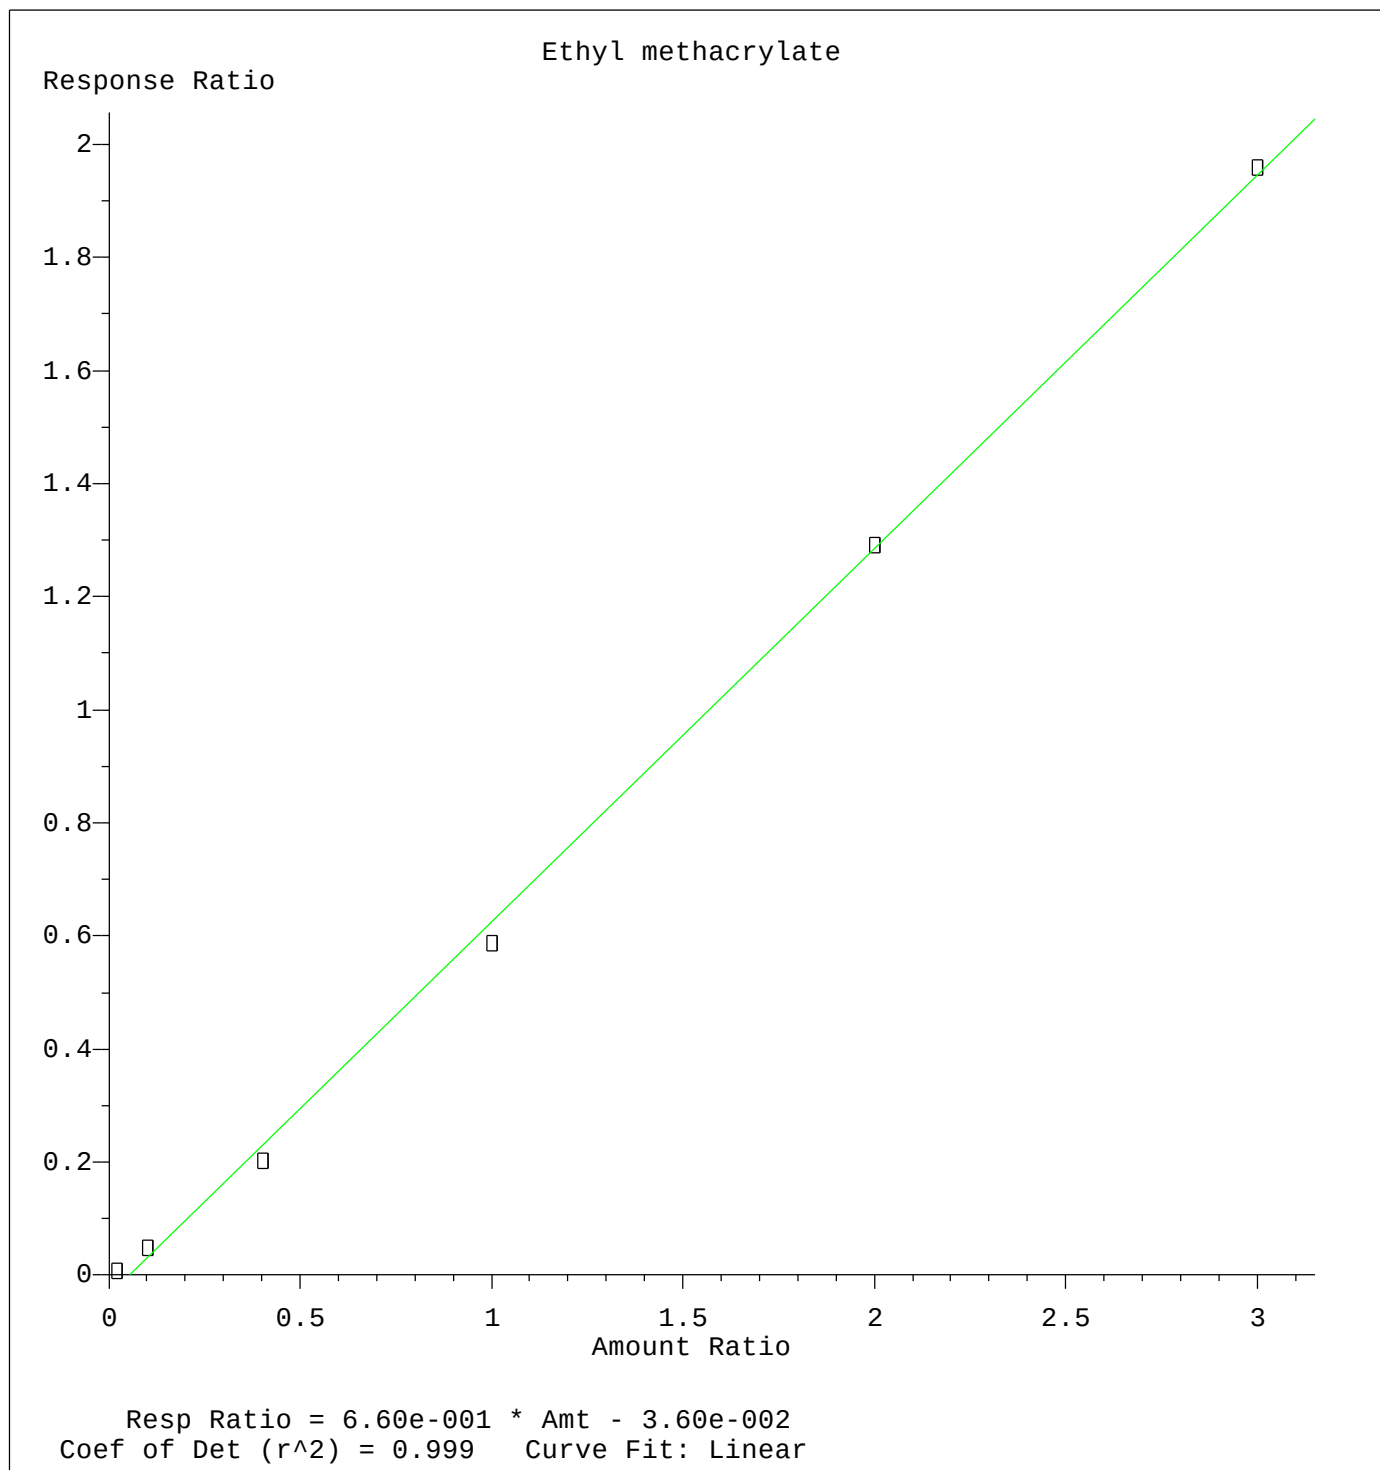

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N042720W.M
Calibration Table Last Updated: Tue Apr 28 02:20:26 2020

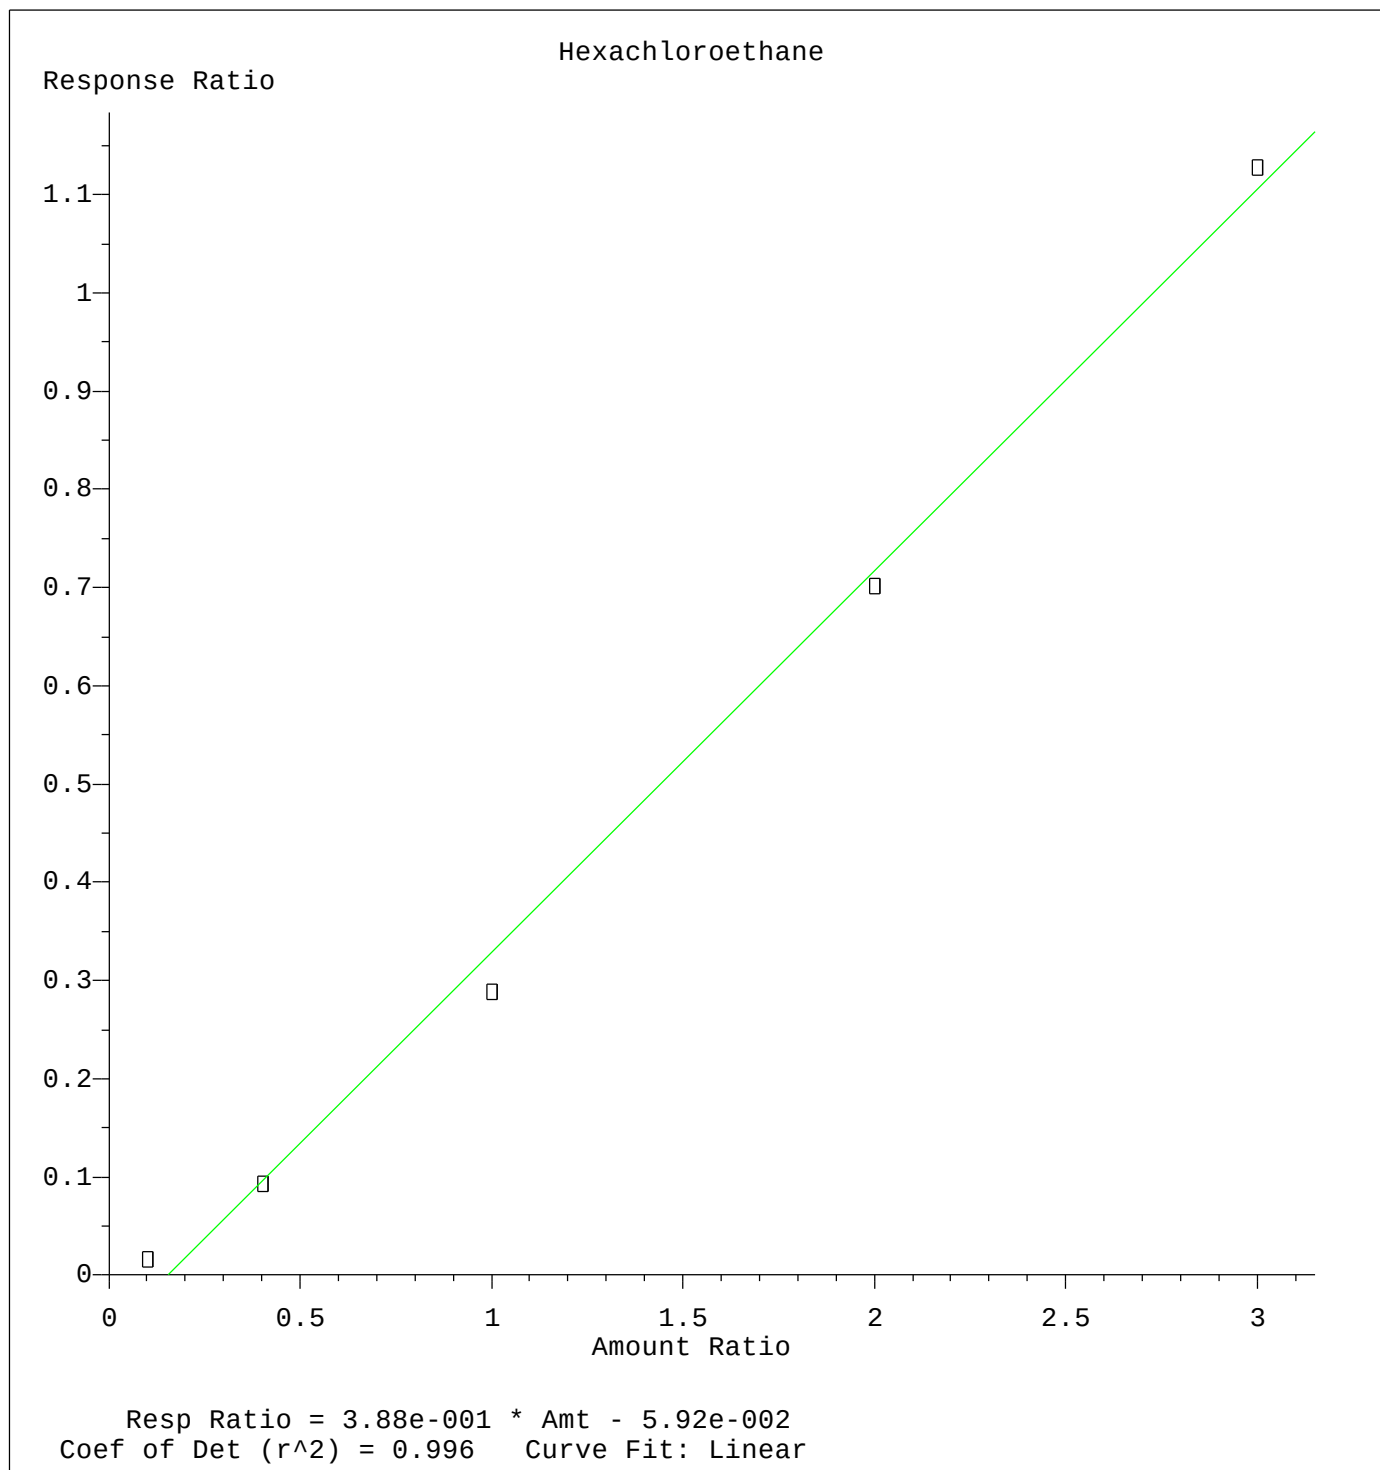


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N042720W.M
Calibration Table Last Updated: Tue Apr 28 02:20:26 2020

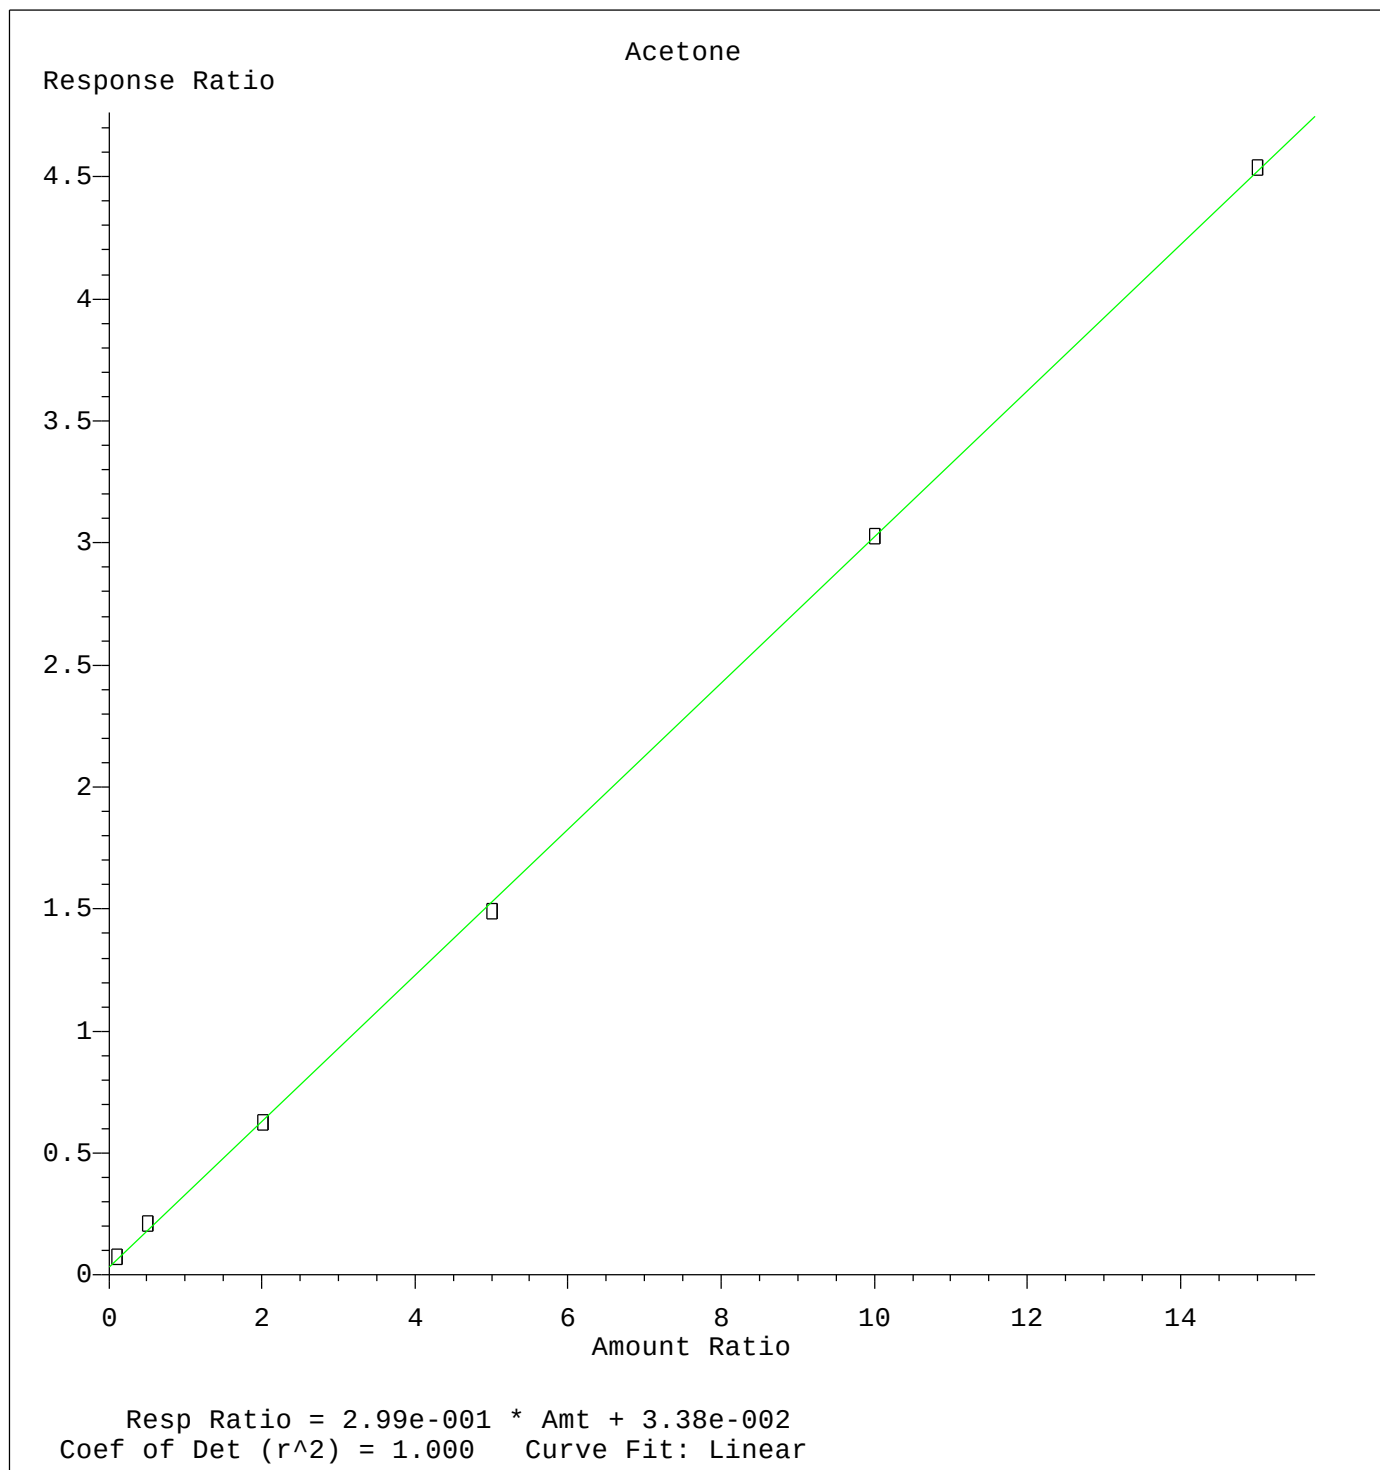

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N042720W.M
Calibration Table Last Updated: Tue Apr 28 02:20:26 2020

Carbon Tetrachloride

Response Ratio

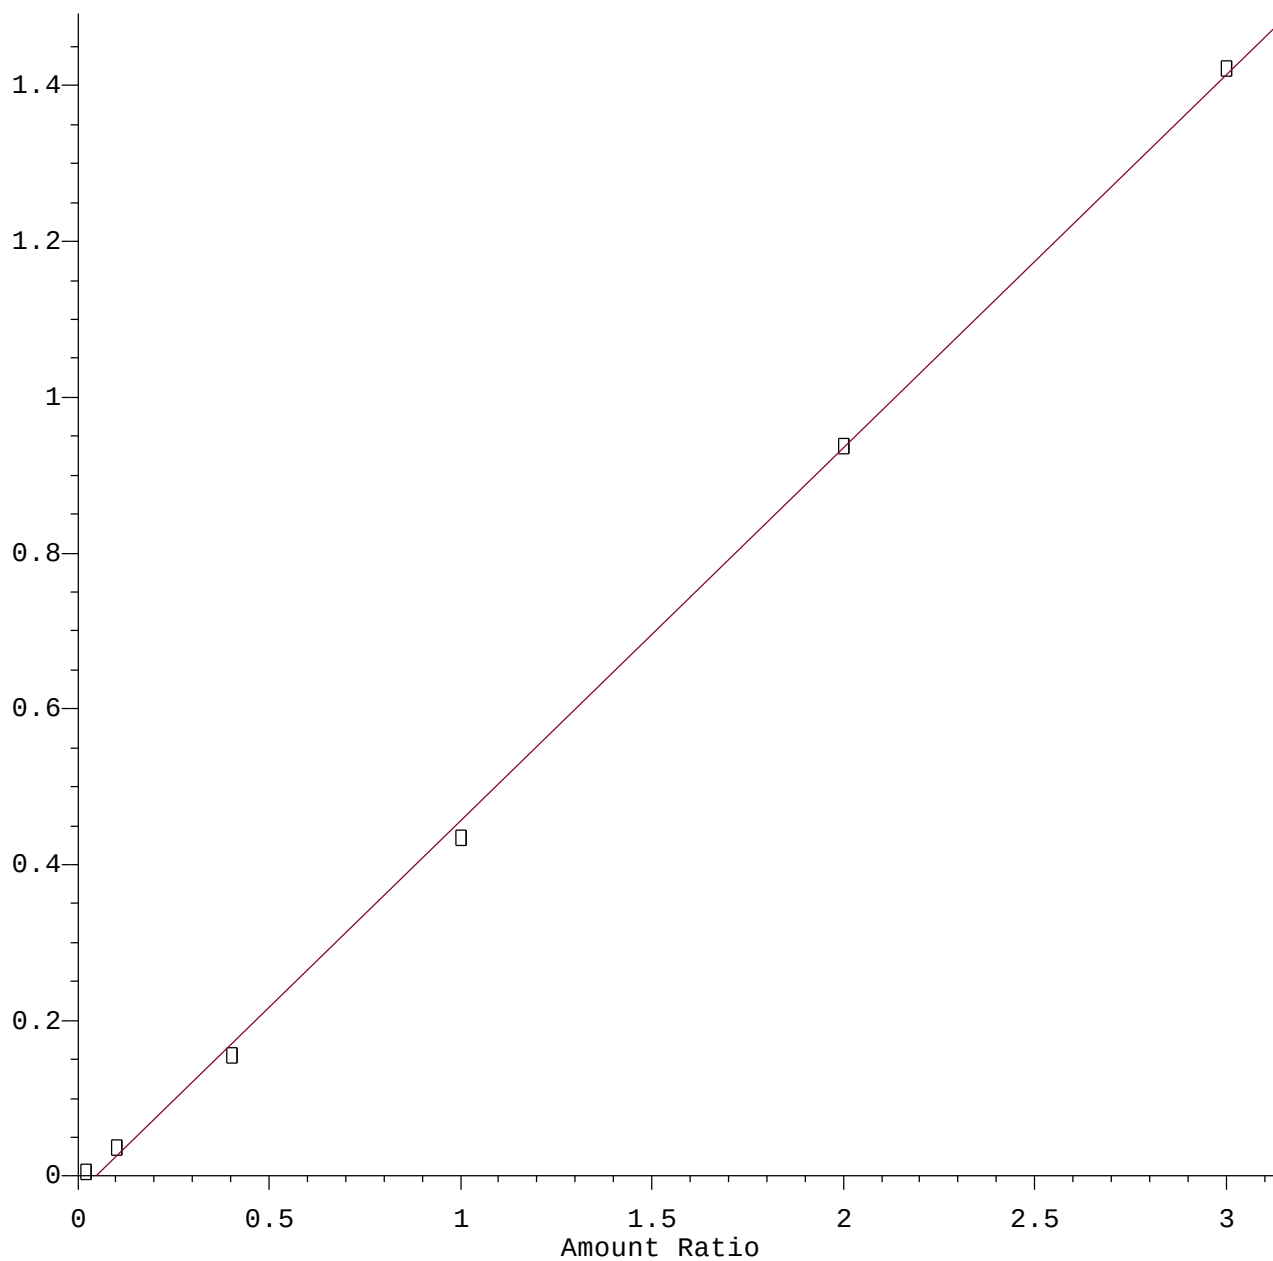

Resp Ratio = $4.79 \times 10^{-1} \times \text{Amt} - 2.19 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N042720W.M
Calibration Table Last Updated: Tue May 05 07:01:08 2020