


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN042720\
 Data File : VN061149.D
 Acq On : 27 Apr 2020 15:10
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N042720W.M
 Title : SW846 8260
 Last Update : Tue Apr 28 02:20:26 2020

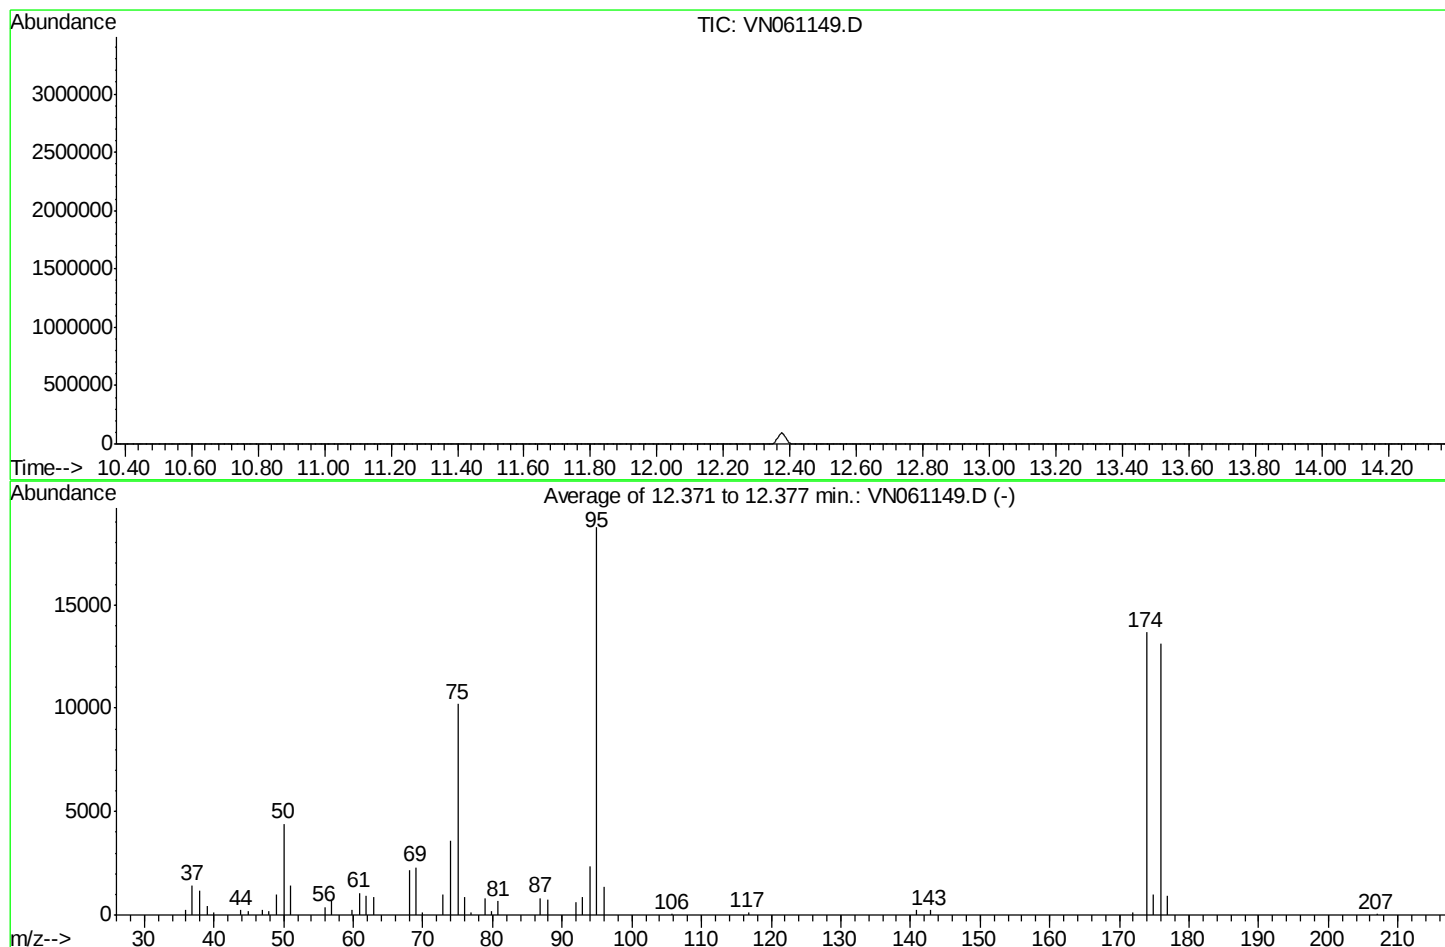

AutoFind: Scans 3353, 3354, 3355; Background Corrected with Scan 3341

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.5	4401	PASS
75	95	30	60	54.3	10186	PASS
95	95	100	100	100.0	18746	PASS
96	95	5	9	7.1	1336	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	72.8	13653	PASS
175	174	5	9	7.2	986	PASS
176	174	95	101	96.3	13144	PASS
177	176	5	9	6.9	912	PASS