


Ethyl methacrylate

Response Ratio

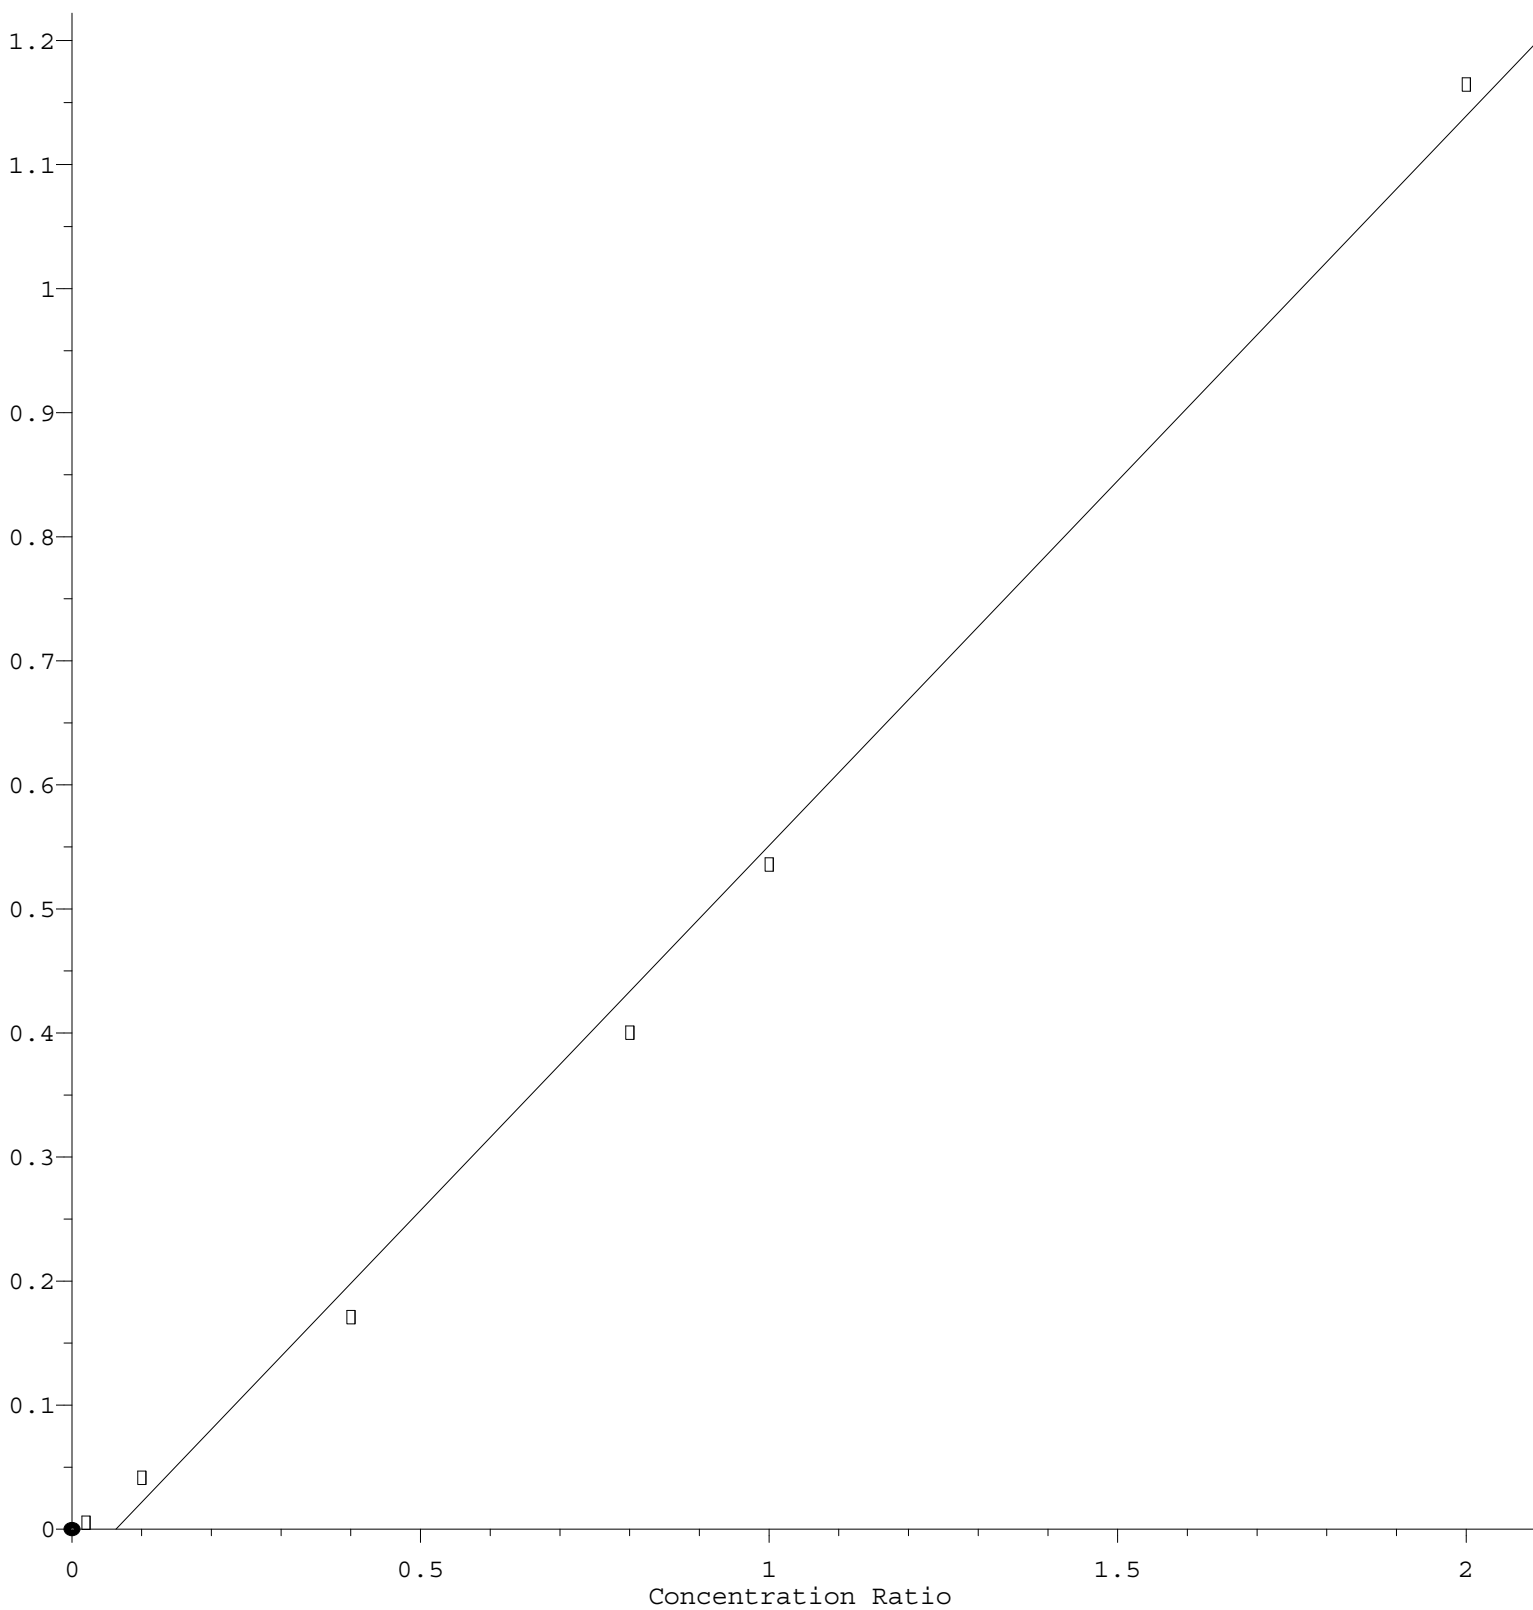

$$\text{Response} = 5.884\text{e-}001 * \text{Amt} - 3.729\text{e-}002$$


Coef of Det (r^2) = 0.995693 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N042721W.M

Calibration Table Last Updated: Tue Apr 27 16:02:50 2021

Methyl Acetate

Response Ratio

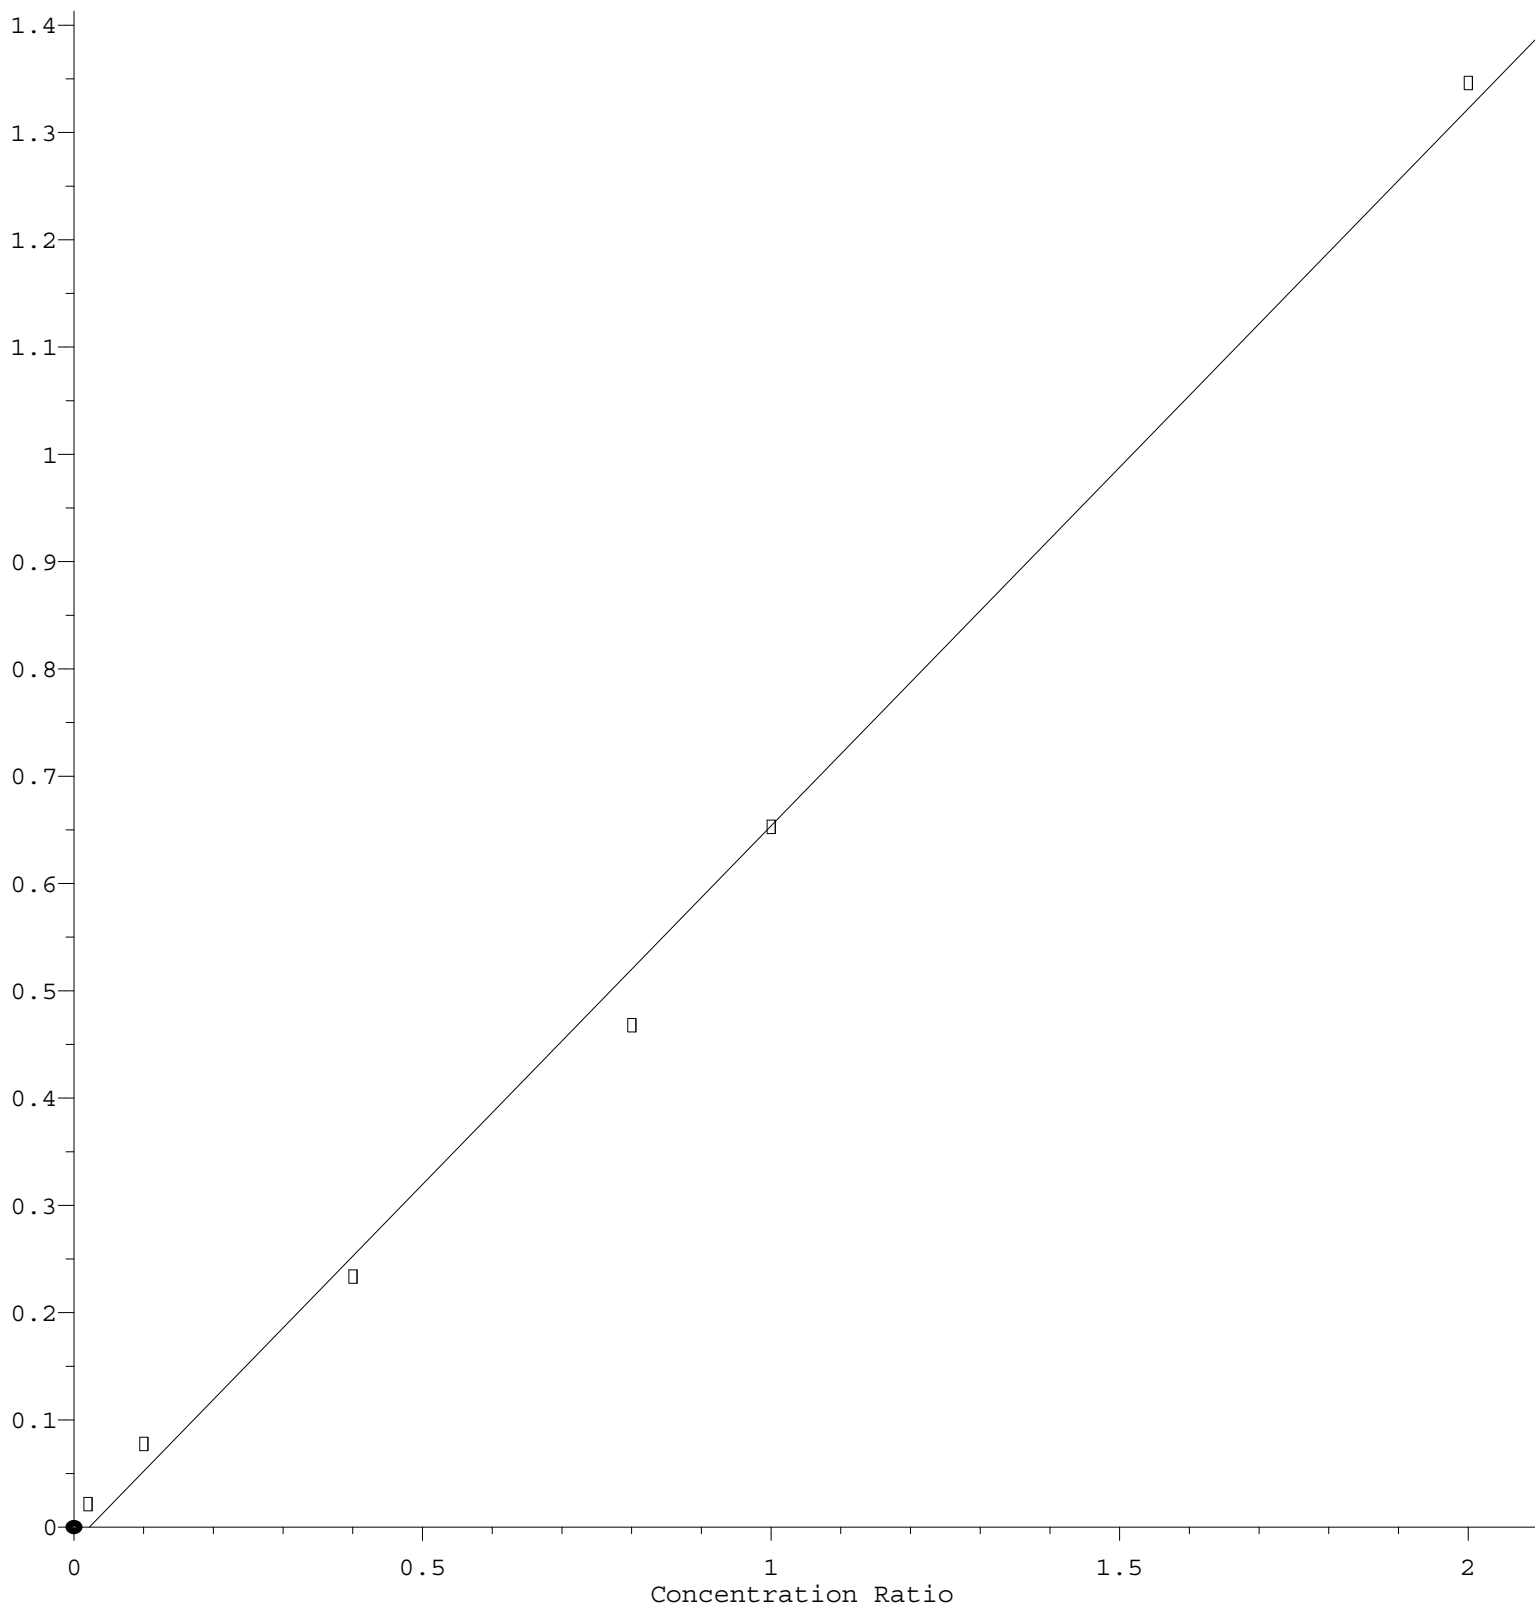


$$\text{Response} = 6.686\text{e-}001 * \text{Amt} - 1.489\text{e-}002$$

Coef of Det (r^2) = 0.996008 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N042721W.M

Calibration Table Last Updated: Tue Apr 27 16:02:50 2021


trans-1,4-Dichloro-2-butene

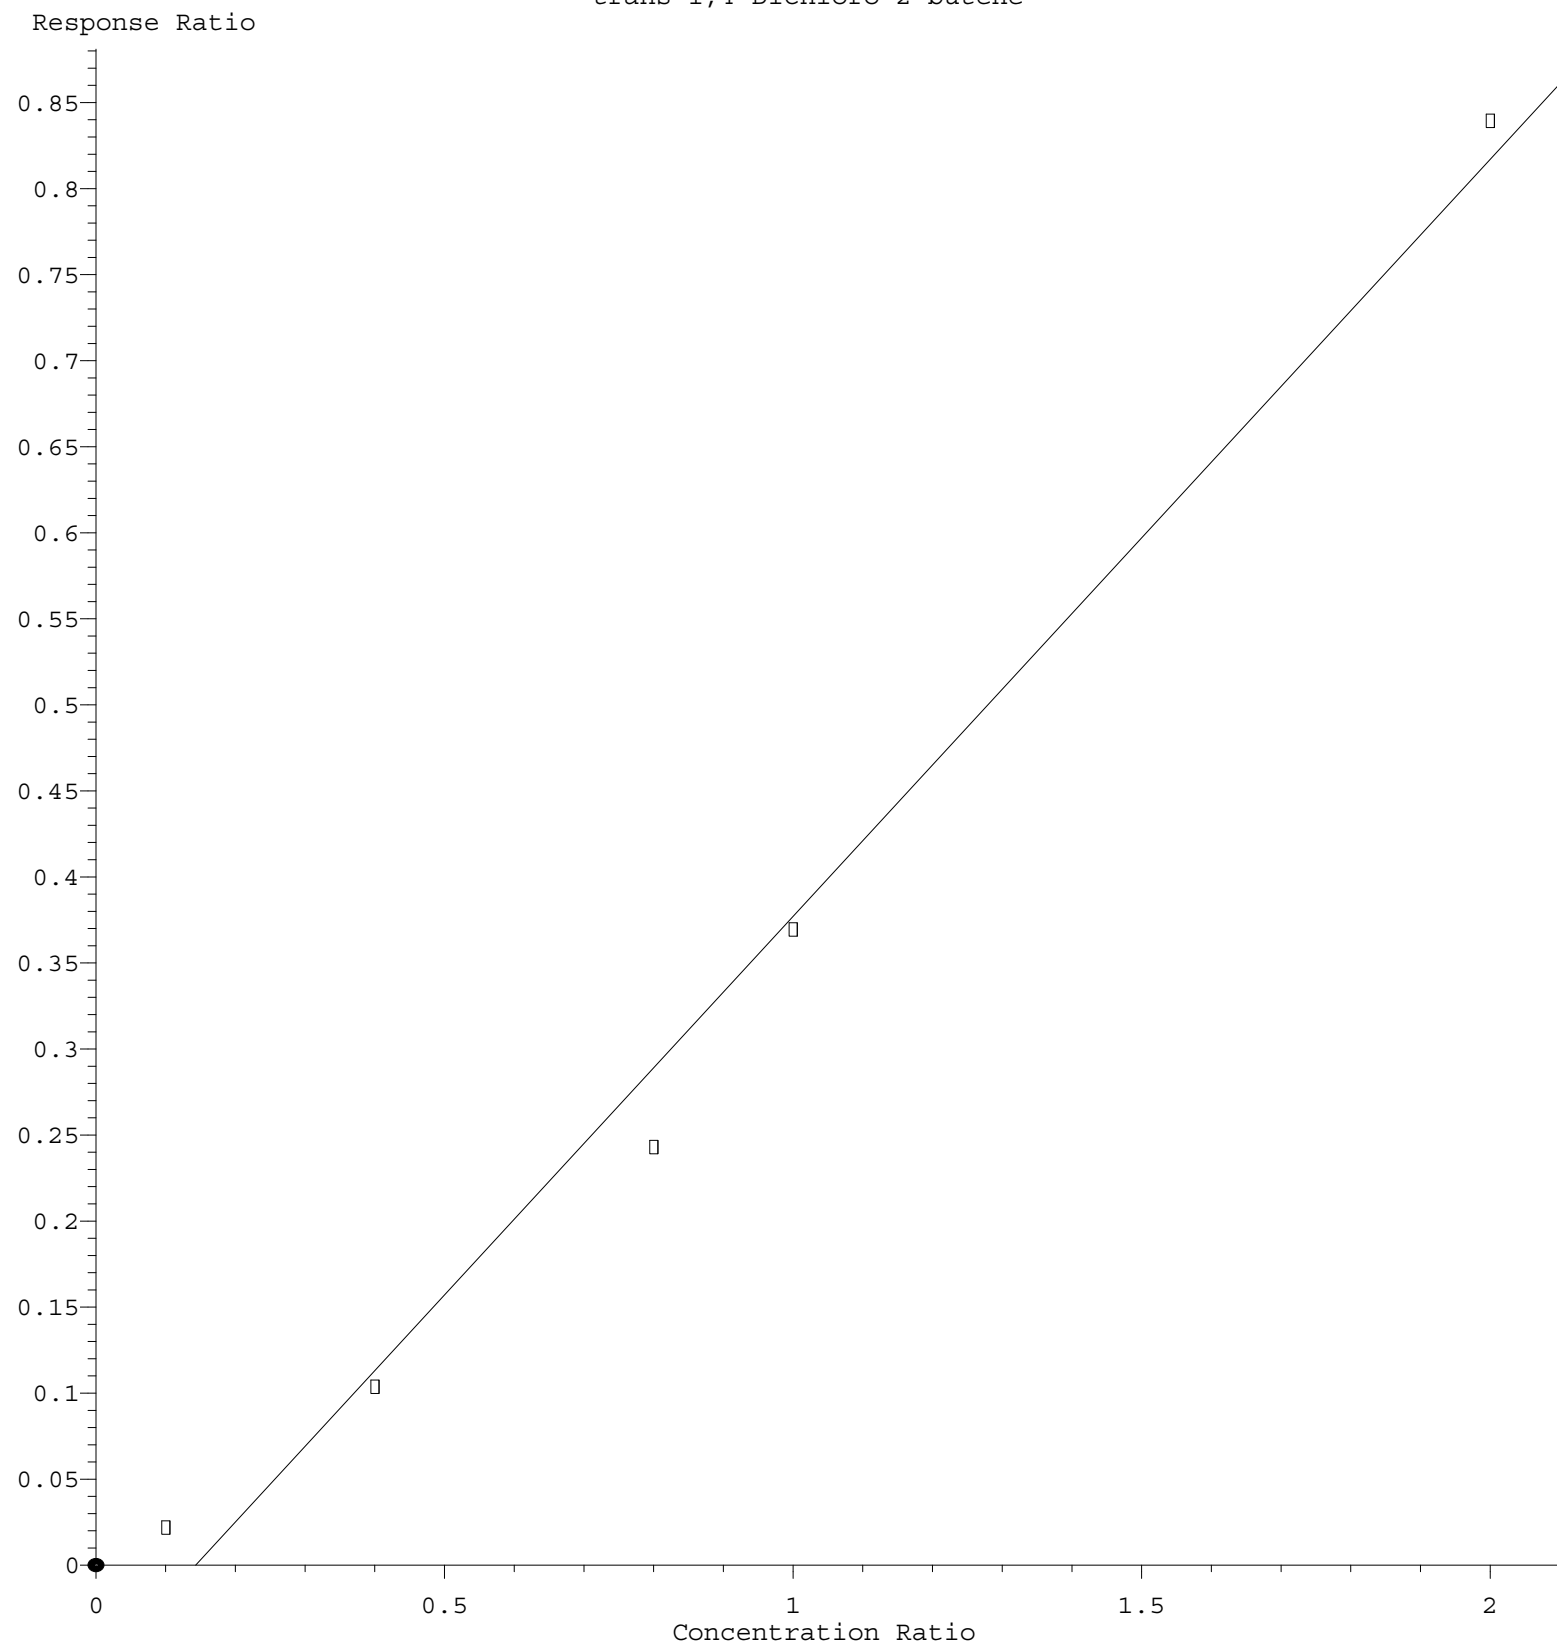

Response = $4.402e-001 * \text{Amt} - 6.311e-002$
Coef of Det (r^2) = 0.989299 Curve Fit: Linear
Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N042721W.M
Calibration Table Last Updated: Tue Apr 27 16:02:50 2021

Styrene


Response Ratio

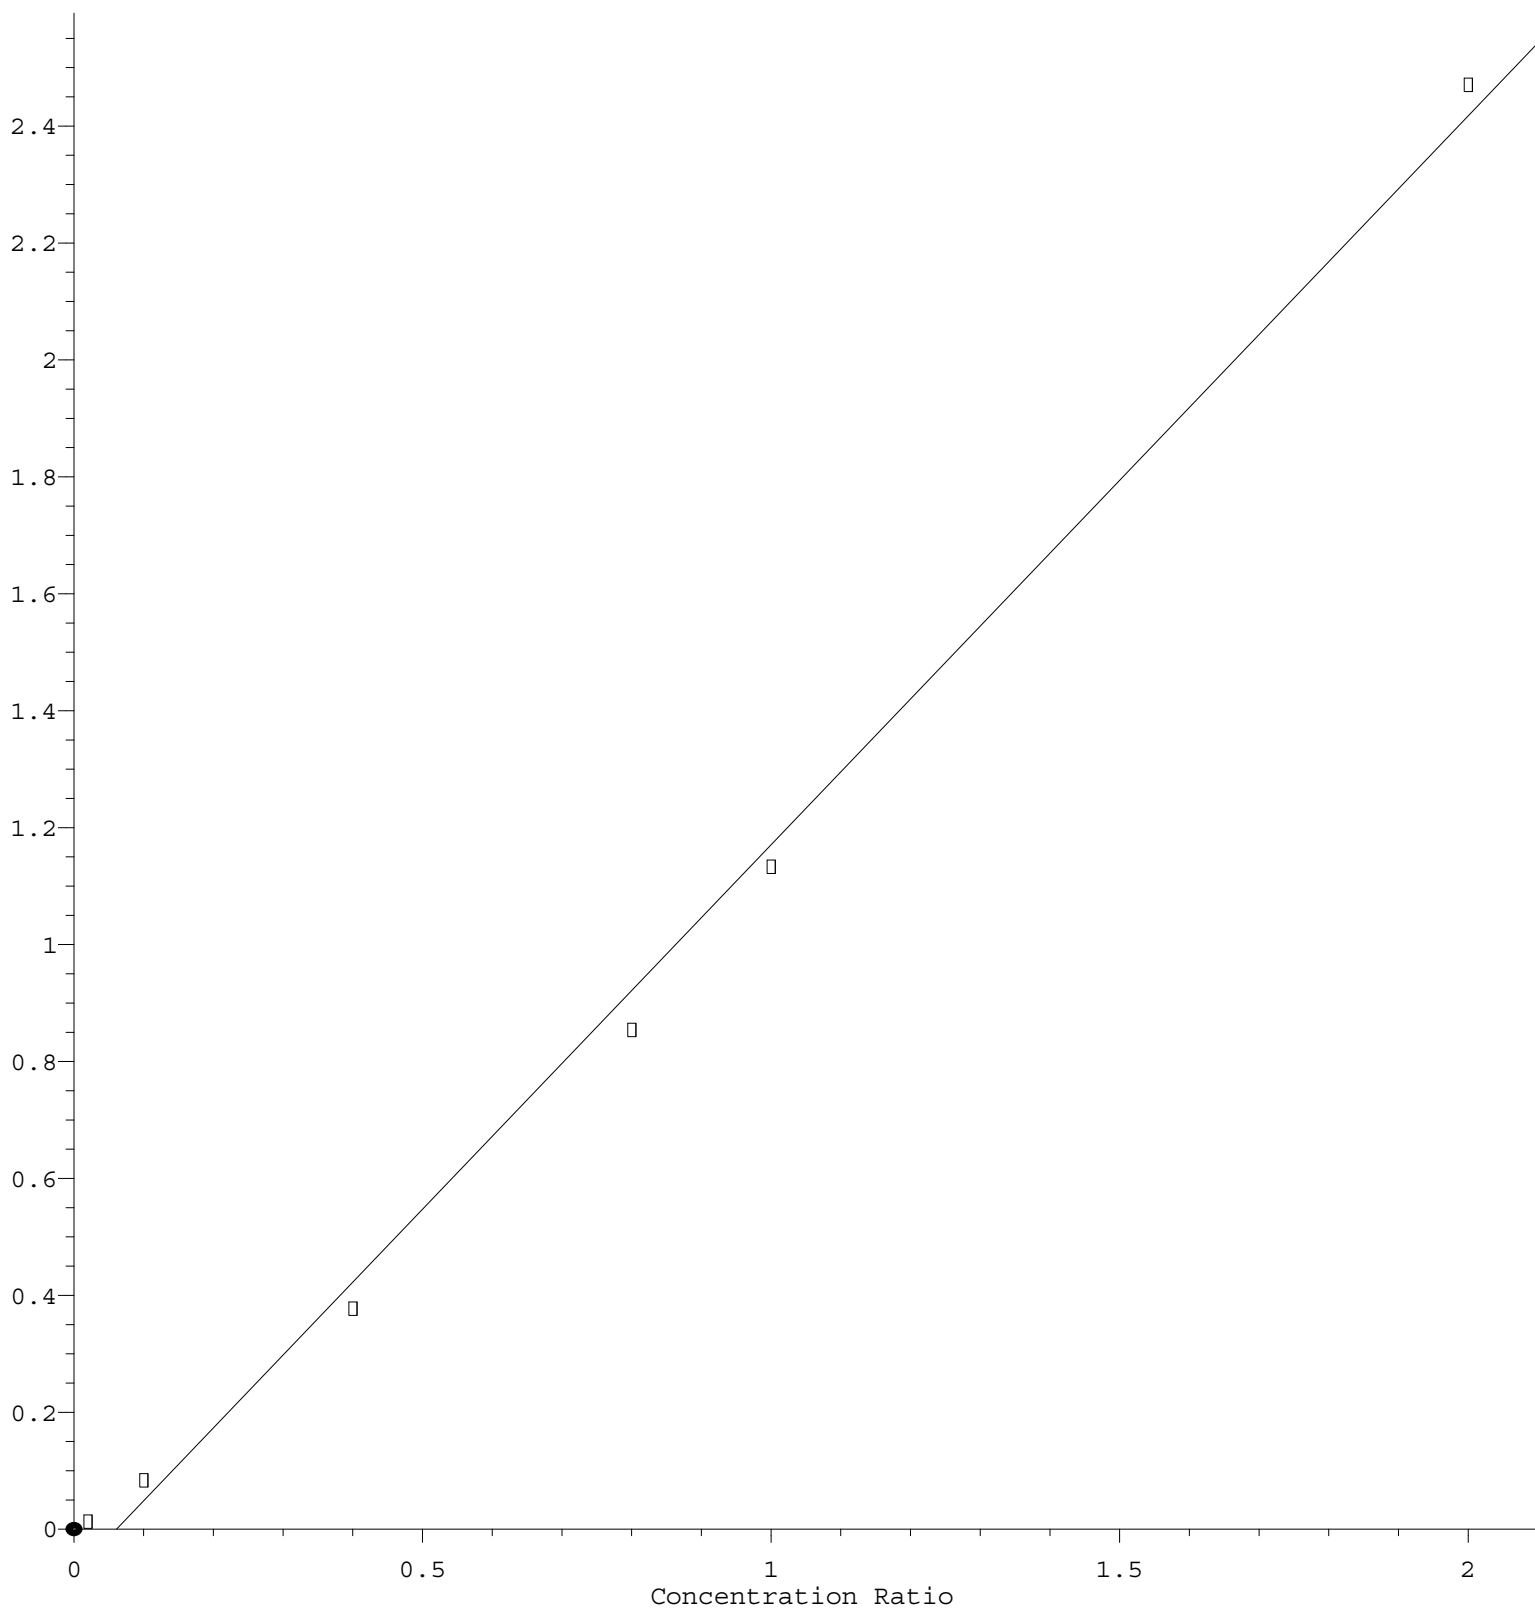

Response = 1.247e+000 * Amt - 7.590e-002
 Coef of Det (r^2) = 0.996155 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N042721W.M
 Calibration Table Last Updated: Tue Apr 27 16:02:50 2021

2-Hexanone

Response Ratio

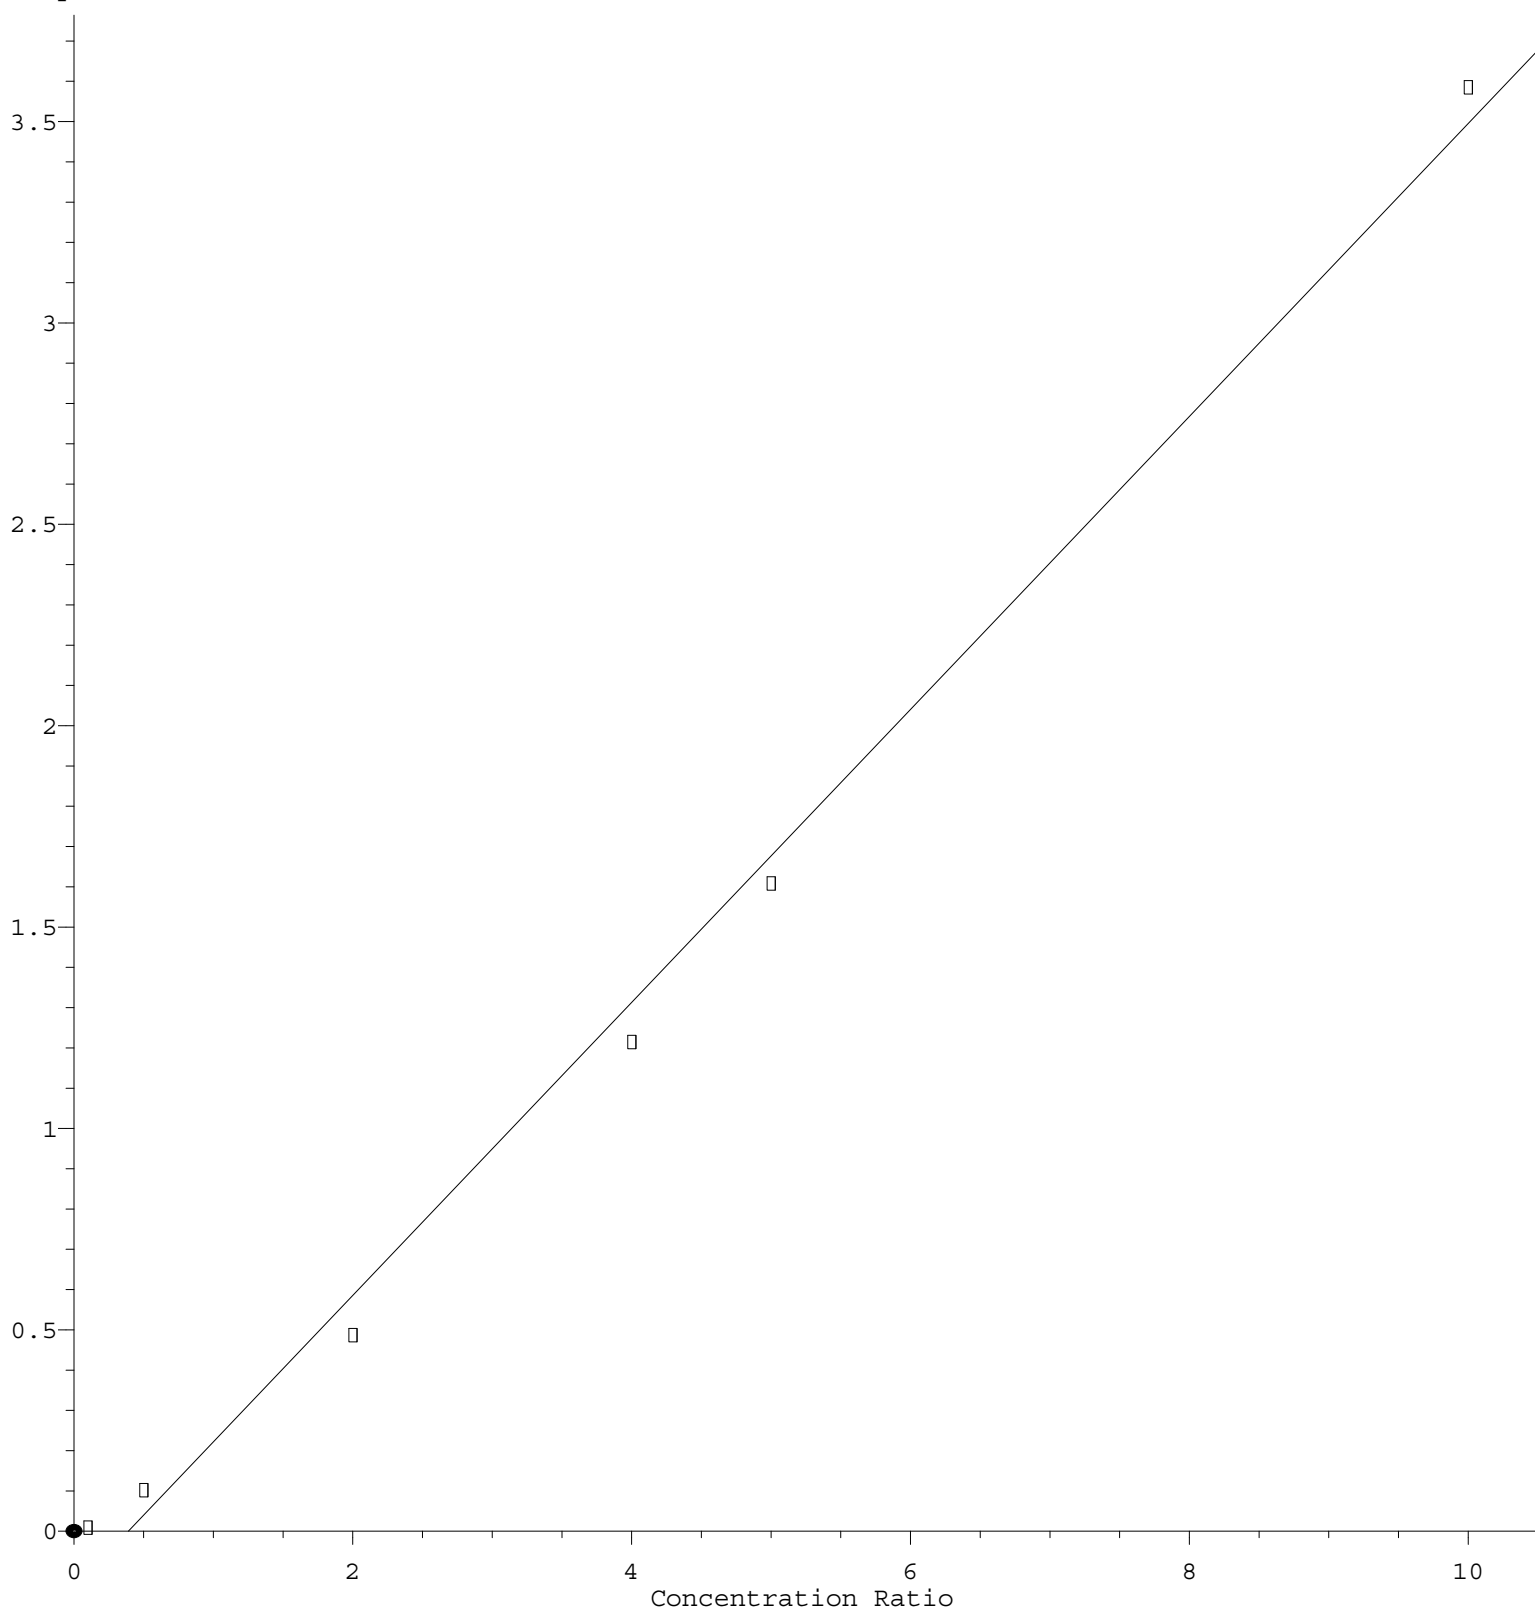

$$\text{Response} = 3.638\text{e-}001 * \text{Amt} - 1.422\text{e-}001$$


Coef of Det (r^2) = 0.994531 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N042721W.M

Calibration Table Last Updated: Tue Apr 27 16:02:50 2021

2-Chloroethyl Vinyl ether

Response Ratio

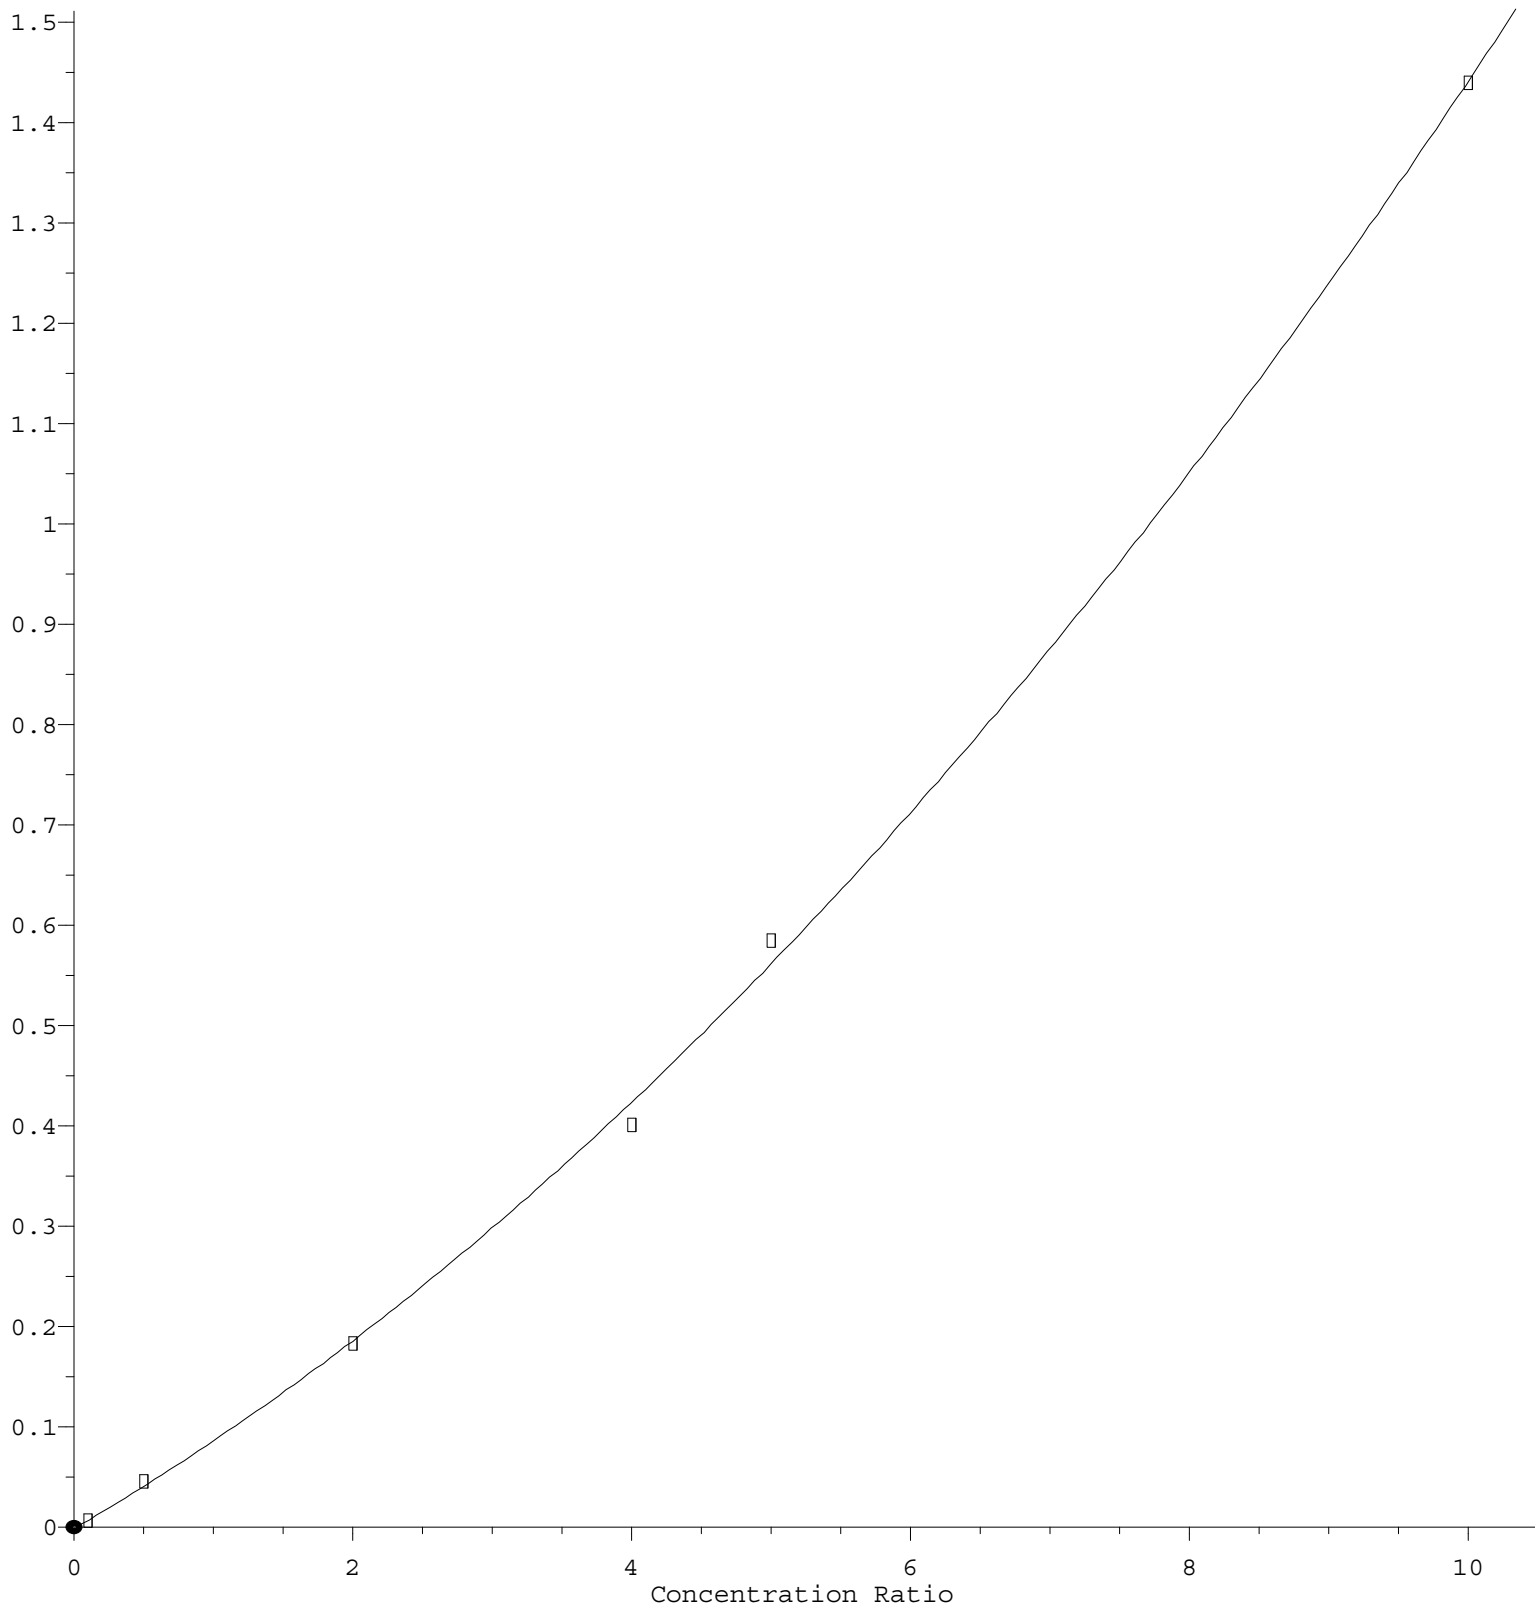

$R = 6.332e-003 A^2 + 8.096e-002 A - 1.363e-003$
 Coef of Det (r^2) = 0.999242 Curve Fit: Quadratic
 Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N042721W.M
 Calibration Table Last Updated: Tue Apr 27 16:02:50 2021