


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN042721\
Data File : VN066771.D
Acq On : 27 Apr 2021 10:22
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N042721W.M
Title : SW846 8260
Last Update : Tue Apr 27 16:02:50 2021

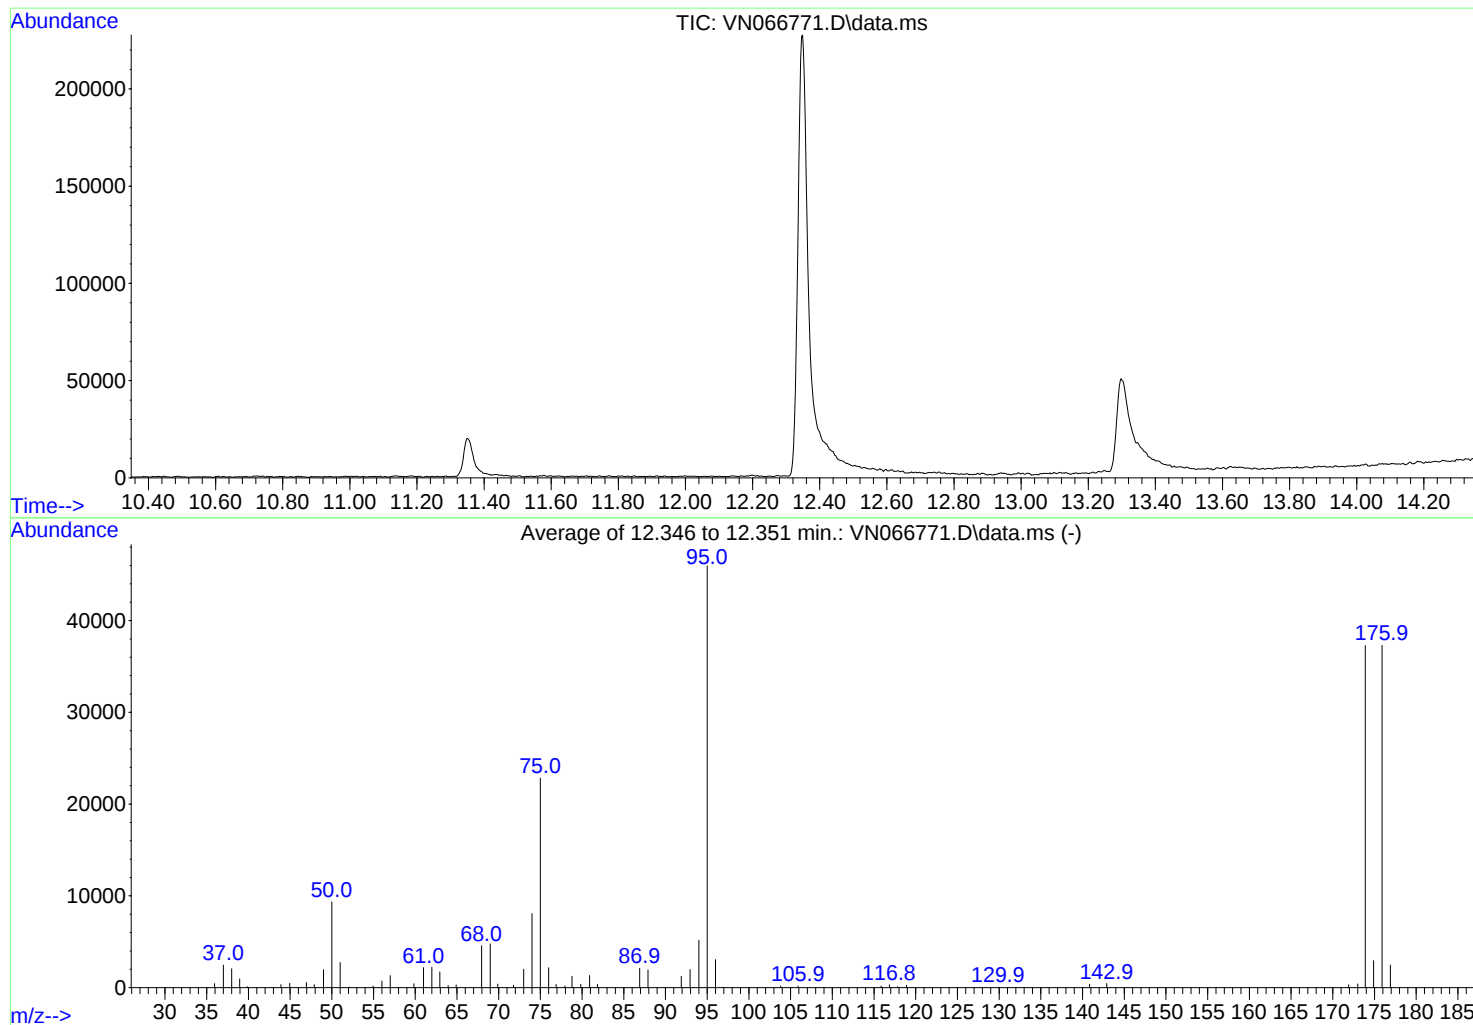

AutoFind: Scans 3961, 3962, 3963; Background Corrected with Scan 3945

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.3	9346	PASS
75	95	30	60	49.7	22837	PASS
95	95	100	100	100.0	45963	PASS
96	95	5	9	6.6	3054	PASS
173	174	0.00	2	1.1	404	PASS
174	95	50	100	81.1	37285	PASS
175	174	5	9	7.9	2949	PASS
176	174	95	101	100.0	37296	PASS
177	176	5	9	6.6	2454	PASS