

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN042722\
 Data File : VN072212.D
 Acq On : 27 Apr 2022 13:41
 Operator : JC\MD
 Sample : N2522-03
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 NWB-1766

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N042622W.M
 Title : SW846 8260

Signal : TIC: VN072212.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.687	277	289	325	rBV	3177571	8904708	100.00%	24.197%
2	4.287	382	391	401	rBV2	63473	189065	2.12%	0.514%
3	4.569	428	439	463	rBV	171054	572277	6.43%	1.555%
4	7.645	953	962	979	rBV	67619	192640	2.16%	0.523%
5	8.016	1014	1025	1030	rBV	229023	545864	6.13%	1.483%
6	8.081	1030	1036	1053	rVB	406398	955624	10.73%	2.597%
7	8.433	1085	1096	1109	rBV2	295922	862613	9.69%	2.344%
8	8.963	1177	1186	1196	rBV	658333	1345784	15.11%	3.657%
9	10.327	1408	1418	1426	rBV	98767	186252	2.09%	0.506%
10	10.439	1426	1437	1442	rVV	1059710	1966695	22.09%	5.344%
11	10.504	1442	1448	1465	rVB	765043	1453444	16.32%	3.949%
12	10.686	1471	1479	1498	rBV	339251	755256	8.48%	2.052%
13	11.739	1650	1658	1670	rBV	1090855	1921208	21.58%	5.221%
14	11.945	1684	1693	1703	rBV2	243406	477566	5.36%	1.298%
15	12.274	1739	1749	1759	rBV	348438	573335	6.44%	1.558%
16	12.727	1818	1826	1837	rBV	866468	1449175	16.27%	3.938%
17	12.980	1862	1869	1872	rBV	150427	264262	2.97%	0.718%
18	13.010	1872	1874	1878	rVV	98822	139850	1.57%	0.380%
19	13.051	1878	1881	1888	rVB	130283	207324	2.33%	0.563%
20	13.215	1901	1909	1916	rBV	165729	273449	3.07%	0.743%
21	13.363	1928	1934	1942	rBV	260038	404816	4.55%	1.100%
22	13.668	1979	1986	1997	rVV2	979245	2142189	24.06%	5.821%
23	13.768	1997	2003	2009	rVV	81490	143581	1.61%	0.390%
24	13.868	2015	2020	2023	rVV3	282503	518149	5.82%	1.408%
25	13.904	2023	2026	2036	rVB2	202863	365771	4.11%	0.994%
26	14.063	2047	2053	2059	rBV	112196	179394	2.01%	0.487%
27	14.121	2059	2063	2066	rBV	85714	142587	1.60%	0.387%
28	14.151	2066	2068	2073	rVB	104047	140723	1.58%	0.382%
29	14.210	2073	2078	2084	rVB	215190	323547	3.63%	0.879%
30	14.274	2084	2089	2092	rBV2	54747	91571	1.03%	0.249%
31	14.321	2092	2097	2103	rVB2	216020	359234	4.03%	0.976%
32	14.457	2114	2120	2125	rBV2	102864	170480	1.91%	0.463%
33	14.533	2125	2133	2136	rVV	137852	243502	2.73%	0.662%
34	14.574	2136	2140	2144	rVV	246652	383454	4.31%	1.042%
35	14.615	2144	2147	2151	rVV	70321	105938	1.19%	0.288%
36	14.757	2162	2171	2174	rVV3	64818	128333	1.44%	0.349%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN042722\
Data File : VN072212.D
Acq On : 27 Apr 2022 13:41
Operator : JC\MD
Sample : N2522-03
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
NWB-1766

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N042622W.M
Title : SW846 8260

37	14.804	2174	2179	2184	rVV	237491	425696	4.78%	1.157%
38	14.845	2184	2186	2191	rVV	73118	102572	1.15%	0.279%
39	14.921	2191	2199	2206	rVV2	631851	1466829	16.47%	3.986%
40	14.974	2206	2208	2218	rVV3	49473	118067	1.33%	0.321%
41	15.080	2219	2226	2234	rVV	481249	849256	9.54%	2.308%
42	15.192	2234	2245	2248	rVV2	160929	427498	4.80%	1.162%
43	15.227	2249	2251	2256	rVV	127255	200491	2.25%	0.545%
44	15.309	2257	2265	2272	rVB3	198958	488953	5.49%	1.329%
45	15.498	2293	2297	2302	rVV	68899	124141	1.39%	0.337%
46	15.557	2302	2307	2312	rVV	154298	284717	3.20%	0.774%
47	15.639	2312	2321	2339	rVB6	136561	595163	6.68%	1.617%
48	15.798	2339	2348	2355	rBV	130569	262621	2.95%	0.714%
49	15.974	2367	2378	2379	rBV4	117569	216575	2.43%	0.589%
50	16.009	2380	2384	2395	rVV	341375	728463	8.18%	1.979%
51	16.180	2406	2413	2429	rVB3	102586	312542	3.51%	0.849%
52	16.339	2429	2440	2451	rBV2	264570	615501	6.91%	1.673%
53	16.539	2461	2474	2481	rBV2	94671	256674	2.88%	0.697%
54	16.615	2481	2487	2501	rVB6	85648	245638	2.76%	0.667%




Sum of corrected areas: 36801057

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN042722\
Data File : VN072212.D
Acq On : 27 Apr 2022 13:41
Operator : JC\MD
Sample : N2522-03
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
NWB-1766

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N042622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

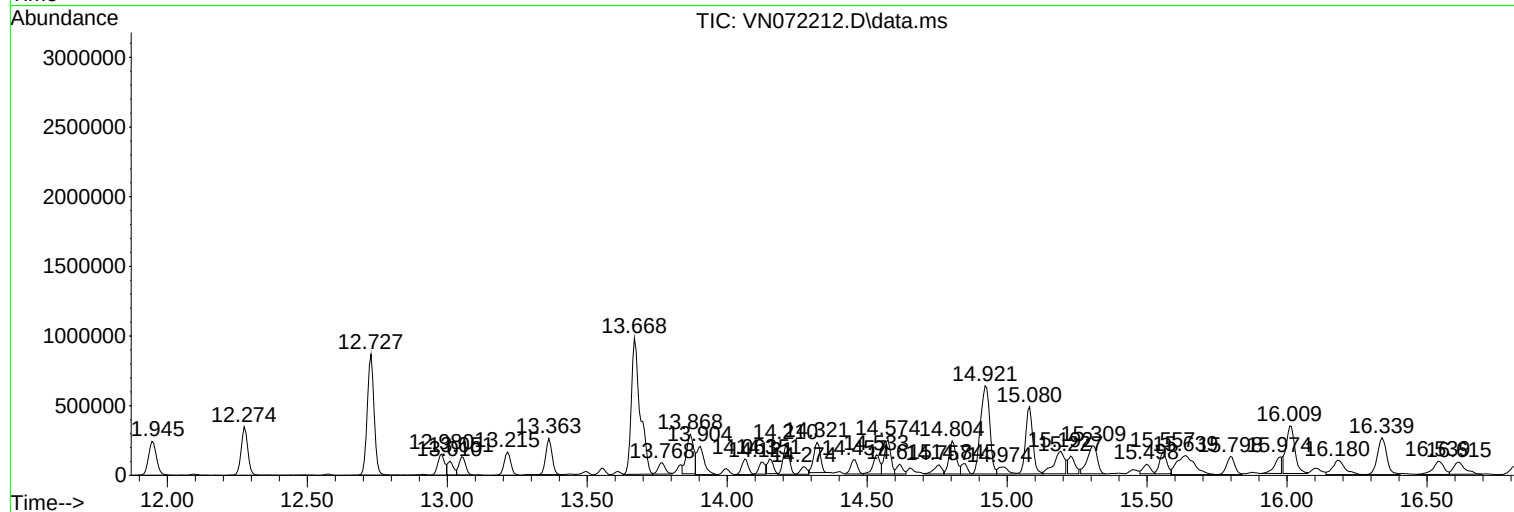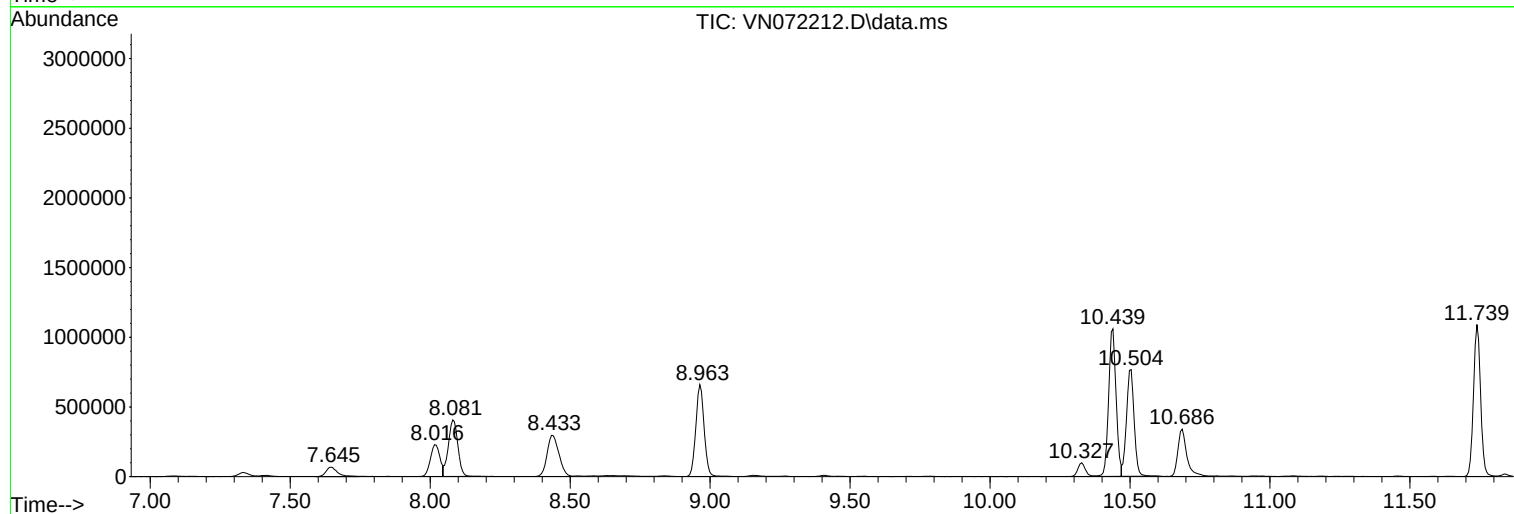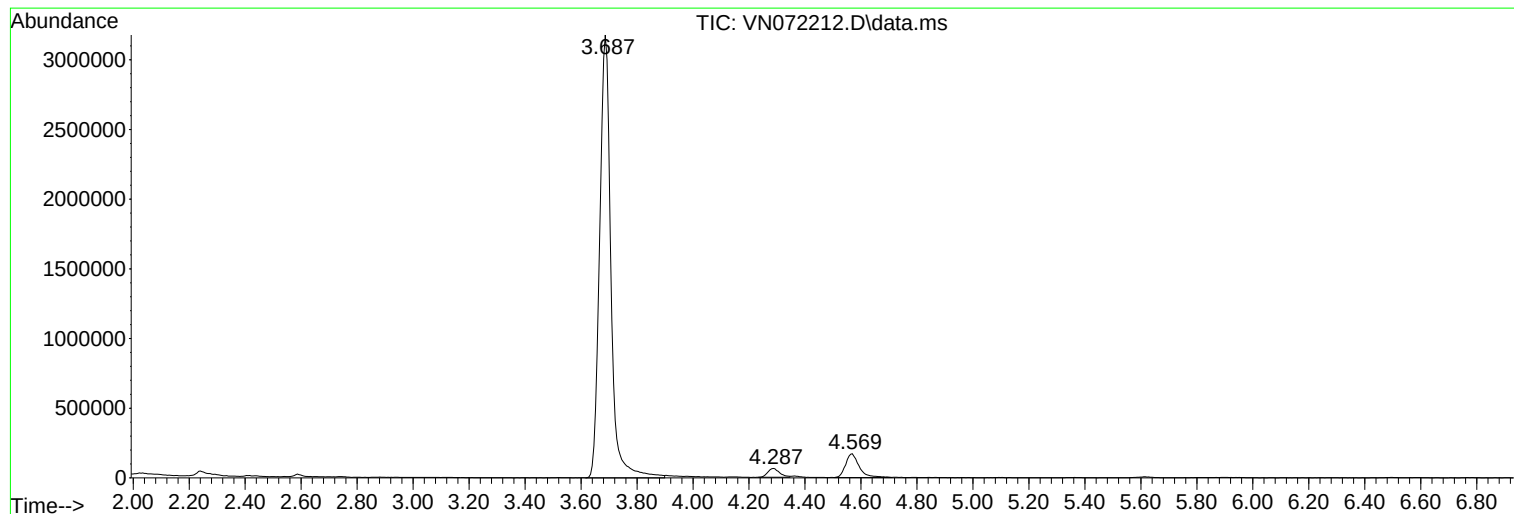

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN042722\
Data File : VN072212.D
Acq On : 27 Apr 2022 13:41
Operator : JC\MD
Sample : N2522-03
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
NWB-1766

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N042622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN042722\
Data File : VN072212.D
Acq On : 27 Apr 2022 13:41
Operator : JC\MD
Sample : N2522-03
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
NWB-1766

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N042622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
