
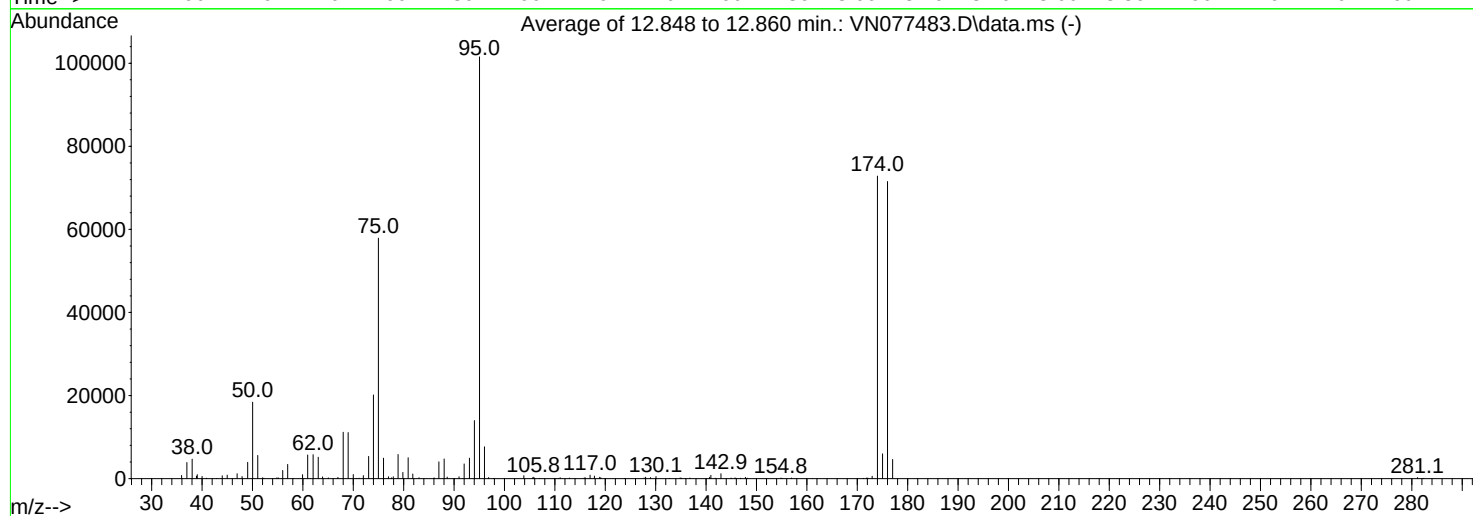


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN042723\
Data File : VN077483.D
Acq On : 27 Apr 2023 08:35
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N042423W.M
Title : SW846 8260
Last Update : Tue Apr 25 02:50:59 2023

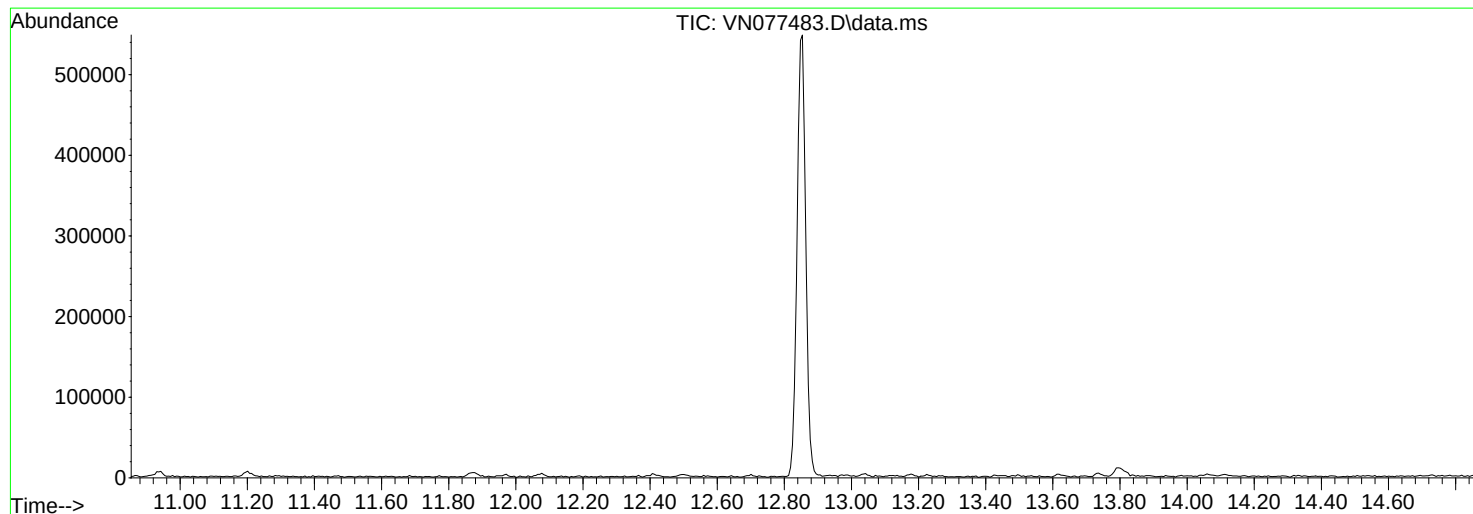

AutoFind: Scans 1855, 1856, 1857; Background Corrected with Scan 1846

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.1	18424	PASS
75	95	30	60	57.0	57896	PASS
95	95	100	100	100.0	101531	PASS
96	95	5	9	7.5	7659	PASS
173	174	0.00	2	0.8	563	PASS
174	95	50	100	71.7	72824	PASS
175	174	5	9	8.2	5990	PASS
176	174	95	101	98.2	71517	PASS
177	176	5	9	6.4	4605	PASS

Average of 12.848 to 12.860 min.: VN077483.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	782	46.95	1197	58.10	54	70.60	6
37.00	3911	47.95	492	59.95	964	71.15	13
38.05	4717	49.05	3933	60.95	5703	72.00	72
38.90	617	50.05	18424	62.05	5768	73.05	536
39.05	967	51.05	5577	63.05	5176	74.00	20131
40.00	551	52.05	246	63.90	425	75.00	57896
40.90	109	52.30	82	65.05	185	76.00	4940
42.90	54	54.80	163	66.95	313	77.00	482
44.00	703	55.10	221	68.00	11184	77.60	191
45.00	841	56.00	1962	69.00	11105	77.95	450
46.00	53	57.00	3444	70.00	1009	78.90	5822

Average of 12.848 to 12.860 min.: VN077483.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
79.85	1493	94.05	13986	110.70	53	128.00	333
80.90	5062	95.05	101531	111.05	226	129.00	267
81.80	1109	96.05	7659	112.90	143	130.05	485
83.05	225	96.85	265	115.80	173	132.70	67
86.05	188	97.80	52	116.00	250	134.85	176
87.00	4052	103.85	723	117.00	839	135.10	107
88.05	4737	105.60	227	117.85	625	135.90	51
88.65	374	105.80	362	118.90	334	136.80	175
91.00	462	106.00	123	119.10	240	140.70	345
92.00	3530	107.00	66	123.80	58	140.95	809
93.05	4942	109.90	63	127.70	147	141.80	109

Average of 12.848 to 12.860 min.: VN077483.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
142.95	1205	161.10	59				
144.95	154	171.20	67				
145.75	204	171.80	150				
146.00	93	172.10	142				
146.85	123	172.95	563				
147.80	329	174.00	72824				
148.20	123	175.00	5990				
151.90	51	176.00	71517				
154.85	155	177.00	4605				
155.10	81	281.15	256				
156.95	151	282.30	92				

Instrument :

MSVOA_N

ClientSampleId :

BFB