


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN042821\
Data File : VN066799.D
Acq On : 28 Apr 2021 8:55
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N042721W.M
Title : SW846 8260
Last Update : Tue Apr 27 16:02:50 2021

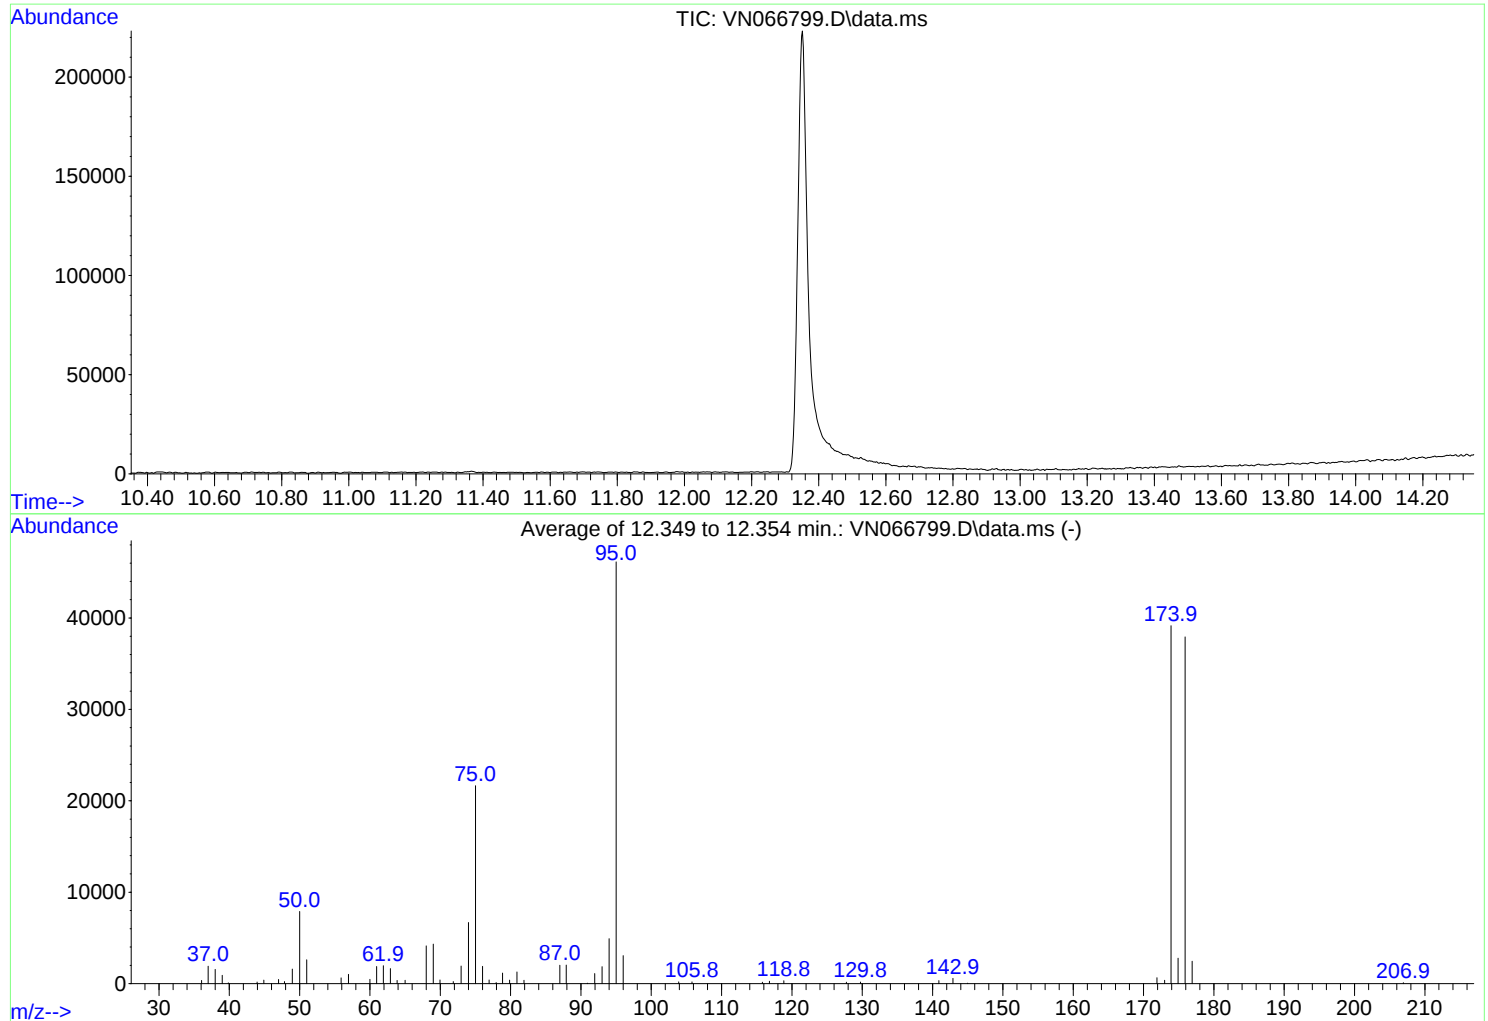

AutoFind: Scans 3962, 3963, 3964; Background Corrected with Scan 3946

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.1	7901	PASS
75	95	30	60	46.9	21659	PASS
95	95	100	100	100.0	46139	PASS
96	95	5	9	6.6	3063	PASS
173	174	0.00	2	0.9	365	PASS
174	95	50	100	84.9	39152	PASS
175	174	5	9	7.1	2779	PASS
176	174	95	101	96.9	37928	PASS
177	176	5	9	6.5	2448	PASS