


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN042823\
Data File : VN077494.D
Acq On : 28 Apr 2023 09:24
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N042823W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Fri Apr 28 16:20:59 2023

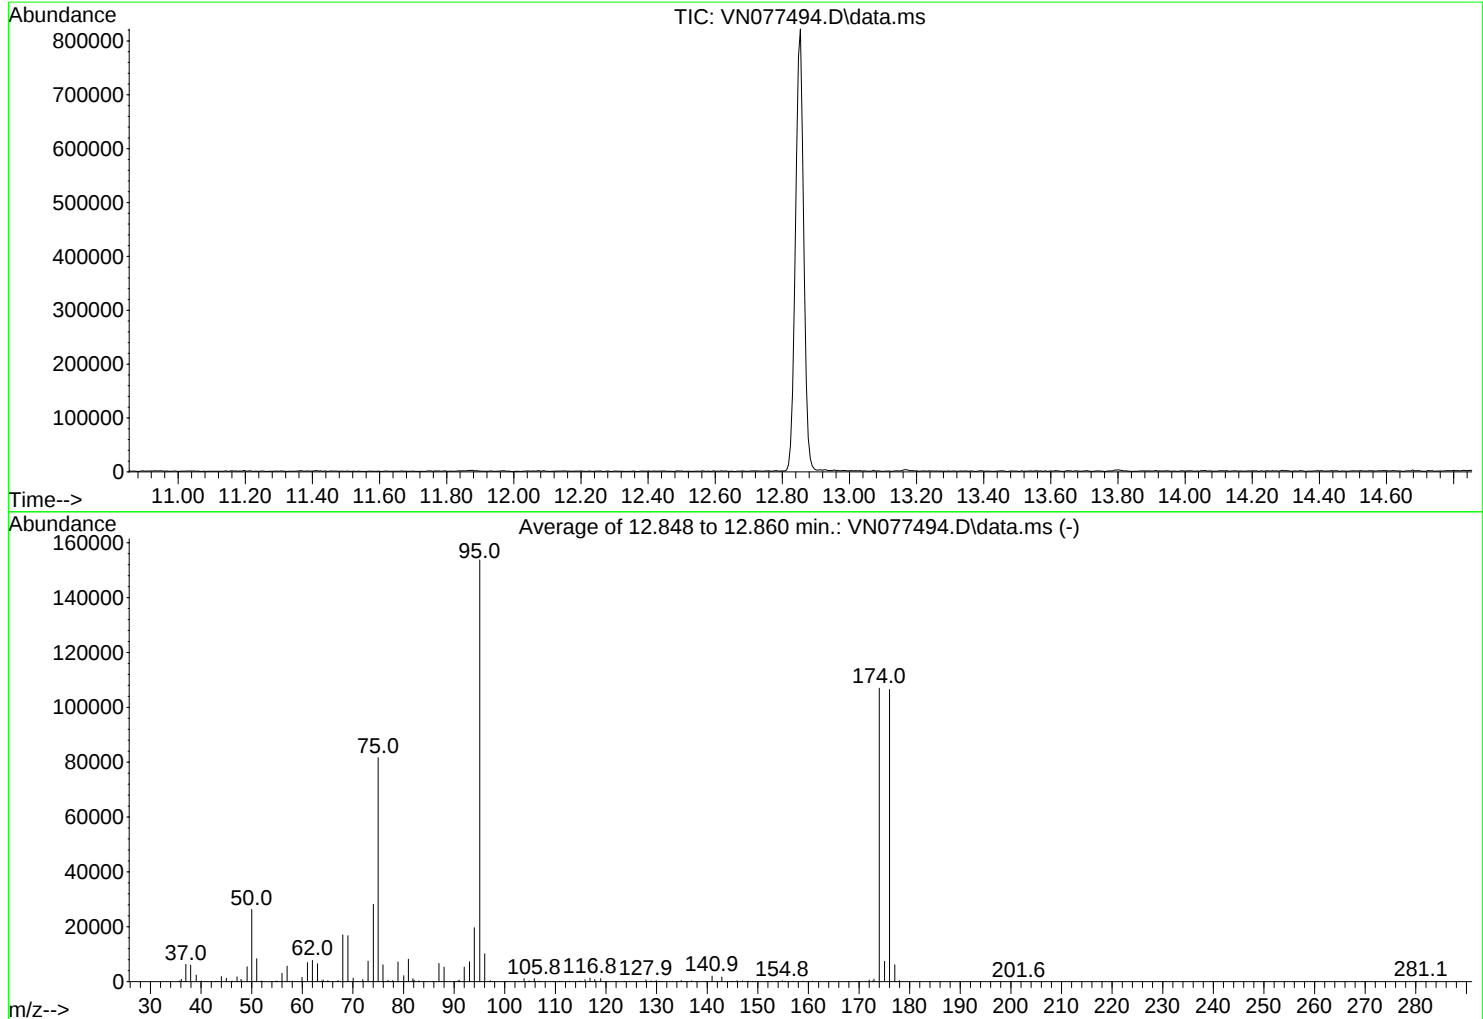

AutoFind: Scans 1855, 1856, 1857; Background Corrected with Scan 1846

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.1	26309	PASS
75	95	30	60	53.1	81661	PASS
95	95	100	100	100.0	153760	PASS
96	95	5	9	6.6	10137	PASS
173	174	0.00	2	0.9	928	PASS
174	95	50	100	69.6	106949	PASS
175	174	5	9	6.9	7413	PASS
176	174	95	101	99.6	106509	PASS
177	176	5	9	5.8	6129	PASS