
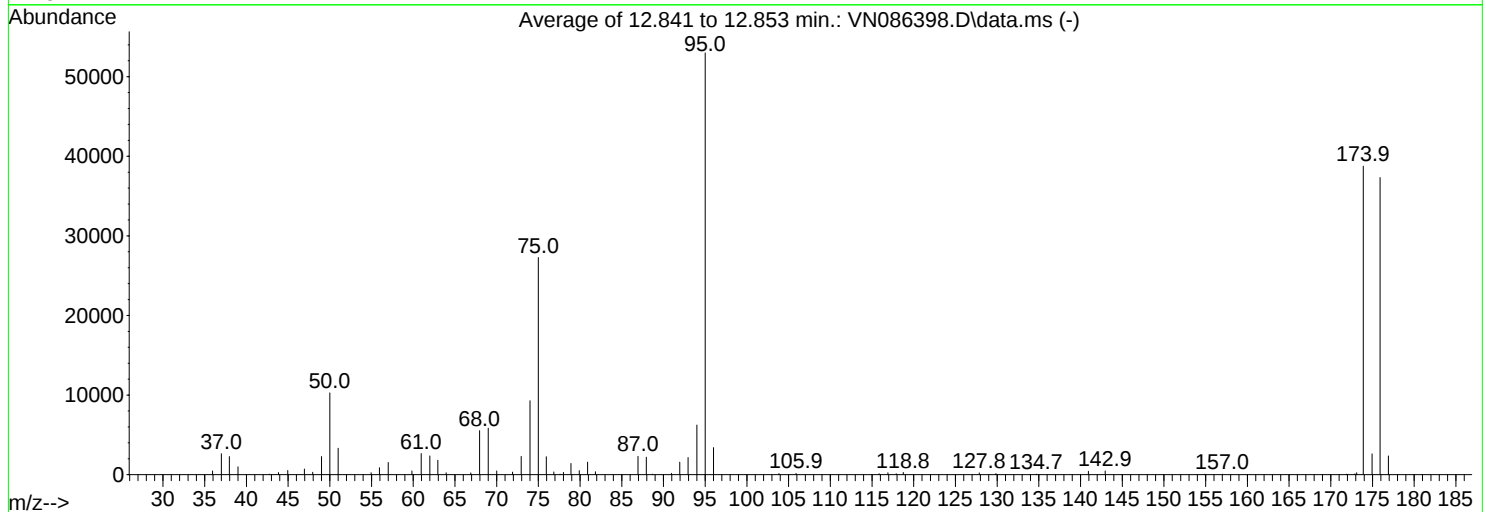


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN042825\
Data File : VN086398.D
Acq On : 28 Apr 2025 09:25
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N041525W.M
Title : SW846 8260
Last Update : Wed Apr 16 04:19:23 2025

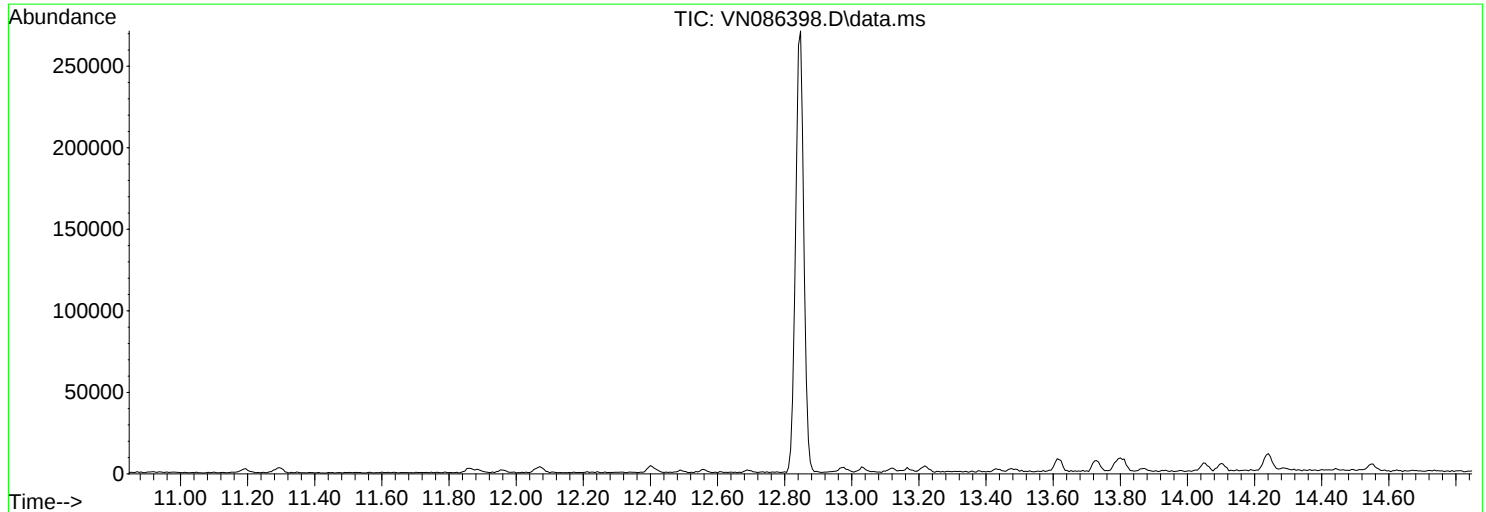

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1842

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.4	10269	PASS
75	95	30	60	51.5	27275	PASS
95	95	100	100	100.0	52992	PASS
96	95	5	9	6.4	3392	PASS
173	174	0.00	2	0.6	246	PASS
174	95	50	100	73.1	38749	PASS
175	174	5	9	6.7	2608	PASS
176	174	95	101	96.3	37325	PASS
177	176	5	9	6.3	2353	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	470	51.00	3312	69.00	5832	79.90	491
37.00	2639	54.95	233	70.00	465	80.90	156
37.95	2274	55.95	867	71.90	325	81.85	35
39.00	985	57.00	1534	72.95	2287	86.95	229
42.80	52	59.85	454	74.00	9293	87.95	2198
43.85	266	60.95	2648	75.00	27275	88.70	57
44.95	520	62.00	2359	75.95	2252	90.95	168
46.95	712	62.95	1802	76.85	348	91.95	1576
47.95	303	63.95	238	77.60	60	92.95	2146
49.00	2279	66.90	224	78.00	287	94.00	6241
50.00	10269	67.95	5536	78.90	1400	95.00	52992

Average of 12.841 to 12.853 min.: VN086398.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
96.00	3392	142.95	466				
103.85	139	154.90	60				
105.90	166	157.00	66				
115.85	122	171.90	55				
116.90	243	172.90	107				
117.90	114	173.10	246				
118.75	277	173.90	38749				
127.85	216	174.95	2608				
129.85	142	175.90	37325				
134.70	52	176.90	2353				
140.95	431						

Instrument :

MSVOA_N

ClientSampleId :

BFB