



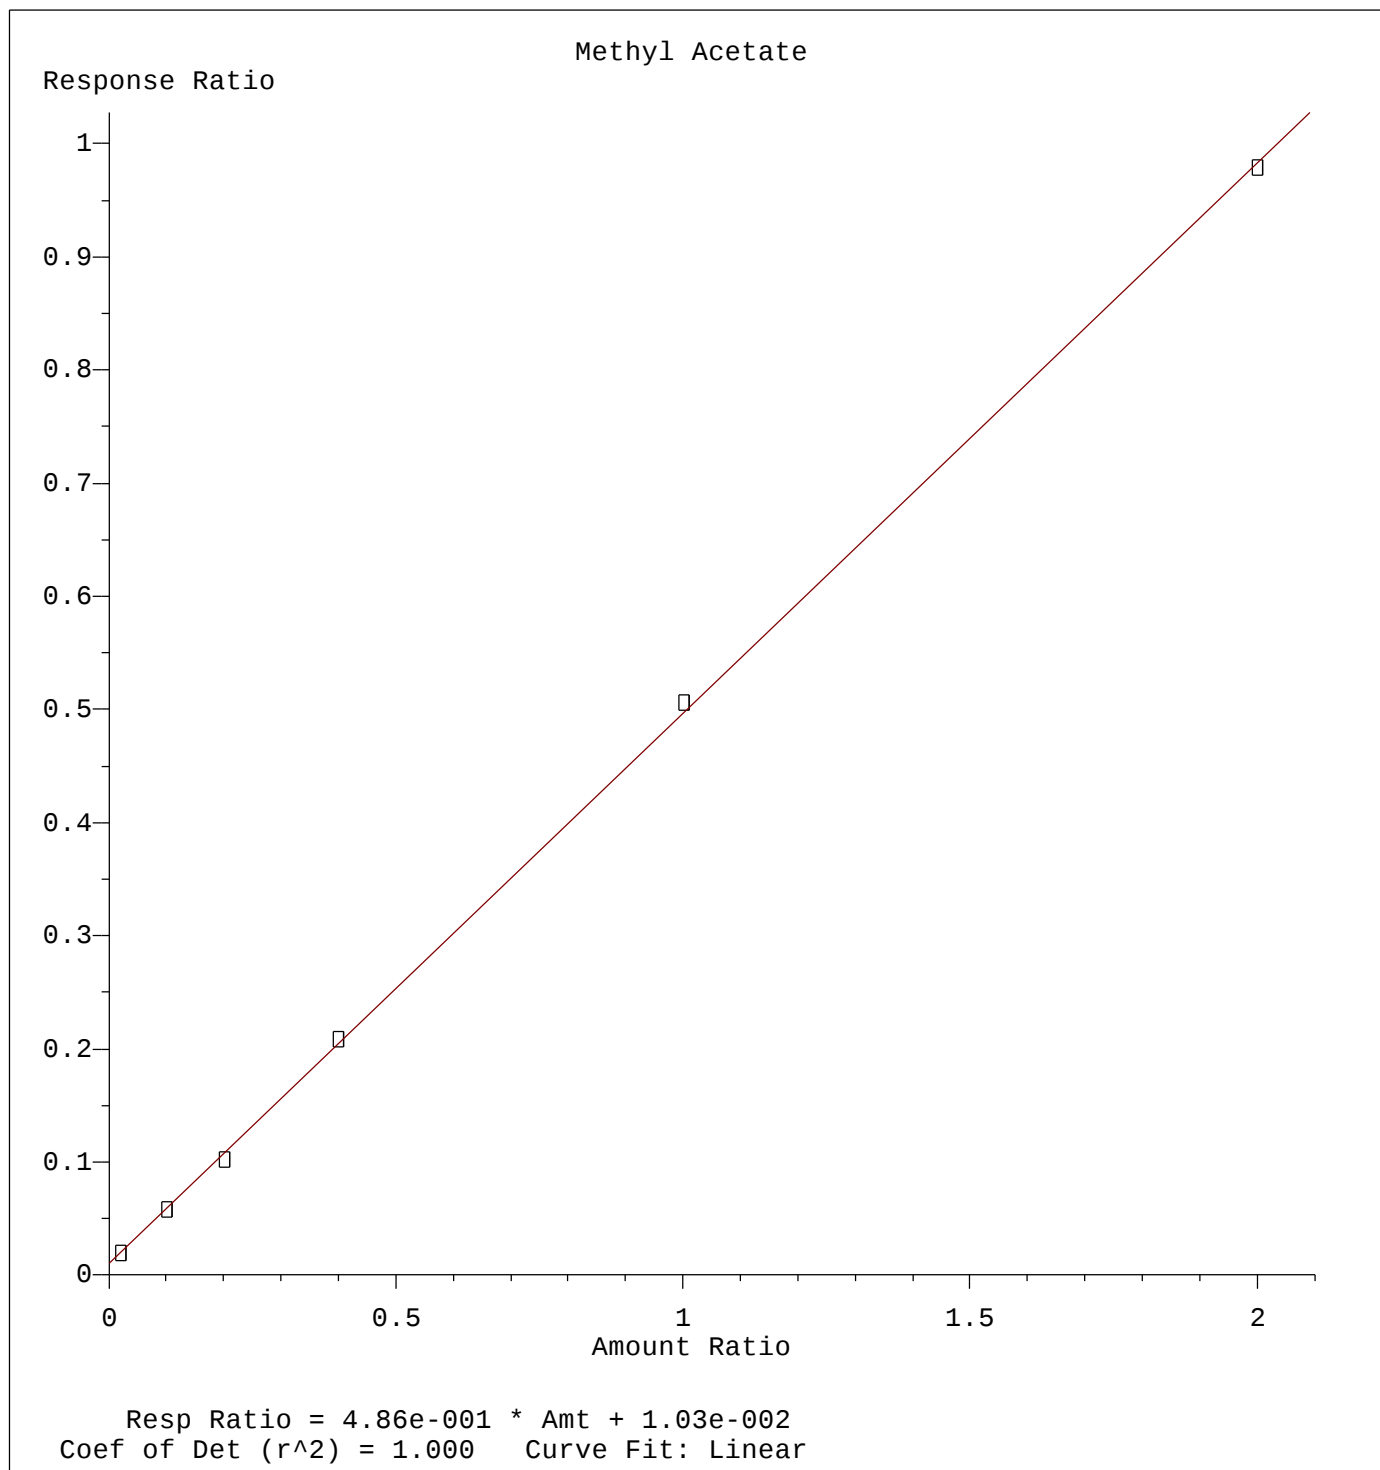


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N042919W.M
Calibration Table Last Updated: Tue Apr 30 04:20:38 2019

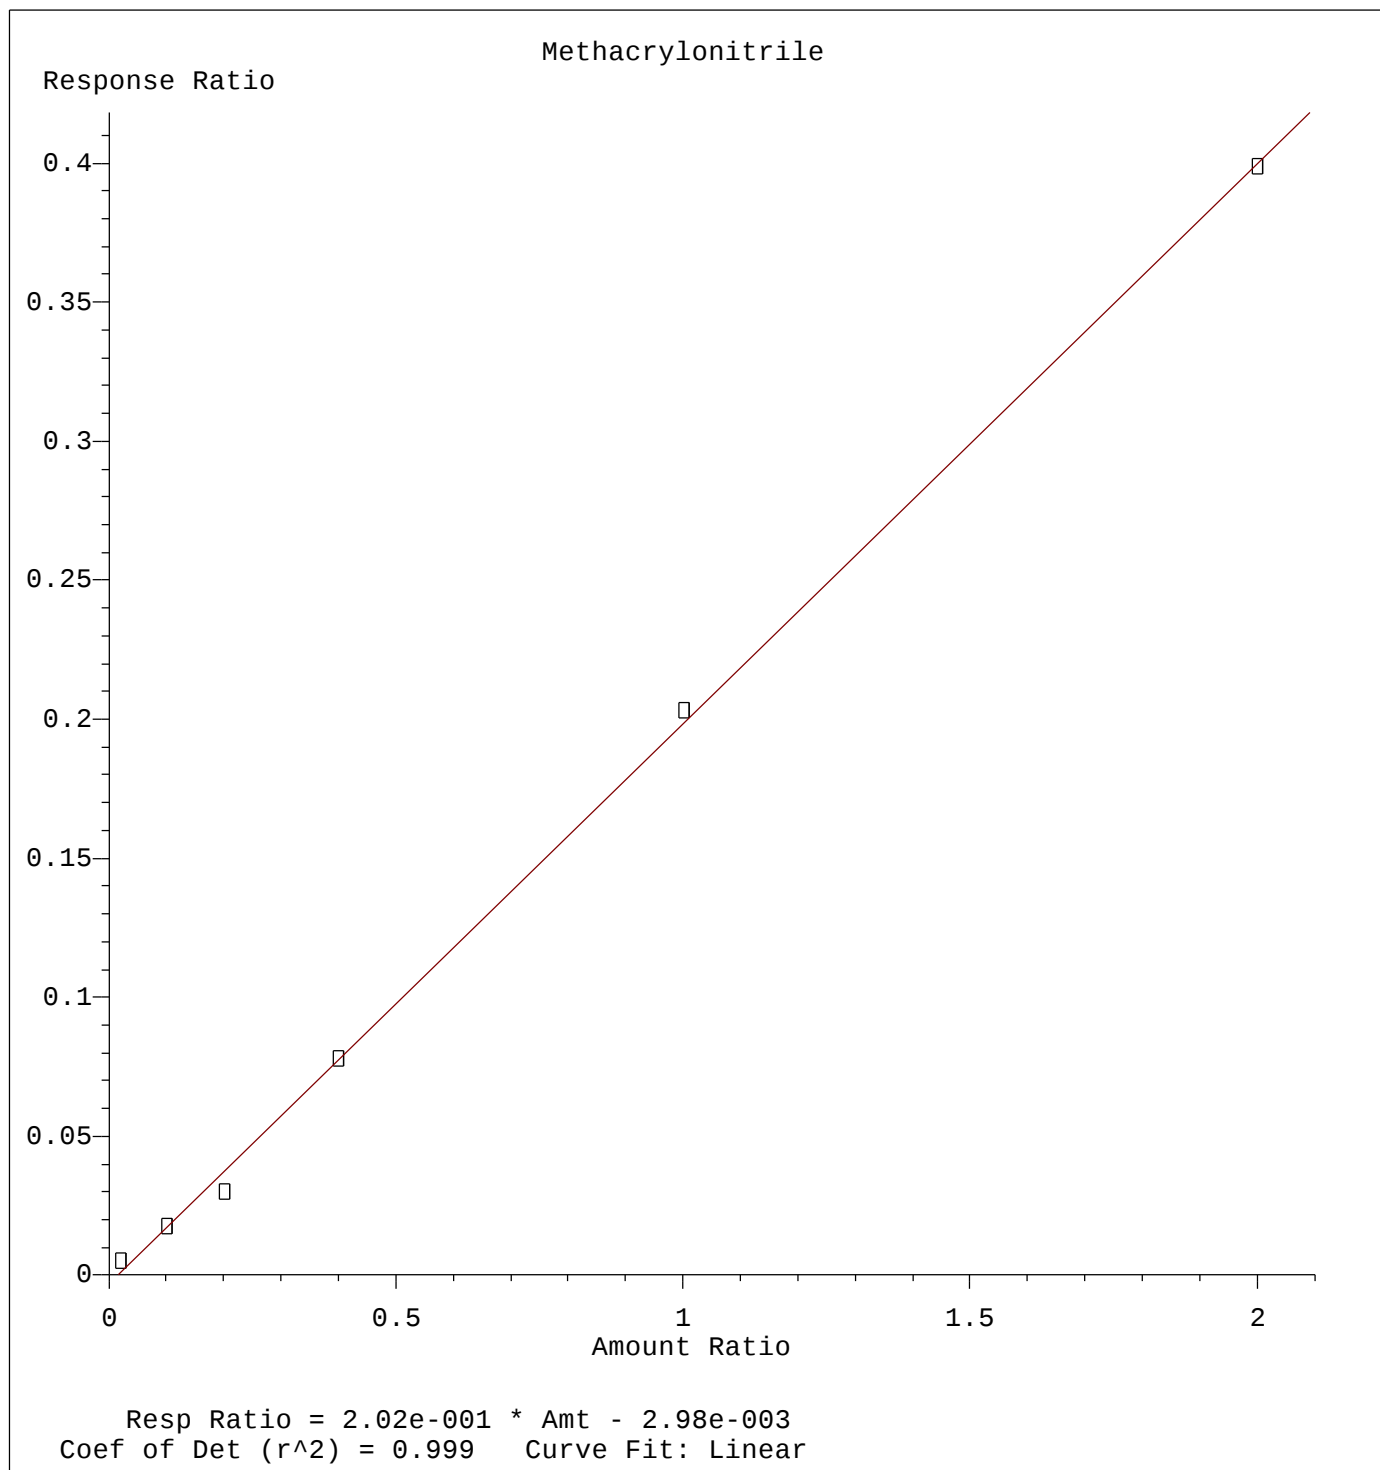

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N042919W.M
Calibration Table Last Updated: Tue Apr 30 04:20:38 2019


2-Chloroethyl Vinyl ether

Response Ratio

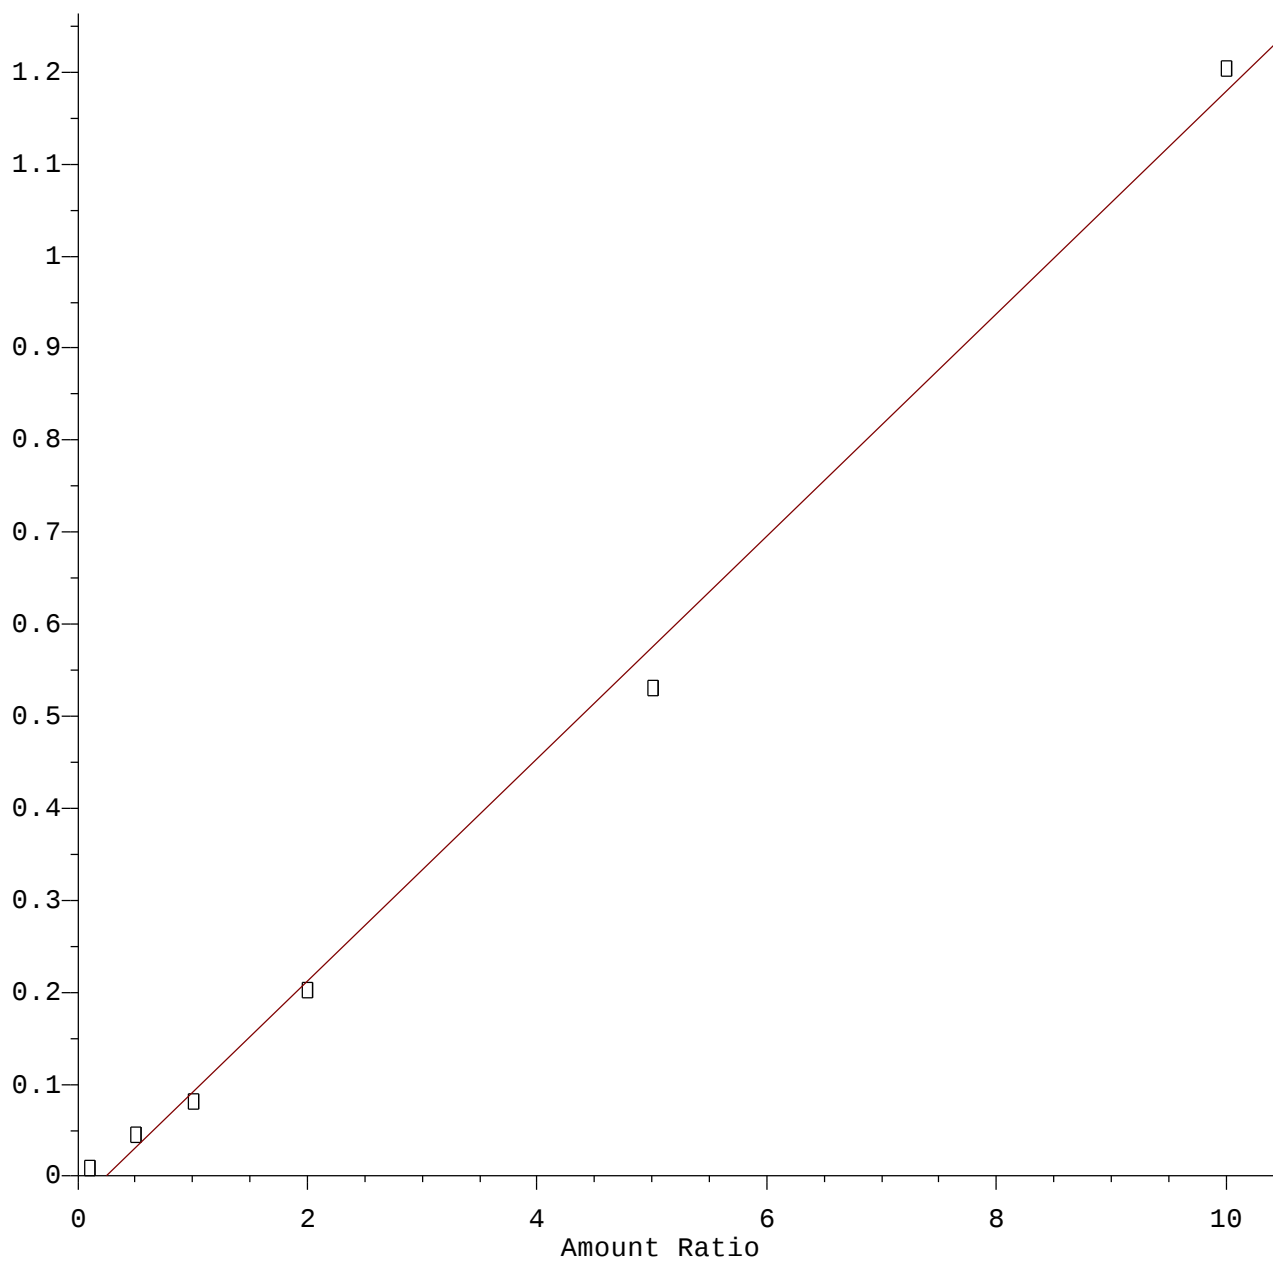

Resp Ratio = $1.21 \times 10^{-1} \times \text{Amt} - 3.00 \times 10^{-2}$
Coef of Det (r^2) = 0.996 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N042919W.M
Calibration Table Last Updated: Tue Apr 30 04:20:38 2019

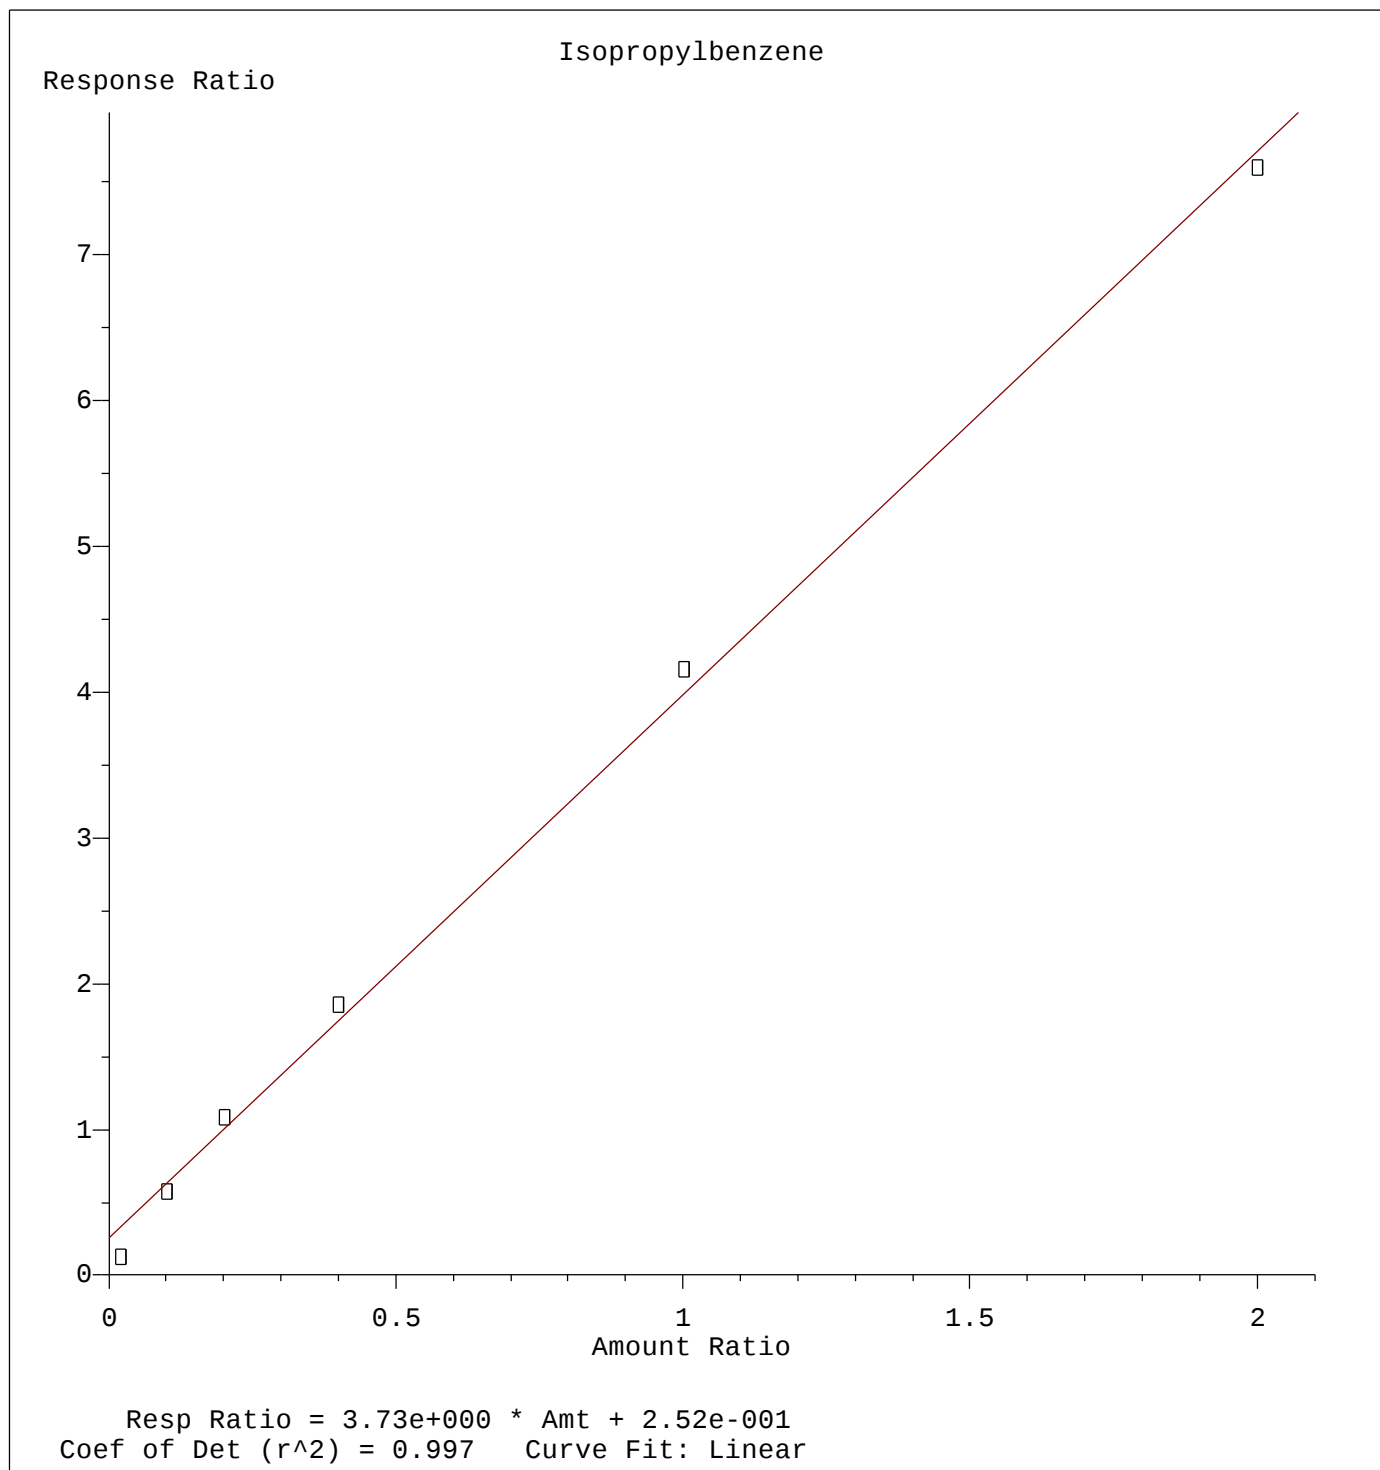

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N042919W.M
Calibration Table Last Updated: Tue Apr 30 04:20:38 2019

1,1,2,2-Tetrachloroethane

Response Ratio

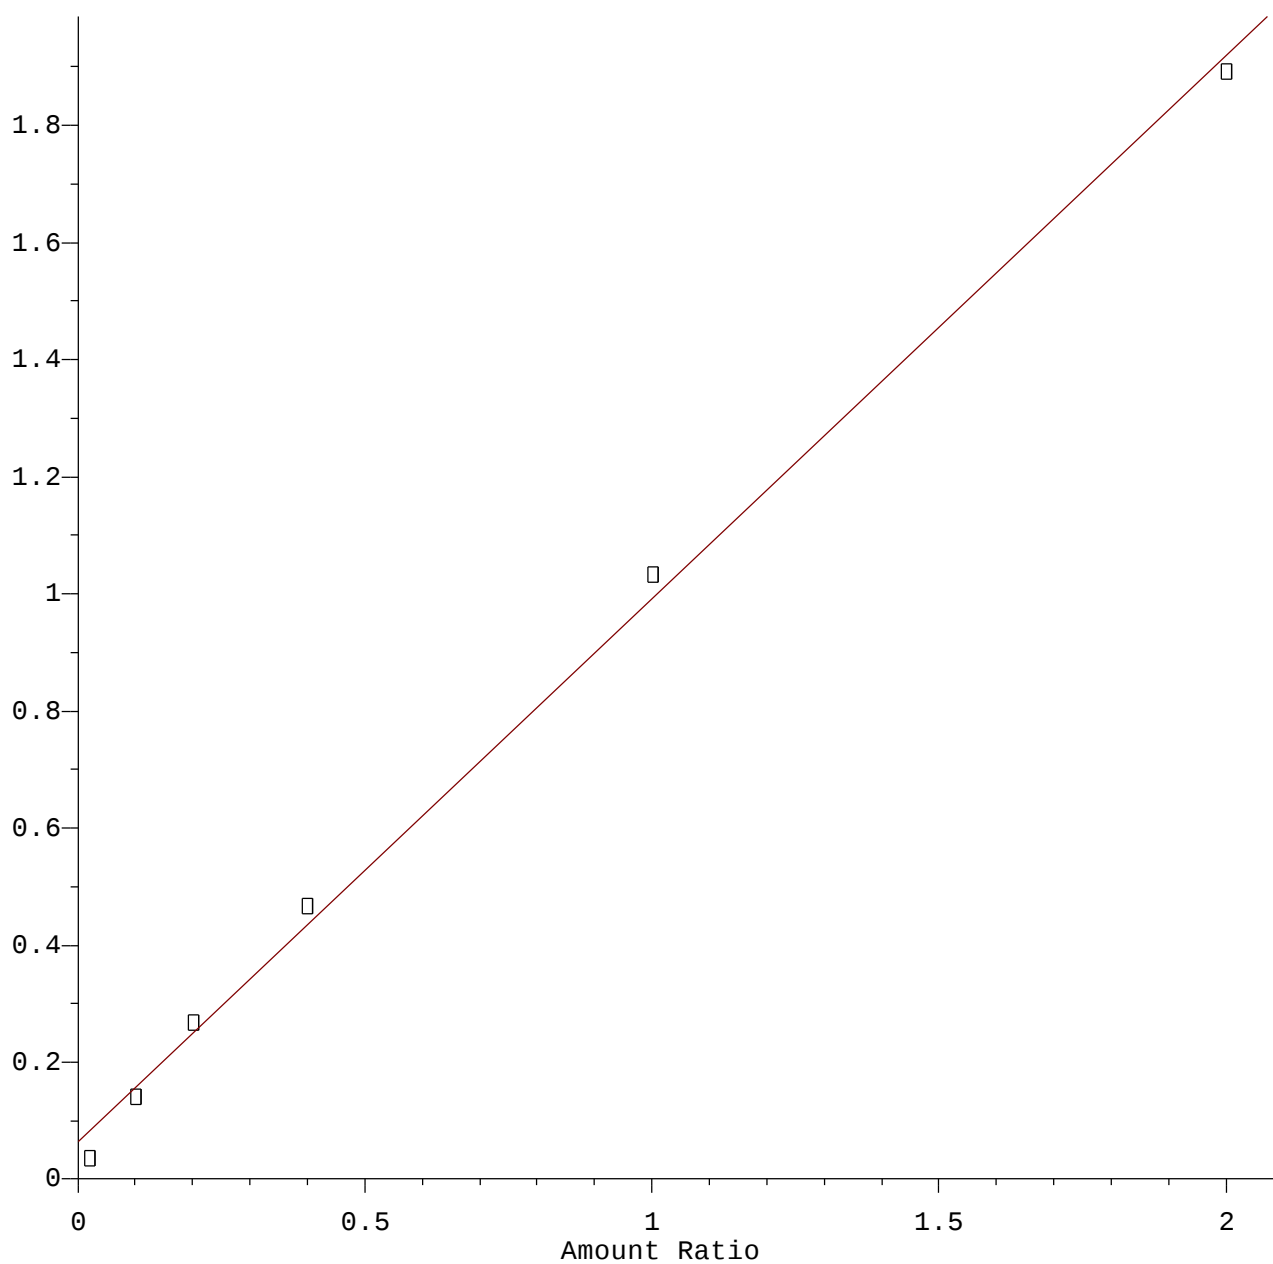


Resp Ratio = $9.28 \times 10^{-1} \times \text{Amt} + 6.30 \times 10^{-2}$
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N042919W.M
Calibration Table Last Updated: Tue Apr 30 04:20:38 2019


1,2,3-Trichloropropane

Response Ratio

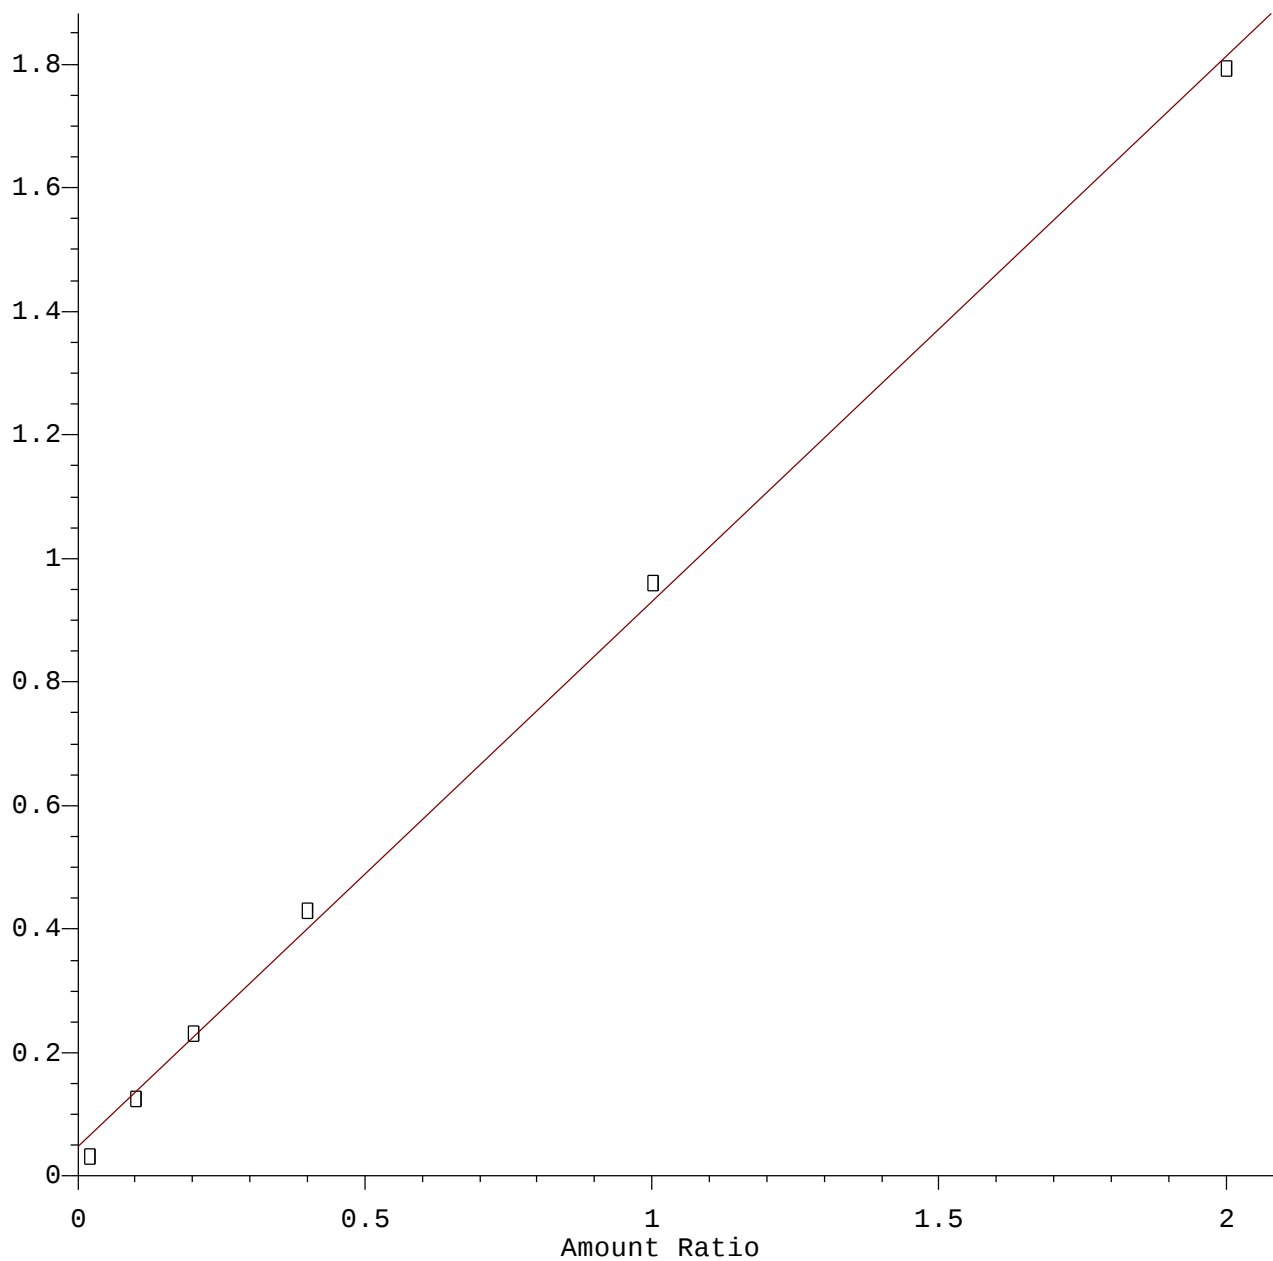


Resp Ratio = $8.83 \times 10^{-1} \times \text{Amt} + 4.68 \times 10^{-2}$
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N042919W.M
Calibration Table Last Updated: Tue Apr 30 04:20:38 2019

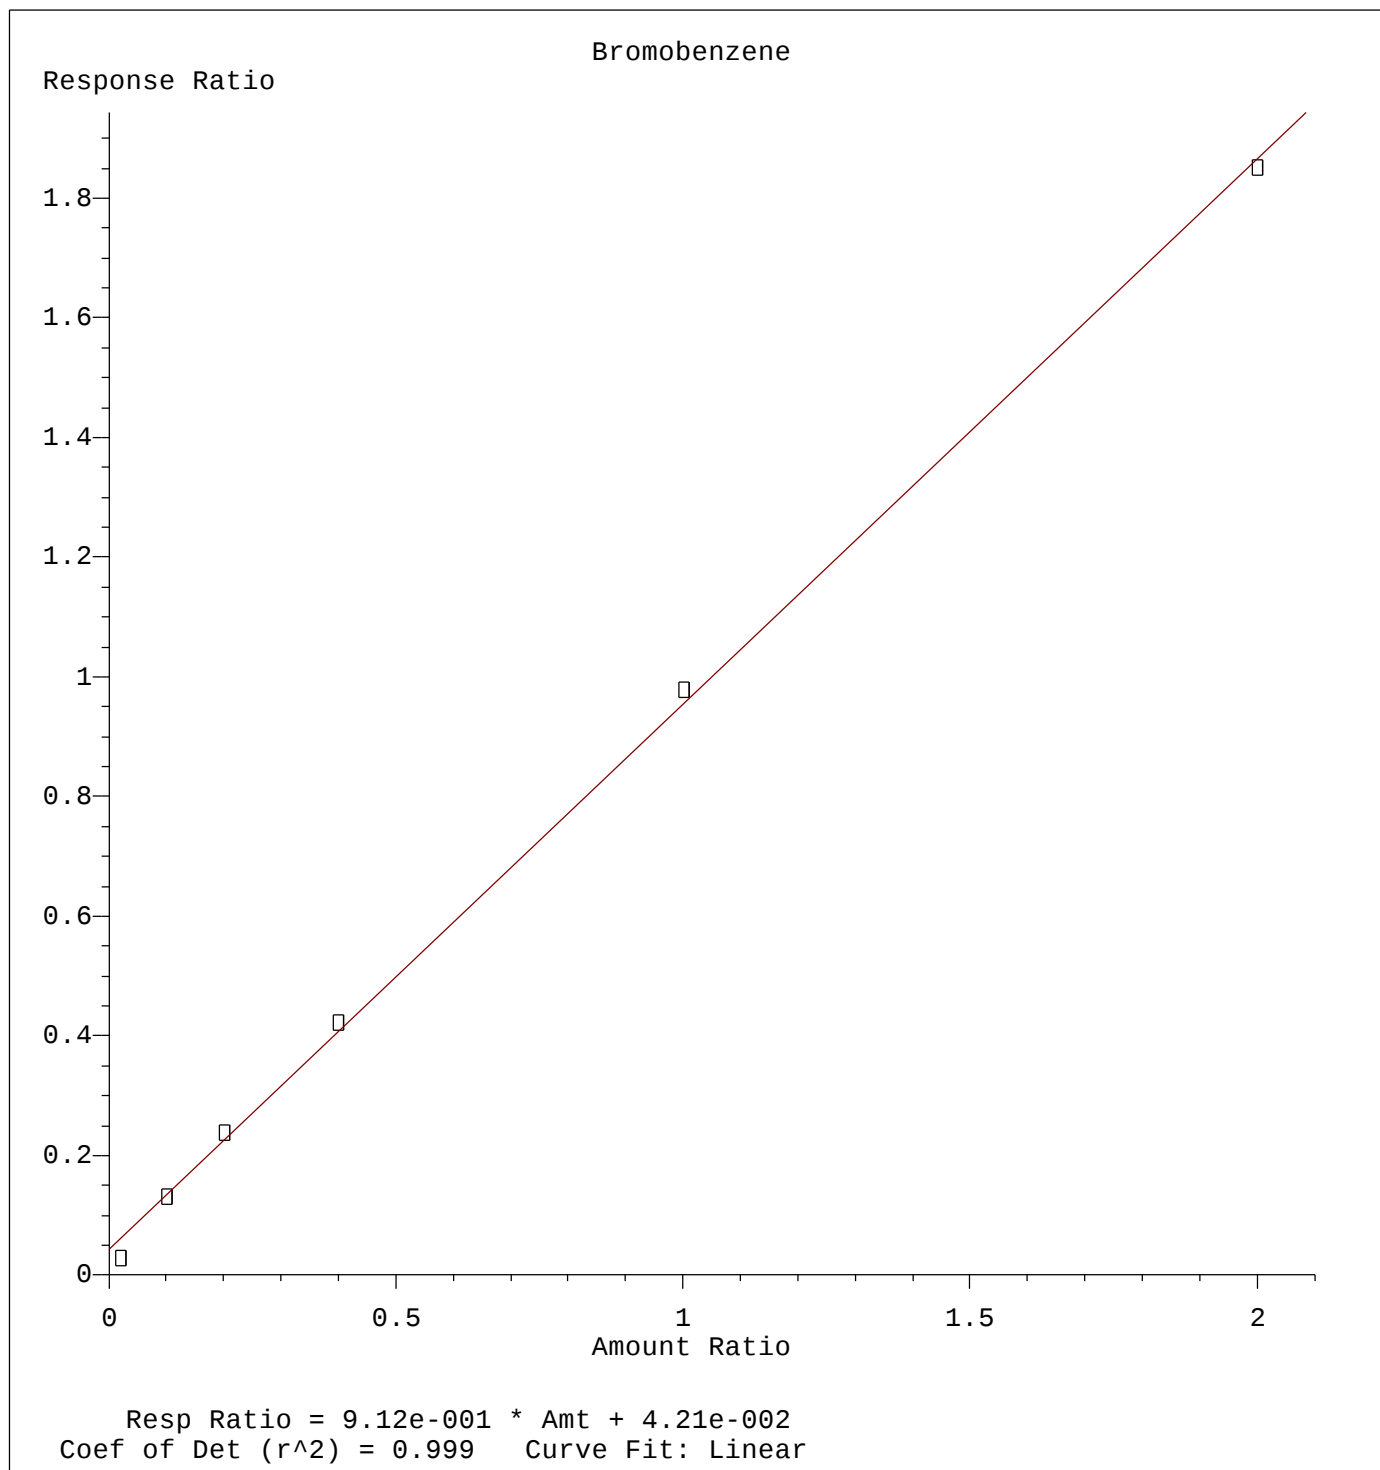


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N042919W.M
Calibration Table Last Updated: Tue Apr 30 04:20:38 2019

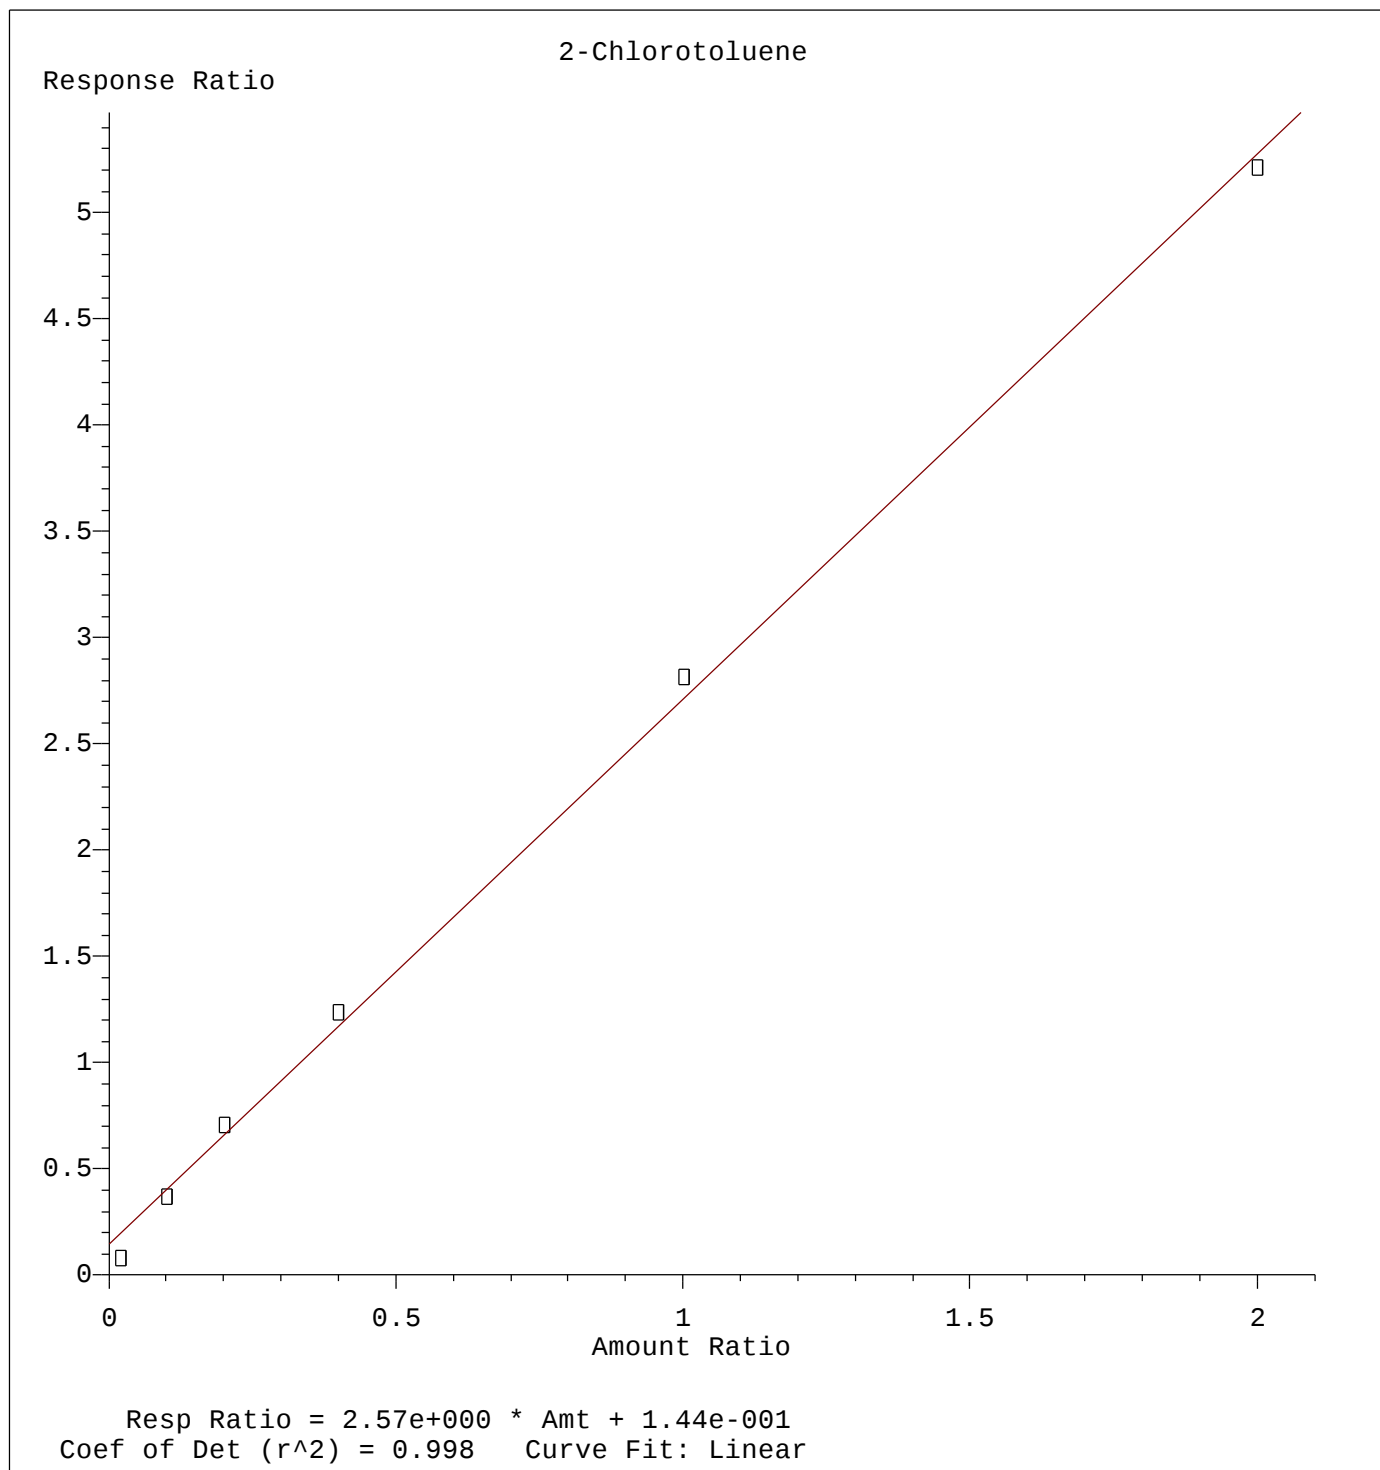

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N042919W.M
Calibration Table Last Updated: Tue Apr 30 04:20:38 2019


tert-Butylbenzene

Response Ratio

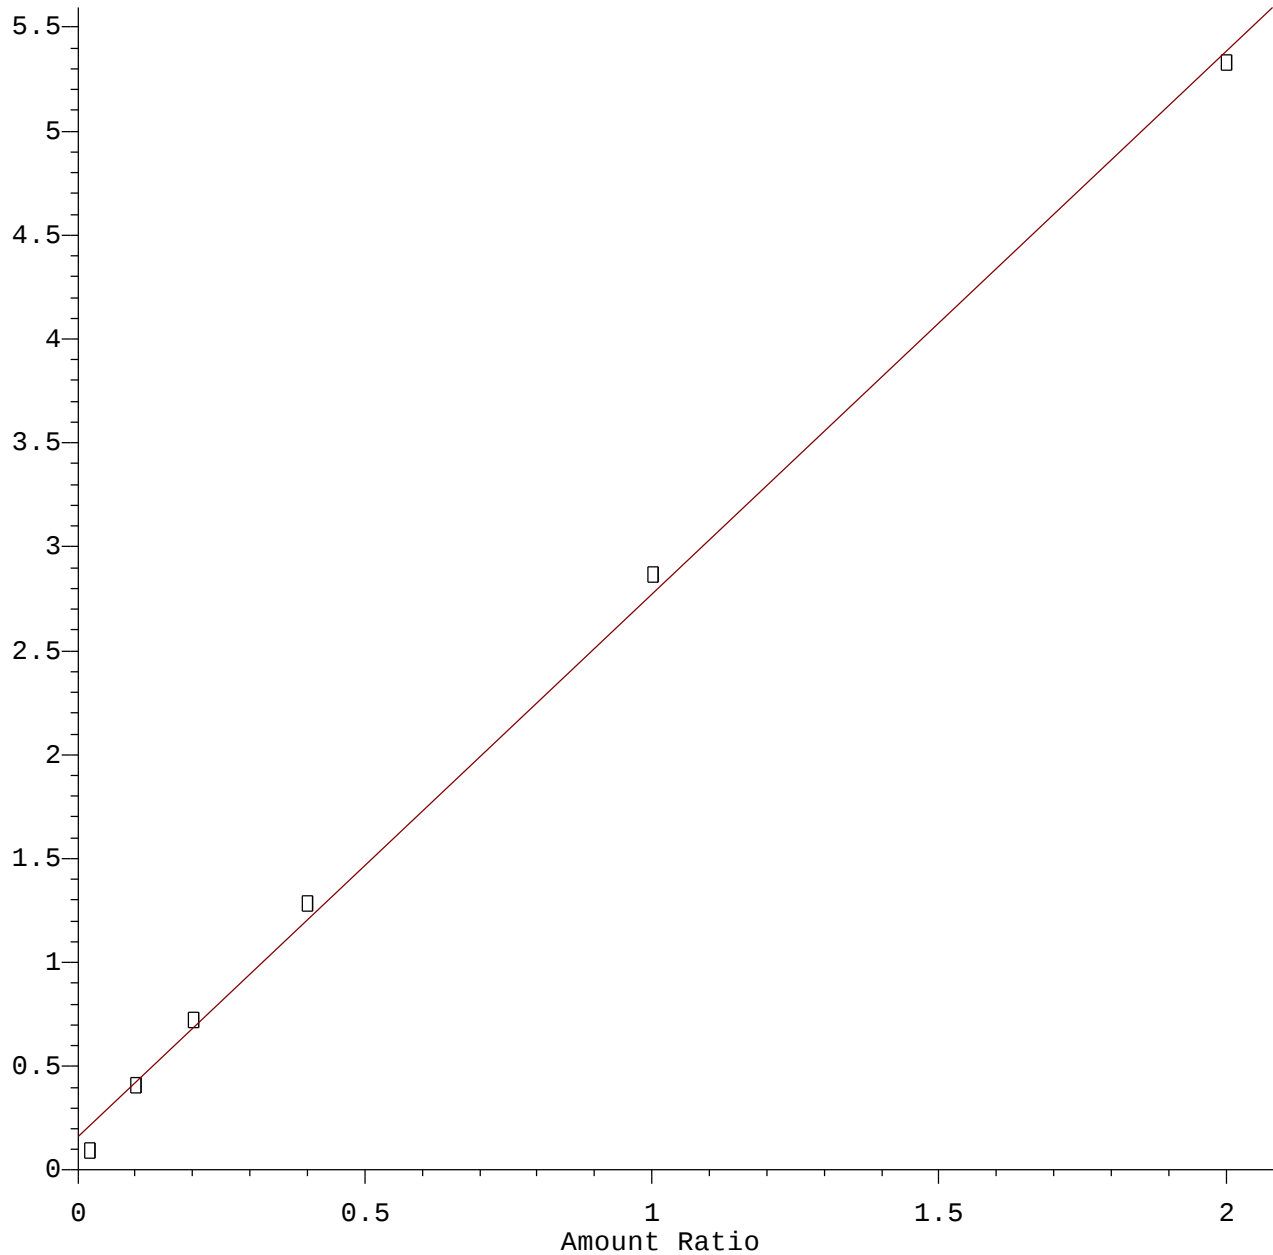

Resp Ratio = 2.61e+000 * Amt + 1.62e-001
Coef of Det (r^2) = 0.998 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N042919W.M
Calibration Table Last Updated: Tue Apr 30 04:20:38 2019

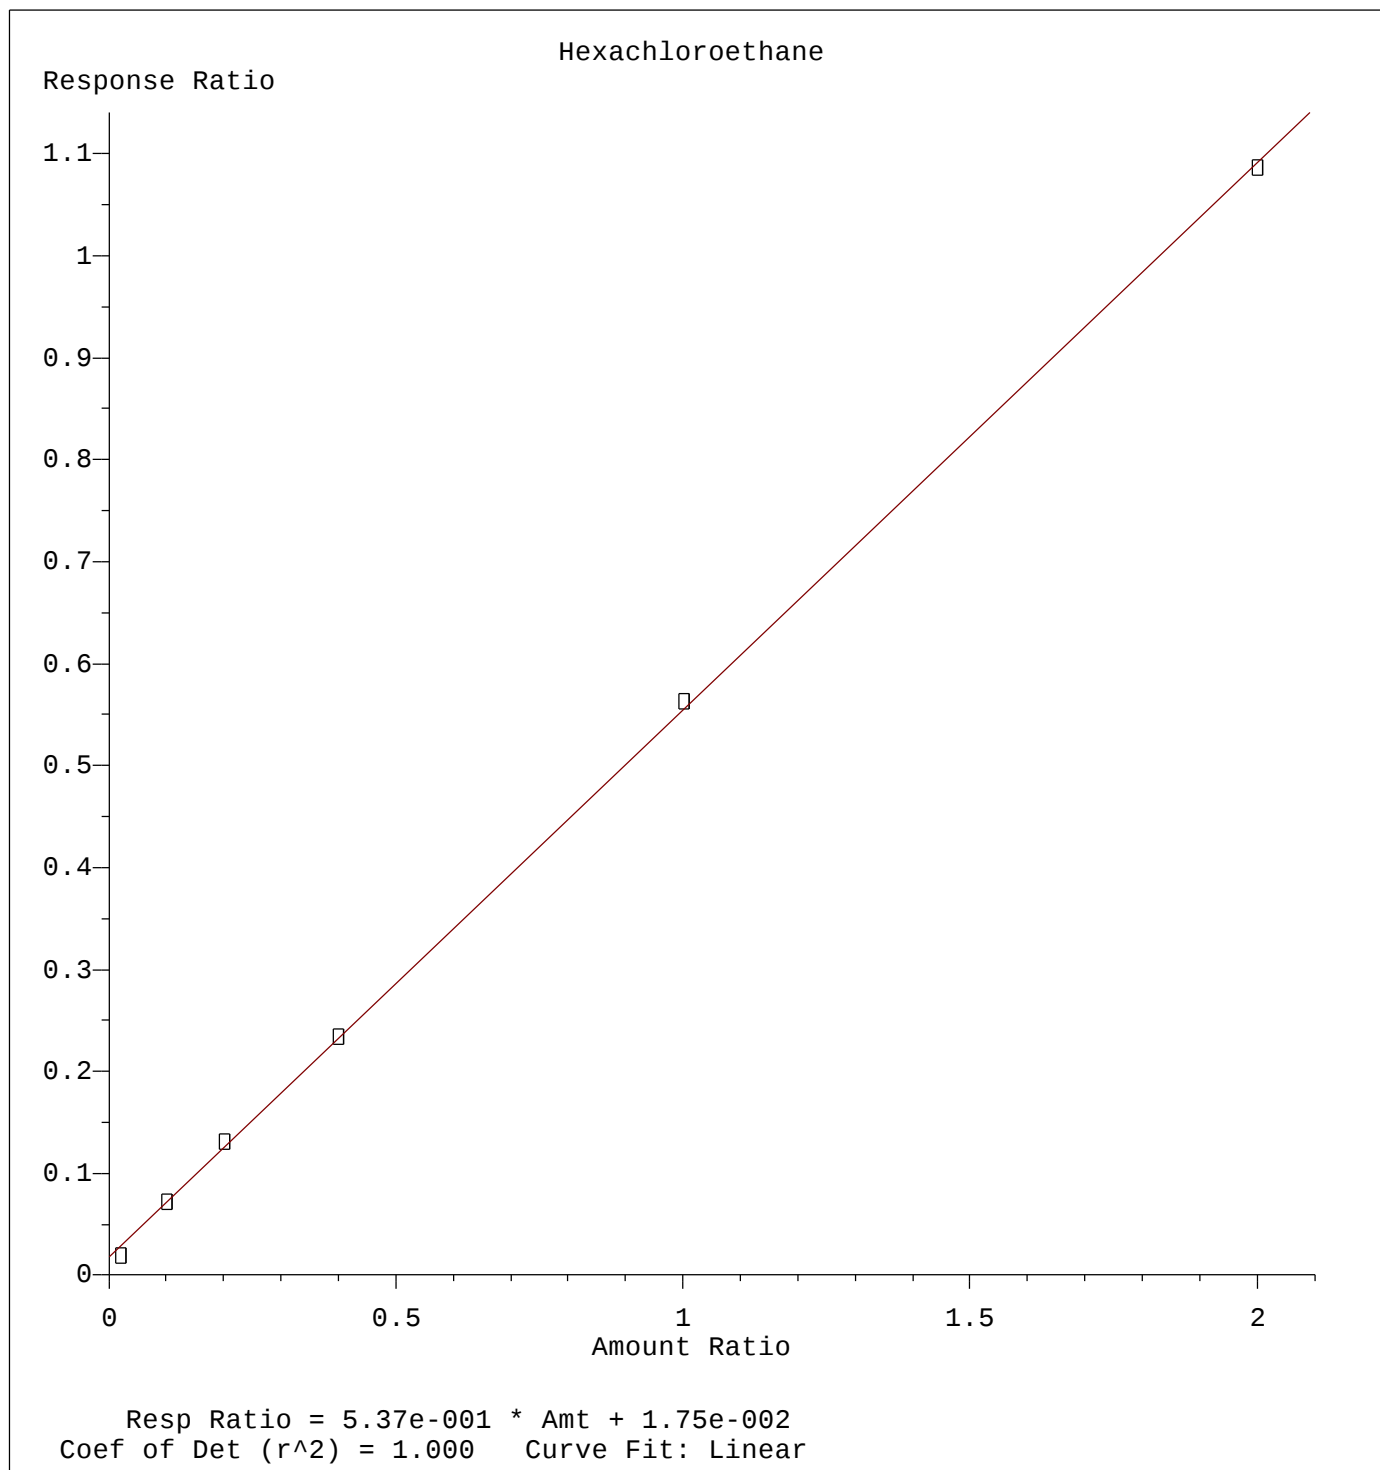

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N042919W.M
Calibration Table Last Updated: Tue Apr 30 04:20:38 2019


1,2,4-Trichlorobenzene

Response Ratio

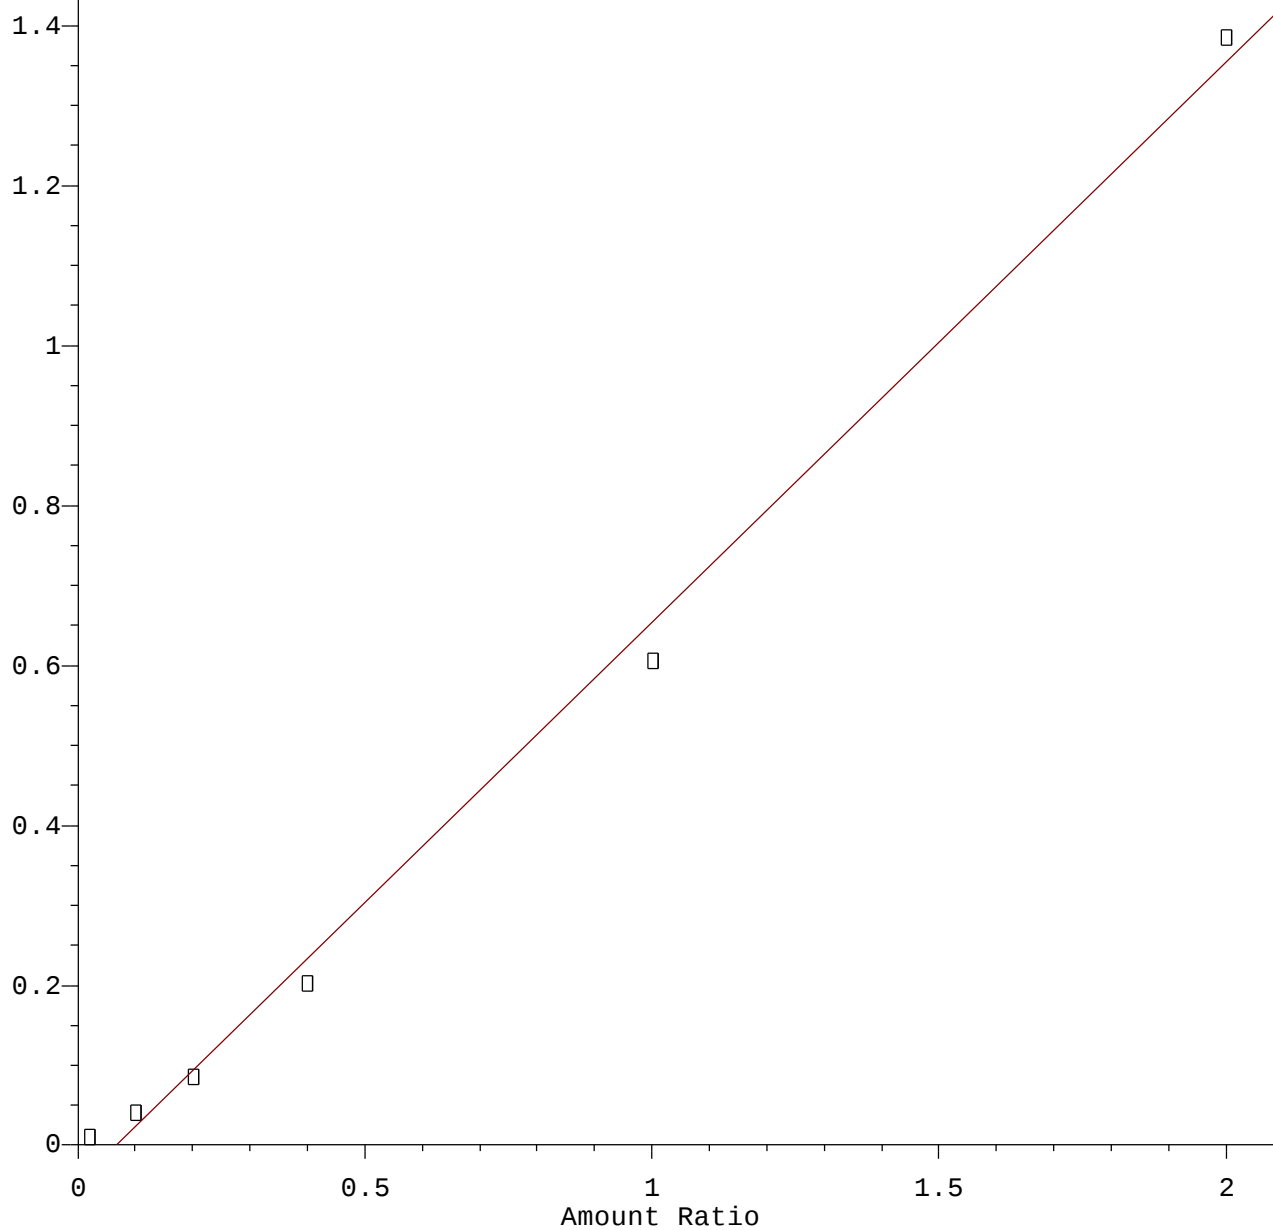


Resp Ratio = $7.00\text{e-}001$ * Amt - $4.64\text{e-}002$
Coef of Det (r^2) = 0.996 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N042919W.M
Calibration Table Last Updated: Tue Apr 30 04:20:38 2019

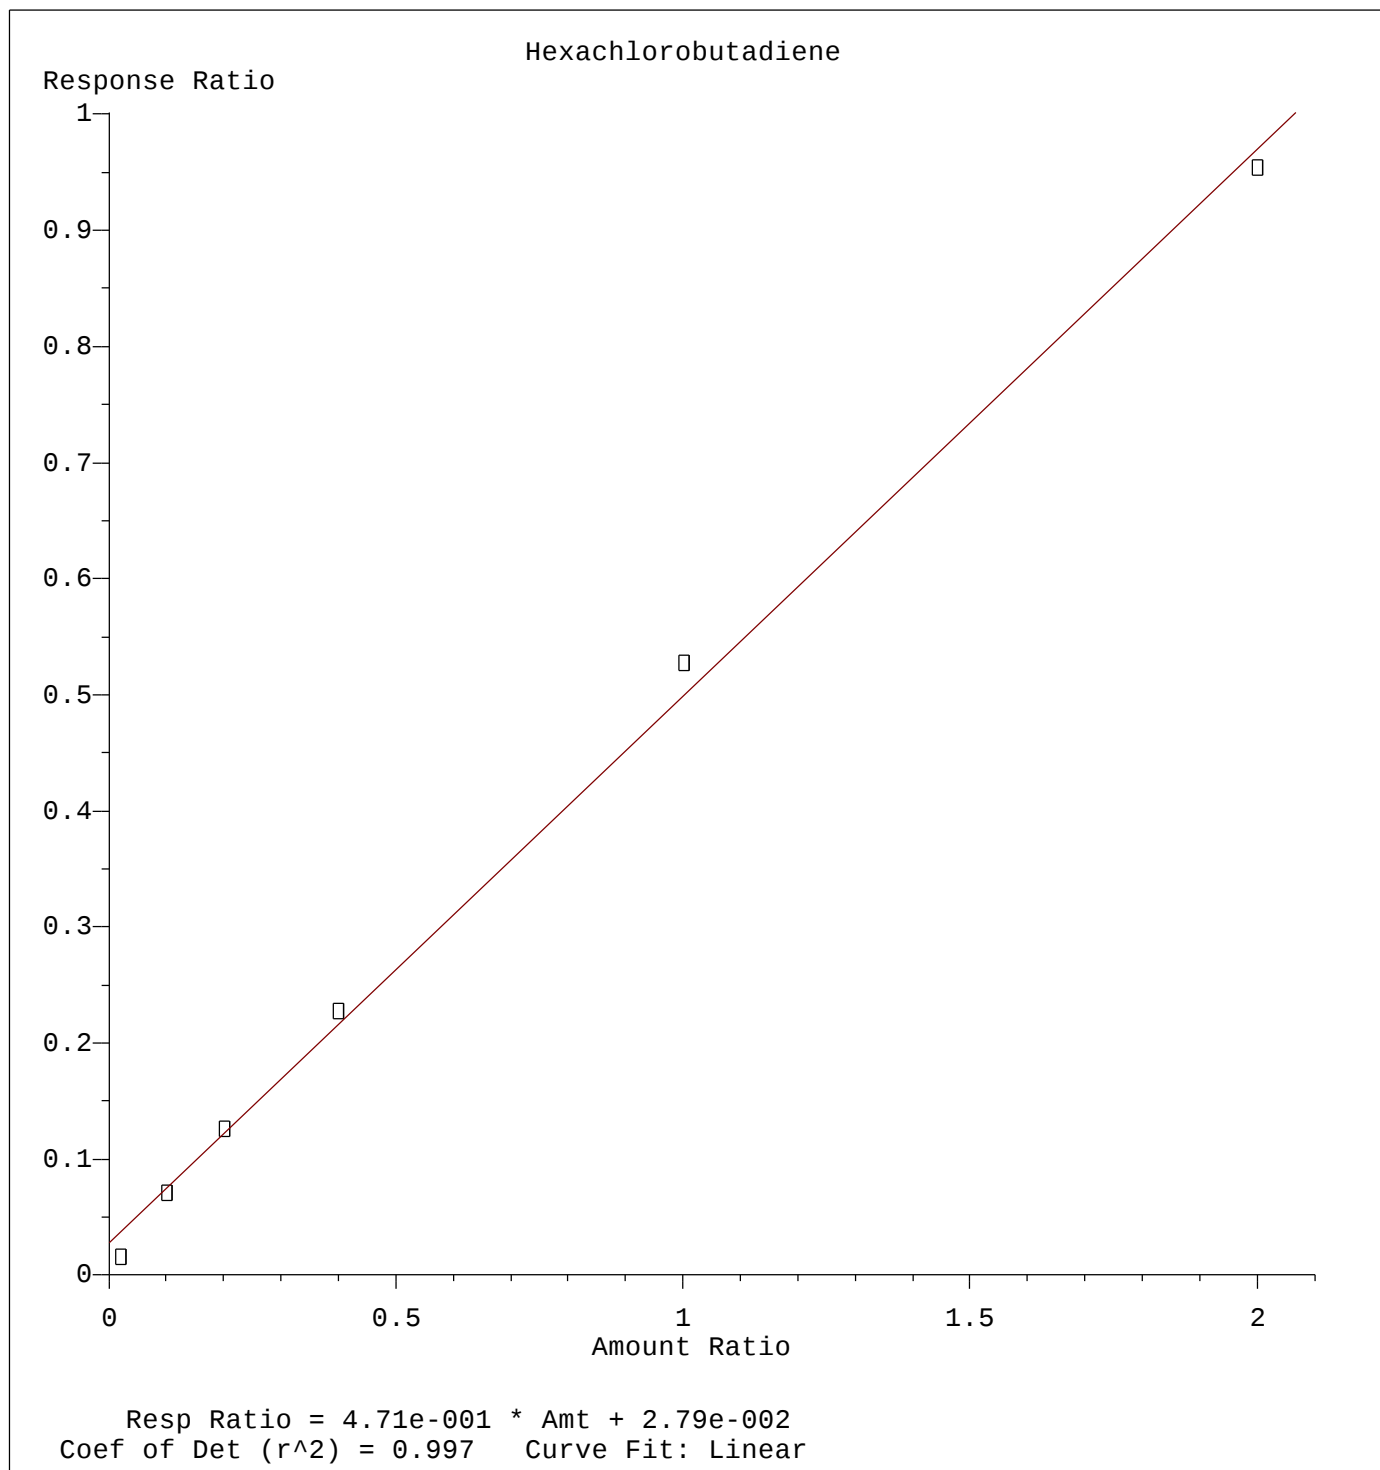


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N042919W.M
Calibration Table Last Updated: Tue Apr 30 04:20:38 2019

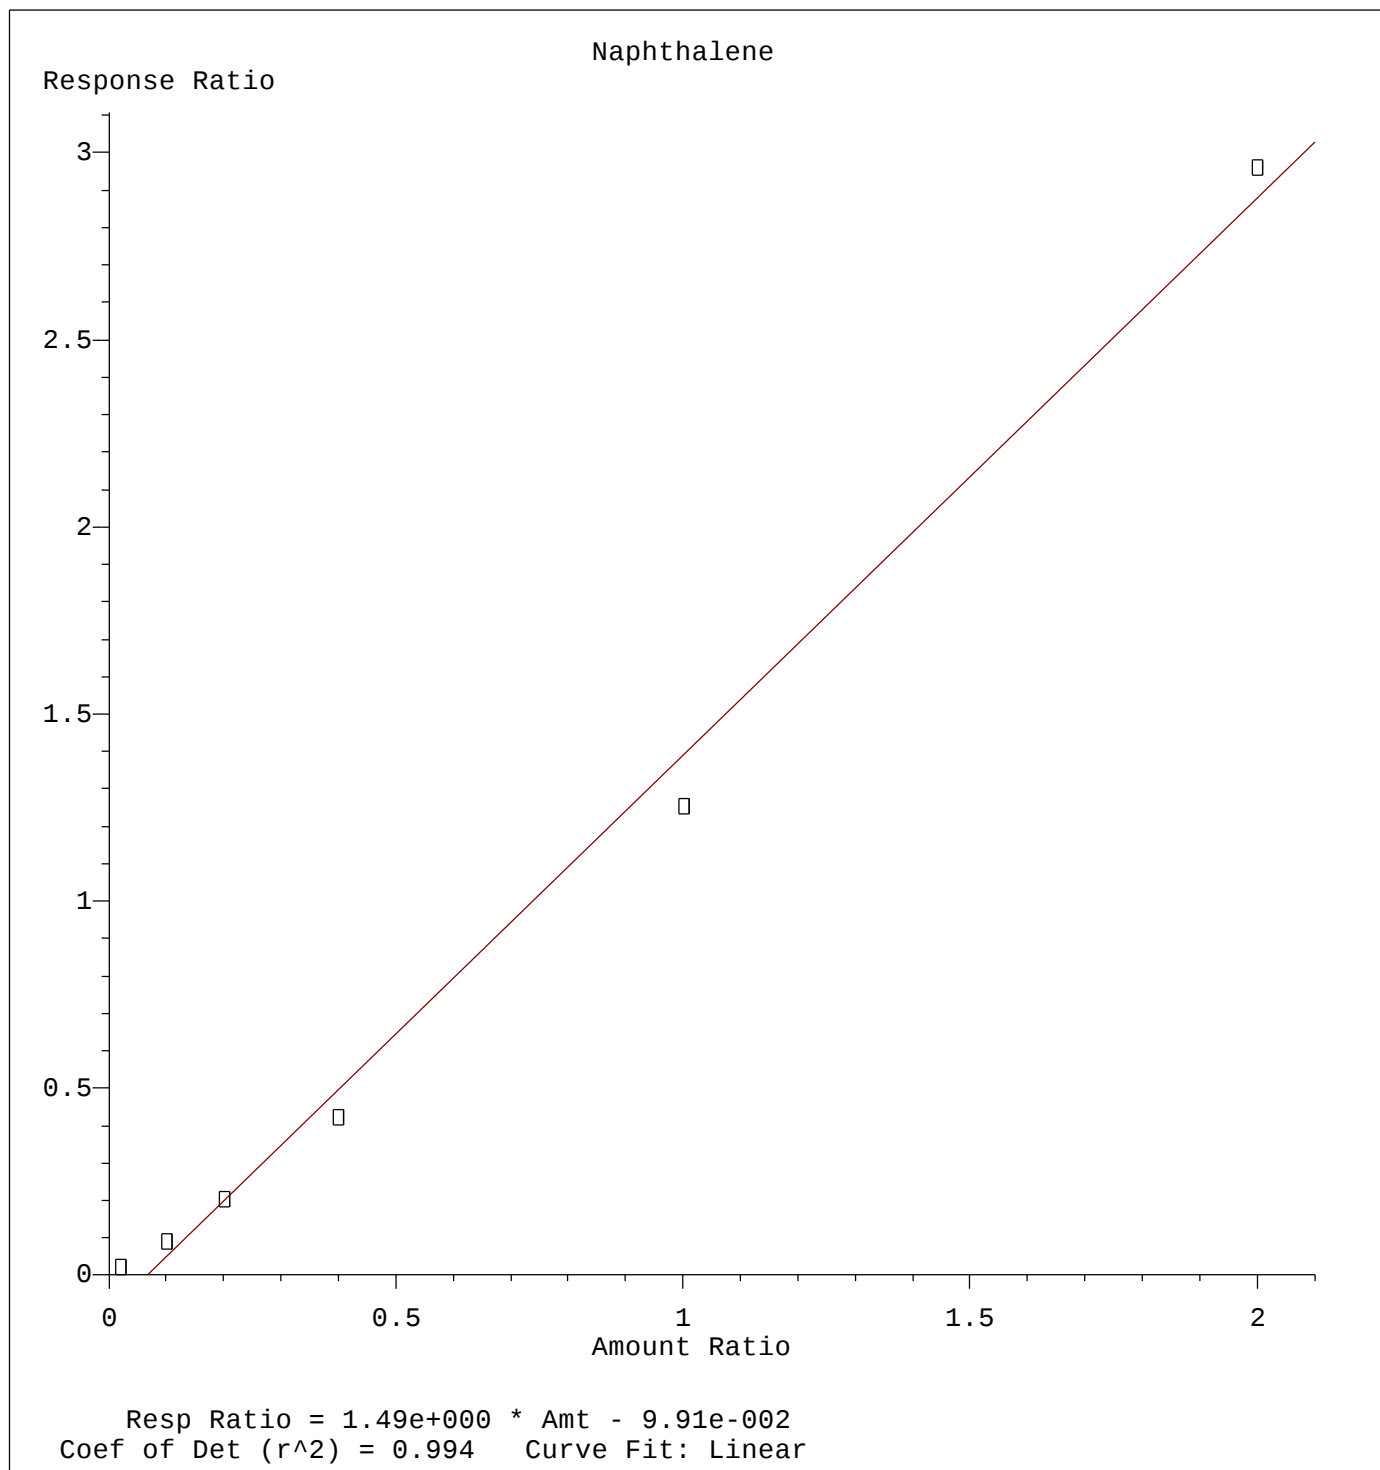

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N042919W.M
Calibration Table Last Updated: Tue Apr 30 04:20:38 2019

1,2,3-Trichlorobenzene

Response Ratio

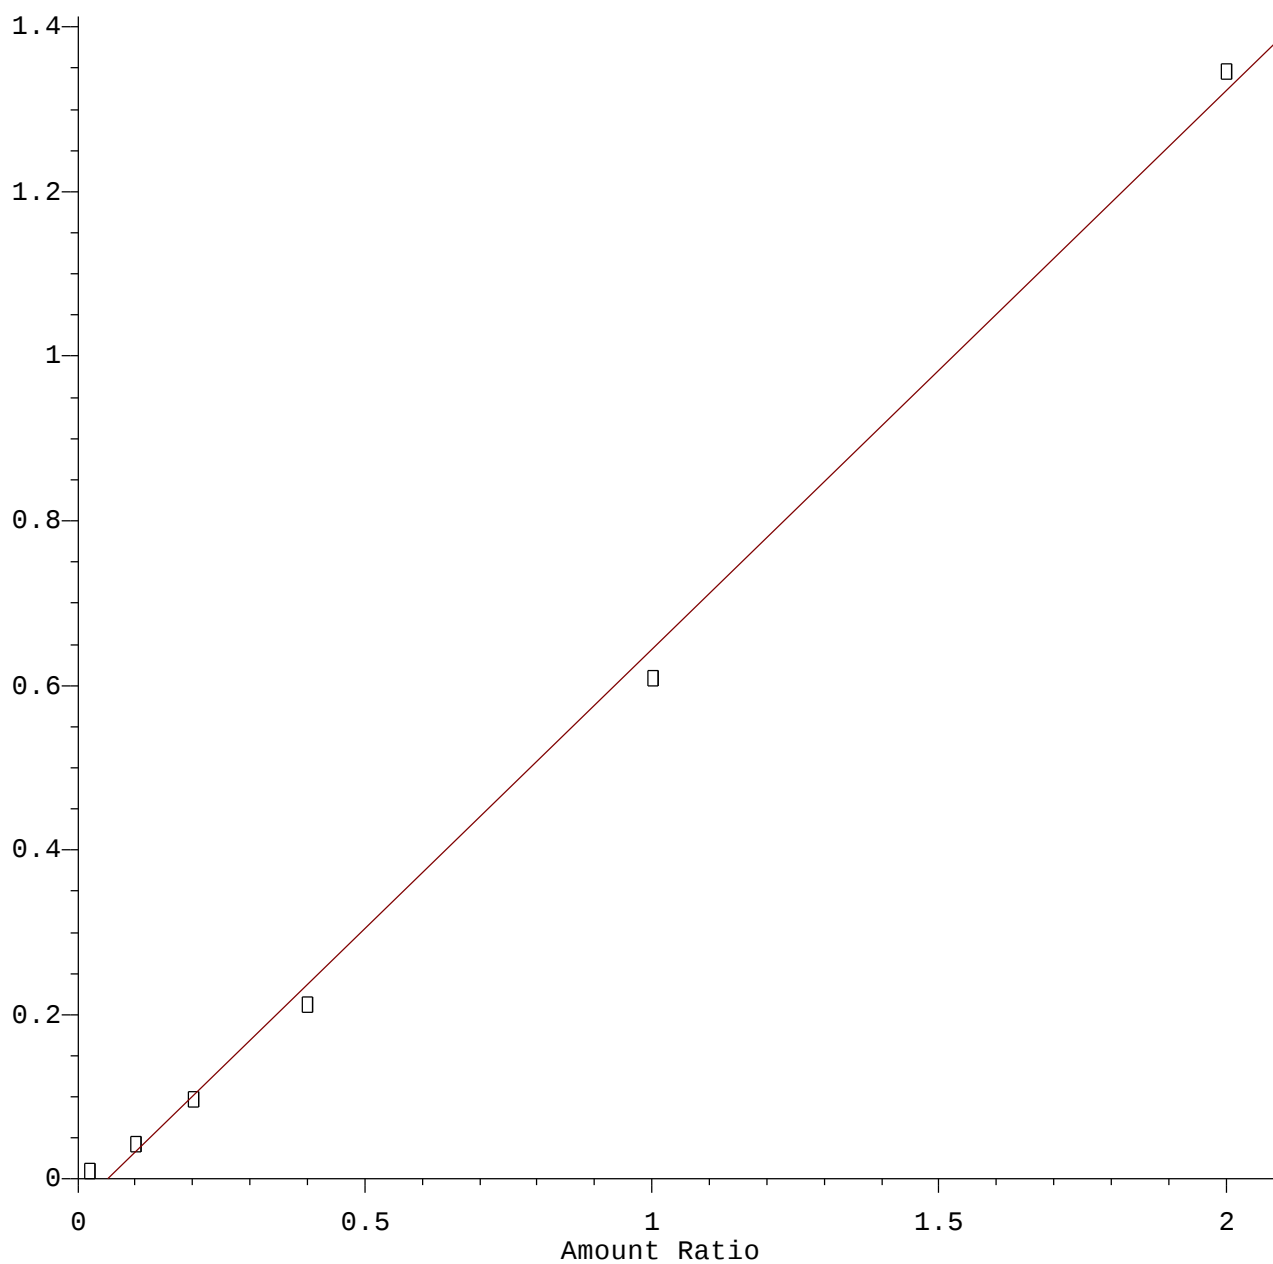

Resp Ratio = $6.79 \times 10^{-1} \times \text{Amt} - 3.55 \times 10^{-2}$
Coef of Det (r^2) = 0.997 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N042919W.M
Calibration Table Last Updated: Tue Apr 30 04:20:38 2019