


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN042920\
 Data File : VN061180.D
 Acq On : 29 Apr 2020 9:32
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N042720W.M
 Title : SW846 8260
 Last Update : Wed Apr 29 08:14:26 2020

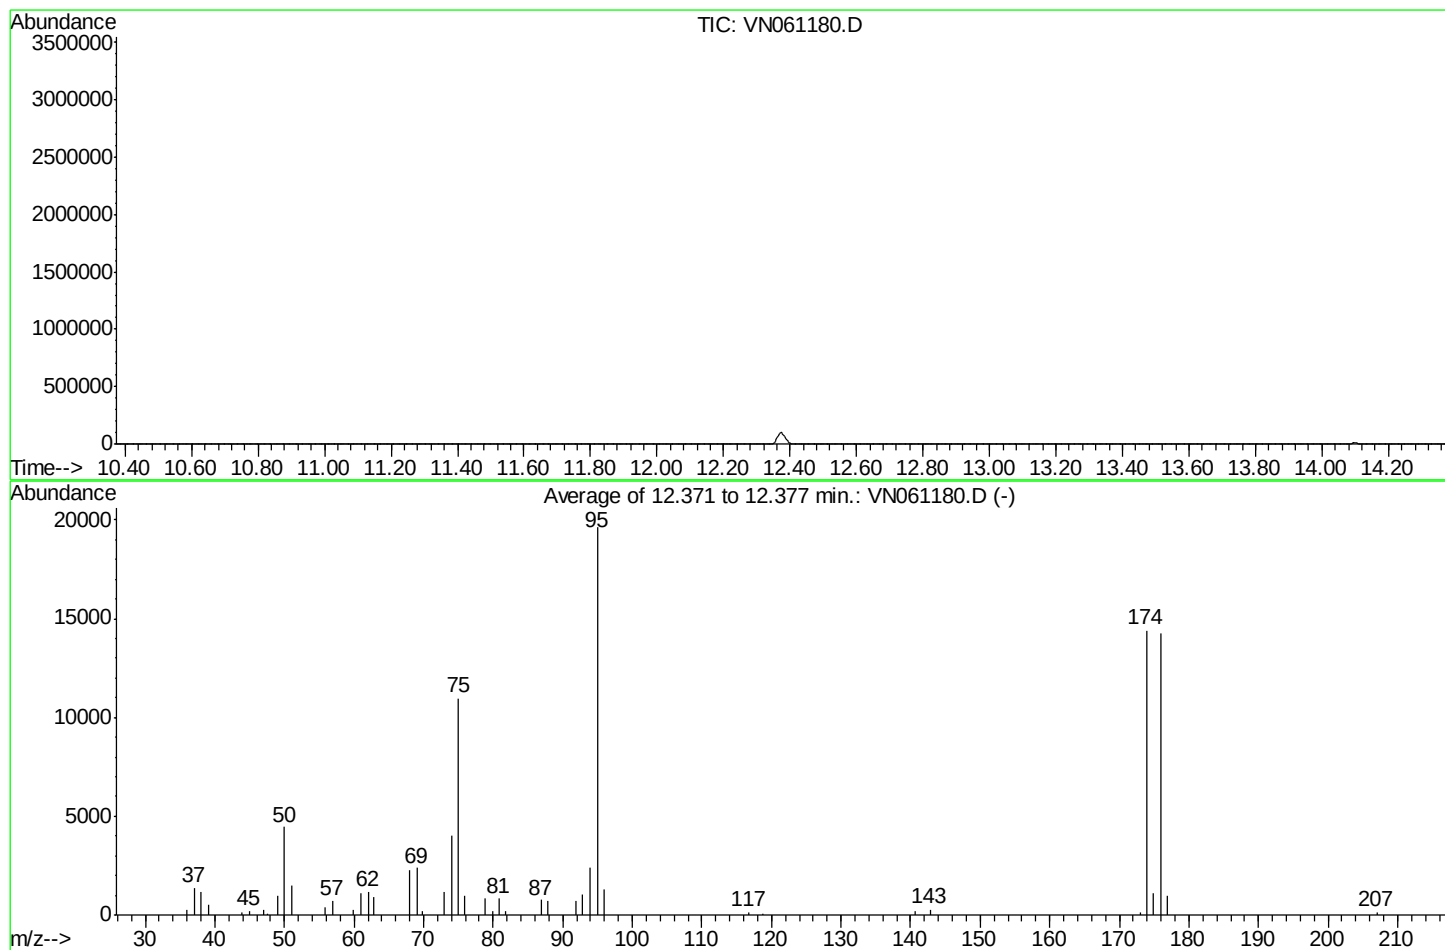

AutoFind: Scans 3353, 3354, 3355; Background Corrected with Scan 3341

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.7	4450	PASS
75	95	30	60	55.8	10954	PASS
95	95	100	100	100.0	19624	PASS
96	95	5	9	6.5	1276	PASS
173	174	0.00	2	1.0	144	PASS
174	95	50	100	73.4	14408	PASS
175	174	5	9	7.8	1119	PASS
176	174	95	101	99.0	14260	PASS
177	176	5	9	7.0	992	PASS