


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN042921\
Data File : VN066852.D
Acq On : 29 Apr 2021 9:27
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N042721W.M
Title : SW846 8260
Last Update : Tue Apr 27 16:02:50 2021

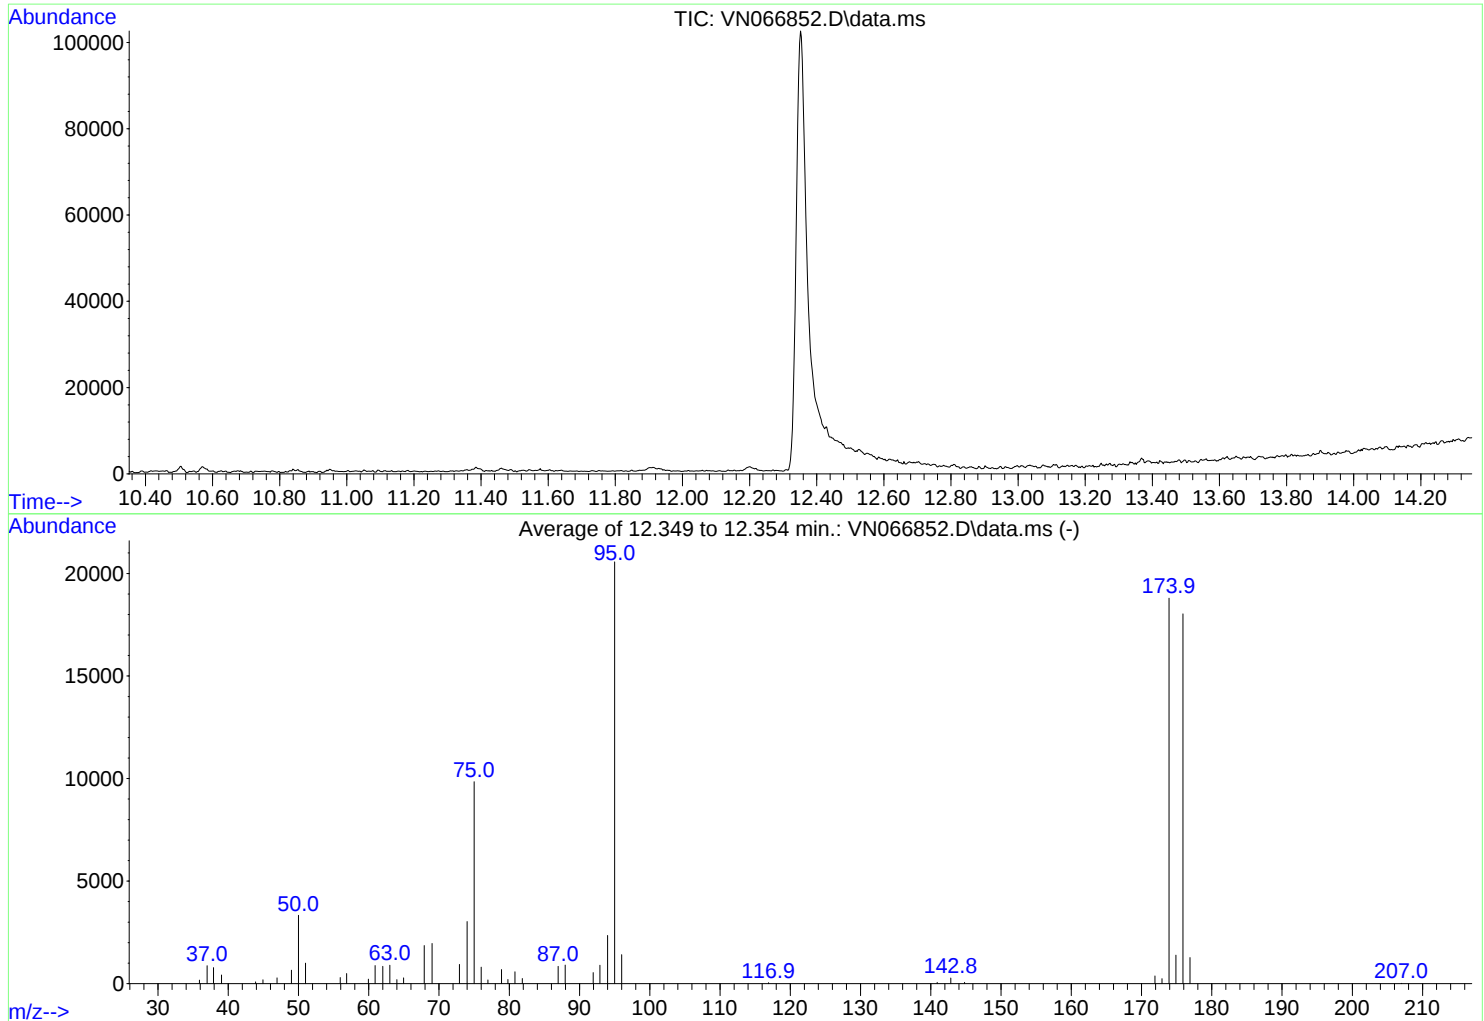

AutoFind: Scans 3962, 3963, 3964; Background Corrected with Scan 3947

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.2	3330	PASS
75	95	30	60	47.9	9848	PASS
95	95	100	100	100.0	20568	PASS
96	95	5	9	6.9	1411	PASS
173	174	0.00	2	1.3	244	PASS
174	95	50	100	91.4	18795	PASS
175	174	5	9	7.4	1387	PASS
176	174	95	101	95.9	18029	PASS
177	176	5	9	7.1	1272	PASS