


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN042921\
Data File : VN066878.D
Acq On : 29 Apr 2021 22:04
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N042721W.M
Title : SW846 8260
Last Update : Tue Apr 27 16:02:50 2021

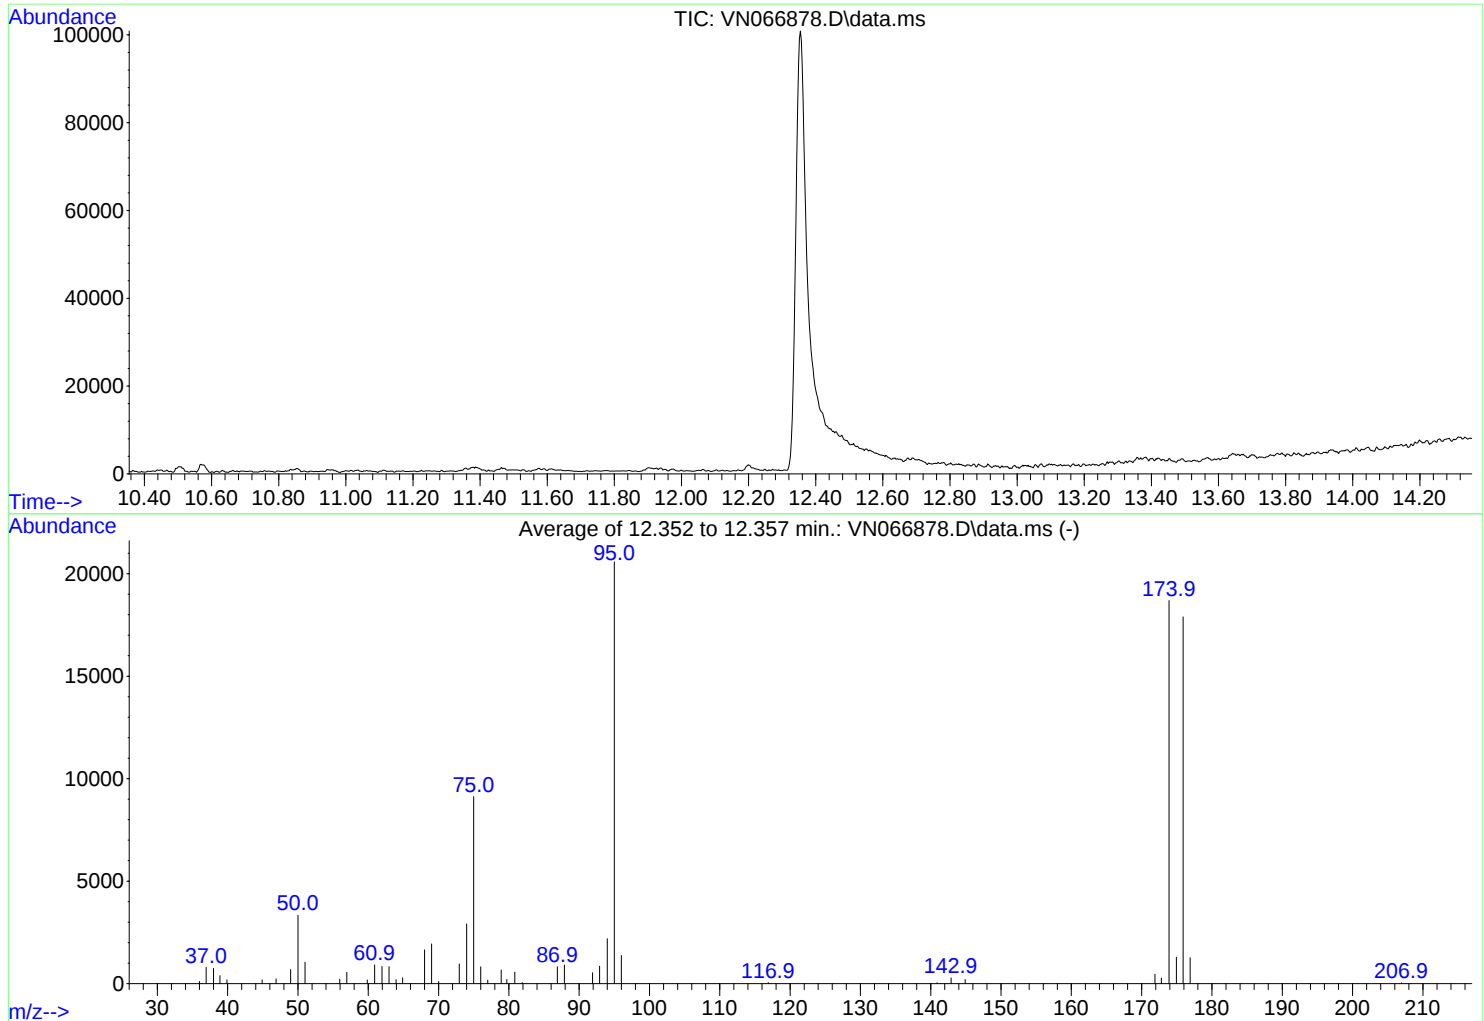

AutoFind: Scans 3963, 3964, 3965; Background Corrected with Scan 3947

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.2	3334	PASS
75	95	30	60	44.4	9128	PASS
95	95	100	100	100.0	20579	PASS
96	95	5	9	6.7	1378	PASS
173	174	0.00	2	1.5	273	PASS
174	95	50	100	90.8	18685	PASS
175	174	5	9	6.9	1291	PASS
176	174	95	101	95.8	17896	PASS
177	176	5	9	7.1	1268	PASS