

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN042923\
 Data File : VN077513.D
 Acq On : 29 Apr 2023 11:35
 Operator : JC\MD
 Sample : VN0429WBL01
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0429WBL01

Quant Time: May 01 01:22:27 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N042423W.M
 Quant Title : SW846 8260
 QLast Update : Tue Apr 25 02:50:59 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.231	168	539630	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.107	114	996667	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.866	117	888198	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.795	152	306500	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.583	65	357586	50.782	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	= 101.560%	
35) Dibromofluoromethane	8.172	113	316166	52.779	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 105.560%	
50) Toluene-d8	10.572	98	1225871	53.395	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	= 106.780%	
62) 4-Bromofluorobenzene	12.854	95	375360	49.971	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	= 99.940%	
Target Compounds						
					Qvalue	
2) Dichlorodifluoromethane	2.143	85	60	0.318	ug/l #	43
3) Chloromethane	2.372	50	1636	0.302	ug/l #	78
10) Methyl Iodide	4.601	142	2017	0.267	ug/l #	79
13) Acrolein	4.184	56	422	0.375	ug/l #	16
15) Acrylonitrile	5.731	53	1613	0.629	ug/l #	38
16) Acetone	4.443	43	997	0.445	ug/l #	40
17) Carbon Disulfide	4.725	76	4106	0.268	ug/l #	51
18) Methyl Acetate	5.048	43	1959	0.226	ug/l #	67
25) 2-Butanone	7.495	43	1254	0.395	ug/l #	81
31) Cyclohexane	8.231	56	13521	1.355	ug/l #	38
36) 1,1-Dichloropropene	8.231	75	46149	5.332	ug/l #	50
38) Carbon Tetrachloride	8.225	117	62664	6.563	ug/l #	15
49) 1,4-Dioxane	9.689	88	70	0.539	ug/l #	63
51) 4-Methyl-2-Pentanone	10.436	43	2480	0.372	ug/l	95
59) 2-Hexanone	11.195	43	6407	1.321	ug/l	93
74) N-amyl acetate	12.495	43	3452	0.410	ug/l #	92
76) 1,2,3-Trichloropropane	12.854	75	196170	27.524	ug/l #	1
77) Bromobenzene	12.983	156	2028	0.327	ug/l	100
78) n-propylbenzene	13.036	91	6619	0.210	ug/l	98
81) trans-1,4-Dichloro-2-b...	12.854	75	196170	77.759	ug/l #	15
82) 4-Chlorotoluene	13.230	91	6567	0.362	ug/l	90
87) 1,3-Dichlorobenzene	13.736	146	3834	0.348	ug/l	72
88) 1,4-Dichlorobenzene	13.818	146	6375	0.586	ug/l #	52
89) n-Butylbenzene	14.065	91	6460	0.385	ug/l	93
91) 1,2-Dichlorobenzene	14.113	146	5013	0.458	ug/l	94
92) 1,2-Dibromo-3-Chloropr...	14.724	75	894	0.541	ug/l	91
93) 1,2,4-Trichlorobenzene	15.401	180	3865	2.505	ug/l	83
94) Hexachlorobutadiene	15.495	225	631	0.286	ug/l	90
95) Naphthalene	15.583	128	2162	1.404	ug/l #	77
96) 1,2,3-Trichlorobenzene	15.795	180	1148	1.037	ug/l #	48


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN042923\
Data File : VN077513.D
Acq On : 29 Apr 2023 11:35
Operator : JC\MD
Sample : VN0429WBL01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0429WBL01

Quant Time: May 01 01:22:27 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N042423W.M
Quant Title : SW846 8260
QLast Update : Tue Apr 25 02:50:59 2023
Response via : Initial Calibration




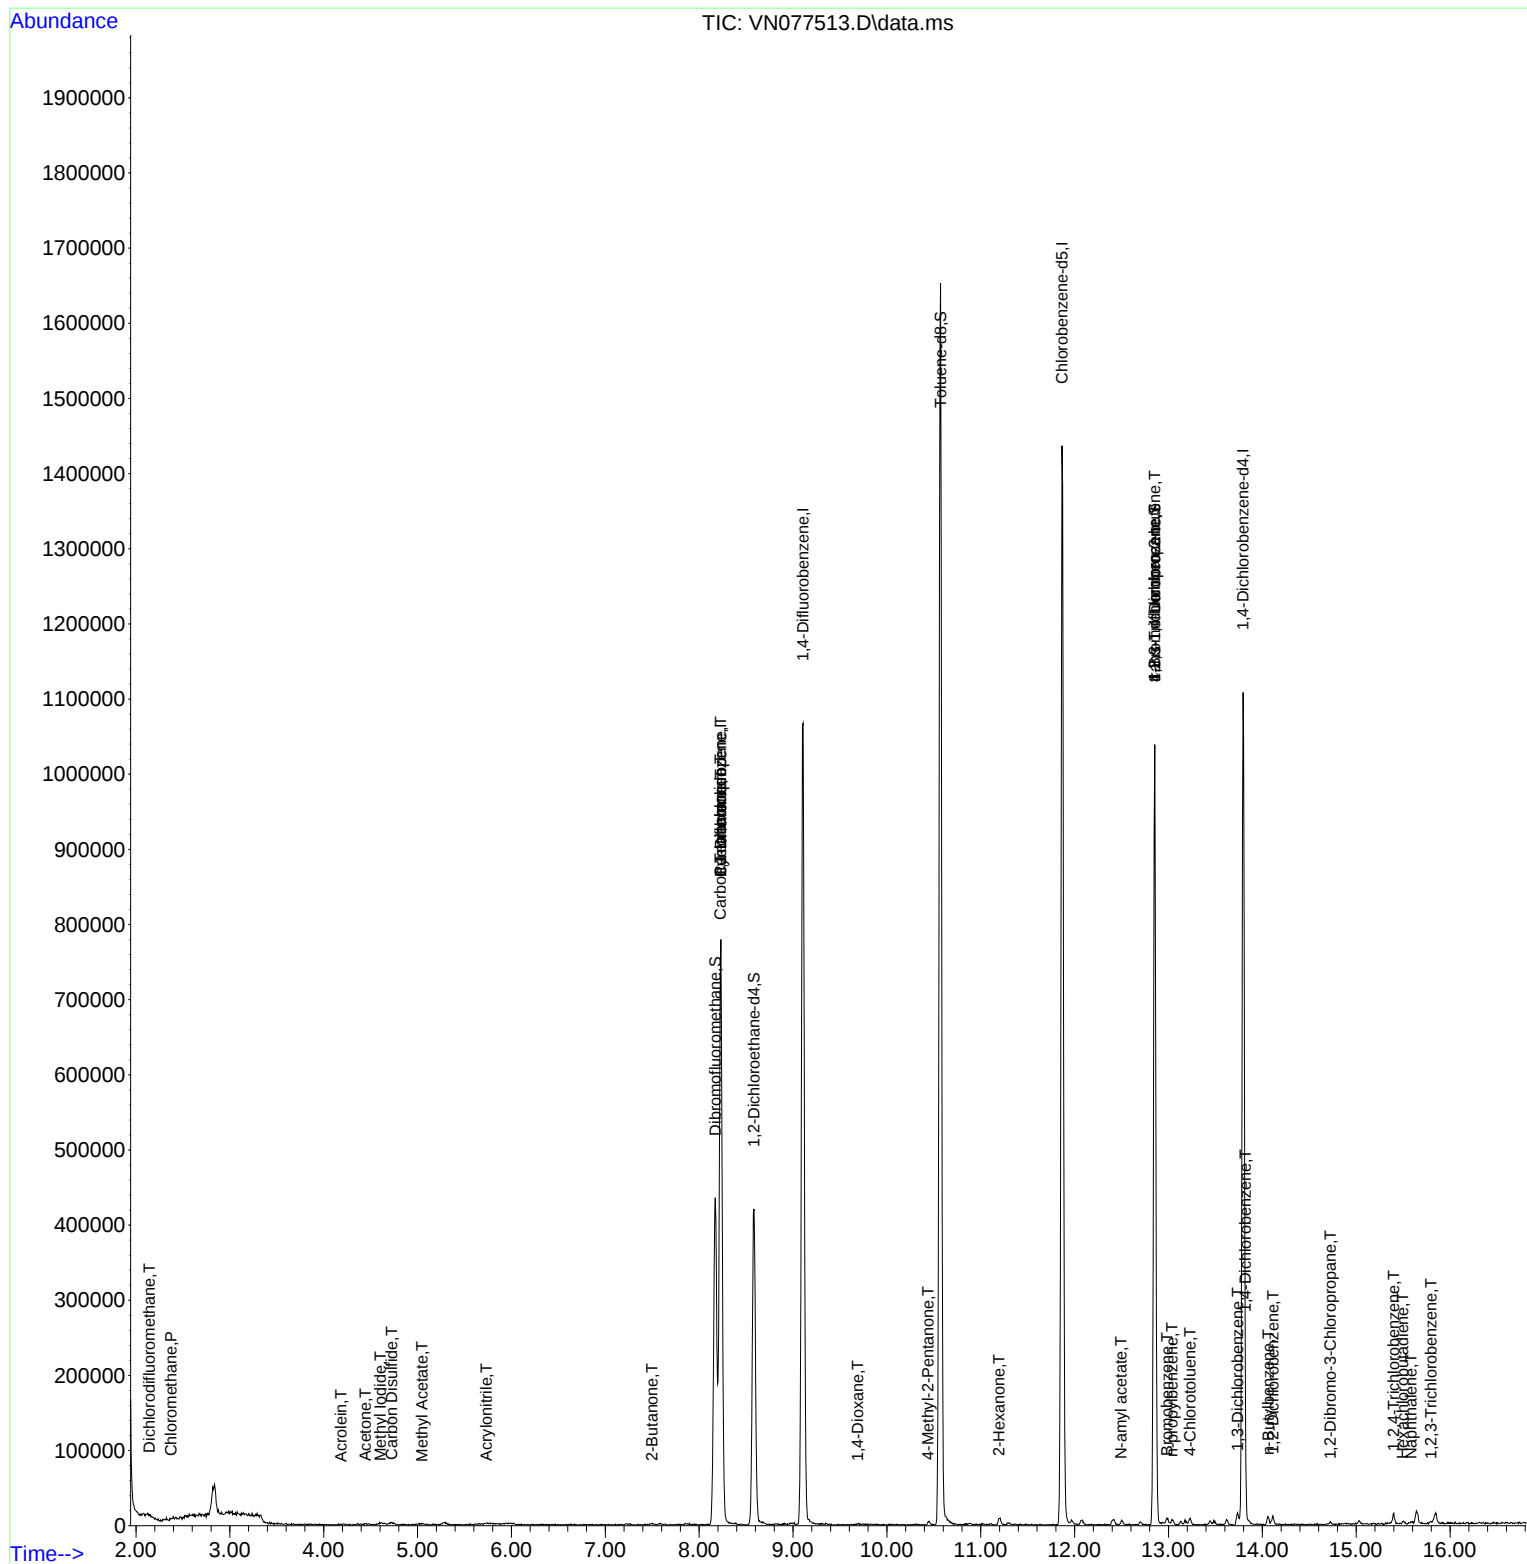




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.231 min Scan# 10
Delta R.T. -0.000 min
Lab File: VN077513.D
Acq: 29 Apr 2023 11:35




Instrument :
MSVOA_N
ClientSampleId :
VN0429WBL01


Tgt Ion:168 Resp: 539630
Ion Ratio Lower Upper
168 100
99 64.4 53.0 79.6

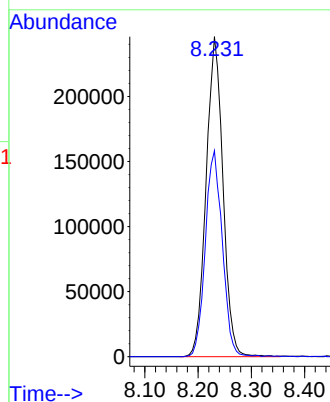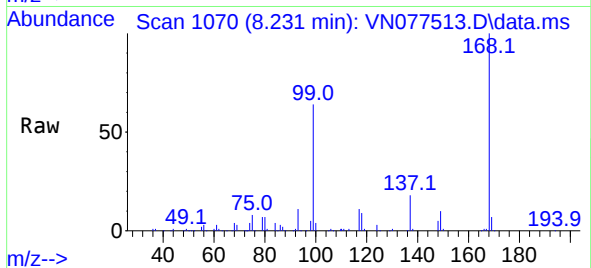

#2
Dichlorodifluoromethane
Concen: 0.318 ug/l
RT: 2.143 min Scan# 35
Delta R.T. 0.006 min
Lab File: VN077513.D
Acq: 29 Apr 2023 11:35

Tgt Ion: 85 Resp: 60
Ion Ratio Lower Upper
85 100
87 0.0 15.8 47.4#


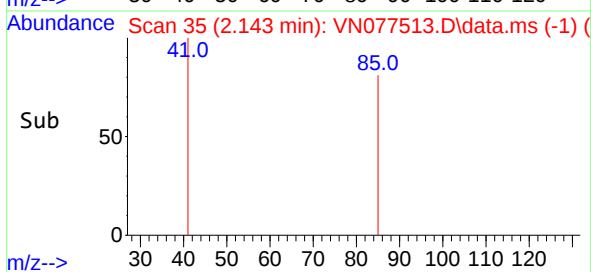
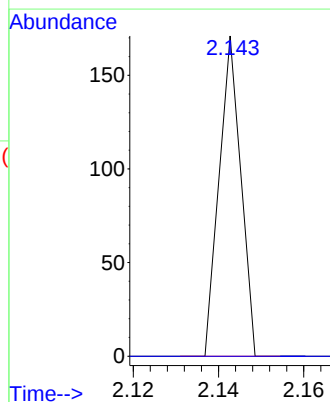



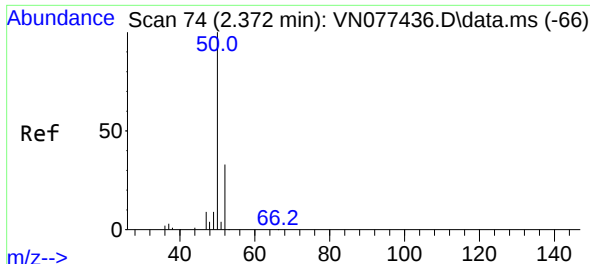

#3
Chloromethane
Concen: 0.302 ug/l
RT: 2.372 min Scan# 74
Delta R.T. -0.000 min
Lab File: VN077513.D
Acq: 29 Apr 2023 11:35




Instrument :
MSVOA_N
ClientSampleId :
VN0429WBL01


Tgt Ion: 50 Resp: 1636
Ion Ratio Lower Upper
50 100
52 20.9 26.5 39.7#

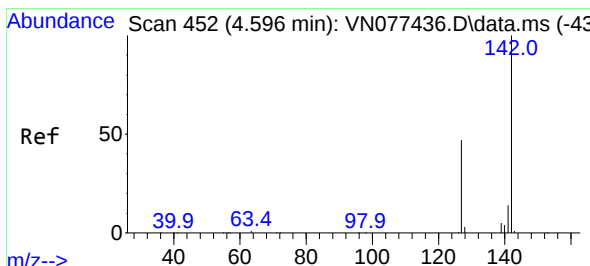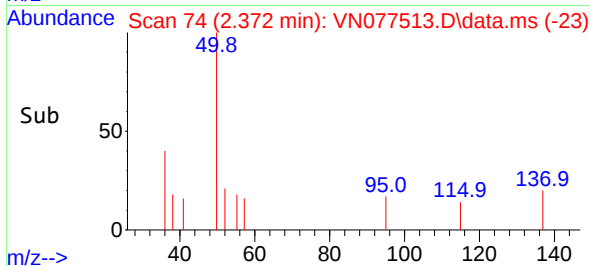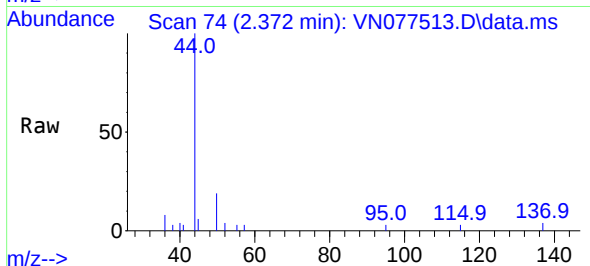

#10
Methyl Iodide
Concen: 0.267 ug/l
RT: 4.601 min Scan# 453
Delta R.T. 0.006 min
Lab File: VN077513.D
Acq: 29 Apr 2023 11:35

Tgt Ion: 142 Resp: 2017
Ion Ratio Lower Upper
142 100
127 35.5 37.6 56.4#
141 0.0 11.4 17.0#


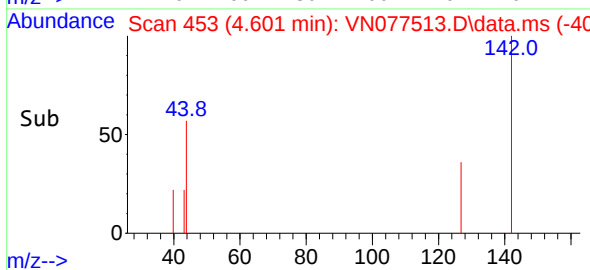

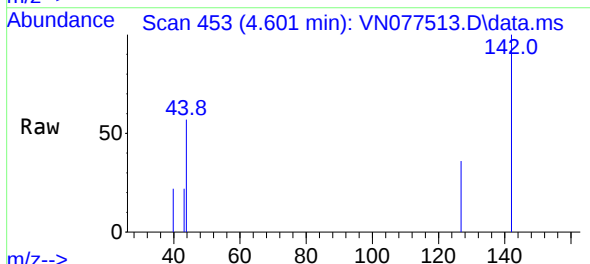




#13
Acrolein
Concen: 0.375 ug/l
RT: 4.184 min Scan# 382
Delta R.T. -0.000 min
Lab File: VN077513.D
Acq: 29 Apr 2023 11:35




Instrument :
MSVOA_N
ClientSampleId :
VN0429WBL01


Tgt Ion: 56 Resp: 422
Ion Ratio Lower Upper
56 100
55 0.0 54.5 81.7#



#15
Acrylonitrile
Concen: 0.629 ug/l
RT: 5.731 min Scan# 645
Delta R.T. -0.000 min
Lab File: VN077513.D
Acq: 29 Apr 2023 11:35

Tgt Ion: 53 Resp: 1613
Ion Ratio Lower Upper
53 100
52 25.7 65.3 97.9#
51 0.0 28.9 43.3#


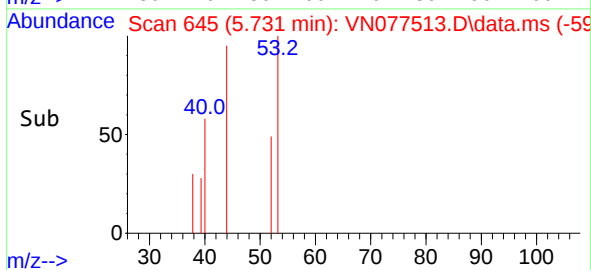






#16
Acetone
Concen: 0.445 ug/l
RT: 4.443 min Scan# 41
Delta R.T. 0.012 min
Lab File: VN077513.D
Acq: 29 Apr 2023 11:35




Instrument :
MSVOA_N
ClientSampleId :
VN0429WBL01


Tgt Ion: 43 Resp: 997
Ion Ratio Lower Upper
43 100
58 0.0 28.0 42.0#

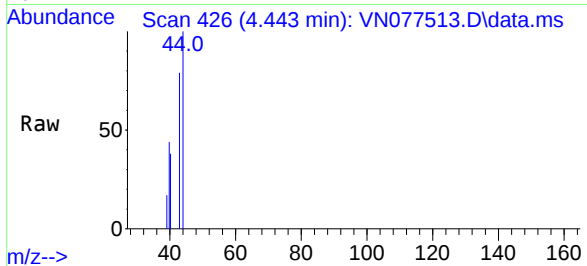

#17
Carbon Disulfide
Concen: 0.268 ug/l
RT: 4.725 min Scan# 474
Delta R.T. -0.000 min
Lab File: VN077513.D
Acq: 29 Apr 2023 11:35

Tgt Ion: 76 Resp: 4106
Ion Ratio Lower Upper
76 100
78 27.2 7.4 11.0#


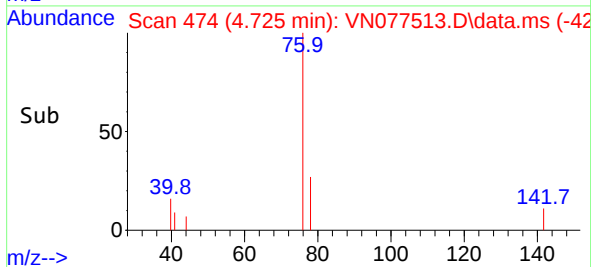

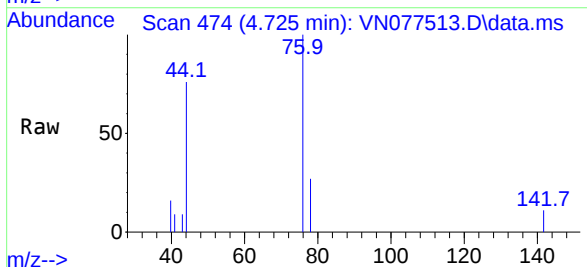




#18
Methyl Acetate
Concen: 0.226 ug/l
RT: 5.048 min Scan# 51
Delta R.T. 0.012 min
Lab File: VN077513.D
Acq: 29 Apr 2023 11:35




Instrument :
MSVOA_N
ClientSampleId :
VN0429WBL01


Tgt Ion: 43 Resp: 1959
Ion Ratio Lower Upper
43 100
74 13.9 26.2 39.4#

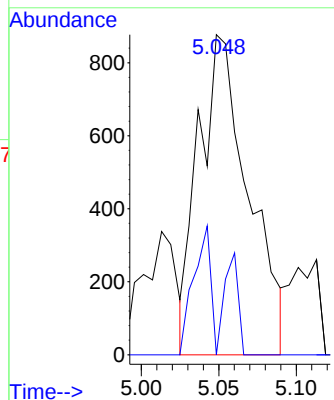

#25
2-Butanone
Concen: 0.395 ug/l
RT: 7.495 min Scan# 945
Delta R.T. 0.006 min
Lab File: VN077513.D
Acq: 29 Apr 2023 11:35

Tgt Ion: 43 Resp: 1254
Ion Ratio Lower Upper
43 100
72 48.9 30.2 45.2#


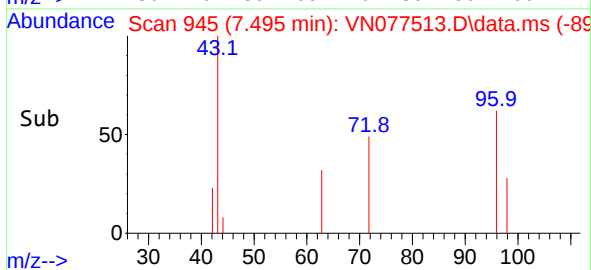
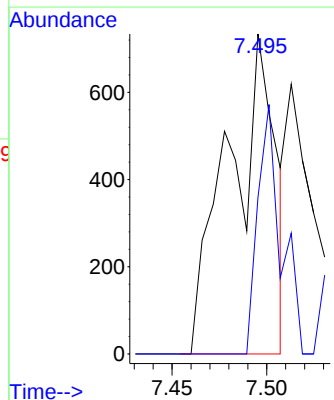



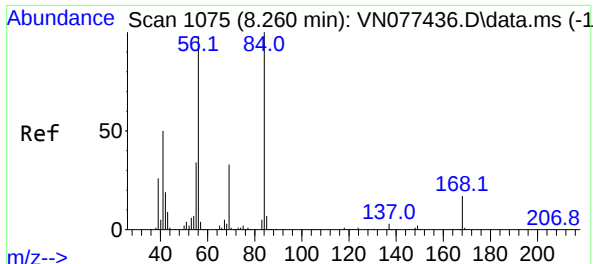

#31
Cyclohexane
Concen: 1.355 ug/l
RT: 8.231 min Scan# 1075
Delta R.T. -0.030 min
Lab File: VN077513.D
Acq: 29 Apr 2023 11:35




Instrument :
MSVOA_N
ClientSampleId :
VN0429WBL01


Tgt Ion: 56 Resp: 13521
Ion Ratio Lower Upper
56 100
69 122.1 26.8 40.2#
84 134.4 81.8 122.6#

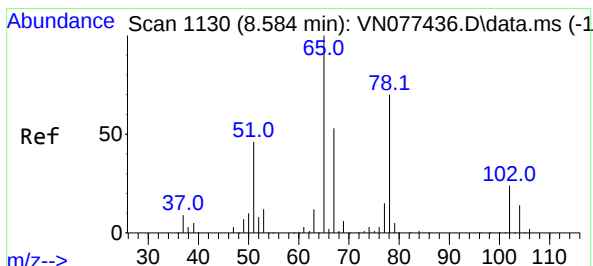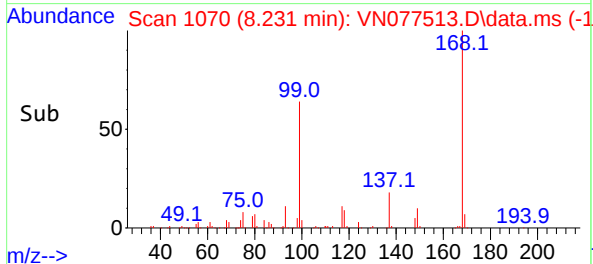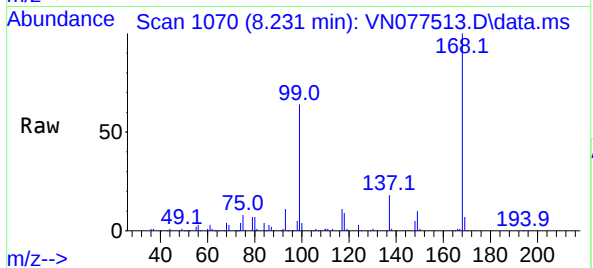

#33
1,2-Dichloroethane-d4
Concen: 50.782 ug/l
RT: 8.583 min Scan# 1130
Delta R.T. -0.000 min
Lab File: VN077513.D
Acq: 29 Apr 2023 11:35

Tgt Ion: 65 Resp: 357586
Ion Ratio Lower Upper
65 100
67 51.6 0.0 106.6


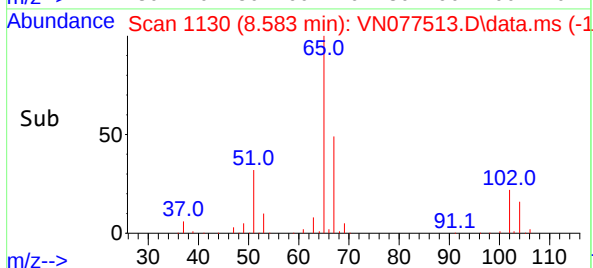
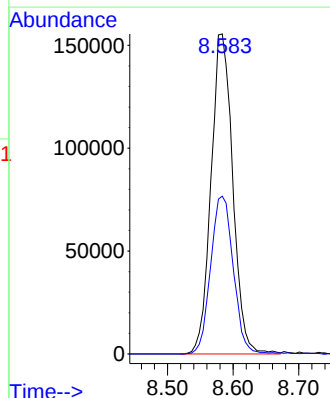
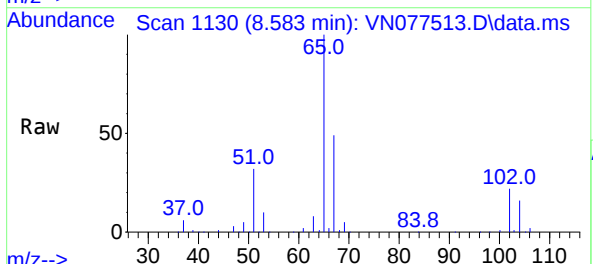


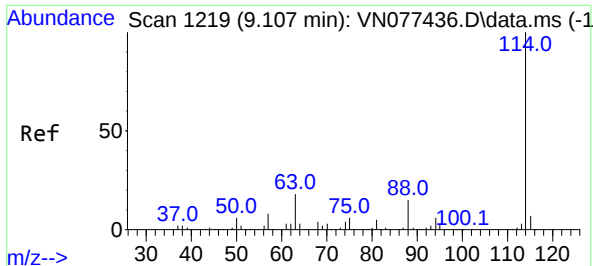

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 9.107 min Scan# 11
Delta R.T. -0.000 min
Lab File: VN077513.D
Acq: 29 Apr 2023 11:35




Instrument :
MSVOA_N
ClientSampleId :
VN0429WBL01


Tgt Ion:114 Resp: 996667
Ion Ratio Lower Upper
114 100
63 18.7 0.0 36.4
88 15.1 0.0 30.6

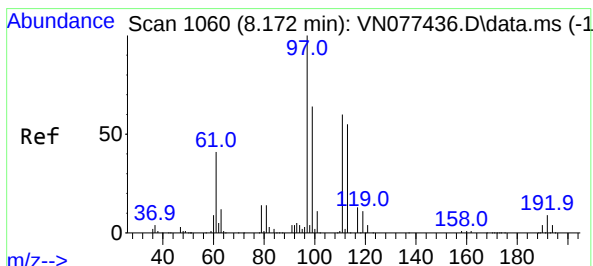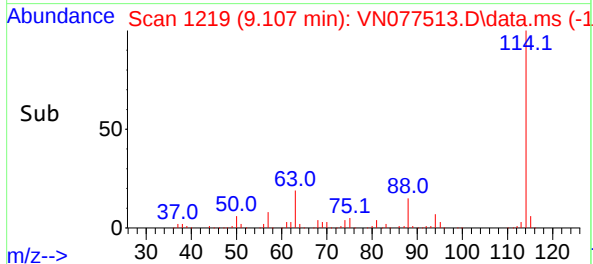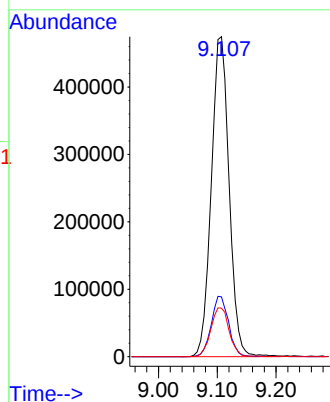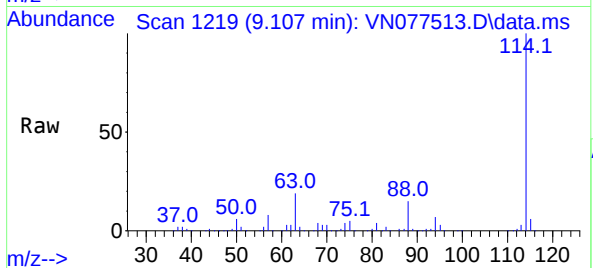

#35
Dibromofluoromethane
Concen: 52.779 ug/l
RT: 8.172 min Scan# 1060
Delta R.T. -0.000 min
Lab File: VN077513.D
Acq: 29 Apr 2023 11:35

Tgt Ion:113 Resp: 316166
Ion Ratio Lower Upper
113 100
111 104.6 82.6 123.8
192 16.6 12.7 19.1


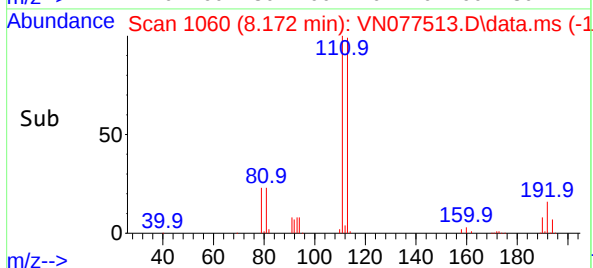

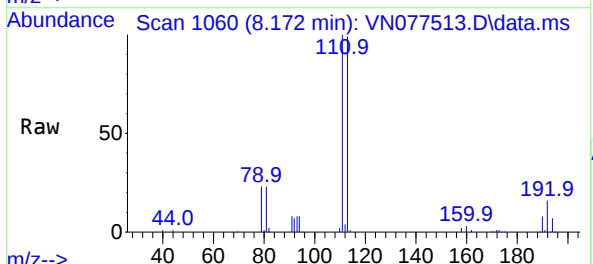


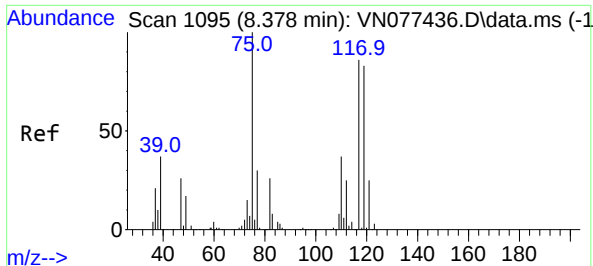

#36
1,1-Dichloropropene
Concen: 5.332 ug/l
RT: 8.231 min Scan# 1069
Delta R.T. -0.147 min
Lab File: VN077513.D
Acq: 29 Apr 2023 11:35




Instrument :
MSVOA_N
ClientSampleId :
VN0429WBL01


Tgt Ion: 75 Resp: 46149
Ion Ratio Lower Upper
75 100
110 11.5 19.1 57.3#
77 0.0 25.0 37.4#

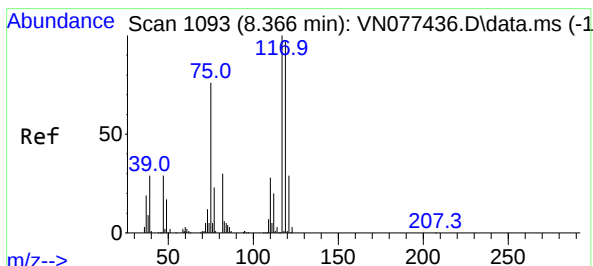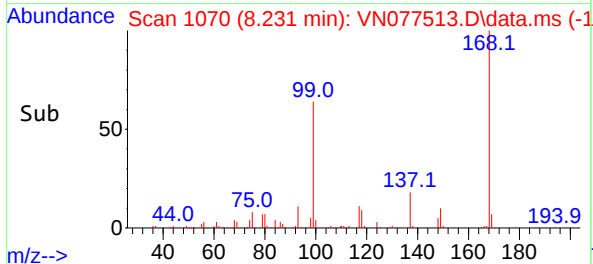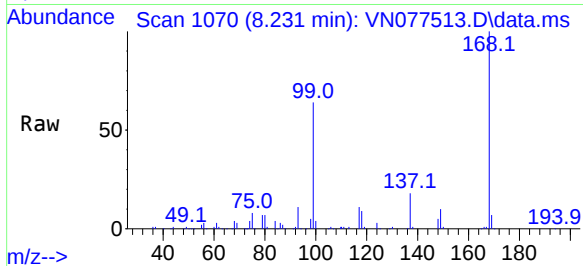

#38
Carbon Tetrachloride
Concen: 6.563 ug/l
RT: 8.225 min Scan# 1069
Delta R.T. -0.141 min
Lab File: VN077513.D
Acq: 29 Apr 2023 11:35

Tgt Ion: 117 Resp: 62664
Ion Ratio Lower Upper
117 100
119 4.2 77.3 115.9#
121 0.0 23.3 34.9#


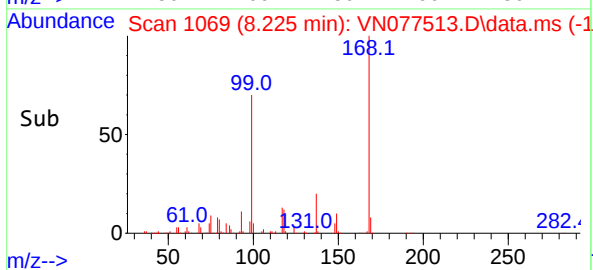

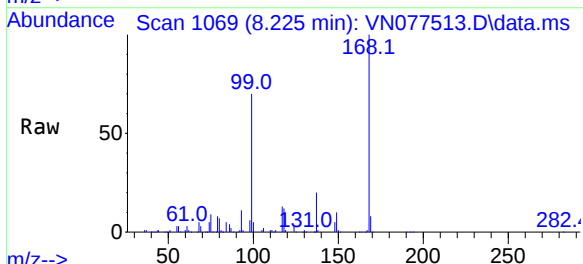


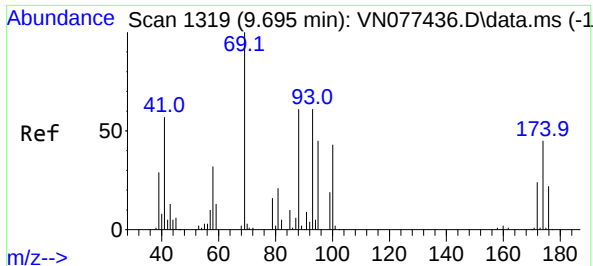

#49
1,4-Dioxane
Concen: 0.539 ug/l
RT: 9.689 min Scan# 11
Delta R.T. -0.006 min
Lab File: VN077513.D
Acq: 29 Apr 2023 11:35




Instrument :
MSVOA_N
ClientSampleId :
VN0429WBL01


Tgt Ion: 88 Resp: 70
Ion Ratio Lower Upper
88 100
43 0.0 17.0 25.6#
58 84.3 47.0 70.4#

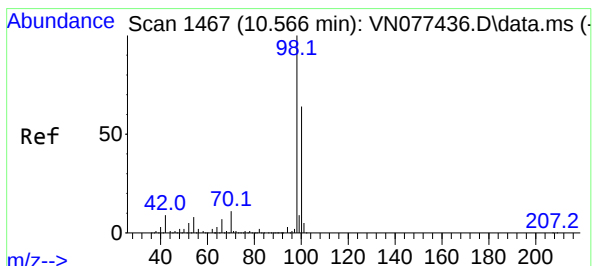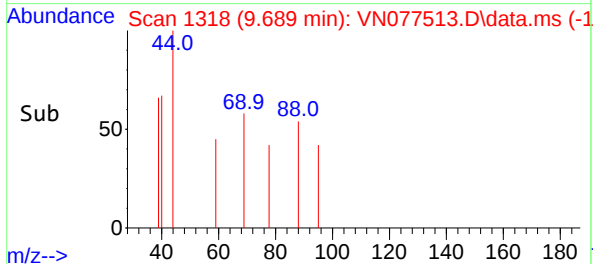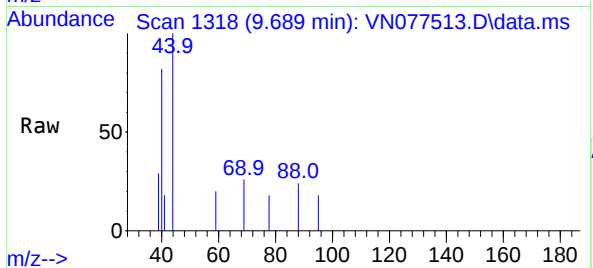

#50
Toluene-d8
Concen: 53.395 ug/l
RT: 10.572 min Scan# 1468
Delta R.T. 0.006 min
Lab File: VN077513.D
Acq: 29 Apr 2023 11:35

Tgt Ion: 98 Resp: 1225871
Ion Ratio Lower Upper
98 100
100 63.9 52.0 78.0


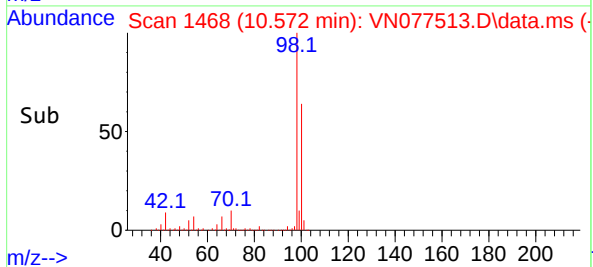

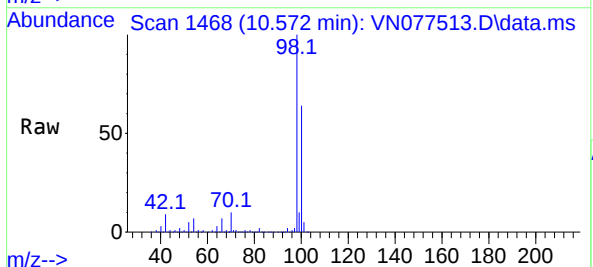




#51
4-Methyl-2-Pentanone
Concen: 0.372 ug/l
RT: 10.436 min Scan# 1445
Delta R.T. -0.012 min
Lab File: VN077513.D
Acq: 29 Apr 2023 11:35




Instrument :
MSVOA_N
ClientSampleId :
VN0429WBL01


Tgt Ion: 43 Resp: 2480
Ion Ratio Lower Upper
43 100
58 42.5 36.6 54.8



#59
2-Hexanone
Concen: 1.321 ug/l
RT: 11.195 min Scan# 1574
Delta R.T. -0.000 min
Lab File: VN077513.D
Acq: 29 Apr 2023 11:35

Tgt Ion: 43 Resp: 6407
Ion Ratio Lower Upper
43 100
58 57.6 31.7 95.1


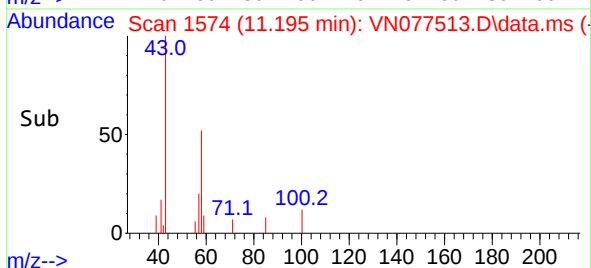
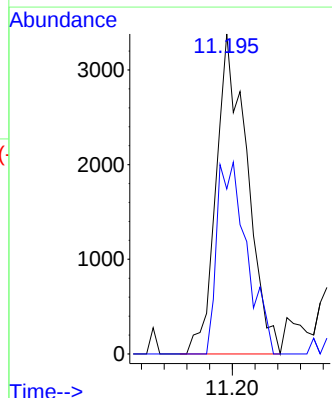



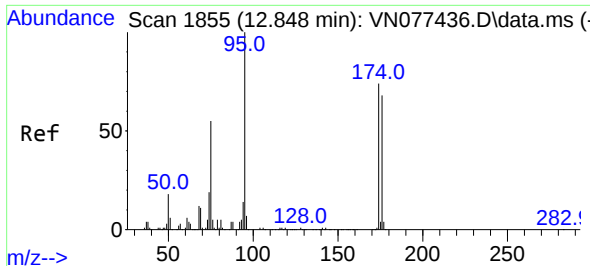

#62
4-Bromofluorobenzene
Concen: 49.971 ug/l
RT: 12.854 min Scan# 1856
Delta R.T. 0.006 min
Lab File: VN077513.D
Acq: 29 Apr 2023 11:35




Instrument :
MSVOA_N
ClientSampleId :
VN0429WBL01


Tgt Ion: 95 Resp: 375360
Ion Ratio Lower Upper
95 100
174 69.6 0.0 143.8
176 66.8 0.0 135.8

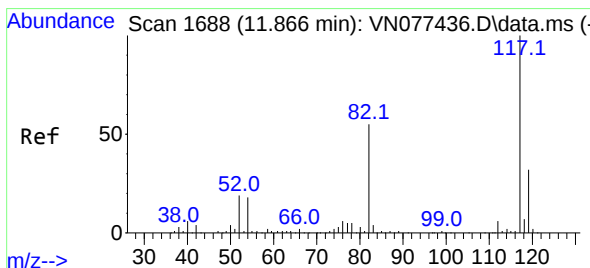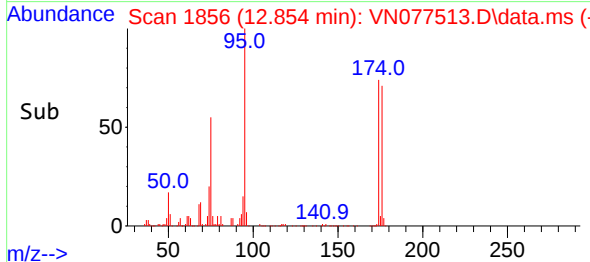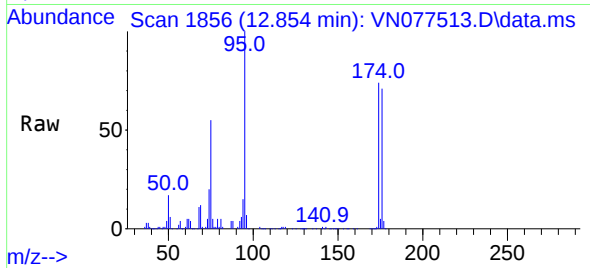

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.866 min Scan# 1688
Delta R.T. -0.000 min
Lab File: VN077513.D
Acq: 29 Apr 2023 11:35

Tgt Ion: 117 Resp: 888198
Ion Ratio Lower Upper
117 100
82 55.3 44.0 66.0
119 32.8 25.6 38.4


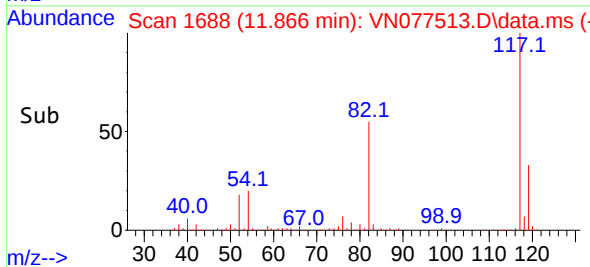

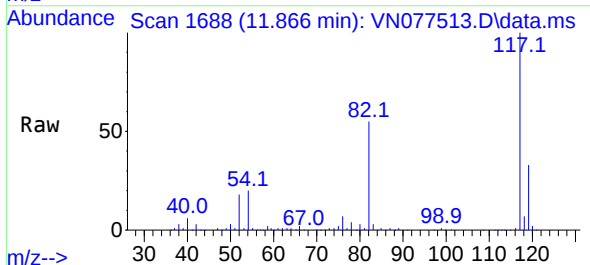




#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.795 min Scan# 2016
Delta R.T. -0.000 min
Lab File: VN077513.D
Acq: 29 Apr 2023 11:35




Instrument :
MSVOA_N
ClientSampleId :
VN0429WBL01


Tgt Ion:152 Resp: 306500
Ion Ratio Lower Upper
152 100
115 64.7 32.3 96.8
150 158.8 0.0 355.8

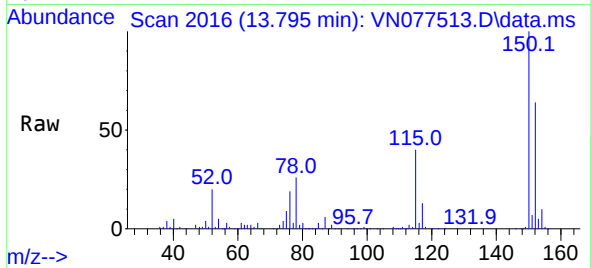

#74
N-ethyl acetate
Concen: 0.410 ug/l
RT: 12.495 min Scan# 1795
Delta R.T. -0.000 min
Lab File: VN077513.D
Acq: 29 Apr 2023 11:35

Tgt Ion: 43 Resp: 3452
Ion Ratio Lower Upper
43 100
70 49.2 43.4 65.2
55 20.8 21.4 32.0#
61 25.0 22.8 34.2


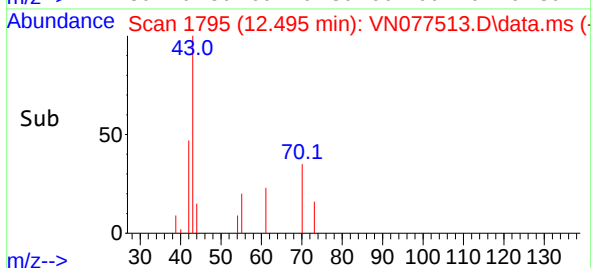
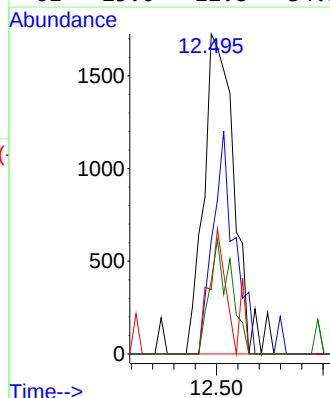





#76
1,2,3-Trichloropropane
Concen: 27.524 ug/l
RT: 12.854 min Scan# 1856
Delta R.T. -0.141 min
Lab File: VN077513.D
Acq: 29 Apr 2023 11:35




Instrument :
MSVOA_N
ClientSampleId :
VN0429WBL01


Tgt Ion: 75 Resp: 196170
Ion Ratio Lower Upper
75 100
77 1.1 84.5 253.5#



#77
Bromobenzene
Concen: 0.327 ug/l
RT: 12.983 min Scan# 1878
Delta R.T. -0.000 min
Lab File: VN077513.D
Acq: 29 Apr 2023 11:35

Tgt Ion:156 Resp: 2028
Ion Ratio Lower Upper
156 100
77 215.4 107.7 323.3
158 95.6 48.4 145.3


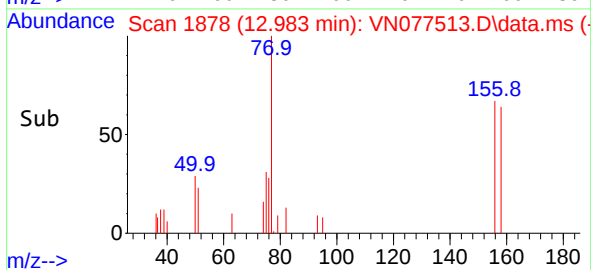






#78
n-propylbenzene
Concen: 0.210 ug/l
RT: 13.036 min Scan# 11
Delta R.T. -0.000 min
Lab File: VN077513.D
Acq: 29 Apr 2023 11:35




Instrument :
MSVOA_N
ClientSampleId :
VN0429WBL01


Tgt Ion: 91 Resp: 6619
Ion Ratio Lower Upper
91 100
120 21.8 11.5 34.4

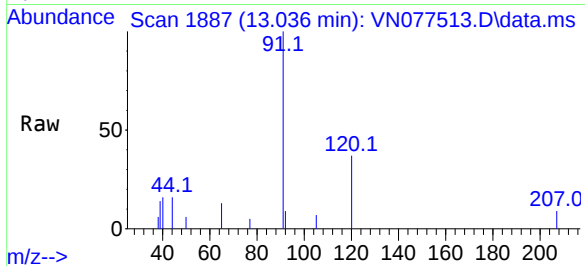

#81
trans-1,4-Dichloro-2-butene
Concen: 77.759 ug/l
RT: 12.854 min Scan# 1856
Delta R.T. 0.112 min
Lab File: VN077513.D
Acq: 29 Apr 2023 11:35

Tgt Ion: 75 Resp: 196170
Ion Ratio Lower Upper
75 100
53 0.0 67.4 101.2#
89 0.0 38.8 58.2#


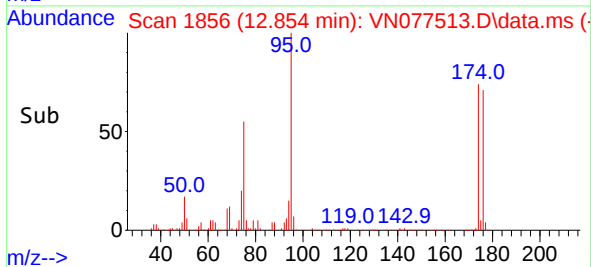

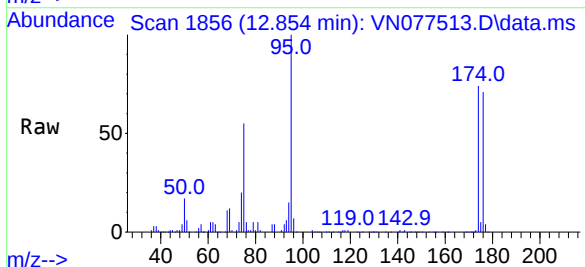




#82
4-Chlorotoluene
Concen: 0.362 ug/l
RT: 13.230 min Scan# 1919
Delta R.T. 0.006 min
Lab File: VN077513.D
Acq: 29 Apr 2023 11:35




Instrument :
MSVOA_N
ClientSampleId :
VN0429WBL01


Tgt Ion: 91 Resp: 6567
Ion Ratio Lower Upper
91 100
126 27.5 16.7 50.0

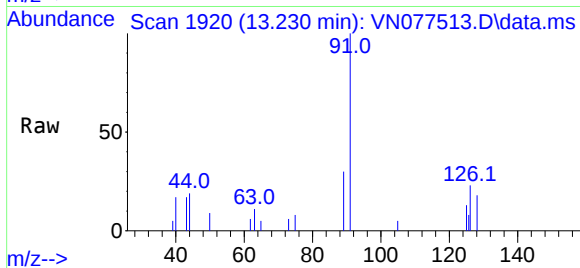

#87
1,3-Dichlorobenzene
Concen: 0.348 ug/l
RT: 13.736 min Scan# 2006
Delta R.T. -0.000 min
Lab File: VN077513.D
Acq: 29 Apr 2023 11:35

Tgt Ion: 146 Resp: 3834
Ion Ratio Lower Upper
146 100
111 65.5 22.1 66.3
148 82.7 32.0 96.0


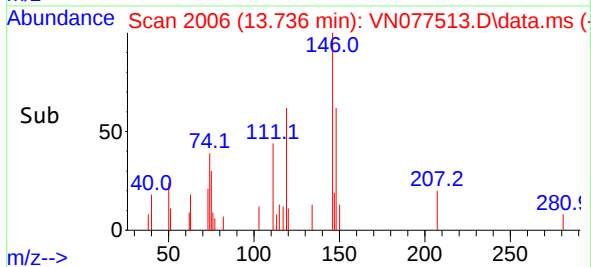

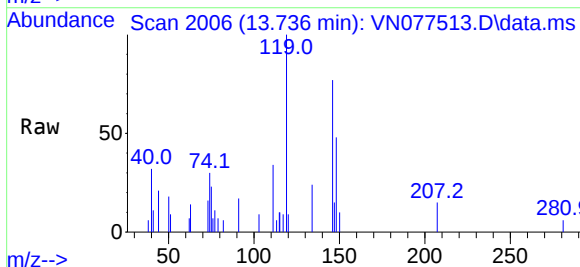




#88
1,4-Dichlorobenzene
Concen: 0.586 ug/l
RT: 13.818 min Scan# 2019
Delta R.T. 0.006 min
Lab File: VN077513.D
Acq: 29 Apr 2023 11:35




Instrument :
MSVOA_N
ClientSampleId :
VN0429WBL01


Tgt Ion:146 Resp: 6375
Ion Ratio Lower Upper
146 100
111 0.0 20.6 61.8#
148 91.5 31.6 94.8

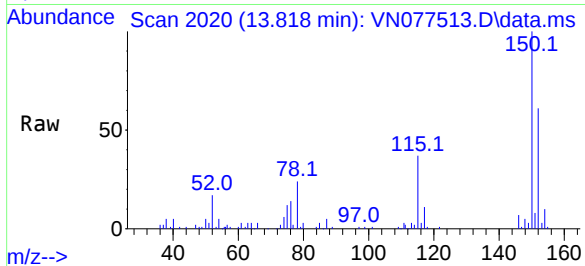

#89
n-Butylbenzene
Concen: 0.385 ug/l
RT: 14.065 min Scan# 2062
Delta R.T. 0.005 min
Lab File: VN077513.D
Acq: 29 Apr 2023 11:35

Tgt Ion: 91 Resp: 6460
Ion Ratio Lower Upper
91 100
92 59.1 26.4 79.0
134 23.6 12.6 37.6


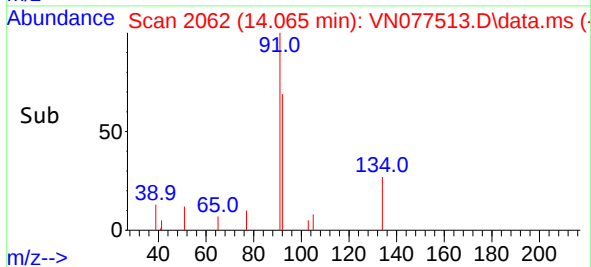

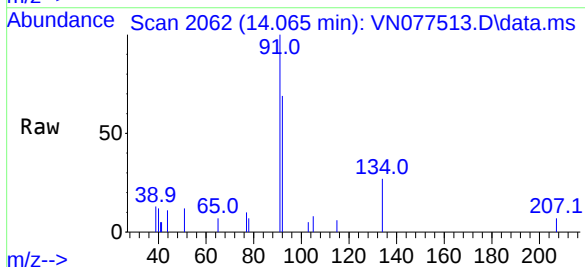




#91
1,2-Dichlorobenzene
Concen: 0.458 ug/l
RT: 14.113 min Scan# 2069
Delta R.T. 0.006 min
Lab File: VN077513.D
Acq: 29 Apr 2023 11:35




Instrument :
MSVOA_N
ClientSampleId :
VN0429WBL01


Tgt Ion:	146	Resp:	5013
Ion	Ratio	Lower	Upper
146	100		
111	36.5	22.0	66.0
148	61.4	31.8	95.3

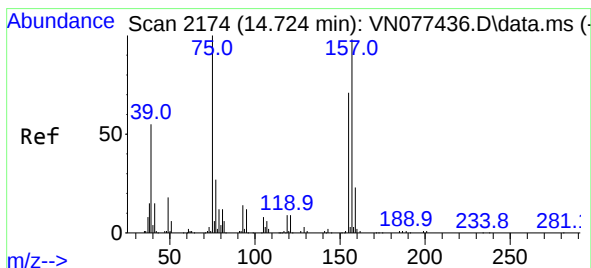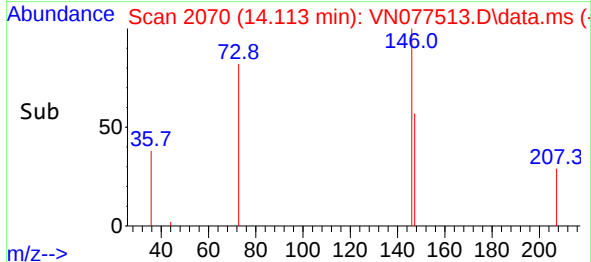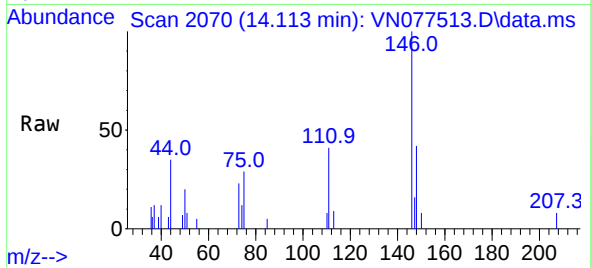

#92
1,2-Dibromo-3-Chloropropane
Concen: 0.541 ug/l
RT: 14.724 min Scan# 2174
Delta R.T. 0.000 min
Lab File: VN077513.D
Acq: 29 Apr 2023 11:35

Tgt Ion:	75	Resp:	894
Ion	Ratio	Lower	Upper
75	100		
155	80.5	39.1	117.2
157	86.2	50.3	150.9

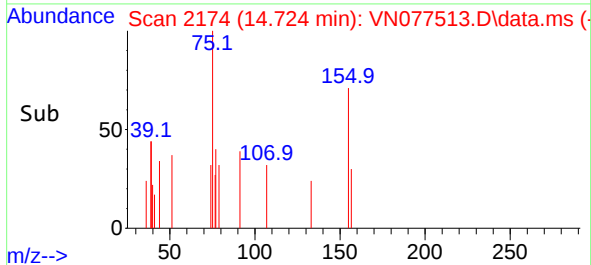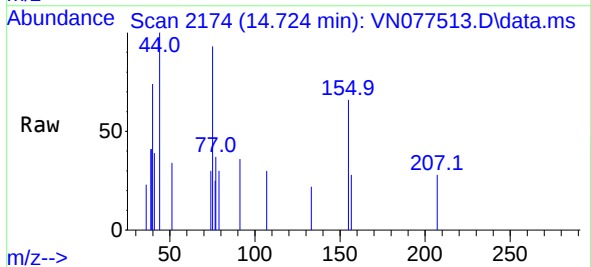



#93

1,2,4-Trichlorobenzene

Concen: 2.505 ug/l

RT: 15.401 min Scan# 21

Delta R.T. 0.030 min

Lab File: VN077513.D

Acq: 29 Apr 2023 11:35

Instrument :

MSVOA_N

ClientSampleId :

VN0429WBL01





Tgt Ion:180 Resp: 3865

Ion Ratio Lower Upper

180 100

182 107.2 46.1 138.2

145 45.1 16.6 49.8

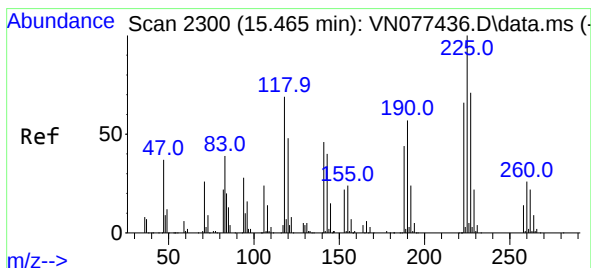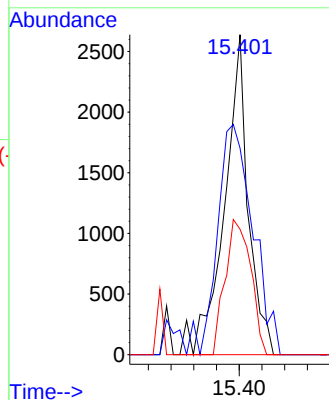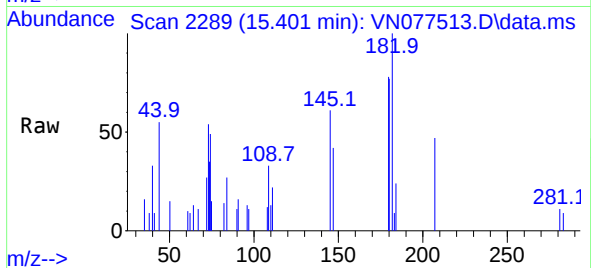

#94

Hexachlorobutadiene

Concen: 0.286 ug/l

RT: 15.495 min Scan# 2305

Delta R.T. 0.030 min

Lab File: VN077513.D

Acq: 29 Apr 2023 11:35




Tgt Ion:225 Resp: 631


Ion Ratio Lower Upper

225 100

223 61.0 31.3 93.8

227 49.3 31.9 95.9


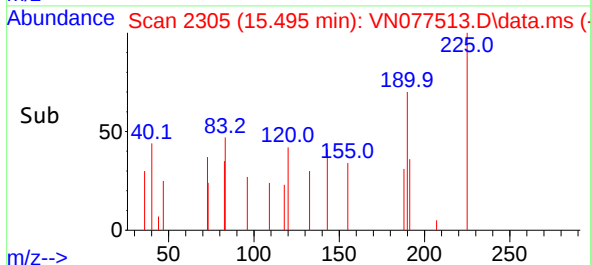
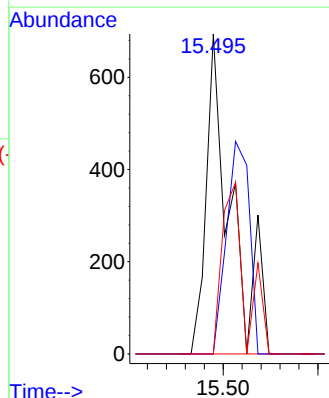
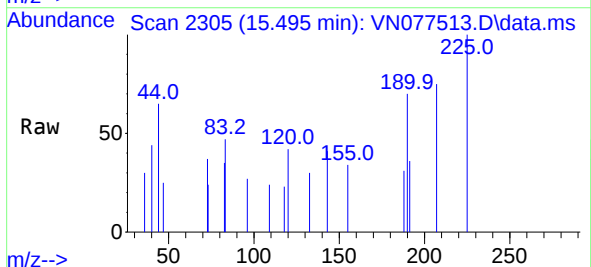




#95
Naphthalene
Concen: 1.404 ug/l
RT: 15.583 min Scan# 2162
Delta R.T. -0.006 min
Lab File: VN077513.D
Acq: 29 Apr 2023 11:35

Instrument :
MSVOA_N
ClientSampleId :
VN0429WBL01

Tgt Ion:128 Resp: 2162
Ion Ratio Lower Upper
128 100
127 0.0 10.0 15.0#
129 15.9 8.7 13.1#

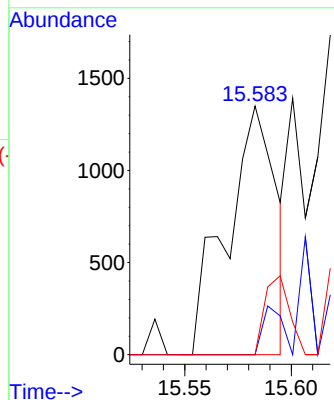

#96
1,2,3-Trichlorobenzene
Concen: 1.037 ug/l
RT: 15.795 min Scan# 2356
Delta R.T. 0.041 min
Lab File: VN077513.D
Acq: 29 Apr 2023 11:35

Tgt Ion:180 Resp: 1148
Ion Ratio Lower Upper
180 100
182 28.7 46.2 138.6#
145 28.1 17.5 52.6

