


#3
Chloromethane
Concen: 17.934 ug/l
RT: 2.360 min Scan# 69
Delta R.T. 0.000 min
Lab File: VN081917.D
Acq: 29 Apr 2024 16:45



Instrument :
MSVOA_N
ClientSampleId :
VSTDCCC020EC



Tgt Ion: 50 Resp: 50414
Ion Ratio Lower Upper
50 100
52 31.2 25.4 38.0


Manual Integrations
APPROVED

Reviewed By :John
Carlone

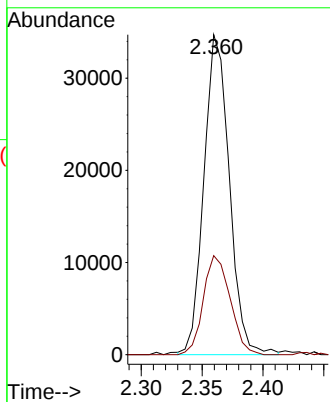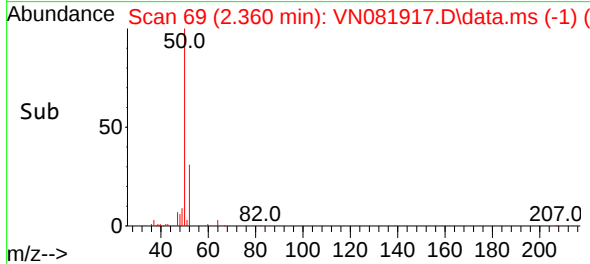


04/30/2024
Supervised By :Mahesh
Dadoda



04/30/2024




#4
Vinyl Chloride
Concen: 18.121 ug/l
RT: 2.518 min Scan# 96
Delta R.T. 0.000 min
Lab File: VN081917.D
Acq: 29 Apr 2024 16:45

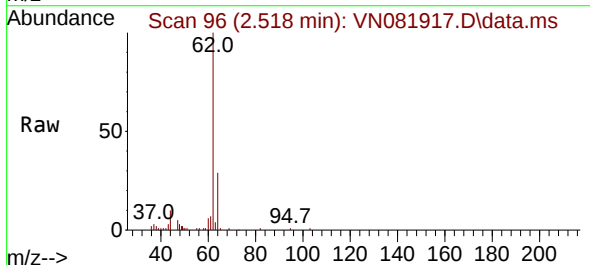


Tgt Ion: 62 Resp: 48121
Ion Ratio Lower Upper
62 100
64 25.8 24.1 36.1

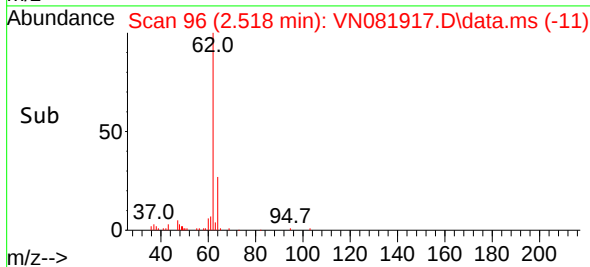



#5
Bromomethane
Concen: 15.948 ug/l
RT: 2.959 min Scan# 171
Delta R.T. -0.006 min
Lab File: VN081917.D
Acq: 29 Apr 2024 16:45



Instrument :
MSVOA_N
ClientSampleId :
VSTDCCC020EC



Tgt Ion: 94 Resp: 22099
Ion Ratio Lower Upper
94 100
96 74.9 72.8 109.2


Manual Integrations
APPROVED

Reviewed By :John
Carlone

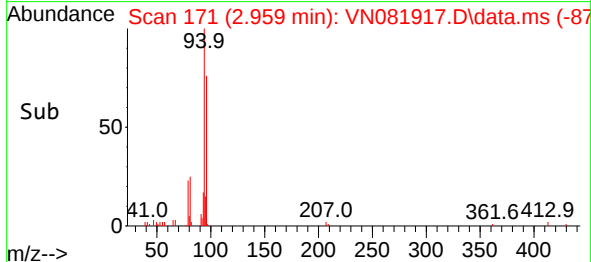




04/30/2024
Supervised By :Mahesh
Dadoda


04/30/2024



#6
Chloroethane
Concen: 18.494 ug/l
RT: 3.124 min Scan# 199
Delta R.T. 0.000 min
Lab File: VN081917.D
Acq: 29 Apr 2024 16:45

Tgt Ion: 64 Resp: 27810
Ion Ratio Lower Upper
64 100
66 34.5 26.7 40.1

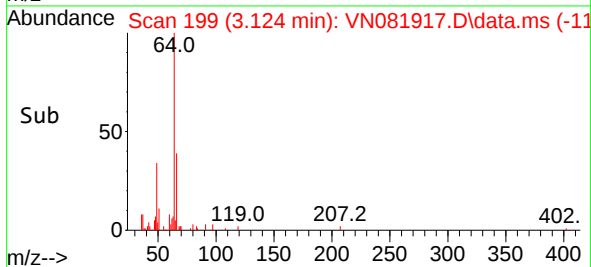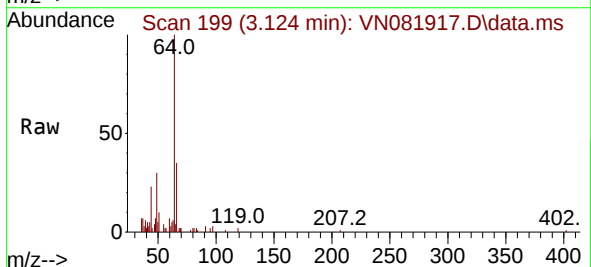





#7
 Trichlorofluoromethane
 Concen: 19.518 ug/l
 RT: 3.501 min Scan# 263
 Delta R.T. 0.000 min
 Lab File: VN081917.D
 Acq: 29 Apr 2024 16:45

Instrument :
 MSVOA_N
 ClientSampleId :
 VSTDCCC020EC

Tgt Ion:101 Resp: 75840
 Ion Ratio Lower Upper
 101 100
 103 56.2 53.0 79.4



Manual Integrations
 APPROVED

Reviewed By :John
 Carlone

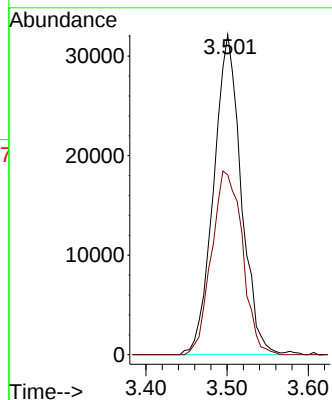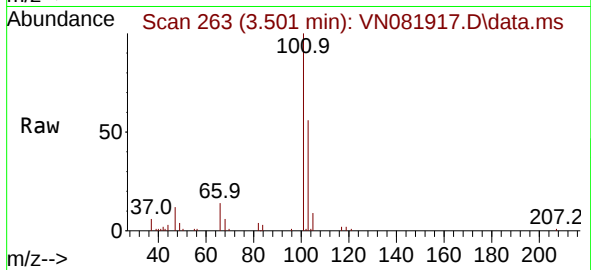




04/30/2024
 Supervised By :Mahesh
 Dadoda


04/30/2024

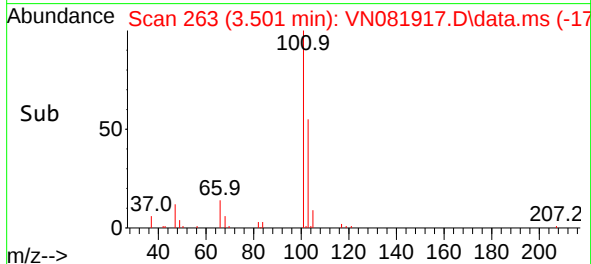

#8
 Diethyl Ether
 Concen: 19.311 ug/l
 RT: 3.959 min Scan# 341
 Delta R.T. 0.000 min
 Lab File: VN081917.D
 Acq: 29 Apr 2024 16:45


Tgt Ion: 74 Resp: 36325
 Ion Ratio Lower Upper
 74 100
 45 93.4 16.4 147.4

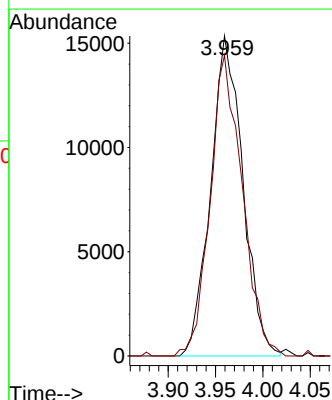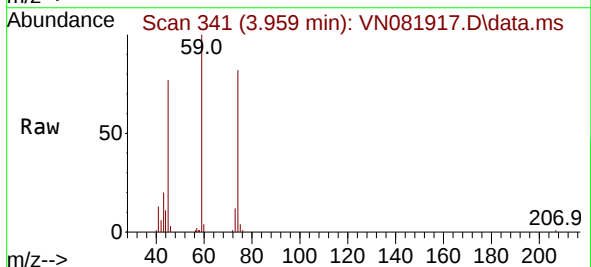



#11
Methyl Iodide
Concen: 19.271 ug/l
RT: 4.595 min Scan# 449
Delta R.T. 0.000 min
Lab File: VN081917.D
Acq: 29 Apr 2024 16:45



Instrument :
MSVOA_N
ClientSampleId :
VSTDCCC020EC



Tgt Ion:142 Resp: 45899
Ion Ratio Lower Upper
142 100
127 38.4 26.3 78.9
141 11.2 8.3 24.9


Manual Integrations
APPROVED

Reviewed By :John
Carlone

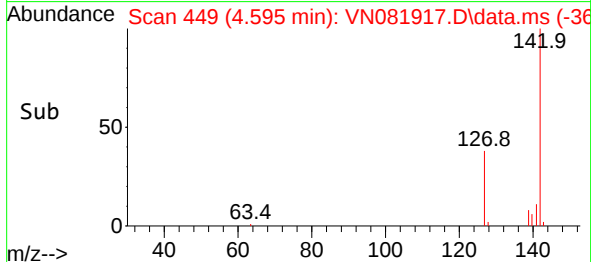


04/30/2024
Supervised By :Mahesh
Dadoda



04/30/2024




#12
Methyl Acetate
Concen: 19.395 ug/l
RT: 5.030 min Scan# 523
Delta R.T. 0.000 min
Lab File: VN081917.D
Acq: 29 Apr 2024 16:45

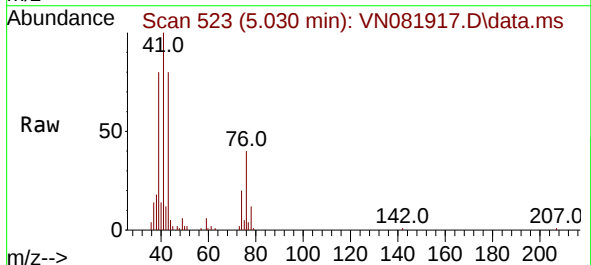


Tgt Ion: 43 Resp: 63292
Ion Ratio Lower Upper
43 100
74 25.2 27.7 41.5#

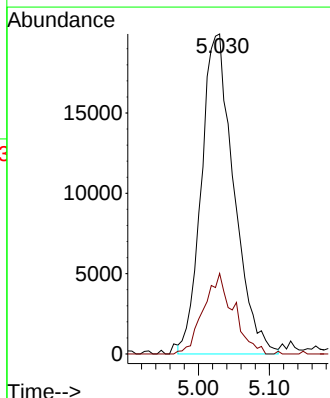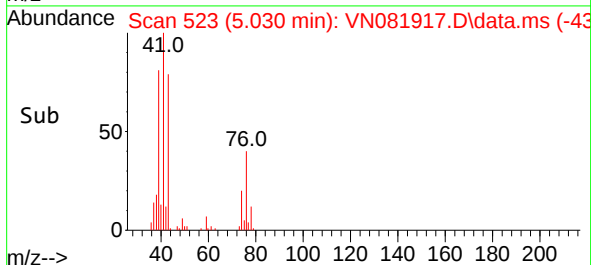



#15
Acetone
Concen: 103.225 ug/l
RT: 4.436 min Scan# 41
Delta R.T. 0.012 min
Lab File: VN081917.D
Acq: 29 Apr 2024 16:45



Instrument :
MSVOA_N
ClientSampleId :
VSTDCCC020EC



Tgt Ion: 58 Resp: 34450
Ion Ratio Lower Upper
58 100
43 275.4 223.1 334.7


Manual Integrations
APPROVED

Reviewed By :John
Carlone

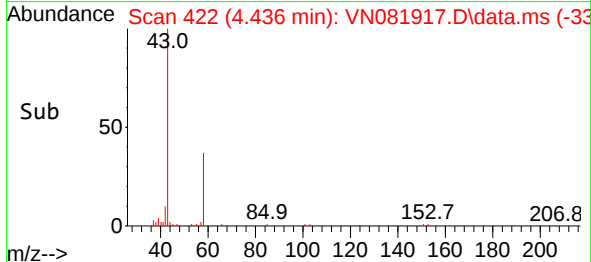


04/30/2024
Supervised By :Mahesh
Dadoda



04/30/2024




#16
Carbon Disulfide
Concen: 18.363 ug/l
RT: 4.718 min Scan# 470
Delta R.T. 0.000 min
Lab File: VN081917.D
Acq: 29 Apr 2024 16:45

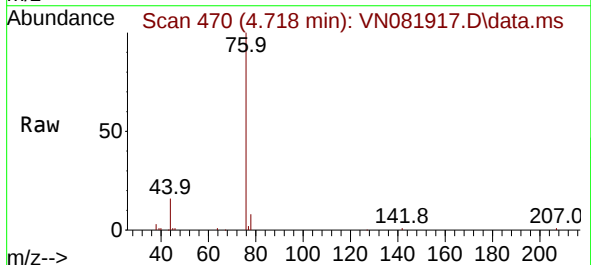


Tgt Ion: 76 Resp: 132582
Ion Ratio Lower Upper
76 100
78 8.1 6.3 9.5

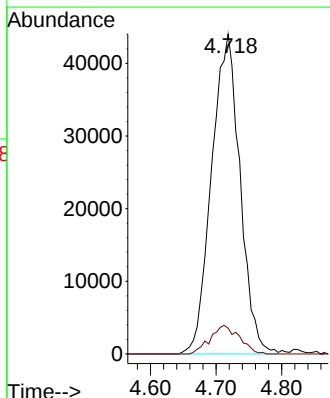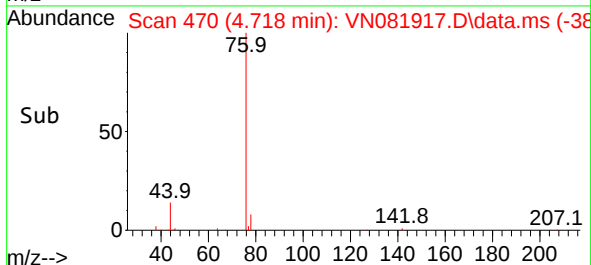



#17
 Allyl chloride
 Concen: 18.968 ug/l
 RT: 5.024 min Scan# 51
 Delta R.T. 0.006 min
 Lab File: VN081917.D
 Acq: 29 Apr 2024 16:45



Instrument :
 MSVOA_N
 ClientSampleId :
 VSTDCCC020EC



Tgt Ion: 41 Resp: 86788
 Ion Ratio Lower Upper
 41 100
 39 71.5 37.6 112.9
 76 45.1 27.8 83.4


Manual Integrations
 APPROVED

Reviewed By :John
 Carlone

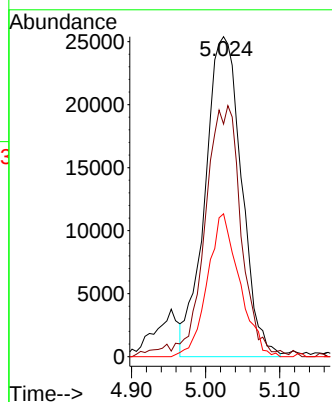




04/30/2024
 Supervised By :Mahesh
 Dadoda


04/30/2024



#18
 Methylene Chloride
 Concen: 18.775 ug/l
 RT: 5.283 min Scan# 566
 Delta R.T. -0.006 min
 Lab File: VN081917.D
 Acq: 29 Apr 2024 16:45


Tgt Ion: 84 Resp: 55674
 Ion Ratio Lower Upper
 84 100
 49 132.4 86.0 129.0#
 51 41.0 30.0 45.0
 86 71.2 53.0 79.4

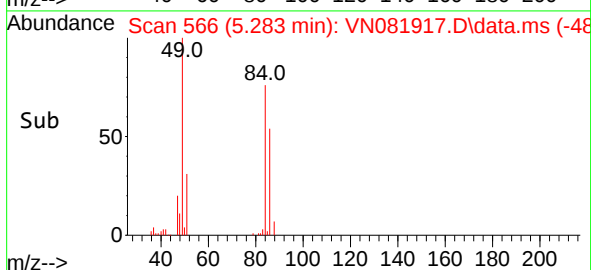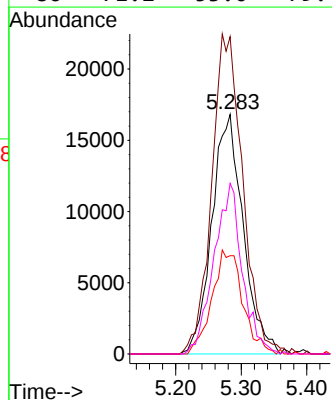



#21
1,1-Dichloroethane
Concen: 19.235 ug/l
RT: 6.577 min Scan# 785
Delta R.T. 0.006 min
Lab File: VN081917.D
Acq: 29 Apr 2024 16:45



Instrument :
MSVOA_N
ClientSampleId :
VSTDCCC020EC



Tgt Ion: 63 Resp: 103108
Ion Ratio Lower Upper
63 100
98 5.2 4.1 12.3
100 4.8 3.0 9.0


Manual Integrations
APPROVED

Reviewed By :John
Carlone

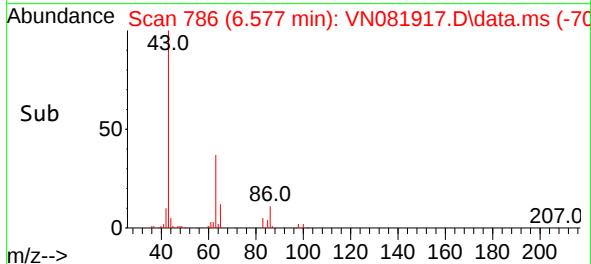




04/30/2024
Supervised By :Mahesh
Dadoda


04/30/2024



#22
cis-1,2-Dichloroethene
Concen: 19.223 ug/l
RT: 7.489 min Scan# 941
Delta R.T. 0.006 min
Lab File: VN081917.D
Acq: 29 Apr 2024 16:45


Tgt Ion: 96 Resp: 63547
Ion Ratio Lower Upper
96 100
61 149.7 113.5 170.3
98 66.9 52.0 78.0

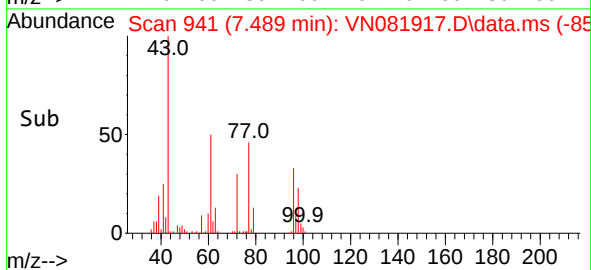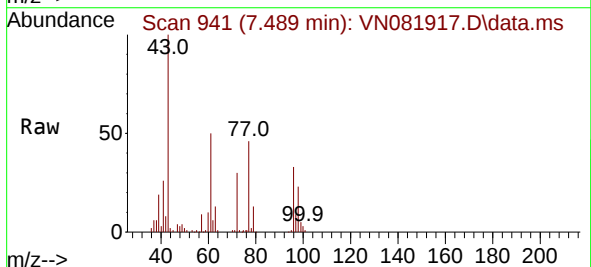

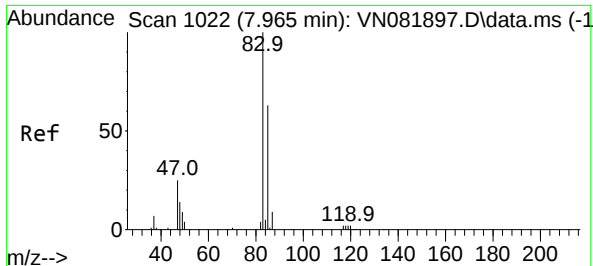

#25
Chloroform
Concen: 18.903 ug/l
RT: 7.971 min Scan# 1023
Delta R.T. 0.006 min
Lab File: VN081917.D
Acq: 29 Apr 2024 16:45



Instrument :
MSVOA_N
ClientSampleId :
VSTDCCC020EC

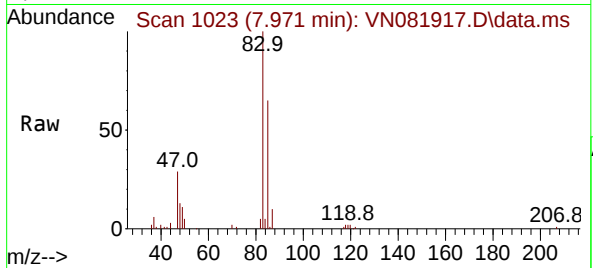

Tgt Ion: 83 Resp: 97484
Ion Ratio Lower Upper
83 100
85 65.0 50.9 76.3


Manual Integrations
APPROVED

Reviewed By :John
Carlone

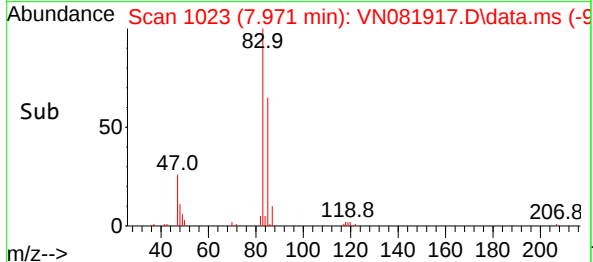




04/30/2024
Supervised By :Mahesh
Dadoda


04/30/2024

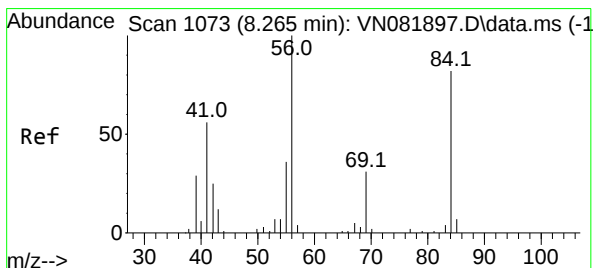

#26
Cyclohexane
Concen: 19.354 ug/l
RT: 8.259 min Scan# 1072
Delta R.T. -0.006 min
Lab File: VN081917.D
Acq: 29 Apr 2024 16:45


Tgt Ion: 56 Resp: 89716
Ion Ratio Lower Upper
56 100
89 0.6 19.3 28.9#
84 88.0 71.3 106.9

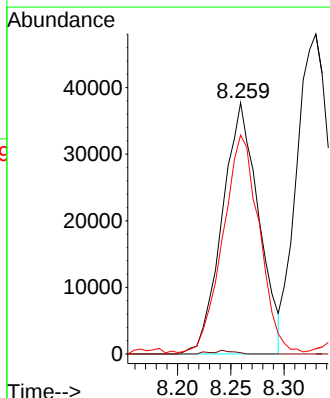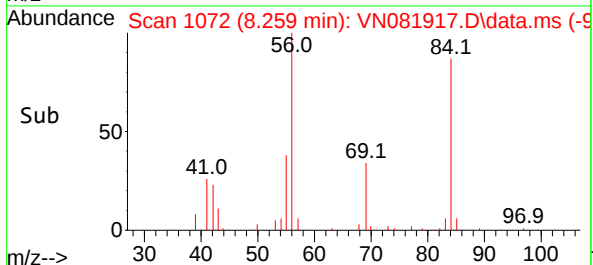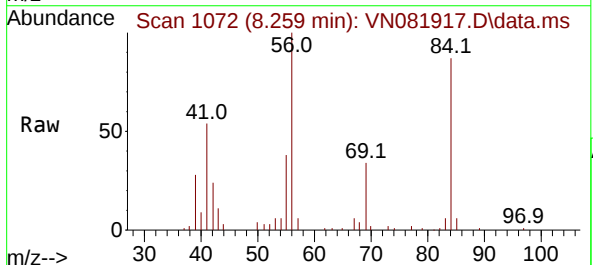



#29
1,1-Dichloropropene
Concen: 18.774 ug/l m
RT: 8.371 min Scan# 1092
Delta R.T. -0.006 min
Lab File: VN081917.D
Acq: 29 Apr 2024 16:45



Instrument :
MSVOA_N
ClientSampleId :
VSTDCCC020EC



Tgt Ion: 75 Resp: 71780
Ion Ratio Lower Upper
75 100
110 32.6 0.0 70.2
77 31.7 0.0 61.4


Manual Integrations
APPROVED

Reviewed By :John
Carlone

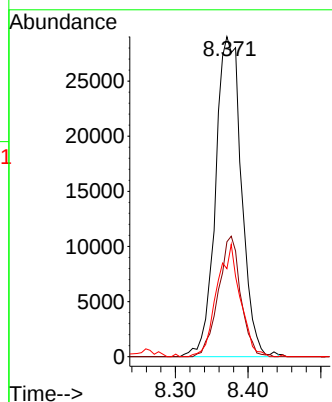




04/30/2024
Supervised By :Mahesh
Dadoda


04/30/2024



#30
2-Butanone
Concen: 92.727 ug/l
RT: 7.489 min Scan# 941
Delta R.T. 0.006 min
Lab File: VN081917.D
Acq: 29 Apr 2024 16:45


Tgt Ion: 43 Resp: 182761
Ion Ratio Lower Upper
43 100
57 8.4 6.7 10.1
72 28.8 24.0 36.0

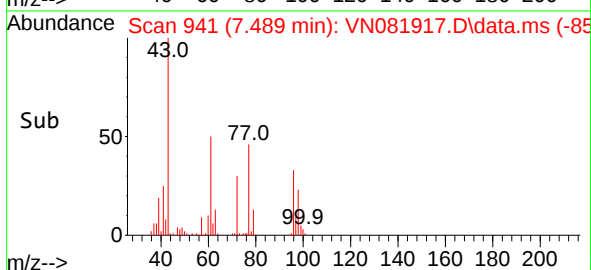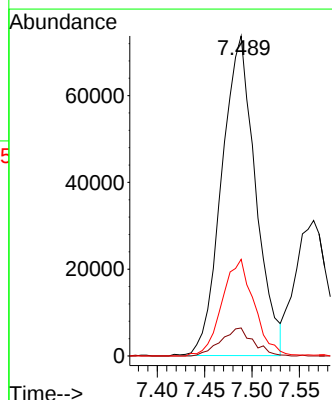



#33
Carbon Tetrachloride
Concen: 18.601 ug/l
RT: 8.365 min Scan# 1090
Delta R.T. 0.000 min
Lab File: VN081917.D
Acq: 29 Apr 2024 16:45



Instrument :
MSVOA_N
ClientSampleId :
VSTDCCC020EC



Tgt Ion: 117 Resp: 6638
Ion Ratio Lower Upper
117 100
119 90.1 77.7 116.5
121 30.1 27.0 40.6


Manual Integrations
APPROVED

Reviewed By :John
Carlone

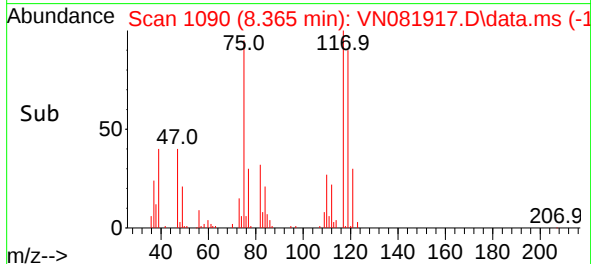




04/30/2024
Supervised By :Mahesh
Dadoda


04/30/2024



#34
Benzene
Concen: 19.159 ug/l
RT: 8.606 min Scan# 1131
Delta R.T. 0.000 min
Lab File: VN081917.D
Acq: 29 Apr 2024 16:45


Tgt Ion: 78 Resp: 233701
Ion Ratio Lower Upper
78 100
77 24.6 19.2 28.8
51 18.7 13.3 19.9

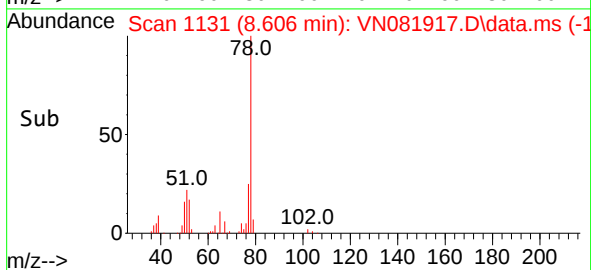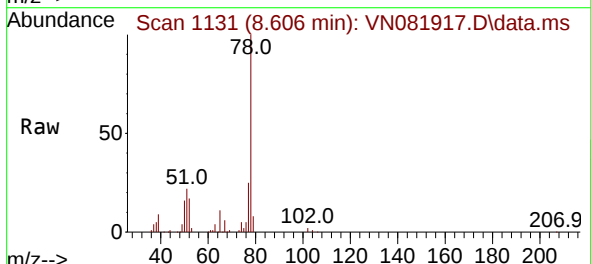

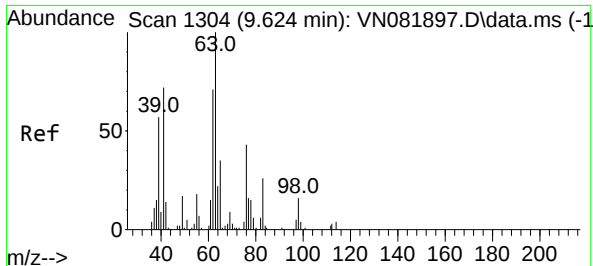

#39
1,2-Dichloropropane
Concen: 19.945 ug/l
RT: 9.624 min Scan# 1304
Delta R.T. 0.000 min
Lab File: VN081917.D
Acq: 29 Apr 2024 16:45



Instrument :
MSVOA_N
ClientSampleId :
VSTDCCC020EC

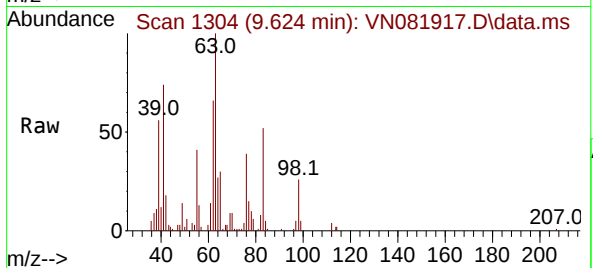

Tgt Ion: 63 Resp: 6242
Ion Ratio Lower Upper
63 100
65 29.7 25.0 37.4


Manual Integrations
APPROVED

Reviewed By :John
Carlone

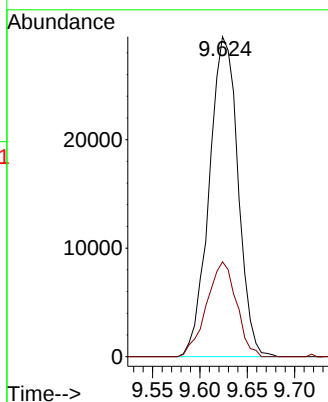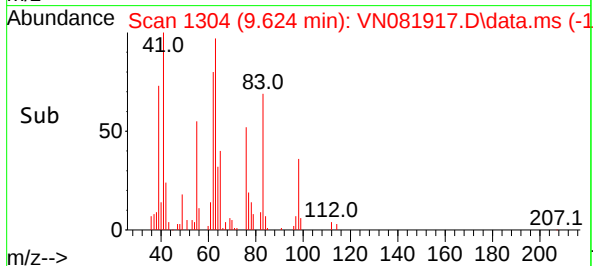




04/30/2024
Supervised By :Mahesh
Dadoda


04/30/2024

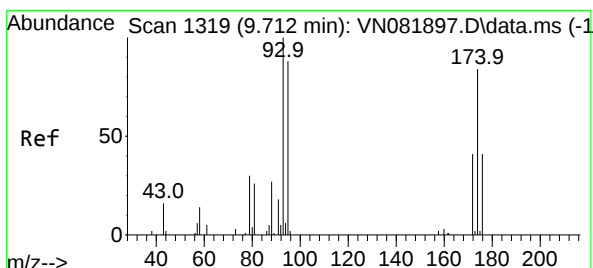

#40
Dibromomethane
Concen: 18.223 ug/l
RT: 9.712 min Scan# 1319
Delta R.T. 0.000 min
Lab File: VN081917.D
Acq: 29 Apr 2024 16:45


Tgt Ion: 93 Resp: 36641
Ion Ratio Lower Upper
93 100
95 85.6 0.0 164.6
174 81.7 0.0 193.2

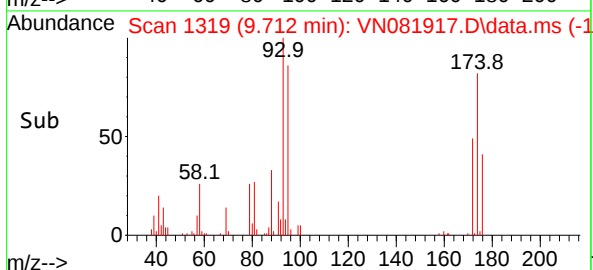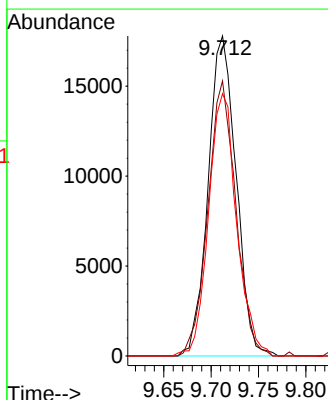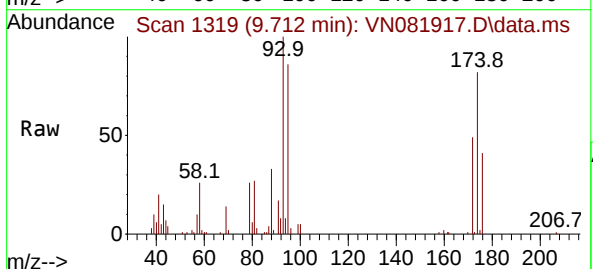



#43
Ethyl Acetate
Concen: 17.994 ug/l
RT: 7.565 min Scan# 911
Delta R.T. 0.012 min
Lab File: VN081917.D
Acq: 29 Apr 2024 16:45



Instrument :
MSVOA_N
ClientSampleId :
VSTDCCC020EC



Tgt Ion: 43 Resp: 77325
Ion Ratio Lower Upper
43 100
45 15.5 10.6 15.8


Manual Integrations
APPROVED

Reviewed By :John
Carlone

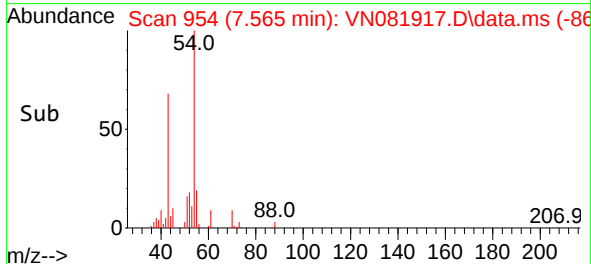


04/30/2024
Supervised By :Mahesh
Dadoda



04/30/2024




#44
Isopropyl Acetate
Concen: 18.504 ug/l
RT: 8.694 min Scan# 1146
Delta R.T. 0.006 min
Lab File: VN081917.D
Acq: 29 Apr 2024 16:45

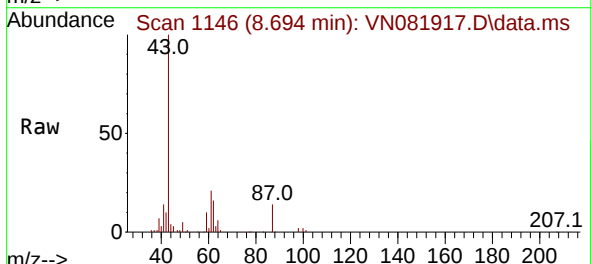


Tgt Ion: 43 Resp: 141170
Ion Ratio Lower Upper
43 100
61 26.1 25.0 37.4

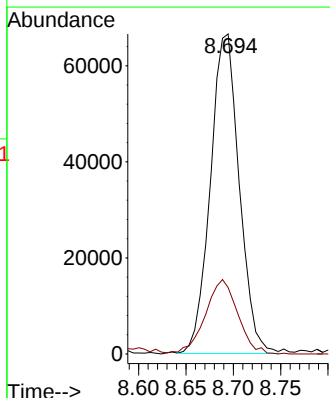

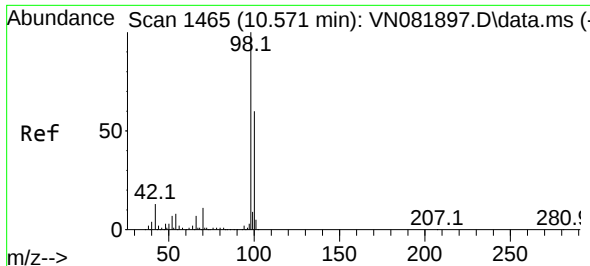

#63
Toluene-d8
Concen: 29.592 ug/l
RT: 10.571 min Scan# 1465
Delta R.T. 0.000 min
Lab File: VN081917.D
Acq: 29 Apr 2024 16:45



Instrument :
MSVOA_N
ClientSampleId :
VSTDCCC020EC



Tgt Ion: 98 Resp: 32177
Ion Ratio Lower Upper
98 100
100 66.0 52.7 79.1


Manual Integrations
APPROVED

Reviewed By :John
Carlone

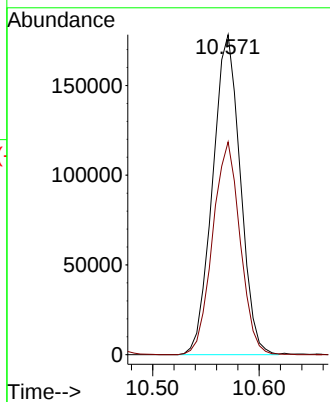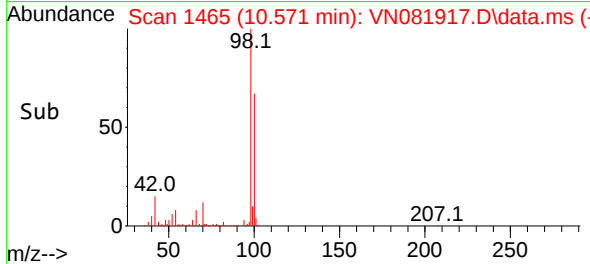


04/30/2024
Supervised By :Mahesh
Dadoda



04/30/2024




#64
Chlorobenzene
Concen: 19.049 ug/l
RT: 11.894 min Scan# 1690
Delta R.T. 0.000 min
Lab File: VN081917.D
Acq: 29 Apr 2024 16:45

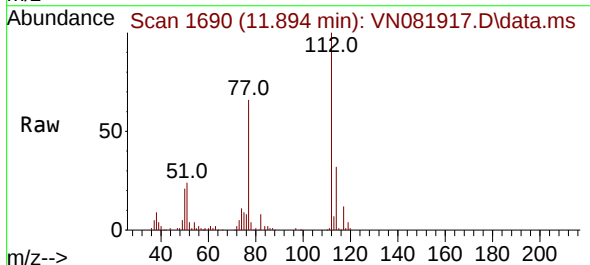


Tgt Ion:112 Resp: 150101
Ion Ratio Lower Upper
112 100
114 32.2 26.6 39.8

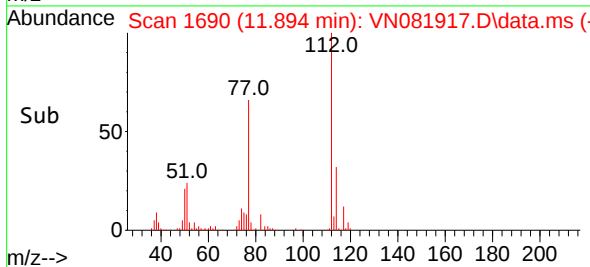



#69
Styrene
Concen: 18.620 ug/l
RT: 12.412 min Scan# 1778
Delta R.T. 0.000 min
Lab File: VN081917.D
Acq: 29 Apr 2024 16:45



Instrument :
MSVOA_N
ClientSampleId :
VSTDCCC020EC



Tgt Ion:104 Resp: 161910
Ion Ratio Lower Upper
104 100
78 52.2 42.6 64.0
103 53.7 43.7 65.5


Manual Integrations
APPROVED

Reviewed By :John
Carlone

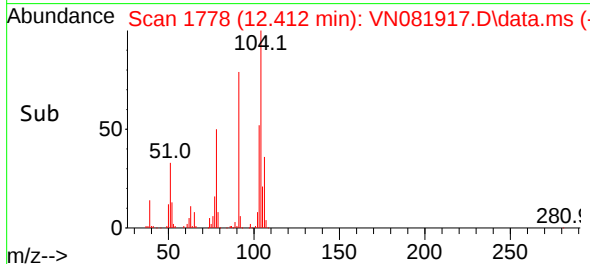


04/30/2024
Supervised By :Mahesh
Dadoda



04/30/2024




#70
Isopropylbenzene
Concen: 18.914 ug/l
RT: 12.700 min Scan# 1827
Delta R.T. 0.006 min
Lab File: VN081917.D
Acq: 29 Apr 2024 16:45

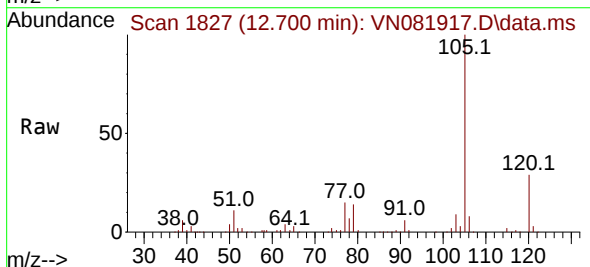


Tgt Ion:105 Resp: 248832
Ion Ratio Lower Upper
105 100
120 26.3 17.8 33.1

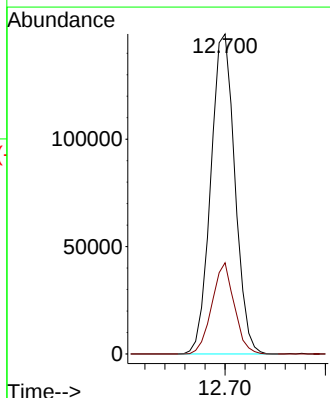

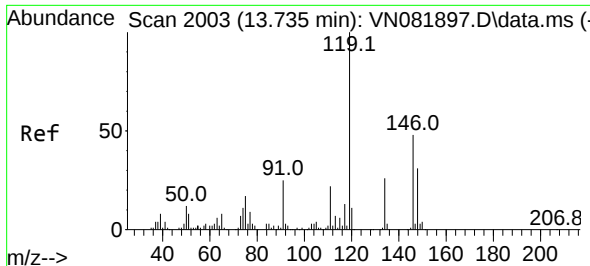

#83
1,3-Dichlorobenzene
Concen: 19.258 ug/l
RT: 13.735 min Scan# 2003
Delta R.T. 0.000 min
Lab File: VN081917.D
Acq: 29 Apr 2024 16:45



Instrument :
MSVOA_N
ClientSampleId :
VSTDCCC020EC



Tgt Ion:146 Resp: 9765
Ion Ratio Lower Upper
146 100
111 43.2 22.4 67.0
148 63.9 32.1 96.5


Manual Integrations
APPROVED

Reviewed By :John
Carlone

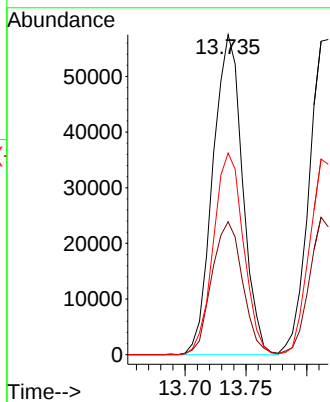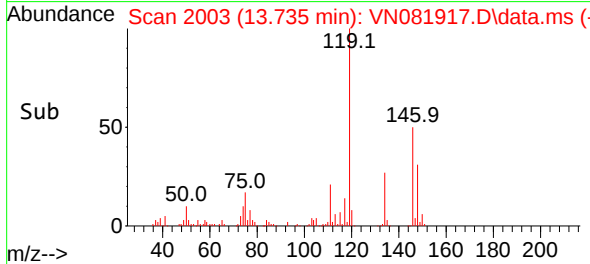


04/30/2024
Supervised By :Mahesh
Dadoda



04/30/2024




#84
1,4-Dichlorobenzene
Concen: 19.123 ug/l
RT: 13.818 min Scan# 2017
Delta R.T. 0.006 min
Lab File: VN081917.D
Acq: 29 Apr 2024 16:45

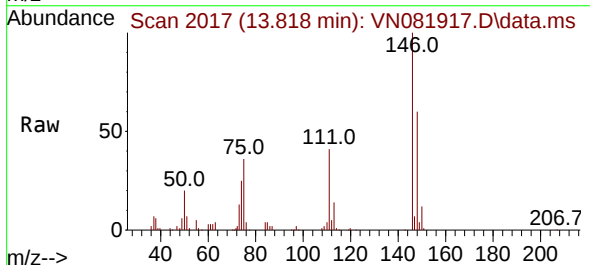

Tgt Ion:146 Resp: 97468
Ion Ratio Lower Upper
146 100
111 41.6 21.3 63.9
148 61.6 31.9 95.5

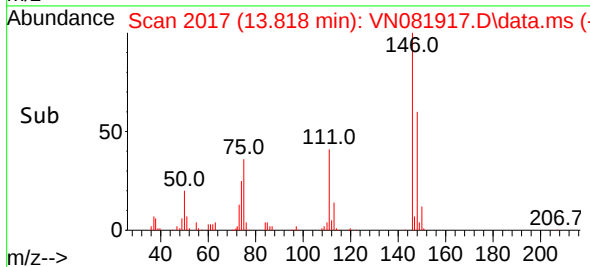





#85
n-Butylbenzene
Concen: 19.750 ug/l
RT: 14.059 min Scan# 2058
Delta R.T. 0.000 min
Lab File: VN081917.D
Acq: 29 Apr 2024 16:45

Instrument :
MSVOA_N
ClientSampleId :
VSTDCCC020EC

Tgt Ion: 91 Resp: 183340
Ion Ratio Lower Upper
91 100
92 54.9 0.0 105.0
134 23.5 0.0 51.8



Manual Integrations
APPROVED

Reviewed By :John
Carlone

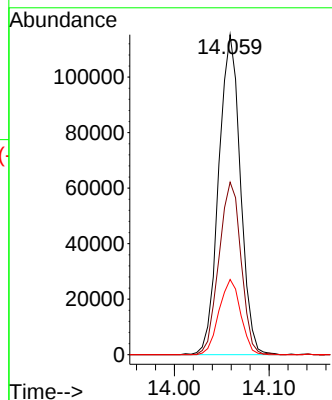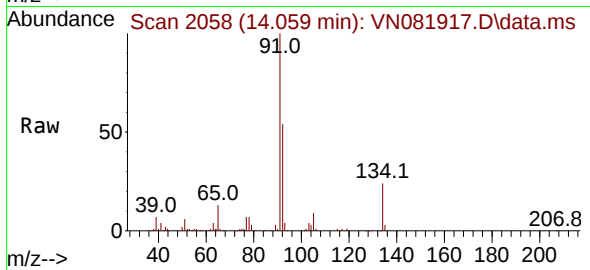

04/30/2024
Supervised By :Mahesh
Dadoda

04/30/2024

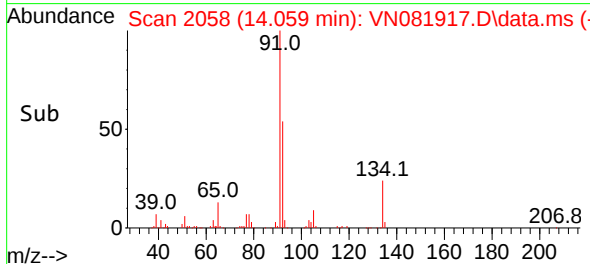

#86
Hexachloroethane
Concen: 19.277 ug/l
RT: 14.335 min Scan# 2105
Delta R.T. 0.000 min
Lab File: VN081917.D
Acq: 29 Apr 2024 16:45

Tgt Ion:117 Resp: 39062
Ion Ratio Lower Upper
117 100
201 54.8 38.0 114.0

