
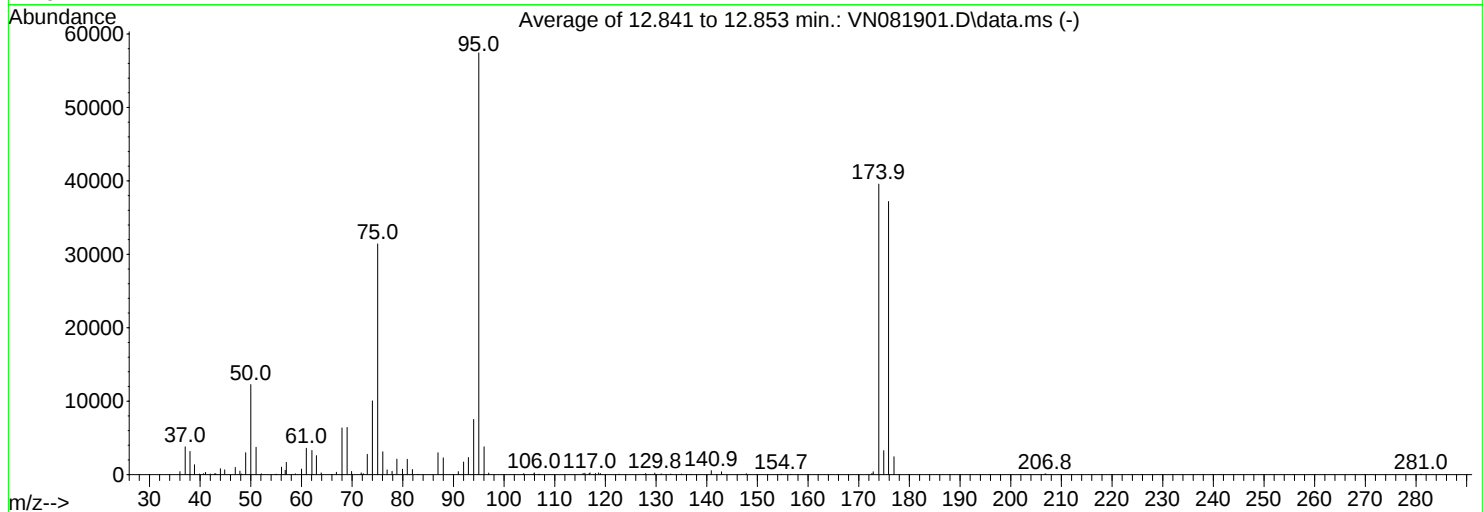


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN042924\
Data File : VN081901.D
Acq On : 29 Apr 2024 08:32
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N042624W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Sat Apr 27 04:37:27 2024

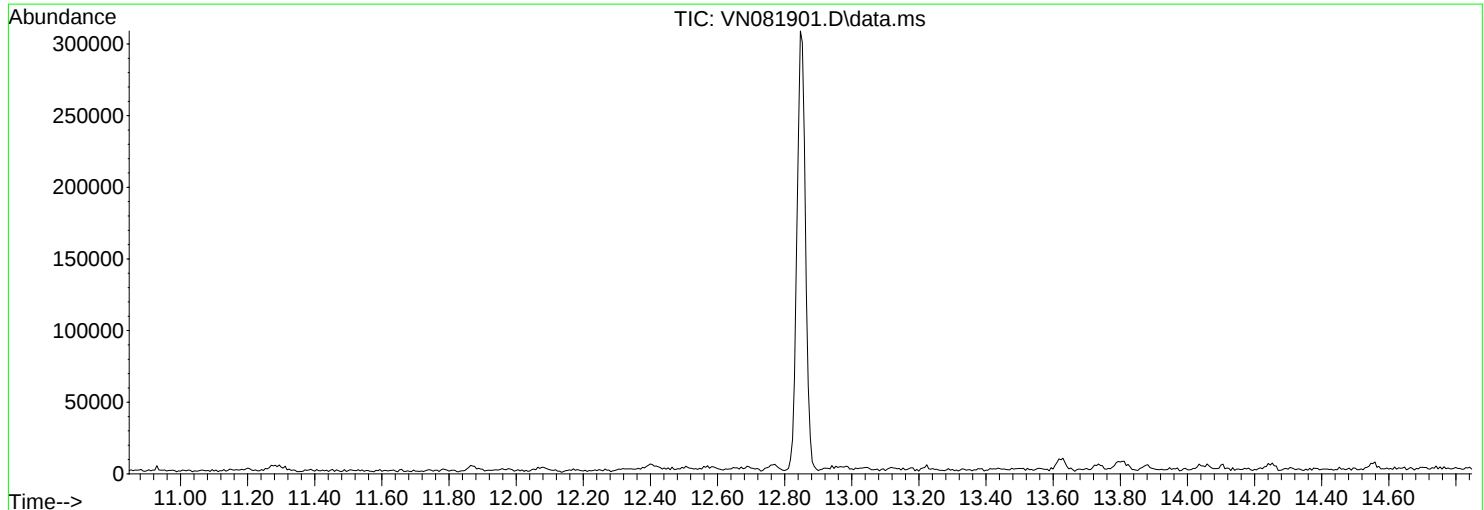

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.4	12263	PASS
75	95	30	60	54.7	31421	PASS
95	95	100	100	100.0	57437	PASS
96	95	5	9	6.6	3790	PASS
173	174	0.00	2	1.0	387	PASS
174	95	50	100	68.9	39576	PASS
175	174	5	9	8.3	3276	PASS
176	174	95	101	94.0	37195	FAIL*
177	176	5	9	6.6	2450	PASS