


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN043019\
Data File : VN055297.D
Acq On : 30 Apr 2019 10:23
Operator : JC/SP
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N042919W.M
Title : SW846 8260
Last Update : Tue Apr 30 07:16:52 2019

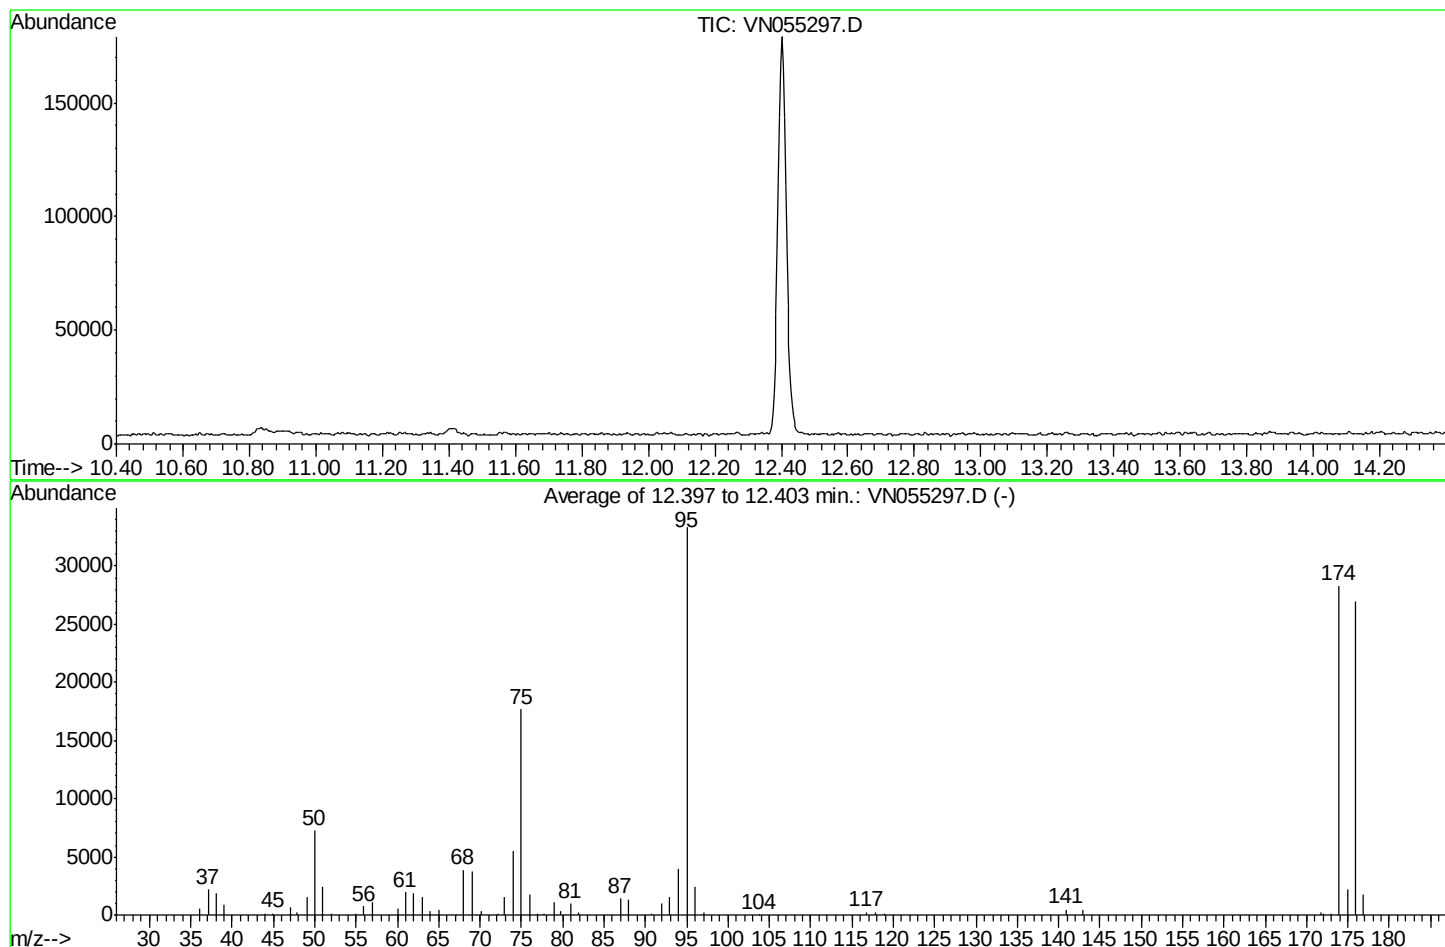

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3292

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.7	7243	PASS
75	95	30	60	53.1	17682	PASS
95	95	100	100	100.0	33330	PASS
96	95	5	9	7.1	2376	PASS
173	174	0.00	2	0.5	151	PASS
174	95	50	100	84.9	28309	PASS
175	174	5	9	7.6	2158	PASS
176	174	95	101	95.2	26962	PASS
177	176	5	9	6.6	1770	PASS