

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN043021\
 Data File : VN066908.D
 Acq On : 30 Apr 2021 14:30
 Operator : JC/MD
 Sample : M2204-05 200X
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 ANTIFREEZE-1906

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N042721W.M

Title : SW846 8260

Signal : TIC: VN066908.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.753	737	757	782	rBV	92051	239500	15.27%	3.041%
2	5.963	1563	1581	1606	rBV5	10344	36029	2.30%	0.458%
3	7.513	2136	2159	2173	rBV	206454	520725	33.19%	6.612%
4	7.591	2173	2188	2214	rVB	358938	869219	55.40%	11.038%
5	7.953	2303	2323	2354	rBV	214218	513089	32.70%	6.515%
6	8.519	2514	2534	2569	rBV	506145	1065233	67.90%	13.527%
7	10.029	3080	3097	3114	rBV	850640	1568871	100.00%	19.922%
8	10.093	3116	3121	3139	rVB	34901	57742	3.68%	0.733%
9	11.351	3573	3590	3619	rBV	610791	1153640	73.53%	14.649%
10	12.349	3947	3962	4004	rBV	368403	855402	54.52%	10.862%
11	13.290	4299	4313	4379	rBV	390111	995565	63.46%	12.642%


Sum of corrected areas: 7875015

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN043021\
Data File : VN066908.D
Acq On : 30 Apr 2021 14:30
Operator : JC/MD
Sample : M2204-05 200X
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
ANTIFREEZE-1906

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N042721W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

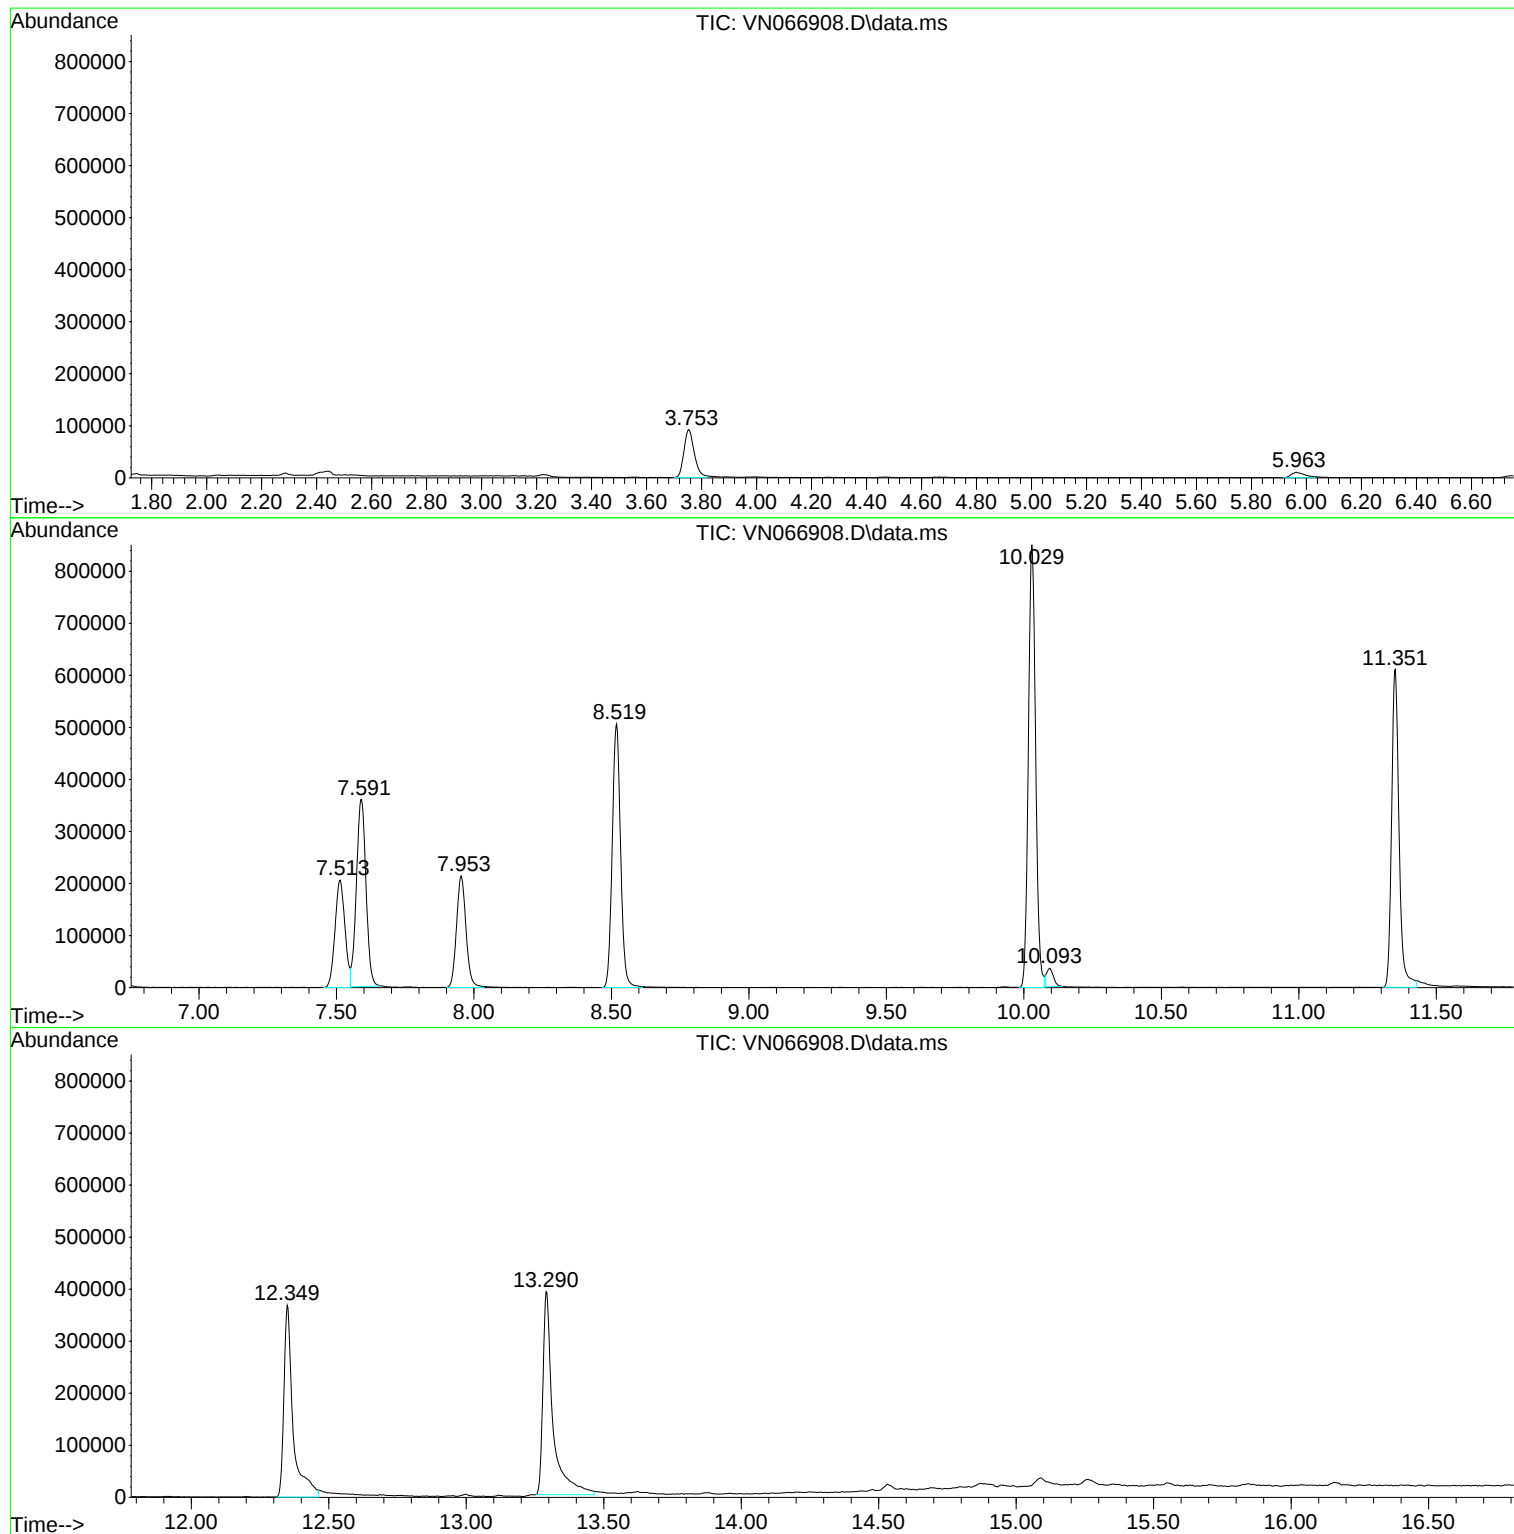

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN043021\
Data File : VN066908.D
Acq On : 30 Apr 2021 14:30
Operator : JC/MD
Sample : M2204-05 200X
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
ANTIFREEZE-1906

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N042721W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN043021\
Data File : VN066908.D
Acq On : 30 Apr 2021 14:30
Operator : JC/MD
Sample : M2204-05 200X
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
ANTIFREEZE-1906

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N042721W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
