

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN043021\
 Data File : VN066911.D
 Acq On : 30 Apr 2021 15:42
 Operator : JC/MD
 Sample : M2204-05 100X
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 ANTIFREEZE-1906

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N042721W.M

Title : SW846 8260

Signal : TIC: VN066911.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.225	550	560	576	rVB	9061	20037	1.16%	0.221%
2	3.753	736	757	794	rBV	181974	479121	27.68%	5.275%
3	5.955	1563	1578	1605	rBV5	19337	67366	3.89%	0.742%
4	7.513	2137	2159	2173	rBV	230494	579958	33.51%	6.385%
5	7.591	2174	2188	2221	rVB	402775	963372	55.67%	10.606%
6	7.953	2300	2323	2359	rBV	238149	578368	33.42%	6.367%
7	8.519	2514	2534	2563	rBV	558477	1174859	67.89%	12.934%
8	10.029	3075	3097	3113	rBV	957329	1730624	100.00%	19.052%
9	10.093	3114	3121	3159	rVB	60896	115854	6.69%	1.275%
10	11.351	3572	3590	3618	rBV	678582	1268514	73.30%	13.965%
11	12.349	3947	3962	4023	rBV	424577	997180	57.62%	10.978%
12	13.290	4297	4313	4368	rBV	445194	1108358	64.04%	12.202%


Sum of corrected areas: 9083611

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN043021\
Data File : VN066911.D
Acq On : 30 Apr 2021 15:42
Operator : JC/MD
Sample : M2204-05 100X
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
ANTIFREEZE-1906

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N042721W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

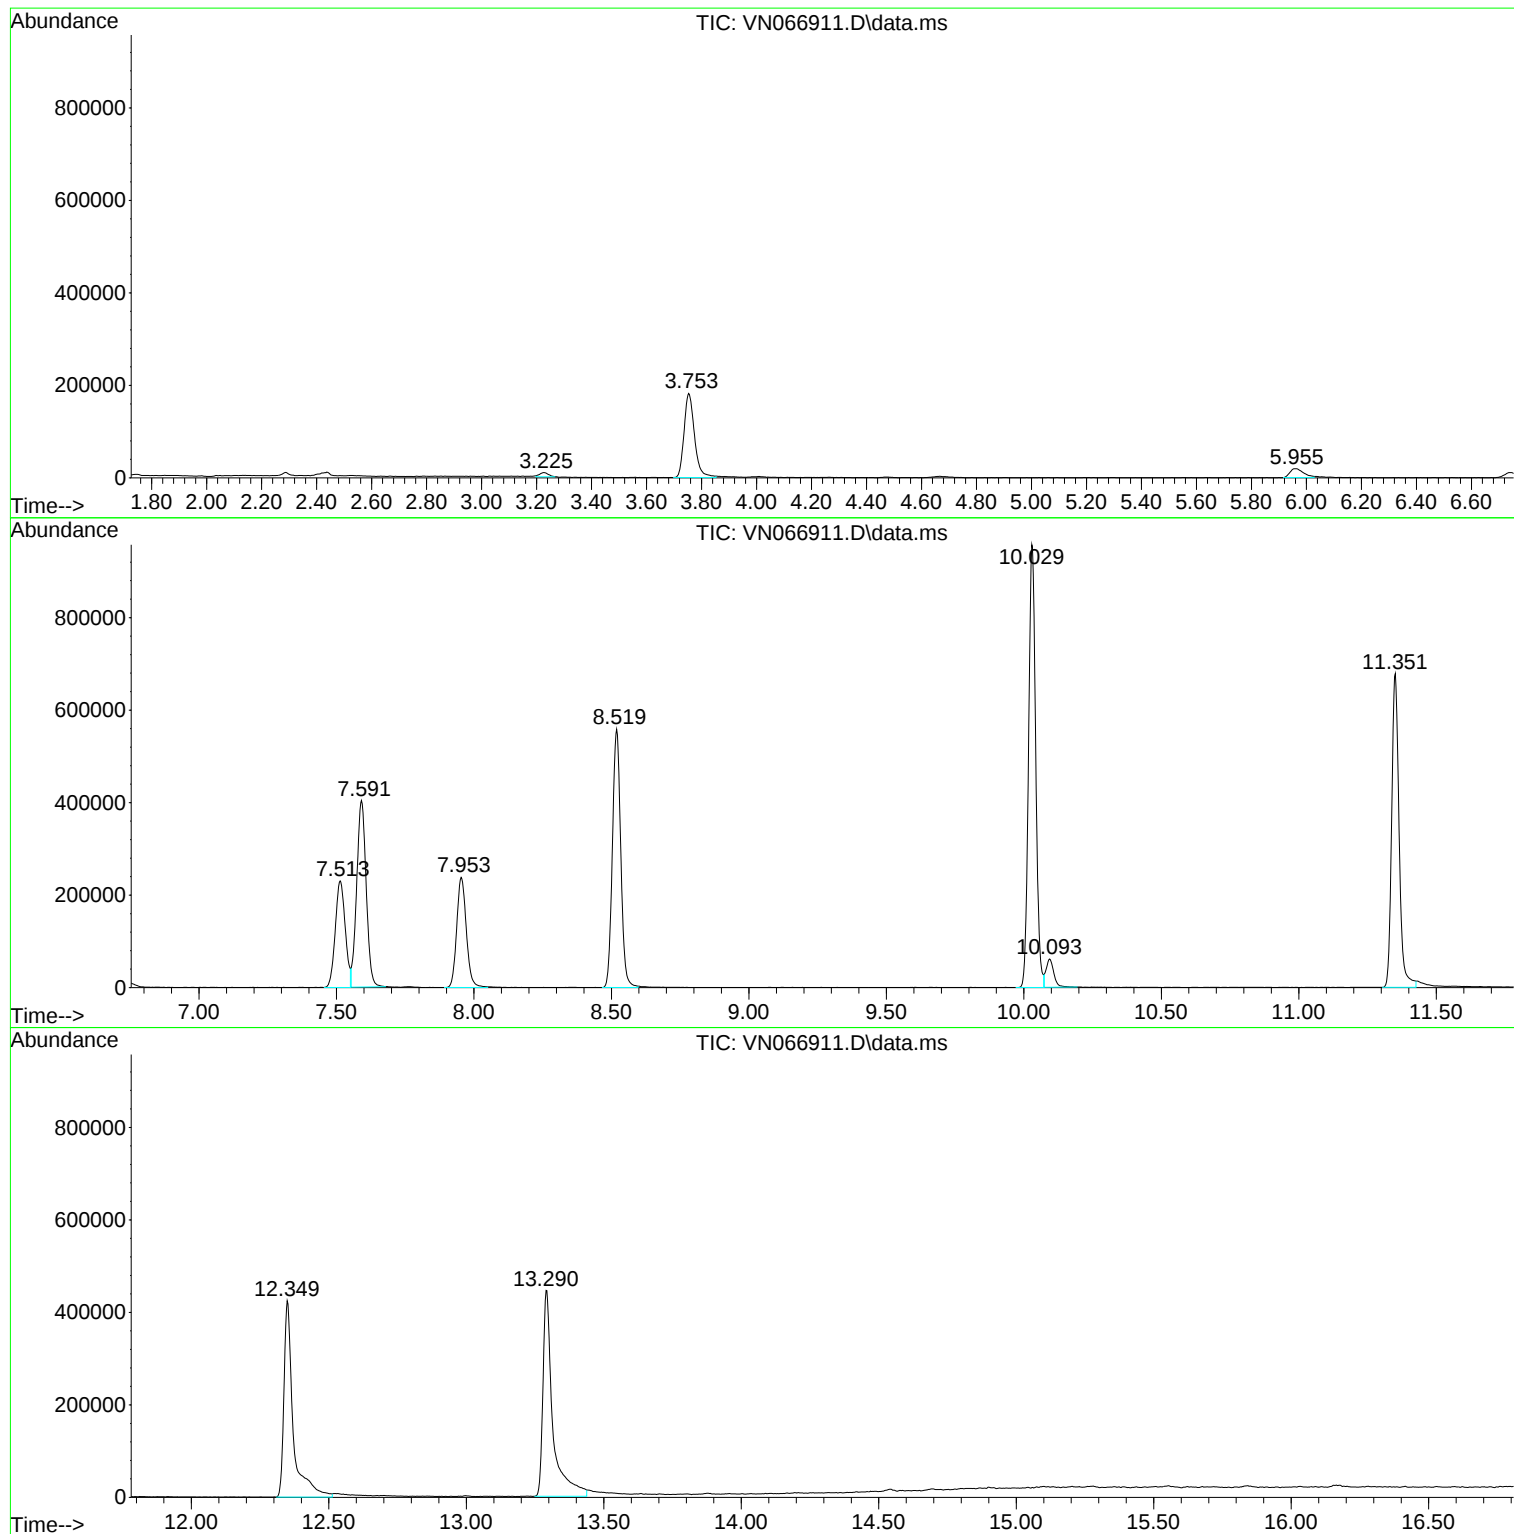

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN043021\
Data File : VN066911.D
Acq On : 30 Apr 2021 15:42
Operator : JC/MD
Sample : M2204-05 100X
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
ANTIFREEZE-1906

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N042721W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN043021\
Data File : VN066911.D
Acq On : 30 Apr 2021 15:42
Operator : JC/MD
Sample : M2204-05 100X
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
ANTIFREEZE-1906

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N042721W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
