
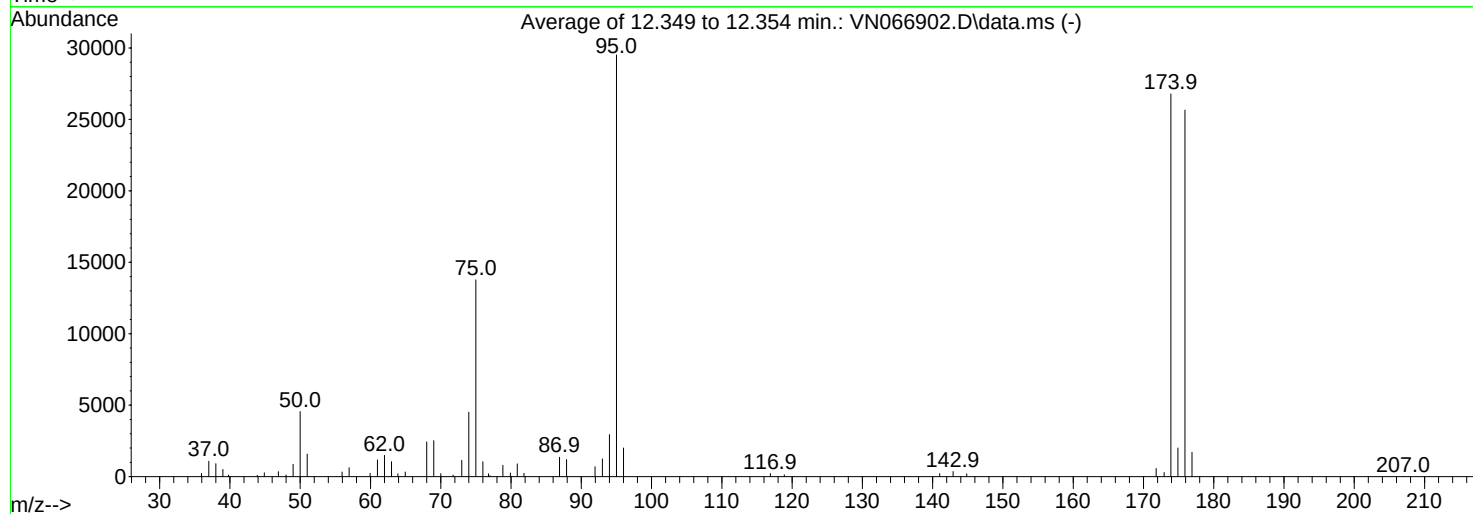


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN043021\
Data File : VN066902.D
Acq On : 30 Apr 2021 9:52
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N042721W.M
Title : SW846 8260
Last Update : Tue Apr 27 16:02:50 2021

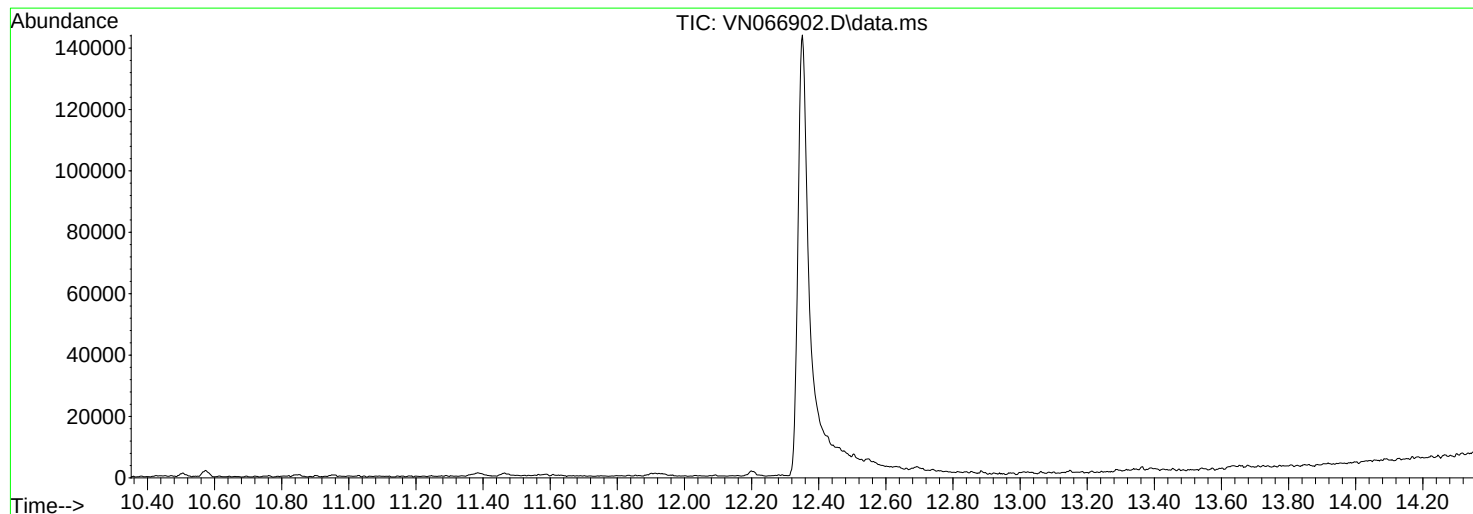

AutoFind: Scans 3962, 3963, 3964; Background Corrected with Scan 3947

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	15.4	4552	PASS
75	95	30	60	46.7	13774	PASS
95	95	100	100	100.0	29515	PASS
96	95	5	9	6.8	2008	PASS
173	174	0.00	2	1.1	293	PASS
174	95	50	100	90.7	26781	PASS
175	174	5	9	7.5	2000	PASS
176	174	95	101	95.8	25656	PASS
177	176	5	9	6.6	1705	PASS