
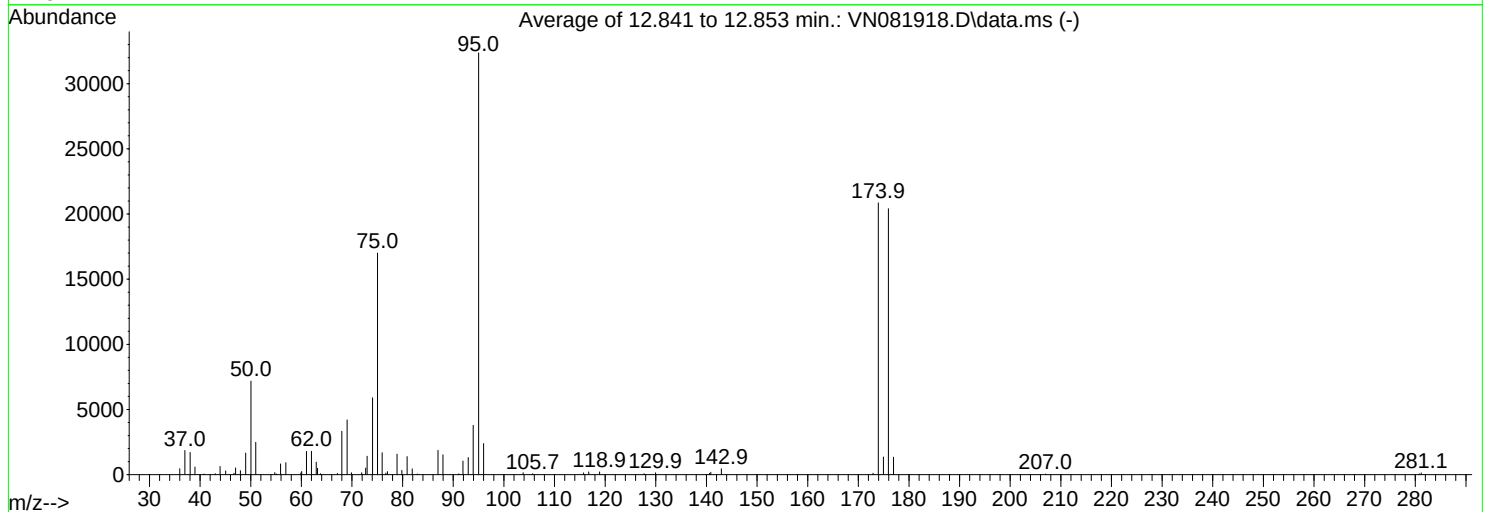


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN043024\
Data File : VN081918.D
Acq On : 30 Apr 2024 08:46
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N042524W.M
Title : SW846 8260
Last Update : Fri Apr 26 05:26:49 2024

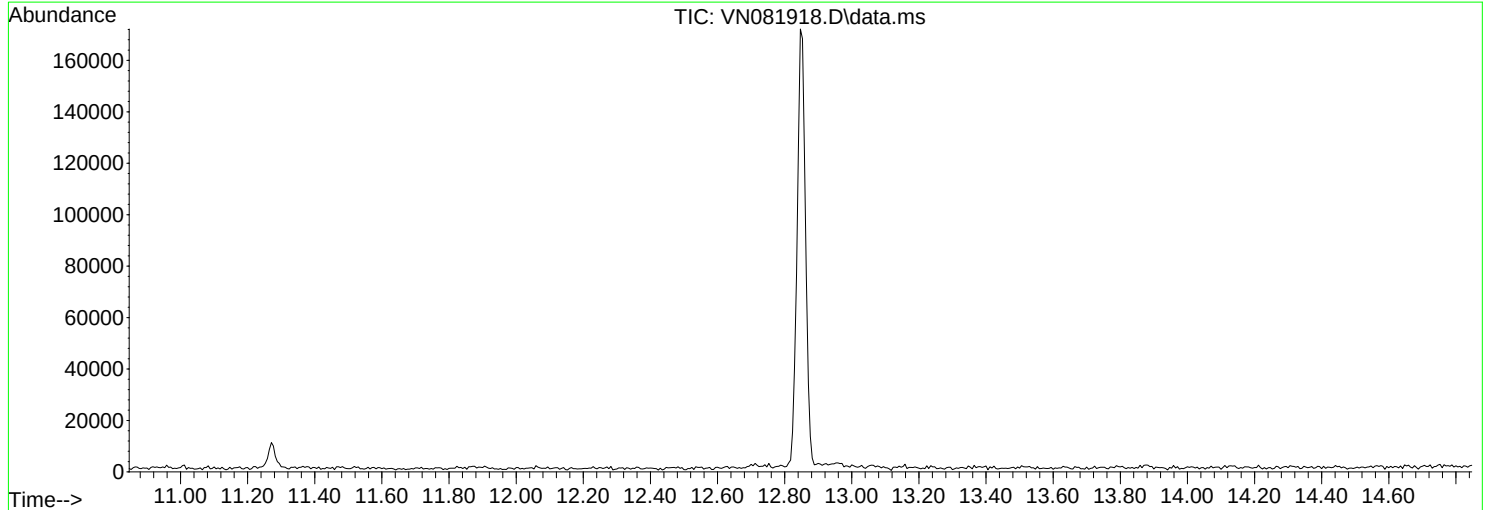

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.2	7189	PASS
75	95	30	60	52.5	17000	PASS
95	95	100	100	100.0	32368	PASS
96	95	5	9	7.3	2379	PASS
173	174	0.00	2	0.5	109	PASS
174	95	50	100	64.4	20857	PASS
175	174	5	9	6.5	1351	PASS
176	174	95	101	97.9	20410	PASS
177	176	5	9	6.6	1344	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	450	49.00	1662	62.95	958	75.05	1700
37.00	1851	50.05	7189	63.20	495	75.95	1684
38.05	1712	51.00	2486	63.80	78	76.70	111
39.00	594	54.75	166	67.10	94	77.00	230
40.80	53	55.10	55	68.00	3329	78.90	1570
43.00	71	55.90	822	69.05	4194	79.85	327
43.95	625	56.95	918	69.90	152	80.90	1387
45.05	287	59.90	135	71.90	146	81.90	446
46.70	107	60.05	244	72.70	506	82.90	51
47.00	510	61.00	1786	73.00	1411	87.00	1862
47.95	311	62.00	1798	74.05	5890	87.95	1526

Average of 12.841 to 12.853 min.: VN081918.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
91.10	64	127.70	69	280.80	60		
91.90	1050	129.95	144	281.15	134		
92.95	1310	140.60	105				
93.95	3778	140.85	182				
95.00	32368	142.95	460				
96.00	2379	172.90	109				
103.80	152	173.95	20857				
105.70	75	174.95	1351				
115.75	132	175.95	20410				
116.75	204	176.95	1344				
118.90	206	207.00	52				

Instrument :

MSVOA_N

ClientSampleId :

BFB