

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN043025\
 Data File : VN086440.D
 Acq On : 30 Apr 2025 16:40
 Operator : JC\MD
 Sample : PB167775ZHE#10
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 PB167775ZHE#10

Manual Integrations
 APPROVED

Reviewed By : John Carlone 05/02/2025
 Supervised By : Semsettin Yesilyurt 05/05/2025

Quant Time: May 01 01:35:49 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N041525W.M
 Quant Title : SW846 8260
 QLast Update : Wed Apr 16 04:19:23 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.224	168	164148	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.100	114	312852	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	295032	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.788	152	125701	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.577	65	116255	48.841	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery =	97.680%		
35) Dibromofluoromethane	8.165	113	74074	51.016	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	102.040%		
50) Toluene-d8	10.565	98	397306	51.198	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery =	102.400%		
62) 4-Bromofluorobenzene	12.847	95	139975	49.453	ug/l	0.00
Spiked Amount 50.000	Range 77 - 121		Recovery =	98.900%		
Target Compounds						
					Qvalue	
11) Tert butyl alcohol	5.518	59	7894	18.176	ug/l #	91
16) Acetone	4.430	43	36289	39.285	ug/l	97
20) Methylene Chloride	5.271	84	7736	3.516	ug/l	89
25) 2-Butanone	7.482	43	35835	24.187	ug/l	97
43) Isopropyl Acetate	8.688	43	39517m	5.444	ug/l	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN043025\
Data File : VN086440.D
Acq On : 30 Apr 2025 16:40
Operator : JC\MD
Sample : PB167775ZHE#10
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 17 Sample Multiplier: 1


Instrument :
MSVOA_N
ClientSampleId :
PB167775ZHE#10

Manual Integrations
APPROVED

Reviewed By :John Carlone 05/02/2025
Supervised By :Semsettin Yesilyurt 05/05/2025


Quant Time: May 01 01:35:49 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N041525W.M
Quant Title : SW846 8260
QLast Update : Wed Apr 16 04:19:23 2025
Response via : Initial Calibration

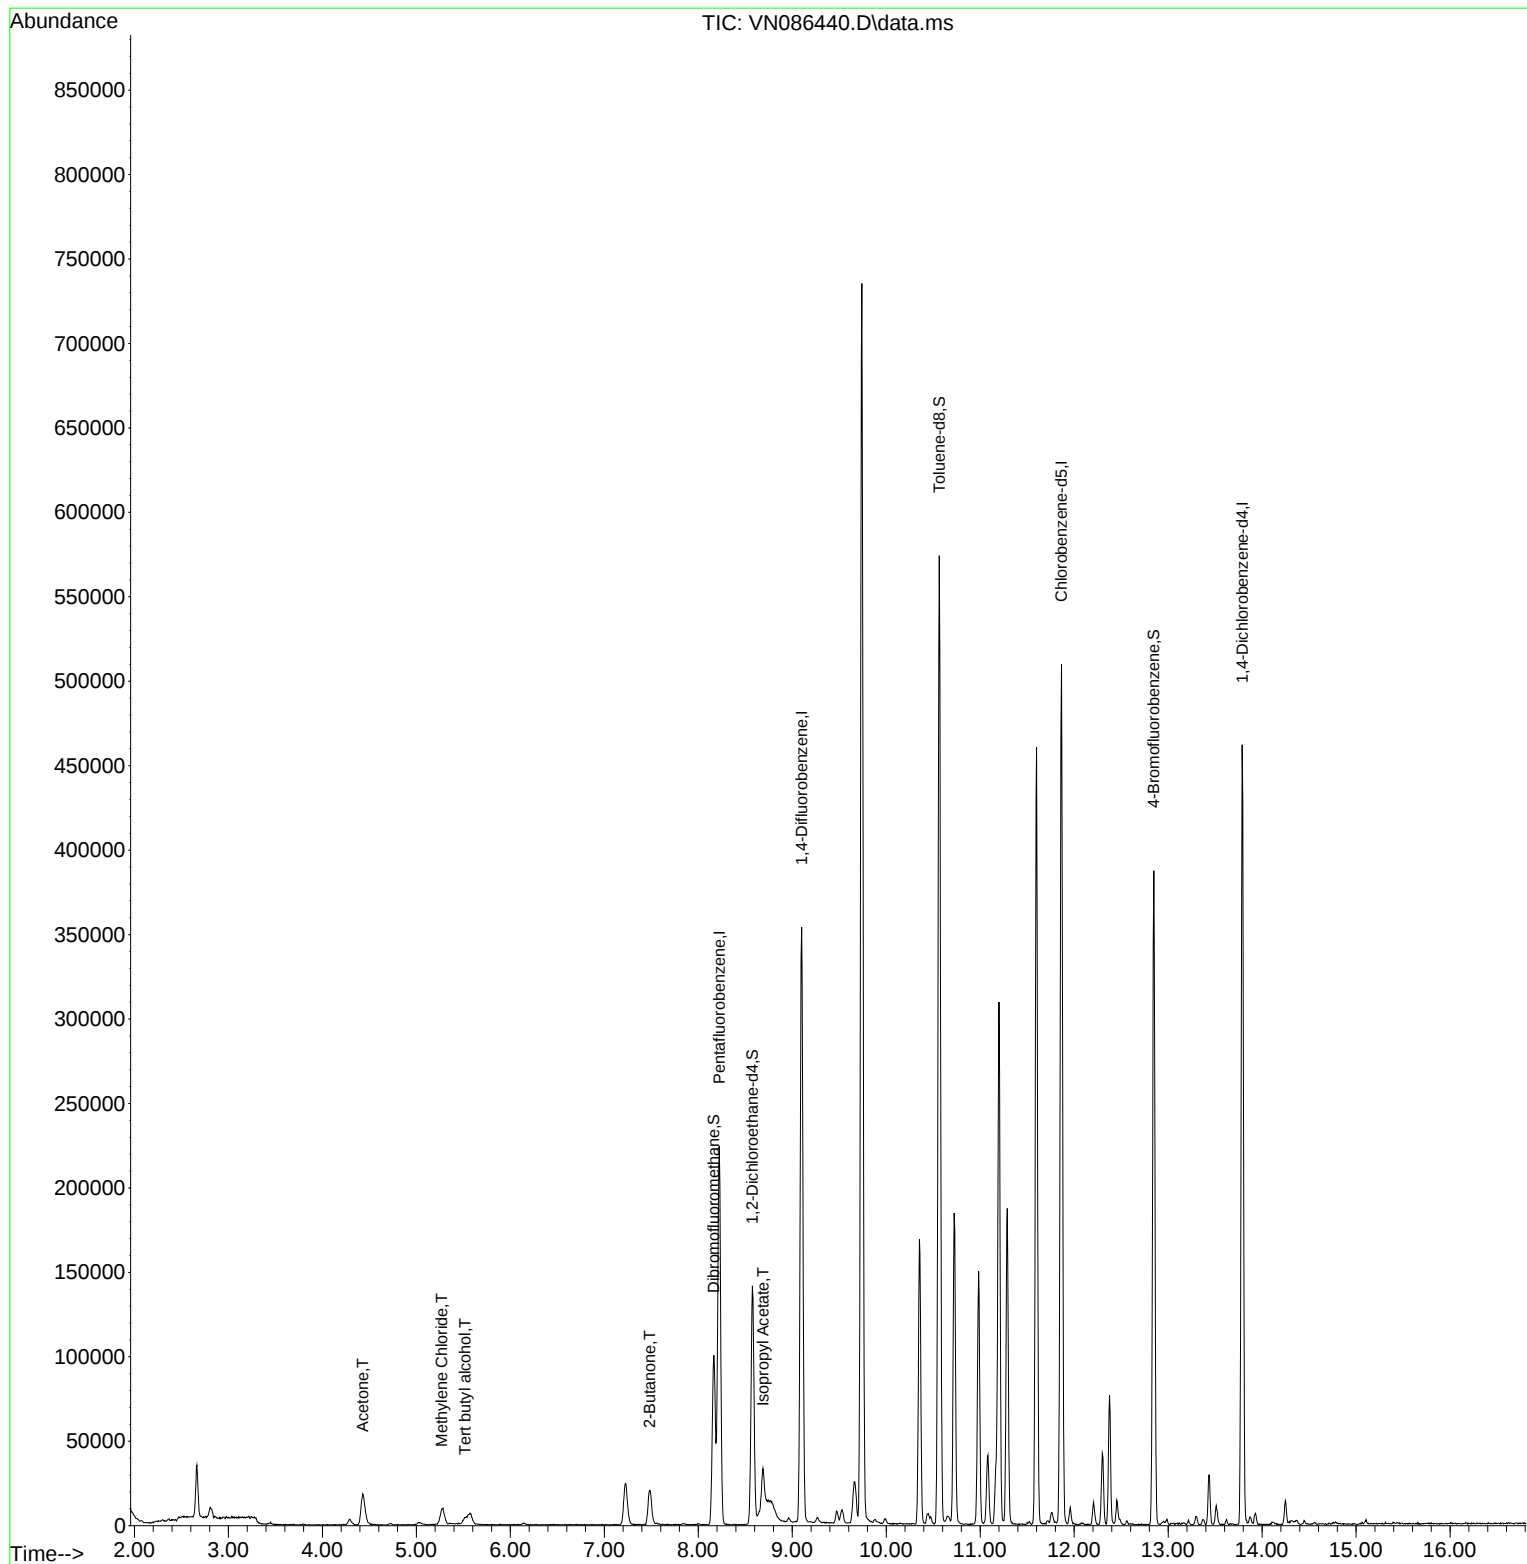



#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.224 min Scan# 1066
Delta R.T. 0.006 min
Lab File: VN086440.D
Acq: 30 Apr 2025 16:40




Instrument :
MSVOA_N
ClientSampleId :
PB167775ZHE#10



Tgt Ion:168 Resp: 16414
Ion Ratio Lower Upper
168 100
99 59.9 52.5 78.7




Manual Integrations
APPROVED


Reviewed By :John Carlone 05/02/2025
Supervised By :Semsettin Yesilyurt 05/05/2025

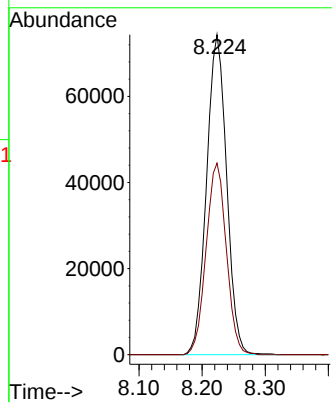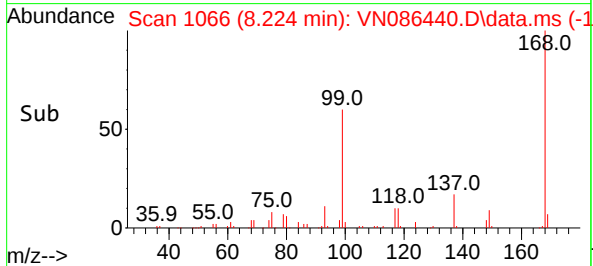

#11
Tert butyl alcohol
Concen: 18.176 ug/l
RT: 5.518 min Scan# 606
Delta R.T. 0.006 min
Lab File: VN086440.D
Acq: 30 Apr 2025 16:40


Tgt Ion: 59 Resp: 7894
Ion Ratio Lower Upper
59 100
57 6.9 8.3 12.5#

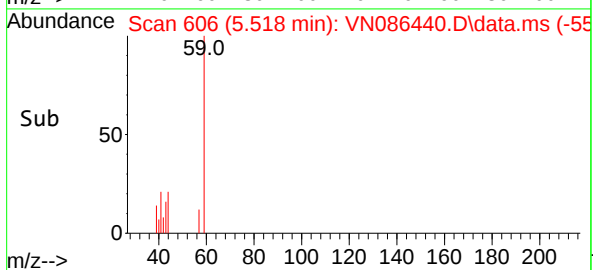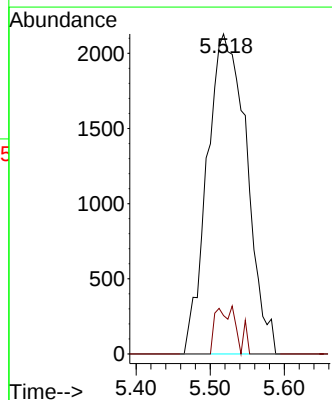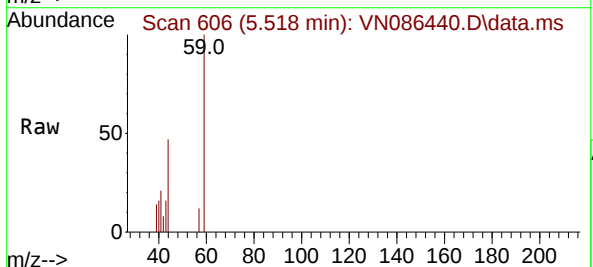

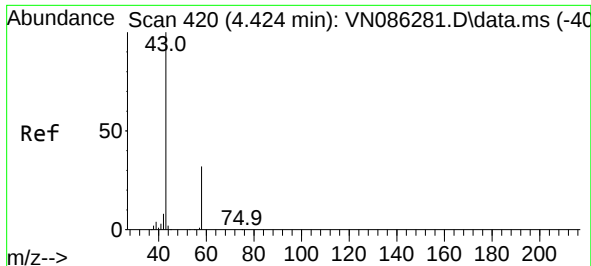

#16
Acetone
Concen: 39.285 ug/l
RT: 4.430 min Scan# 41
Delta R.T. 0.006 min
Lab File: VN086440.D
Acq: 30 Apr 2025 16:40




Instrument :
MSVOA_N
ClientSampleId :
PB167775ZHE#10

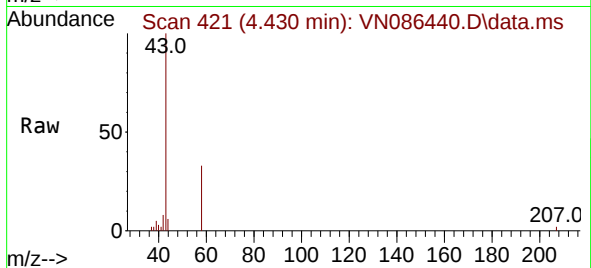

Tgt Ion: 43 Resp: 36289
Ion Ratio Lower Upper
43 100
58 33.2 25.3 37.9




Manual Integrations
APPROVED


Reviewed By :John Carlone 05/02/2025
Supervised By :Semsettin Yesilyurt 05/05/2025

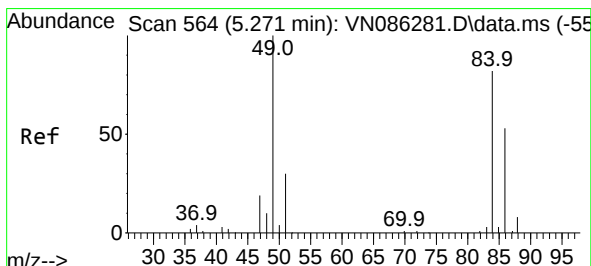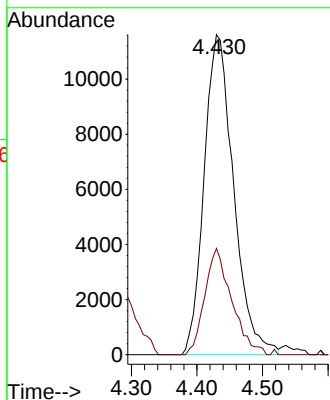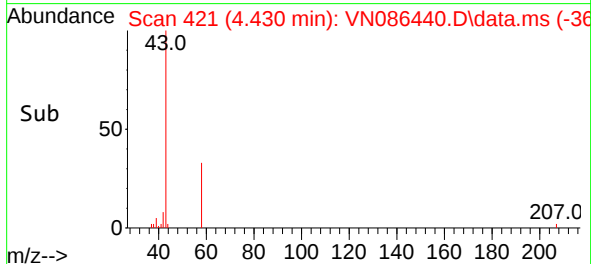

#20
Methylene Chloride
Concen: 3.516 ug/l
RT: 5.271 min Scan# 564
Delta R.T. -0.000 min
Lab File: VN086440.D
Acq: 30 Apr 2025 16:40


Tgt Ion: 84 Resp: 7736
Ion Ratio Lower Upper
84 100
49 110.6 98.2 147.2
51 32.5 29.8 44.6
86 55.4 52.0 78.0

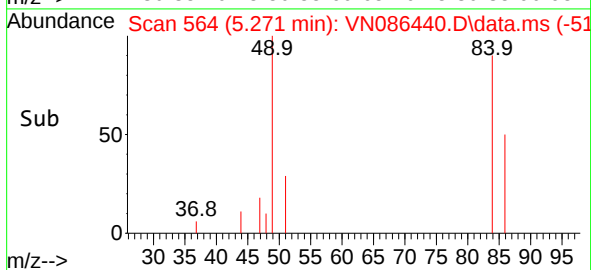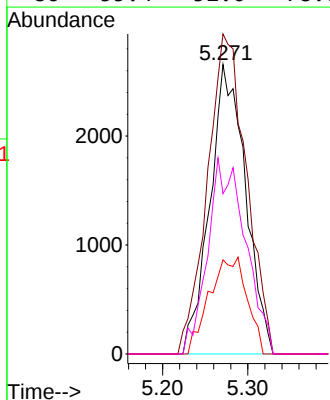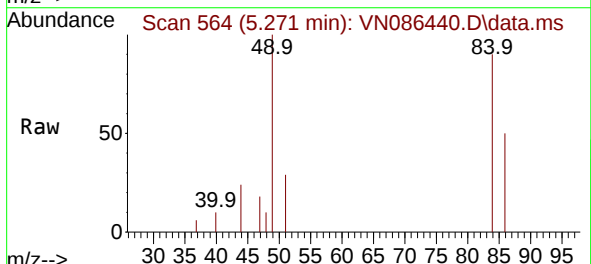

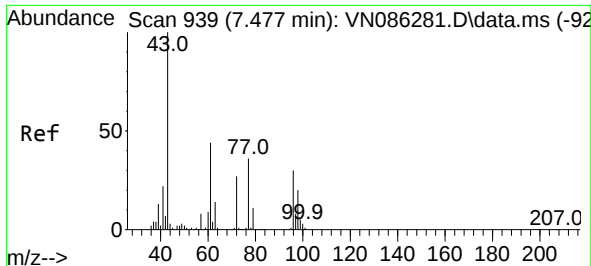

#25
2-Butanone
Concen: 24.187 ug/l
RT: 7.482 min Scan# 940
Delta R.T. 0.006 min
Lab File: VN086440.D
Acq: 30 Apr 2025 16:40




Instrument :
MSVOA_N
ClientSampleId :
PB167775ZHE#10

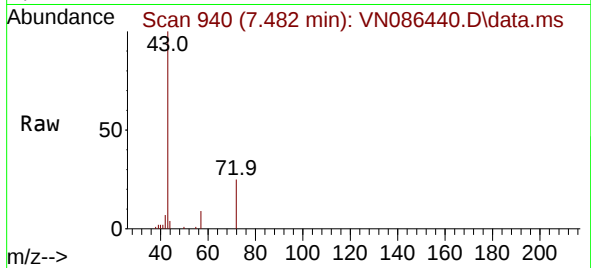

Tgt Ion: 43 Resp: 3583
Ion Ratio Lower Upper
43 100
72 25.5 21.7 32.5




Manual Integrations
APPROVED


Reviewed By :John Carlone 05/02/2025
Supervised By :Semsettin Yesilyurt 05/05/2025

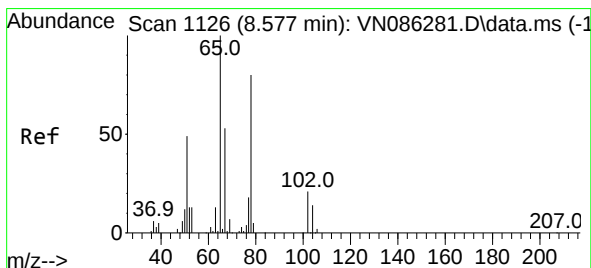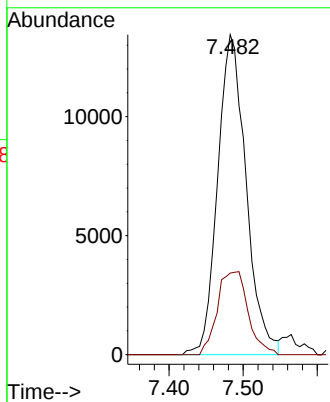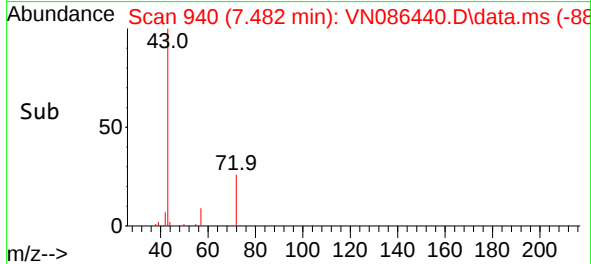

#33
1,2-Dichloroethane-d4
Concen: 48.841 ug/l
RT: 8.577 min Scan# 1126
Delta R.T. -0.000 min
Lab File: VN086440.D
Acq: 30 Apr 2025 16:40


Tgt Ion: 65 Resp: 116255
Ion Ratio Lower Upper
65 100
67 52.3 0.0 106.0

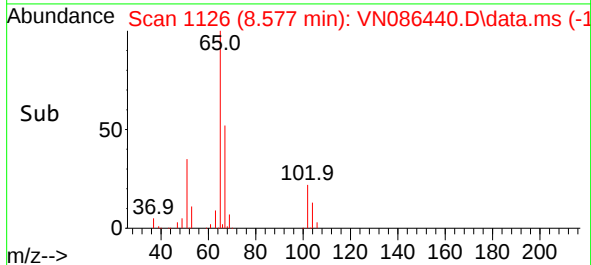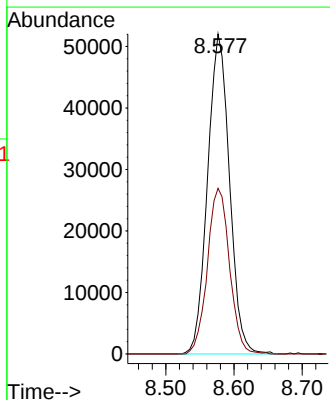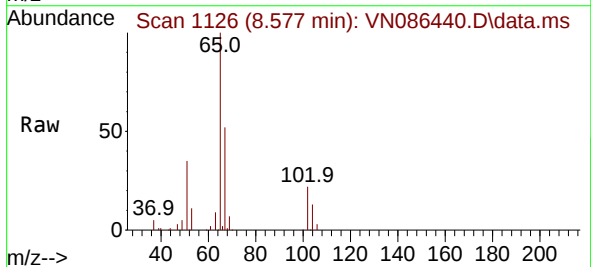



#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 9.100 min Scan# 11
Delta R.T. -0.000 min
Lab File: VN086440.D
Acq: 30 Apr 2025 16:40




Instrument :
MSVOA_N
ClientSampleId :
PB167775ZHE#10



Tgt Ion:114 Resp: 31285
Ion Ratio Lower Upper
114 100
63 20.5 0.0 42.6
88 15.1 0.0 31.8




Manual Integrations
APPROVED


Reviewed By :John Carlone 05/02/2025
Supervised By :Semsettin Yesilyurt 05/05/2025

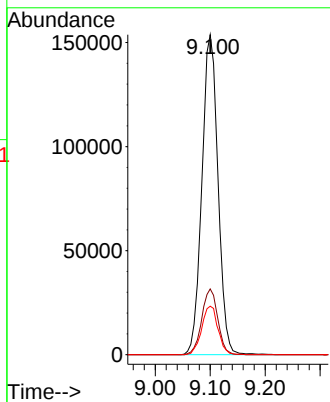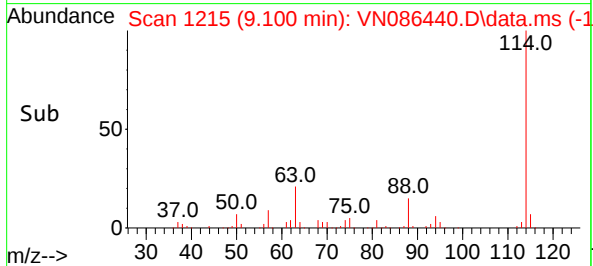

#35
Dibromofluoromethane
Concen: 51.016 ug/l
RT: 8.165 min Scan# 1056
Delta R.T. -0.000 min
Lab File: VN086440.D
Acq: 30 Apr 2025 16:40


Tgt Ion:113 Resp: 74074
Ion Ratio Lower Upper
113 100
111 103.0 83.4 125.0
192 17.3 13.7 20.5

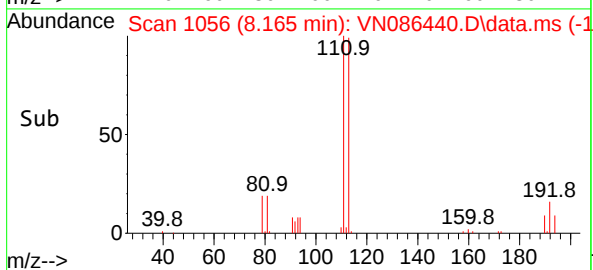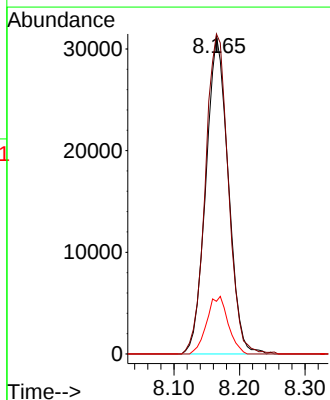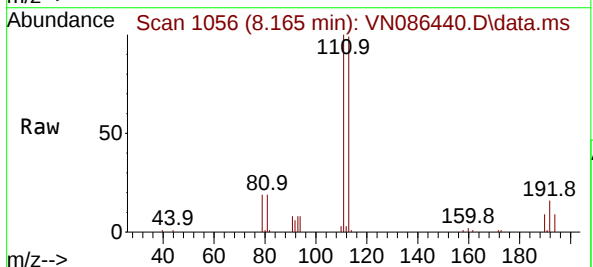



#43
Isopropyl Acetate
Concen: 5.444 ug/l m
RT: 8.688 min Scan# 1145
Delta R.T. 0.005 min
Lab File: VN086440.D
Acq: 30 Apr 2025 16:40




Instrument : MSVOA_N
ClientSampleId : PB167775ZHE#10




Tgt Ion: 43 Resp: 39517
Ion Ratio Lower Upper
43 100
61 13.3 20.5 30.7
87 9.0 10.5 15.7

Manual Integrations
APPROVED



Reviewed By :John Carlone 05/02/2025
Supervised By :Semsettin Yesilyurt 05/05/2025

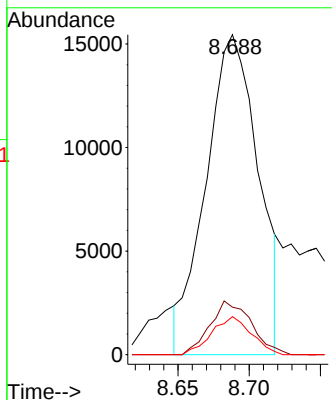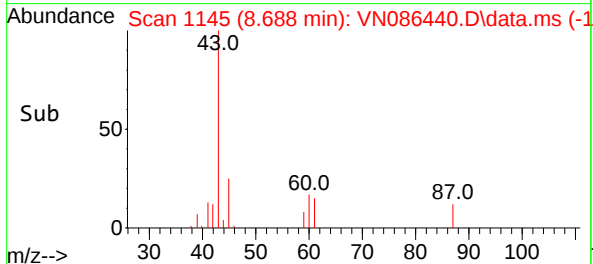


#50
Toluene-d8
Concen: 51.198 ug/l
RT: 10.565 min Scan# 1464
Delta R.T. -0.000 min
Lab File: VN086440.D
Acq: 30 Apr 2025 16:40

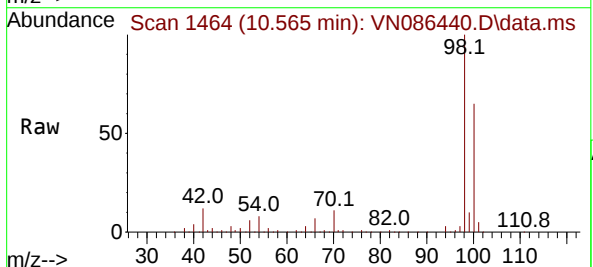


Tgt Ion: 98 Resp: 397306
Ion Ratio Lower Upper
98 100
100 65.3 52.5 78.7

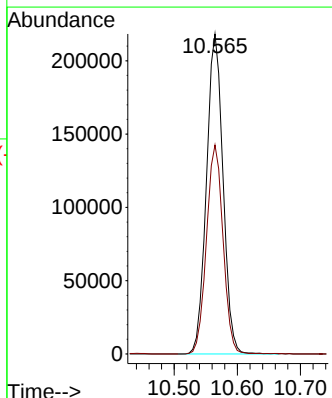

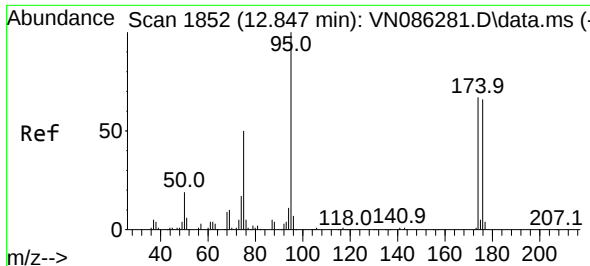

#62
4-Bromofluorobenzene
Concen: 49.453 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. -0.000 min
Lab File: VN086440.D
Acq: 30 Apr 2025 16:40




Instrument :
MSVOA_N
ClientSampleId :
PB167775ZHE#10

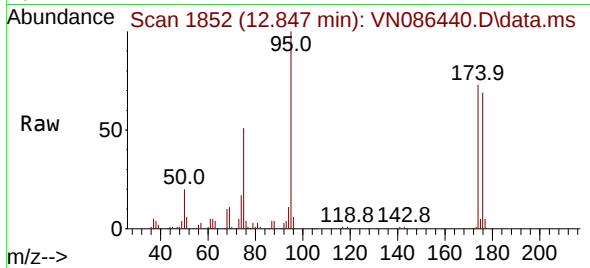


Tgt Ion: 95 Resp: 139975
Ion Ratio Lower Upper
95 100
174 73.0 0.0 133.4
176 70.1 0.0 129.2

Manual Integrations
APPROVED



Reviewed By :John Carlone 05/02/2025
Supervised By :Semsettin Yesilyurt 05/05/2025

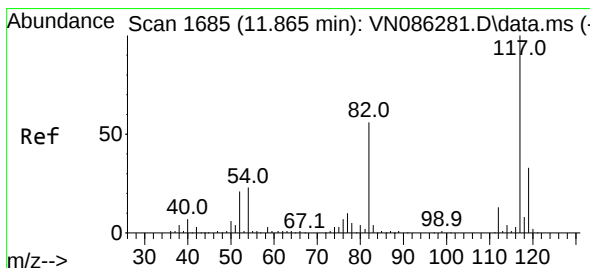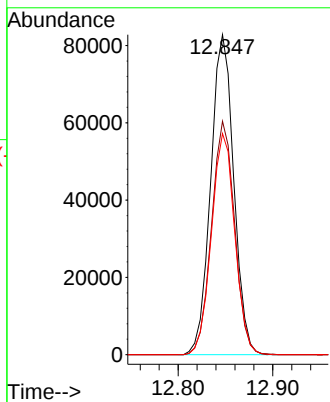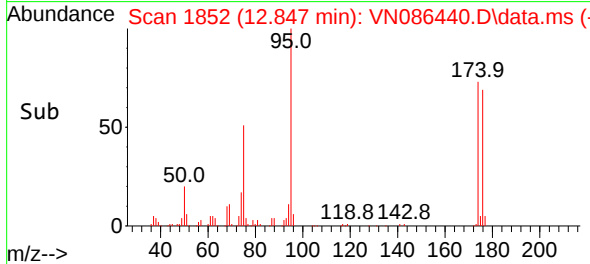


#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.865 min Scan# 1685
Delta R.T. -0.000 min
Lab File: VN086440.D
Acq: 30 Apr 2025 16:40

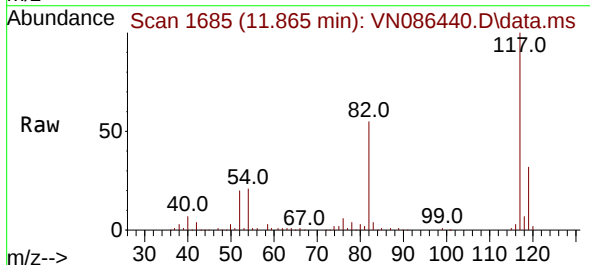


Tgt Ion:117 Resp: 295032
Ion Ratio Lower Upper
117 100
82 55.4 44.7 67.1
119 31.9 26.4 39.6

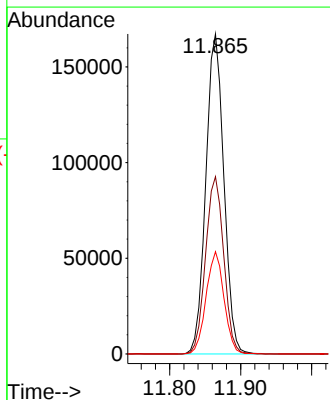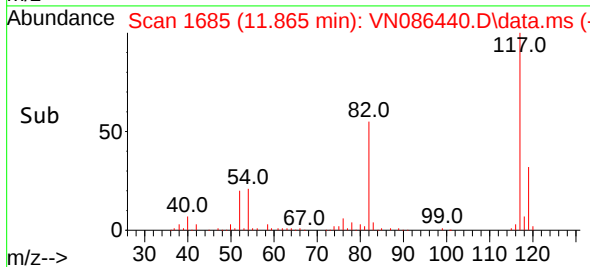

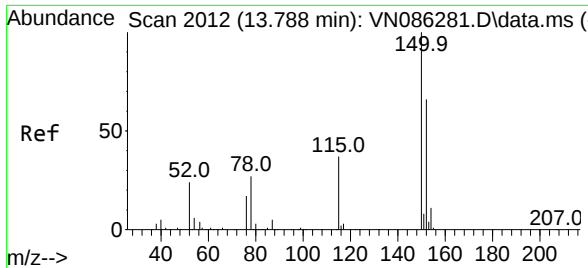

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 13.788 min Scan# 20
 Delta R.T. -0.000 min
 Lab File: VN086440.D
 Acq: 30 Apr 2025 16:40

Instrument :
 MSVOA_N
 ClientSampleId :
 PB167775ZHE#10

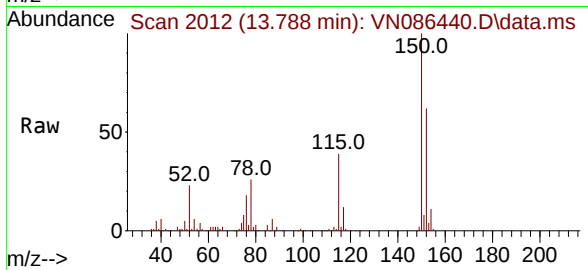

Tgt Ion:152 Resp: 12570
 Ion Ratio Lower Upper
 152 100
 115 61.2 31.9 95.9
 150 156.3 0.0 352.0

Manual Integrations
 APPROVED

Reviewed By :John Carlone 05/02/2025
 Supervised By :Semsettin Yesilyurt 05/05/2025

