
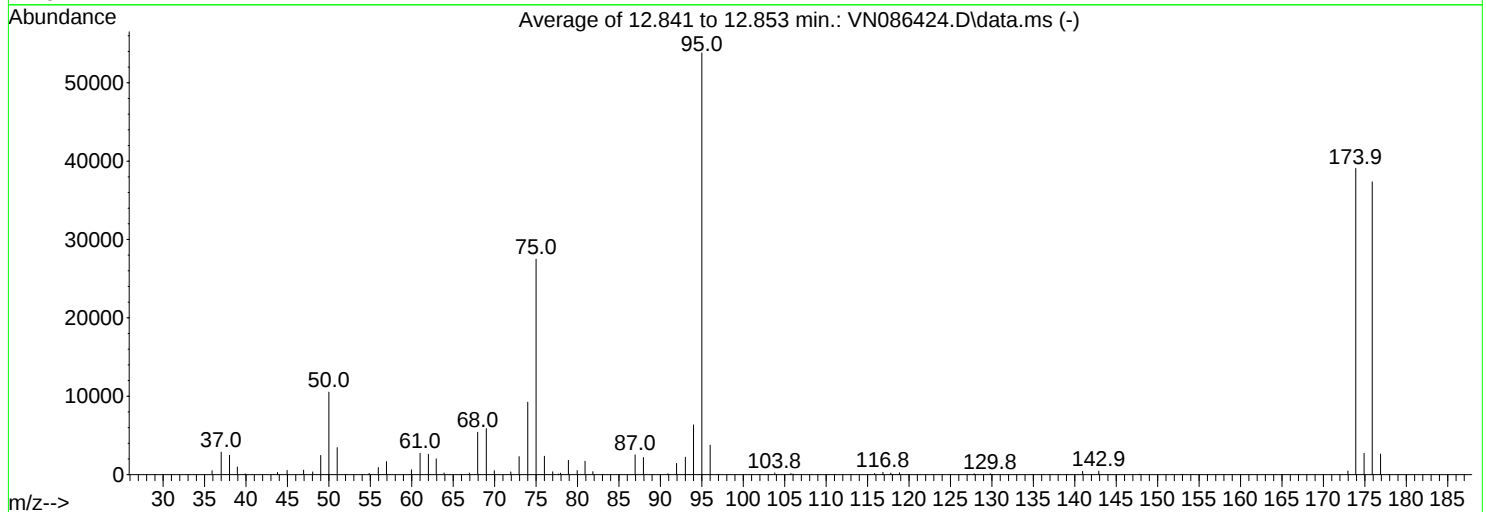


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN043025\
Data File : VN086424.D
Acq On : 30 Apr 2025 09:43
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N041525W.M
Title : SW846 8260
Last Update : Wed Apr 16 04:19:23 2025

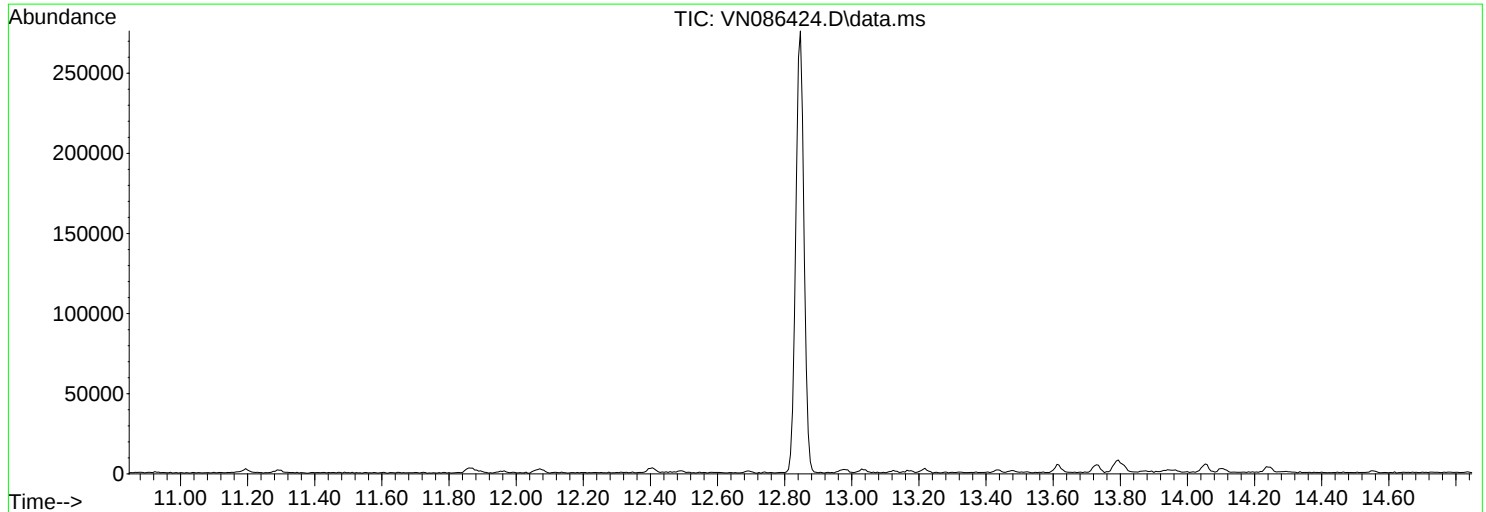

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1842

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.6	10530	PASS
75	95	30	60	51.1	27504	PASS
95	95	100	100	100.0	53816	PASS
96	95	5	9	7.0	3755	PASS
173	174	0.00	2	1.2	473	PASS
174	95	50	100	72.6	39069	PASS
175	174	5	9	7.0	2718	PASS
176	174	95	101	95.6	37352	PASS
177	176	5	9	7.1	2644	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	517	51.00	3461	69.00	5886	79.95	521
37.00	2876	54.85	168	69.95	506	80.90	172
38.00	2464	55.95	924	71.95	353	81.85	38
38.95	986	56.95	1677	72.95	2304	86.95	253
39.90	98	59.95	604	74.00	9247	87.95	2189
43.80	294	61.00	2722	75.00	27504	90.90	131
44.95	559	62.00	2600	76.00	2345	91.95	1429
46.95	572	62.95	2019	77.00	364	93.00	2229
48.05	348	63.90	230	77.70	87	94.00	6353
49.00	2446	66.95	202	77.95	179	95.00	53816
50.00	10530	67.95	5412	78.90	1811	96.00	3755

Average of 12.841 to 12.853 min.: VN086424.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
103.80	228	147.80	52				
105.75	140	172.95	473				
106.00	74	173.90	39069				
115.85	136	174.90	2718				
116.85	301	175.90	37352				
117.80	196	176.90	2644				
118.85	237	177.90	51				
127.85	119						
129.80	131						
140.95	427						
142.90	455						

Instrument :

MSVOA_N

ClientSampleId :

BFB