


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN050119\
Data File : VN055316.D
Acq On : 1 May 2019 9:18
Operator : JC/SP
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N042919W.M
Title : SW846 8260
Last Update : Tue Apr 30 07:16:52 2019

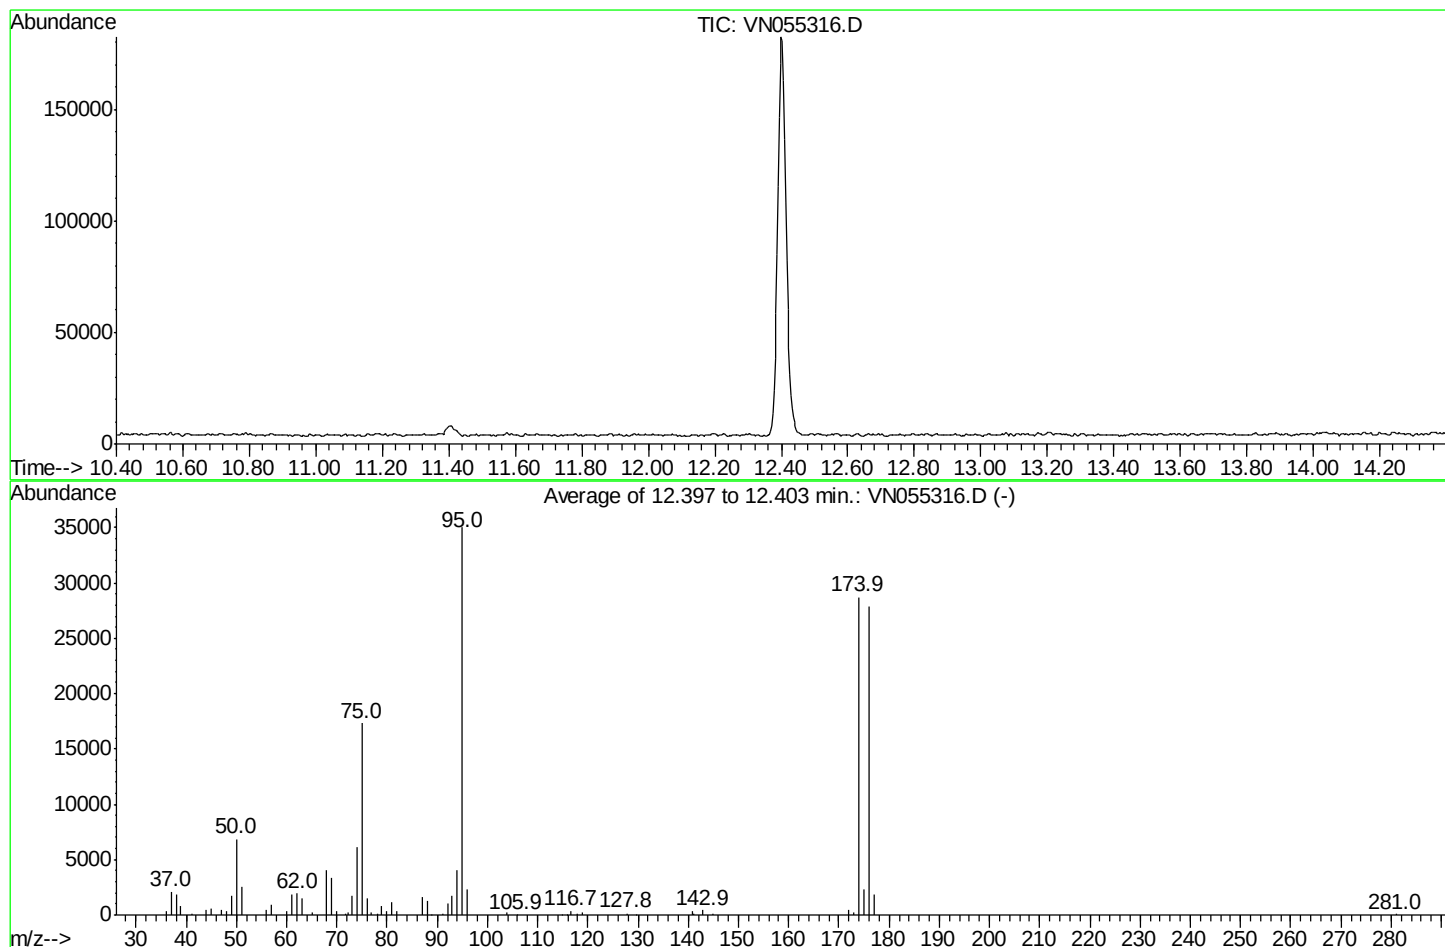

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.6	6863	PASS
75	95	30	60	49.4	17298	PASS
95	95	100	100	100.0	35021	PASS
96	95	5	9	6.6	2299	PASS
173	174	0.00	2	0.7	213	PASS
174	95	50	100	81.9	28688	PASS
175	174	5	9	8.0	2300	PASS
176	174	95	101	97.0	27840	PASS
177	176	5	9	6.6	1849	PASS