


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN050120\
 Data File : VN061245.D
 Acq On : 2 May 2020 00:13
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N042720W.M
 Title : SW846 8260
 Last Update : Wed Apr 29 08:14:26 2020

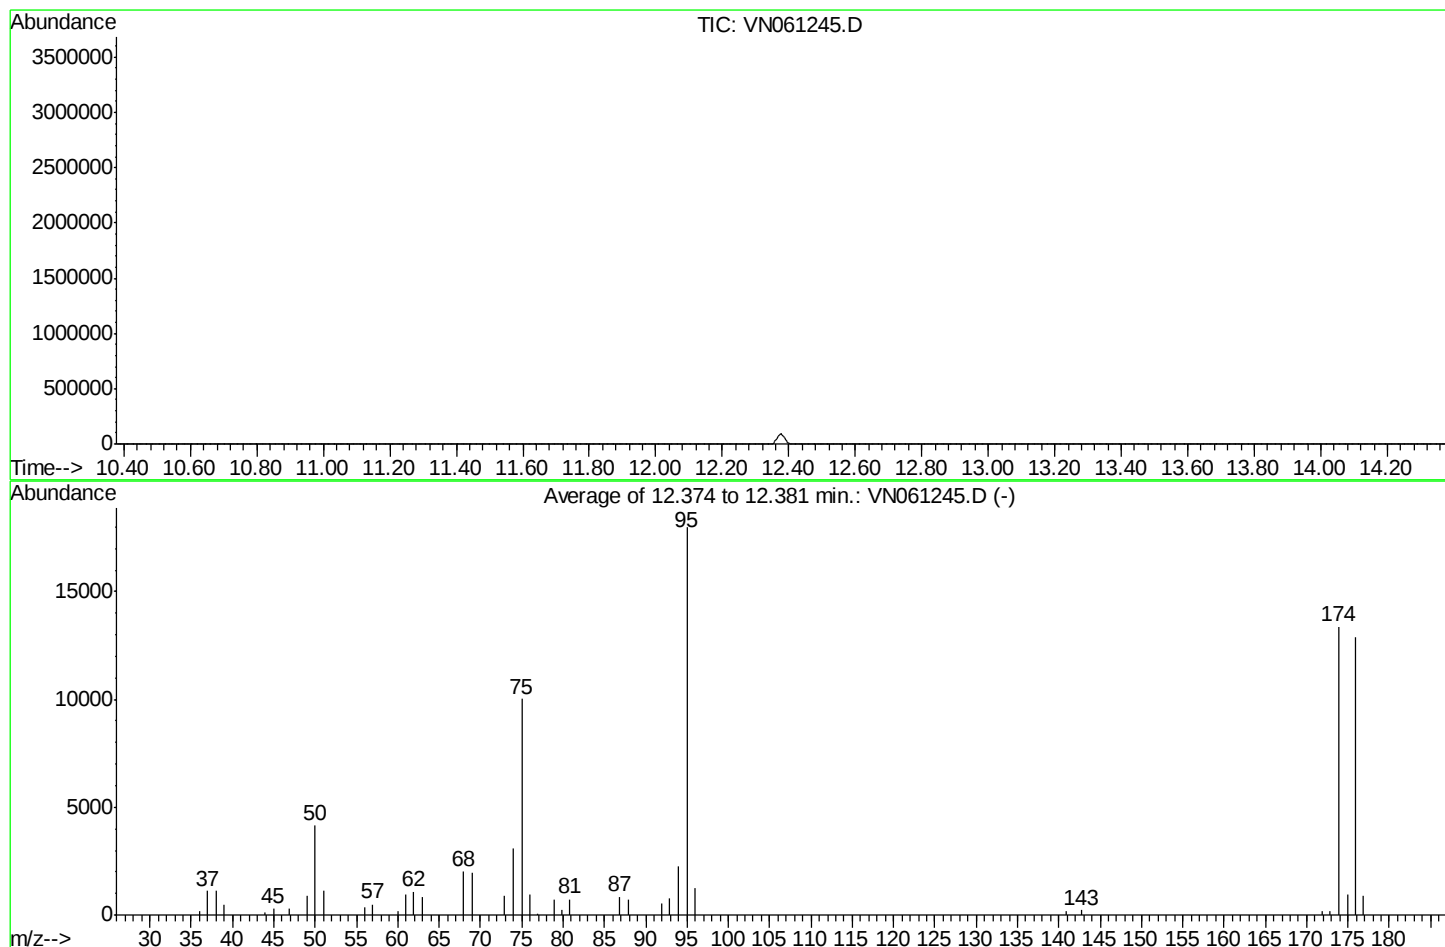

AutoFind: Scans 3354, 3355, 3356; Background Corrected with Scan 3342

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.0	4142	PASS
75	95	30	60	55.8	10031	PASS
95	95	100	100	100.0	17981	PASS
96	95	5	9	6.9	1245	PASS
173	174	0.00	2	1.3	174	PASS
174	95	50	100	74.4	13373	PASS
175	174	5	9	7.2	961	PASS
176	174	95	101	96.4	12893	PASS
177	176	5	9	7.1	916	PASS