
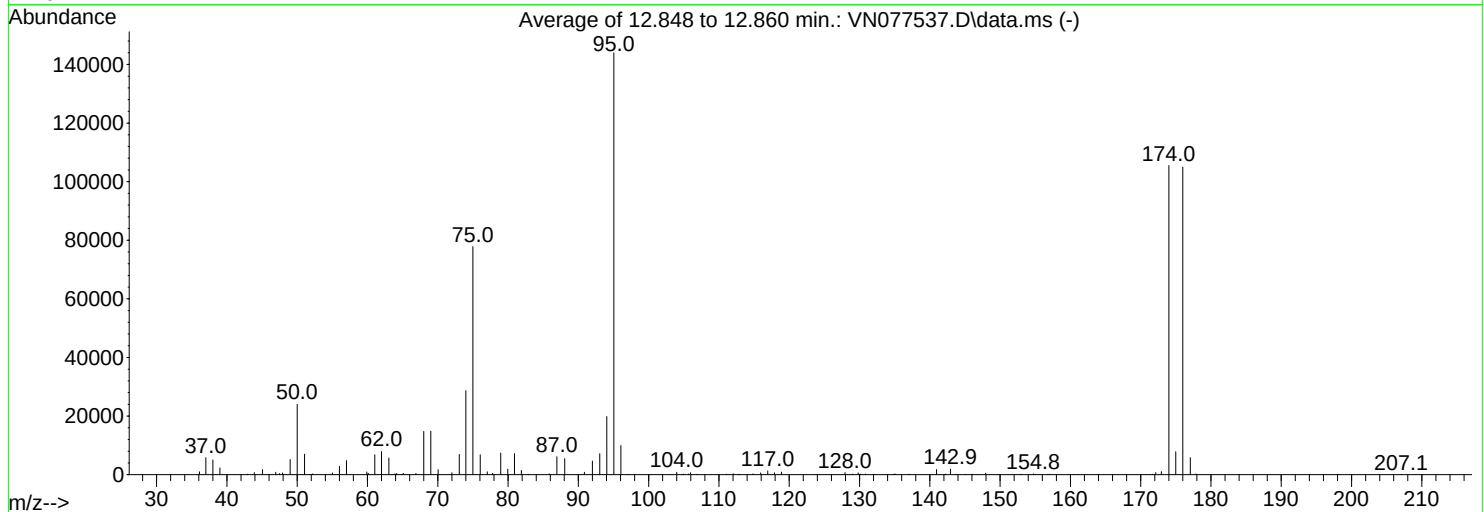


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN050123\
Data File : VN077537.D
Acq On : 01 May 2023 10:08
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N042423W.M
Title : SW846 8260
Last Update : Tue Apr 25 02:50:59 2023

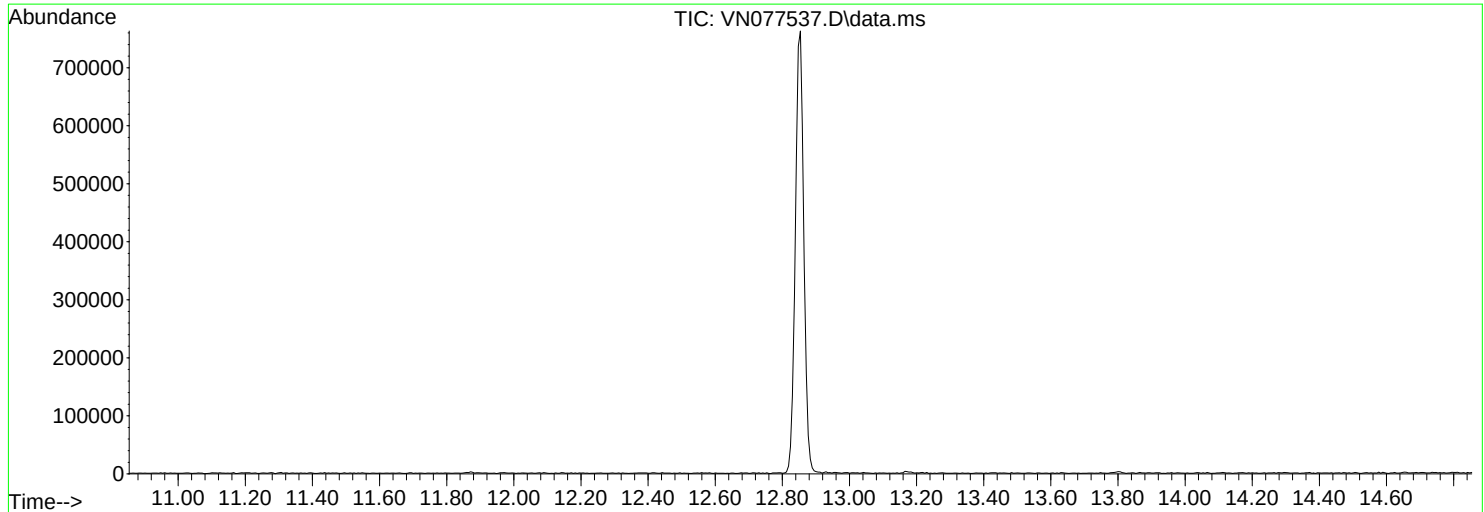

AutoFind: Scans 1855, 1856, 1857; Background Corrected with Scan 1842

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.7	23981	PASS
75	95	30	60	54.1	77829	PASS
95	95	100	100	100.0	143960	PASS
96	95	5	9	6.9	9923	PASS
173	174	0.00	2	1.0	1052	PASS
174	95	50	100	73.3	105528	PASS
175	174	5	9	7.4	7791	PASS
176	174	95	101	99.4	104936	PASS
177	176	5	9	5.5	5782	PASS

Average of 12.848 to 12.860 min.: VN077537.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.10	990	47.50	385	58.00	113	68.00	1475
37.00	5780	47.90	606	59.90	951	69.00	1484
38.00	5046	48.10	190	60.10	477	70.05	172
39.00	2295	49.00	5154	61.05	6793	72.00	68
41.10	77	50.00	23981	62.00	7931	73.05	6865
42.90	179	51.05	7013	63.05	5659	74.00	28701
43.90	723	51.80	74	63.90	267	75.00	77829
44.00	80	52.20	259	64.15	408	76.05	6785
45.05	1767	55.00	601	64.80	131	77.05	1015
46.00	153	56.00	2818	65.10	433	77.80	470
46.95	807	57.00	4815	66.90	443	78.00	116

Average of 12.848 to 12.860 min.: VN077537.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
78.95	7354	94.05	19808	109.95	125	127.95	720
79.95	1869	95.05	143960	111.10	146	128.60	57
80.90	7232	96.05	9923	112.05	271	129.00	148
81.90	1414	97.10	75	112.80	119	129.80	576
82.90	133	103.00	75	113.00	110	130.10	159
85.85	264	104.00	835	114.85	261	130.85	204
86.95	6117	104.70	67	115.95	576	134.80	89
88.05	5477	104.95	191	116.95	1279	135.05	271
90.85	814	105.70	213	117.90	674	137.05	192
92.00	4659	105.95	686	118.90	899	140.95	1735
93.05	7139	106.85	127	123.80	55	142.20	162

Average of 12.848 to 12.860 min.: VN077537.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
142.95	1883	157.10	172	177.05	5782		
143.75	109	160.60	78	177.85	201		
145.05	129	161.10	61	207.10	63		
146.05	163	170.70	57				
146.90	60	171.30	58				
147.95	489	171.70	156				
149.70	64	172.15	735				
152.95	199	172.95	1052				
154.75	288	174.00	105528				
155.00	95	175.00	7791				
156.80	108	176.00	104936				

Instrument :

MSVOA_N

ClientSampleId :

BFB