

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN050124\
 Data File : VN081959.D
 Acq On : 01 May 2024 16:15
 Operator : JC\MD
 Sample : P2329-01
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: May 02 01:43:06 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N042524W.M
 Quant Title : SW846 8260
 QLast Update : Fri Apr 26 05:26:49 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.229	168	192190	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	386265	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	336703	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	134370	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.577	65	147139	45.362	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery =	90.720%		
35) Dibromofluoromethane	8.165	113	111261	47.841	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	95.680%		
50) Toluene-d8	10.571	98	466910	51.119	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery =	102.240%		
62) 4-Bromofluorobenzene	12.853	95	160053	44.328	ug/l	0.00
Spiked Amount 50.000	Range 64 - 133		Recovery =	88.660%		
Target Compounds						Qvalue
2) Dichlorodifluoromethane	2.083	85	29114	10.791	ug/l	95
4) Vinyl Chloride	2.512	62	11579	4.545	ug/l	94
5) Bromomethane	2.959	94	258	Below Cal		89
6) Chloroethane	3.136	64	634	0.492	ug/l #	44
9) 1,1,2-Trichlorotrifluo...	4.377	101	336242	146.953	ug/l	92
12) 1,1-Dichloroethene	4.342	96	88727	38.117	ug/l	98
13) Acrolein	4.183	56	63	Below Cal	#	1
16) Acetone	4.447	43	2398	Below Cal	#	67
21) trans-1,2-Dichloroethene	5.794	96	20591	8.113	ug/l #	91
24) 1,1-Dichloroethane	6.571	63	78672	15.864	ug/l	97
25) 2-Butanone	7.494	43	1001	0.544	ug/l #	1
27) cis-1,2-Dichloroethene	7.488	96	1413683	476.668	ug/l	99
31) Cyclohexane	8.224	56	6168	1.262	ug/l #	46
32) 1,1,1-Trichloroethane	8.171	97	4685	1.069	ug/l #	48
36) 1,1-Dichloropropene	8.218	75	19444	5.139	ug/l #	48
38) Carbon Tetrachloride	8.229	117	20777	5.619	ug/l #	17
39) Methylcyclohexane	9.359	83	228765	49.785	ug/l #	1
40) Benzene	8.606	78	19066	1.679	ug/l	91
42) 1,2-Dichloroethane	8.671	62	12600	2.987	ug/l	99
43) Isopropyl Acetate	8.688	43	5447	0.708	ug/l #	72
44) Trichloroethene	9.359	130	12526193	4783.450	ug/l	70
45) 1,2-Dichloropropane	9.359	63	57063	19.197	ug/l #	1
49) 1,4-Dioxane	9.694	88	1169	20.946	ug/l #	76
52) Toluene	10.623	92	2091	0.307	ug/l	90
55) 1,1,2-Trichloroethane	11.029	97	1022	0.382	ug/l #	60
60) Dibromochloromethane	11.106	129	143715	50.724	ug/l #	11
64) Tetrachloroethene	11.106	164	139422	57.013	ug/l	92
76) 1,2,3-Trichloropropane	12.847	75	88919	25.523	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.847	75	88919	52.299	ug/l #	12
87) 1,3-Dichlorobenzene	13.811	146	3245	0.696	ug/l #	49
88) 1,4-Dichlorobenzene	13.811	146	3245	0.706	ug/l #	45


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN050124\
Data File : VN081959.D
Acq On : 01 May 2024 16:15
Operator : JC\MD
Sample : P2329-01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :

Quant Time: May 02 01:43:06 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N042524W.M
Quant Title : SW846 8260
QLast Update : Fri Apr 26 05:26:49 2024
Response via : Initial Calibration

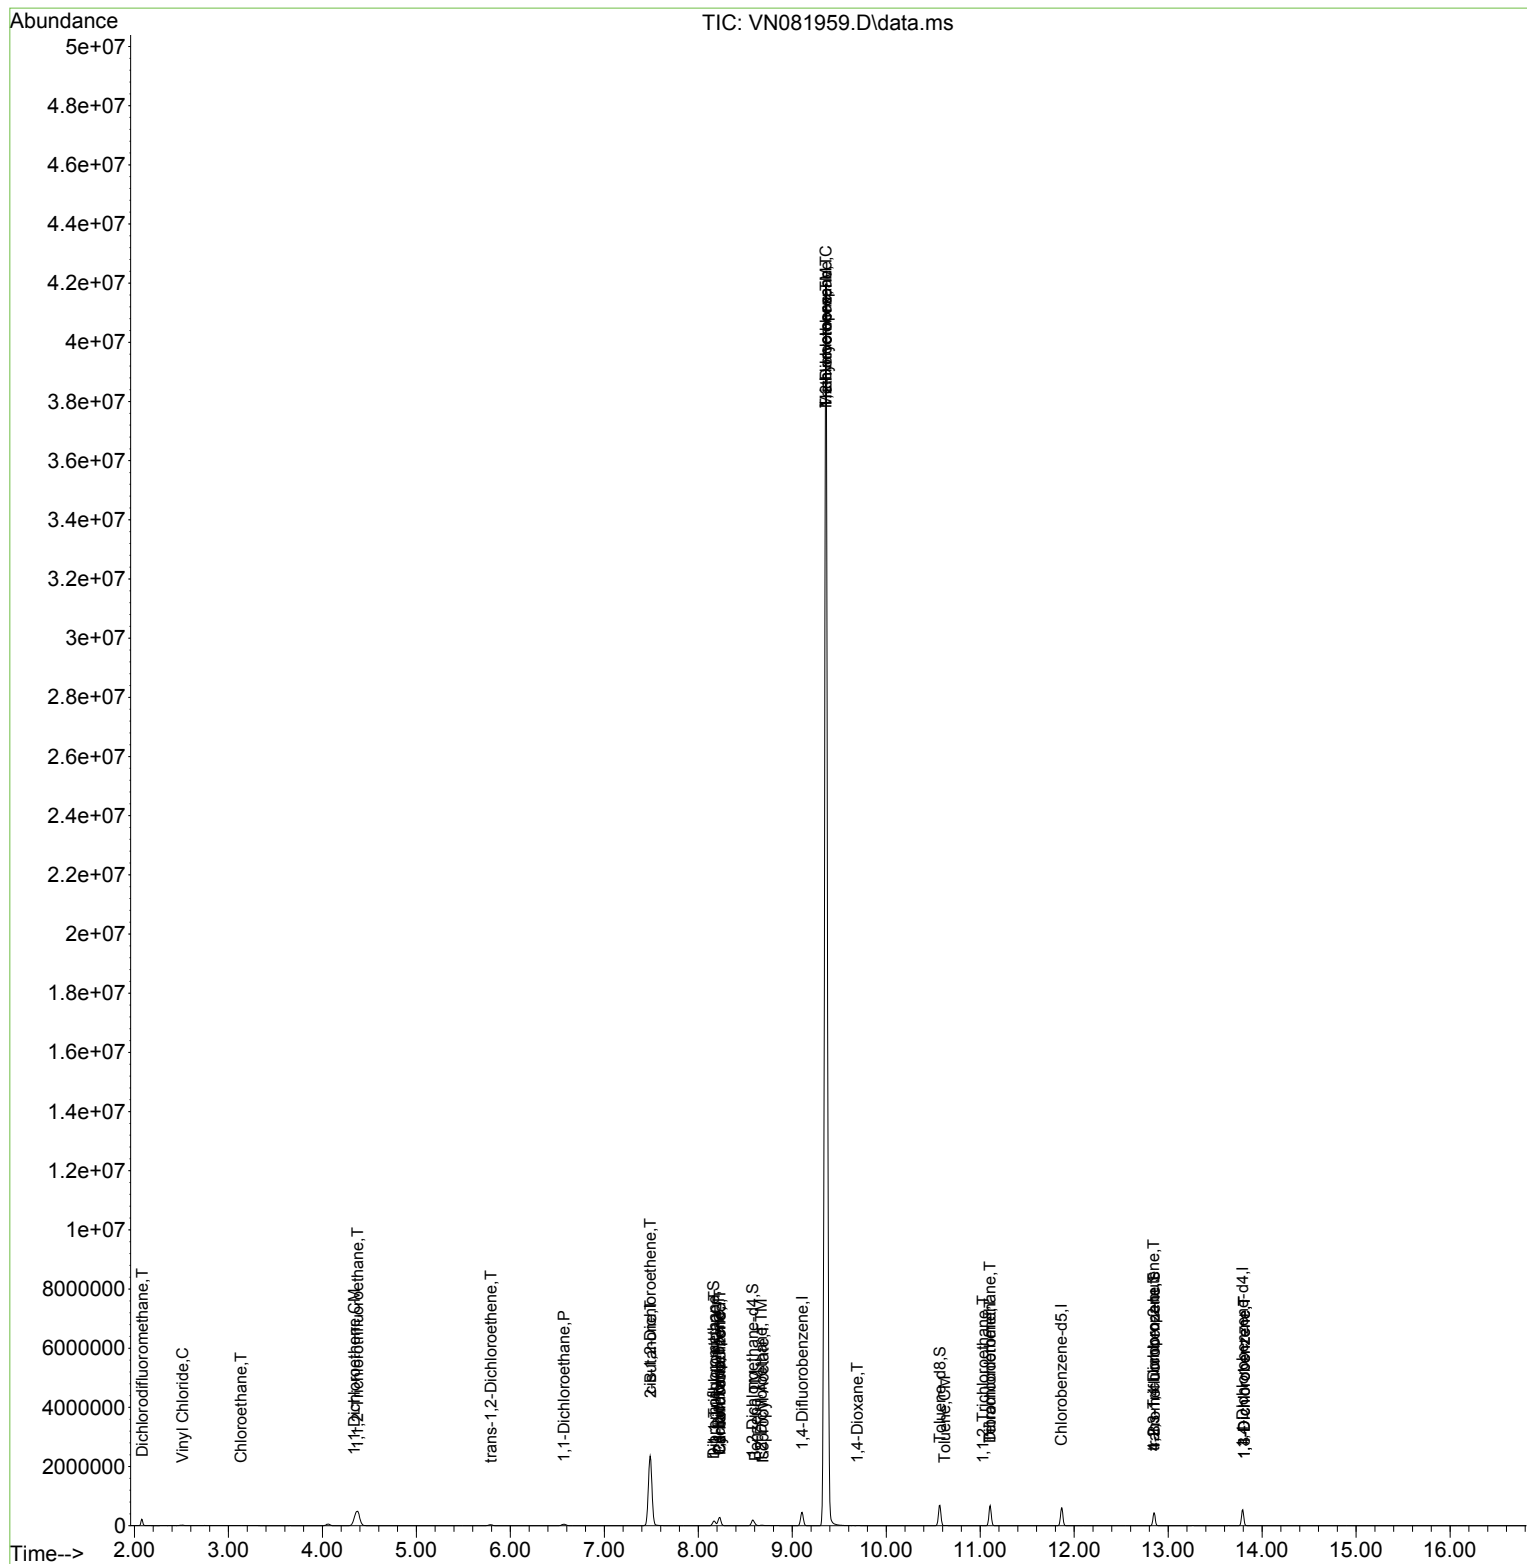



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 8.229 min Scan# 10

Delta R.T. 0.005 min

Lab File: VN081959.D

Acq: 01 May 2024 16:15

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion:168 Resp: 192190

Ion Ratio Lower Upper

168 100

99 60.1 48.2 72.4

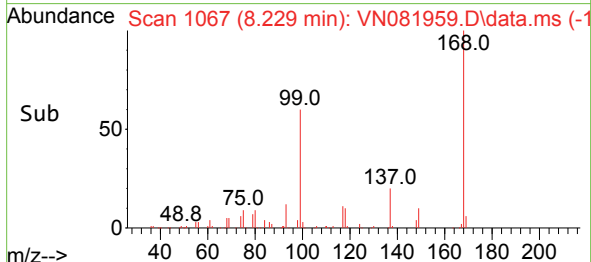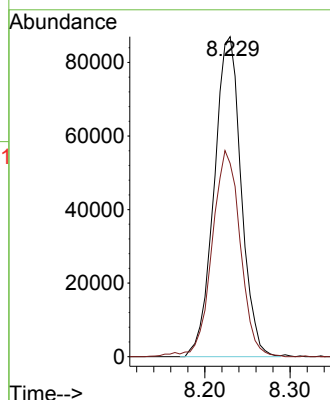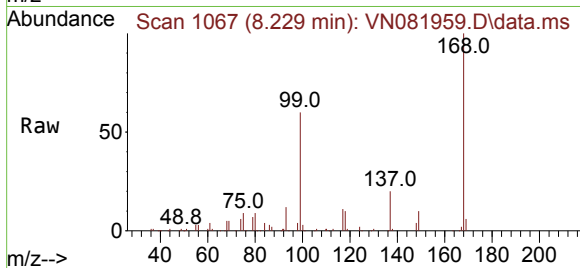

#2

Dichlorodifluoromethane

Concen: 10.791 ug/l

RT: 2.083 min Scan# 22

Delta R.T. -0.041 min

Lab File: VN081959.D




Acq: 01 May 2024 16:15


Tgt Ion: 85 Resp: 29114

Ion Ratio Lower Upper

85 100

87 28.7 15.8 47.4

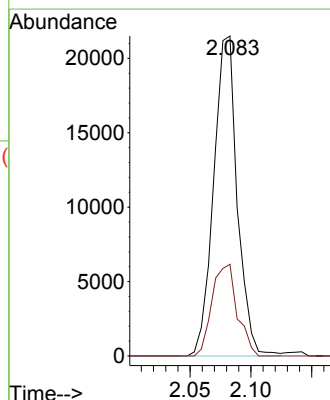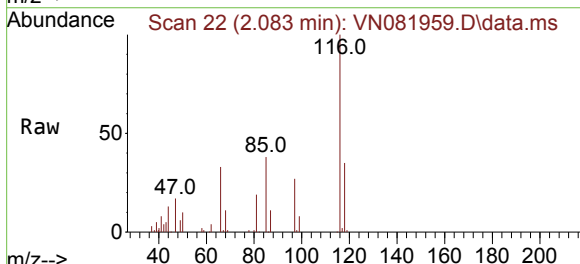



#4

Vinyl Chloride

Concen: 4.545 ug/l

RT: 2.512 min Scan# 91

Delta R.T. -0.006 min

Lab File: VN081959.D

Acq: 01 May 2024 16:15

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion: 62 Resp: 11579

Ion Ratio Lower Upper

62 100

64 33.9 24.6 37.0

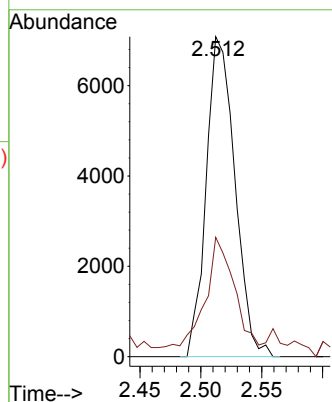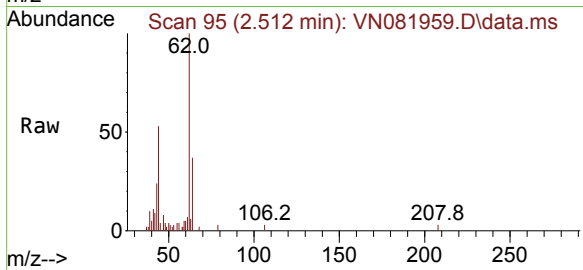

#5

Bromomethane

Concen: Below Cal

RT: 2.959 min Scan# 171

Delta R.T. 0.011 min

Lab File: VN081959.D




Acq: 01 May 2024 16:15


Tgt Ion: 94 Resp: 258

Ion Ratio Lower Upper

94 100

96 83.0 74.8 112.2




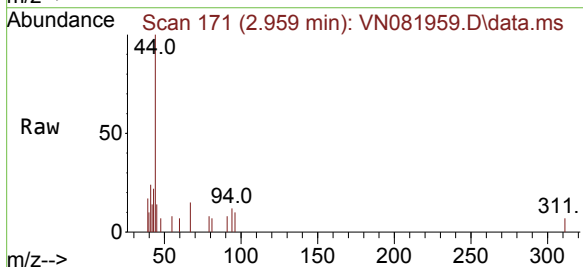




#6
Chloroethane
Concen: 0.492 ug/l
RT: 3.136 min Scan# 201
Delta R.T. 0.012 min
Lab File: VN081959.D
Acq: 01 May 2024 16:15




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 64 Resp: 634
Ion Ratio Lower Upper
64 100
66 0.0 24.7 37.1#

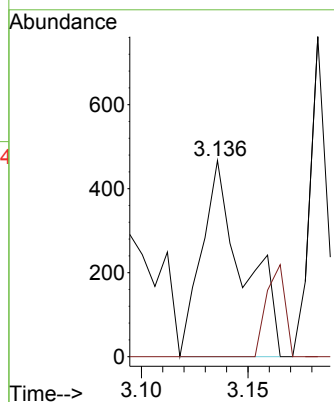

#9
1,1,2-Trichlorotrifluoroethane
Concen: 146.953 ug/l
RT: 4.377 min Scan# 412
Delta R.T. -0.000 min
Lab File: VN081959.D
Acq: 01 May 2024 16:15

Tgt Ion: 101 Resp: 336242
Ion Ratio Lower Upper
101 100
85 45.5 37.3 55.9
151 63.8 59.2 88.8



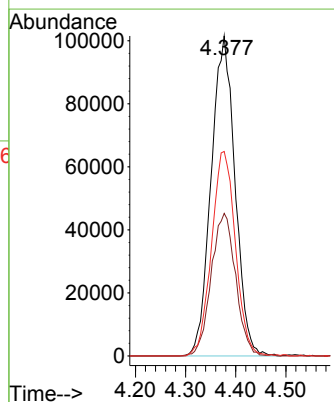





#12
1,1-Dichloroethene
Concen: 38.117 ug/l
RT: 4.342 min Scan# 405
Delta R.T. 0.006 min
Lab File: VN081959.D
Acq: 01 May 2024 16:15




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 96 Resp: 88727
Ion Ratio Lower Upper
96 100
61 150.8 119.7 179.5
98 58.6 49.6 74.4



#13
Acrolein
Concen: Below Cal
RT: 4.183 min Scan# 379
Delta R.T. 0.006 min
Lab File: VN081959.D
Acq: 01 May 2024 16:15

Tgt Ion: 56 Resp: 63
Ion Ratio Lower Upper
56 100
55 195.2 55.8 83.8#









#16
Acetone
Concen: Below Cal
RT: 4.447 min Scan# 41
Delta R.T. 0.023 min
Lab File: VN081959.D
Acq: 01 May 2024 16:15




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 43 Resp: 2398
Ion Ratio Lower Upper
43 100
58 13.5 25.2 37.8#



#21
trans-1,2-Dichloroethene
Concen: 8.113 ug/l
RT: 5.794 min Scan# 653
Delta R.T. 0.006 min
Lab File: VN081959.D
Acq: 01 May 2024 16:15

Tgt Ion: 96 Resp: 20591
Ion Ratio Lower Upper
96 100
61 120.1 96.5 144.7
98 43.5 51.3 76.9#









#24
1,1-Dichloroethane
Concen: 15.864 ug/l
RT: 6.571 min Scan# 71
Delta R.T. 0.006 min
Lab File: VN081959.D
Acq: 01 May 2024 16:15




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 63 Resp: 78672
Ion Ratio Lower Upper
63 100
98 7.8 3.6 10.9
100 3.9 2.6 7.8



#25
2-Butanone
Concen: 0.544 ug/l
RT: 7.494 min Scan# 942
Delta R.T. 0.018 min
Lab File: VN081959.D
Acq: 01 May 2024 16:15


Tgt Ion: 43 Resp: 1001
Ion Ratio Lower Upper
43 100
72 946.2 25.3 37.9#








#27
 cis-1,2-Dichloroethene
 Concen: 476.668 ug/l
 RT: 7.488 min Scan# 941
 Delta R.T. 0.006 min
 Lab File: VN081959.D
 Acq: 01 May 2024 16:15

Instrument :
 MSVOA_N
 ClientSampleId :



Tgt Ion: 96 Resp: 1413683




Ion	Ratio	Lower	Upper
96	100		
61	134.7	0.0	268.0
98	63.0	0.0	126.8




#31
 Cyclohexane
 Concen: 1.262 ug/l
 RT: 8.224 min Scan# 1066
 Delta R.T. -0.035 min
 Lab File: VN081959.D
 Acq: 01 May 2024 16:15

Tgt Ion: 56 Resp: 6168

Ion	Ratio	Lower	Upper
56	100		
69	152.1	24.4	36.6#
84	96.7	77.0	115.4





#32

1,1,1-Trichloroethane

Concen: 1.069 ug/l

RT: 8.171 min Scan# 1056

Delta R.T. 0.006 min

Lab File: VN081959.D

Acq: 01 May 2024 16:15

Instrument :

MSVOA_N

ClientSampleId :





Tgt Ion: 97 Resp: 4685

Ion Ratio Lower Upper

97 100

99 0.0 50.3 75.5#

61 38.5 36.6 55.0

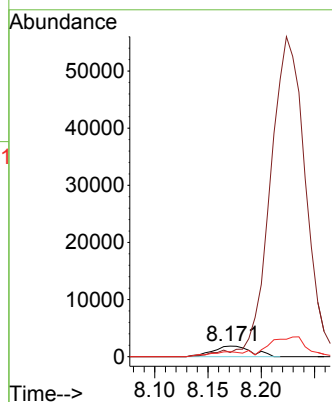

#33

1,2-Dichloroethane-d4

Concen: 45.362 ug/l

RT: 8.577 min Scan# 1126

Delta R.T. -0.000 min

Lab File: VN081959.D




Acq: 01 May 2024 16:15


Tgt Ion: 65 Resp: 147139

Ion Ratio Lower Upper

65 100

67 53.5 0.0 103.0





#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.106 min Scan# 11

Delta R.T. 0.006 min

Lab File: VN081959.D

Acq: 01 May 2024 16:15

Instrument :

MSVOA_N

ClientSampleId :





Tgt Ion:114 Resp: 386265

Ion Ratio Lower Upper

114 100

63 20.9 0.0 41.0

88 16.2 0.0 31.4

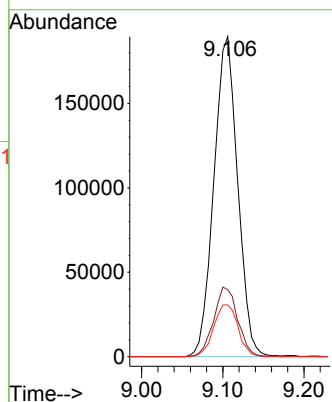

#35

Dibromofluoromethane

Concen: 47.841 ug/l

RT: 8.165 min Scan# 1056

Delta R.T. -0.000 min

Lab File: VN081959.D

Acq: 01 May 2024 16:15




Tgt Ion:113 Resp: 111261


Ion Ratio Lower Upper

113 100

111 102.7 83.4 125.2

192 15.6 14.0 21.0





#36

1,1-Dichloropropene

Concen: 5.139 ug/l

RT: 8.218 min Scan# 1065

Delta R.T. -0.153 min


Lab File: VN081959.D

Acq: 01 May 2024 16:15




Instrument :

MSVOA_N

ClientSampleId :



Tgt Ion:	75	Resp:	19444
Ion Ratio	Lower	Upper	
75	100		
110	7.7	17.8	53.5#
77	0.0	25.0	37.4#

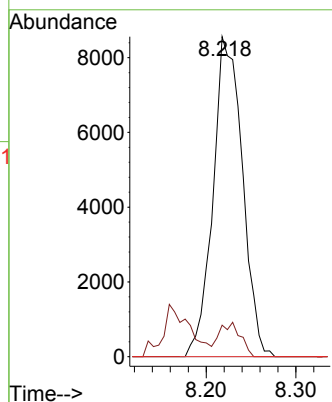

#38

Carbon Tetrachloride

Concen: 5.619 ug/l




RT: 8.229 min Scan# 1067


Delta R.T. -0.129 min

Lab File: VN081959.D

Acq: 01 May 2024 16:15

Tgt Ion:	117	Resp:	20777
Ion Ratio	Lower	Upper	
117	100		
119	6.3	76.5	114.7#
121	0.0	23.9	35.9#

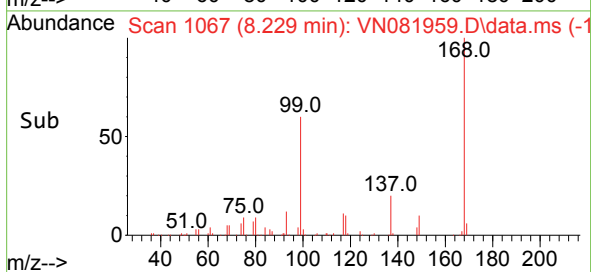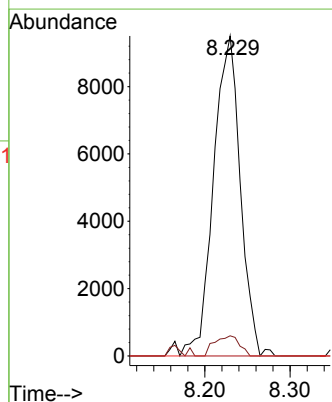



#39

Methylcyclohexane

Concen: 49.785 ug/l

RT: 9.359 min Scan# 1129

Delta R.T. -0.241 min


Lab File: VN081959.D

Acq: 01 May 2024 16:15

Instrument :

MSVOA_N

ClientSampleId :






Tgt Ion: 83 Resp: 228765

Ion Ratio Lower Upper

83 100

55 0.2 53.0 79.6#

98 186.8 37.1 55.7#

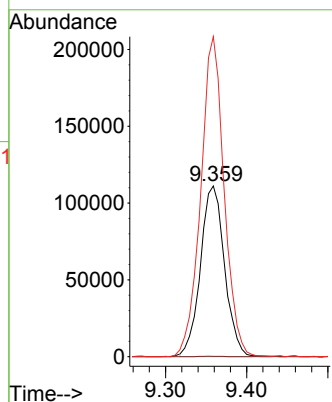

#40

Benzene

Concen: 1.679 ug/l

RT: 8.606 min Scan# 1131

Delta R.T. -0.000 min

Lab File: VN081959.D




Acq: 01 May 2024 16:15


Tgt Ion: 78 Resp: 19066

Ion Ratio Lower Upper

78 100

77 20.3 20.0 30.0

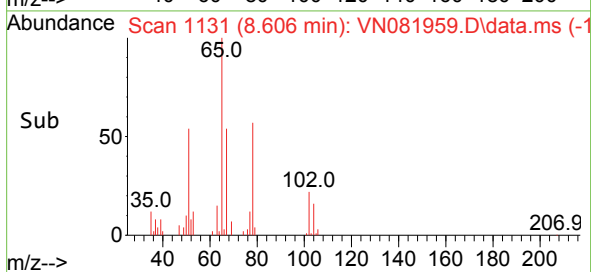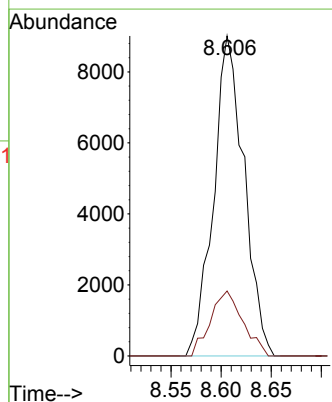



#42

1,2-Dichloroethane

Concen: 2.987 ug/l

RT: 8.671 min Scan# 1142

Delta R.T. -0.000 min

Lab File: VN081959.D

Acq: 01 May 2024 16:15

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion: 62 Resp: 12600

Ion Ratio Lower Upper

62 100

98 9.4 0.0 19.6



#43

Isopropyl Acetate

Concen: 0.708 ug/l

RT: 8.688 min Scan# 1145

Delta R.T. -0.000 min

Lab File: VN081959.D

Acq: 01 May 2024 16:15




Tgt Ion: 43 Resp: 5447


Ion Ratio Lower Upper

43 100

61 15.6 22.8 34.2#

87 0.0 12.0 18.0#





#44

Trichloroethene

Concen: 4783.450 ug/l

RT: 9.359 min Scan# 1259

Delta R.T. 0.006 min

Lab File: VN081959.D

Acq: 01 May 2024 16:15

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion:130 Resp:12526193

Ion Ratio Lower Upper

130 100

95 126.8 0.0 195.4



#45

1,2-Dichloropropane

Concen: 19.197 ug/l

RT: 9.359 min Scan# 1259

Delta R.T. -0.265 min

Lab File: VN081959.D




Acq: 01 May 2024 16:15


Tgt Ion: 63 Resp: 57063

Ion Ratio Lower Upper

63 100


65 474.1 24.1 36.1#








#49
1,4-Dioxane
Concen: 20.946 ug/l
RT: 9.694 min Scan# 1169
Delta R.T. -0.000 min
Lab File: VN081959.D
Acq: 01 May 2024 16:15

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion: 88 Resp: 1169
Ion Ratio Lower Upper
88 100
43 63.0 19.0 28.6#
58 66.1 50.6 76.0

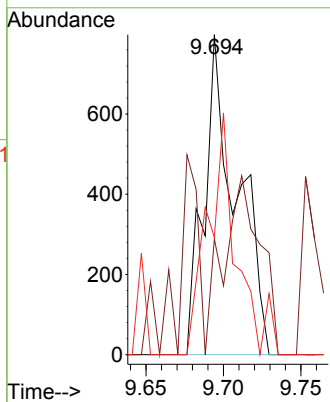

#50
Toluene-d8
Concen: 51.119 ug/l
RT: 10.571 min Scan# 1465
Delta R.T. 0.006 min
Lab File: VN081959.D
Acq: 01 May 2024 16:15

Tgt Ion: 98 Resp: 466910
Ion Ratio Lower Upper
98 100
100 65.9 51.8 77.6


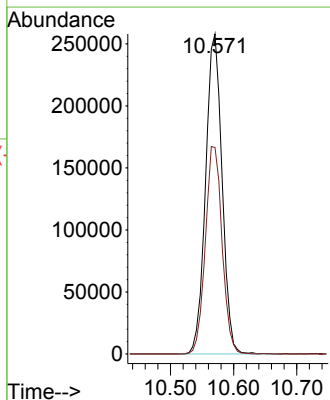
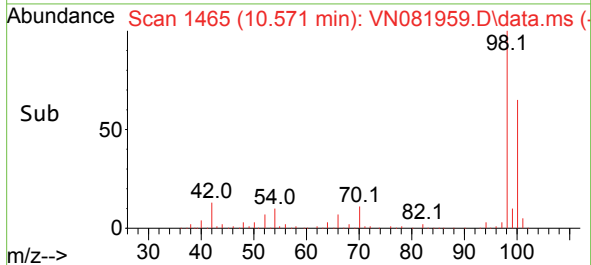



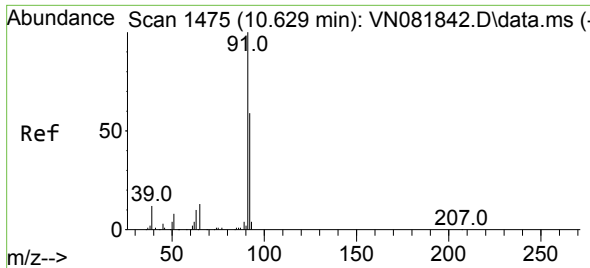

#52
Toluene
Concen: 0.307 ug/l
RT: 10.623 min Scan# 1475
Delta R.T. -0.006 min
Lab File: VN081959.D
Acq: 01 May 2024 16:15




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 92 Resp: 2091
Ion Ratio Lower Upper
92 100
91 185.1 136.7 205.1

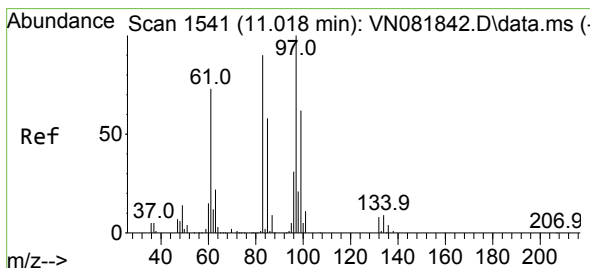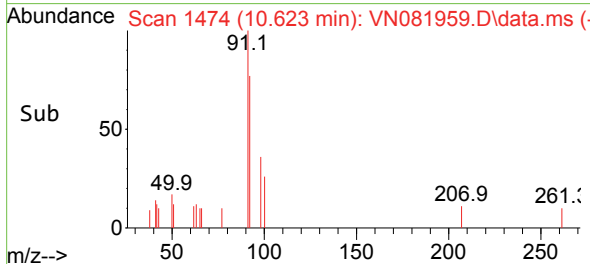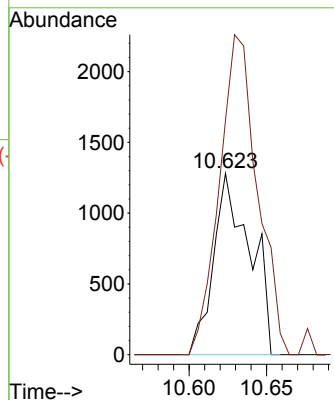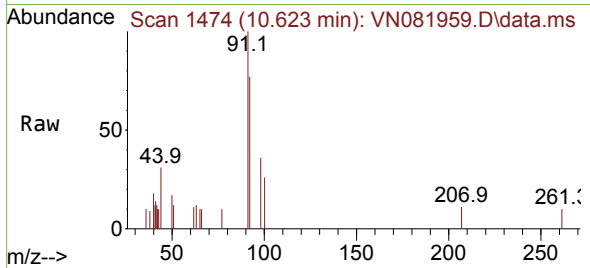

#55
1,1,2-Trichloroethane
Concen: 0.382 ug/l
RT: 11.029 min Scan# 1543
Delta R.T. 0.012 min
Lab File: VN081959.D
Acq: 01 May 2024 16:15

Tgt Ion: 97 Resp: 1022
Ion Ratio Lower Upper
97 100
83 35.6 70.4 105.6#
85 77.9 45.6 68.4#
99 84.9 50.9 76.3#


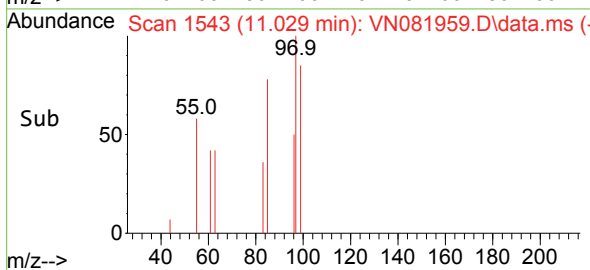
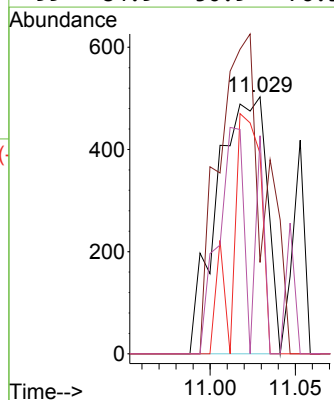
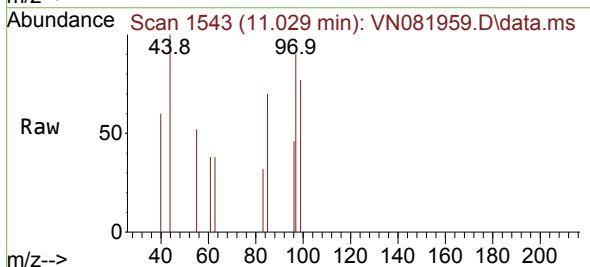


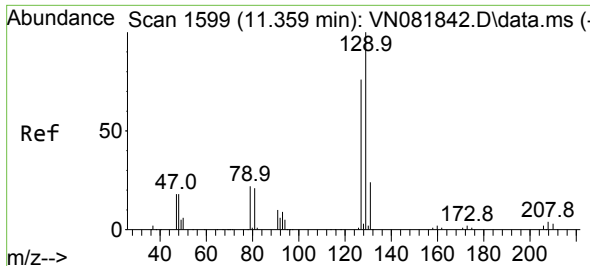

#60
Dibromochloromethane
Concen: 50.724 ug/l
RT: 11.106 min Scan# 11
Delta R.T. -0.253 min
Lab File: VN081959.D
Acq: 01 May 2024 16:15




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:129 Resp: 143715
Ion Ratio Lower Upper
129 100
127 0.2 38.3 114.8#

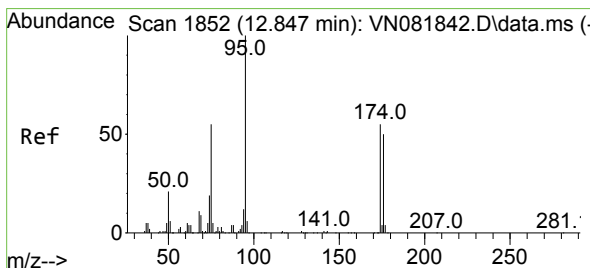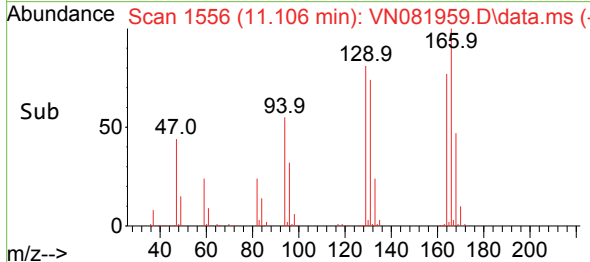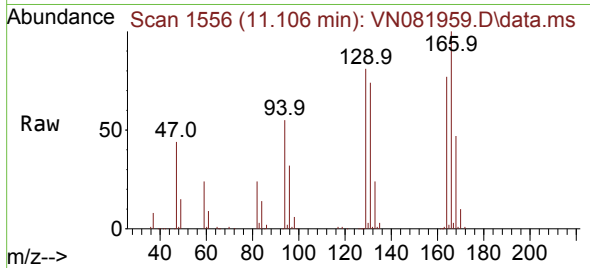

#62
4-Bromofluorobenzene
Concen: 44.328 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. 0.006 min
Lab File: VN081959.D
Acq: 01 May 2024 16:15


Tgt Ion: 95 Resp: 160053
Ion Ratio Lower Upper
95 100
174 62.5 0.0 160.6
176 60.2 0.0 152.8

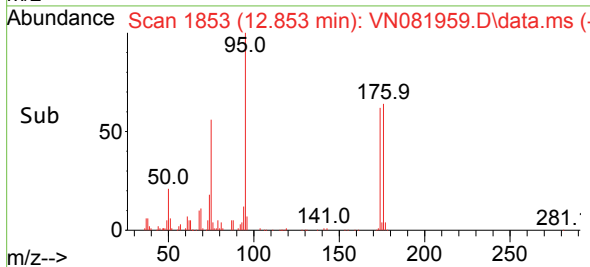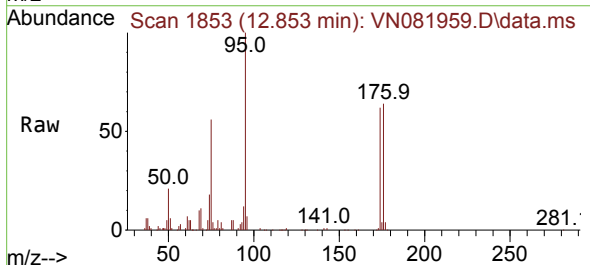






#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.865 min Scan# 117
Delta R.T. -0.000 min
Lab File: VN081959.D
Acq: 01 May 2024 16:15


Instrument :
MSVOA_N
ClientSampleId :





Tgt Ion:117 Resp: 336703
Ion Ratio Lower Upper
117 100
82 60.7 44.6 66.8
119 32.7 25.9 38.9

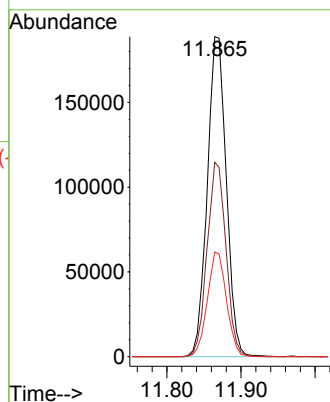


#64
Tetrachloroethene
Concen: 57.013 ug/l
RT: 11.106 min Scan# 1556
Delta R.T. -0.000 min
Lab File: VN081959.D
Acq: 01 May 2024 16:15




Tgt Ion:164 Resp: 139422
Ion Ratio Lower Upper
164 100
166 130.1 97.6 146.4
129 106.0 73.7 110.5
131 96.1 75.8 113.6

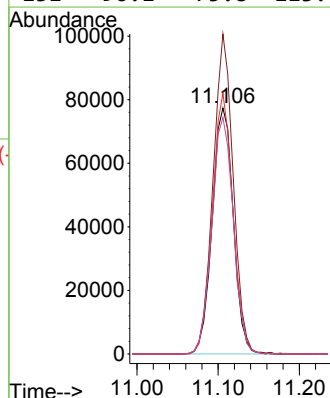






#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.794 min Scan# 20
Delta R.T. -0.000 min
Lab File: VN081959.D
Acq: 01 May 2024 16:15

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion:152 Resp: 134370
Ion Ratio Lower Upper
152 100
115 64.7 30.4 91.3
150 158.7 0.0 353.2

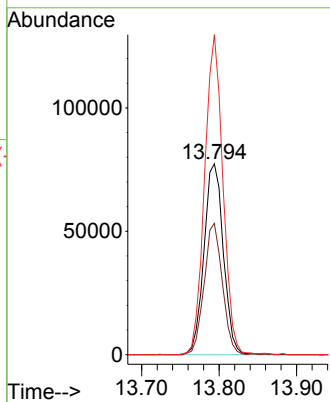

#76
1,2,3-Trichloropropane
Concen: 25.523 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. -0.147 min
Lab File: VN081959.D
Acq: 01 May 2024 16:15

Tgt Ion: 75 Resp: 88919
Ion Ratio Lower Upper
75 100
77 1.2 90.5 271.3#


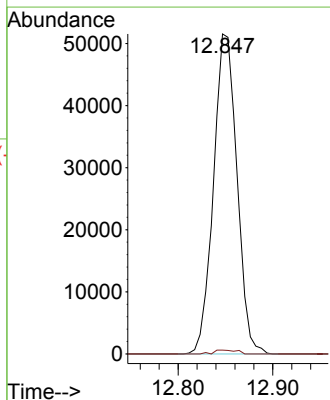




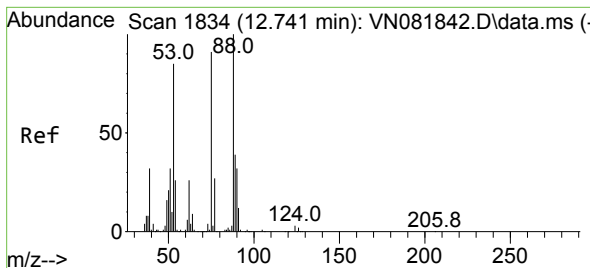

#81
trans-1,4-Dichloro-2-butene
Concen: 52.299 ug/l
RT: 12.847 min Scan# 11
Delta R.T. 0.106 min
Lab File: VN081959.D
Acq: 01 May 2024 16:15




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 75 Resp: 88919
Ion Ratio Lower Upper
75 100
53 0.0 72.9 109.3#
89 0.1 39.1 58.7#

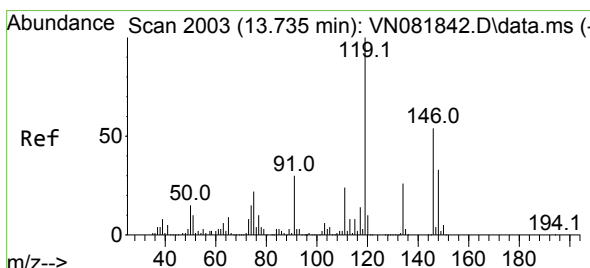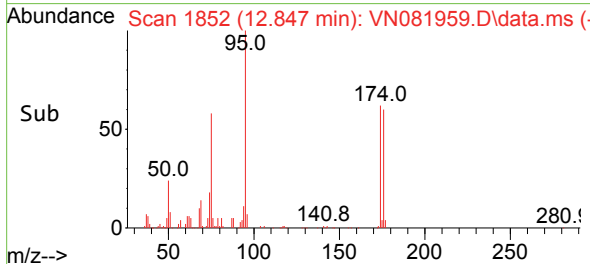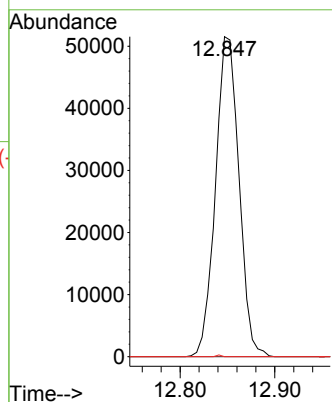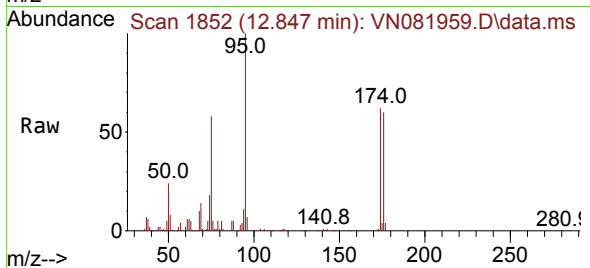

#87
1,3-Dichlorobenzene
Concen: 0.696 ug/l
RT: 13.811 min Scan# 2016
Delta R.T. 0.076 min
Lab File: VN081959.D
Acq: 01 May 2024 16:15


Tgt Ion: 146 Resp: 3245
Ion Ratio Lower Upper
146 100
111 101.4 20.8 62.5#
148 81.8 32.1 96.3

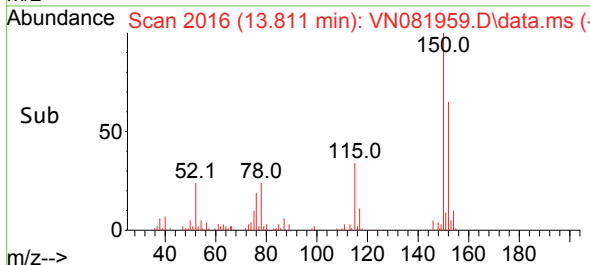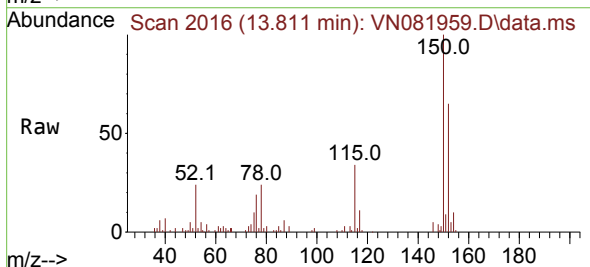

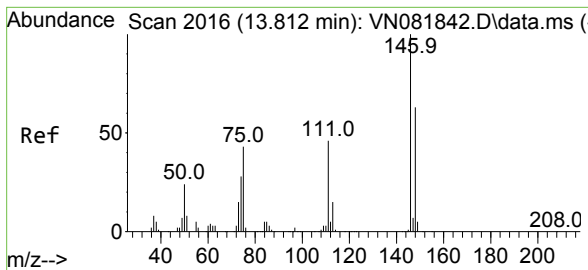

#88
 1,4-Dichlorobenzene
 Concen: 0.706 ug/l
 RT: 13.811 min Scan# 20
 Delta R.T. -0.000 min
 Lab File: VN081959.D
 Acq: 01 May 2024 16:15

Instrument :
 MSVOA_N
 ClientSampleId :

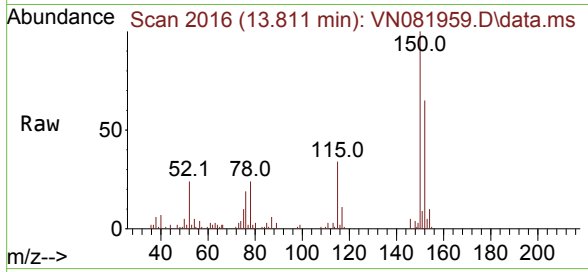

Tgt Ion	Ratio	Lower	Upper
146	100		
111	101.4	19.3	57.9#
148	81.8	31.3	93.9

